

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
 Data File : PP069540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2025 03:57
 Operator : YP\AJ
 Sample : Q1306-02 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH840Y-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/06/2025
 Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 06:35:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.535	3.837	3598236	2464212	2.514	2.761m
2) SA Decachlor...	10.267	8.900	3149967	2743820	2.882	2.453

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020525\
Data File : PP069540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2025 03:57
Operator : YP\AJ
Sample : Q1306-02 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH840Y-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 06:35:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

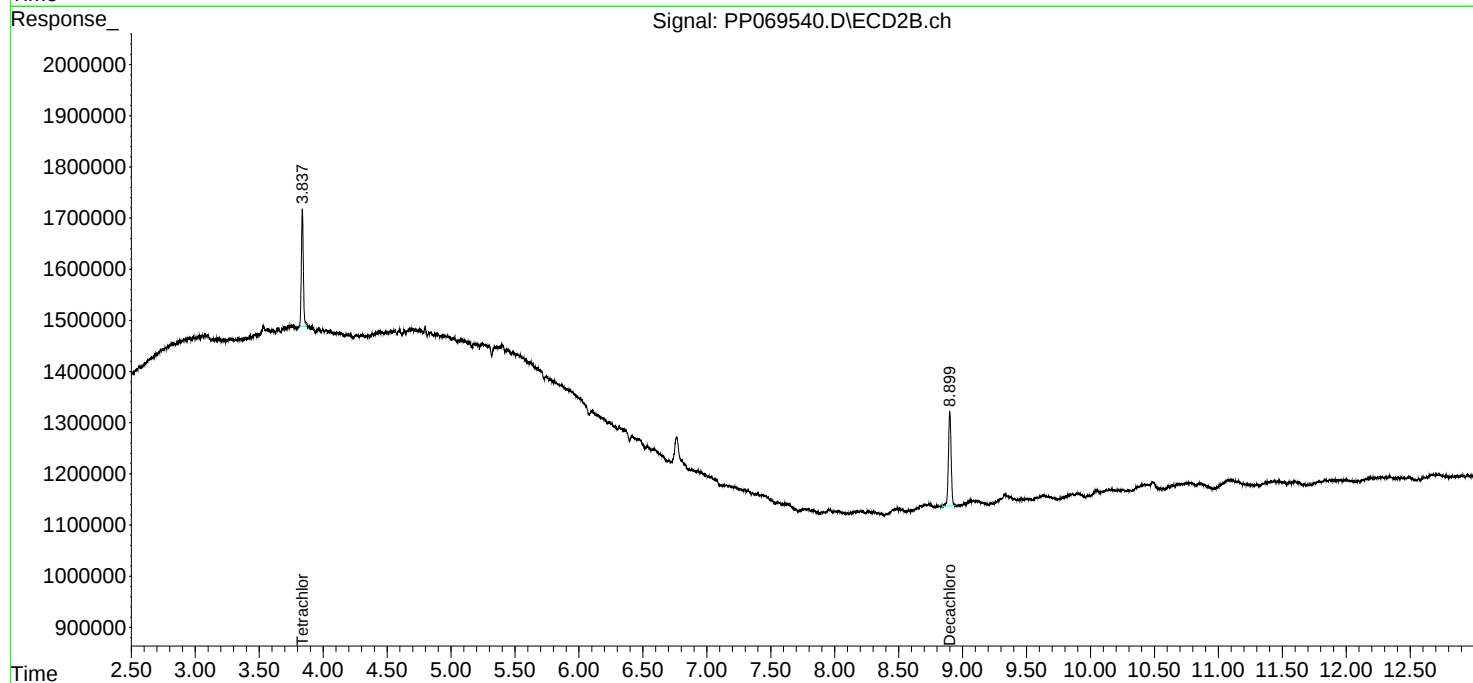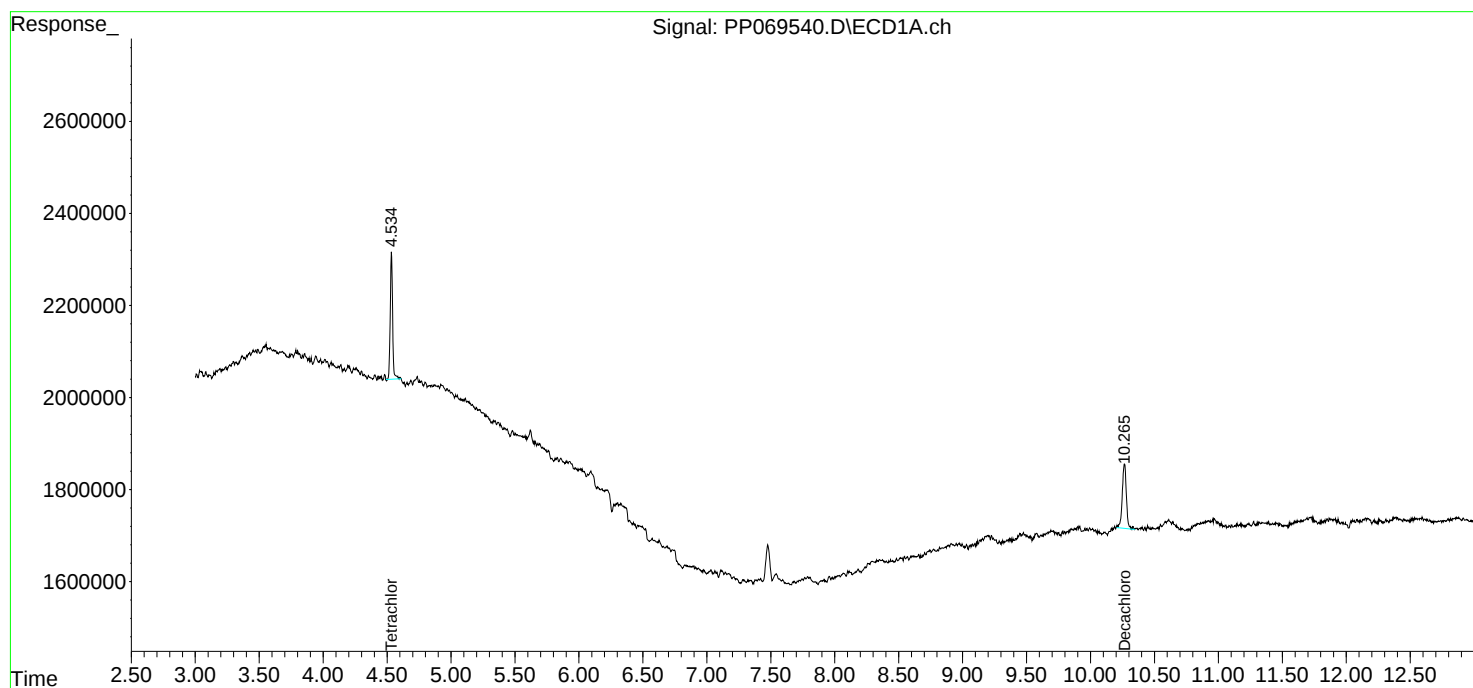

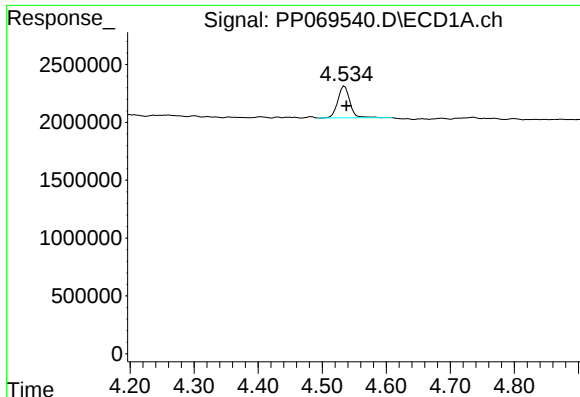

#1 Tetrachloro-m-xylene

R.T.: 4.535 min
Delta R.T.: -0.003 min
Response: 3598236
Conc: 2.51 ng/ml

Instrument :

ECD_P


ClientSampleId :

KMH840Y-1-2

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 02/06/2025
Supervised By :Ankita Jodhani 02/06/2025

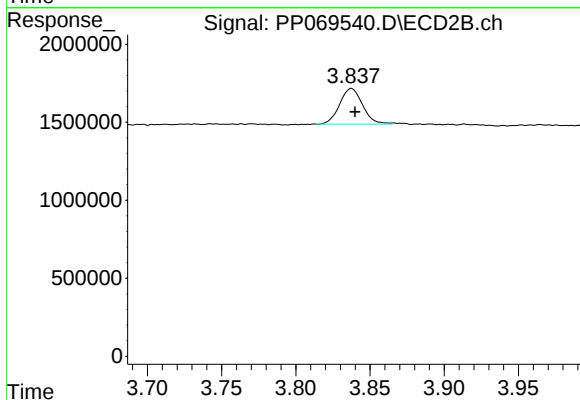


#1 Tetrachloro-m-xylene

R.T.: 3.837 min
Delta R.T.: -0.003 min
Response: 2464212
Conc: 2.76 ng/ml m

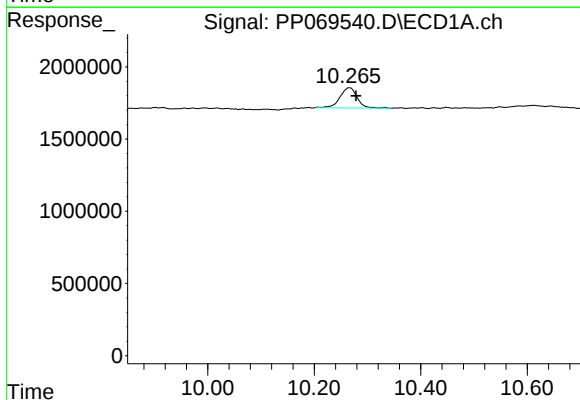

#2 Decachlorobiphenyl

R.T.: 10.267 min
Delta R.T.: -0.012 min
Response: 3149967
Conc: 2.88 ng/ml

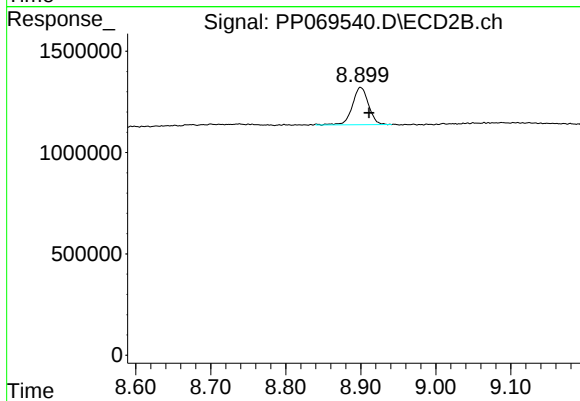

#2 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.011 min
Response: 2743820
Conc: 2.45 ng/ml