

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020819\
 Data File : PP029115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 19:49
 Operator : EI\MA
 Sample : K1348-02
 Misc : hexane
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-01-020719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 23:47:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020619.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 07 06:00:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.961	12.140	10349581	14786703	565.699	547.113
Target Compounds							
7) T	MCPA	12.839	0.000	4710516	0	273.537	N.D. #
8) T	DICHLORPROP	0.000	13.571	0	1185392	N.D.	47.184 #
13) T	2,4-DB	0.000	16.539	0	522683	N.D.	29.989 #
15) T	Picloram	17.510	0.000	325216	0	1.445	N.D. #
16) T	DCPA	0.000	18.119	0	135018	N.D.	0.772 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020819\
Data File : PP029115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 19:49
Operator : EI\MA
Sample : K1348-02
Misc : hexane
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
OK-01-020719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 23:47:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020619.M
Quant Title : 8080.M
QLast Update : Thu Feb 07 06:00:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

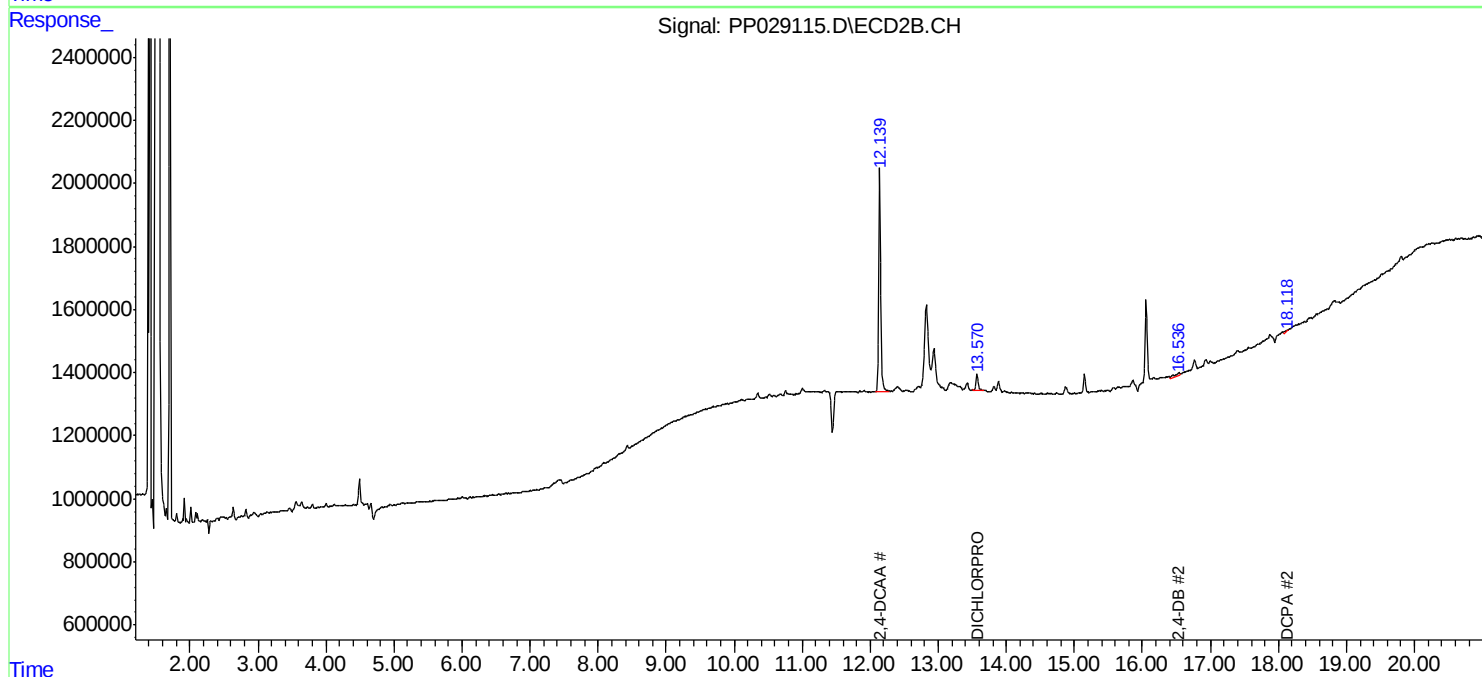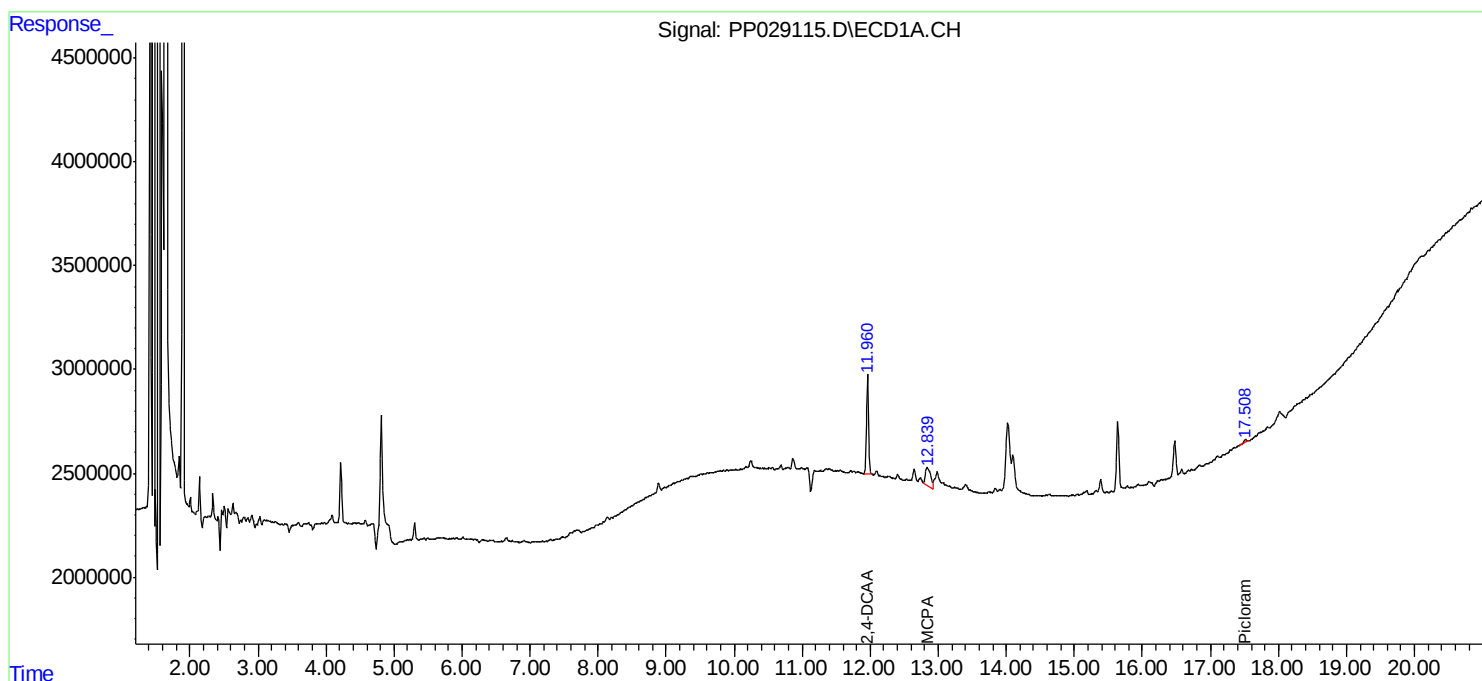


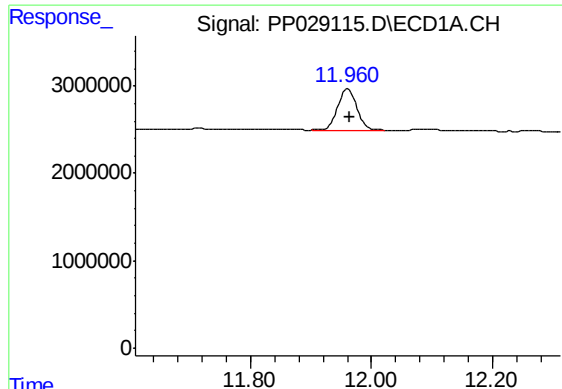

#4 2,4-DCAA


R.T.: 11.961 min
Delta R.T.: -0.004 min
Response: 10349581
Conc: 565.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-020719

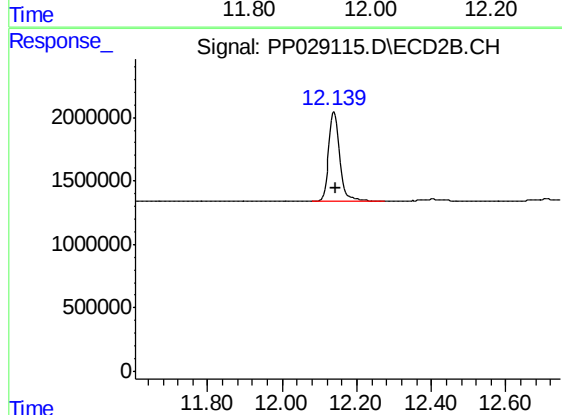


#4 2,4-DCAA

R.T.: 12.140 min
Delta R.T.: -0.002 min
Response: 14786703
Conc: 547.11 ng/ml

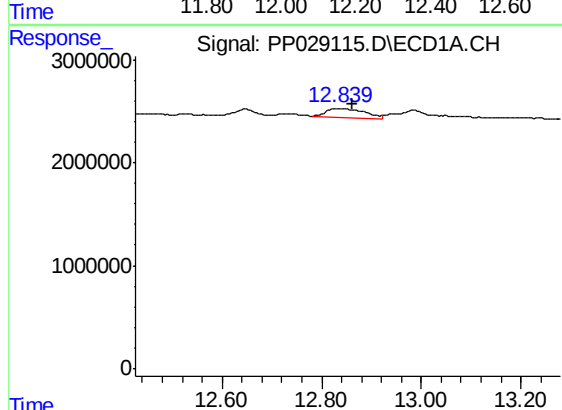


#7 MCPA

R.T.: 12.839 min
Delta R.T.: -0.023 min
Response: 4710516
Conc: 273.54 ug/ml

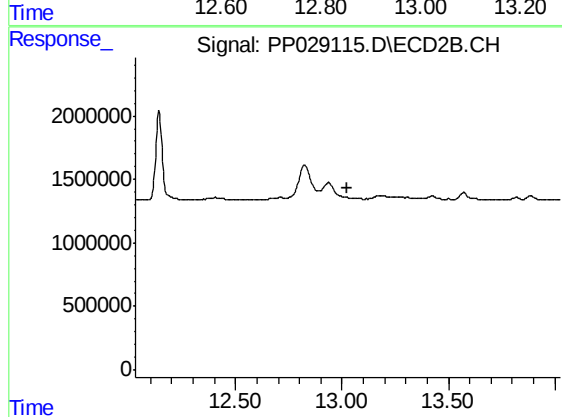

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 13.026 min
Response: 0
Conc: N.D.

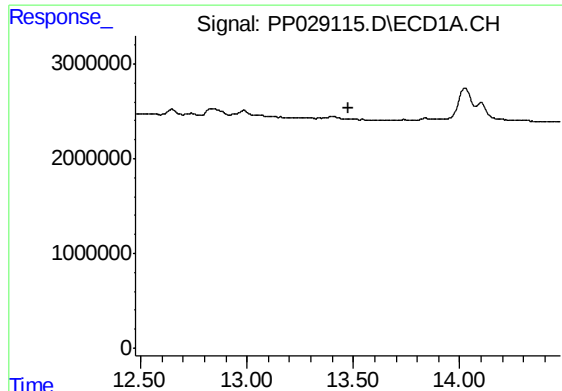

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
OK-01-020719

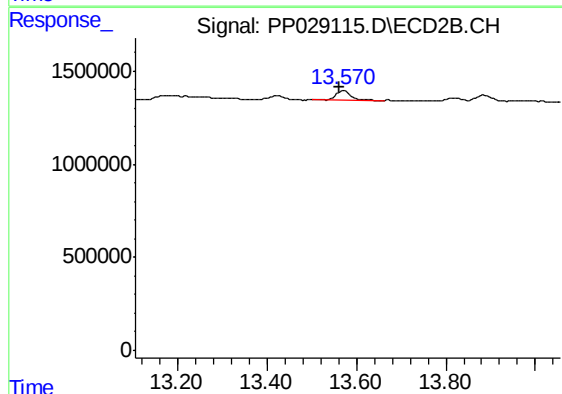


#8 DICHLORPROP

R.T.: 13.571 min
Delta R.T.: 0.008 min
Response: 1185392
Conc: 47.18 ng/ml

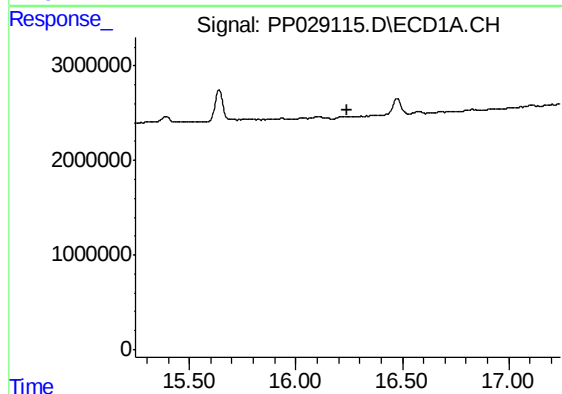


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.244 min
Response: 0
Conc: N.D.

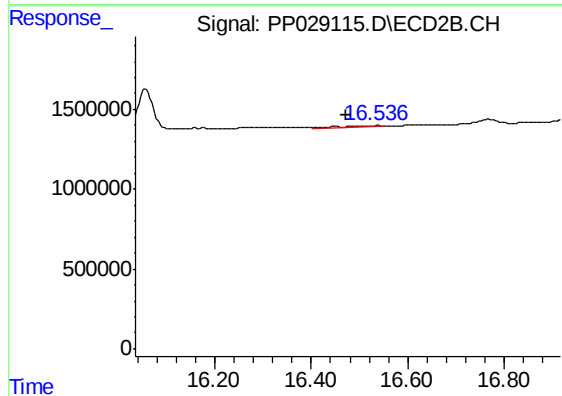

#13 2,4-DB


R.T.: 16.539 min
Delta R.T.: 0.068 min
Response: 522683
Conc: 29.99 ng/ml

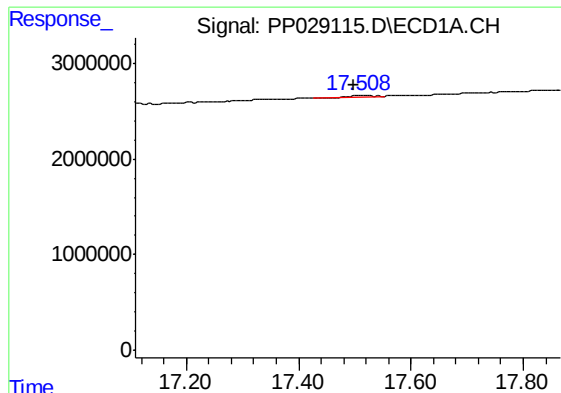

#15 Picloram


R.T.: 17.510 min
Delta R.T.: 0.013 min
Response: 325216
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-020719

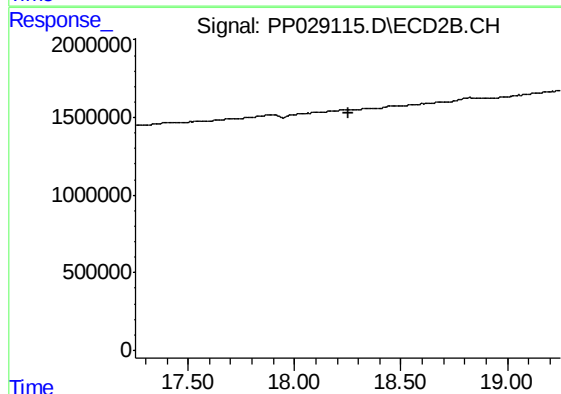


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.251 min
Response: 0
Conc: N.D.

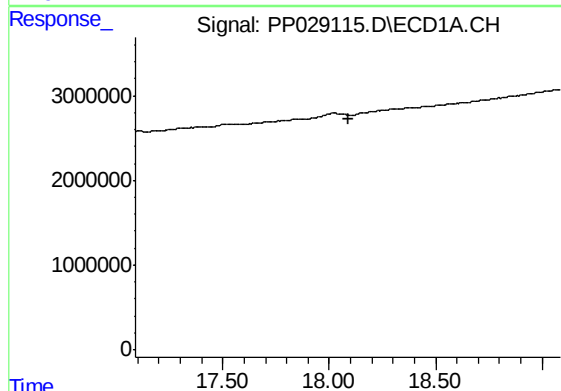

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.088 min
Response: 0
Conc: N.D.

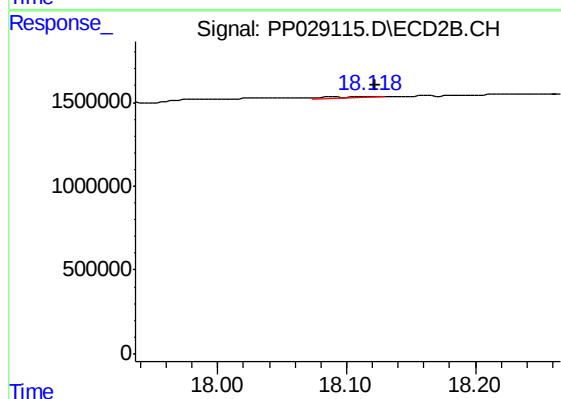

#16 DCPA

R.T.: 18.119 min
Delta R.T.: -0.004 min
Response: 135018
Conc: 0.77 ng/ml