

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020819\
 Data File : PP029120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2019 21:56
 Operator : EI\MA
 Sample : K1411-01
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EIGI-RO-294

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 23:48:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020619.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 07 06:00:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.962	12.142	11372043	15094122	621.586	558.487
Target Compounds							
7) T	MCPA	12.829	0.000	7510654	0	436.140	N.D. #
8) T	DICHLORPROP	0.000	13.572	0	1670468	N.D.	66.493 #
15) T	Picloram	0.000	18.251	0	1588198	N.D.	8.011 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020819\
Data File : PP029120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2019 21:56
Operator : EI\MA
Sample : K1411-01
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
EIGI-RO-294

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 23:48:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020619.M
Quant Title : 8080.M
QLast Update : Thu Feb 07 06:00:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

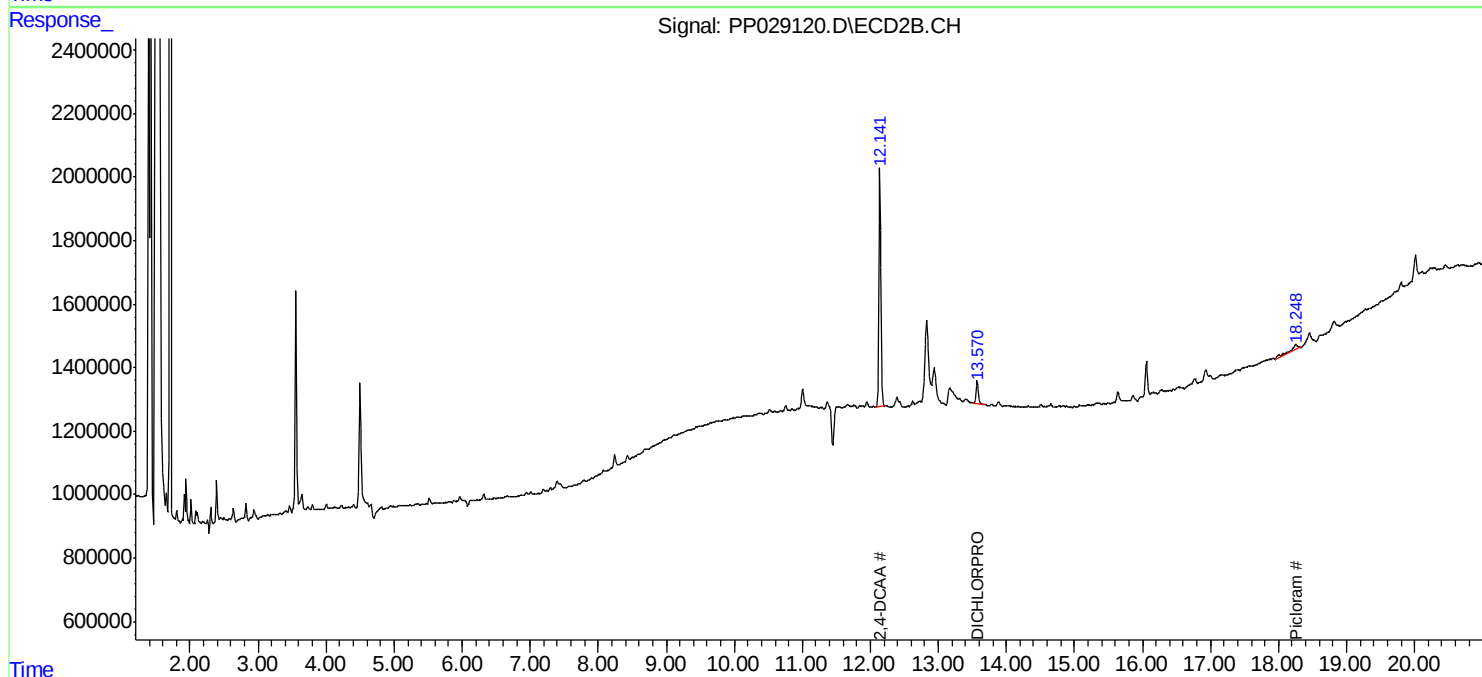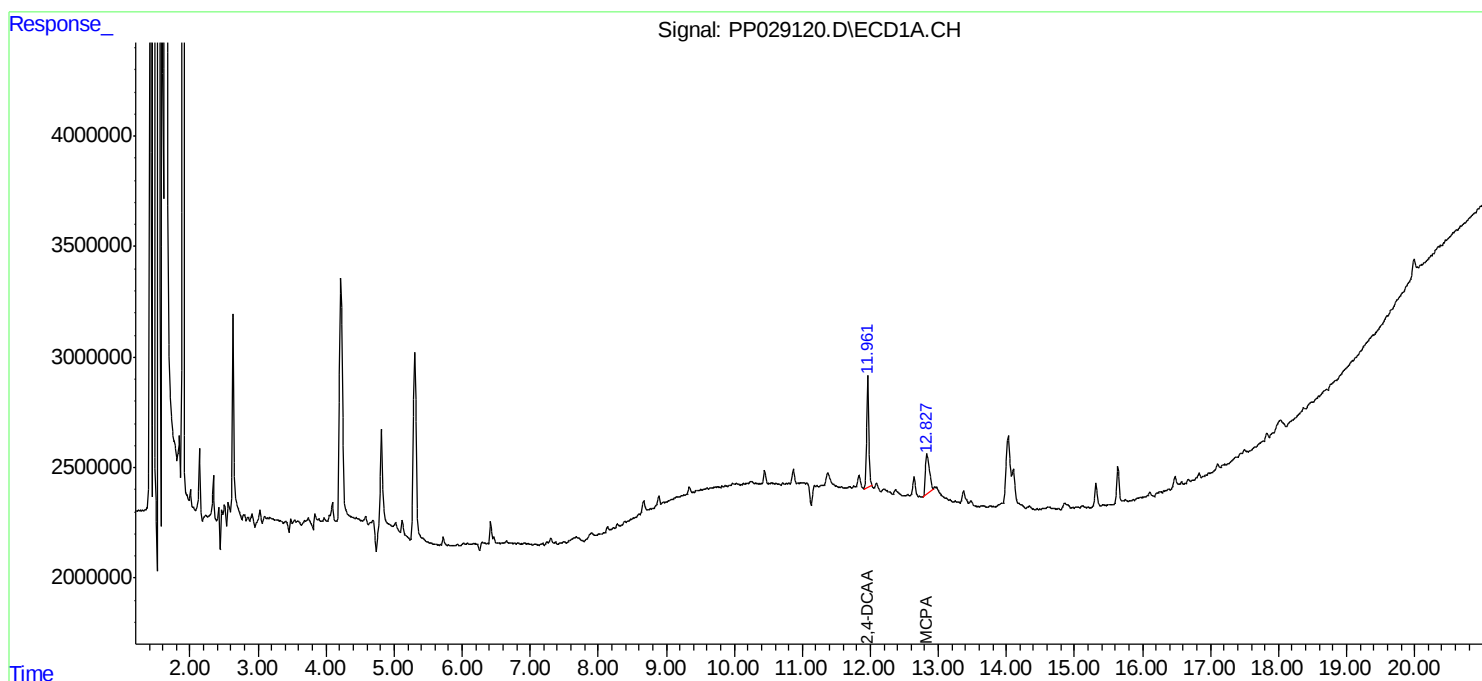


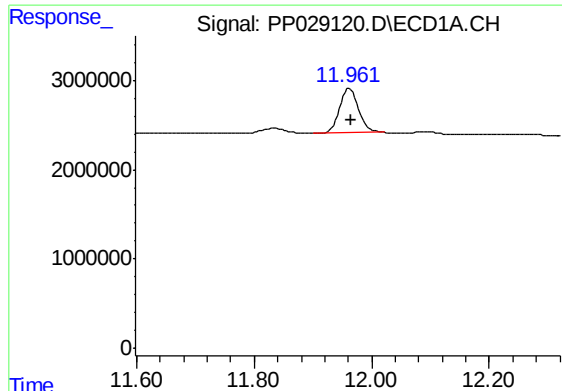

#4 2,4-DCAA


R.T.: 11.962 min
Delta R.T.: -0.003 min
Response: 11372043
Conc: 621.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
EIGI-RO-294

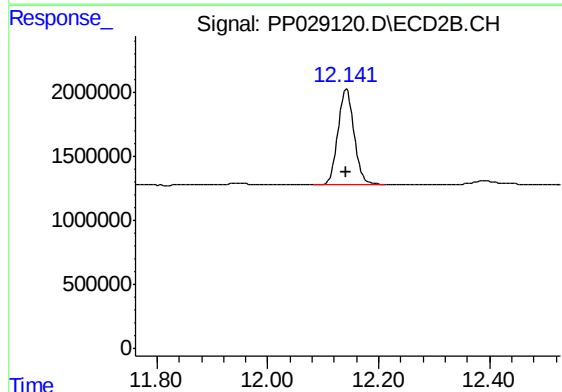


#4 2,4-DCAA

R.T.: 12.142 min
Delta R.T.: 0.000 min
Response: 15094122
Conc: 558.49 ng/ml

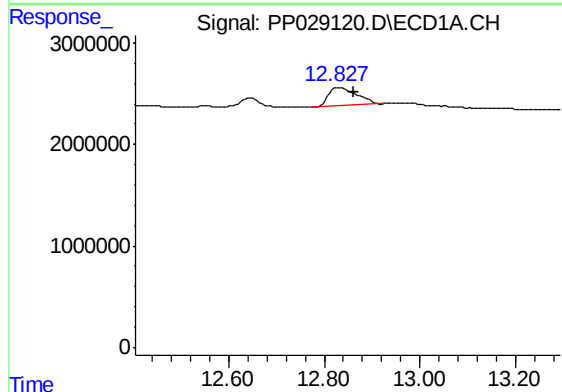


#7 MCPA

R.T.: 12.829 min
Delta R.T.: -0.033 min
Response: 7510654
Conc: 436.14 ug/ml

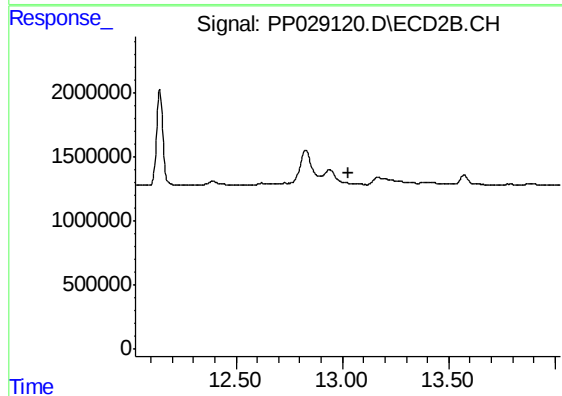

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 13.026 min
Response: 0
Conc: N.D.

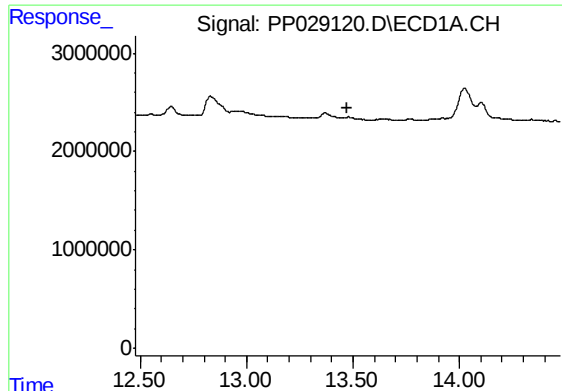

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
EIGI-RO-294

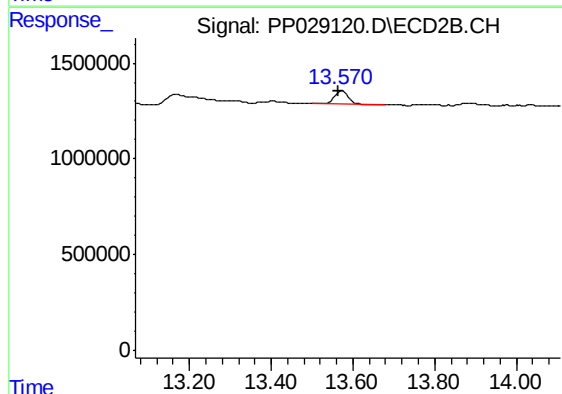


#8 DICHLORPROP

R.T.: 13.572 min
Delta R.T.: 0.009 min
Response: 1670468
Conc: 66.49 ng/ml

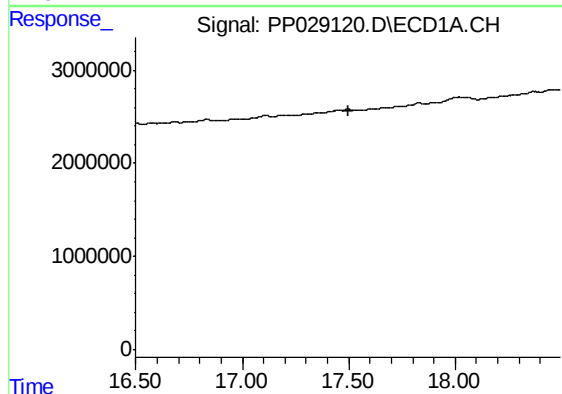

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.497 min
Response: 0
Conc: N.D.

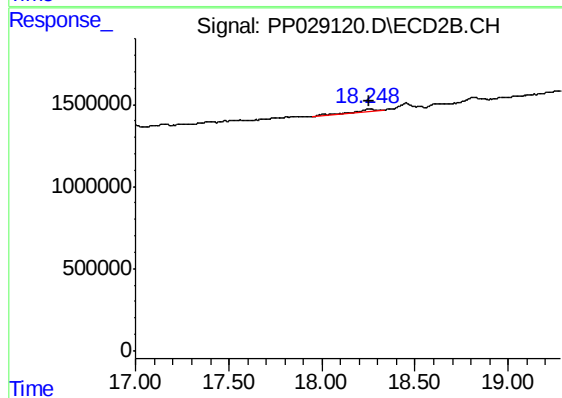

#15 Picloram

R.T.: 18.251 min
Delta R.T.: 0.000 min
Response: 1588198
Conc: 8.01 ng/ml