

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
 Data File : PP033143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2021 16:31
 Operator : DD\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC250

Manual Integrations
 APPROVED

Ankita
 2/9/2021 10:50:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:10:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 02:03:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.730	4.003	1632866	1098046	25.889	25.752
2) SA Decachlor...	10.551	9.268	1157849	908433	25.731	26.017
Target Compounds						
21) L5 AR-1248-1	6.029	5.249	251210	177230	258.204	264.097
22) L5 AR-1248-2	6.321	5.510	358034	261875	263.579m	265.195
23) L5 AR-1248-3	6.535	5.554	439007	277250	262.637	263.842
24) L5 AR-1248-4	6.960	5.738	473707	338001	266.397	265.413
25) L5 AR-1248-5	6.999	6.160	463697	306225	263.054	263.544

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
Data File : PP033143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2021 16:31
Operator : DD\AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:10:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 02:03:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

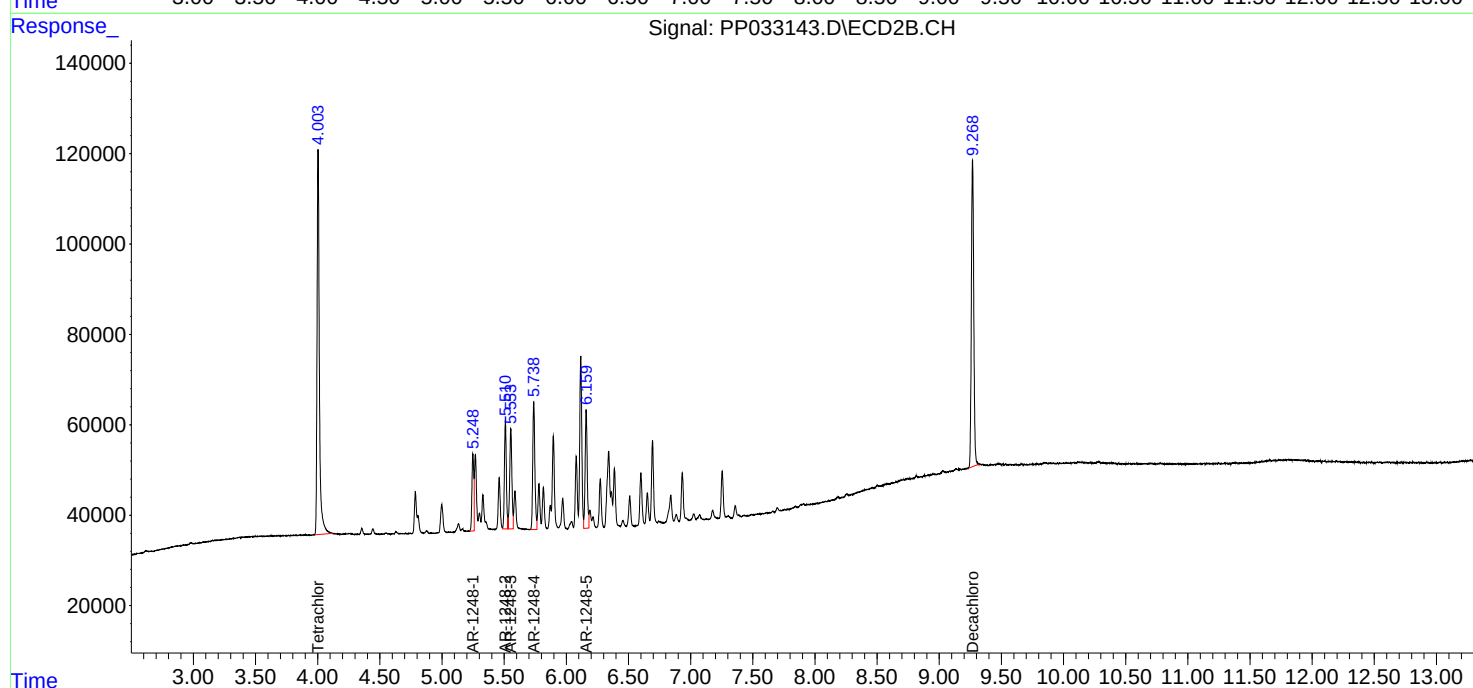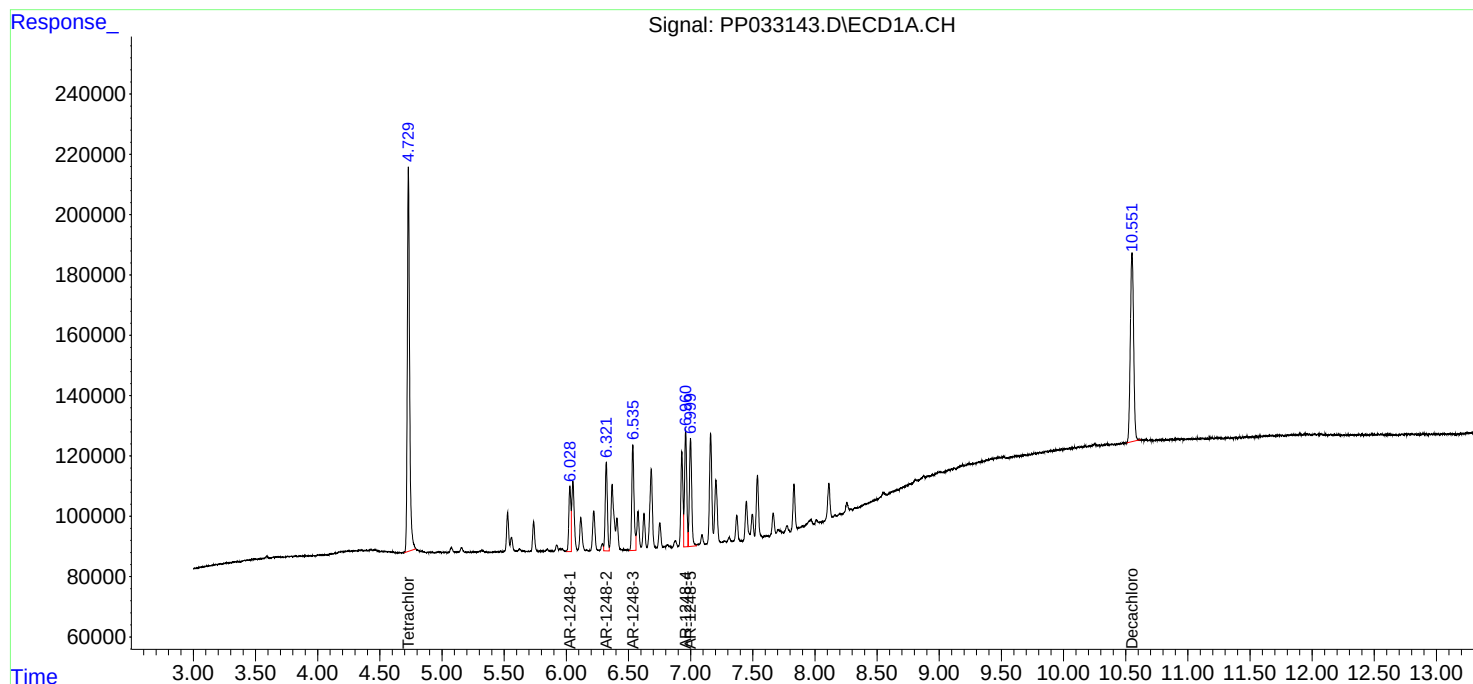

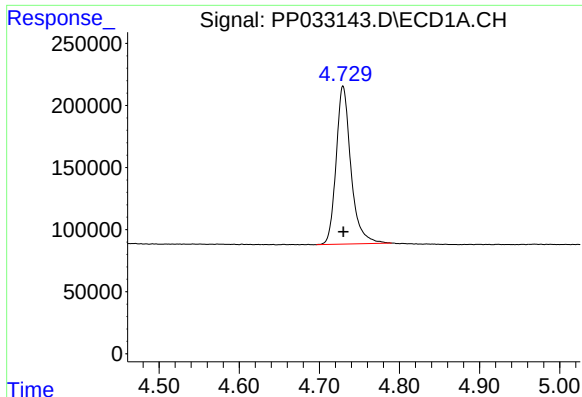


#1 Tetrachloro-m-xylene

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 1632866
Conc: 25.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:42 AM

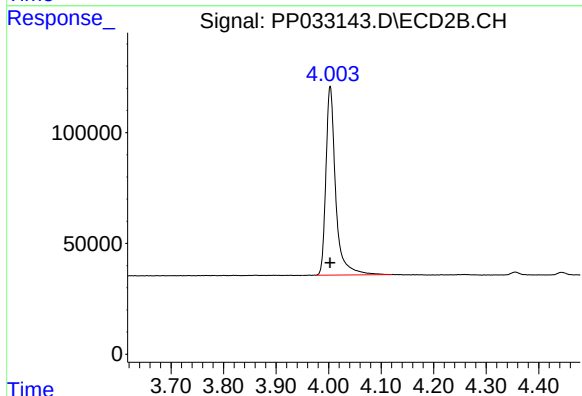


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: 0.000 min
Response: 1098046
Conc: 25.75 ng/ml

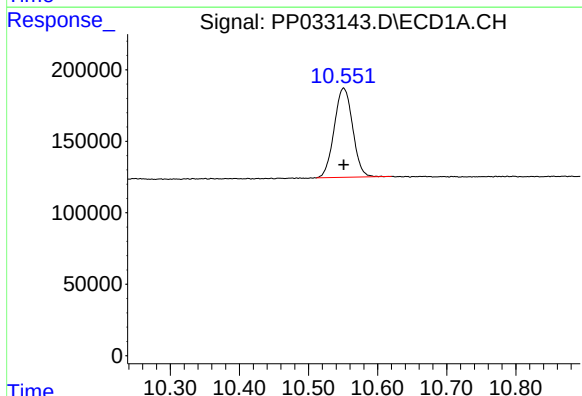


#2 Decachlorobiphenyl

R.T.: 10.551 min
Delta R.T.: 0.000 min
Response: 1157849
Conc: 25.73 ng/ml

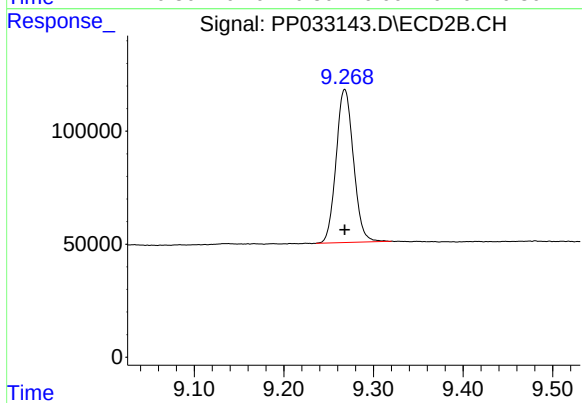

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 908433
Conc: 26.02 ng/ml

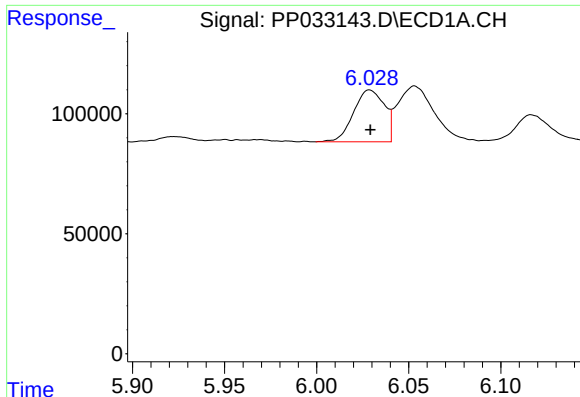


#21 AR-1248-1

R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 251210
Conc: 258.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:42 AM

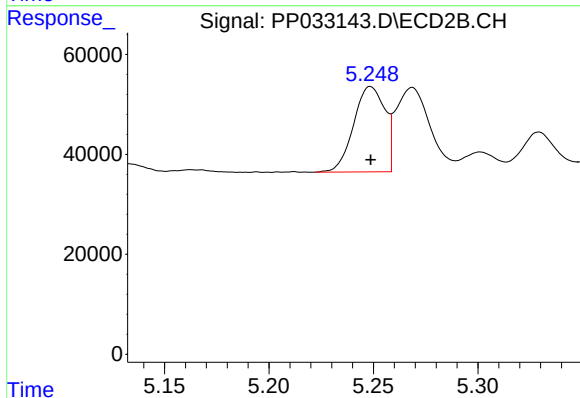


#21 AR-1248-1

R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 177230
Conc: 264.10 ng/ml

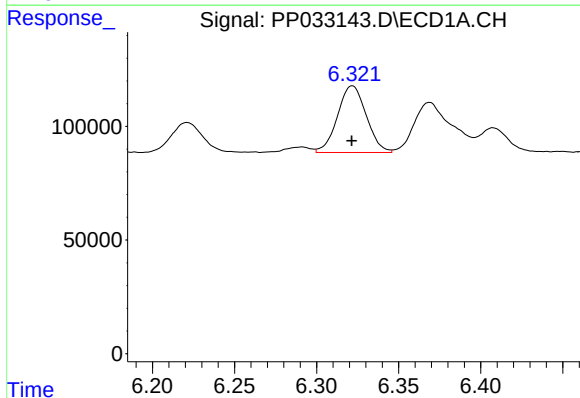


#22 AR-1248-2

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 358034
Conc: 263.58 ng/ml m

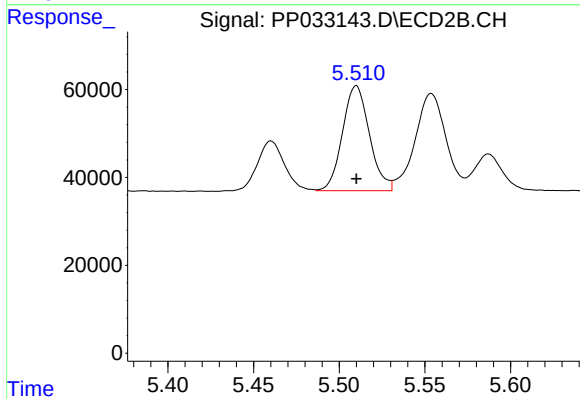

#22 AR-1248-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 261875
Conc: 265.19 ng/ml

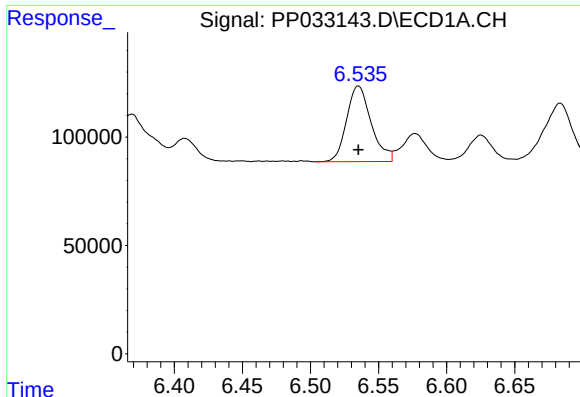


#23 AR-1248-3

R.T.: 6.535 min
Delta R.T.: 0.000 min
Response: 439007
Conc: 262.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:42 AM

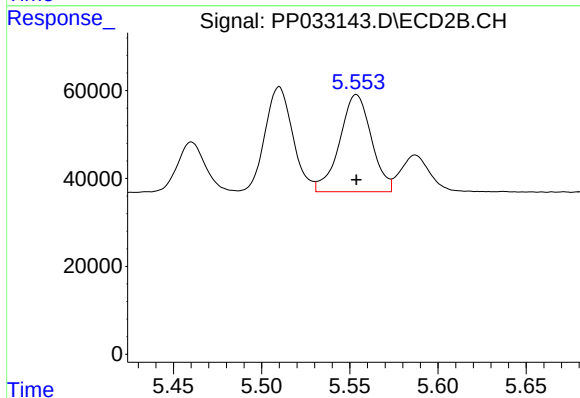


#23 AR-1248-3

R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 277250
Conc: 263.84 ng/ml

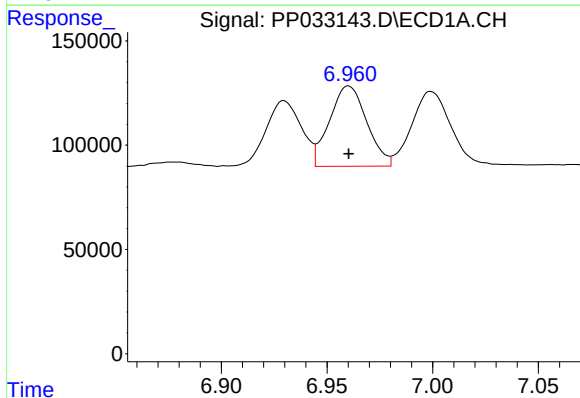


#24 AR-1248-4

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 473707
Conc: 266.40 ng/ml

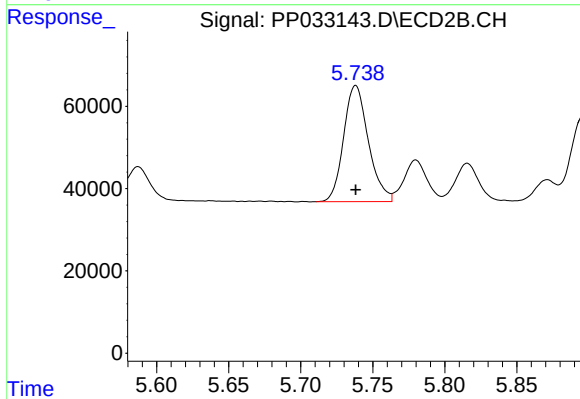

#24 AR-1248-4

R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 338001
Conc: 265.41 ng/ml

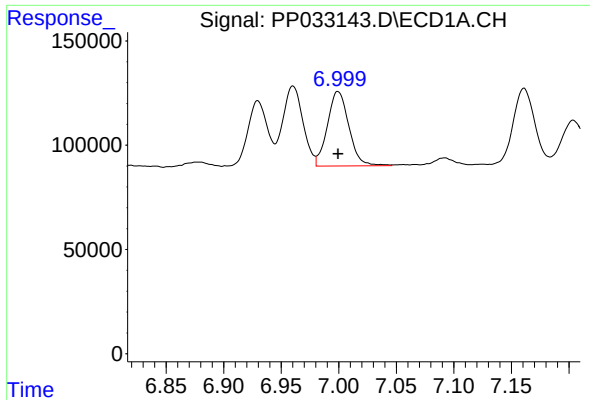


#25 AR-1248-5

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 463697
Conc: 263.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250

Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:42 AM

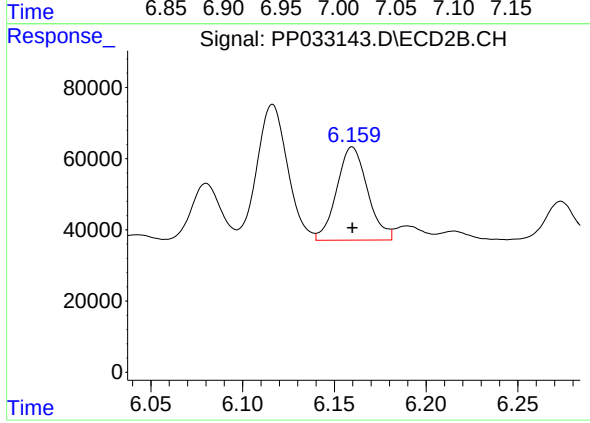

#25 AR-1248-5

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 306225
Conc: 263.54 ng/ml