

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
 Data File : PP033144.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2021 16:48
 Operator : DD\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Ankita
 2/9/2021 10:50:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:13:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 02:03:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.731	4.003	278612	176459	4.523	4.286
2)	SA Decachlor...	10.551	9.268	188010	156370	4.320	4.574
Target Compounds							
21)	L5 AR-1248-1	6.027	5.249	44783	28369	46.918m	43.622
22)	L5 AR-1248-2	6.321	5.510	59439	42343	44.198m	44.137
23)	L5 AR-1248-3	6.536	5.554	70513	44026	43.158m	43.300
24)	L5 AR-1248-4	6.961	5.738	74521	55120	43.272m	44.478
25)	L5 AR-1248-5	7.000	6.160	82452	49943	47.386	44.299m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
Data File : PP033144.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2021 16:48
Operator : DD\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:13:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 02:03:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

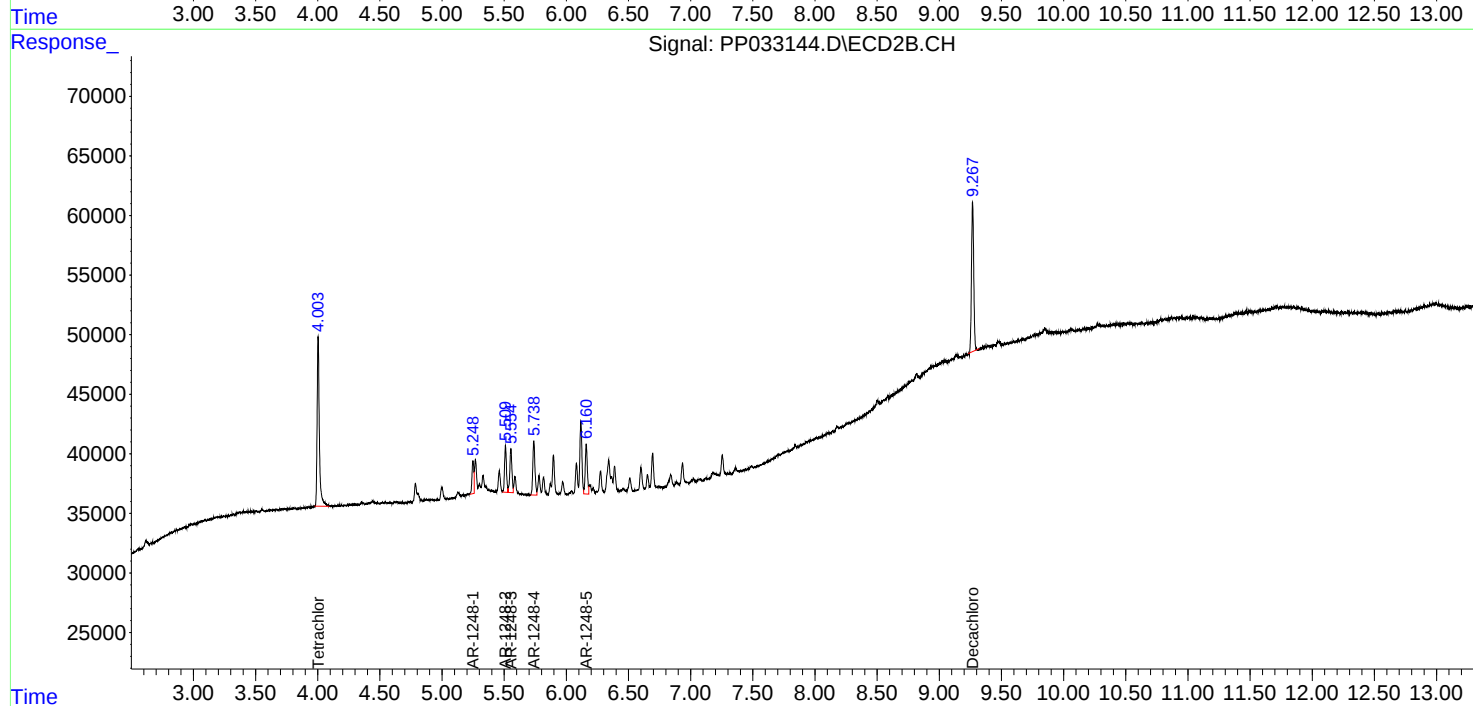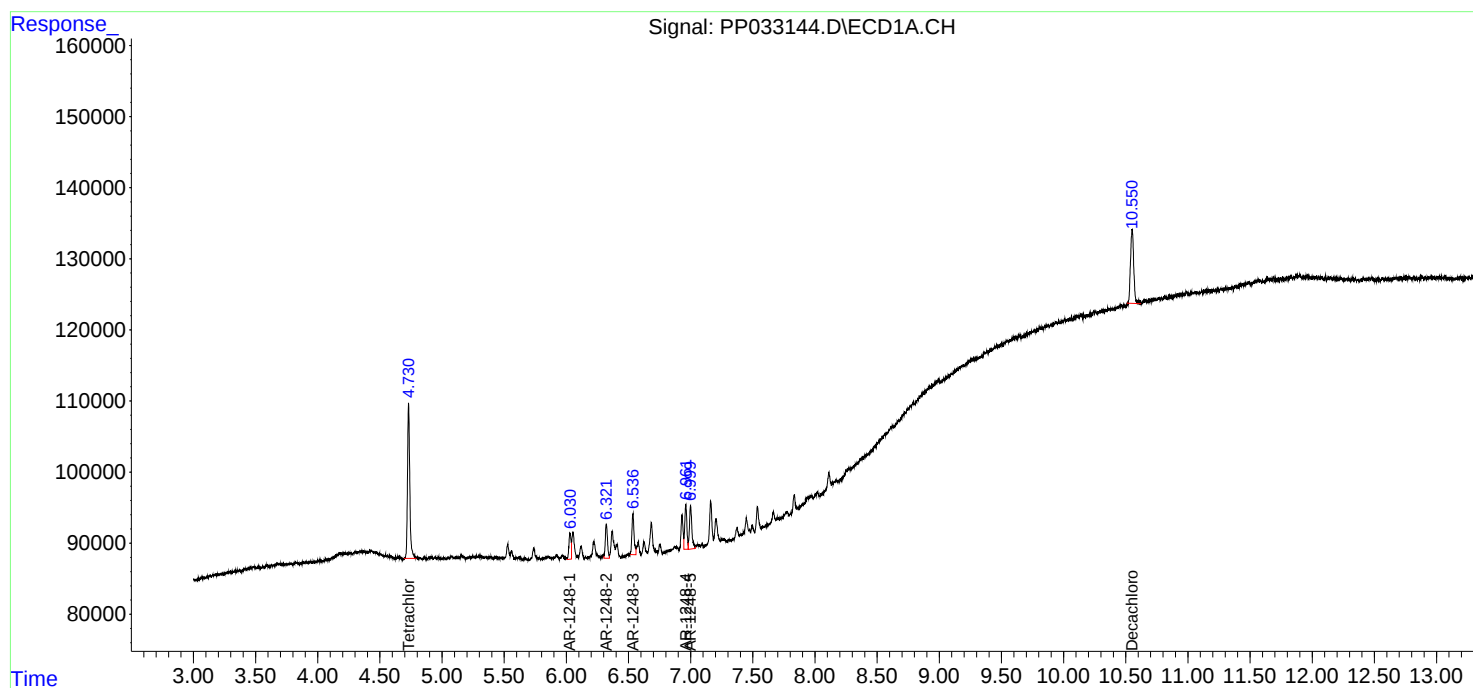

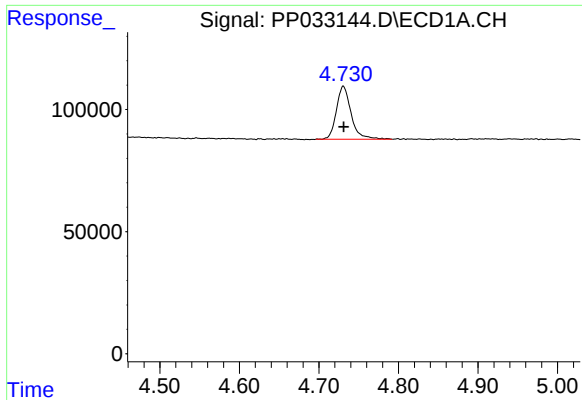


#1 Tetrachloro-m-xylene

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 278612
Conc: 4.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:44 AM

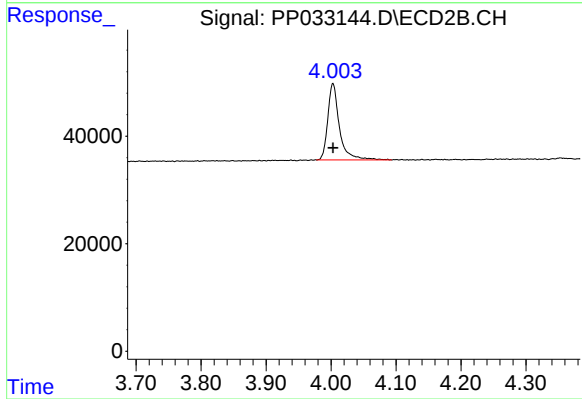


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: 0.000 min
Response: 176459
Conc: 4.29 ng/ml

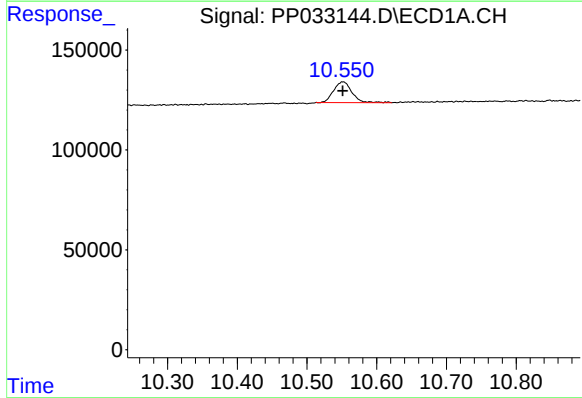


#2 Decachlorobiphenyl

R.T.: 10.551 min
Delta R.T.: 0.000 min
Response: 188010
Conc: 4.32 ng/ml

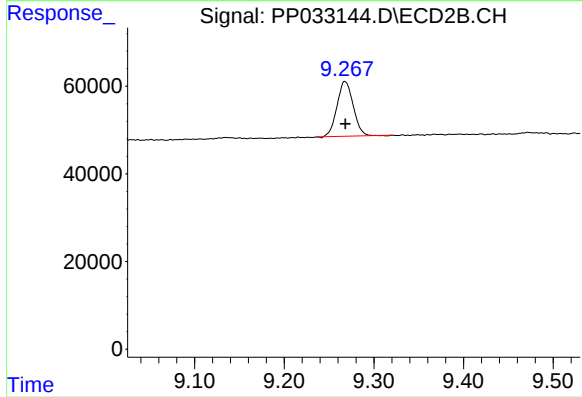

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 156370
Conc: 4.57 ng/ml

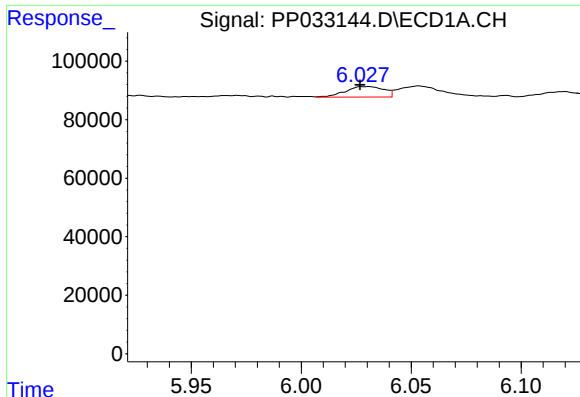


#21 AR-1248-1

R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 44783
Conc: 46.92 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:44 AM

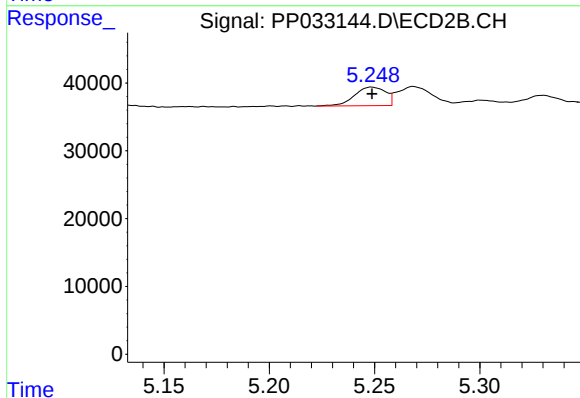


#21 AR-1248-1

R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 28369
Conc: 43.62 ng/ml

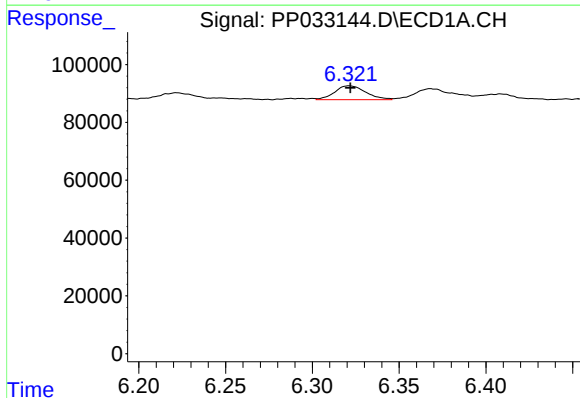


#22 AR-1248-2

R.T.: 6.321 min
Delta R.T.: -0.001 min
Response: 59439
Conc: 44.20 ng/ml m

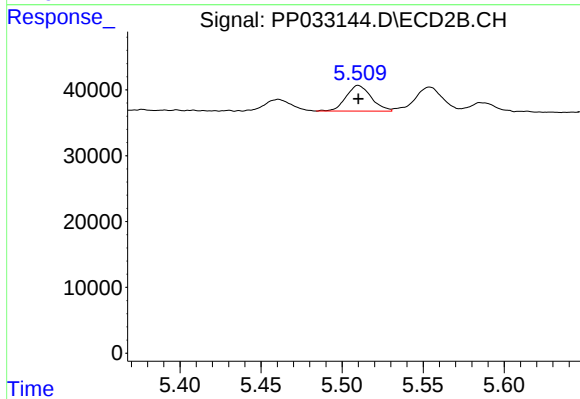

#22 AR-1248-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 42343
Conc: 44.14 ng/ml

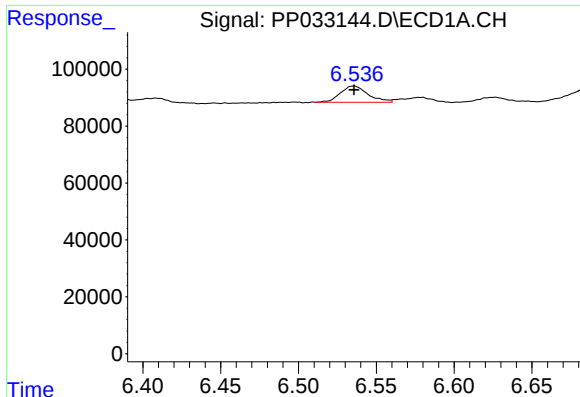


#23 AR-1248-3

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 70513
Conc: 43.16 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:44 AM

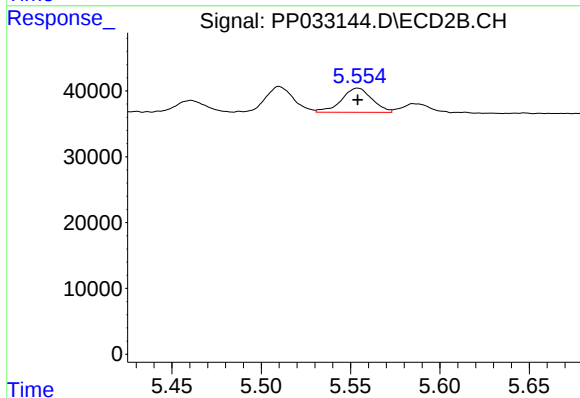


#23 AR-1248-3

R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 44026
Conc: 43.30 ng/ml

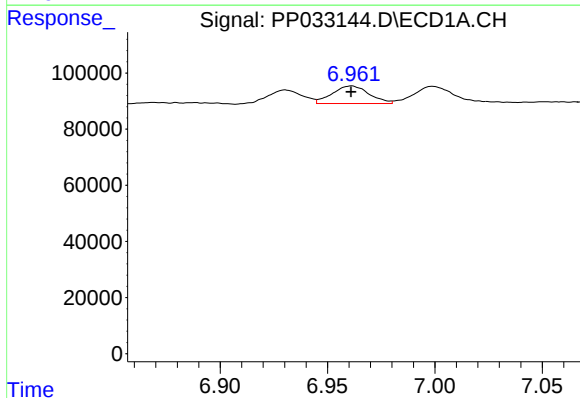


#24 AR-1248-4

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 74521
Conc: 43.27 ng/ml m

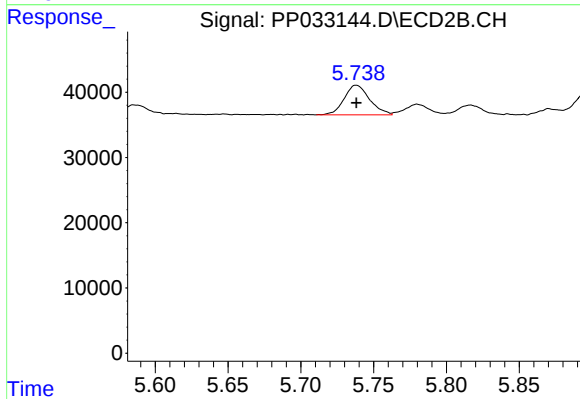

#24 AR-1248-4

R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 55120
Conc: 44.48 ng/ml

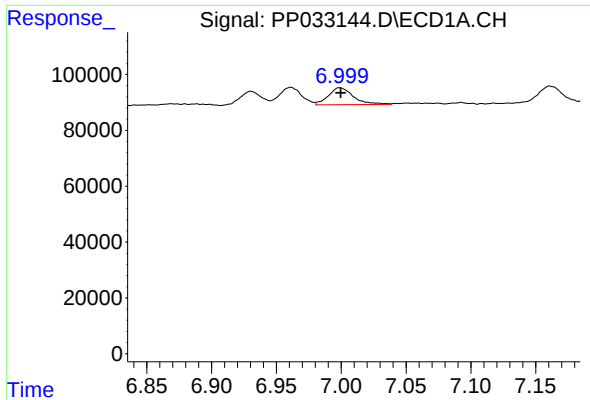


#25 AR-1248-5

R.T.: 7.000 min
Delta R.T.: 0.000 min
Response: 82452
Conc: 47.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Ankita
2/9/2021 10:50:44 AM

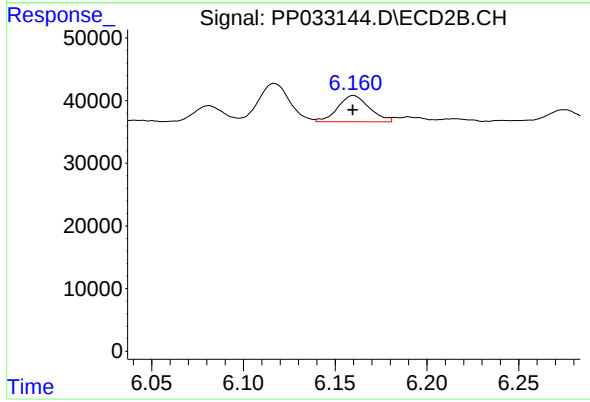

#25 AR-1248-5

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 49943
Conc: 44.30 ng/ml m