

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
 Data File : PP033162.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2021 21:51
 Operator : DD\AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP020821AR1248

Manual Integrations
 APPROVED

Ankita
 2/9/2021 10:51:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:15:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 02:14:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.729	4.001	3005878	2043841	48.795	49.645
2) SA Decachlor...	10.550	9.268	2182480	1712493	50.151	50.090
Target Compounds						
21) L5 AR-1248-1	6.028	5.248	466846	331585	487.586	509.866
22) L5 AR-1248-2	6.320	5.509	635235	480786	479.397m	501.154
23) L5 AR-1248-3	6.535	5.553	789256	512772	487.411	504.322
24) L5 AR-1248-4	6.959	5.737	854901	609683	496.850	491.967
25) L5 AR-1248-5	6.999	6.159	839421	570762	482.425	505.398

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020821\
Data File : PP033162.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2021 21:51
Operator : DD\AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ICVPP020821AR1248


Manual Integrations
APPROVED

Ankita
2/9/2021 10:51:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:15:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 02:14:37 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

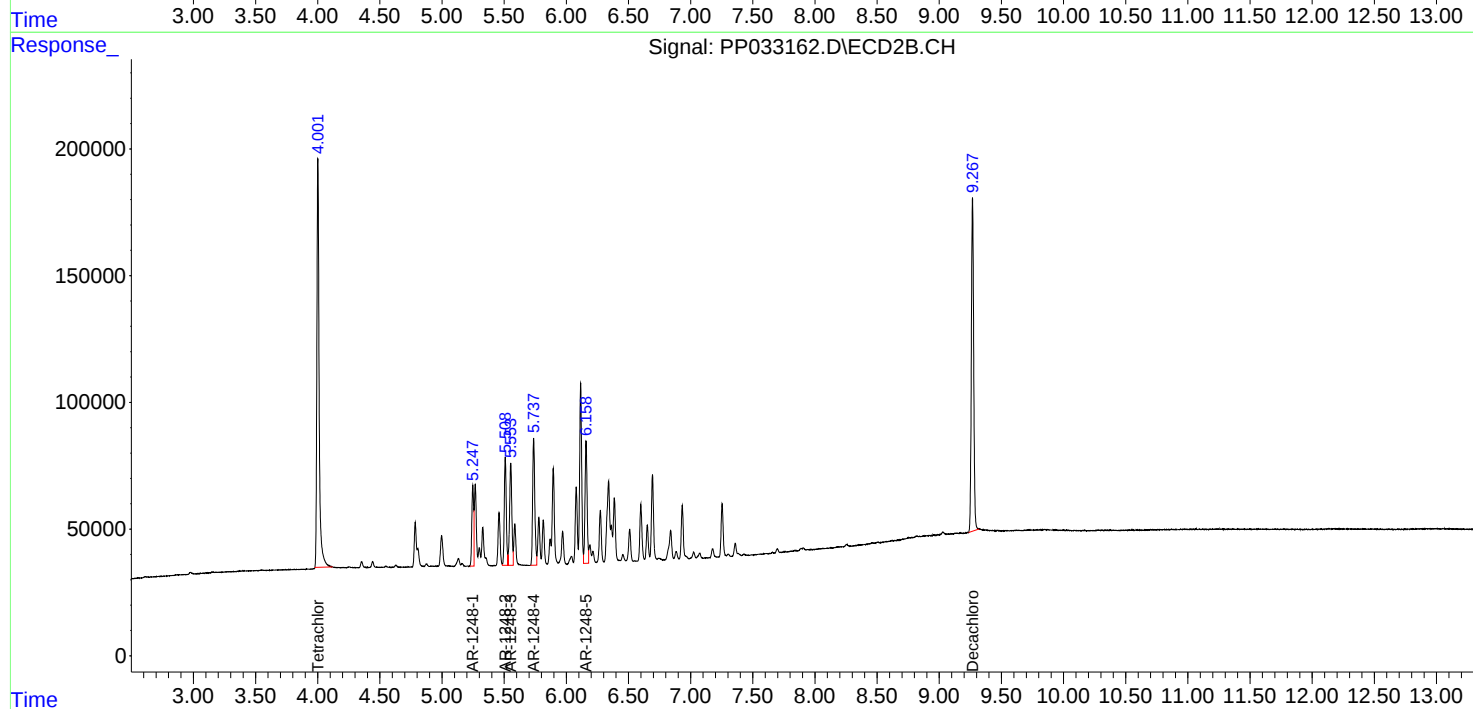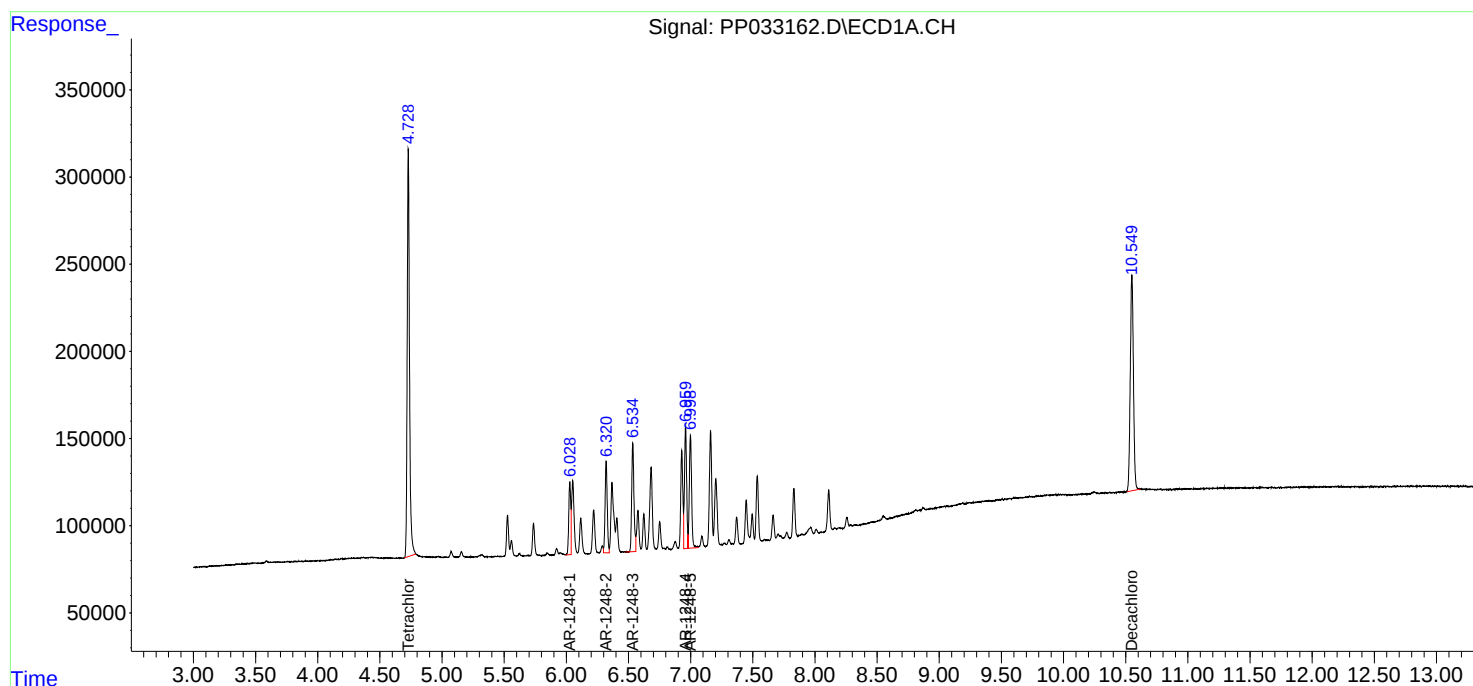

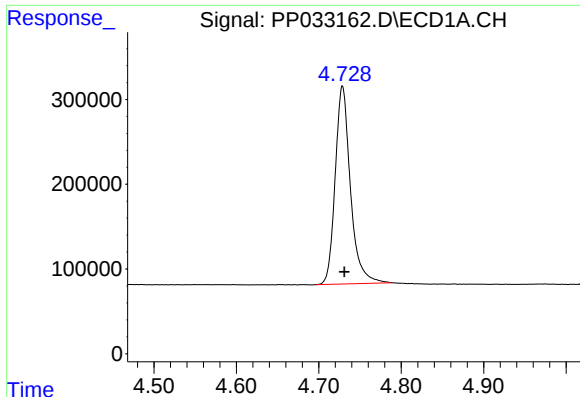


#1 Tetrachloro-m-xylene

R.T.: 4.729 min
Delta R.T.: -0.002 min
Response: 3005878
Conc: 48.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP020821AR1248


Manual Integrations
APPROVED

Ankita
2/9/2021 10:51:11 AM

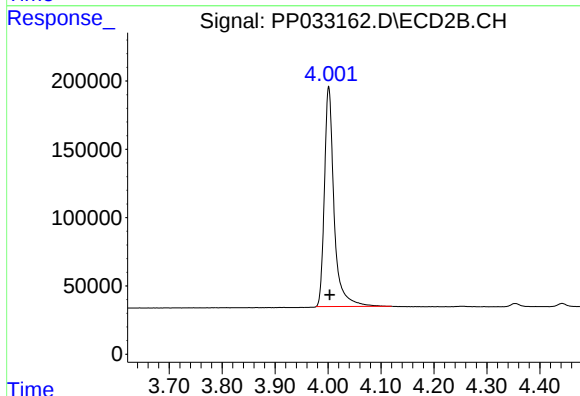


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.002 min
Response: 2043841
Conc: 49.64 ng/ml

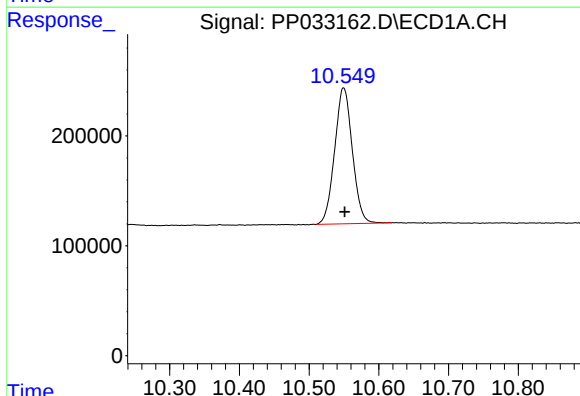


#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: -0.002 min
Response: 2182480
Conc: 50.15 ng/ml

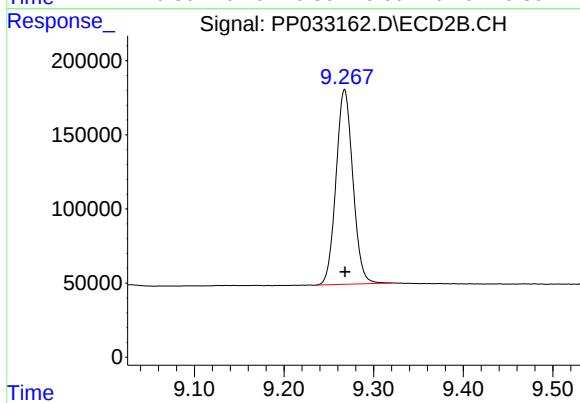

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 1712493
Conc: 50.09 ng/ml

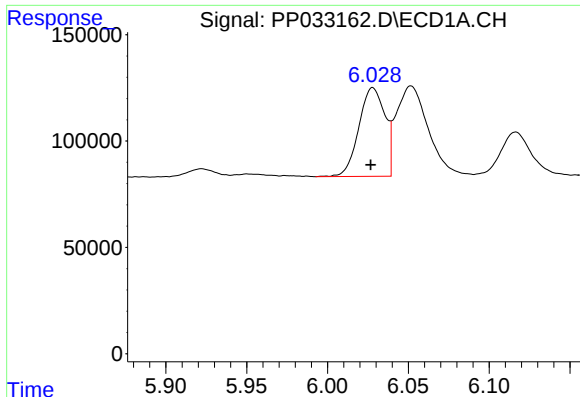


#21 AR-1248-1

R.T.: 6.028 min
Delta R.T.: 0.001 min
Response: 466846
Conc: 487.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP020821AR1248


Manual Integrations
APPROVED

Ankita
2/9/2021 10:51:11 AM

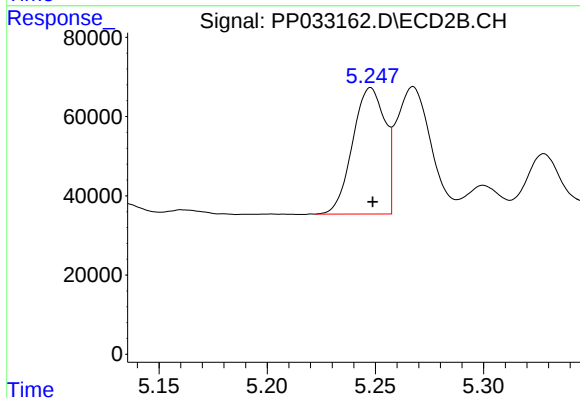


#21 AR-1248-1

R.T.: 5.248 min
Delta R.T.: 0.000 min
Response: 331585
Conc: 509.87 ng/ml

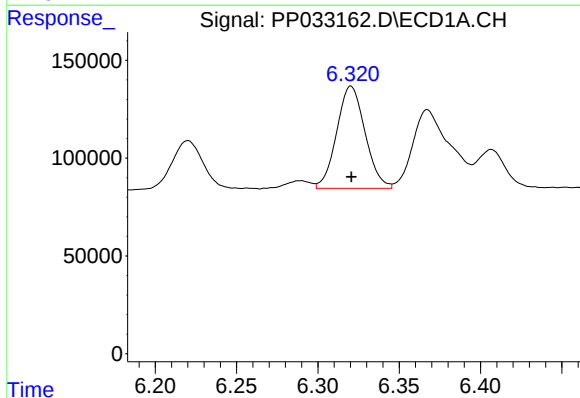


#22 AR-1248-2

R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 635235
Conc: 479.40 ng/ml m

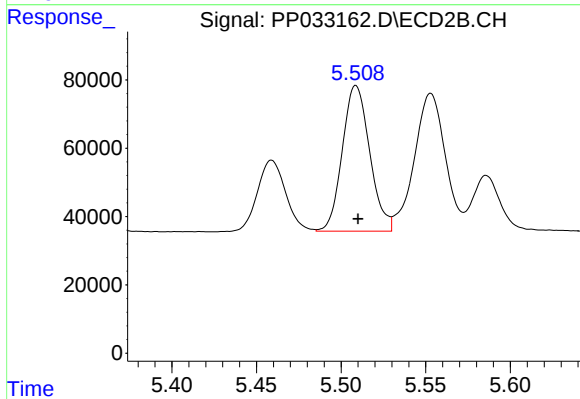

#22 AR-1248-2

R.T.: 5.509 min
Delta R.T.: -0.001 min
Response: 480786
Conc: 501.15 ng/ml

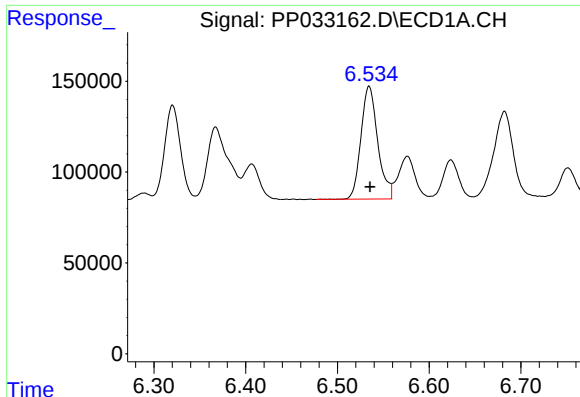


#23 AR-1248-3

R.T.: 6.535 min
Delta R.T.: -0.001 min
Response: 789256
Conc: 487.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP020821AR1248


Manual Integrations
APPROVED

Ankita
2/9/2021 10:51:11 AM

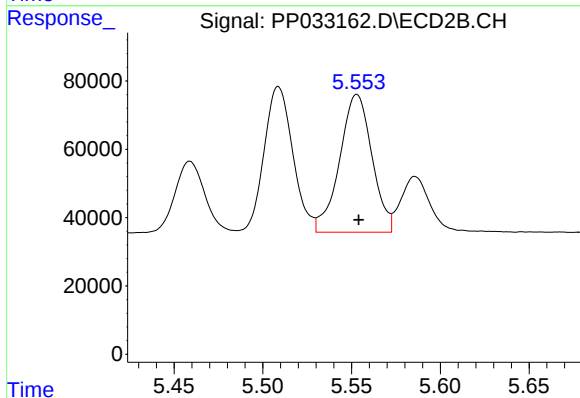


#23 AR-1248-3

R.T.: 5.553 min
Delta R.T.: -0.001 min
Response: 512772
Conc: 504.32 ng/ml

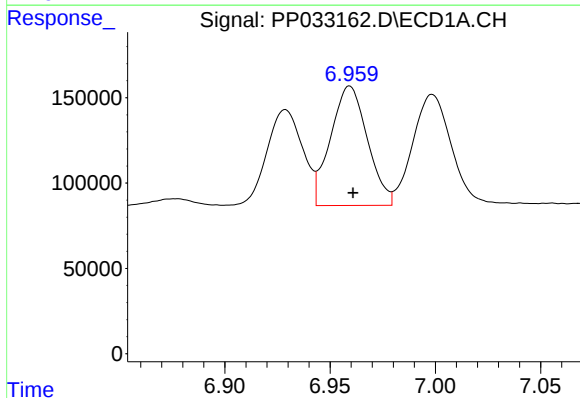


#24 AR-1248-4

R.T.: 6.959 min
Delta R.T.: -0.002 min
Response: 854901
Conc: 496.85 ng/ml

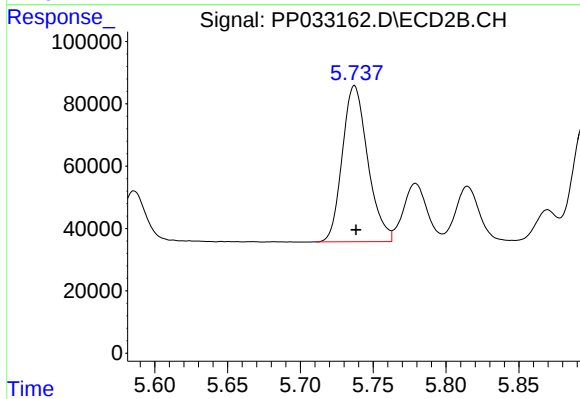

#24 AR-1248-4

R.T.: 5.737 min
Delta R.T.: 0.000 min
Response: 609683
Conc: 491.97 ng/ml

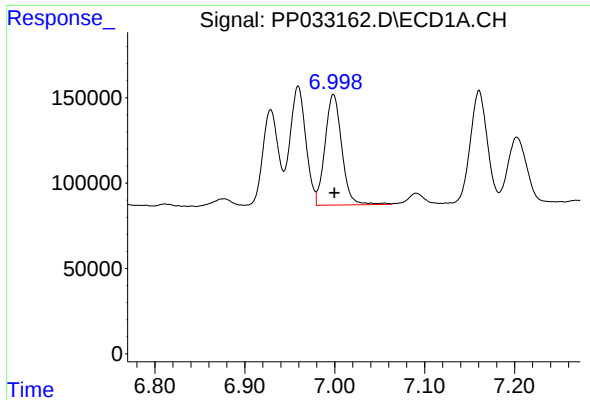


#25 AR-1248-5

R.T.: 6.999 min
Delta R.T.: -0.001 min
Response: 839421
Conc: 482.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
ICVPP020821AR1248

Manual Integrations
APPROVED

Ankita
2/9/2021 10:51:11 AM

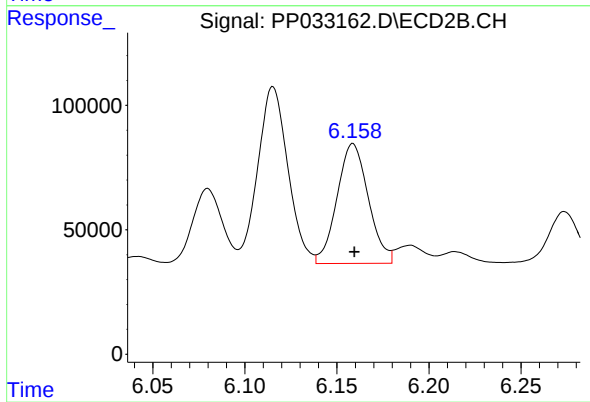

#25 AR-1248-5

R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 570762
Conc: 505.40 ng/ml