

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020822\
 Data File : PP043538.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2022 8:51
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:47:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 10:01:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	0.000	6.192f	0	32021	N.D. 51.590 #
25)	L5	AR-1248-5	0.000	6.192f	0	32021	N.D. 36.691 #
26)	L6	AR-1254-1	0.000	6.192f	0	32021	N.D. 23.904 #
28)	L6	AR-1254-3	0.000	6.763f	0	13983	N.D. 7.596 #
30)	L6	AR-1254-5	8.378f	0.000	5690	0	6.130 N.D. #
36)	L8	AR-1262-1	8.509f	0.000	5939	0	5.489 N.D. #
40)	L8	AR-1262-5	0.000	8.849f	0	18050	N.D. 20.977 #
43)	L9	AR-1268-3	0.000	8.536	0	23874	N.D. 10.193 #
44)	L9	AR-1268-4	0.000	8.849f	0	18050	N.D. 18.241 #
45)	L9	AR-1268-5	10.473f	0.000	9368	0	1.691 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020822\
Data File : PP043538.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2022 8:51
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:47:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 10:01:05 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

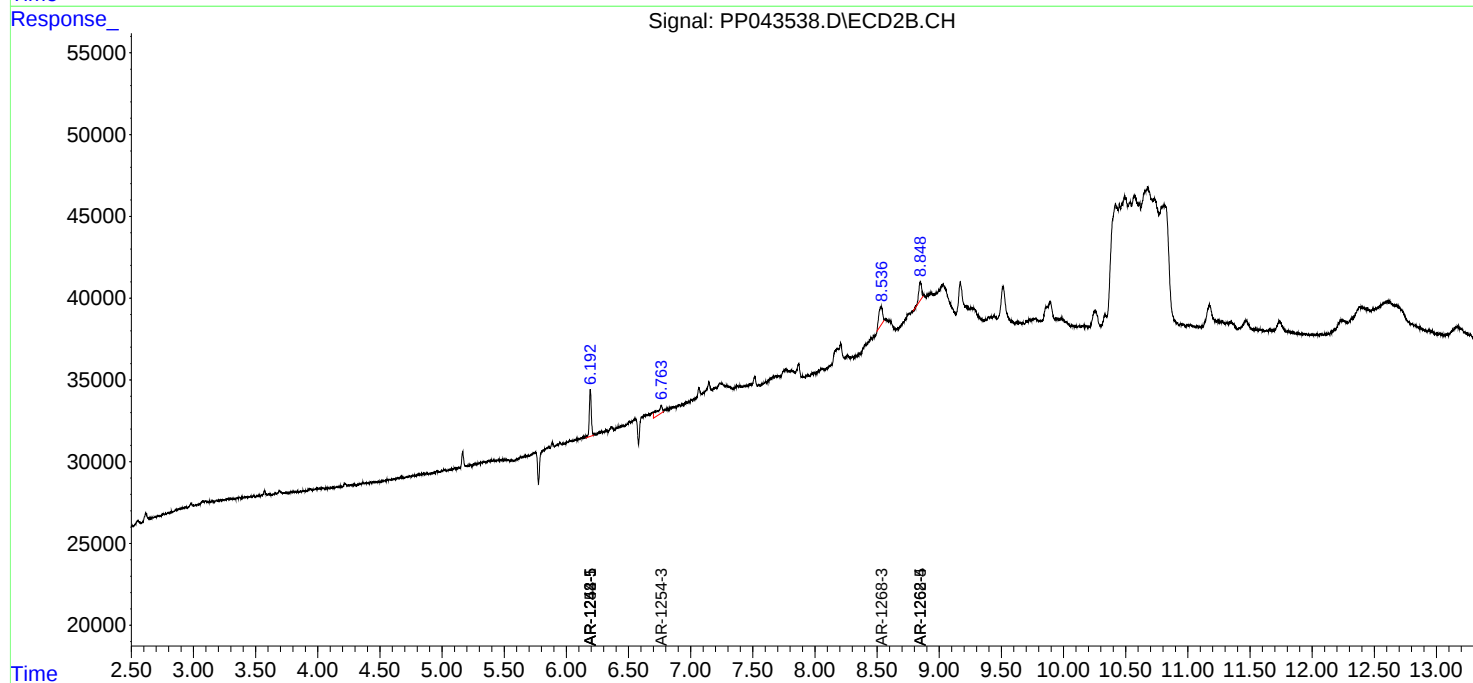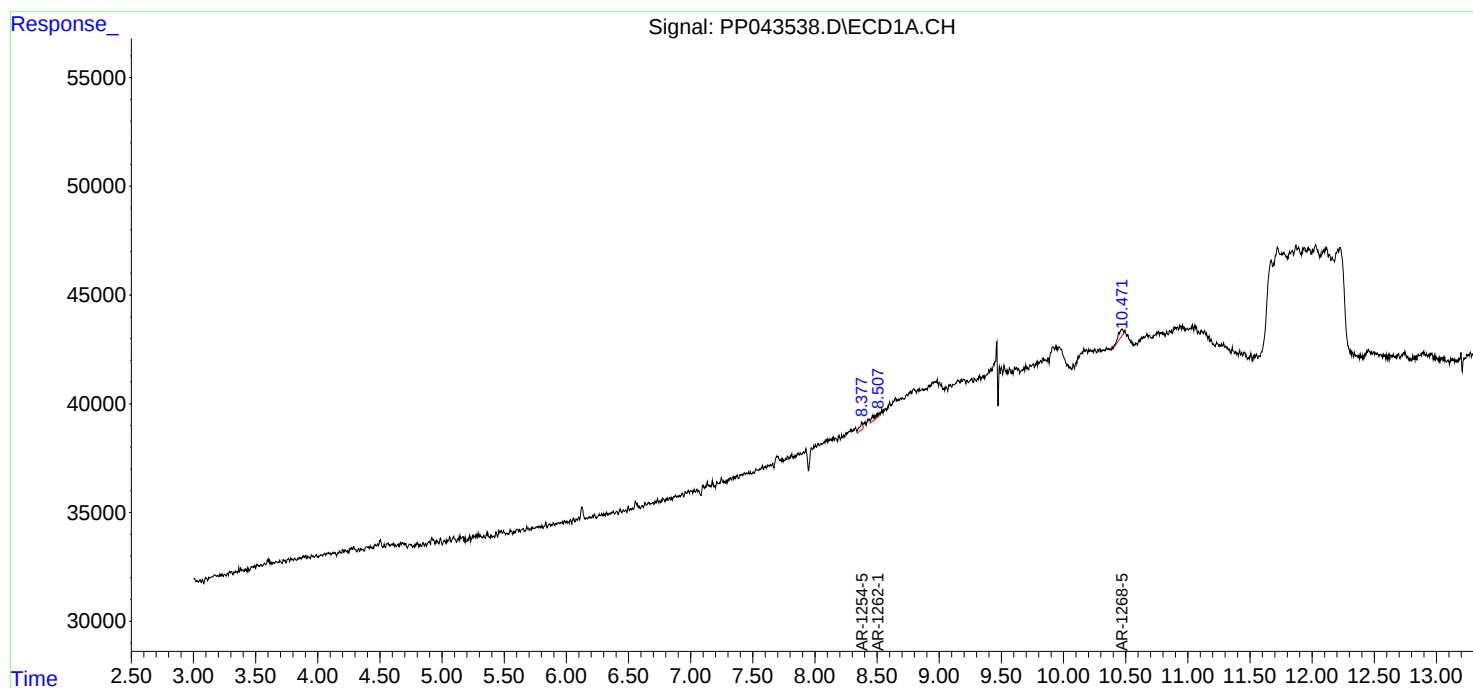


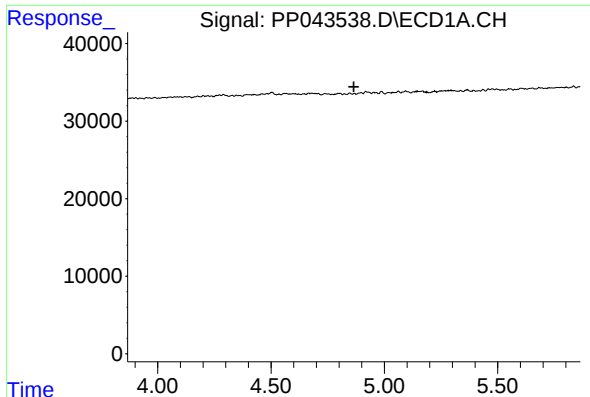

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

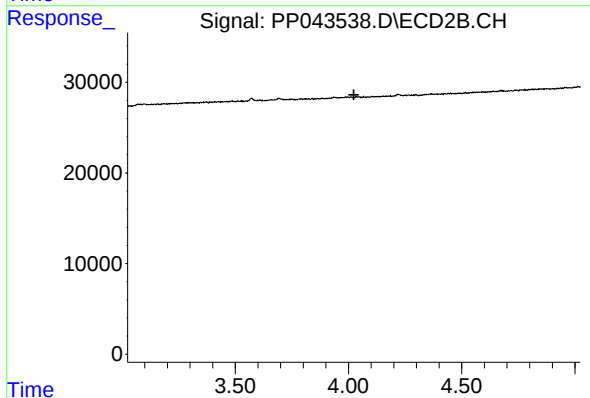


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

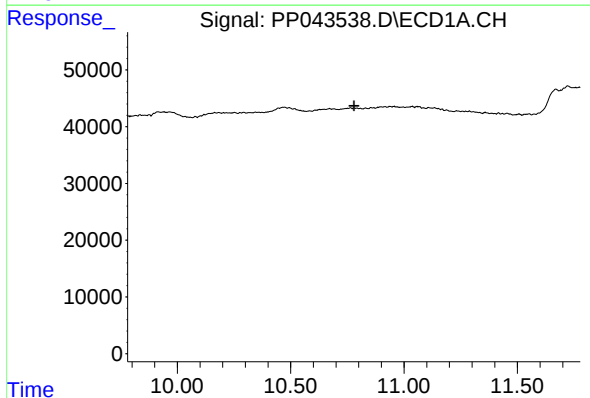


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.779 min
Response: 0
Conc: N.D.

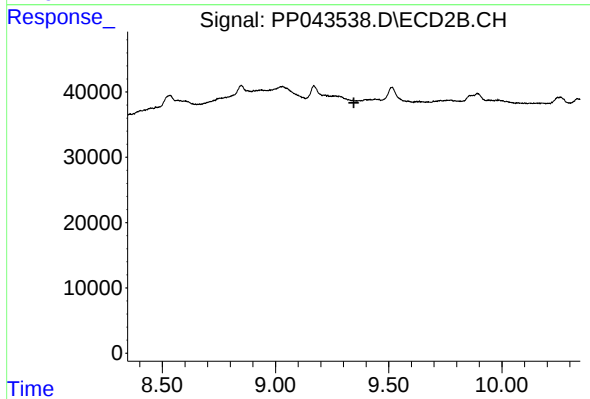

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.347 min
Response: 0
Conc: N.D.

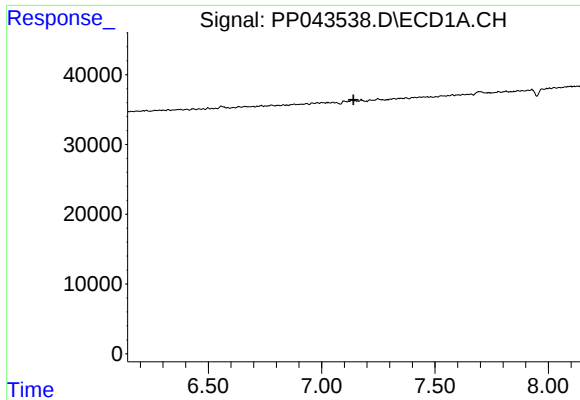

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

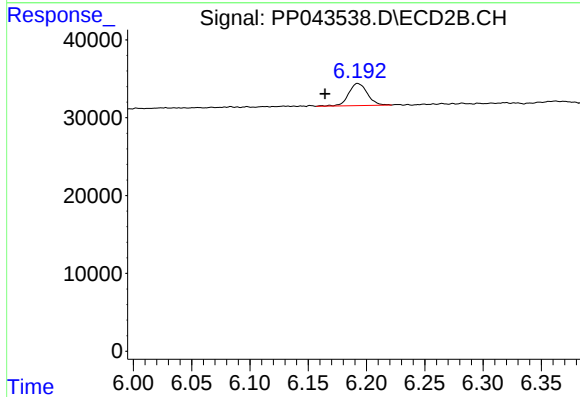


#20 AR-1242-5

R.T.: 6.192 min
Delta R.T.: 0.028 min
Response: 32021
Conc: 51.59 ng/ml

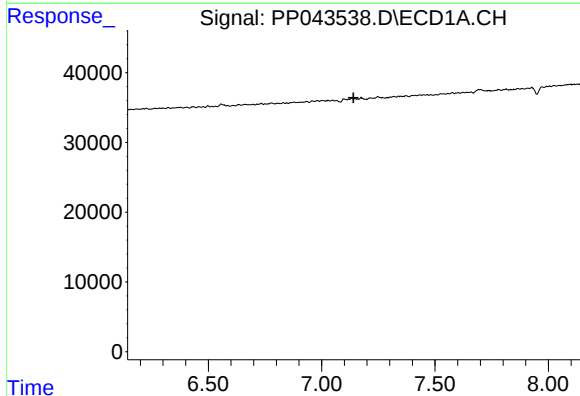


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.141 min
Response: 0
Conc: N.D.

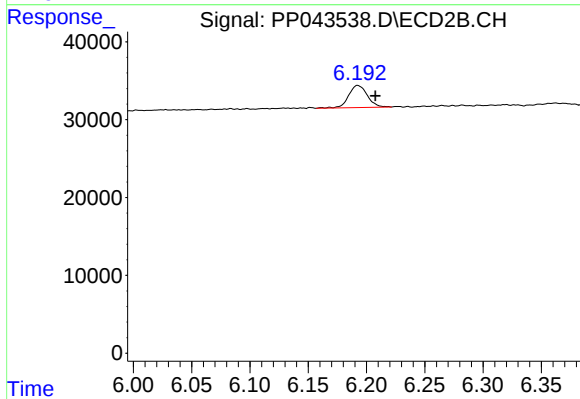

#25 AR-1248-5


R.T.: 6.192 min
Delta R.T.: -0.015 min
Response: 32021
Conc: 36.69 ng/ml

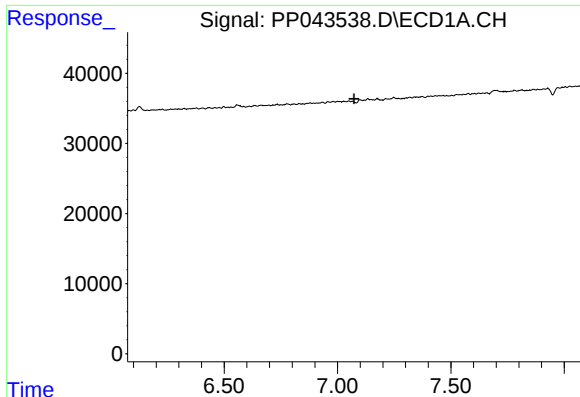

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

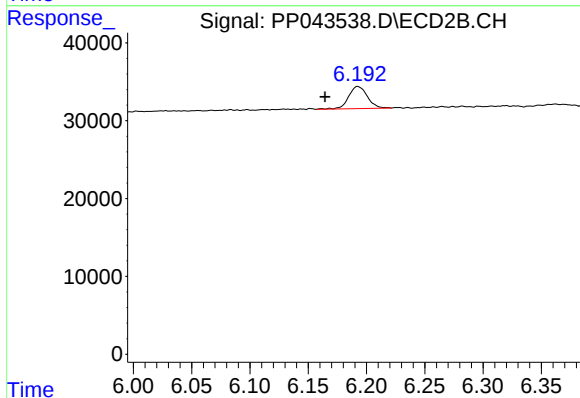


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: 0.028 min
Response: 32021
Conc: 23.90 ng/ml

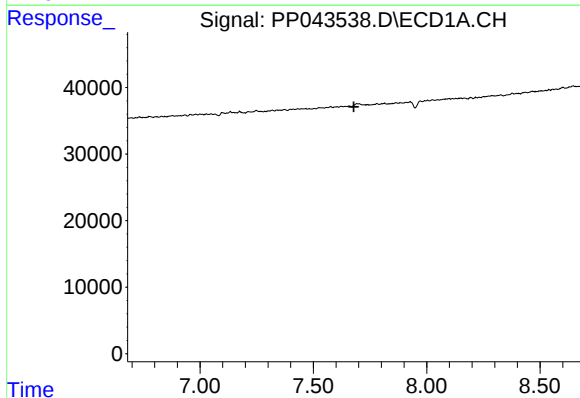


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 7.679 min
Response: 0
Conc: N.D.

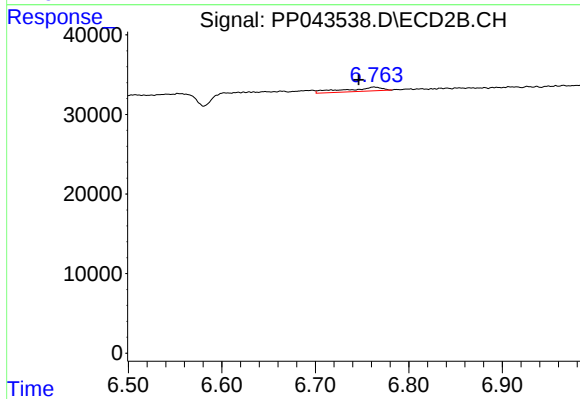

#28 AR-1254-3


R.T.: 6.763 min
Delta R.T.: 0.016 min
Response: 13983
Conc: 7.60 ng/ml

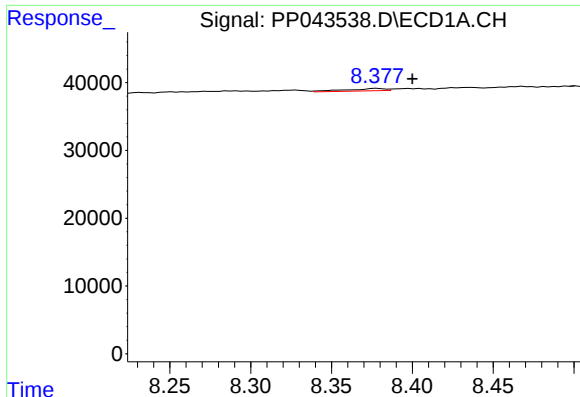

#30 AR-1254-5


R.T.: 8.378 min
Delta R.T.: -0.022 min
Response: 5690
Conc: 6.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

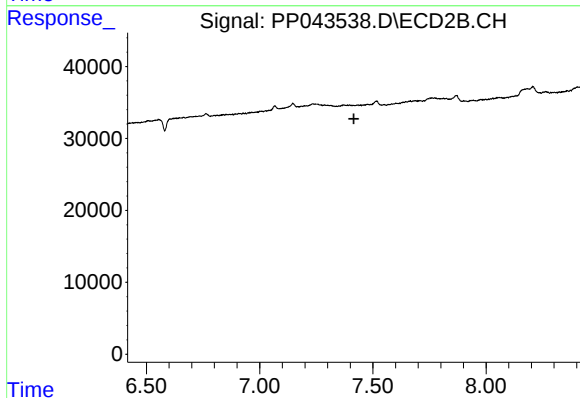


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.416 min
Response: 0
Conc: N.D.

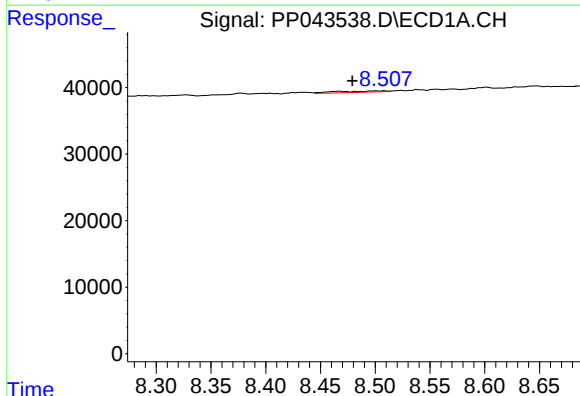


#36 AR-1262-1

R.T.: 8.509 min
Delta R.T.: 0.030 min
Response: 5939
Conc: 5.49 ng/ml

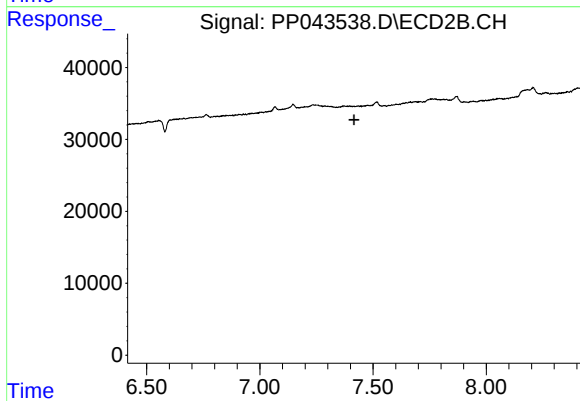

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.416 min
Response: 0
Conc: N.D.

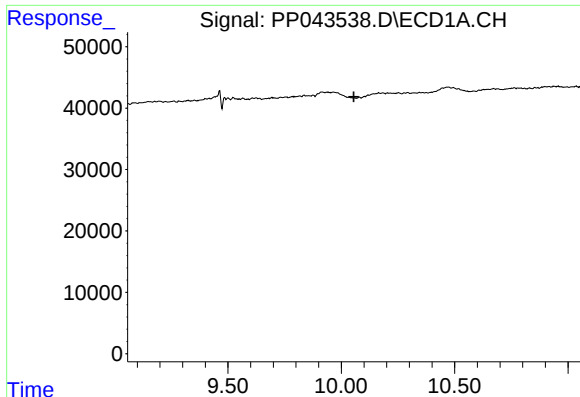

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.055 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

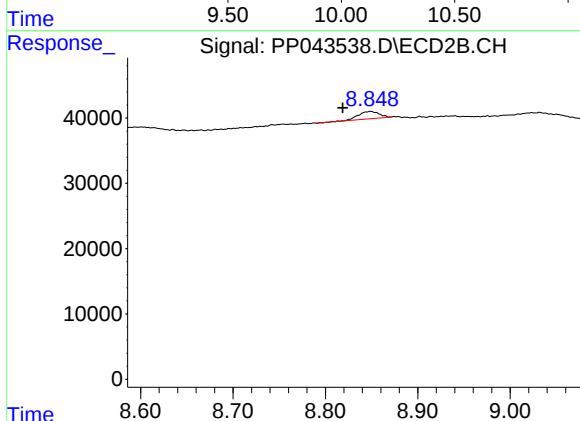


#40 AR-1262-5

R.T.: 8.849 min
Delta R.T.: 0.030 min
Response: 18050
Conc: 20.98 ng/ml

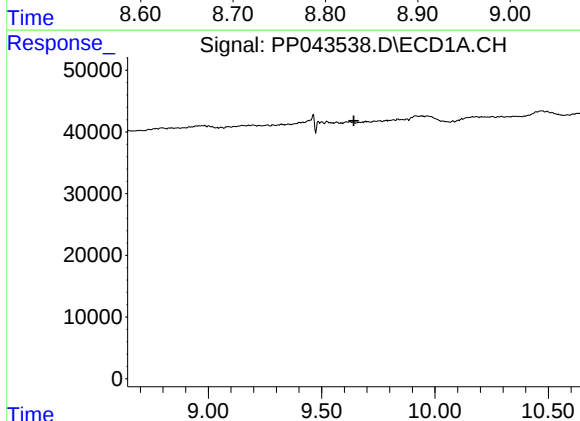


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.641 min
Response: 0
Conc: N.D.

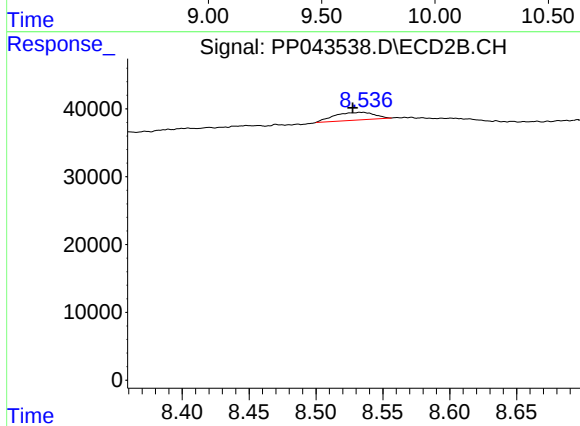

#43 AR-1268-3


R.T.: 8.536 min
Delta R.T.: 0.008 min
Response: 23874
Conc: 10.19 ng/ml

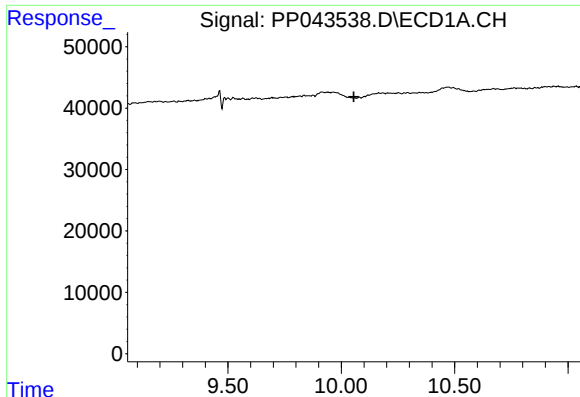

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 10.056 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

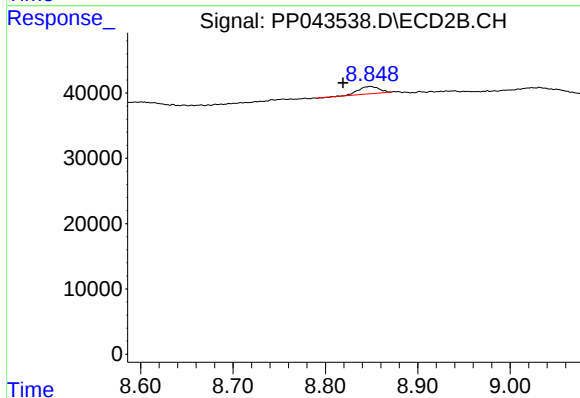


#44 AR-1268-4

R.T.: 8.849 min
Delta R.T.: 0.030 min
Response: 18050
Conc: 18.24 ng/ml

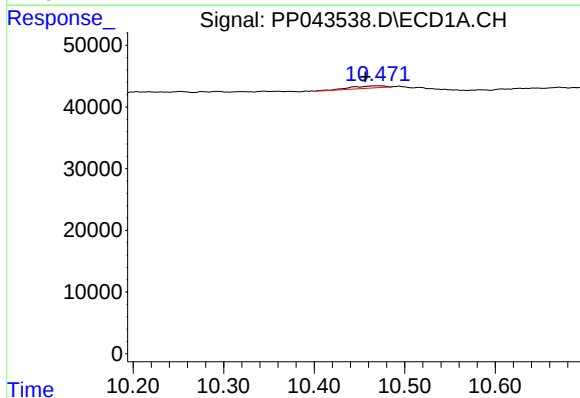

#45 AR-1268-5

R.T.: 10.473 min
Delta R.T.: 0.016 min
Response: 9368
Conc: 1.69 ng/ml

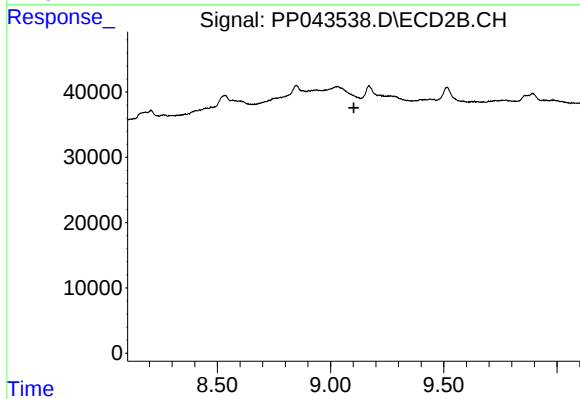

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.103 min
Response: 0
Conc: N.D.