

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020822\
 Data File : PP043541.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2022 10:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:48:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 03 10:01:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.866	4.026	423387	395723	15.427	17.472
2) SA Decachlor...	10.783	9.348	308559	412635	20.115	21.827
Target Compounds						
38) L8 AR-1262-3	0.000	8.225f	0	7798	N.D.	8.215 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020822\
Data File : PP043541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2022 10:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:48:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 03 10:01:05 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

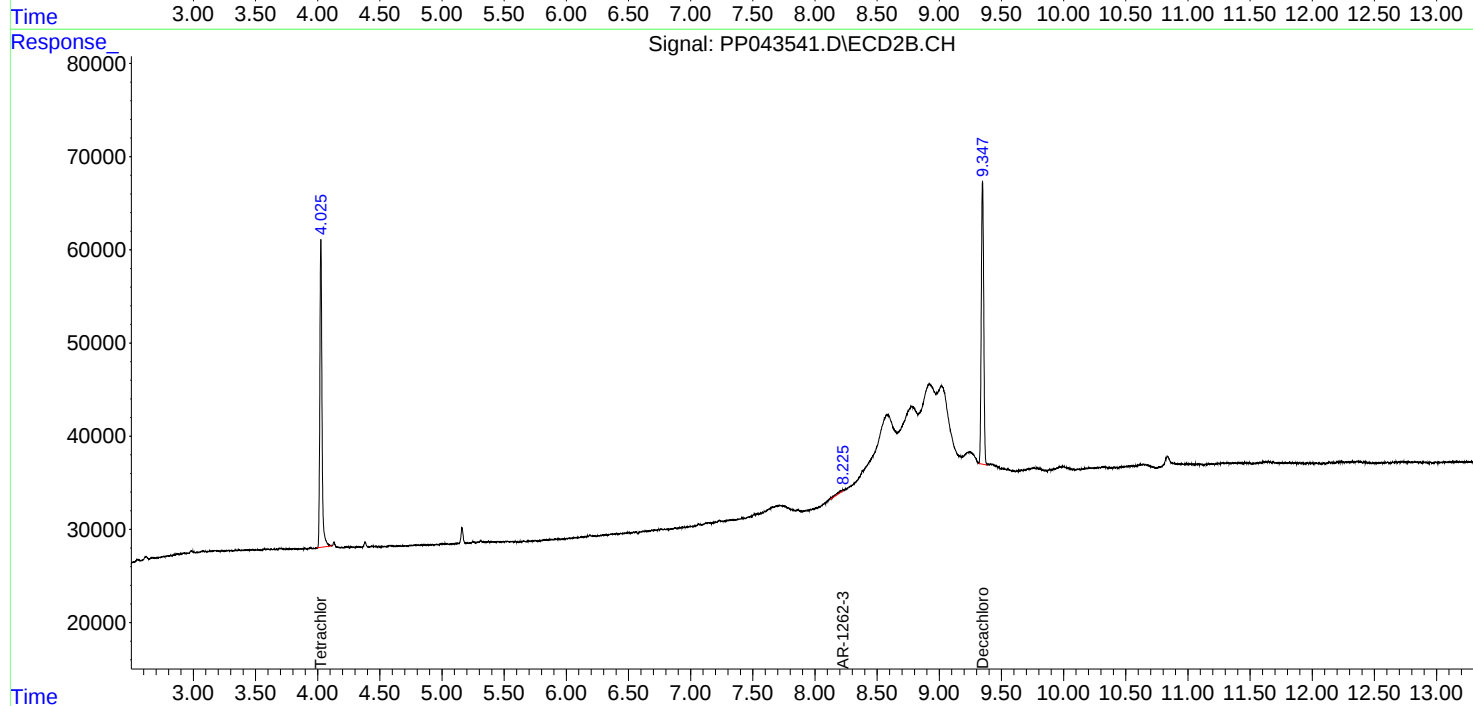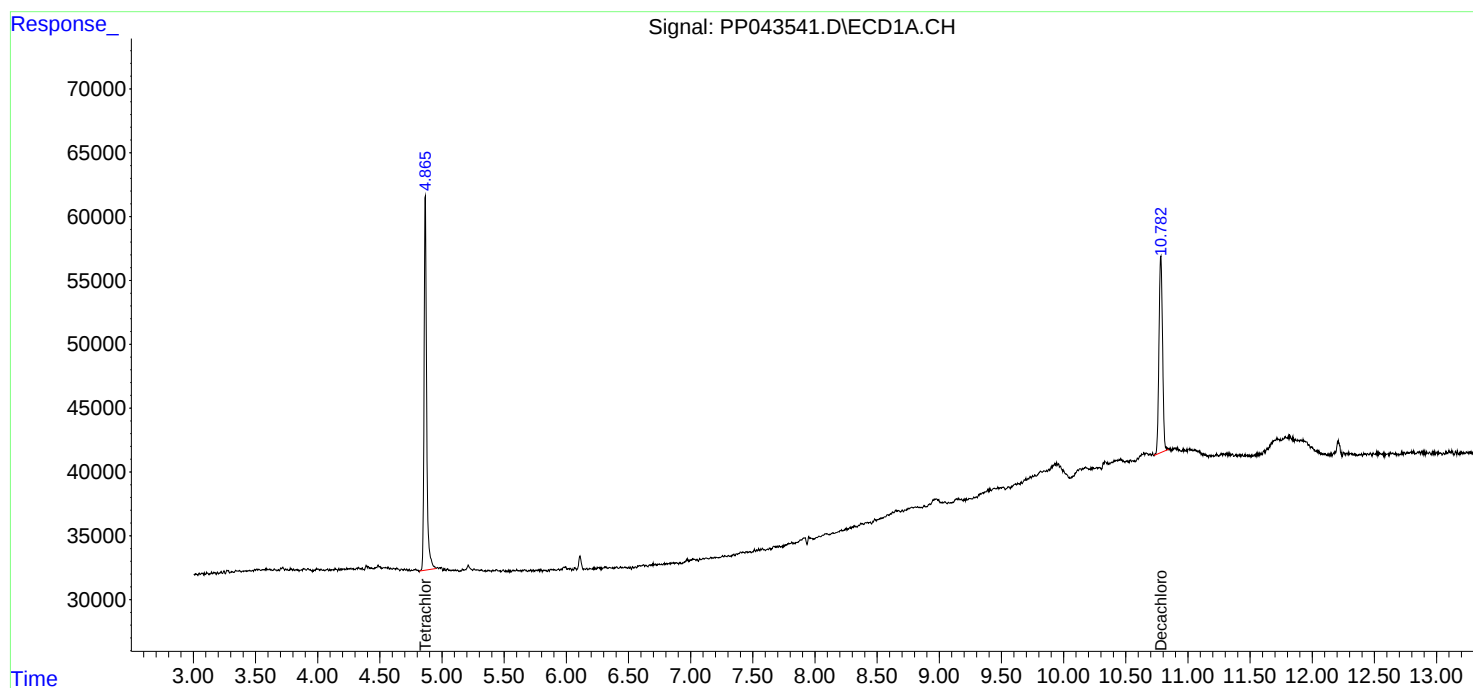


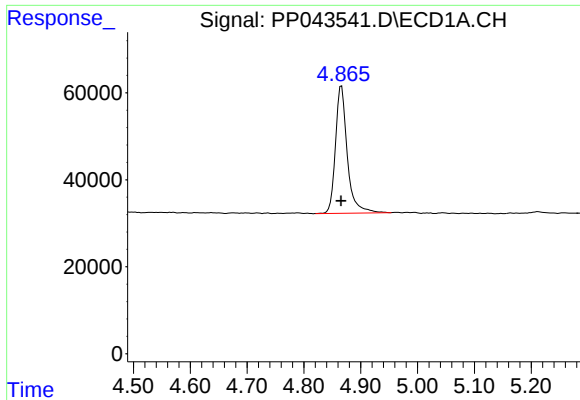

#1 Tetrachloro-m-xylene


R.T.: 4.866 min
Delta R.T.: 0.001 min
Response: 423387
Conc: 15.43 ng/ml

Instrument :
ECD_P
ClientSampleId :

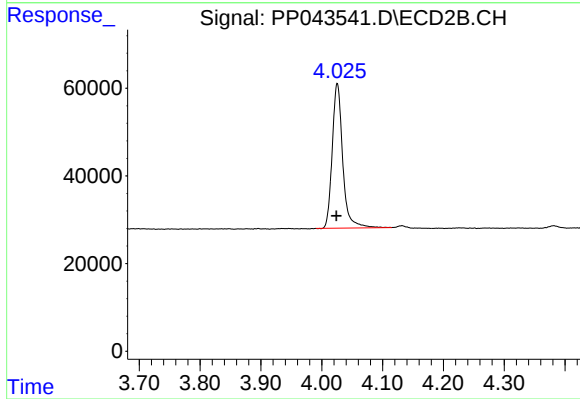


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.002 min
Response: 395723
Conc: 17.47 ng/ml

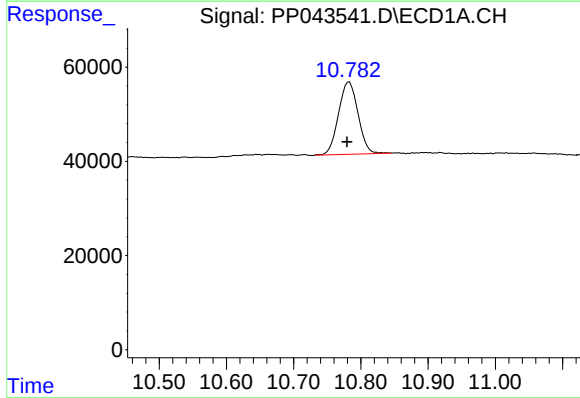


#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: 0.003 min
Response: 308559
Conc: 20.11 ng/ml

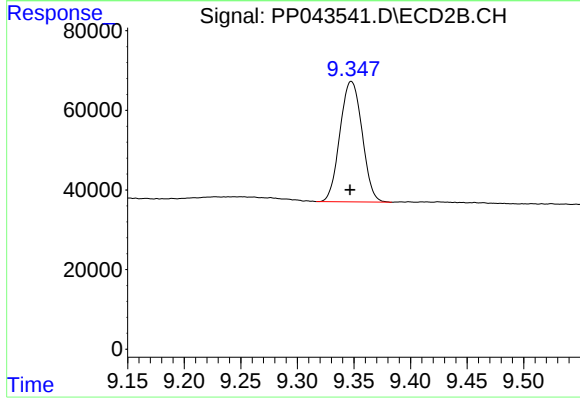

#2 Decachlorobiphenyl


R.T.: 9.348 min
Delta R.T.: 0.001 min
Response: 412635
Conc: 21.83 ng/ml

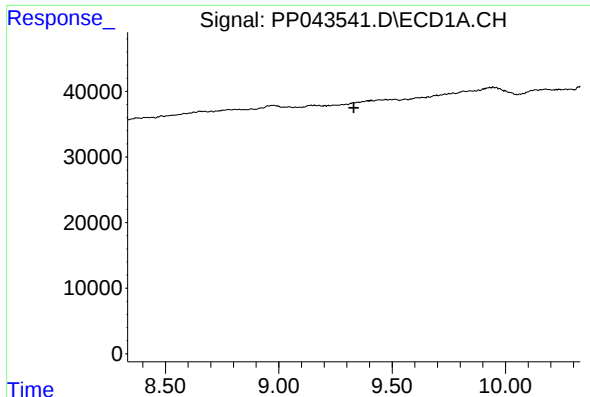

#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

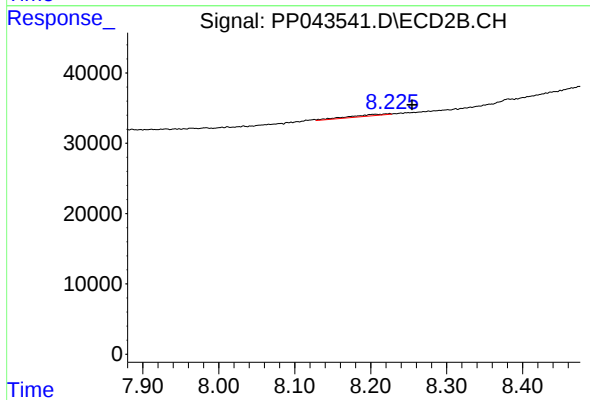

#38 AR-1262-3

R.T.: 8.225 min
Delta R.T.: -0.029 min
Response: 7798
Conc: 8.22 ng/ml