

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020823\
 Data File : PP055469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 19:38
 Operator : YP\AJ
 Sample : 01473-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 005

Manual Integrations
 APPROVED

Reviewed By :Ankita
 Jodhani

02/09/2023
 Supervised By :Sohil
 Jodhani

02/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 22:10:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.339	3.592	22100011	20464768	12.710m	13.632
2) SA Decachlor...	10.078	8.582	35266944	27309649	20.366	20.221

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020823\
Data File : PP055469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 19:38
Operator : YP\AJ
Sample : 01473-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
005

Manual Integrations
APPROVED



Reviewed By :Ankita
Jodhani


02/09/2023
Supervised By :Sohil
Jodhani

02/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 22:10:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

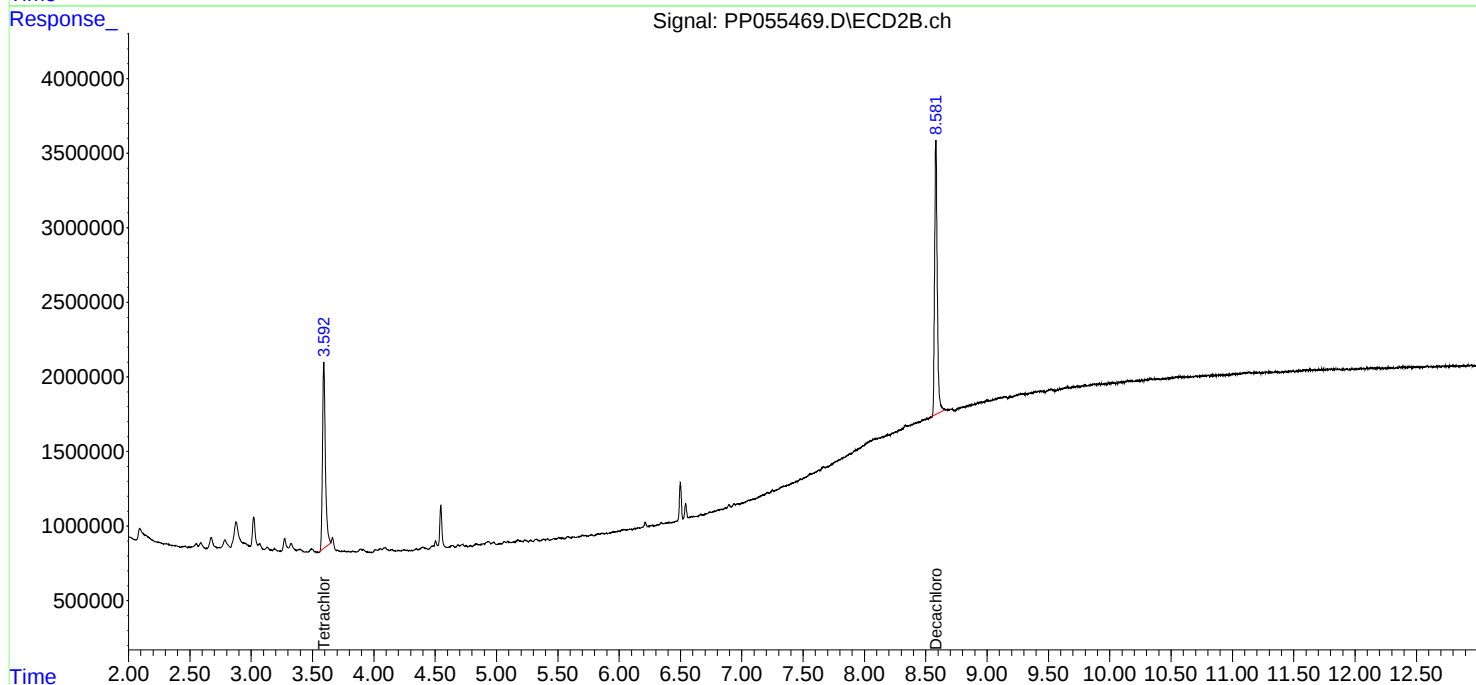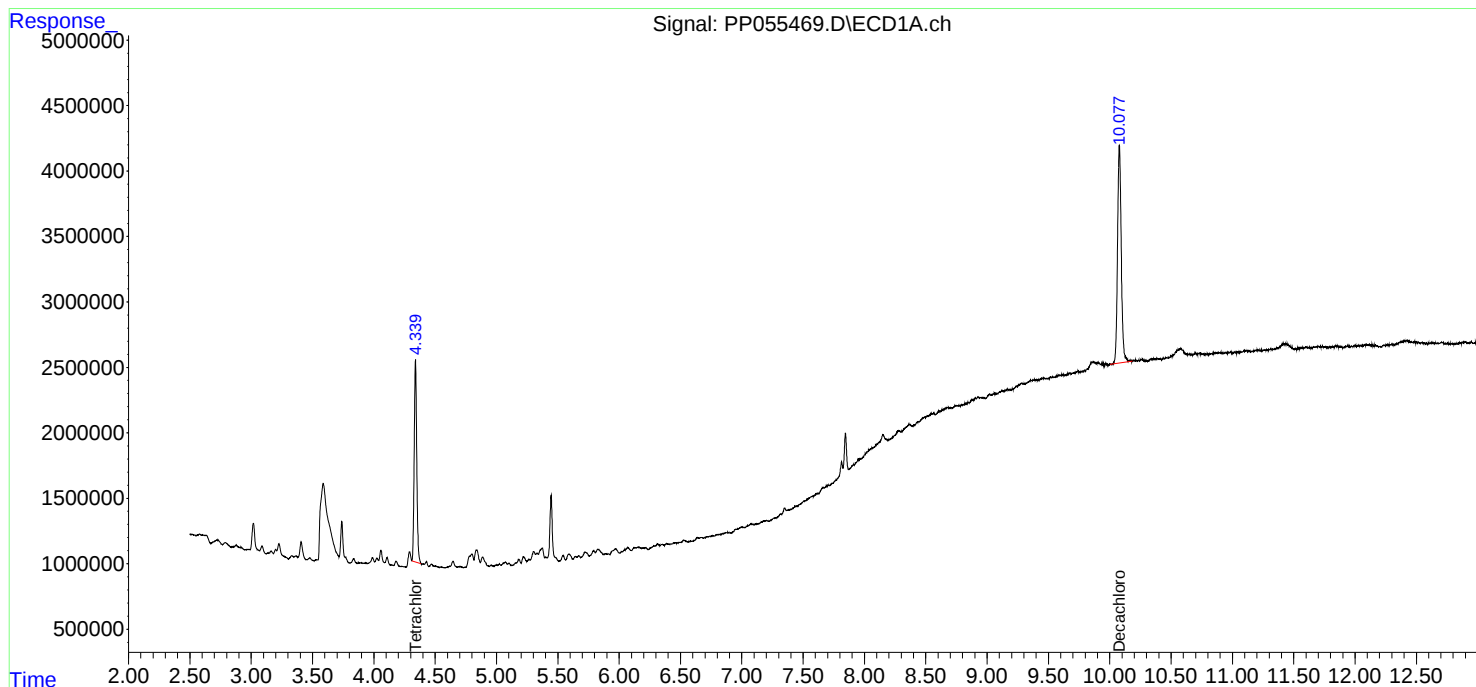

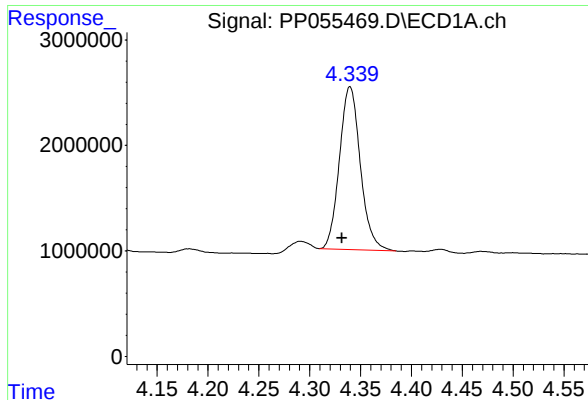

#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: 0.007 min
Response: 22100011
Conc: 12.71 ng/ml


Instrument :
ECD_P
ClientSampleId :
005

Manual Integrations
APPROVED

Reviewed By :Ankita
Jodhani


02/09/2023
Supervised By :Sohil
Jodhani

02/09/2023

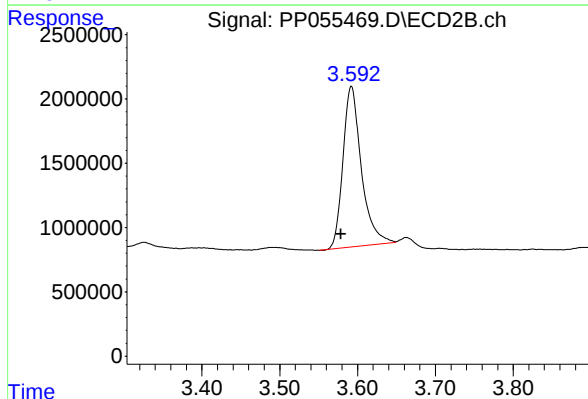


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.014 min
Response: 20464768
Conc: 13.63 ng/ml

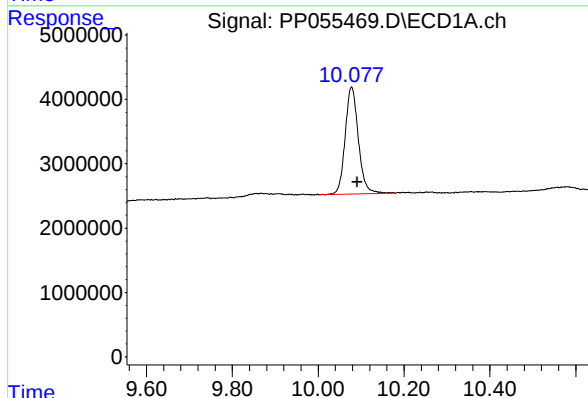

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: -0.013 min
Response: 35266944
Conc: 20.37 ng/ml

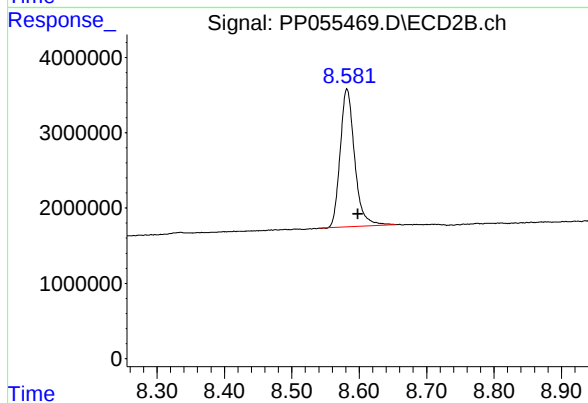

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.016 min
Response: 27309649
Conc: 20.22 ng/ml