

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020921\
 Data File : PP033199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Feb 2021 21:36
 Operator : DD\AJ
 Sample : M1260-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WOOSPK-073-0204

Manual Integrations
 APPROVED

Ankita
 2/10/2021 1:56:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 05:16:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.731	4.003	1133277	919690	18.481	22.491m
2) SA Decachlor...	10.552	9.269	657829	728455	15.101	21.745 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020921\
Data File : PP033199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Feb 2021 21:36
Operator : DD\AJ
Sample : M1260-12
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WOOSPK-073-0204


Manual Integrations
APPROVED

Ankita
2/10/2021 1:56:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 05:16:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

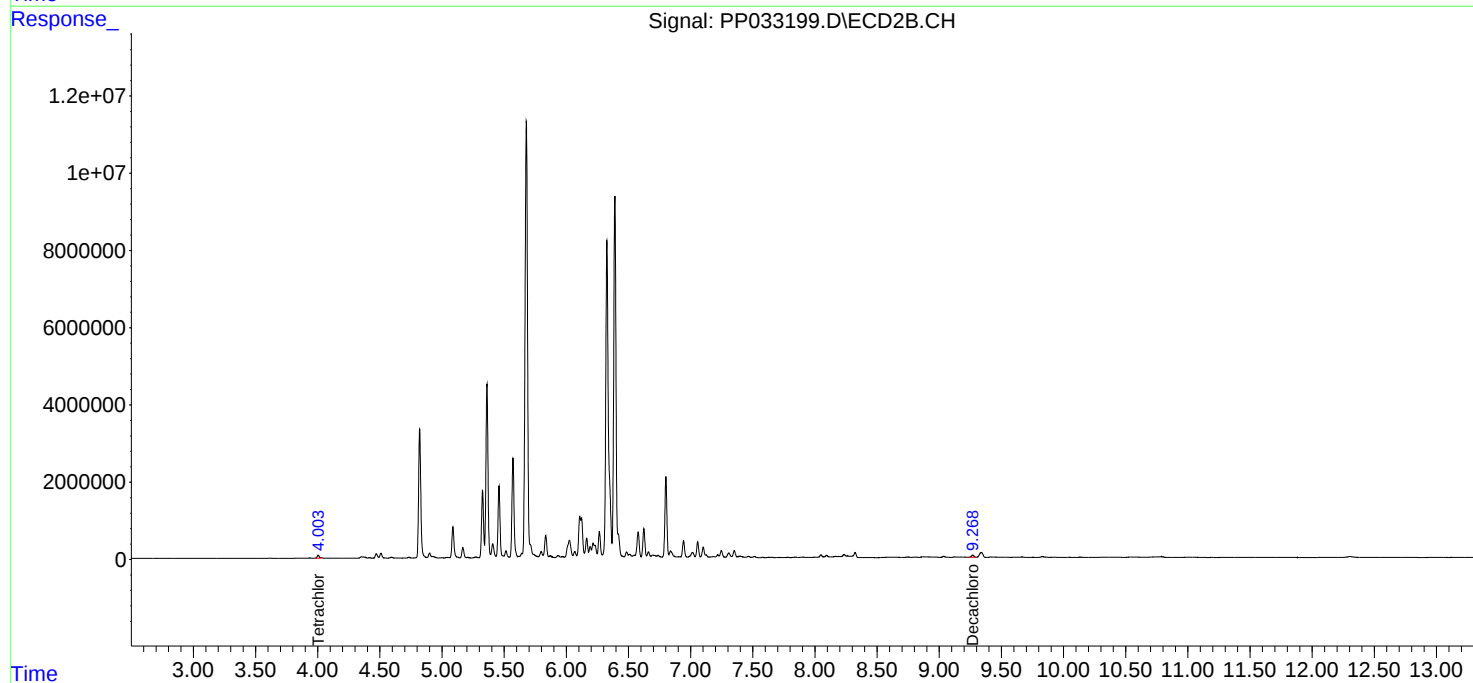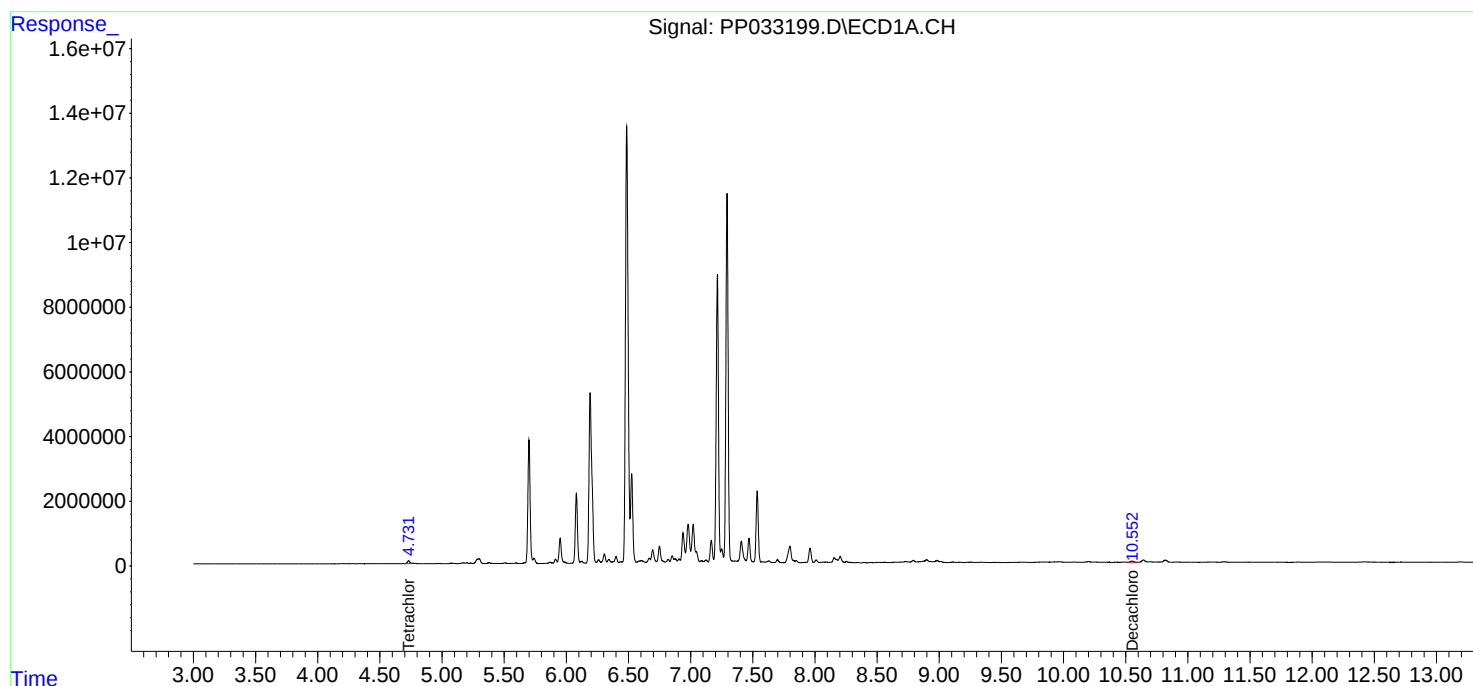

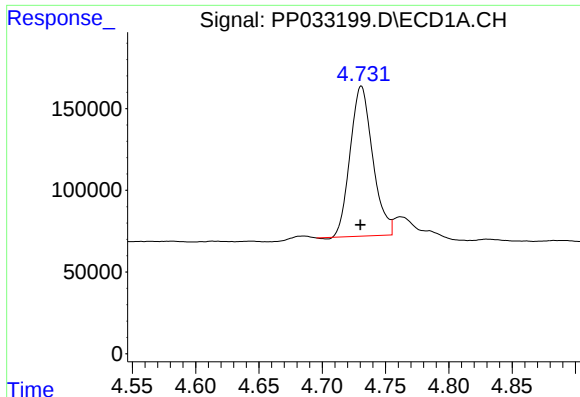


#1 Tetrachloro-m-xylene

R.T.: 4.731 min
Delta R.T.: 0.000 min
Response: 1133277
Conc: 18.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
WOOSPK-073-0204


Manual Integrations
APPROVED

Ankita
2/10/2021 1:56:41 PM

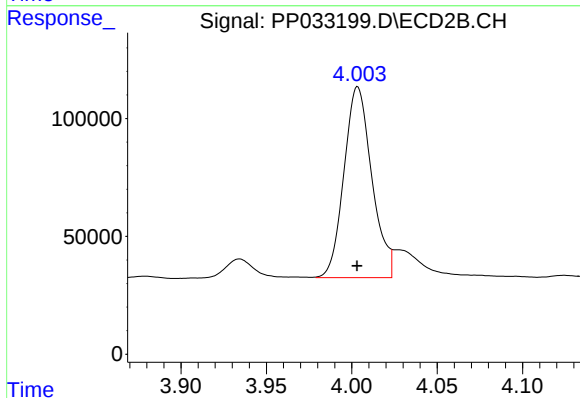


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: 0.000 min
Response: 919690
Conc: 22.49 ng/ml m

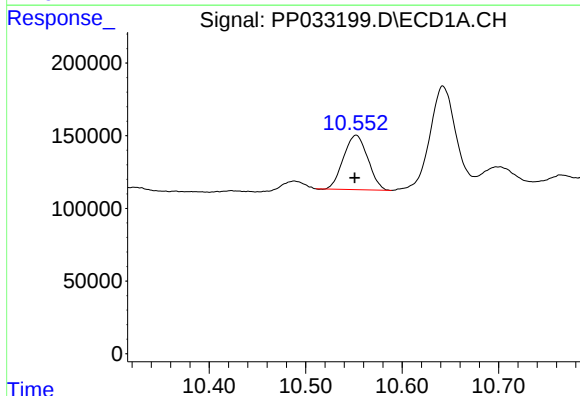

#2 Decachlorobiphenyl

R.T.: 10.552 min
Delta R.T.: 0.001 min
Response: 657829
Conc: 15.10 ng/ml

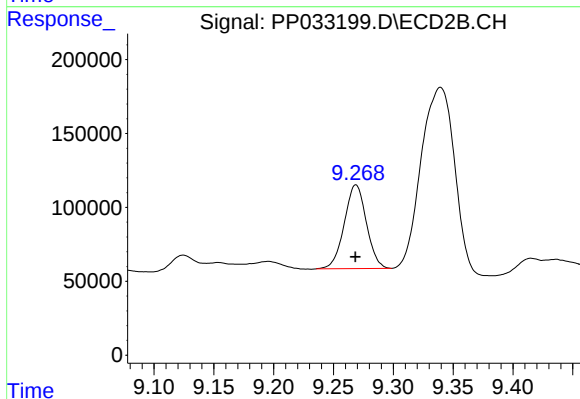

#2 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 728455
Conc: 21.74 ng/ml