

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020923\
 Data File : PP055497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 15:10
 Operator : YP\AJ
 Sample : 01503-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 D2880

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
 Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:39:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.328	3.576	22389013	20043475	12.877m	13.352
2) SA Decachlor...	10.085	8.587	31458735	24877319	18.167	18.420

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020923\
Data File : PP055497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 15:10
Operator : YP\AJ
Sample : 01503-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
D2880


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:39:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

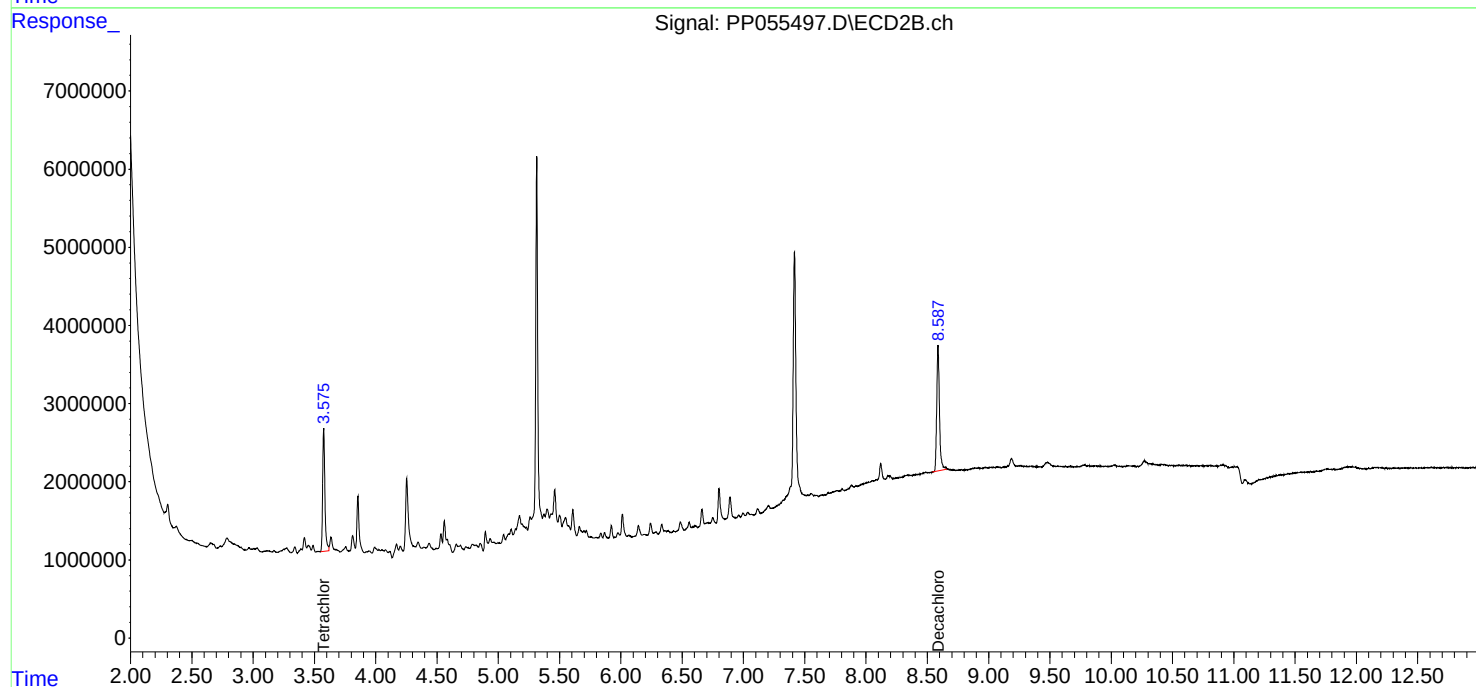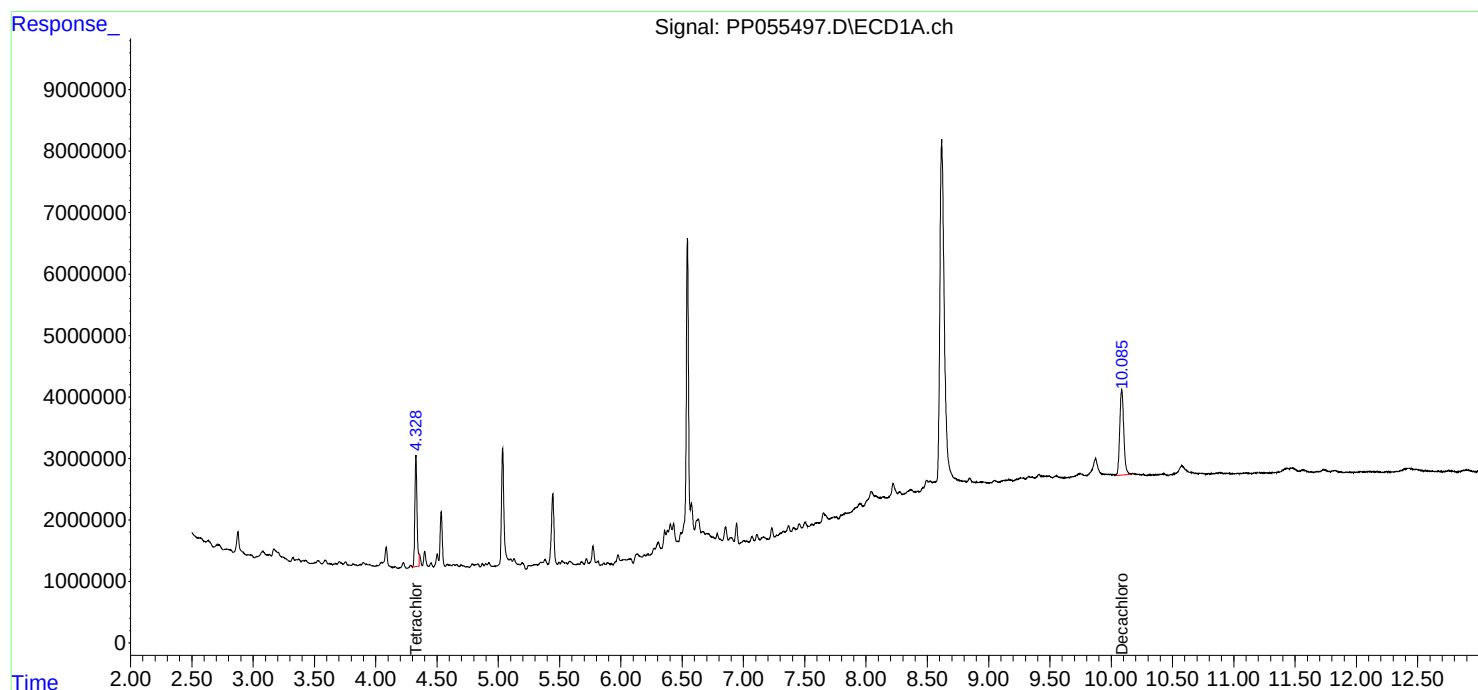

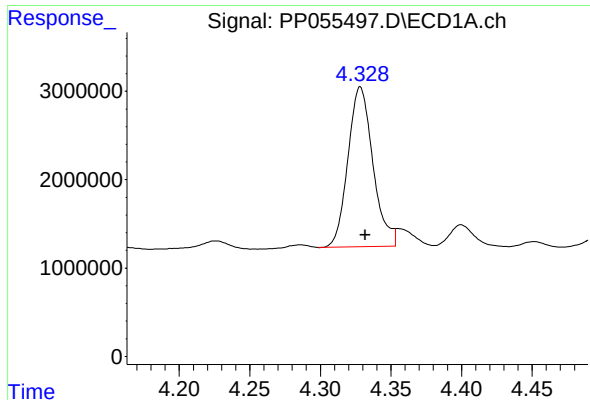


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.004 min
Response: 22389013
Conc: 12.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
D2880


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

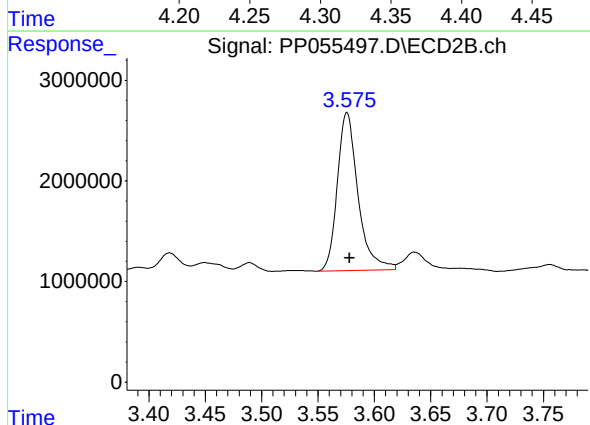


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.003 min
Response: 20043475
Conc: 13.35 ng/ml

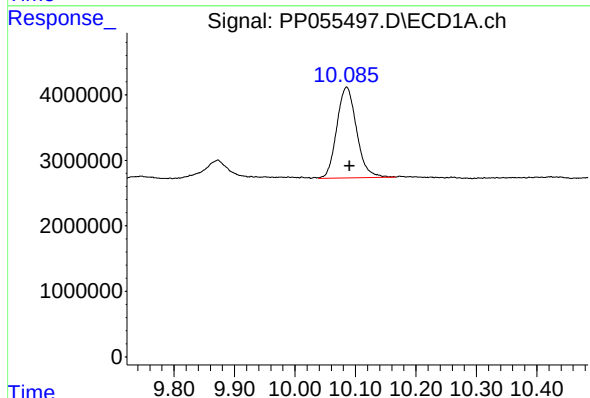

#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: -0.006 min
Response: 31458735
Conc: 18.17 ng/ml

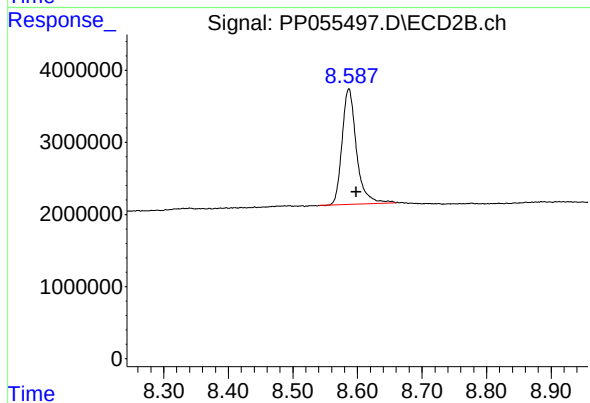

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.011 min
Response: 24877319
Conc: 18.42 ng/ml