

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020923\
 Data File : PP055505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 17:33
 Operator : YP\AJ
 Sample : 01507-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ETGI-330

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
 Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:47:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.329	3.576	30967208	27415631	17.810	18.262
2) SA Decachlor...	10.082	8.583	25543404	19305110	14.751m	14.294

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP020923\
Data File : PP055505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 17:33
Operator : YP\AJ
Sample : 01507-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ETGI-330


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:47:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

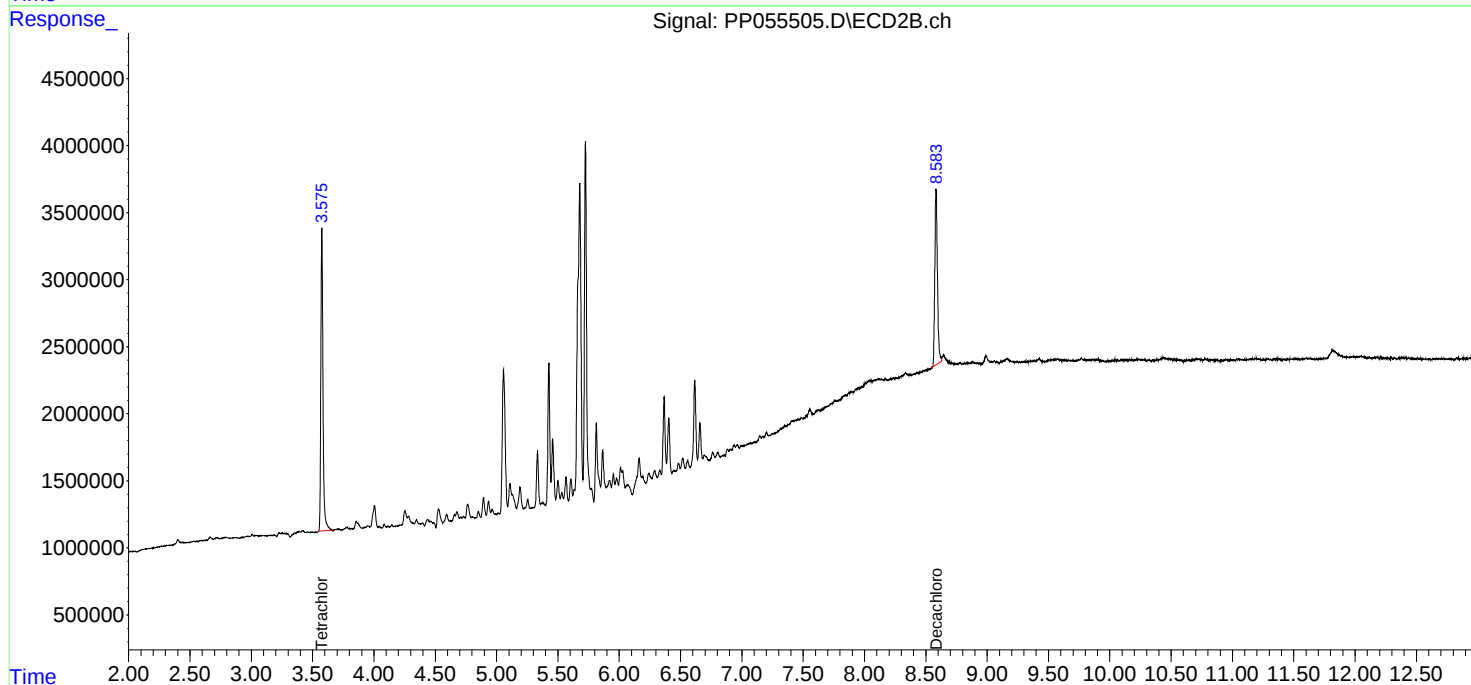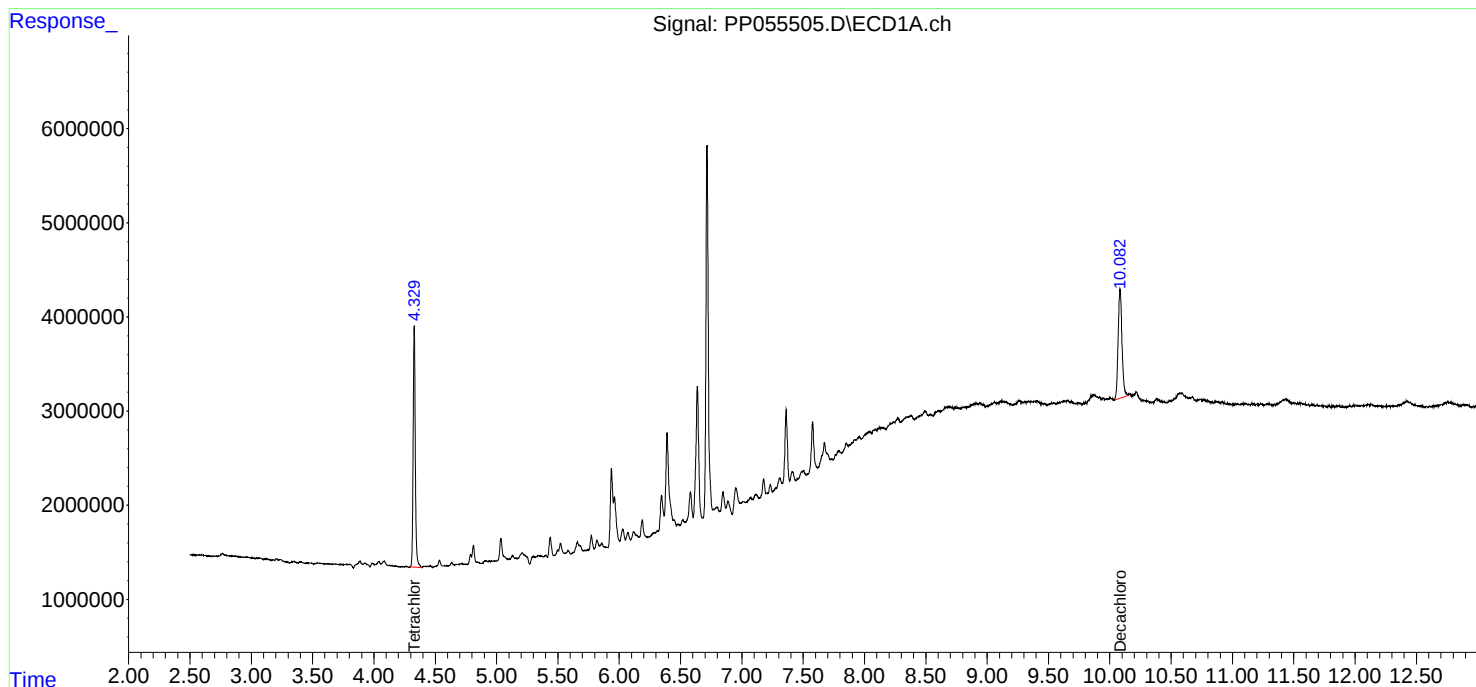

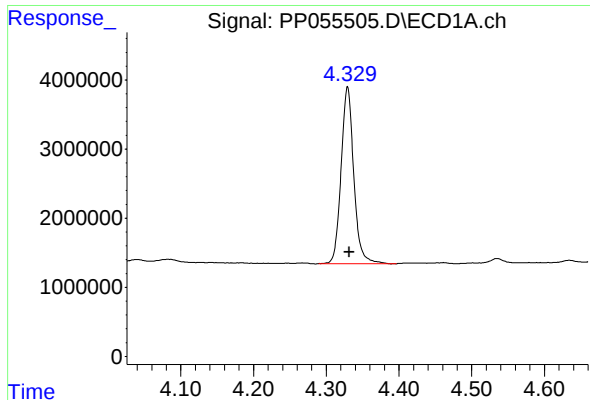


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: -0.003 min
Response: 30967208
Conc: 17.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
ETGI-330


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

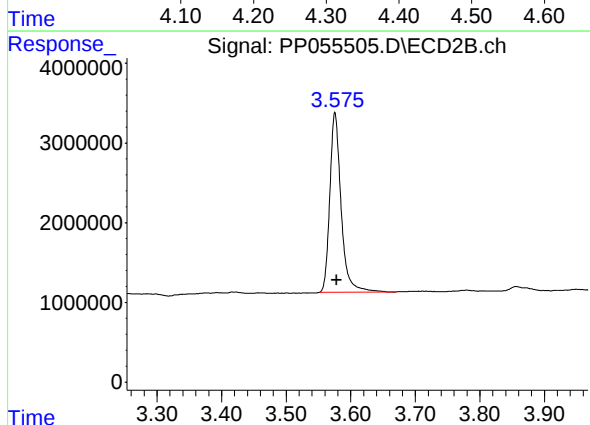


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.003 min
Response: 27415631
Conc: 18.26 ng/ml

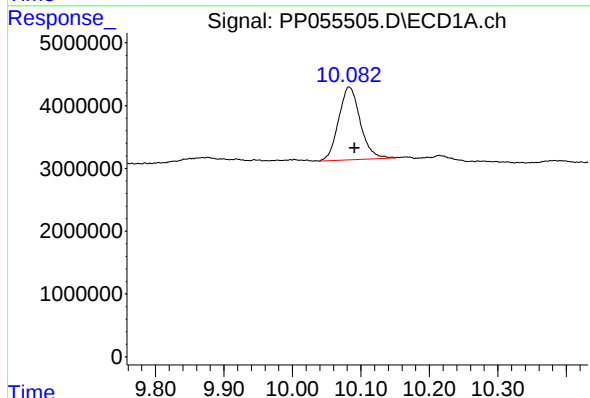

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.009 min
Response: 25543404
Conc: 14.75 ng/ml m

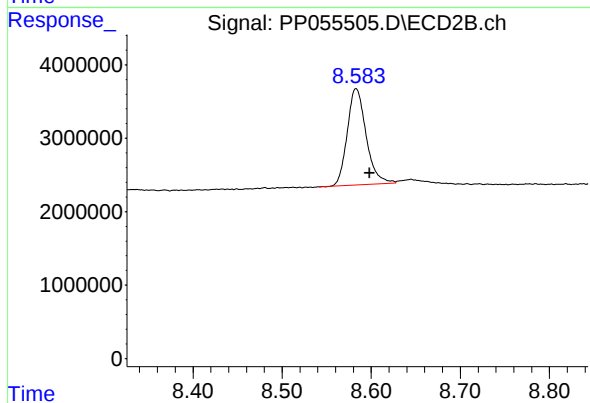

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.015 min
Response: 19305110
Conc: 14.29 ng/ml