

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
 Data File : PP033214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2021 12:04
 Operator : DD\AJ
 Sample : M1339-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-0-5

Manual Integrations
 APPROVED

Ankita
 2/11/2021 11:05:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 12:47:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.728	4.002	1462641	1037314	23.852	25.367
2) SA Decachlor...	10.545	9.263	1057731	868384	24.282m	25.922
Target Compounds						
26) L6 AR-1254-1	6.929	6.112	855823	1005664	455.825	526.209
27) L6 AR-1254-2	7.156	6.271	1442941	810490	492.177	494.314
28) L6 AR-1254-3	7.534	6.690	1713947	1405420	564.300	522.911
29) L6 AR-1254-4	7.828	6.930	1074142	636544	464.338	426.327
30) L6 AR-1254-5	8.255	7.355	1242765	1232938	513.585	509.188

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
Data File : PP033214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2021 12:04
Operator : DD\AJ
Sample : M1339-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-0-5


Manual Integrations
APPROVED

Ankita
2/11/2021 11:05:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 12:47:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

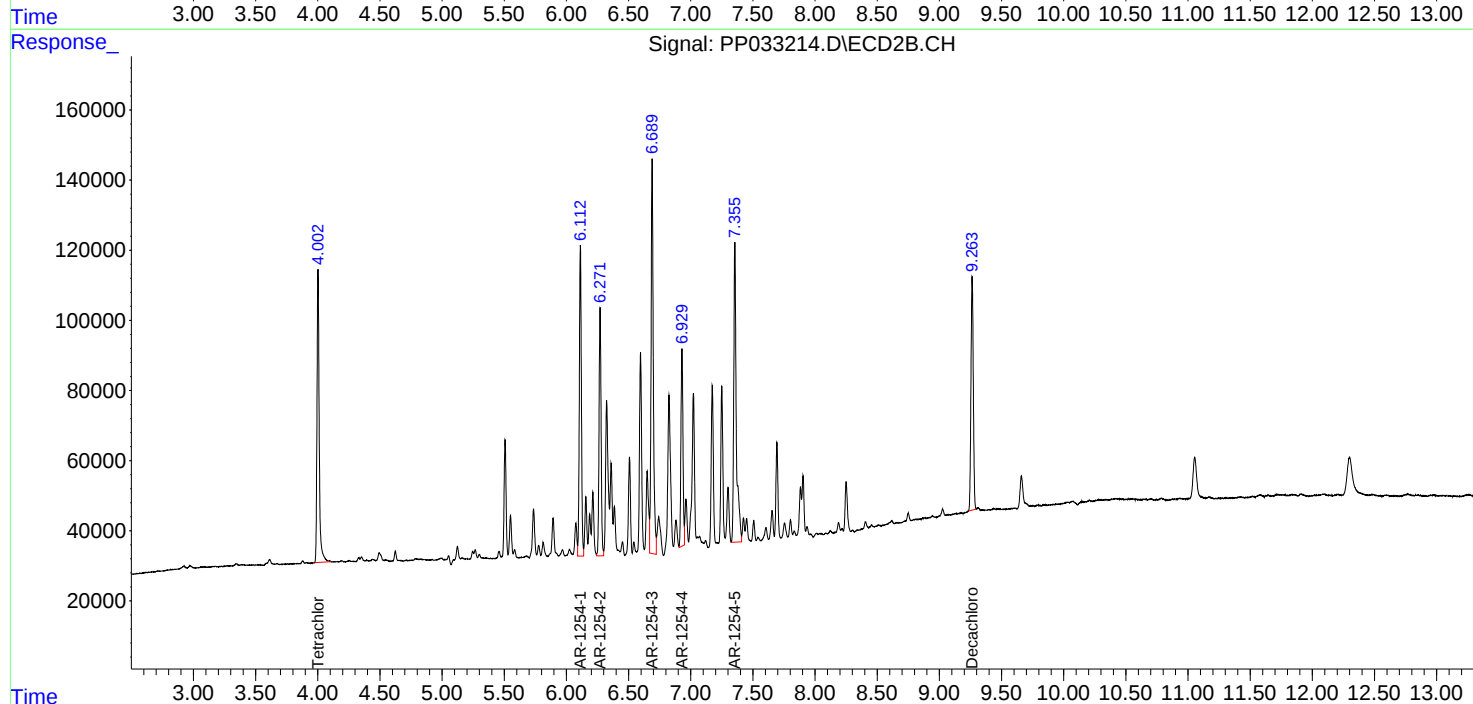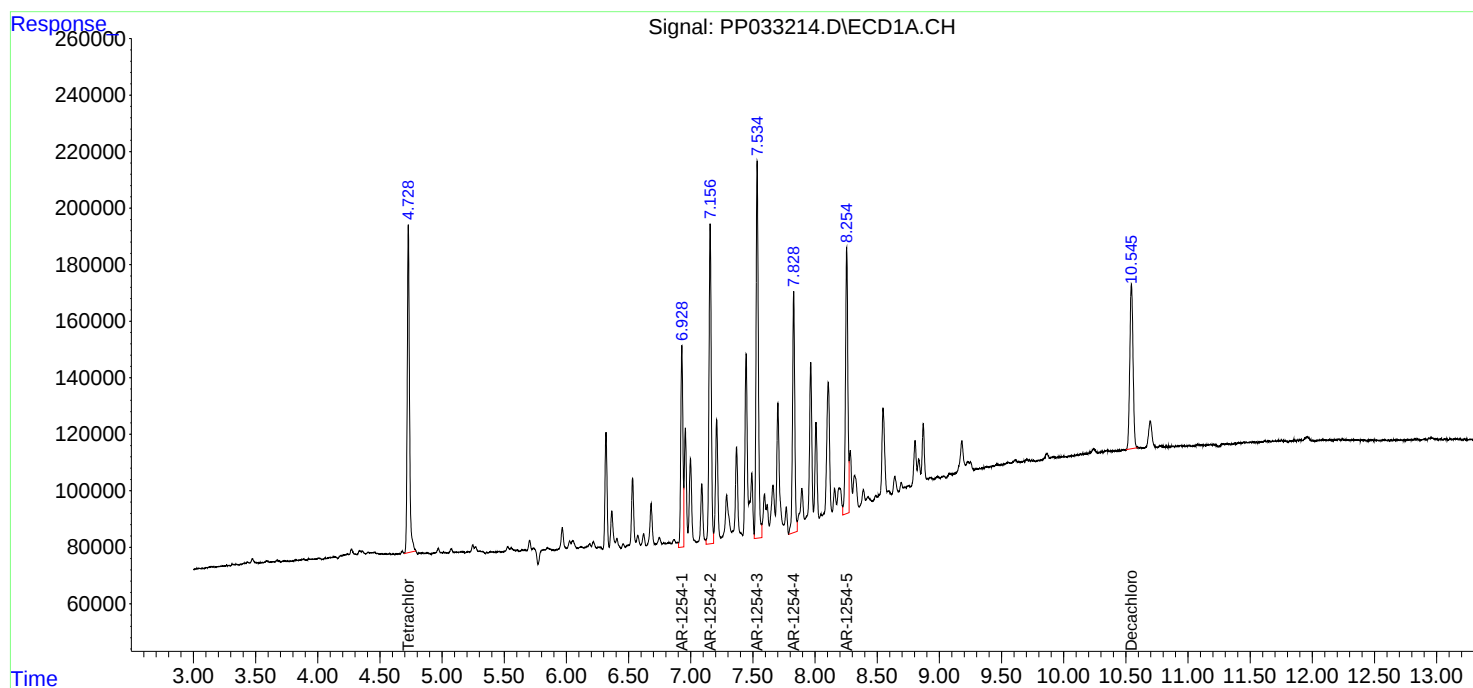

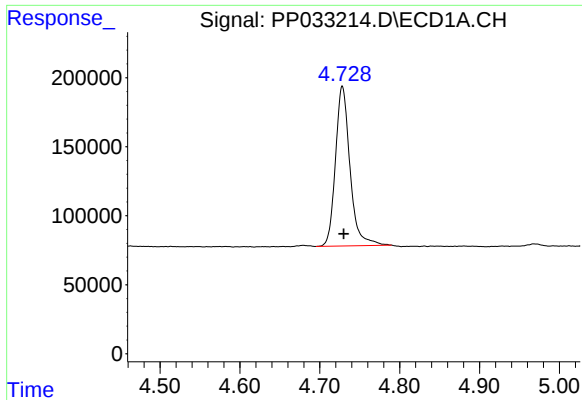


#1 Tetrachloro-m-xylene

R.T.: 4.728 min
Delta R.T.: -0.002 min
Response: 1462641
Conc: 23.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-0-5


Manual Integrations
APPROVED

Ankita
2/11/2021 11:05:39 AM

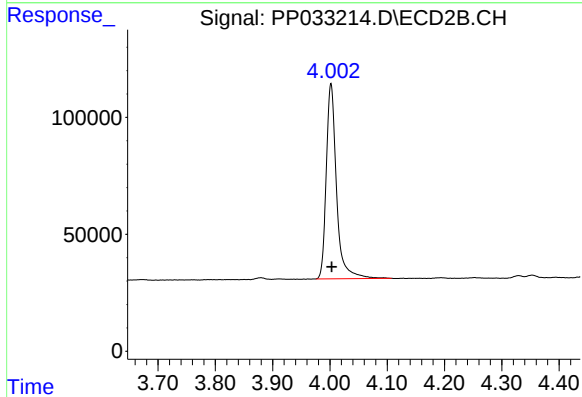


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: 0.000 min
Response: 1037314
Conc: 25.37 ng/ml

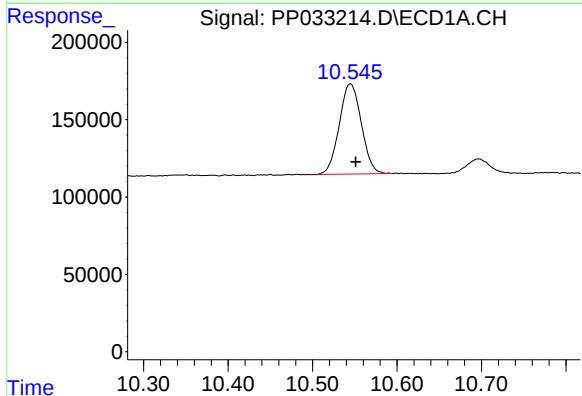


#2 Decachlorobiphenyl

R.T.: 10.545 min
Delta R.T.: -0.006 min
Response: 1057731
Conc: 24.28 ng/ml m

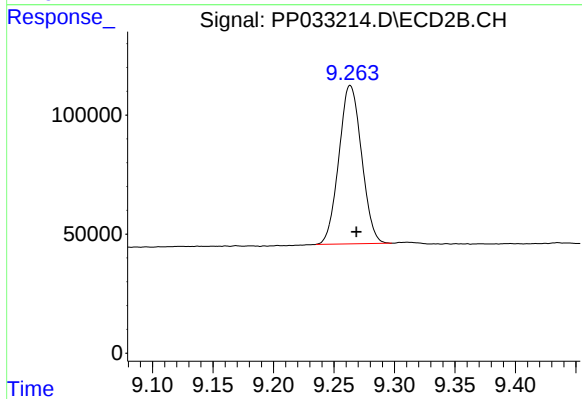

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: -0.005 min
Response: 868384
Conc: 25.92 ng/ml

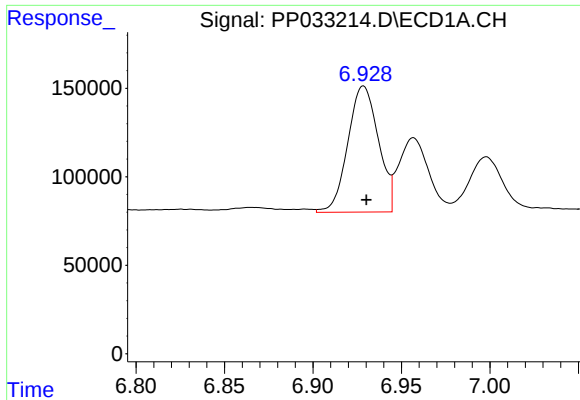


#26 AR-1254-1

R.T.: 6.929 min
Delta R.T.: -0.002 min
Response: 855823
Conc: 455.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-0-5


Manual Integrations
APPROVED

Ankita
2/11/2021 11:05:39 AM

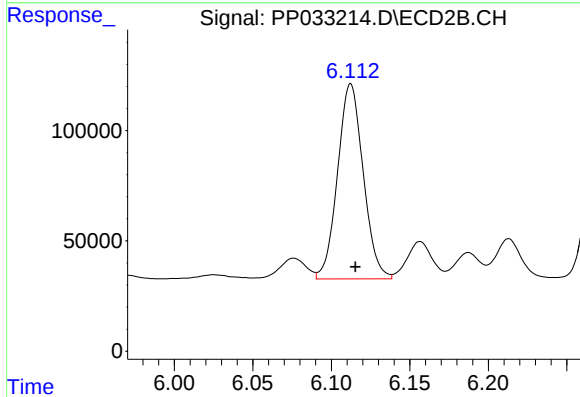


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.003 min
Response: 1005664
Conc: 526.21 ng/ml

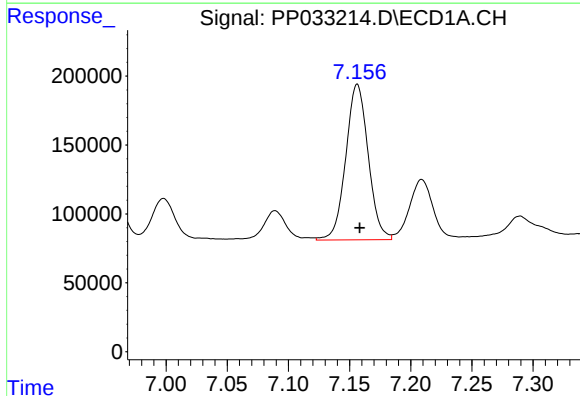


#27 AR-1254-2

R.T.: 7.156 min
Delta R.T.: -0.002 min
Response: 1442941
Conc: 492.18 ng/ml

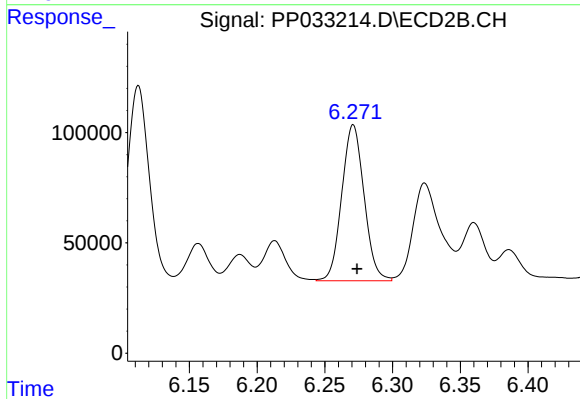

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.003 min
Response: 810490
Conc: 494.31 ng/ml

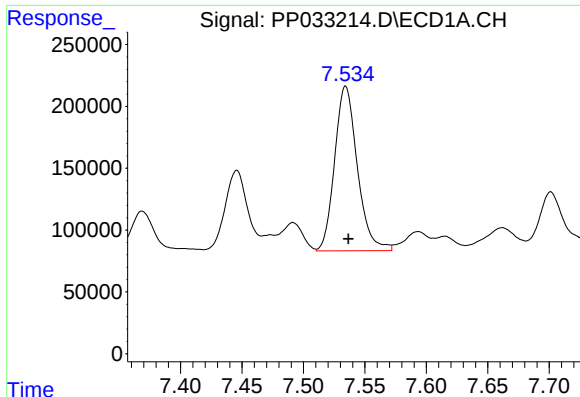


#28 AR-1254-3

R.T.: 7.534 min
Delta R.T.: -0.002 min
Response: 1713947
Conc: 564.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-0-5


Manual Integrations
APPROVED

Ankita
2/11/2021 11:05:39 AM

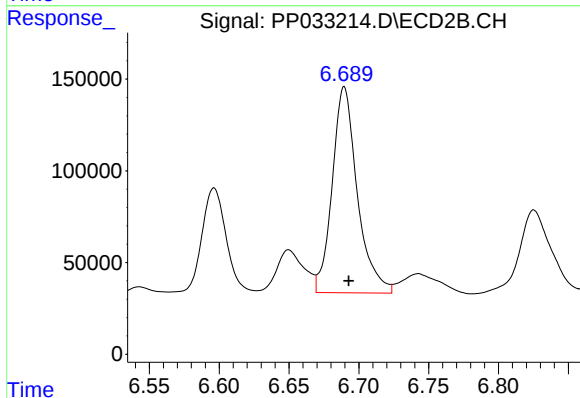


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.003 min
Response: 1405420
Conc: 522.91 ng/ml

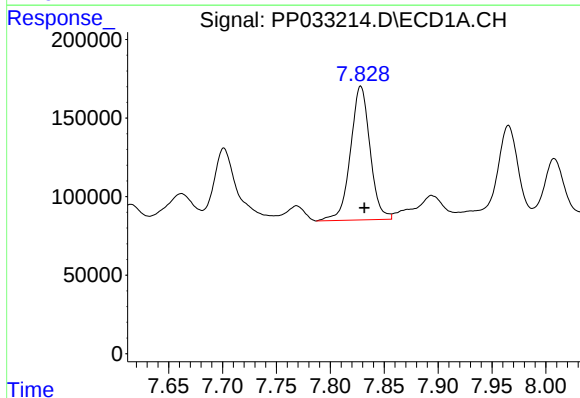


#29 AR-1254-4

R.T.: 7.828 min
Delta R.T.: -0.003 min
Response: 1074142
Conc: 464.34 ng/ml

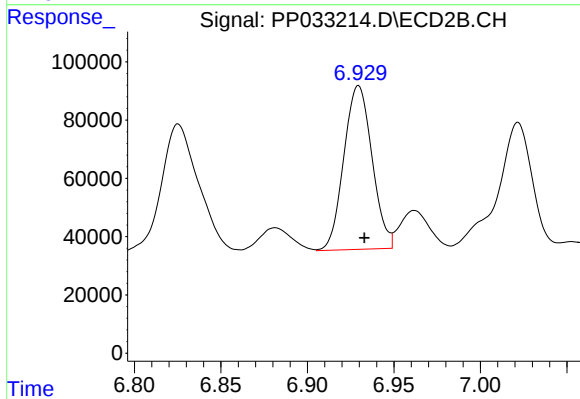

#29 AR-1254-4

R.T.: 6.930 min
Delta R.T.: -0.003 min
Response: 636544
Conc: 426.33 ng/ml

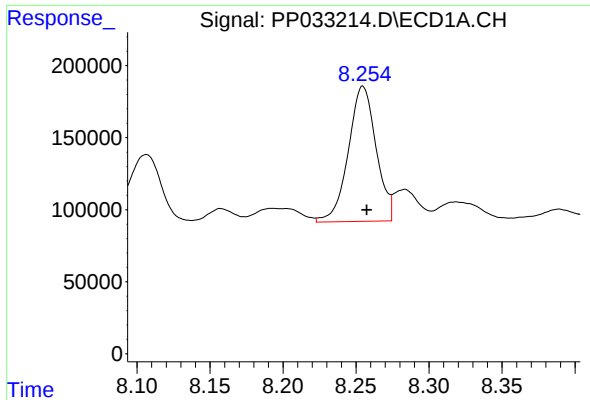


#30 AR-1254-5

R.T.: 8.255 min
Delta R.T.: -0.003 min
Response: 1242765
Conc: 513.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-0-5

Manual Integrations
APPROVED

Ankita
2/11/2021 11:05:39 AM

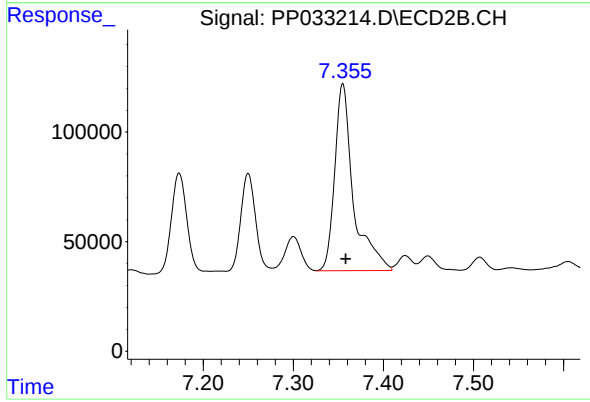

#30 AR-1254-5

R.T.: 7.355 min
Delta R.T.: -0.003 min
Response: 1232938
Conc: 509.19 ng/ml