

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
 Data File : PP033229.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2021 16:23
 Operator : DD\AJ
 Sample : M1348-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AS-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 03:36:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.728	4.001	1364329	1007667	22.248	24.642
2)	SA Decachlor...	10.548	9.265	1033267	843889	23.720	25.191

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
Data File : PP033229.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2021 16:23
Operator : DD\AJ
Sample : M1348-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AS-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 03:36:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

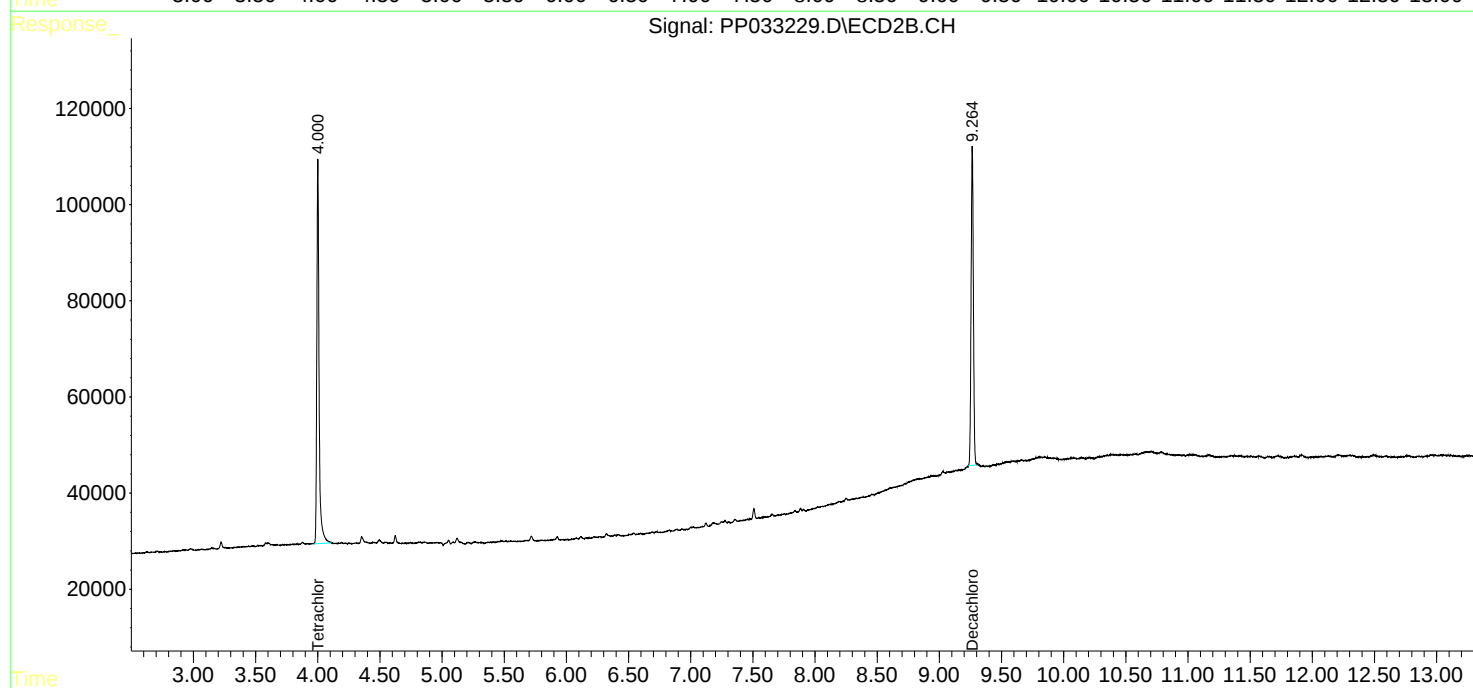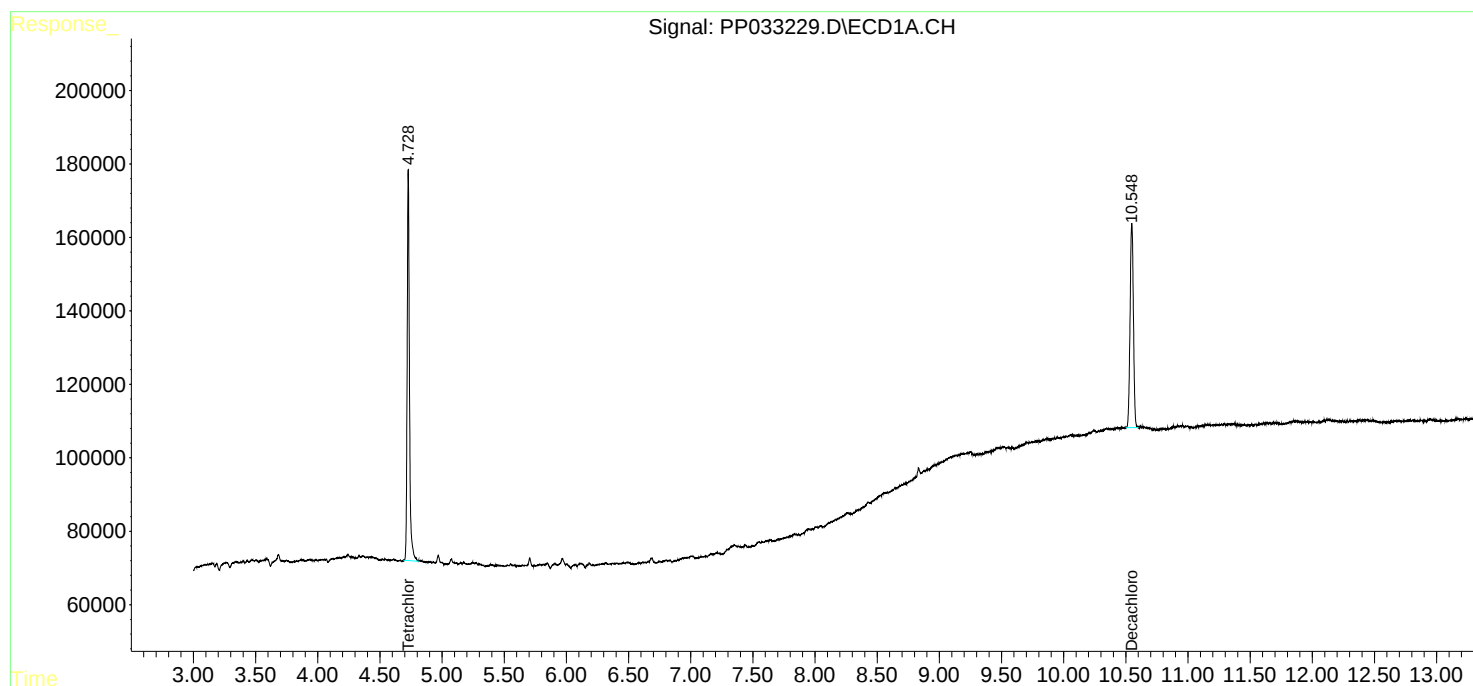


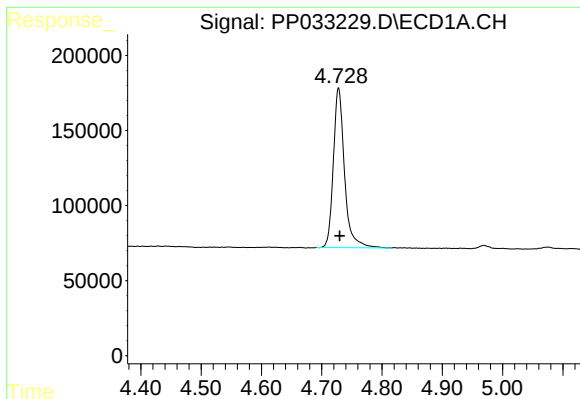

#1 Tetrachloro-m-xylene


R.T.: 4.728 min
Delta R.T.: -0.002 min
Response: 1364329
Conc: 22.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
AS-CON

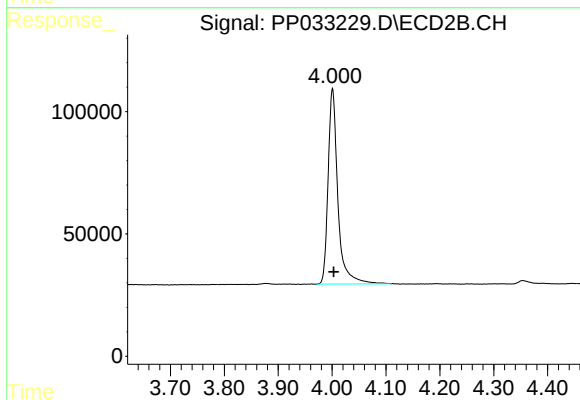


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.002 min
Response: 1007667
Conc: 24.64 ng/ml

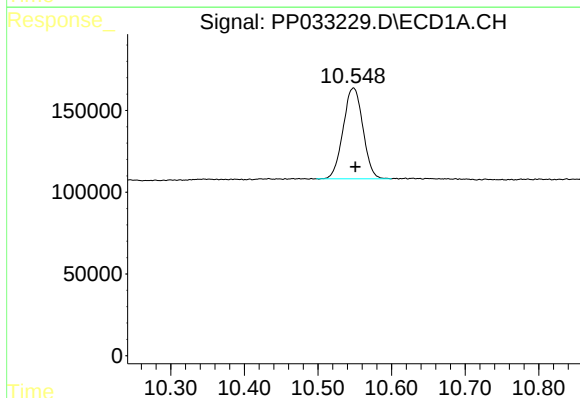

#2 Decachlorobiphenyl

R.T.: 10.548 min
Delta R.T.: -0.003 min
Response: 1033267
Conc: 23.72 ng/ml

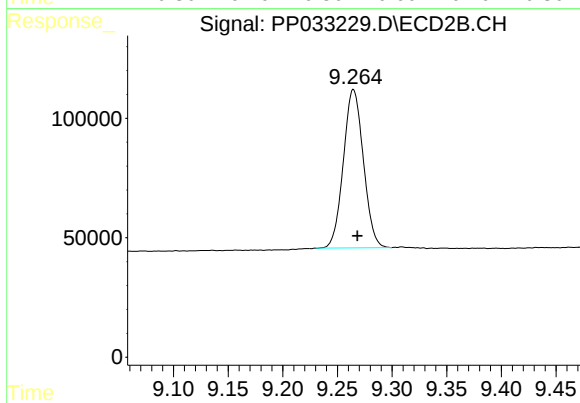

#2 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.004 min
Response: 843889
Conc: 25.19 ng/ml