

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
 Data File : PP033244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2021 20:51
 Operator : DD\AJ
 Sample : M1361-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 T2429-241164

Manual Integrations
 APPROVED

Ankita
 2/11/2021 11:06:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 03:43:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.729	4.003	114042	80560	1.860m	1.970
2) SA Decachlor...	10.548	9.264	118106	91599	2.711	2.734

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021021\
Data File : PP033244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2021 20:51
Operator : DD\AJ
Sample : M1361-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
T2429-241164


Manual Integrations
APPROVED

Ankita
2/11/2021 11:06:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 03:43:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

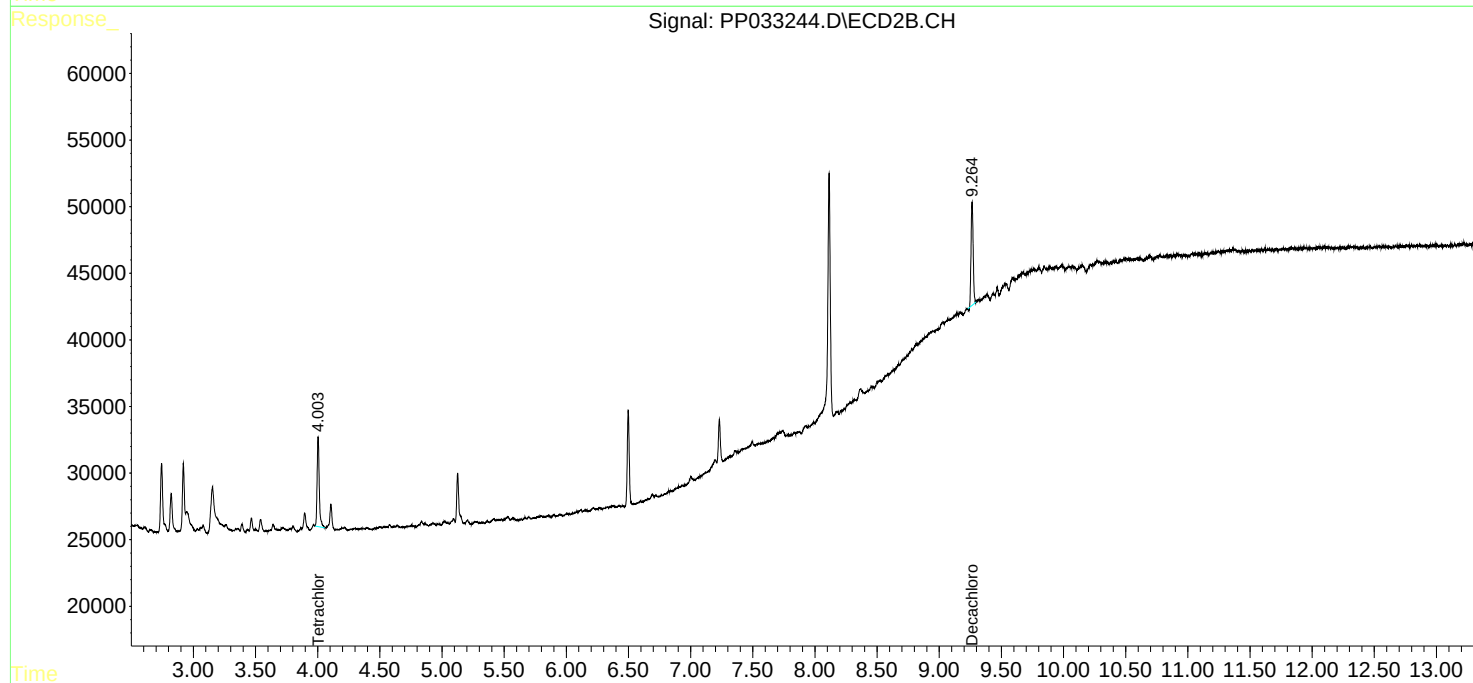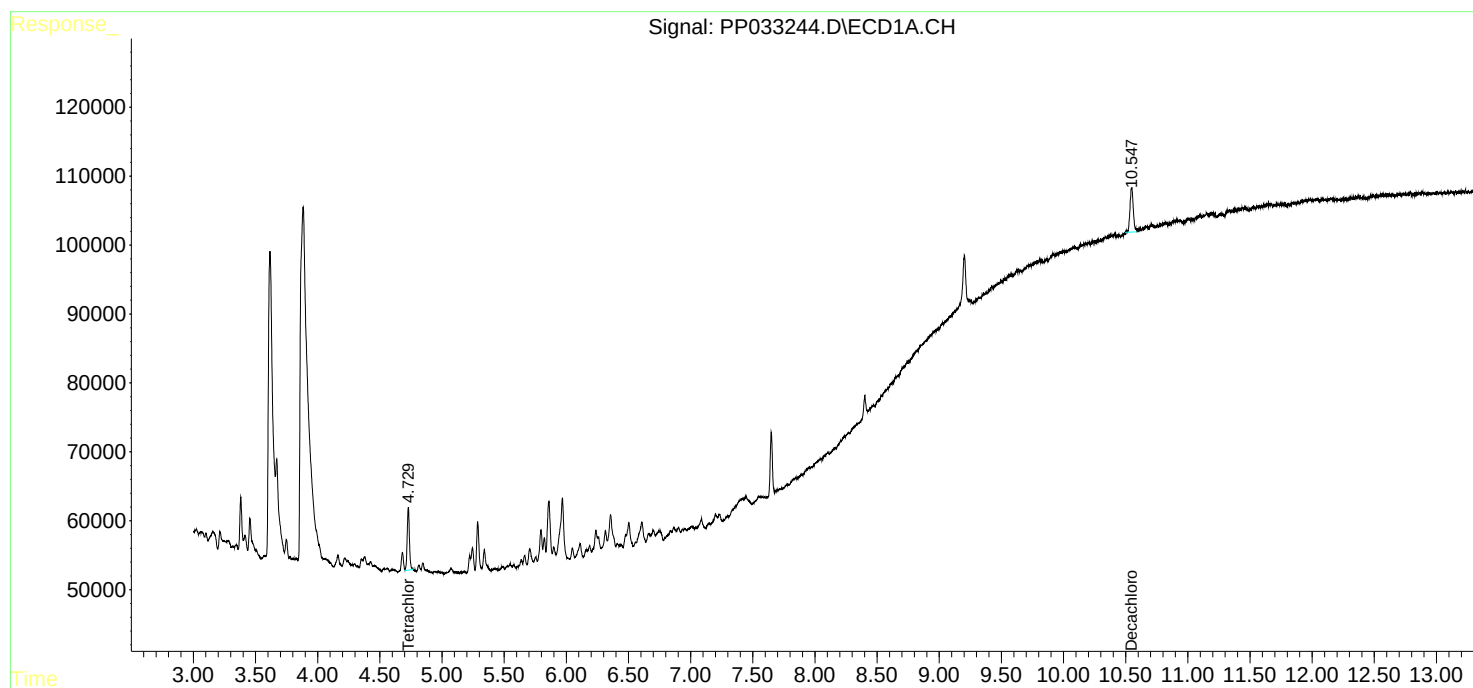

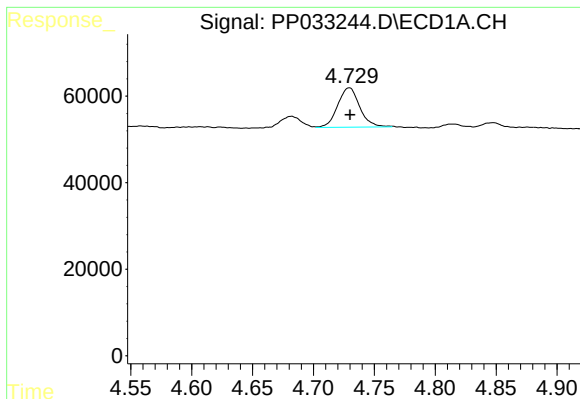


#1 Tetrachloro-m-xylene

R.T.: 4.729 min
Delta R.T.: 0.000 min
Response: 114042
Conc: 1.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
T2429-241164


Manual Integrations
APPROVED

Ankita
2/11/2021 11:06:48 AM

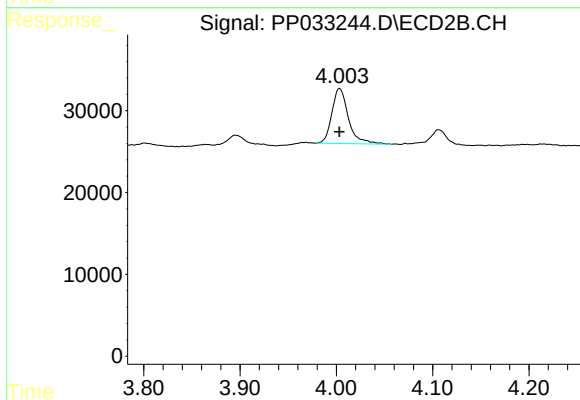


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: 0.000 min
Response: 80560
Conc: 1.97 ng/ml

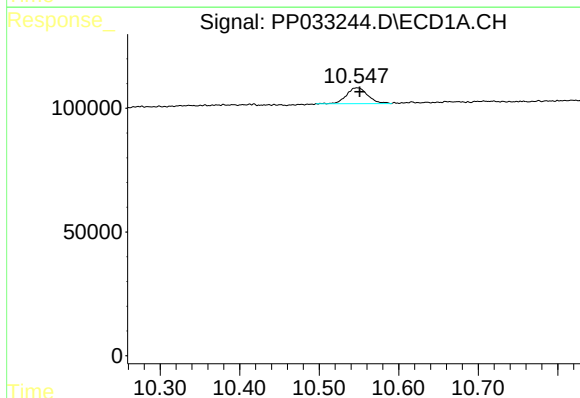

#2 Decachlorobiphenyl

R.T.: 10.548 min
Delta R.T.: -0.003 min
Response: 118106
Conc: 2.71 ng/ml

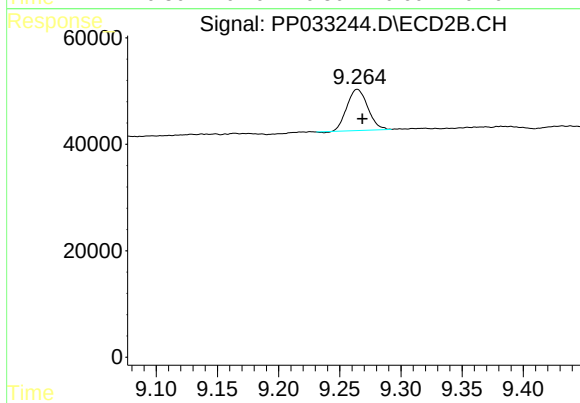

#2 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.004 min
Response: 91599
Conc: 2.73 ng/ml