

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021023\
 Data File : PP055547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 19:25
 Operator : YP\AJ
 Sample : 01491-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OW-TOTE-0208

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
 Supervised By :Sohil Jodhani 02/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 22:01:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.573	24147250	19420366	13.888	12.936
2) SA Decachlor...	10.084	8.586	19168164	16132036	11.069m	11.945

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021023\
Data File : PP055547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 19:25
Operator : YP\AJ
Sample : 01491-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OW-TOTE-0208


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 22:01:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

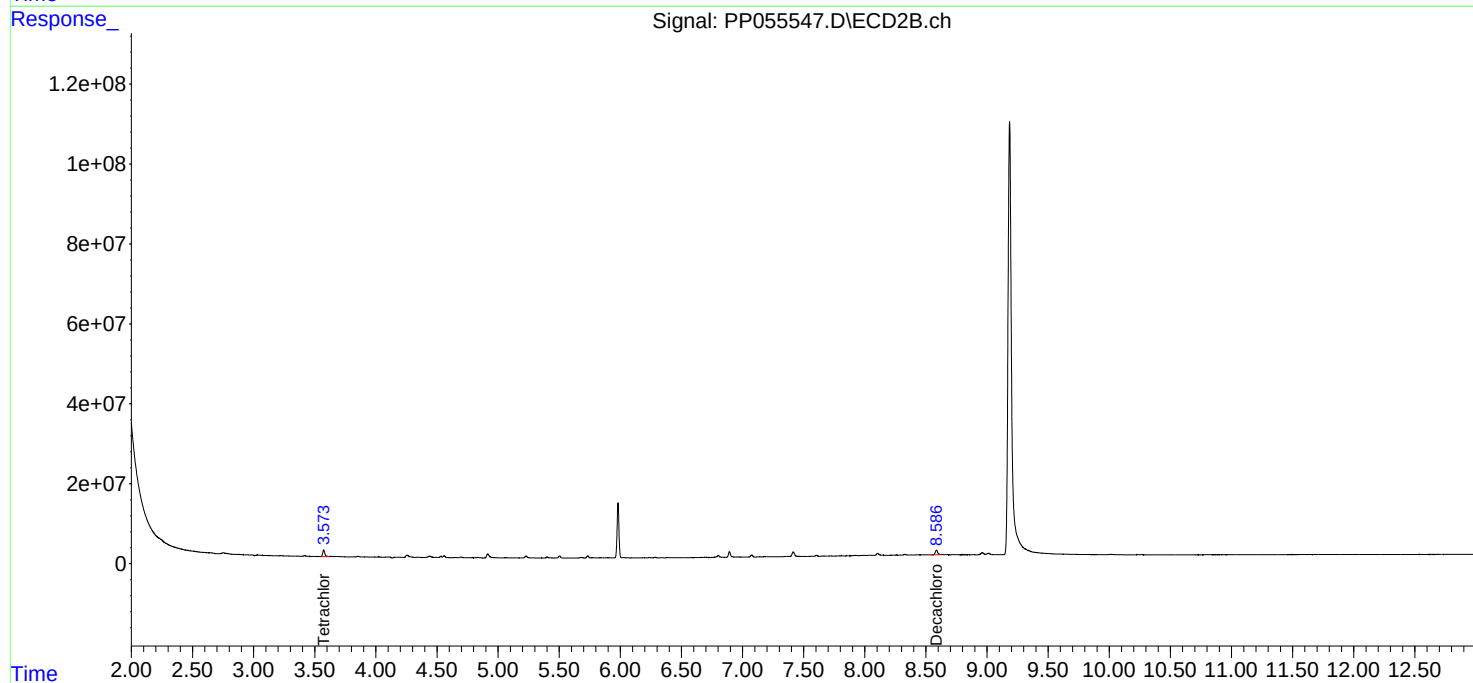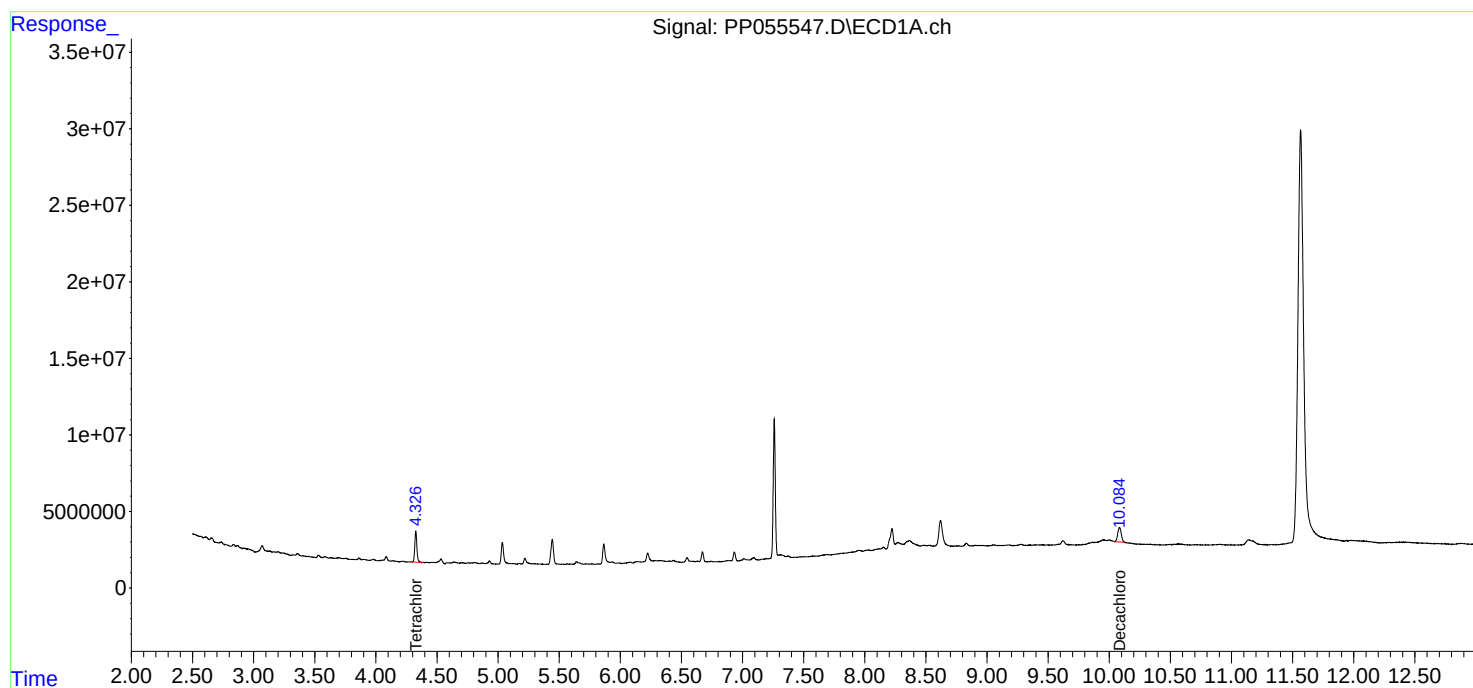

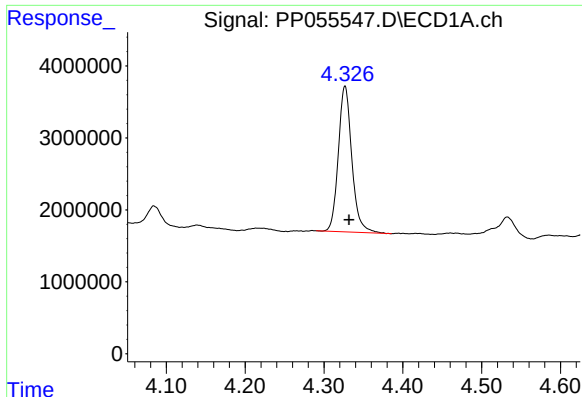


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: -0.005 min
Response: 24147250
Conc: 13.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
OW-TOTE-0208


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

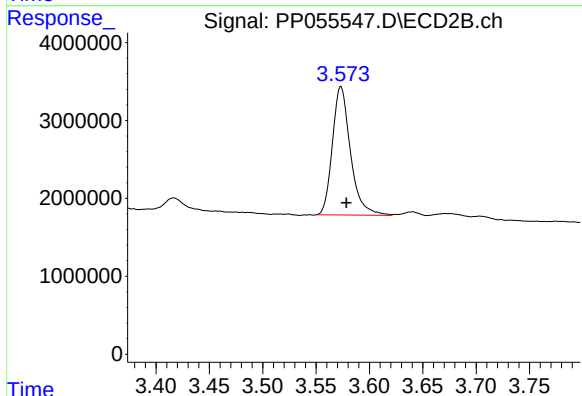


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: -0.005 min
Response: 19420366
Conc: 12.94 ng/ml

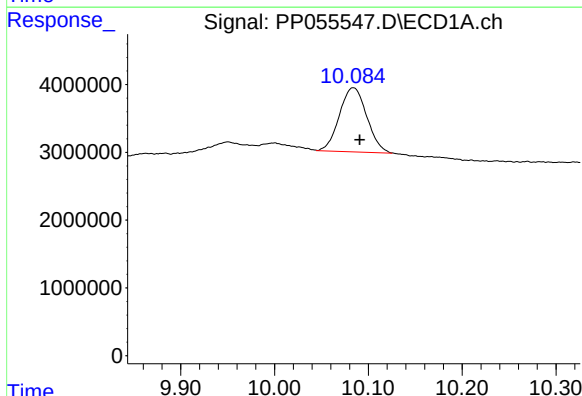

#2 Decachlorobiphenyl

R.T.: 10.084 min
Delta R.T.: -0.007 min
Response: 19168164
Conc: 11.07 ng/ml m

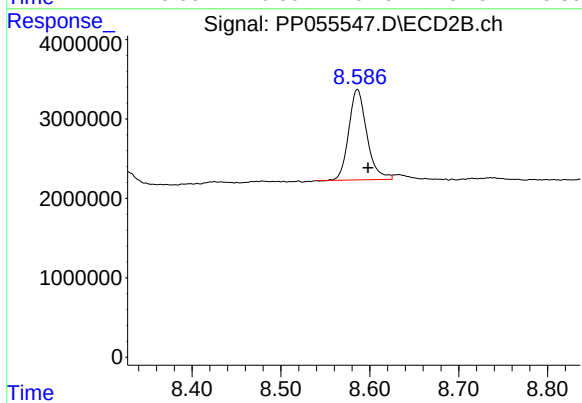

#2 Decachlorobiphenyl

R.T.: 8.586 min
Delta R.T.: -0.012 min
Response: 16132036
Conc: 11.94 ng/ml