

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021023\
 Data File : PP055549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2023 19:58
 Operator : YP\AJ
 Sample : 01507-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HA-WATER-0208

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
 Supervised By :Sohil Jodhani 02/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 22:03:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.576	23540180	19871740	13.539m	13.237
2) SA Decachlor...	10.078	8.582	25968700	20677332	14.996	15.310

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021023\
Data File : PP055549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2023 19:58
Operator : YP\AJ
Sample : 01507-04
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HA-WATER-0208


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 22:03:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

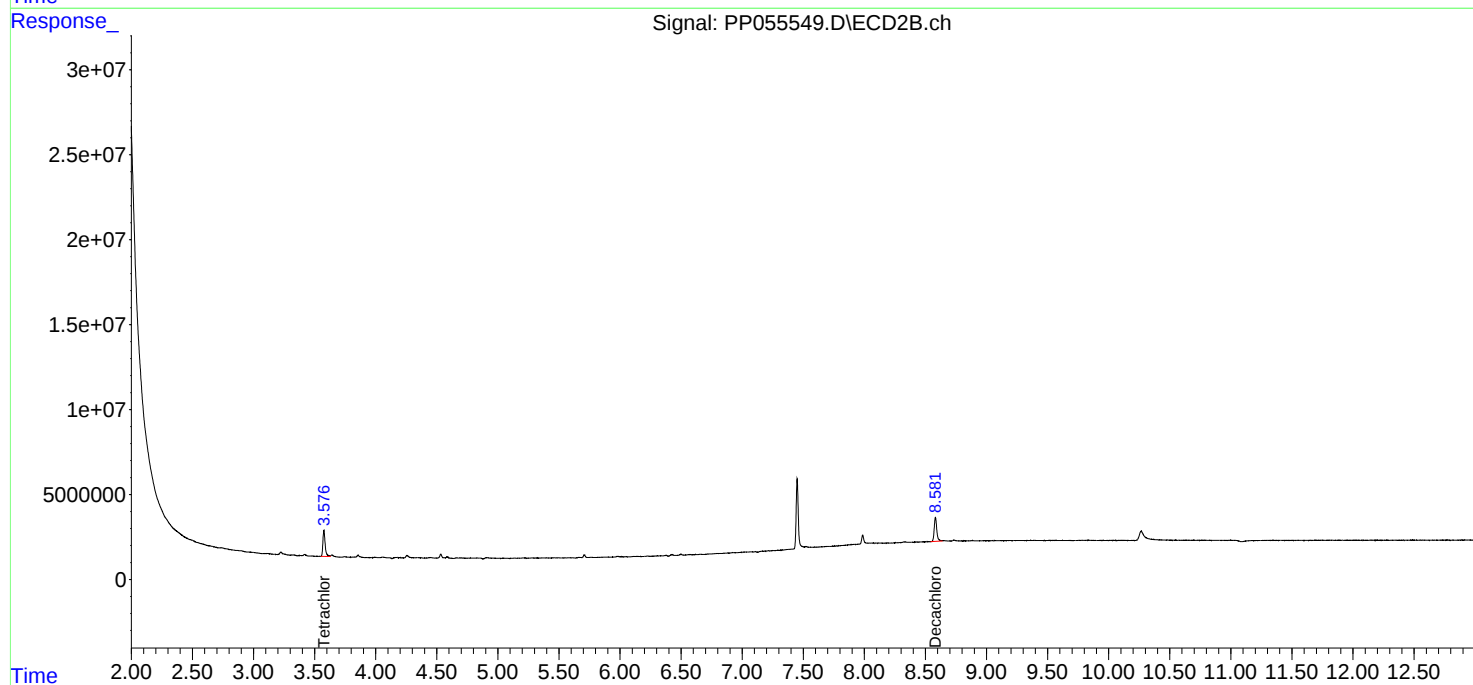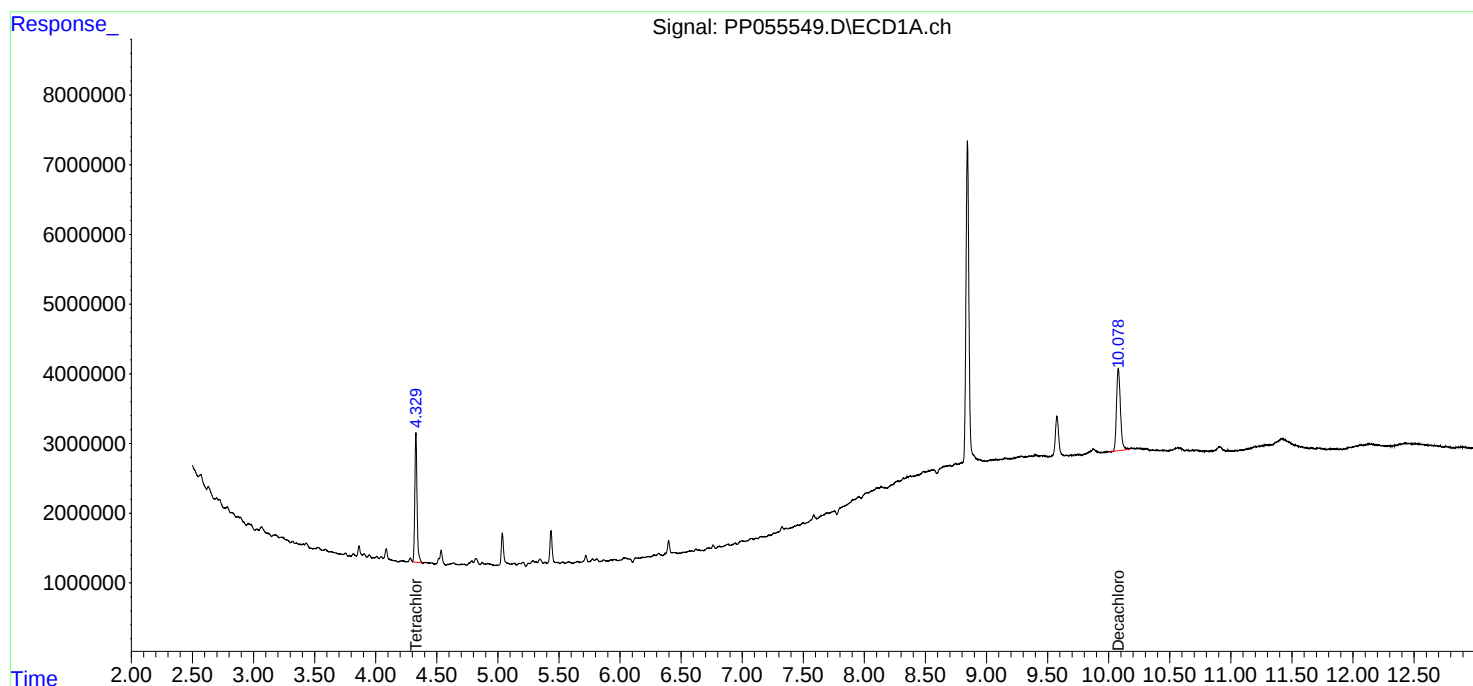

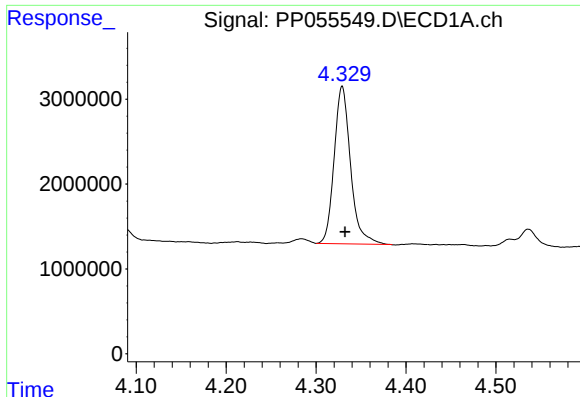


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: -0.003 min
Response: 23540180
Conc: 13.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-WATER-0208


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/13/2023
Supervised By :Sohil Jodhani 02/13/2023

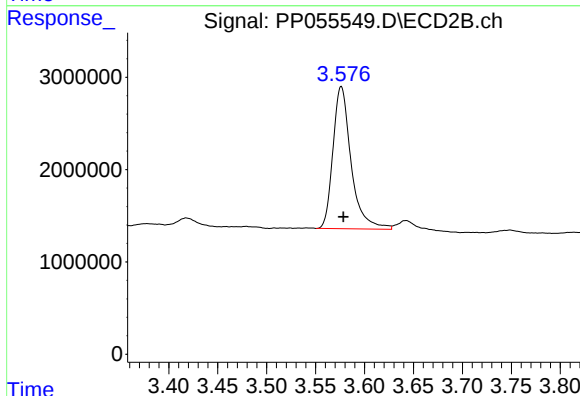


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.002 min
Response: 19871740
Conc: 13.24 ng/ml

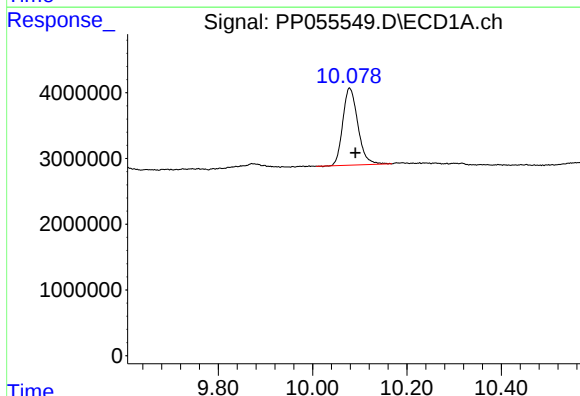

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: -0.013 min
Response: 25968700
Conc: 15.00 ng/ml

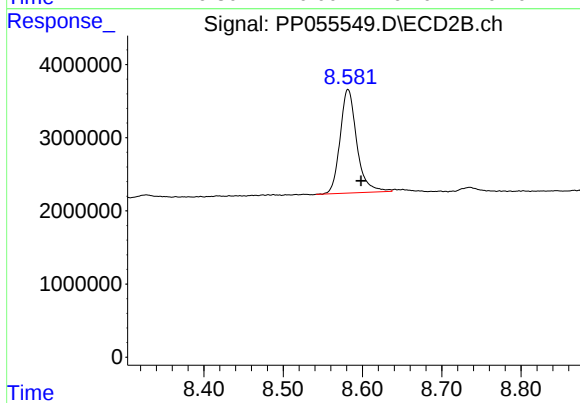

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.016 min
Response: 20677332
Conc: 15.31 ng/ml