

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021025\
 Data File : PP069628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2025 14:42
 Operator : YP\AJ
 Sample : PB166638BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB166638BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/11/2025
 Supervised By :Ankita Jodhani 02/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 05:58:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.535	3.837	33670341	21952996	23.521	24.596
2) SA Decachlor...	10.276	8.897	9114159	26540261	8.339m	23.729 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021025\
Data File : PP069628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2025 14:42
Operator : YP\AJ
Sample : PB166638BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB166638BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2025
Supervised By :Ankita Jodhani 02/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 05:58:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

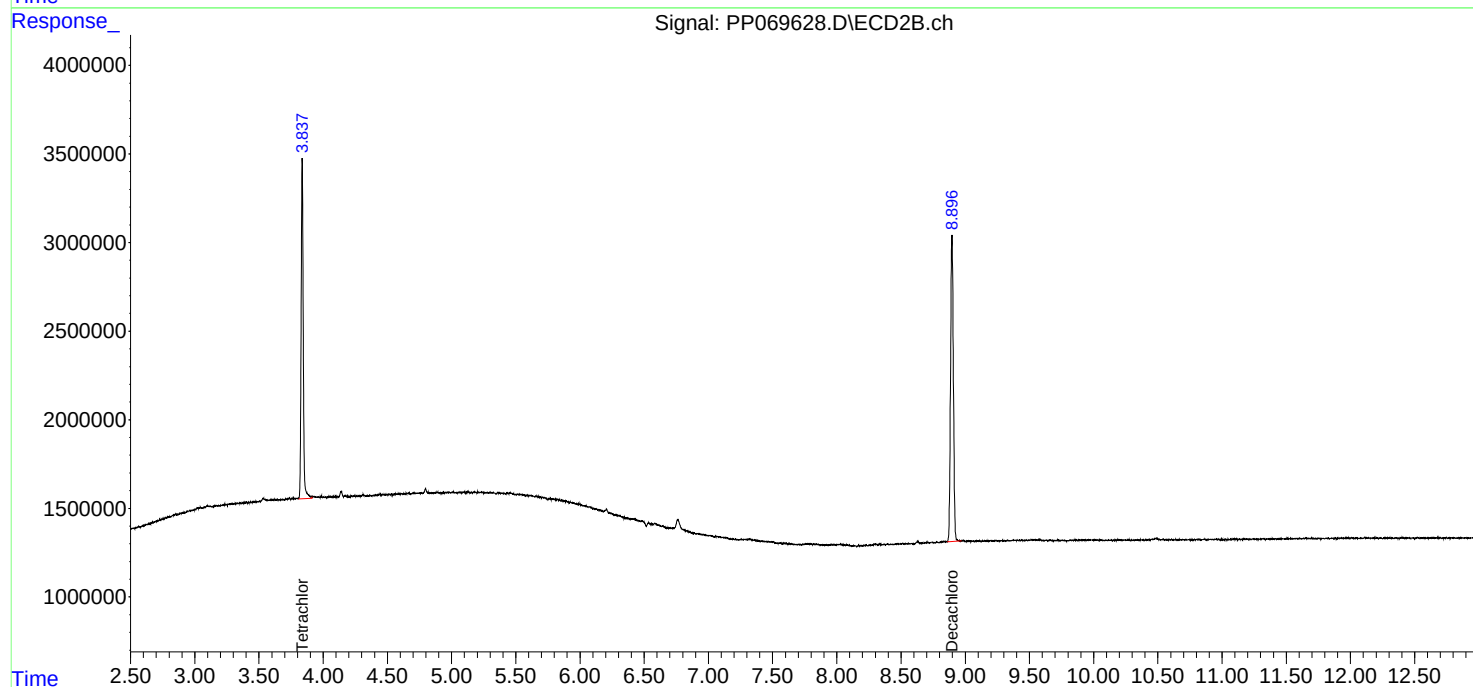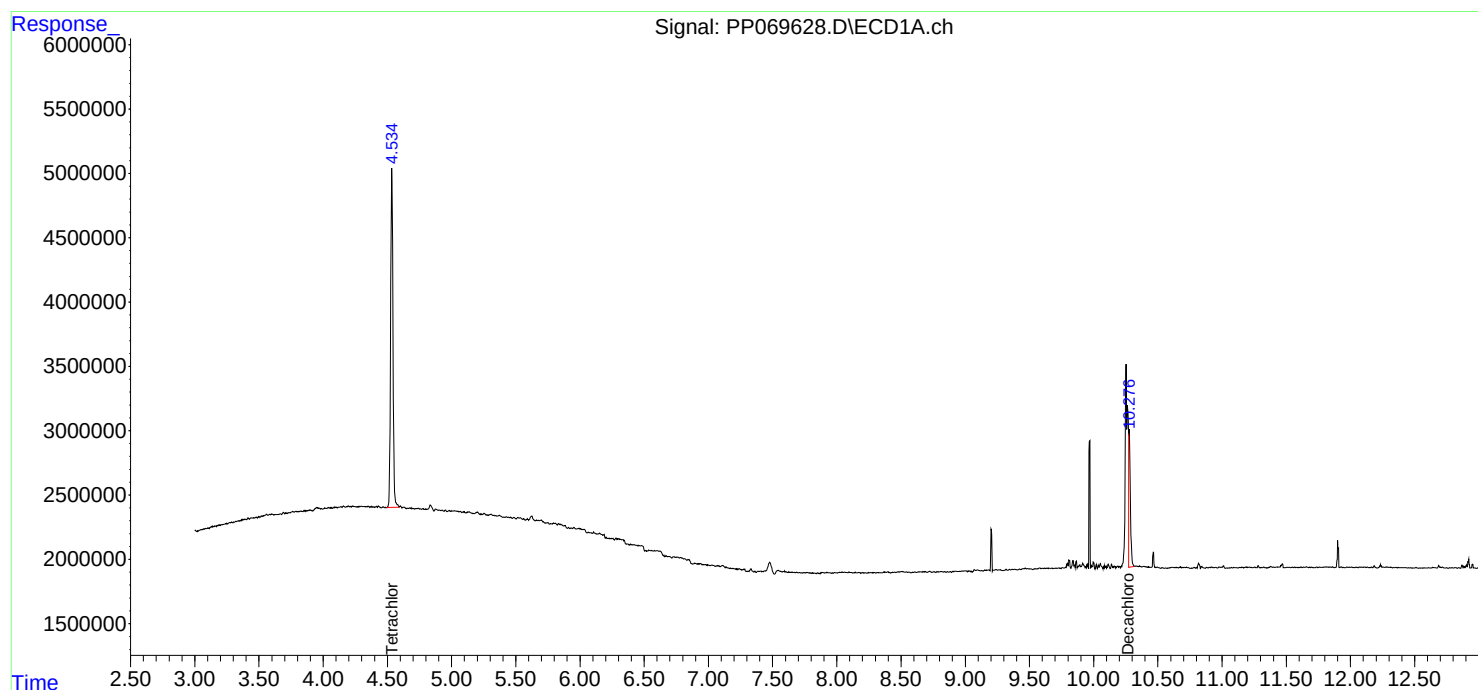

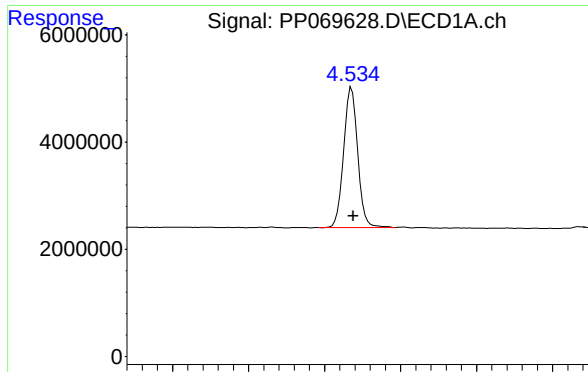


#1 Tetrachloro-m-xylene

R.T.: 4.535 min
Delta R.T.: -0.003 min
Response: 33670341
Conc: 23.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB166638BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2025
Supervised By :Ankita Jodhani 02/11/2025

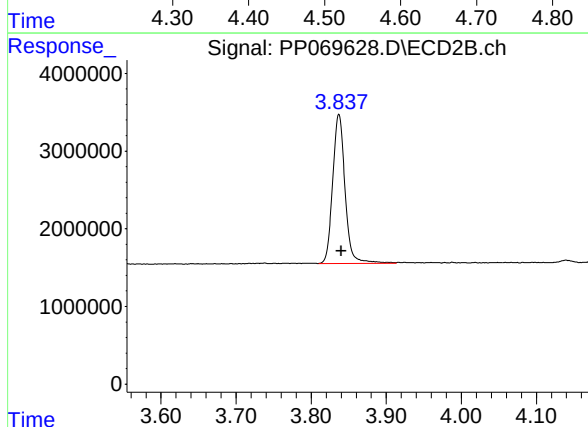


#1 Tetrachloro-m-xylene

R.T.: 3.837 min
Delta R.T.: -0.003 min
Response: 21952996
Conc: 24.60 ng/ml

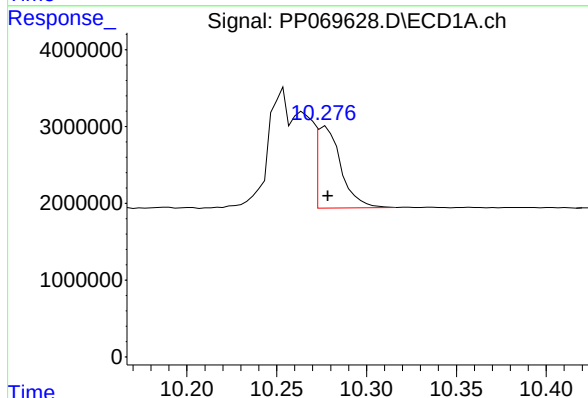

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: -0.002 min
Response: 9114159
Conc: 8.34 ng/ml m

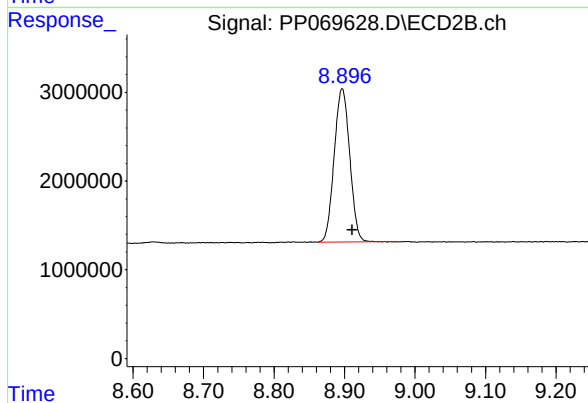

#2 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: -0.014 min
Response: 26540261
Conc: 23.73 ng/ml