

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
 Data File : PP033256.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2021 9:01
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:45:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
28)	L6	AR-1254-3	7.549	0.000	52319	0	17.226 N.D. #
30)	L6	AR-1254-5	8.241f	0.000	17859	0	7.380 N.D. #
32)	L7	AR-1260-2	7.962	0.000	11222	0	3.840 N.D. #
33)	L7	AR-1260-3	8.343	0.000	11852	0	4.631 N.D. #
34)	L7	AR-1260-4	8.550	0.000	32833	0	13.439 N.D. #
35)	L7	AR-1260-5	8.855f	0.000	5610	0	1.042 N.D. #
36)	L8	AR-1262-1	8.343	0.000	11852	0	3.118 N.D. #
37)	L8	AR-1262-2	8.855f	0.000	5610	0	0.896 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
Data File : PP033256.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2021 9:01
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:45:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

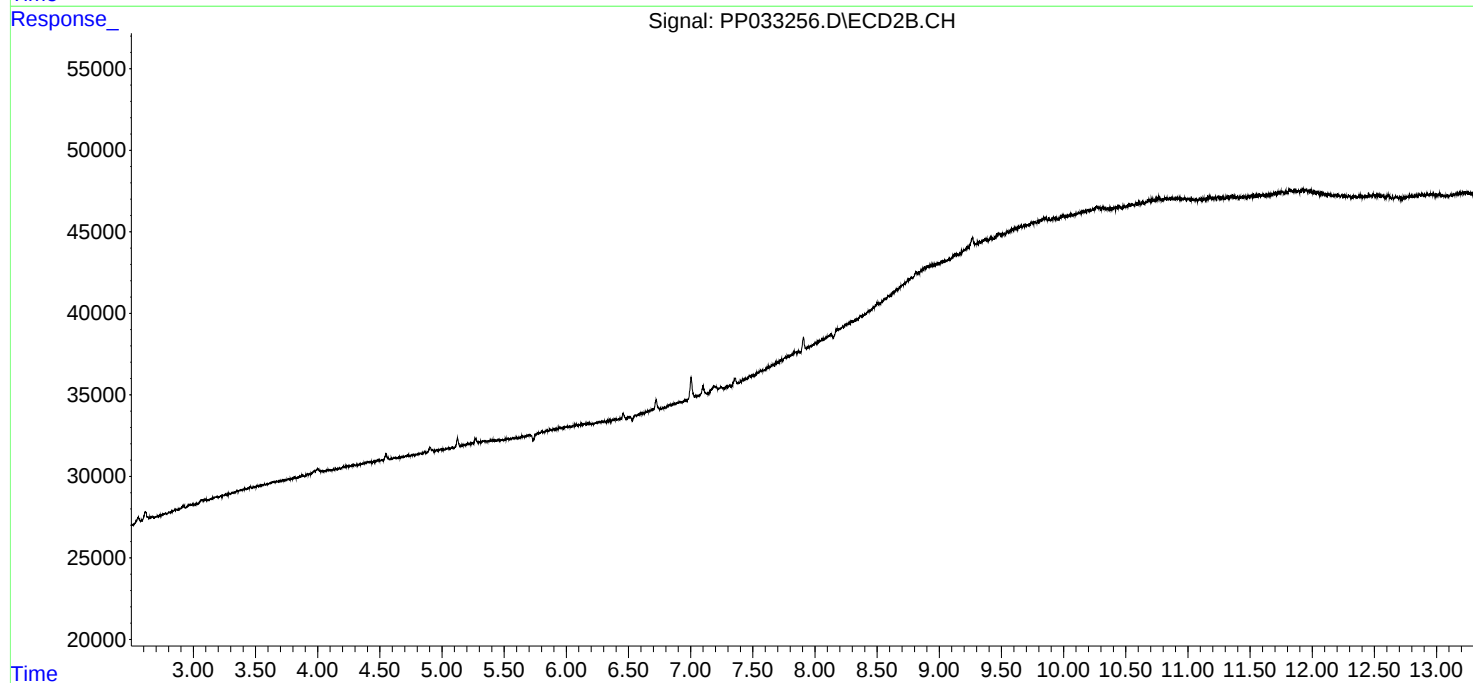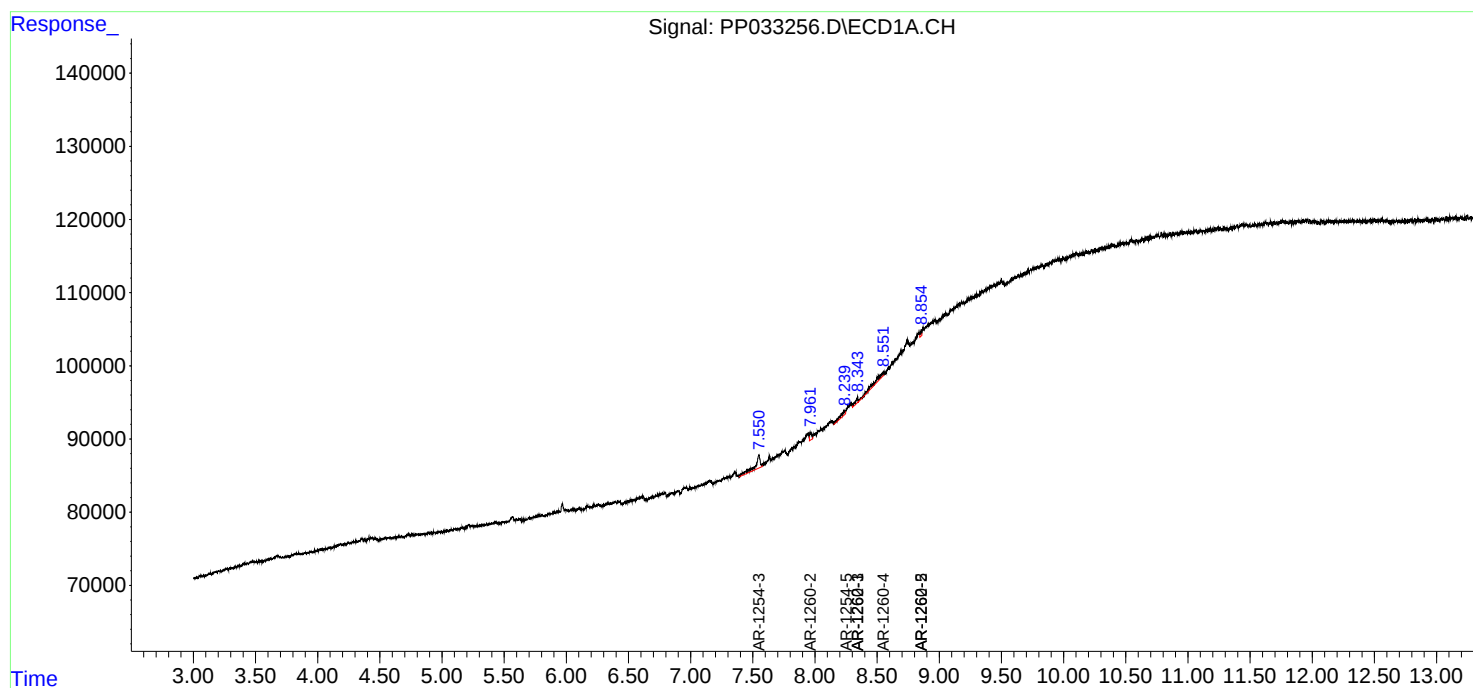


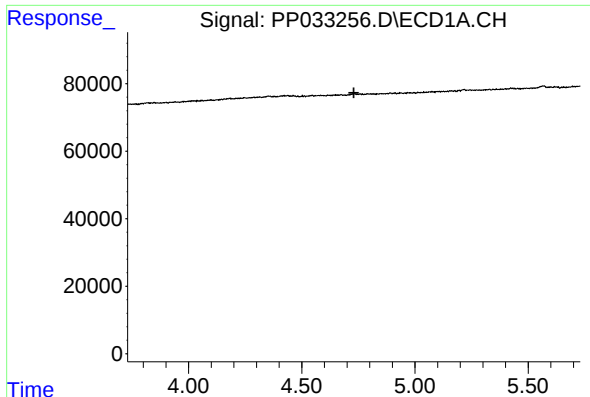

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.730 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

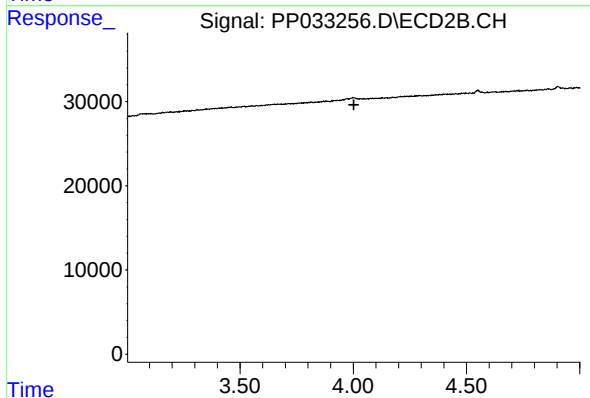


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.003 min
Response: 0
Conc: N.D.

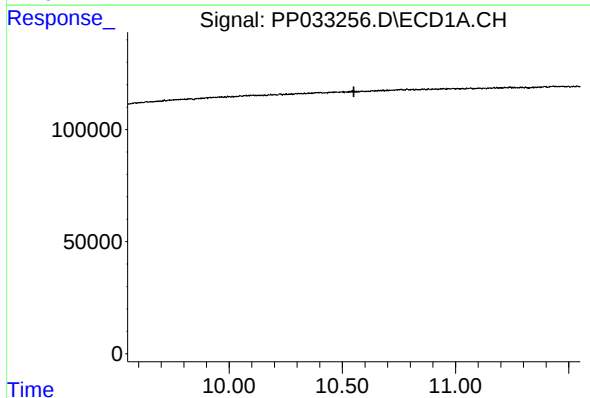


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.551 min
Response: 0
Conc: N.D.

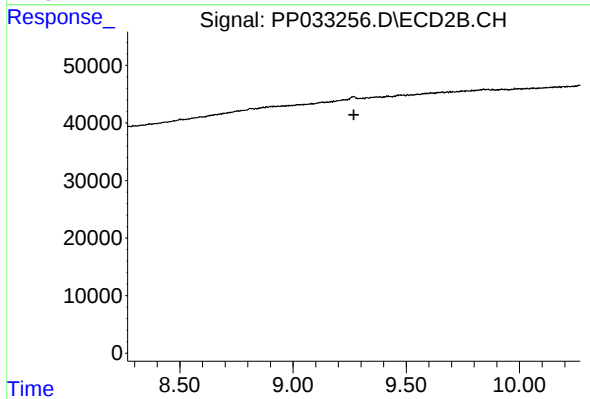

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.268 min
Response: 0
Conc: N.D.

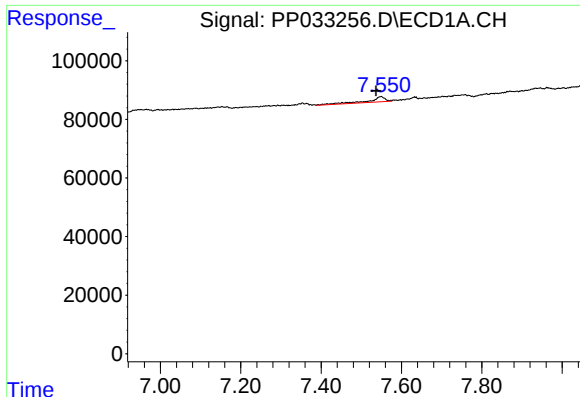

#28 AR-1254-3


R.T.: 7.549 min
Delta R.T.: 0.013 min
Response: 52319
Conc: 17.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

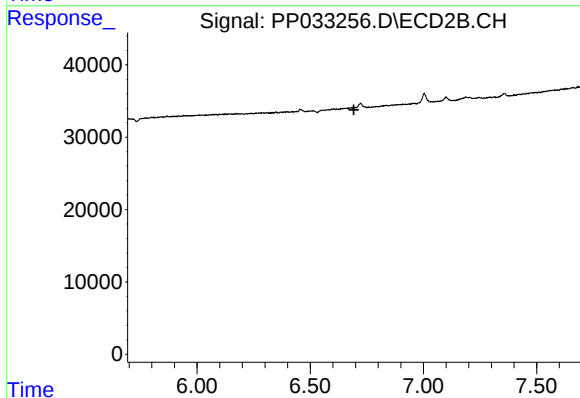


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

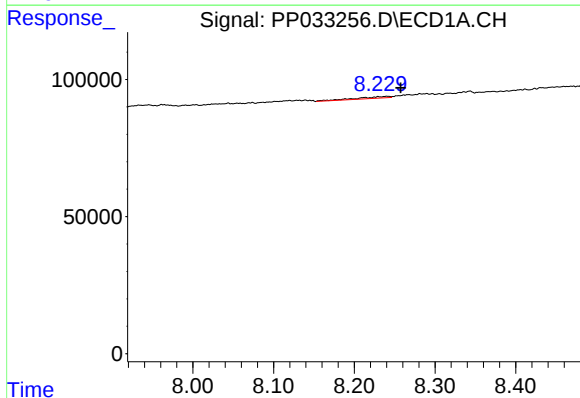


#30 AR-1254-5

R.T.: 8.241 min
Delta R.T.: -0.017 min
Response: 17859
Conc: 7.38 ng/ml

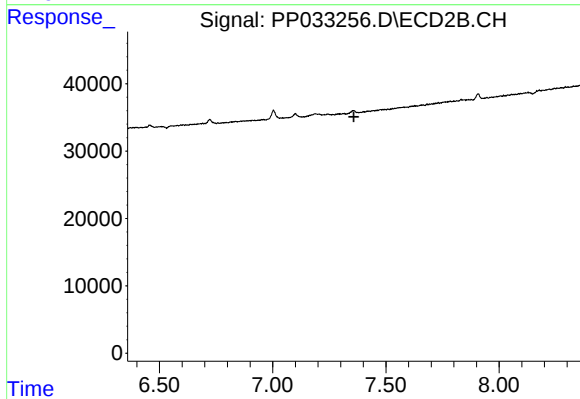

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

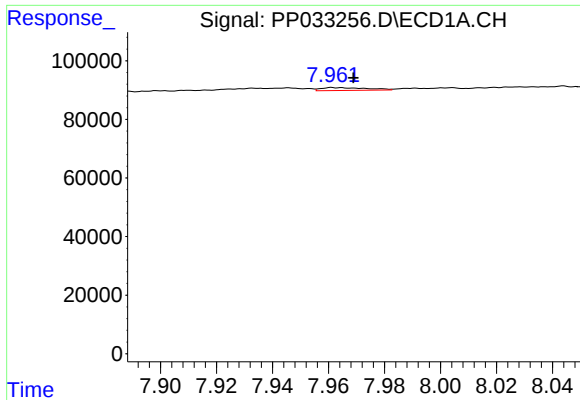

#32 AR-1260-2


R.T.: 7.962 min
Delta R.T.: -0.007 min
Response: 11222
Conc: 3.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

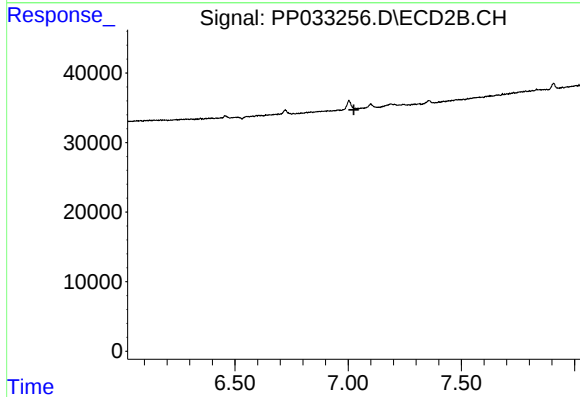


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

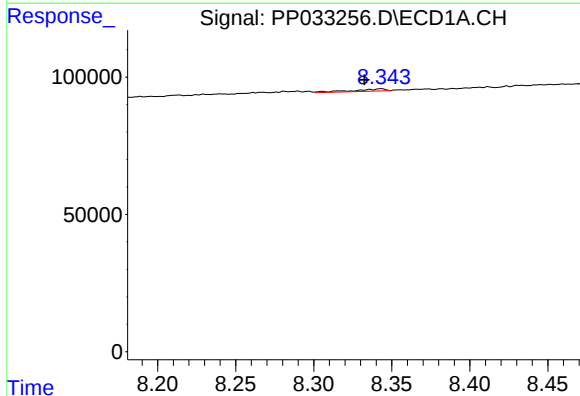


#33 AR-1260-3

R.T.: 8.343 min
Delta R.T.: 0.011 min
Response: 11852
Conc: 4.63 ng/ml

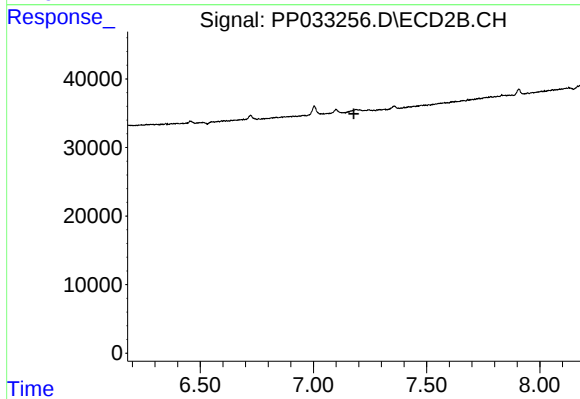

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.179 min
Response: 0
Conc: N.D.

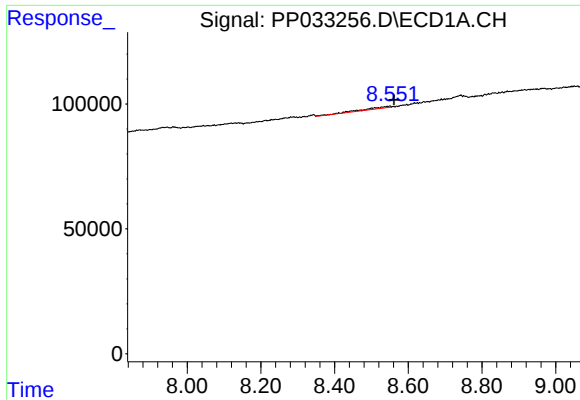

#34 AR-1260-4


R.T.: 8.550 min
Delta R.T.: -0.012 min
Response: 32833
Conc: 13.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

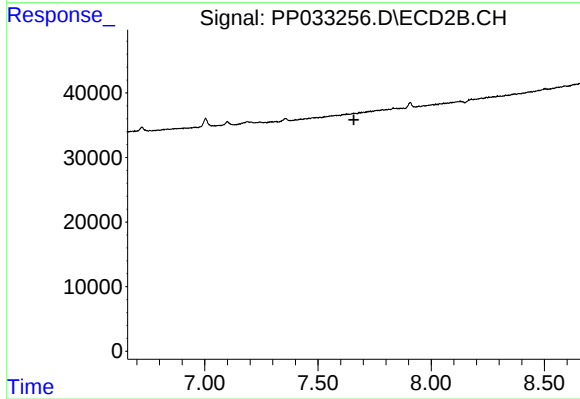


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

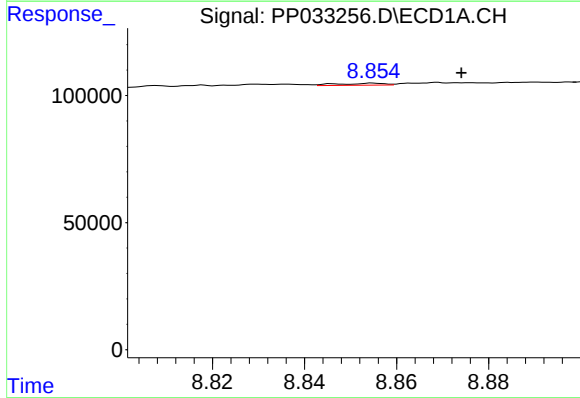


#35 AR-1260-5

R.T.: 8.855 min
Delta R.T.: -0.019 min
Response: 5610
Conc: 1.04 ng/ml

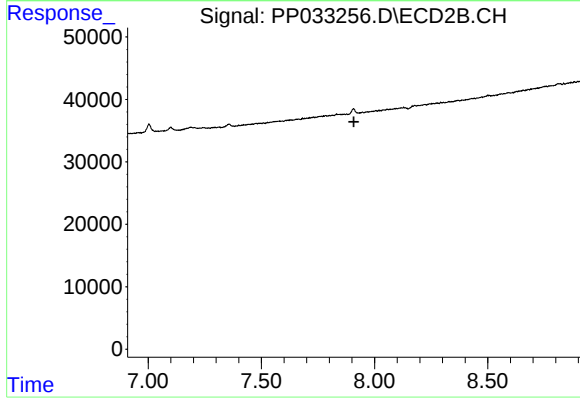

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.908 min
Response: 0
Conc: N.D.

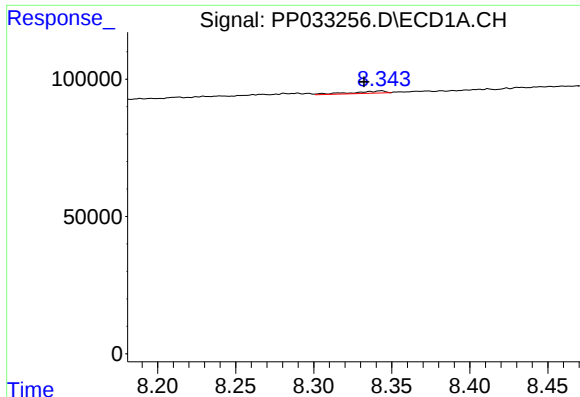

#36 AR-1262-1


R.T.: 8.343 min
Delta R.T.: 0.011 min
Response: 11852
Conc: 3.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

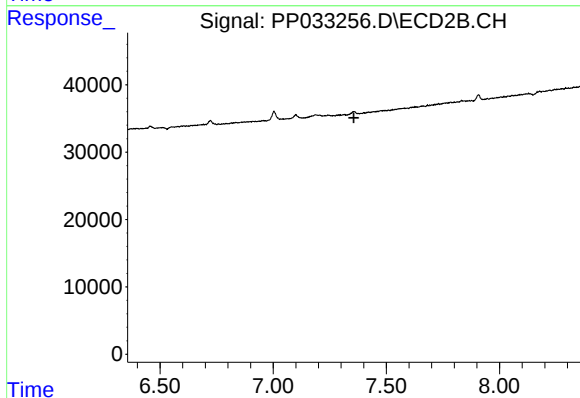


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

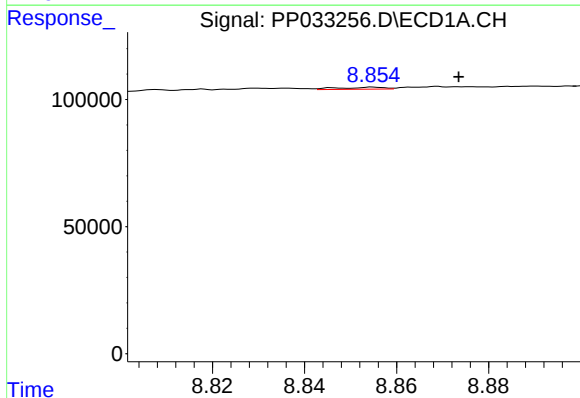

#37 AR-1262-2

R.T.: 8.855 min
Delta R.T.: -0.018 min
Response: 5610
Conc: 0.90 ng/ml

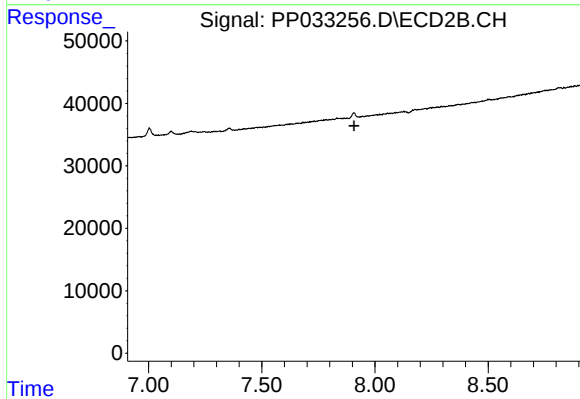

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.