

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
 Data File : PP033284.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2021 18:29
 Operator : DD\AJ
 Sample : M1333-01 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 01:01:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.727	4.000	171591	89994	2.798	2.201
2)	SA Decachlor...	10.545	9.262	104765	85336	2.405	2.547
Target Compounds							
27)	L6 AR-1254-2	7.175f	0.000	58620	0	19.995	N.D. #
28)	L6 AR-1254-3	7.548	0.000	125204	0	41.222	N.D. #
29)	L6 AR-1254-4	7.817	0.000	40633	0	17.565	N.D. #
30)	L6 AR-1254-5	8.277f	0.000	12939	0	5.347	N.D. #
32)	L7 AR-1260-2	7.962	0.000	62249	0	21.299	N.D. #
35)	L7 AR-1260-5	0.000	7.904	0	53591	N.D.	13.928 #
37)	L8 AR-1262-2	0.000	7.904	0	53591	N.D.	12.186 #
45)	L9 AR-1268-5	10.244	0.000	110249	0	6.735	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
Data File : PP033284.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2021 18:29
Operator : DD\AJ
Sample : M1333-01 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 01:01:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

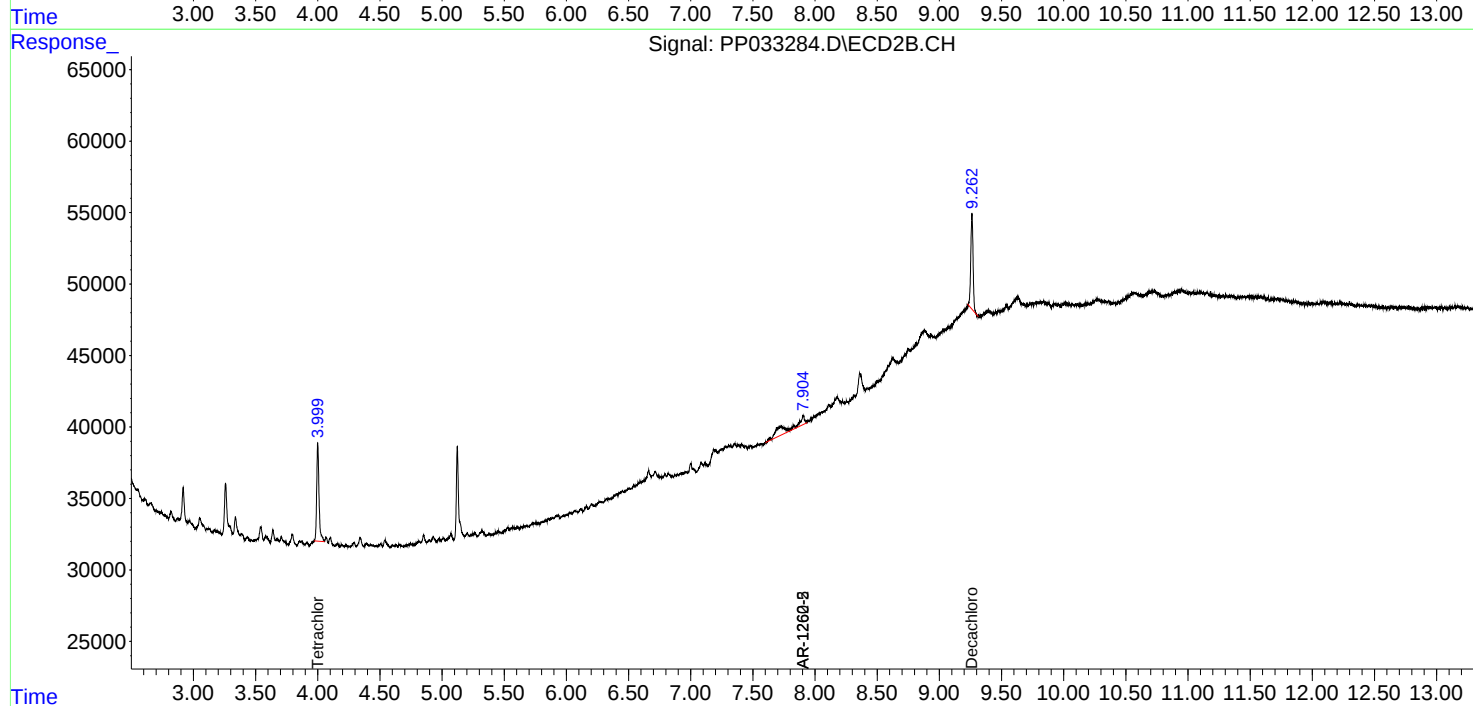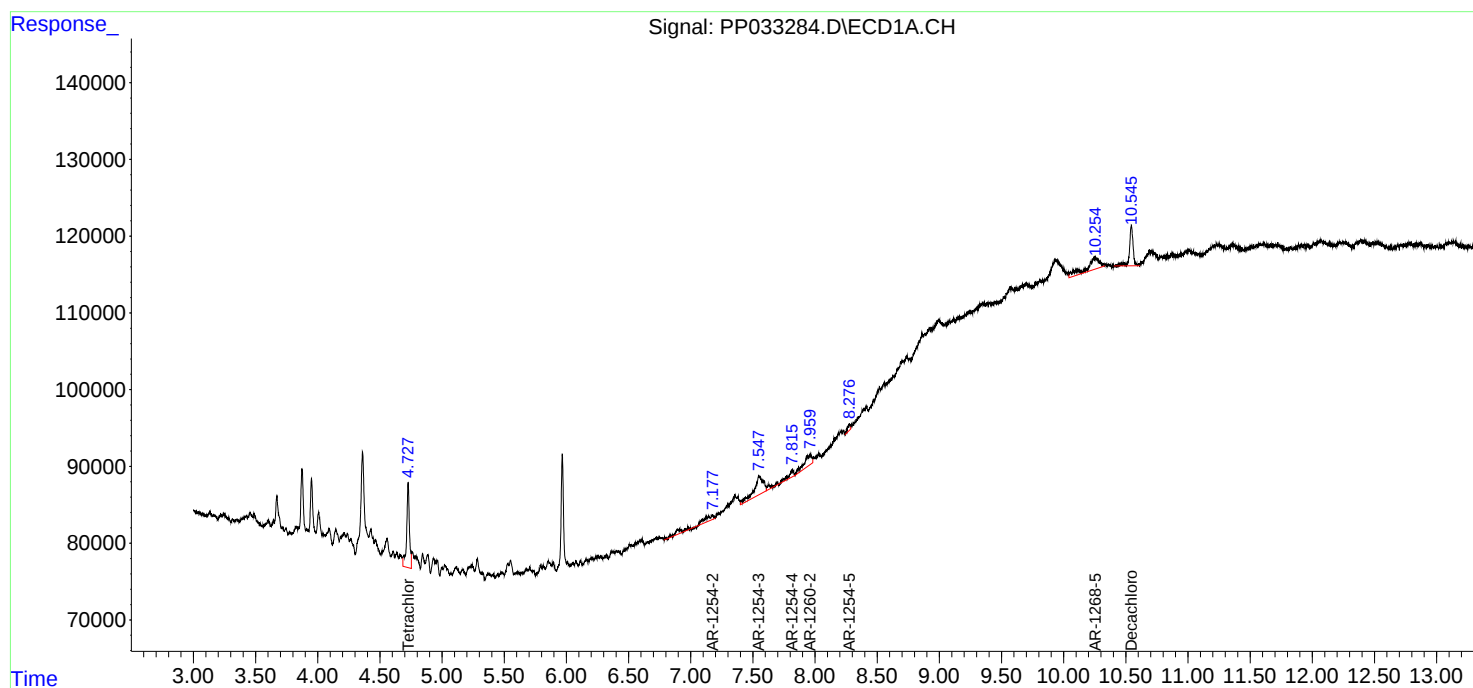


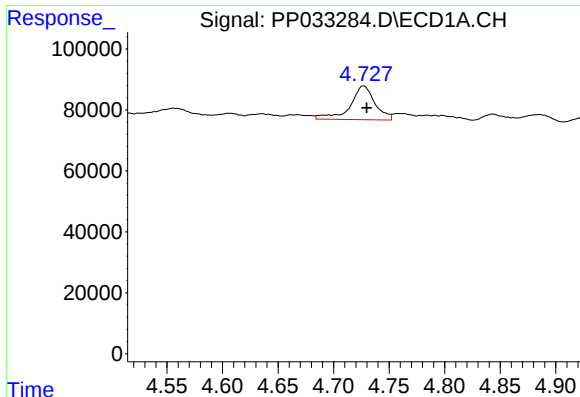

#1 Tetrachloro-m-xylene


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 171591
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :

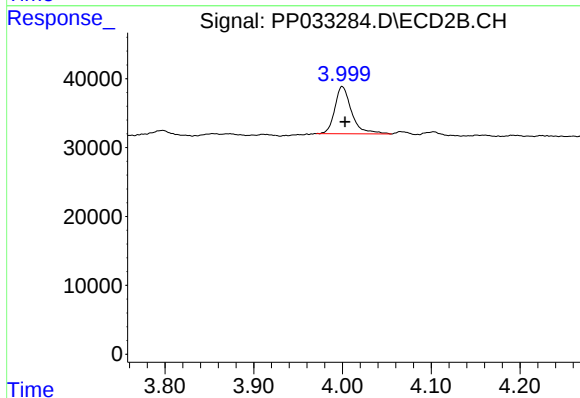


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 89994
Conc: 2.20 ng/ml

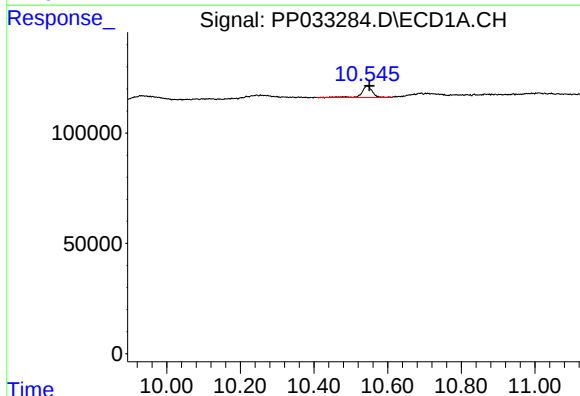


#2 Decachlorobiphenyl

R.T.: 10.545 min
Delta R.T.: -0.006 min
Response: 104765
Conc: 2.41 ng/ml

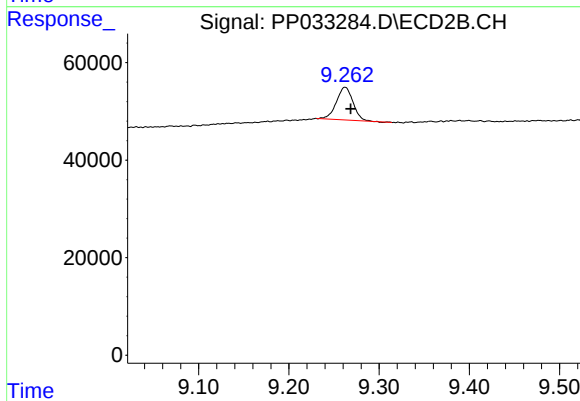

#2 Decachlorobiphenyl


R.T.: 9.262 min
Delta R.T.: -0.006 min
Response: 85336
Conc: 2.55 ng/ml

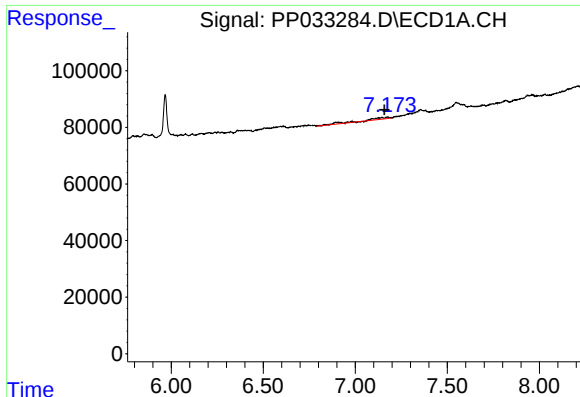

#27 AR-1254-2


R.T.: 7.175 min
Delta R.T.: 0.016 min
Response: 58620
Conc: 20.00 ng/ml

Instrument :
ECD_P
ClientSampleId :

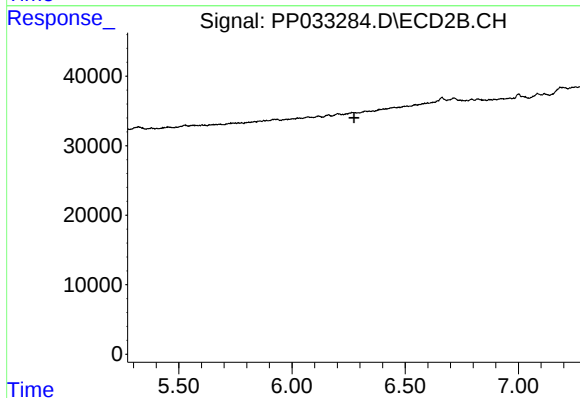


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.274 min
Response: 0
Conc: N.D.

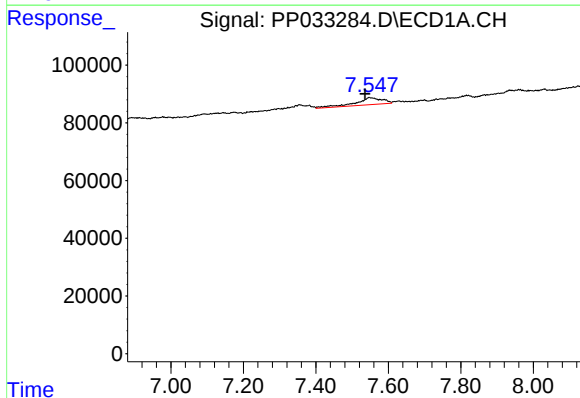


#28 AR-1254-3

R.T.: 7.548 min
Delta R.T.: 0.011 min
Response: 125204
Conc: 41.22 ng/ml

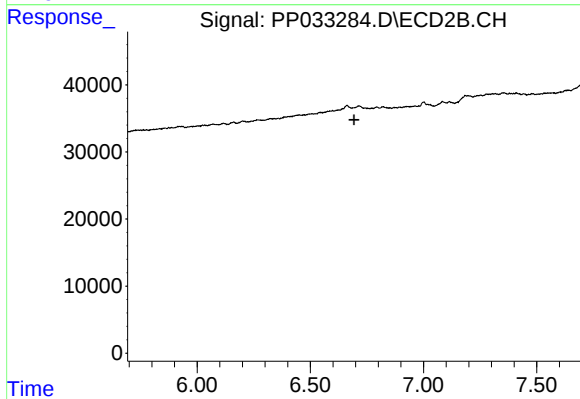

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

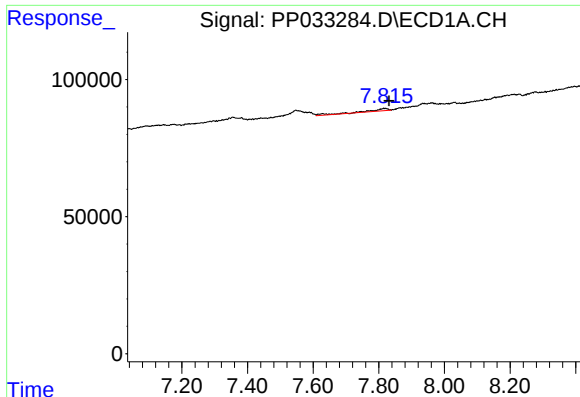

#29 AR-1254-4


R.T.: 7.817 min
Delta R.T.: -0.014 min
Response: 40633
Conc: 17.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

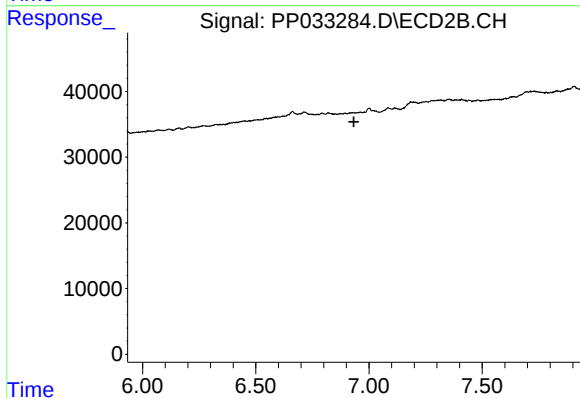


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

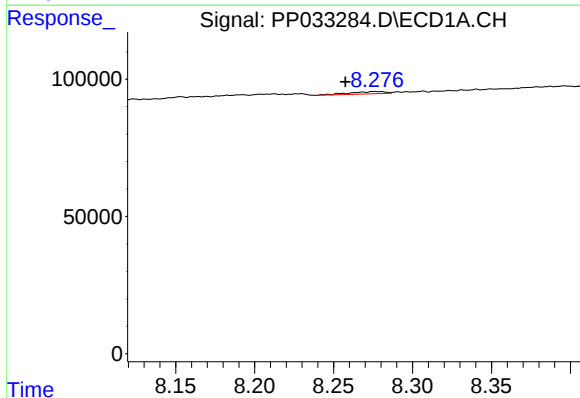


#30 AR-1254-5

R.T.: 8.277 min
Delta R.T.: 0.020 min
Response: 12939
Conc: 5.35 ng/ml

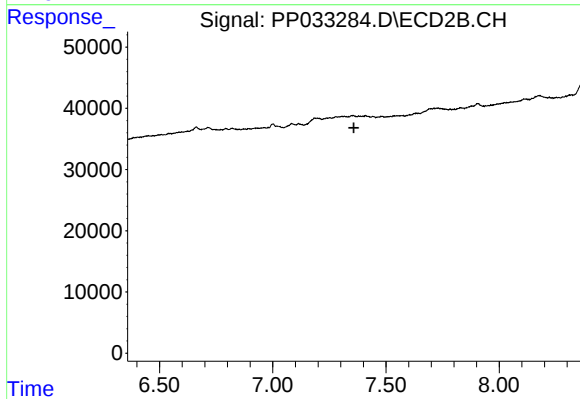

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

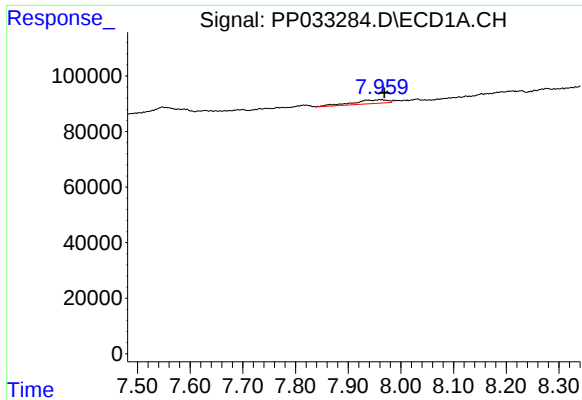

#32 AR-1260-2


R.T.: 7.962 min
Delta R.T.: -0.007 min
Response: 62249
Conc: 21.30 ng/ml

Instrument :
ECD_P
ClientSampleId :

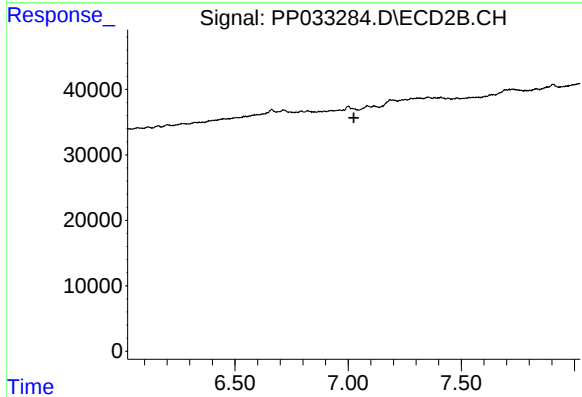


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

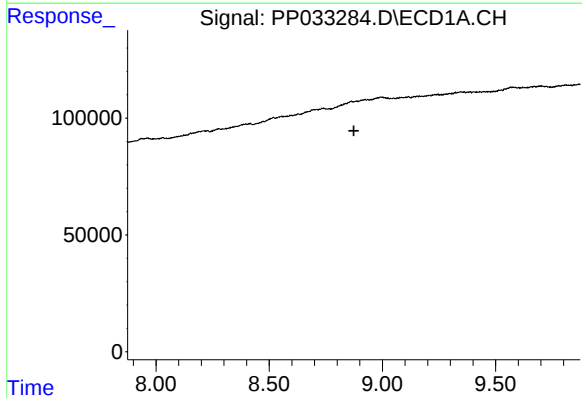


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.874 min
Response: 0
Conc: N.D.

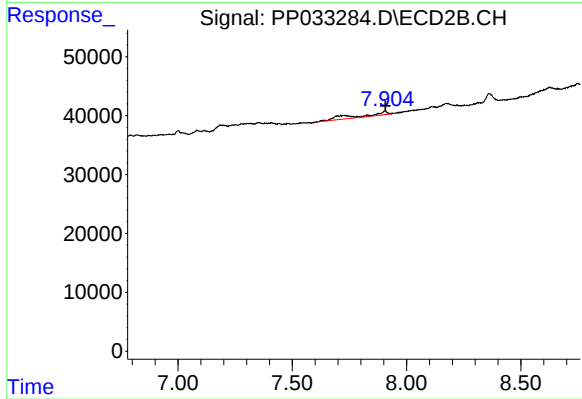

#35 AR-1260-5


R.T.: 7.904 min
Delta R.T.: -0.004 min
Response: 53591
Conc: 13.93 ng/ml

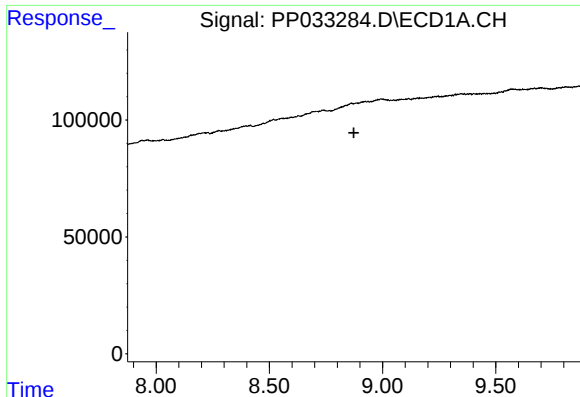

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

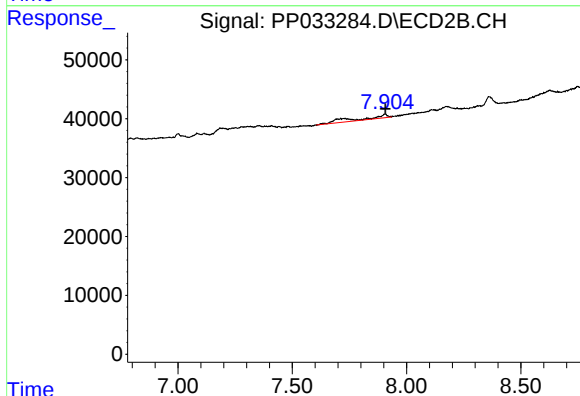


#37 AR-1262-2

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 53591
Conc: 12.19 ng/ml

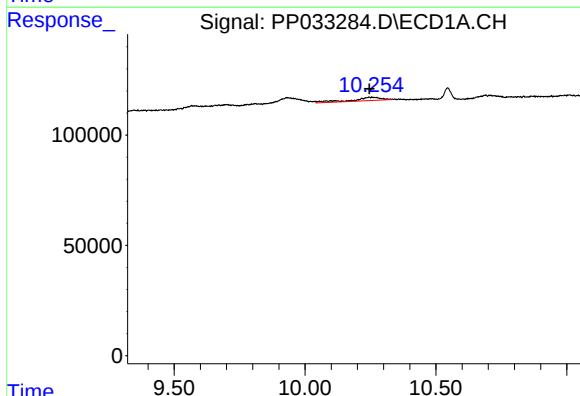

#45 AR-1268-5

R.T.: 10.244 min
Delta R.T.: -0.001 min
Response: 110249
Conc: 6.73 ng/ml

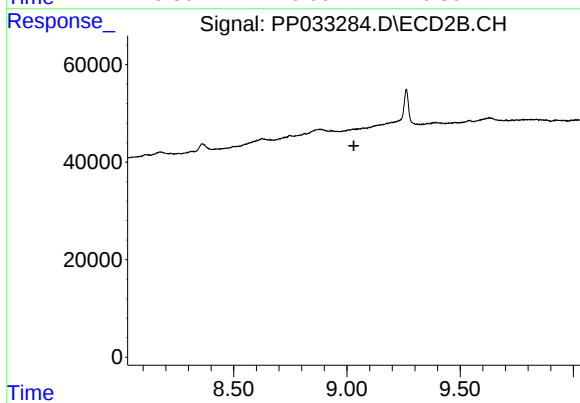

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.031 min
Response: 0
Conc: N.D.