

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
 Data File : PP033285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2021 18:46
 Operator : DD\AJ
 Sample : PB134580BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 01:01:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.727	4.000	1395906	946565	22.763	23.148
2)	SA Decachlor...	10.546	9.262	1041046	865732	23.899	25.843
Target Compounds							
28)	L6 AR-1254-3	7.548	0.000	39387	0	12.968	N.D. #
29)	L6 AR-1254-4	7.824	0.000	14071	0	6.083	N.D. #
31)	L7 AR-1260-1	7.726f	0.000	11638	0	5.316	N.D. #
32)	L7 AR-1260-2	7.952f	0.000	9326	0	3.191	N.D. #
34)	L7 AR-1260-4	8.549	0.000	6864	0	2.809	N.D. #
35)	L7 AR-1260-5	8.862	0.000	8847	0	1.644	N.D. #
37)	L8 AR-1262-2	8.862	0.000	8847	0	1.413	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
Data File : PP033285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2021 18:46
Operator : DD\AJ
Sample : PB134580BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 01:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

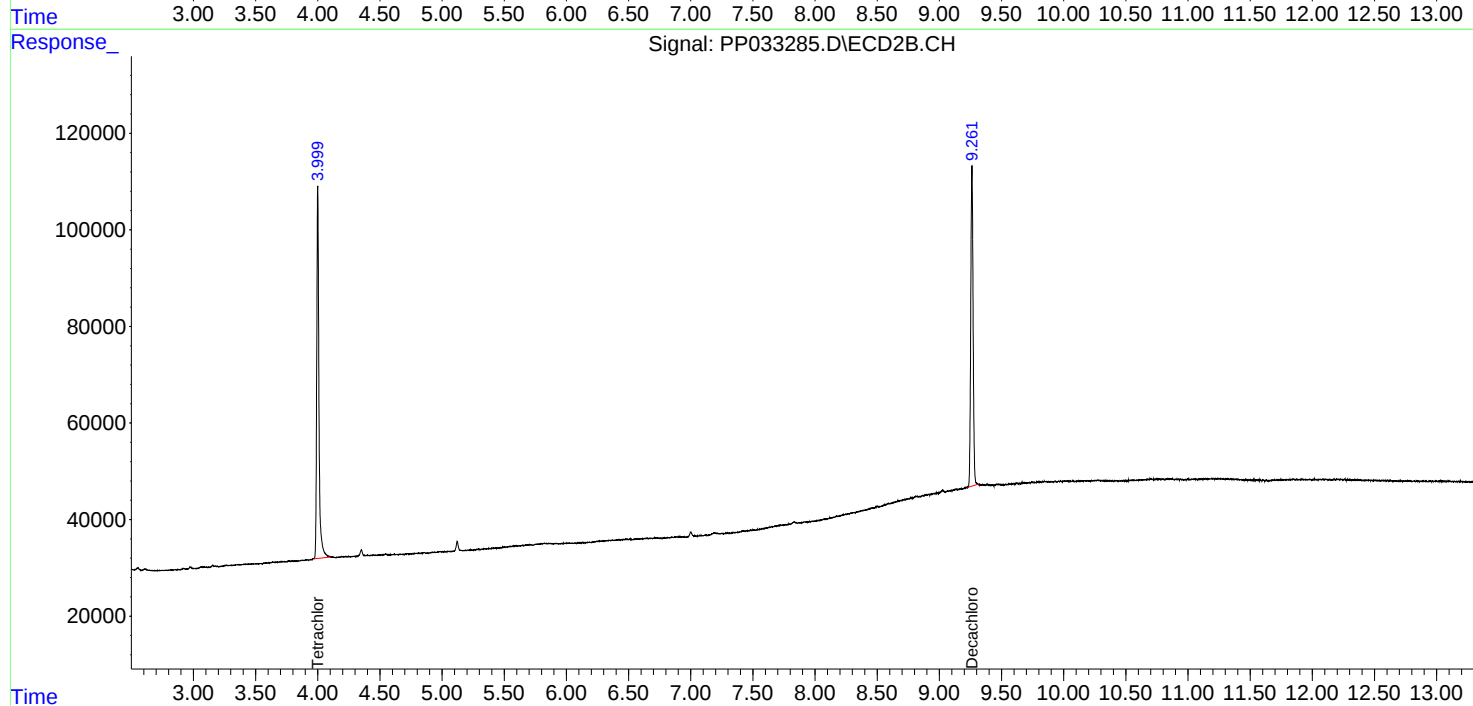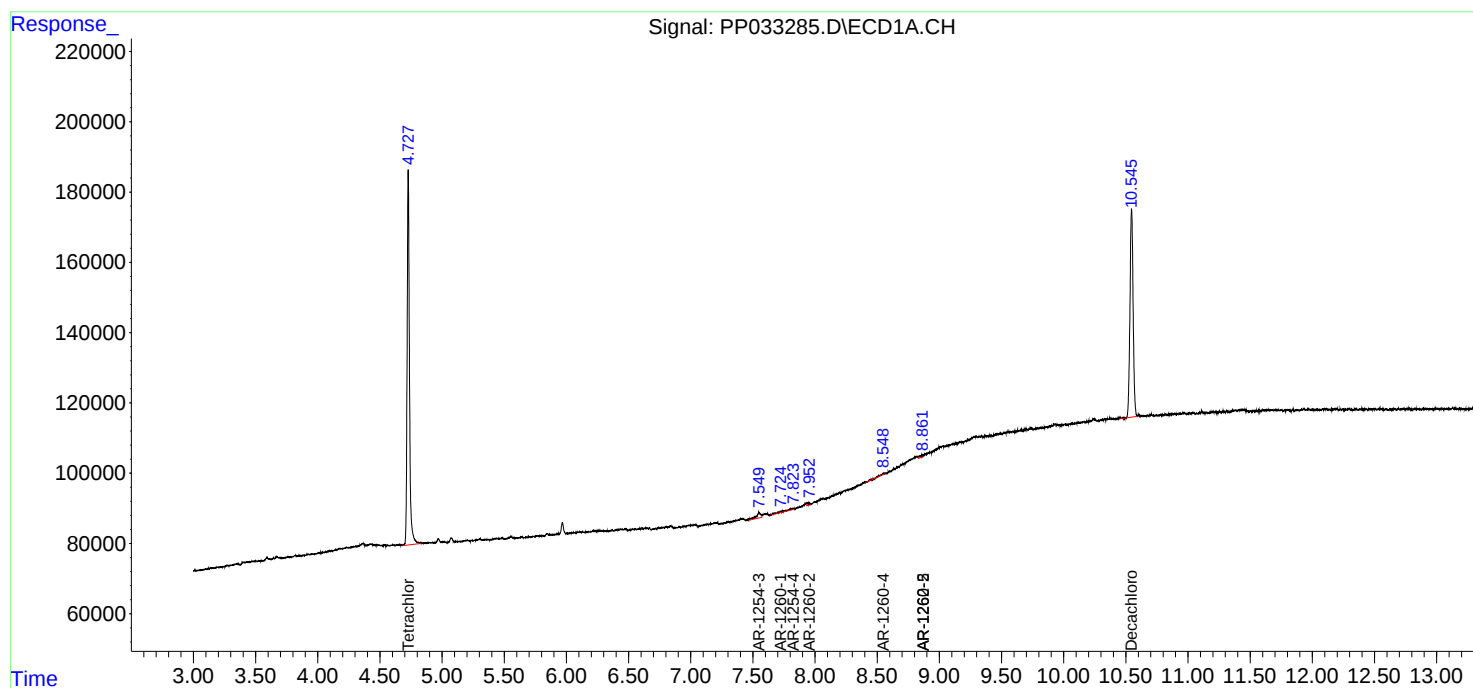


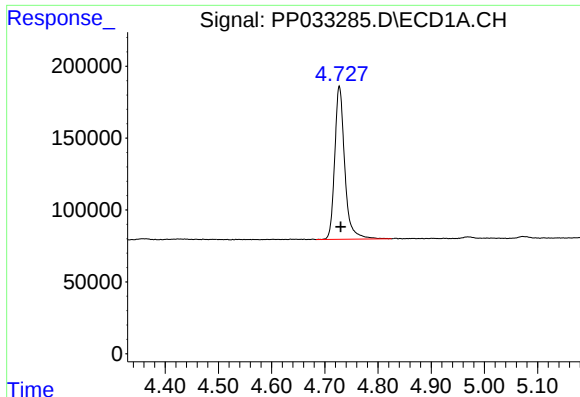

#1 Tetrachloro-m-xylene


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 1395906
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

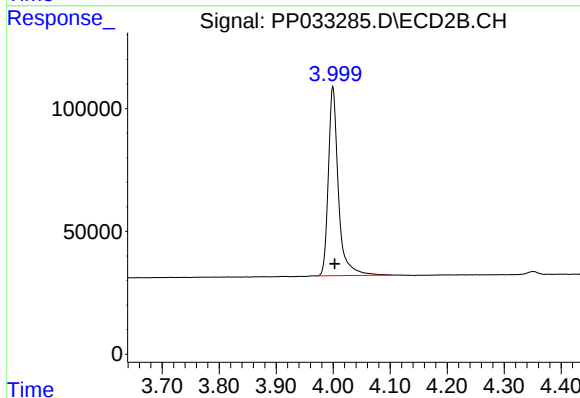


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 946565
Conc: 23.15 ng/ml

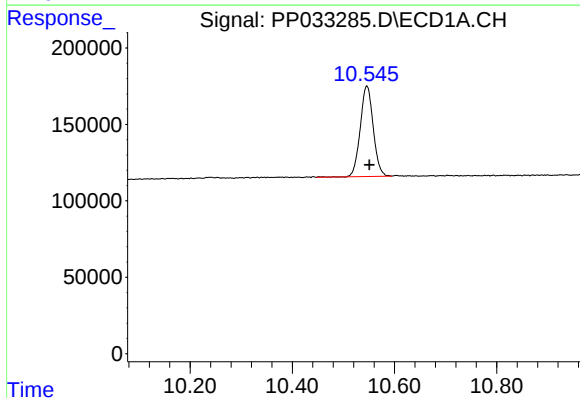


#2 Decachlorobiphenyl

R.T.: 10.546 min
Delta R.T.: -0.005 min
Response: 1041046
Conc: 23.90 ng/ml

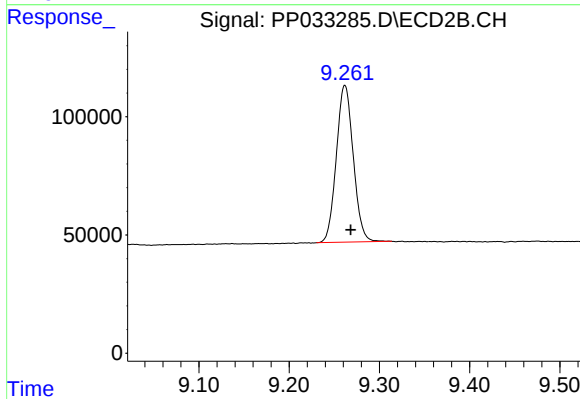

#2 Decachlorobiphenyl


R.T.: 9.262 min
Delta R.T.: -0.007 min
Response: 865732
Conc: 25.84 ng/ml

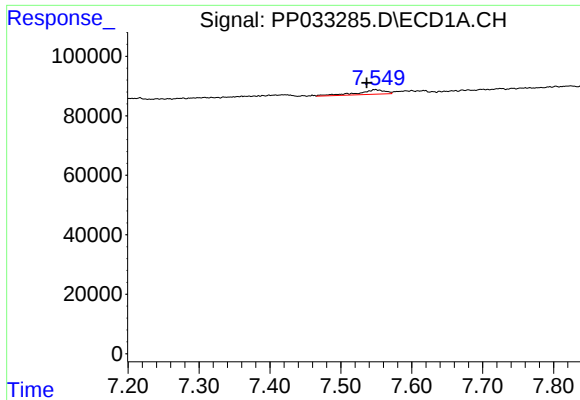

#28 AR-1254-3


R.T.: 7.548 min
Delta R.T.: 0.012 min
Response: 39387
Conc: 12.97 ng/ml

Instrument :
ECD_P
ClientSampleId :

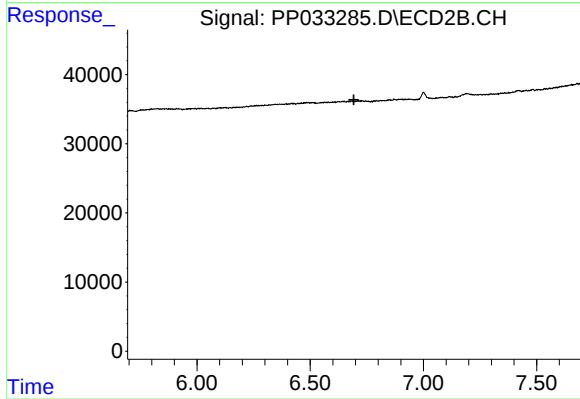


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

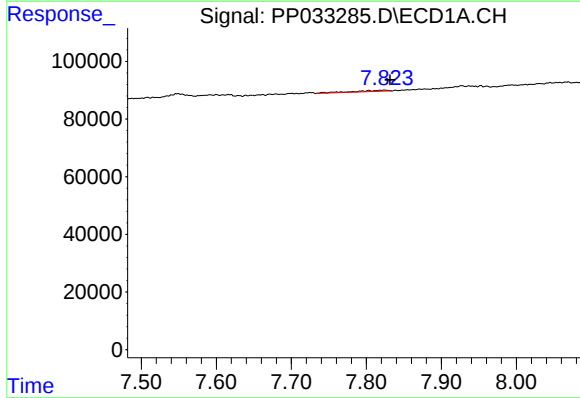


#29 AR-1254-4

R.T.: 7.824 min
Delta R.T.: -0.007 min
Response: 14071
Conc: 6.08 ng/ml

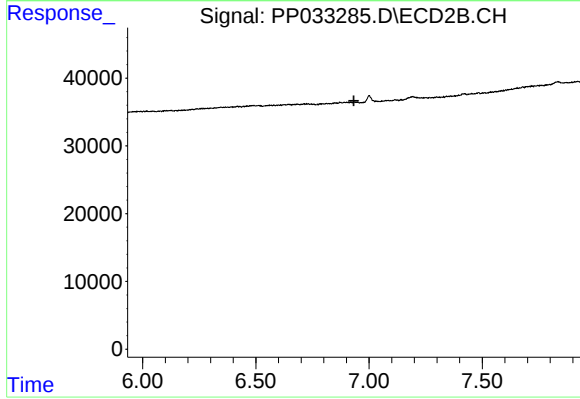

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

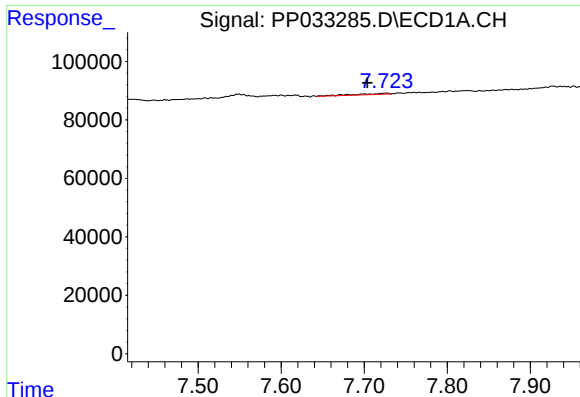

#31 AR-1260-1


R.T.: 7.726 min
Delta R.T.: 0.022 min
Response: 11638
Conc: 5.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

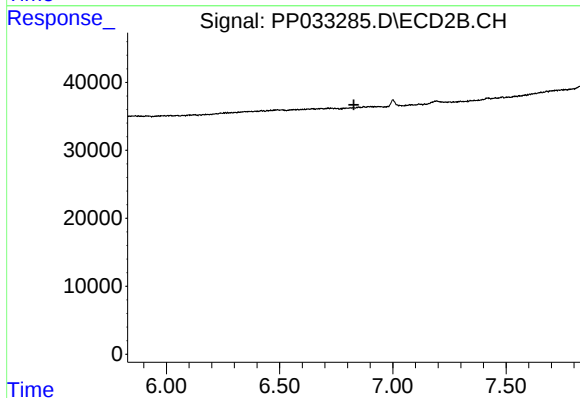


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.828 min
Response: 0
Conc: N.D.

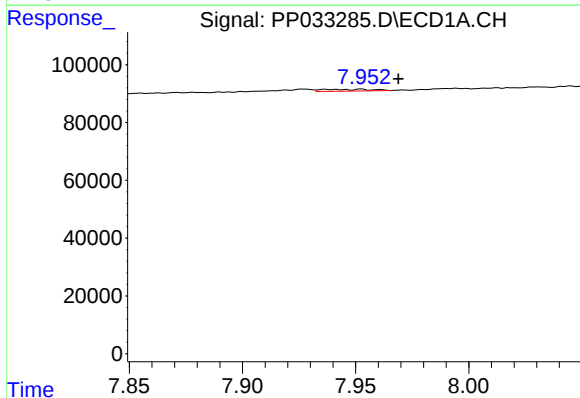


#32 AR-1260-2

R.T.: 7.952 min
Delta R.T.: -0.017 min
Response: 9326
Conc: 3.19 ng/ml

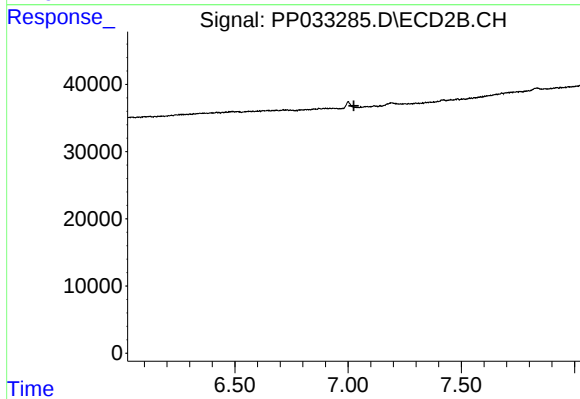

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

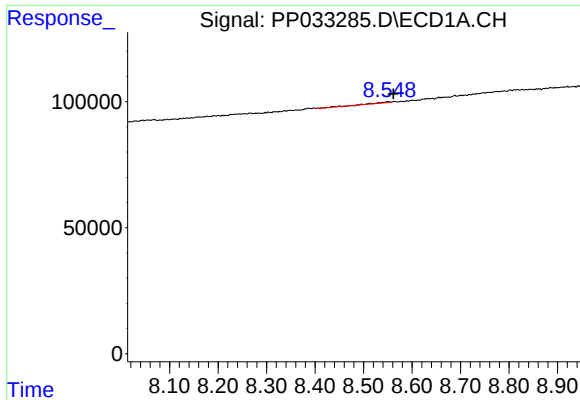

#34 AR-1260-4


R.T.: 8.549 min
Delta R.T.: -0.012 min
Response: 6864
Conc: 2.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

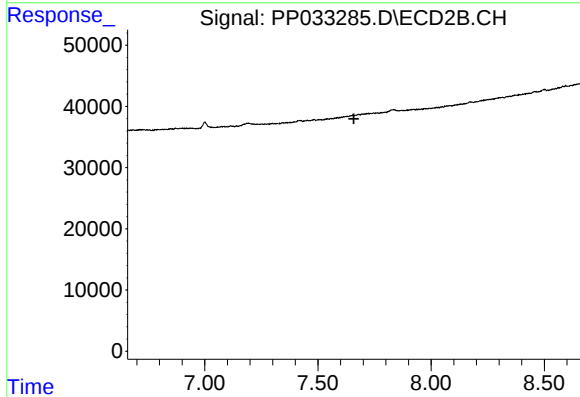


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

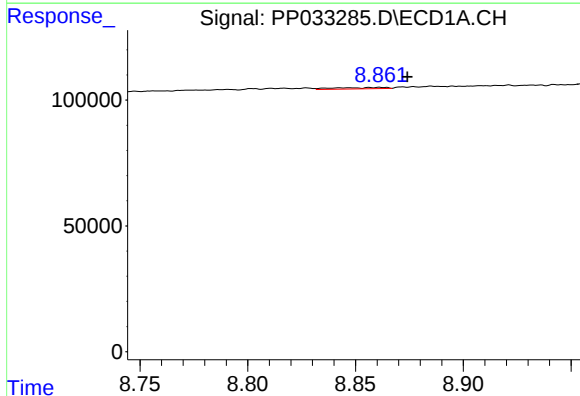


#35 AR-1260-5

R.T.: 8.862 min
Delta R.T.: -0.012 min
Response: 8847
Conc: 1.64 ng/ml

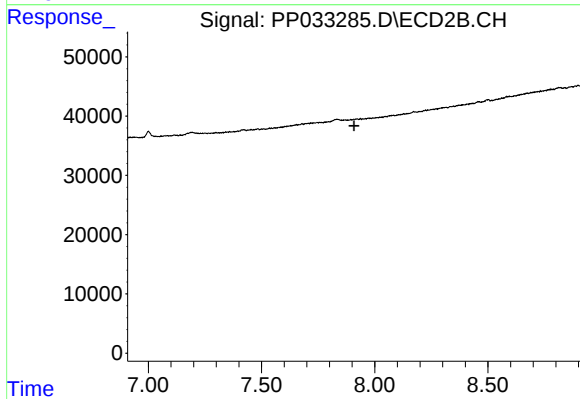

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.908 min
Response: 0
Conc: N.D.

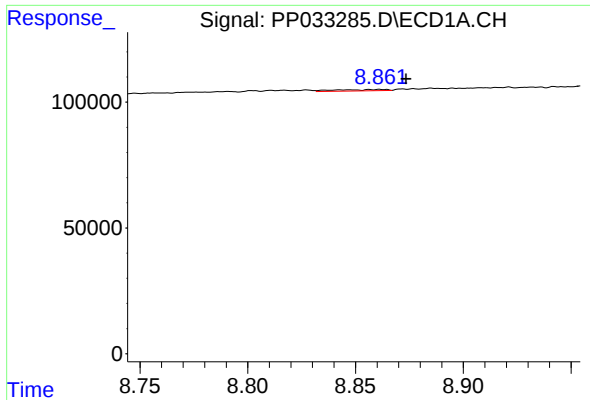

#37 AR-1262-2

R.T.: 8.862 min
Delta R.T.: -0.012 min
Response: 8847
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

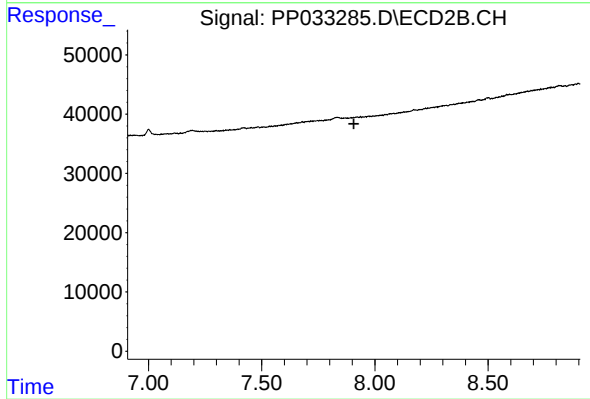

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.