

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
 Data File : PP033272.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2021 14:49
 Operator : DD\AJ
 Sample : M1368-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EXTERIOR-PAINT-CHIPS

Manual Integrations
 APPROVED

Ankita
 2/12/2021 10:10:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 00:54:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.727	4.000	145087	90522	2.366	2.214
2) SA Decachlor...	10.546	9.264	128477	110623	2.949	3.302
Target Compounds						
26) L6 AR-1254-1	6.931	6.114	46384	51839	24.705m	27.125
27) L6 AR-1254-2	7.159	6.270	75526	28823	25.761	17.579 #
28) L6 AR-1254-3	7.538	6.690	116305	40790	38.292	15.177 #
29) L6 AR-1254-4	7.827	6.929	50042	28058	21.633m	18.792m
30) L6 AR-1254-5	8.279f	7.355	224224	134425	92.663	55.516 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021121\
Data File : PP033272.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2021 14:49
Operator : DD\AJ
Sample : M1368-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EXTERIOR-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
2/12/2021 10:10:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 00:54:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

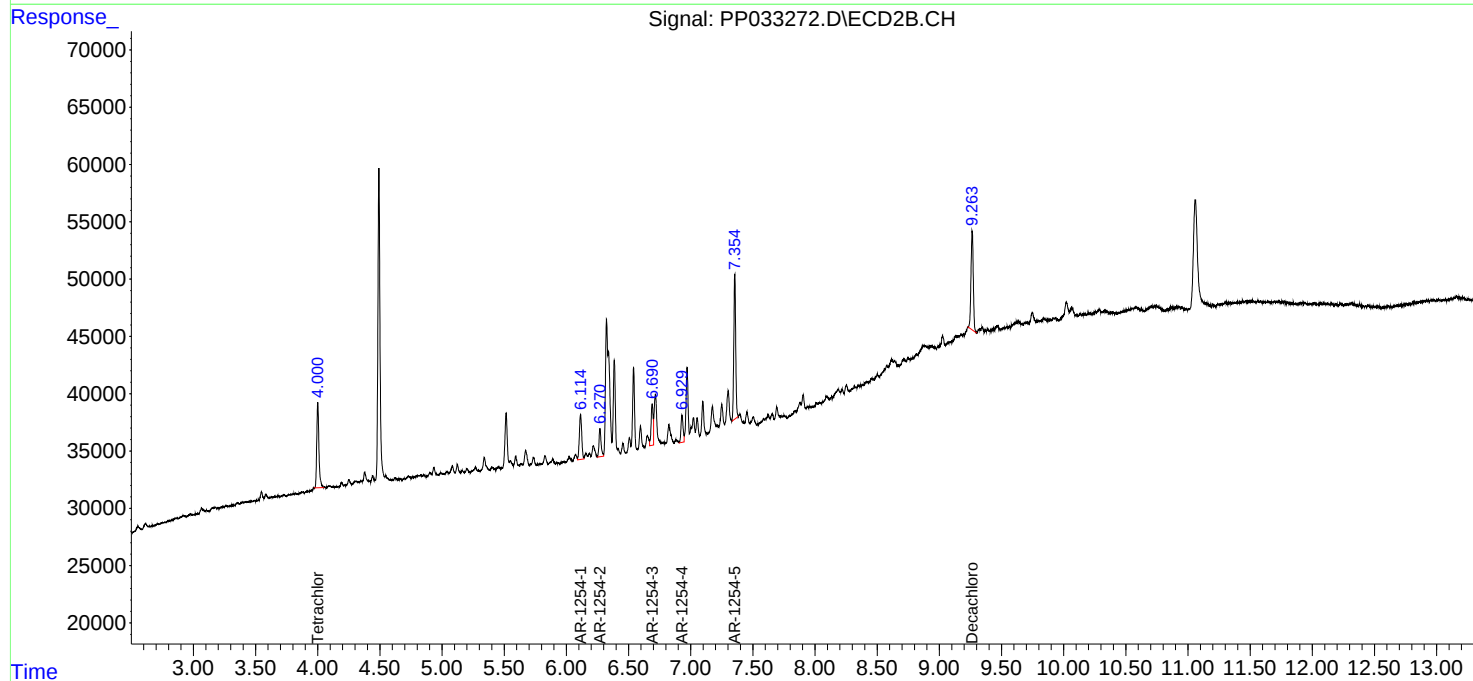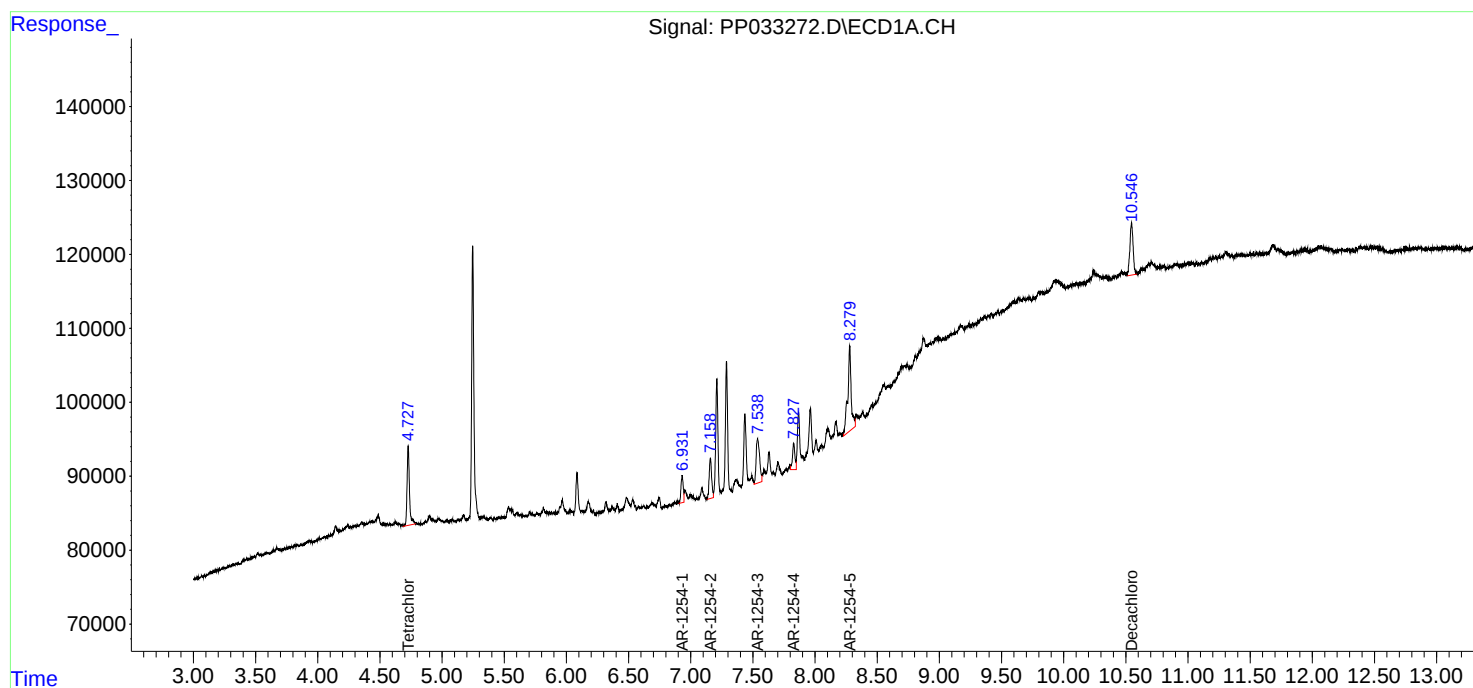

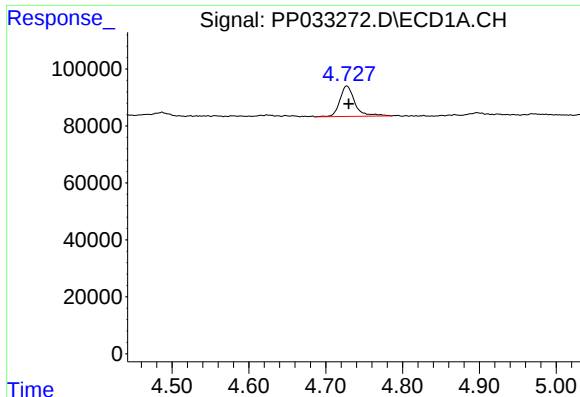


#1 Tetrachloro-m-xylene

R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 145087
Conc: 2.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
EXTERIOR-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
2/12/2021 10:10:37 AM

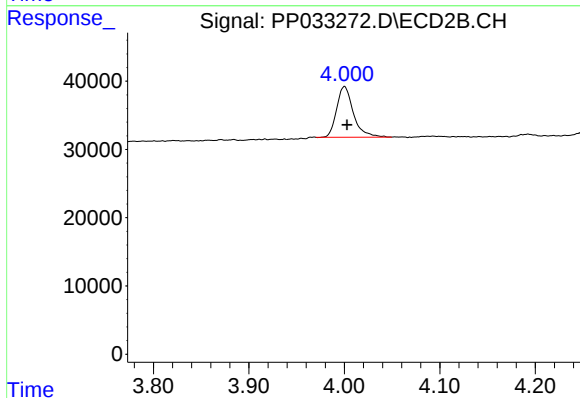


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 90522
Conc: 2.21 ng/ml

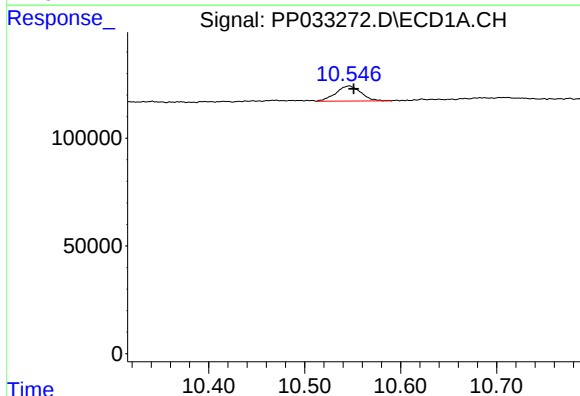


#2 Decachlorobiphenyl

R.T.: 10.546 min
Delta R.T.: -0.005 min
Response: 128477
Conc: 2.95 ng/ml

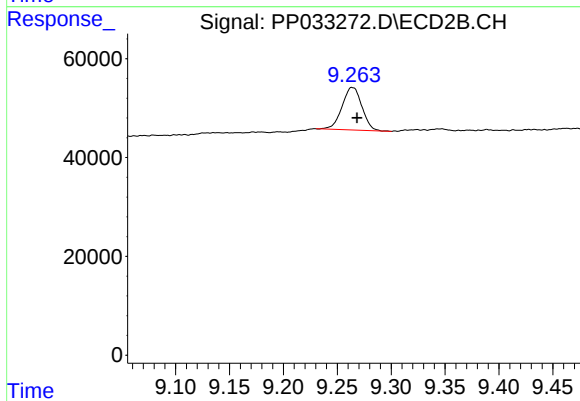

#2 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.004 min
Response: 110623
Conc: 3.30 ng/ml

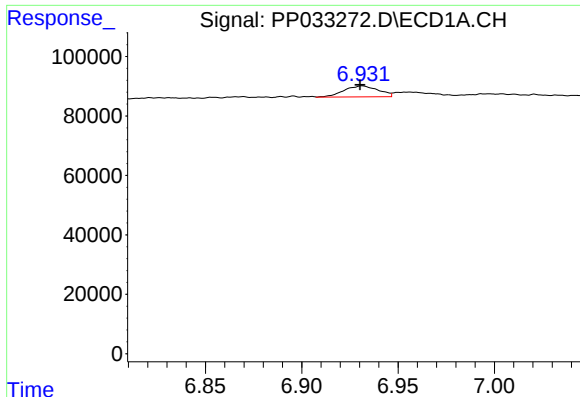


#26 AR-1254-1

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 46384
Conc: 24.70 ng/ml m

Instrument :
ECD_P
ClientSampleId :
EXTERIOR-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
2/12/2021 10:10:37 AM

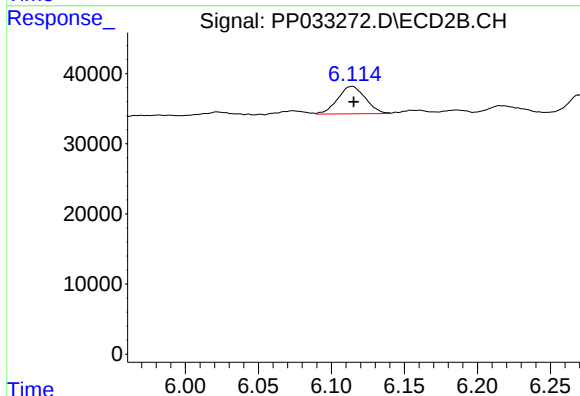


#26 AR-1254-1

R.T.: 6.114 min
Delta R.T.: -0.001 min
Response: 51839
Conc: 27.12 ng/ml

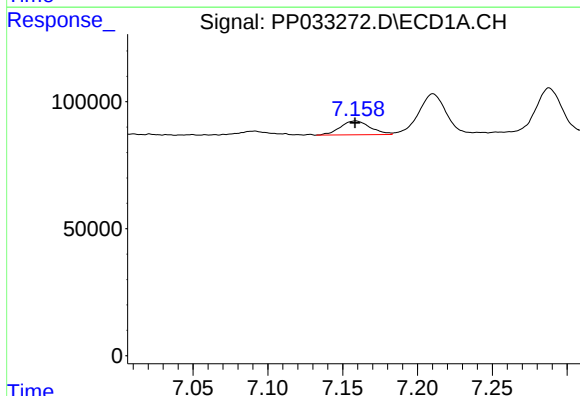


#27 AR-1254-2

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 75526
Conc: 25.76 ng/ml

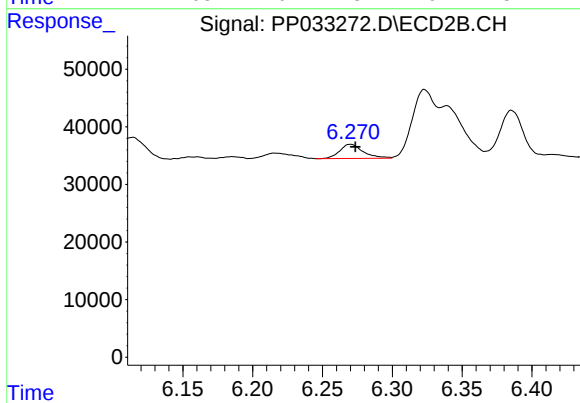

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.004 min
Response: 28823
Conc: 17.58 ng/ml

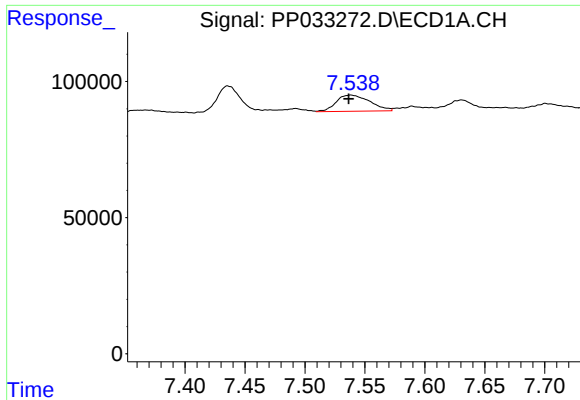


#28 AR-1254-3

R.T.: 7.538 min
Delta R.T.: 0.002 min
Response: 116305
Conc: 38.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
EXTERIOR-PAINT-CHIPS


Manual Integrations
APPROVED

Ankita
2/12/2021 10:10:37 AM

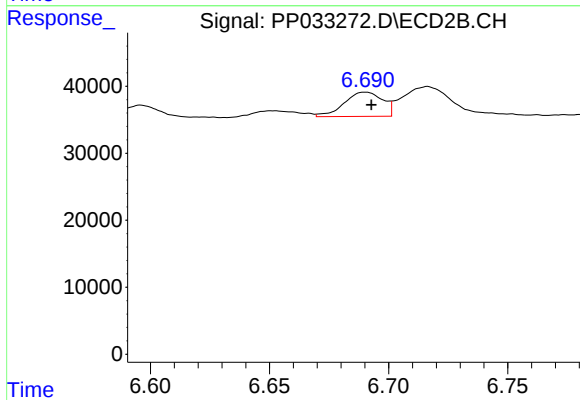


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.003 min
Response: 40790
Conc: 15.18 ng/ml

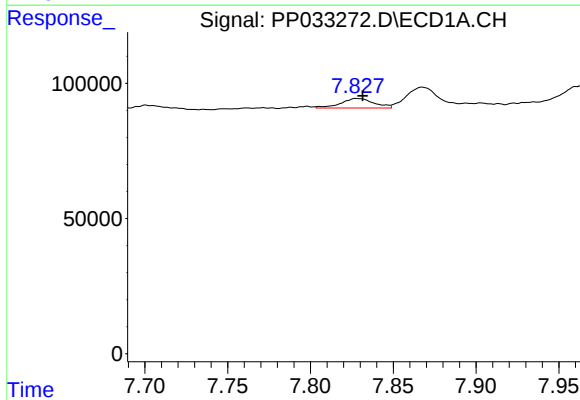


#29 AR-1254-4

R.T.: 7.827 min
Delta R.T.: -0.005 min
Response: 50042
Conc: 21.63 ng/ml m

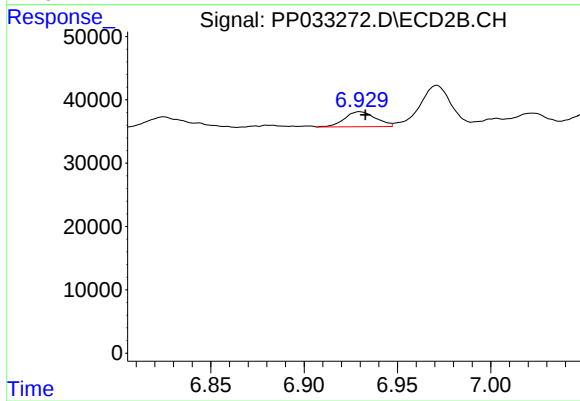

#29 AR-1254-4


R.T.: 6.929 min
Delta R.T.: -0.003 min
Response: 28058
Conc: 18.79 ng/ml m

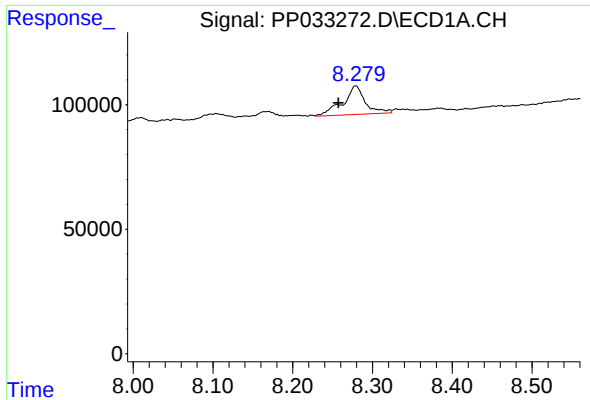

#30 AR-1254-5

R.T.: 8.279 min
Delta R.T.: 0.022 min
Response: 224224
Conc: 92.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
EXTERIOR-PAINT-CHIPS

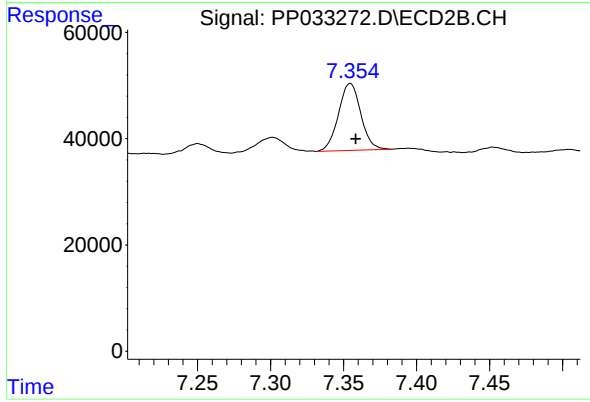

#30 AR-1254-5

R.T.: 7.355 min
Delta R.T.: -0.004 min
Response: 134425
Conc: 55.52 ng/ml

Manual Integrations
APPROVED

Ankita
2/12/2021 10:10:37 AM