

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:16
 Operator : YP\AJ
 Sample : N1523-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:23:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.919	3.174	46631732	44081487	21.090	23.469
2)	SA Decachlor...	10.071	8.554	27367984	35066701	23.039	21.614
Target Compounds							
3)	L1 AR-1016-1	5.170	4.342f	237526	523228	3.273	8.540 #
4)	L1 AR-1016-2	5.201	4.342	409892	523228	3.886	6.193 #
5)	L1 AR-1016-3	5.250	4.511f	642082	107107	9.751	2.293 #
6)	L1 AR-1016-4	5.340f	4.598f	1954416	128842	36.039	3.448 #
7)	L1 AR-1016-5	5.688	4.802	360542	118926	6.864	2.603 #
8)	L2 AR-1221-1	4.137	3.406	881820	603615	34.636	25.305 #
9)	L2 AR-1221-2	4.243	3.487	718186	1295140	37.409	71.713 #
10)	L2 AR-1221-3	4.332	3.571	364990	1072217	6.354	20.784 #
11)	L3 AR-1232-1	4.332	3.571	364990	1072217	7.521	24.921 #
12)	L3 AR-1232-2	4.863f	4.342	2264409	523228	95.556	14.657 #
13)	L3 AR-1232-3	5.201	4.511f	409892	107107	9.520	5.477 #
14)	L3 AR-1232-4	5.340f	4.615	1954416	224991	89.536	13.011 #
15)	L3 AR-1232-5	5.477	4.802	198351	118926	12.298	6.331 #
16)	L4 AR-1242-1	5.170	4.342f	237526	523228	4.227	10.733 #
17)	L4 AR-1242-2	5.201	4.342	409892	523228	4.954	7.771 #
18)	L4 AR-1242-3	5.250	4.511f	642082	107107	12.405	2.853 #
19)	L4 AR-1242-4	5.340f	4.615	1954416	224991	45.758	6.231 #
20)	L4 AR-1242-5	6.162	5.183	132087	1113469	3.059	25.866 #
21)	L5 AR-1248-1	5.170	4.342f	237526	523228	5.794	14.046 #
22)	L5 AR-1248-2	5.477	4.598f	198351	128842	3.491	2.634
23)	L5 AR-1248-3	5.688	4.615	360542	224991	5.404	4.384
24)	L5 AR-1248-4	0.000	4.802	0	118926	N.D.	2.029 #
25)	L5 AR-1248-5	6.162	5.216	132087	152749	1.911	2.666 #
26)	L6 AR-1254-1	6.082f	5.183	604394	1113469	7.999	12.750 #
27)	L6 AR-1254-2	6.348	5.339	627663	183463	5.596	2.405 #
28)	L6 AR-1254-3	6.740	0.000	564782	0	4.881	N.D. #
29)	L6 AR-1254-4	7.061	6.021	445468	318433	5.580	4.035 #
30)	L6 AR-1254-5	7.514	6.493f	463194	2133347	5.401	18.447 #
31)	L7 AR-1260-1	6.895f	5.909	2200126	546586	26.273	6.835 #
32)	L7 AR-1260-2	7.202	6.119	213601	520914	2.360	5.334 #
33)	L7 AR-1260-3	7.593	6.282	1017893	323364	14.042	3.542 #
34)	L7 AR-1260-4	7.827f	6.794	2913537	223395	33.935	2.761 #
35)	L7 AR-1260-5	8.200	7.061	340167	152777	2.195	0.826 #
36)	L8 AR-1262-1	7.593	6.493f	1017893	2133347	10.309	19.406 #
37)	L8 AR-1262-2	8.200	6.794	340167	223395	2.107	2.190
38)	L8 AR-1262-3	8.524	7.347f	905112	3064554	8.273	35.959 #
39)	L8 AR-1262-4	8.627	7.444	532520	183551	11.104	1.182 #
40)	L8 AR-1262-5	0.000	7.976	0	16796	N.D.	0.216 #
41)	L9 AR-1268-1	8.524	7.347f	905112	3064554	4.643	12.096 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:16
 Operator : YP\AJ
 Sample : N1523-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:23:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.627	7.444	532520	183551	3.042	0.812 #
43) L9	AR-1268-3	0.000	7.671	0	1249666	N.D.	6.417 #
44) L9	AR-1268-4	0.000	7.976	0	16796	N.D.	0.187 #
45) L9	AR-1268-5	9.733	8.290	1832085	326112	4.032	0.543 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

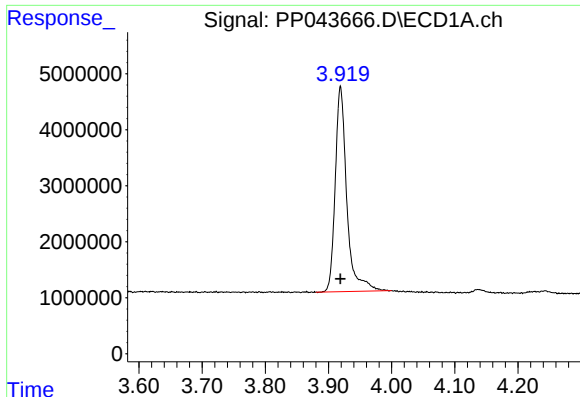

#1 Tetrachloro-m-xylene


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 46631732
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

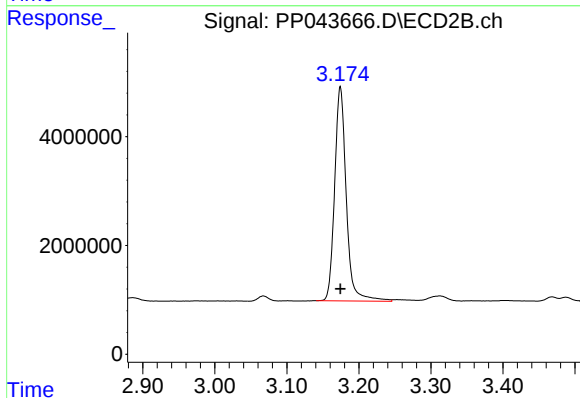


#1 Tetrachloro-m-xylene

R.T.: 3.174 min
Delta R.T.: 0.000 min
Response: 44081487
Conc: 23.47 ng/ml

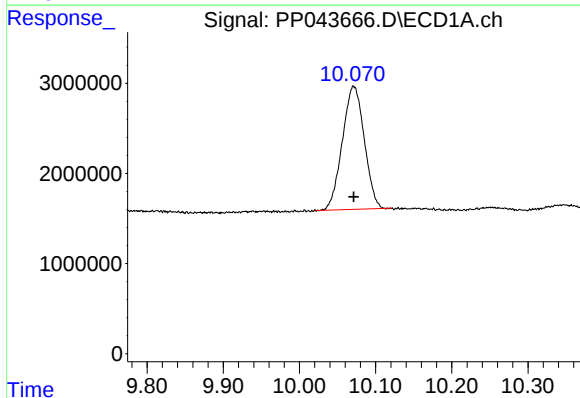


#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.000 min
Response: 27367984
Conc: 23.04 ng/ml

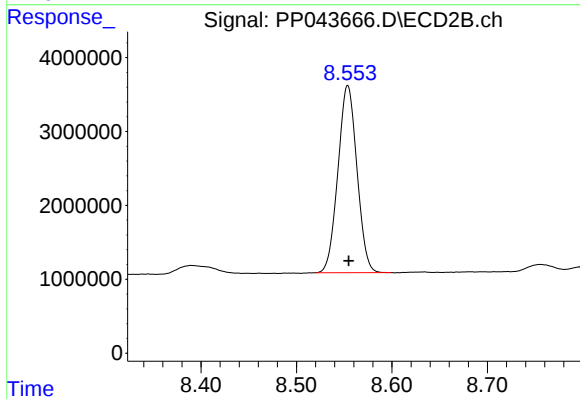

#2 Decachlorobiphenyl


R.T.: 8.554 min
Delta R.T.: -0.001 min
Response: 35066701
Conc: 21.61 ng/ml

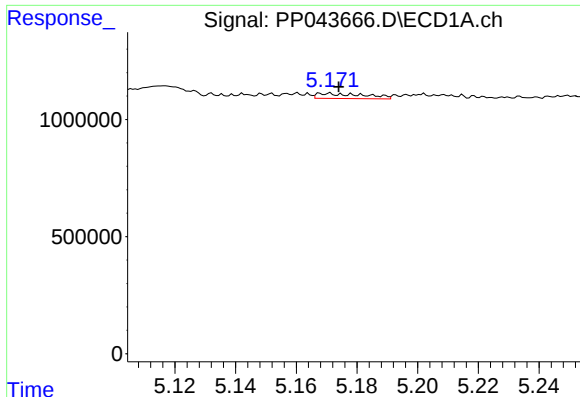

#3 AR-1016-1


R.T.: 5.170 min
Delta R.T.: -0.004 min
Response: 237526
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

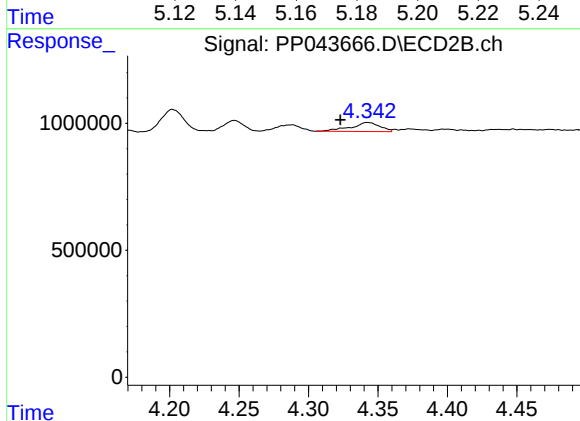


#3 AR-1016-1

R.T.: 4.342 min
Delta R.T.: 0.019 min
Response: 523228
Conc: 8.54 ng/ml

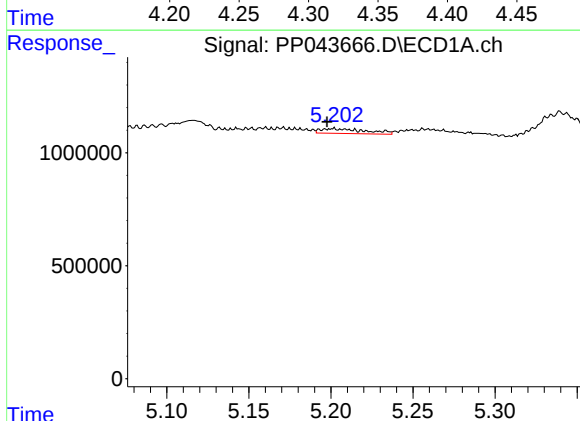


#4 AR-1016-2

R.T.: 5.201 min
Delta R.T.: 0.004 min
Response: 409892
Conc: 3.89 ng/ml

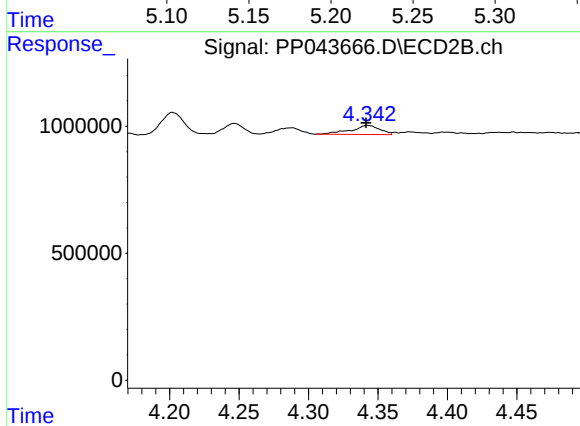

#4 AR-1016-2


R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 523228
Conc: 6.19 ng/ml

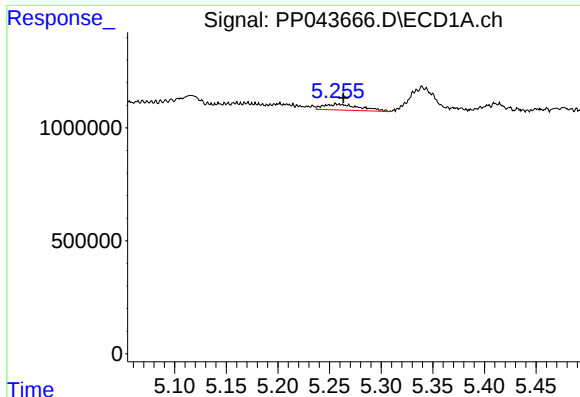

#5 AR-1016-3


R.T.: 5.250 min
Delta R.T.: -0.014 min
Response: 642082
Conc: 9.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

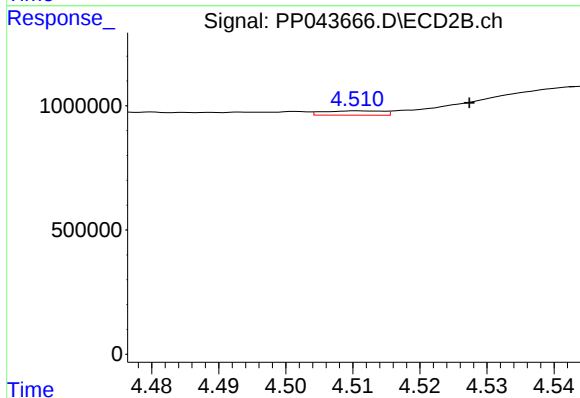


#5 AR-1016-3

R.T.: 4.511 min
Delta R.T.: -0.017 min
Response: 107107
Conc: 2.29 ng/ml

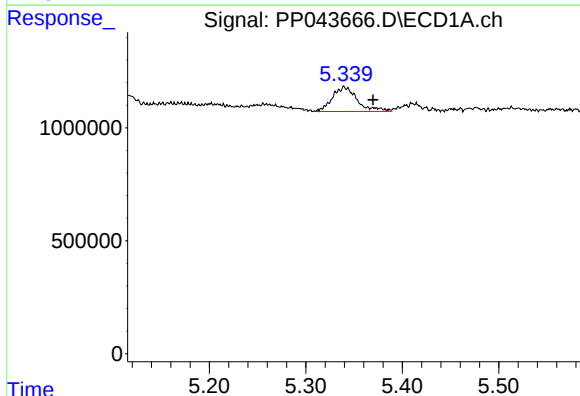


#6 AR-1016-4

R.T.: 5.340 min
Delta R.T.: -0.030 min
Response: 1954416
Conc: 36.04 ng/ml

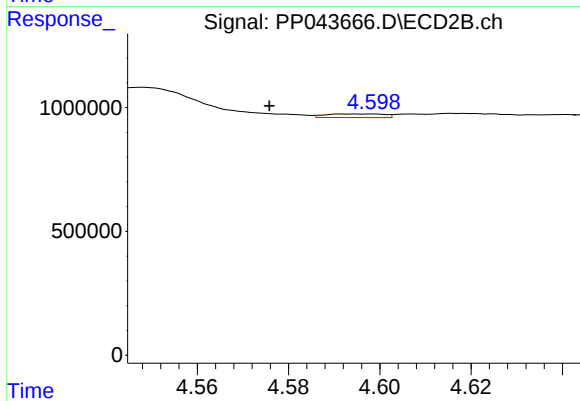

#6 AR-1016-4


R.T.: 4.598 min
Delta R.T.: 0.023 min
Response: 128842
Conc: 3.45 ng/ml

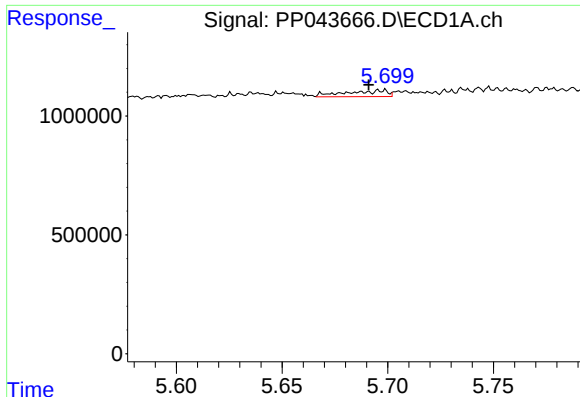

#7 AR-1016-5


R.T.: 5.688 min
Delta R.T.: -0.003 min
Response: 360542
Conc: 6.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

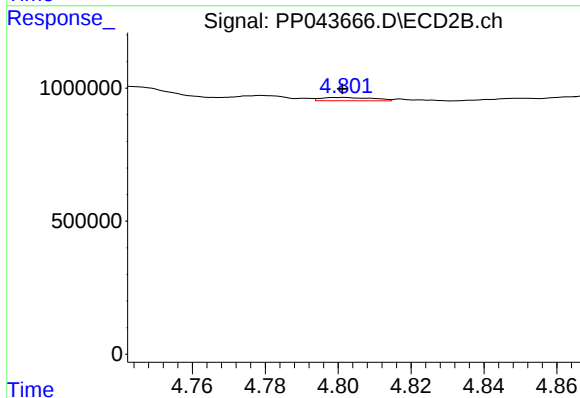


#7 AR-1016-5

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 118926
Conc: 2.60 ng/ml

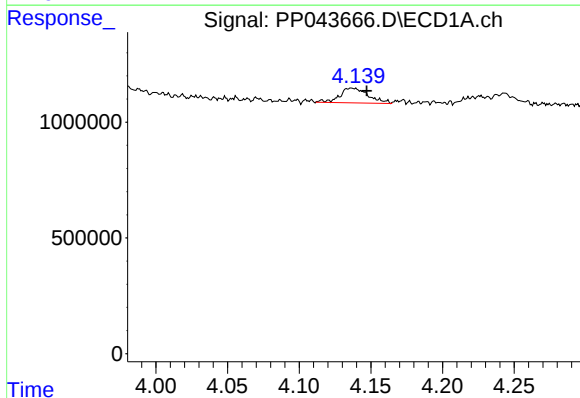


#8 AR-1221-1

R.T.: 4.137 min
Delta R.T.: -0.010 min
Response: 881820
Conc: 34.64 ng/ml

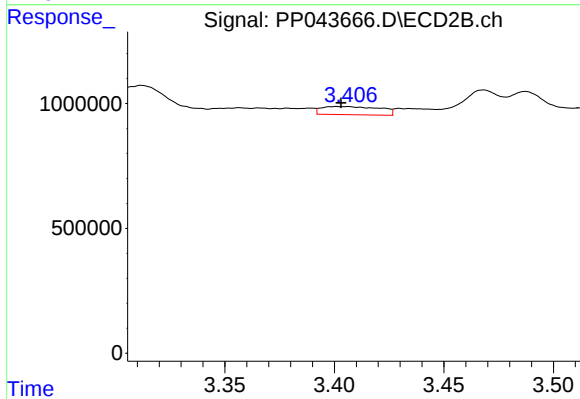

#8 AR-1221-1


R.T.: 3.406 min
Delta R.T.: 0.003 min
Response: 603615
Conc: 25.31 ng/ml

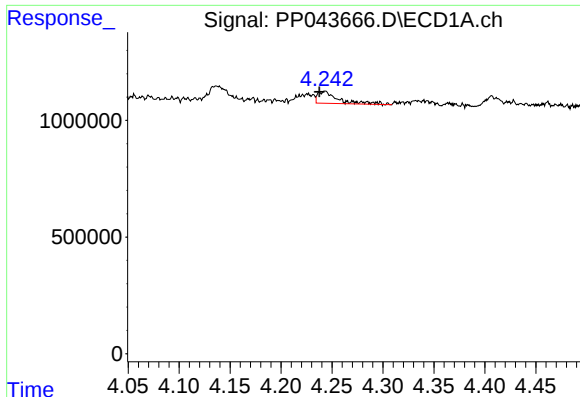

#9 AR-1221-2


R.T.: 4.243 min
Delta R.T.: 0.006 min
Response: 718186
Conc: 37.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

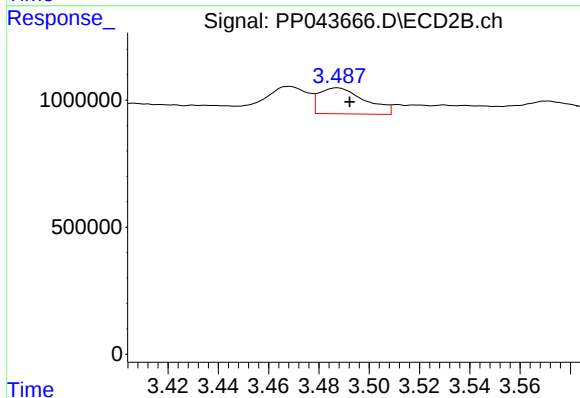


#9 AR-1221-2

R.T.: 3.487 min
Delta R.T.: -0.005 min
Response: 1295140
Conc: 71.71 ng/ml

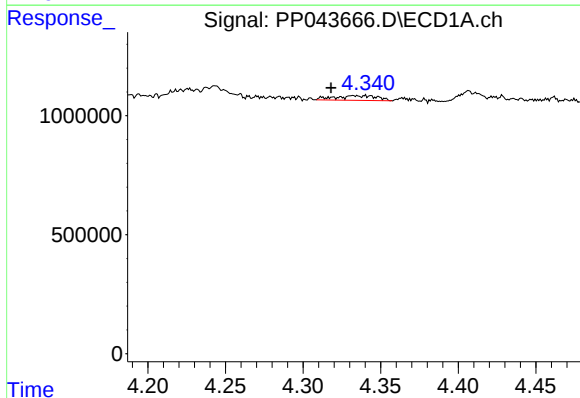


#10 AR-1221-3

R.T.: 4.332 min
Delta R.T.: 0.014 min
Response: 364990
Conc: 6.35 ng/ml

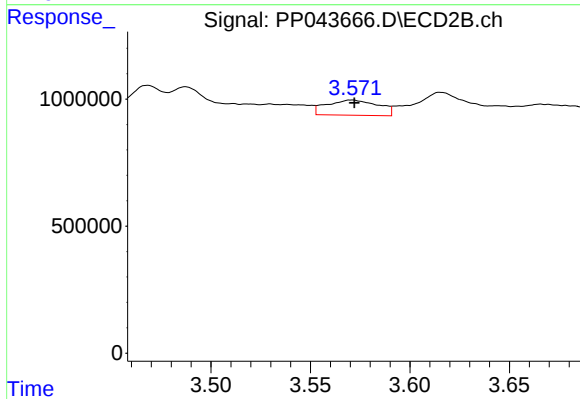

#10 AR-1221-3


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 1072217
Conc: 20.78 ng/ml

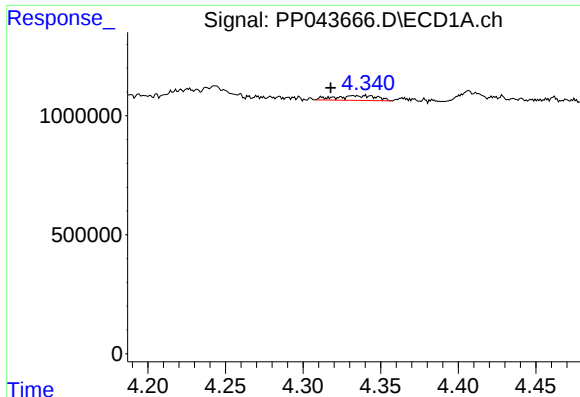

#11 AR-1232-1


R.T.: 4.332 min
Delta R.T.: 0.014 min
Response: 364990
Conc: 7.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

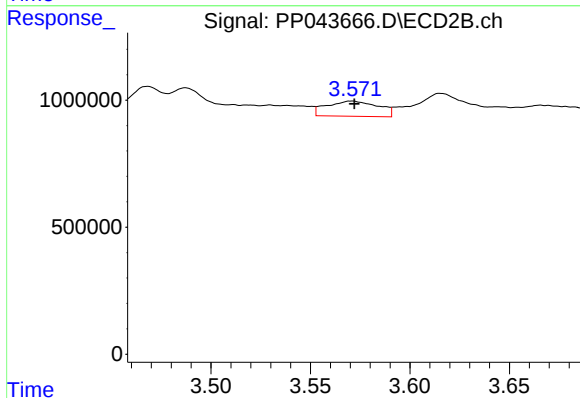


#11 AR-1232-1

R.T.: 3.571 min
Delta R.T.: -0.001 min
Response: 1072217
Conc: 24.92 ng/ml

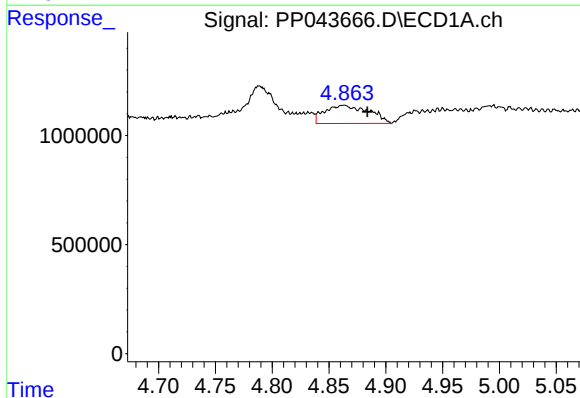


#12 AR-1232-2

R.T.: 4.863 min
Delta R.T.: -0.021 min
Response: 2264409
Conc: 95.56 ng/ml

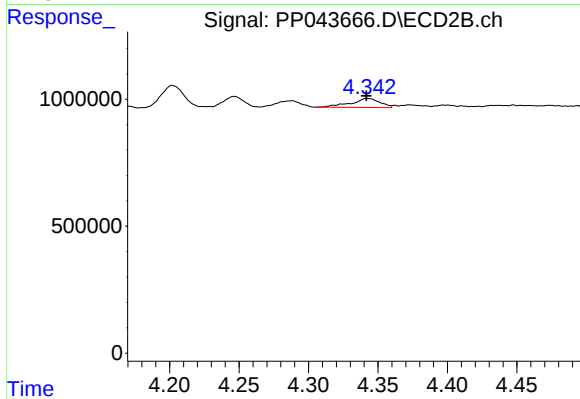

#12 AR-1232-2


R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 523228
Conc: 14.66 ng/ml

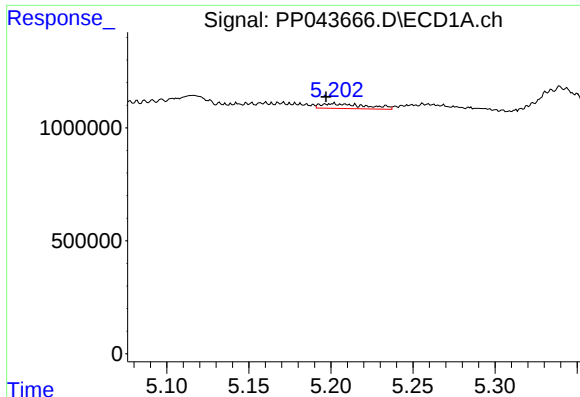

#13 AR-1232-3


R.T.: 5.201 min
Delta R.T.: 0.004 min
Response: 409892
Conc: 9.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

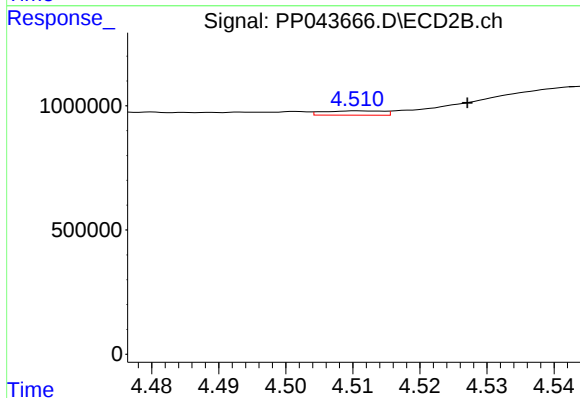


#13 AR-1232-3

R.T.: 4.511 min
Delta R.T.: -0.016 min
Response: 107107
Conc: 5.48 ng/ml

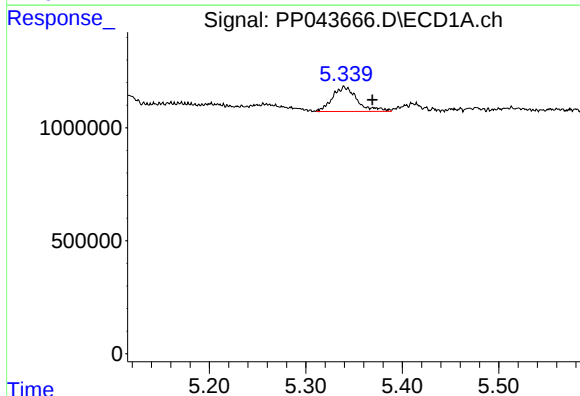


#14 AR-1232-4

R.T.: 5.340 min
Delta R.T.: -0.029 min
Response: 1954416
Conc: 89.54 ng/ml

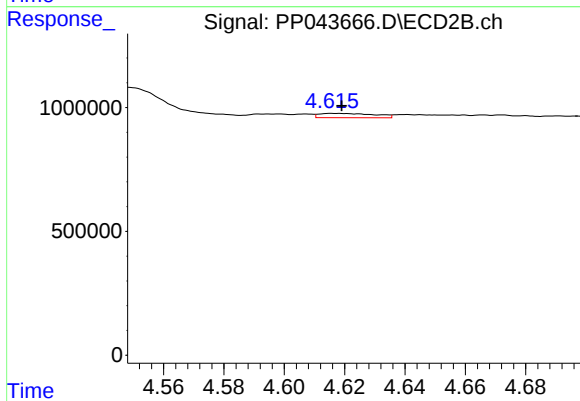

#14 AR-1232-4


R.T.: 4.615 min
Delta R.T.: -0.004 min
Response: 224991
Conc: 13.01 ng/ml

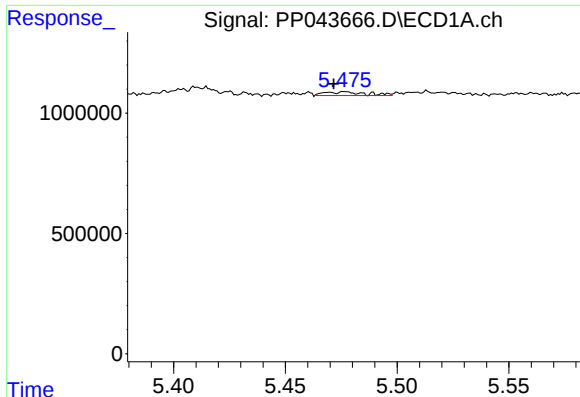

#15 AR-1232-5


R.T.: 5.477 min
Delta R.T.: 0.005 min
Response: 198351
Conc: 12.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

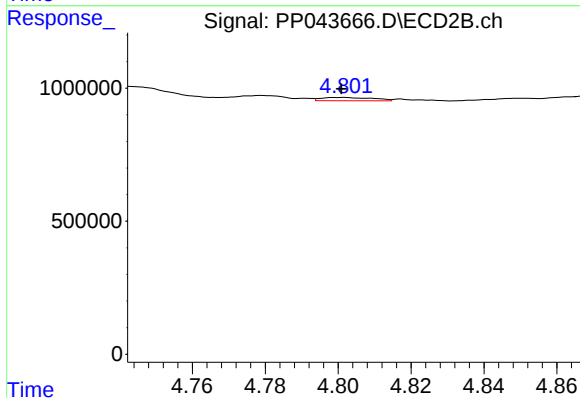


#15 AR-1232-5

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 118926
Conc: 6.33 ng/ml

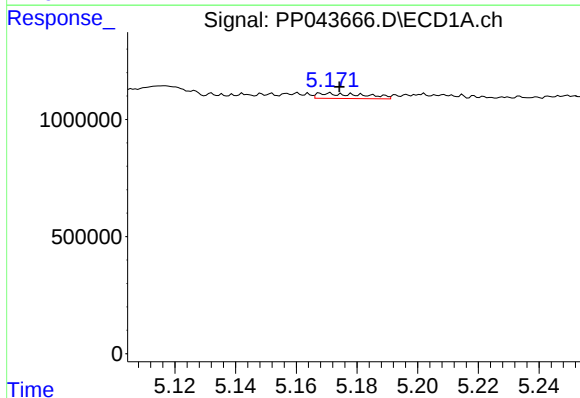


#16 AR-1242-1

R.T.: 5.170 min
Delta R.T.: -0.004 min
Response: 237526
Conc: 4.23 ng/ml

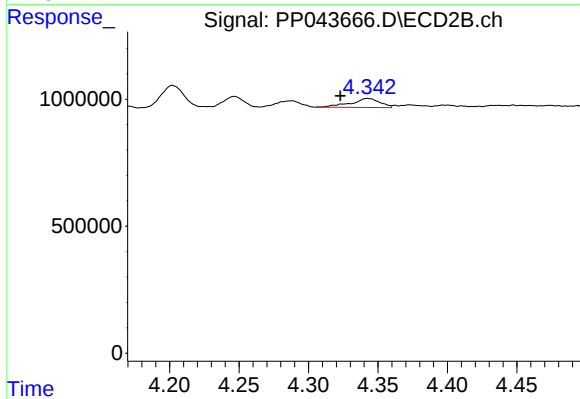

#16 AR-1242-1


R.T.: 4.342 min
Delta R.T.: 0.019 min
Response: 523228
Conc: 10.73 ng/ml

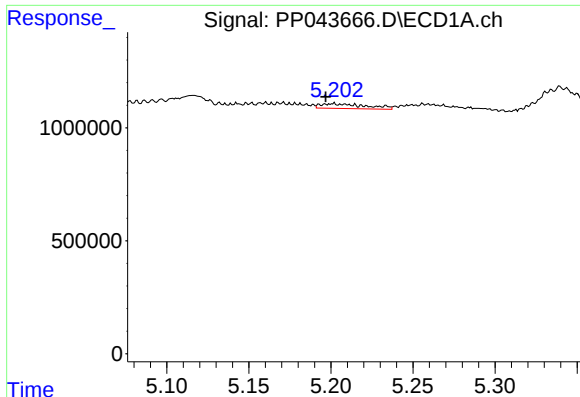

#17 AR-1242-2


R.T.: 5.201 min
Delta R.T.: 0.005 min
Response: 409892
Conc: 4.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

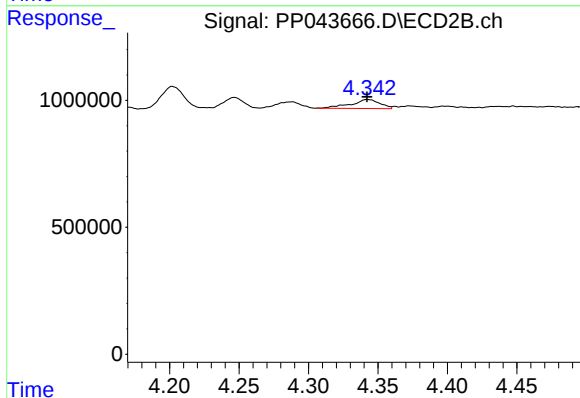


#17 AR-1242-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 523228
Conc: 7.77 ng/ml

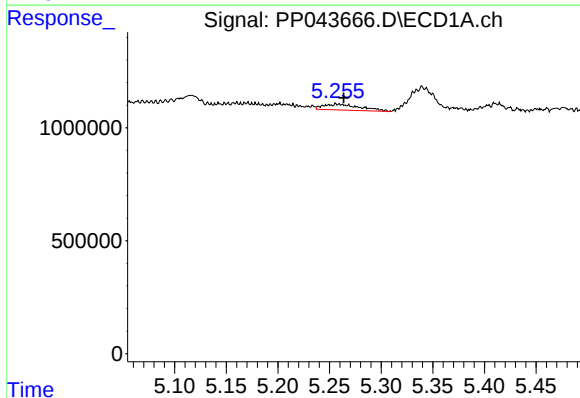


#18 AR-1242-3

R.T.: 5.250 min
Delta R.T.: -0.014 min
Response: 642082
Conc: 12.40 ng/ml

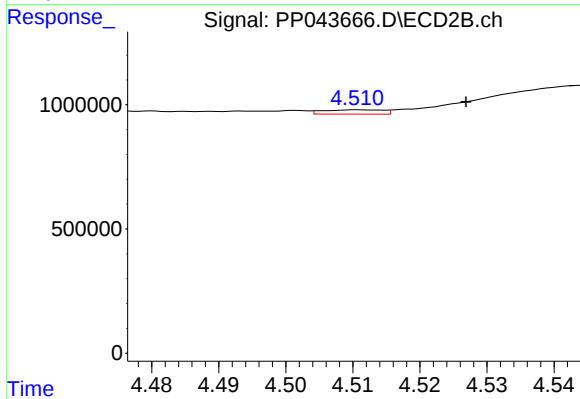

#18 AR-1242-3


R.T.: 4.511 min
Delta R.T.: -0.016 min
Response: 107107
Conc: 2.85 ng/ml

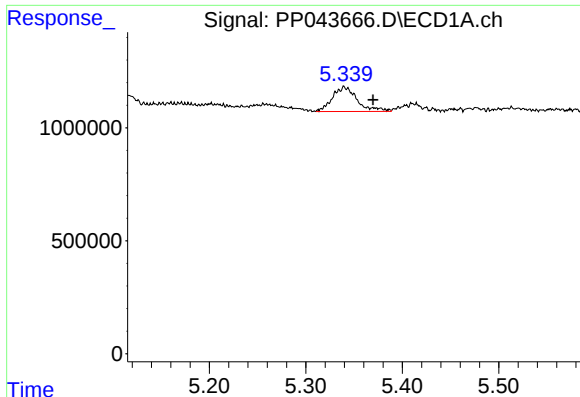

#19 AR-1242-4


R.T.: 5.340 min
Delta R.T.: -0.030 min
Response: 1954416
Conc: 45.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

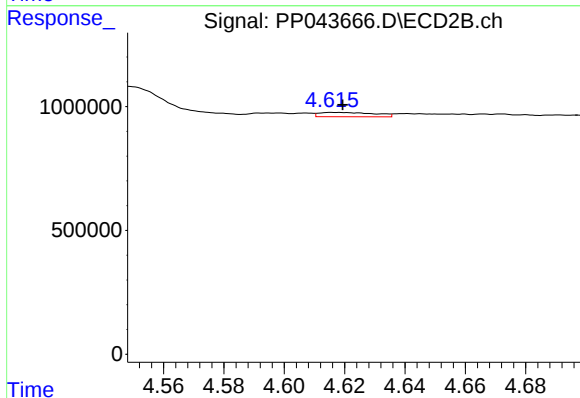


#19 AR-1242-4

R.T.: 4.615 min
Delta R.T.: -0.004 min
Response: 224991
Conc: 6.23 ng/ml

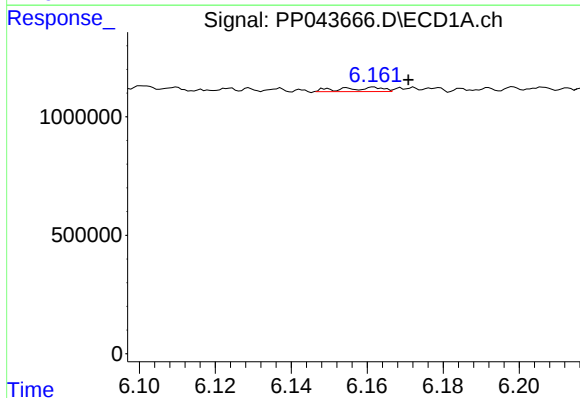


#20 AR-1242-5

R.T.: 6.162 min
Delta R.T.: -0.009 min
Response: 132087
Conc: 3.06 ng/ml

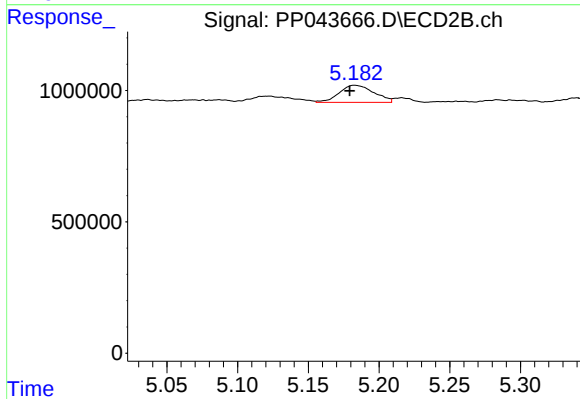

#20 AR-1242-5


R.T.: 5.183 min
Delta R.T.: 0.003 min
Response: 1113469
Conc: 25.87 ng/ml

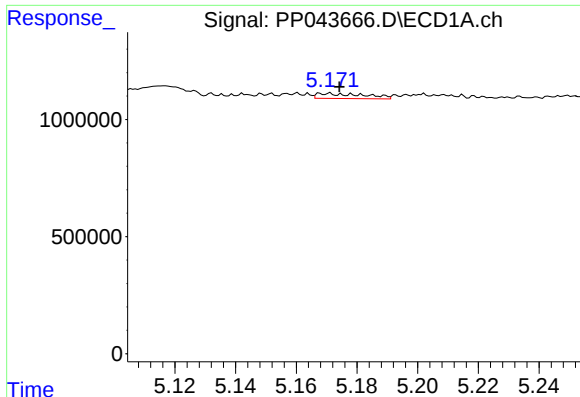

#21 AR-1248-1


R.T.: 5.170 min
Delta R.T.: -0.004 min
Response: 237526
Conc: 5.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

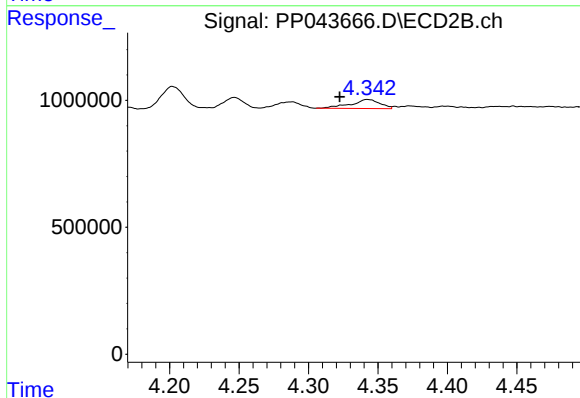


#21 AR-1248-1

R.T.: 4.342 min
Delta R.T.: 0.020 min
Response: 523228
Conc: 14.05 ng/ml

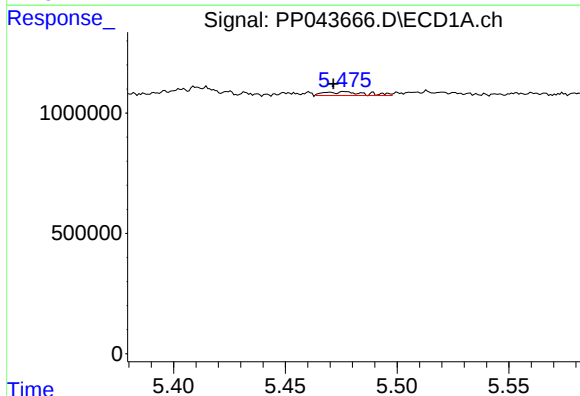


#22 AR-1248-2

R.T.: 5.477 min
Delta R.T.: 0.005 min
Response: 198351
Conc: 3.49 ng/ml

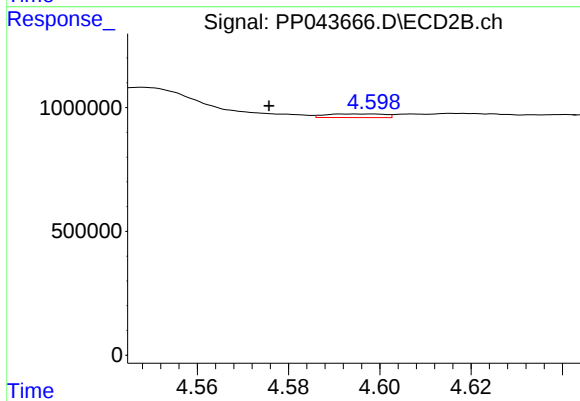

#22 AR-1248-2


R.T.: 4.598 min
Delta R.T.: 0.023 min
Response: 128842
Conc: 2.63 ng/ml

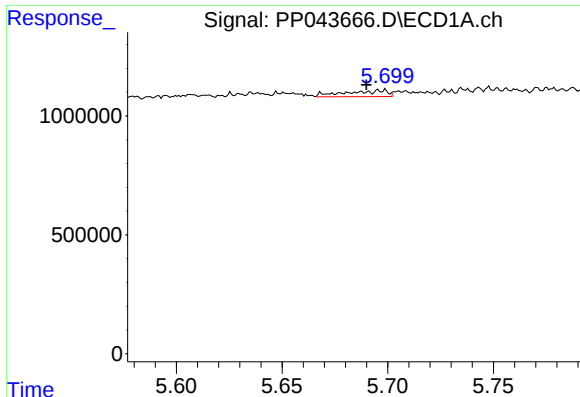

#23 AR-1248-3


R.T.: 5.688 min
Delta R.T.: -0.002 min
Response: 360542
Conc: 5.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

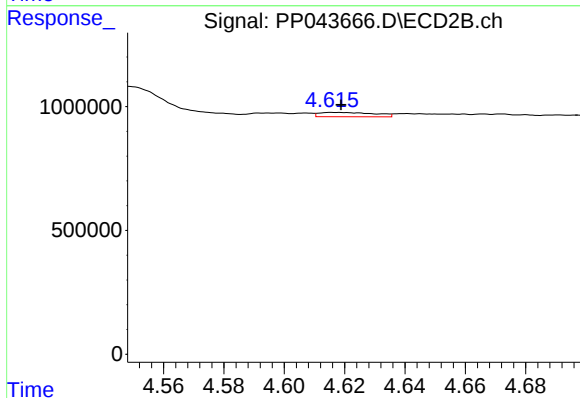


#23 AR-1248-3

R.T.: 4.615 min
Delta R.T.: -0.003 min
Response: 224991
Conc: 4.38 ng/ml

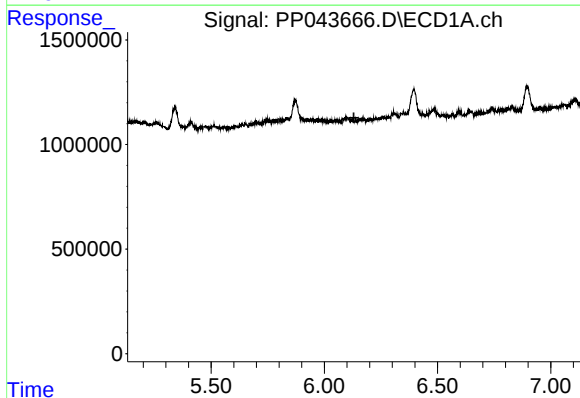


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.130 min
Response: 0
Conc: N.D.

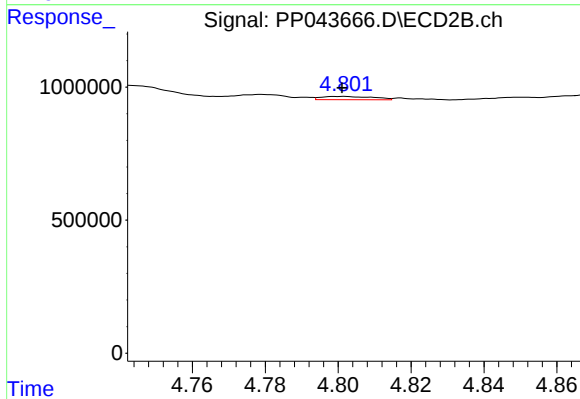

#24 AR-1248-4


R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 118926
Conc: 2.03 ng/ml

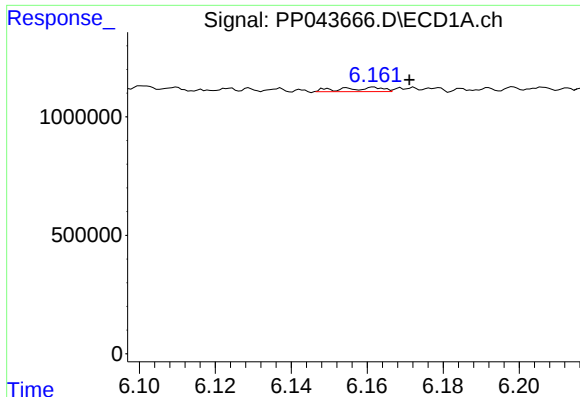

#25 AR-1248-5


R.T.: 6.162 min
Delta R.T.: -0.009 min
Response: 132087
Conc: 1.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

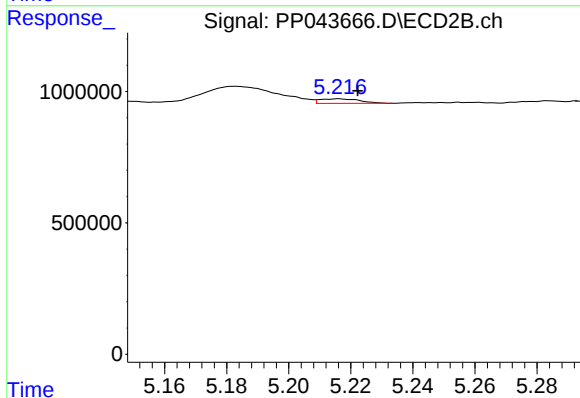


#25 AR-1248-5

R.T.: 5.216 min
Delta R.T.: -0.006 min
Response: 152749
Conc: 2.67 ng/ml

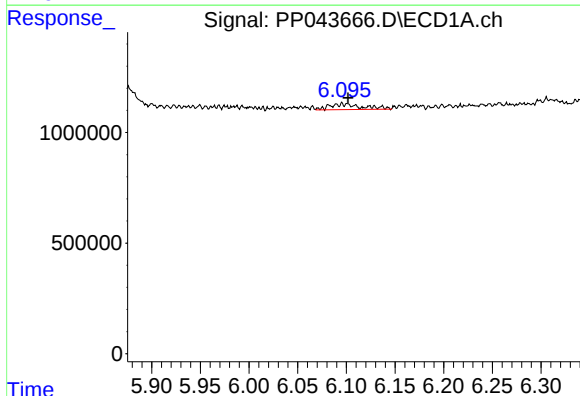


#26 AR-1254-1

R.T.: 6.082 min
Delta R.T.: -0.020 min
Response: 604394
Conc: 8.00 ng/ml

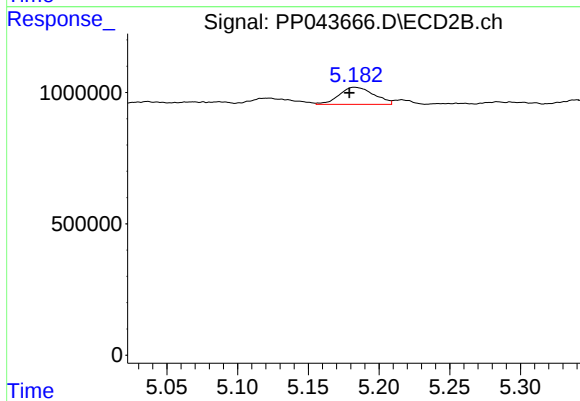

#26 AR-1254-1


R.T.: 5.183 min
Delta R.T.: 0.003 min
Response: 1113469
Conc: 12.75 ng/ml

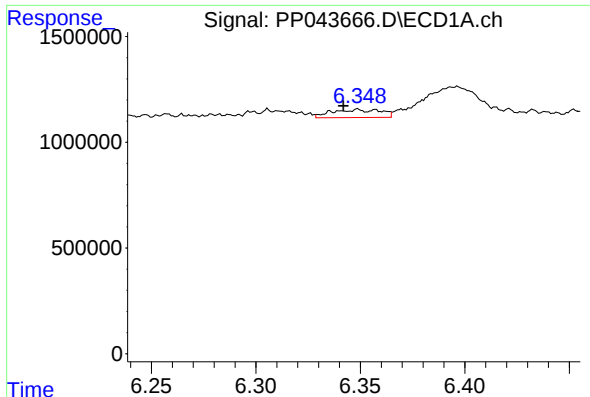

#27 AR-1254-2


R.T.: 6.348 min
Delta R.T.: 0.007 min
Response: 627663
Conc: 5.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

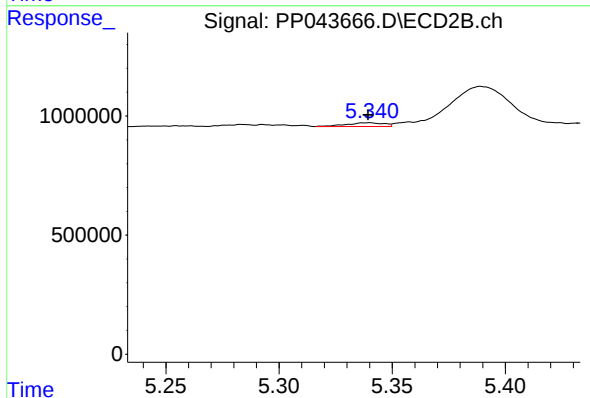


#27 AR-1254-2

R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 183463
Conc: 2.41 ng/ml

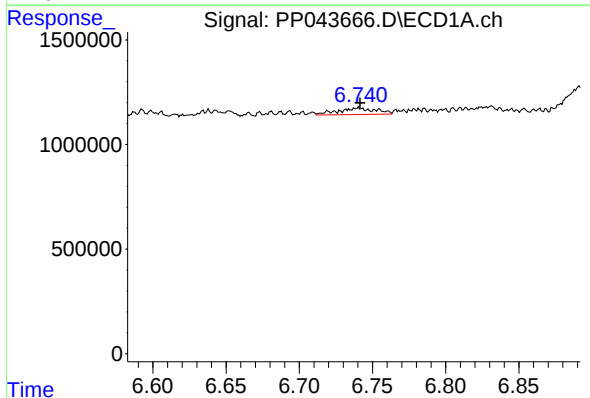


#28 AR-1254-3

R.T.: 6.740 min
Delta R.T.: -0.001 min
Response: 564782
Conc: 4.88 ng/ml

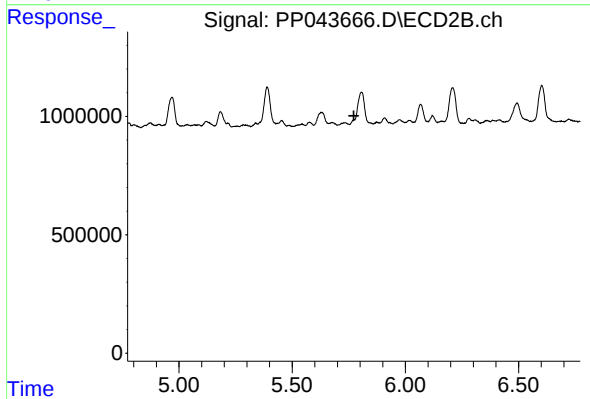

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.772 min
Response: 0
Conc: N.D.

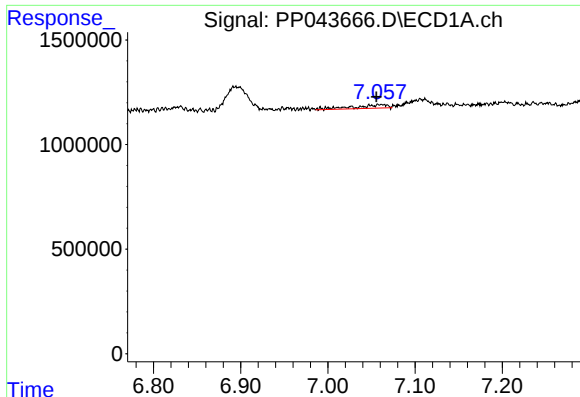

#29 AR-1254-4


R.T.: 7.061 min
Delta R.T.: 0.005 min
Response: 445468
Conc: 5.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

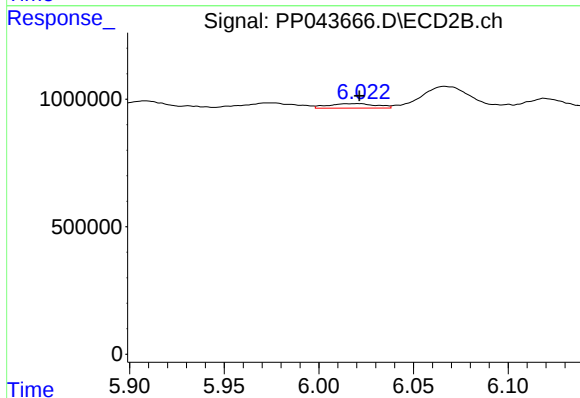


#29 AR-1254-4

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 318433
Conc: 4.03 ng/ml

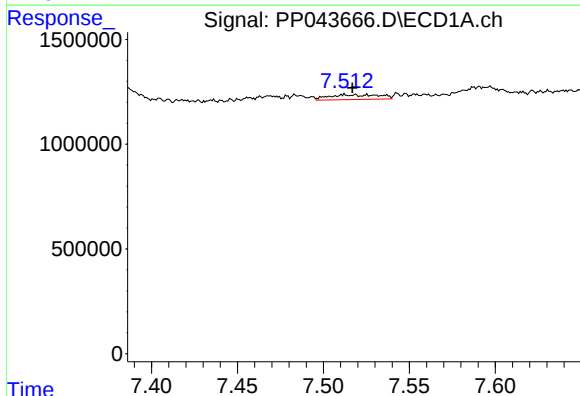


#30 AR-1254-5

R.T.: 7.514 min
Delta R.T.: -0.003 min
Response: 463194
Conc: 5.40 ng/ml

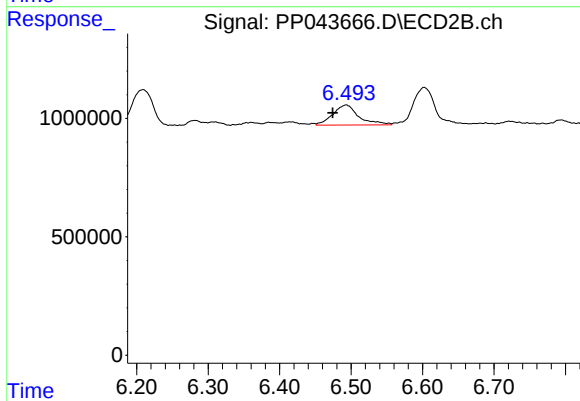

#30 AR-1254-5


R.T.: 6.493 min
Delta R.T.: 0.019 min
Response: 2133347
Conc: 18.45 ng/ml

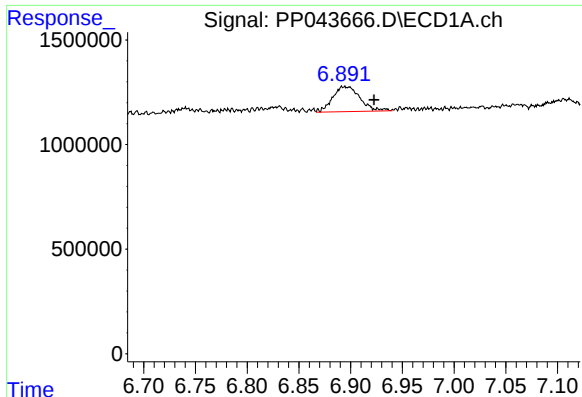

#31 AR-1260-1


R.T.: 6.895 min
Delta R.T.: -0.027 min
Response: 2200126
Conc: 26.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

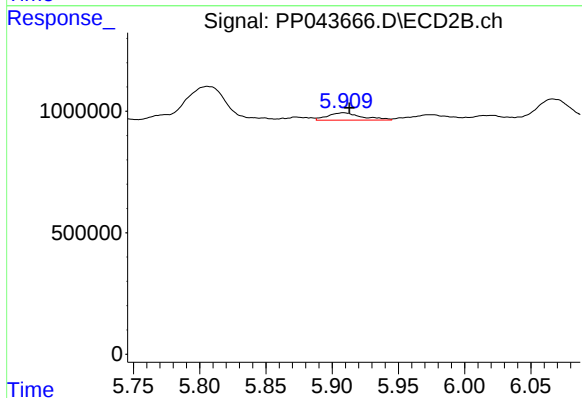


#31 AR-1260-1

R.T.: 5.909 min
Delta R.T.: -0.005 min
Response: 546586
Conc: 6.83 ng/ml

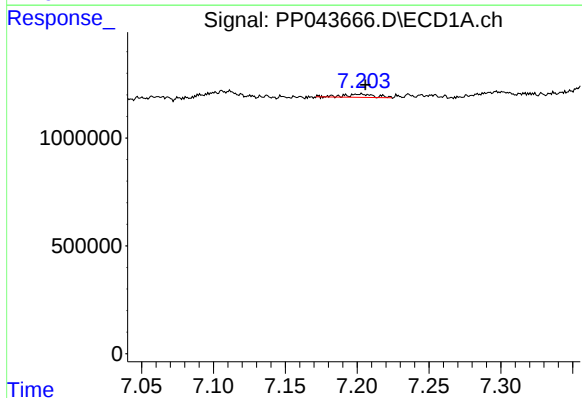


#32 AR-1260-2

R.T.: 7.202 min
Delta R.T.: -0.004 min
Response: 213601
Conc: 2.36 ng/ml

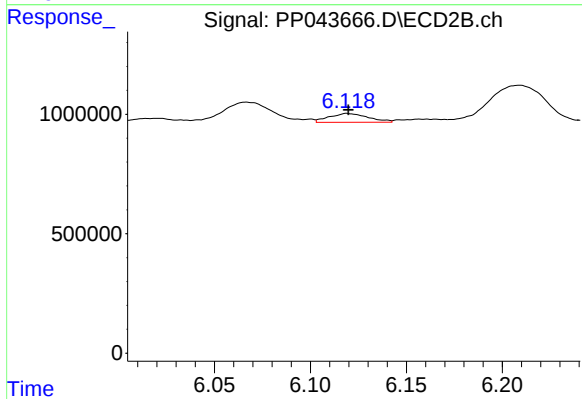

#32 AR-1260-2


R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 520914
Conc: 5.33 ng/ml

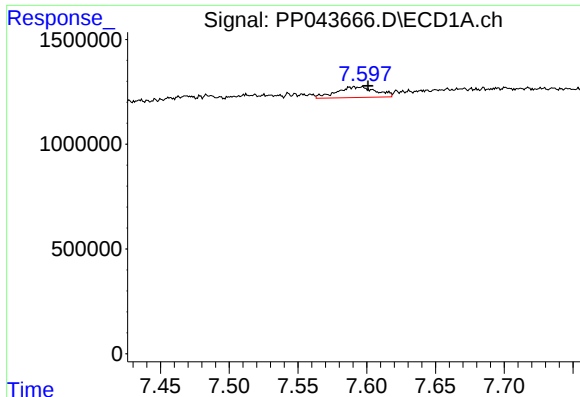

#33 AR-1260-3


R.T.: 7.593 min
Delta R.T.: -0.009 min
Response: 1017893
Conc: 14.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

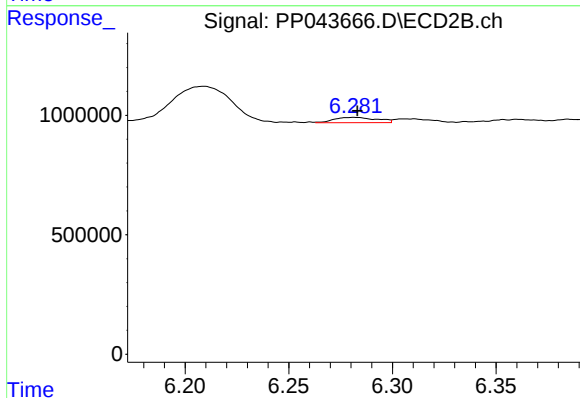


#33 AR-1260-3

R.T.: 6.282 min
Delta R.T.: -0.001 min
Response: 323364
Conc: 3.54 ng/ml

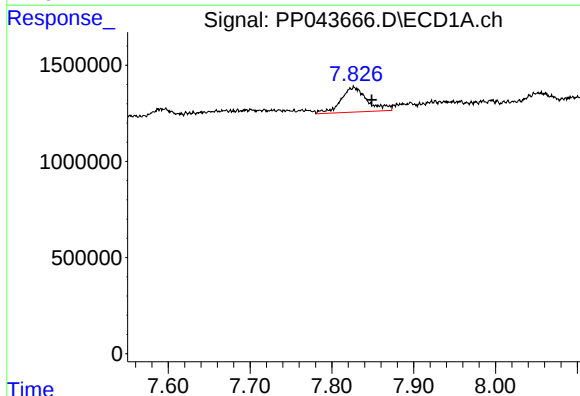


#34 AR-1260-4

R.T.: 7.827 min
Delta R.T.: -0.022 min
Response: 2913537
Conc: 33.94 ng/ml

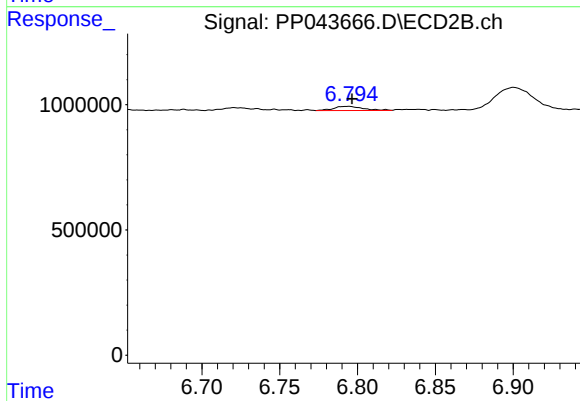

#34 AR-1260-4


R.T.: 6.794 min
Delta R.T.: -0.002 min
Response: 223395
Conc: 2.76 ng/ml

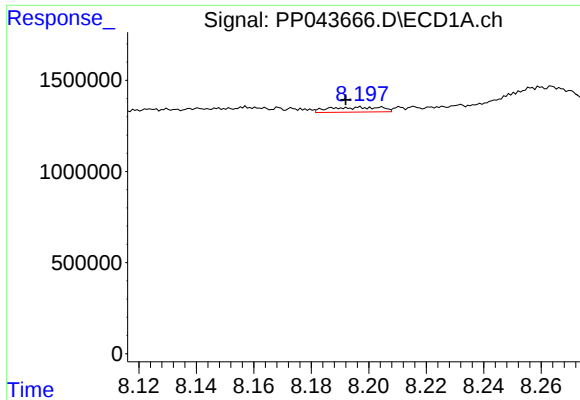

#35 AR-1260-5


R.T.: 8.200 min
Delta R.T.: 0.008 min
Response: 340167
Conc: 2.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

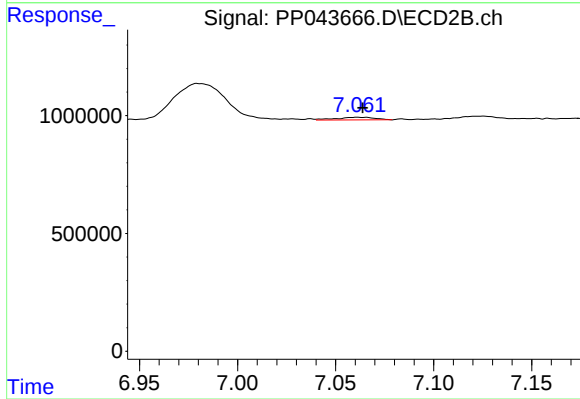


#35 AR-1260-5

R.T.: 7.061 min
Delta R.T.: -0.003 min
Response: 152777
Conc: 0.83 ng/ml

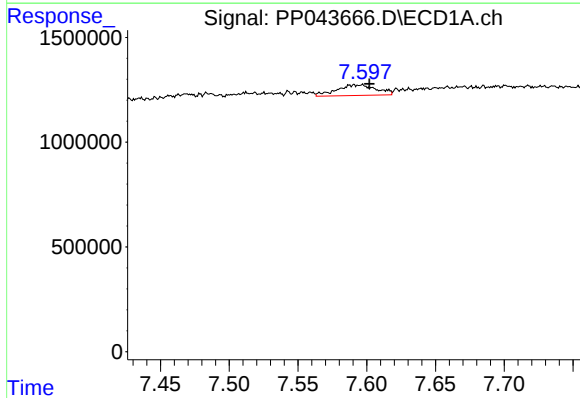


#36 AR-1262-1

R.T.: 7.593 min
Delta R.T.: -0.010 min
Response: 1017893
Conc: 10.31 ng/ml

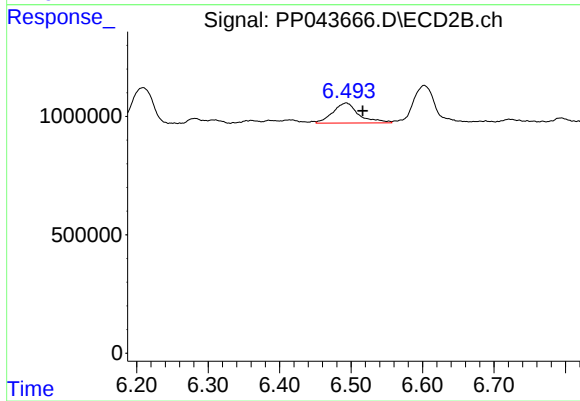

#36 AR-1262-1


R.T.: 6.493 min
Delta R.T.: -0.023 min
Response: 2133347
Conc: 19.41 ng/ml

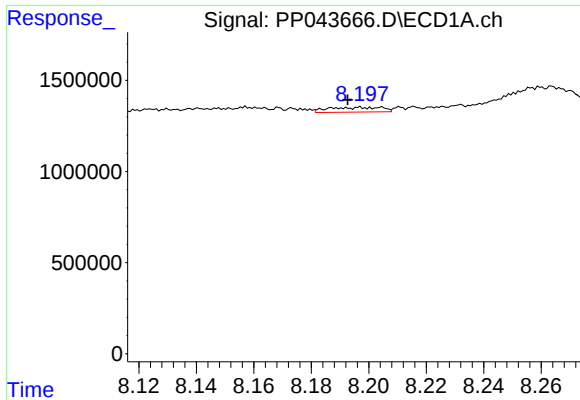

#37 AR-1262-2


R.T.: 8.200 min
Delta R.T.: 0.008 min
Response: 340167
Conc: 2.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

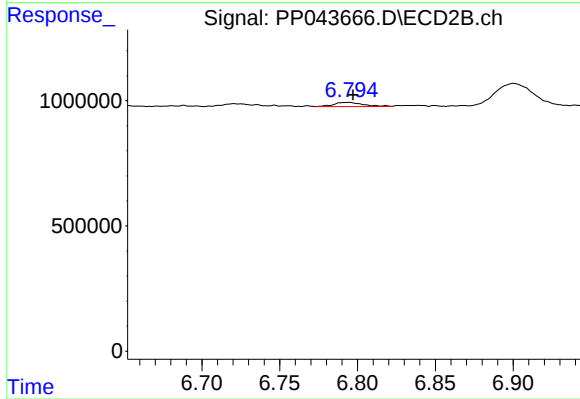


#37 AR-1262-2

R.T.: 6.794 min
Delta R.T.: -0.003 min
Response: 223395
Conc: 2.19 ng/ml

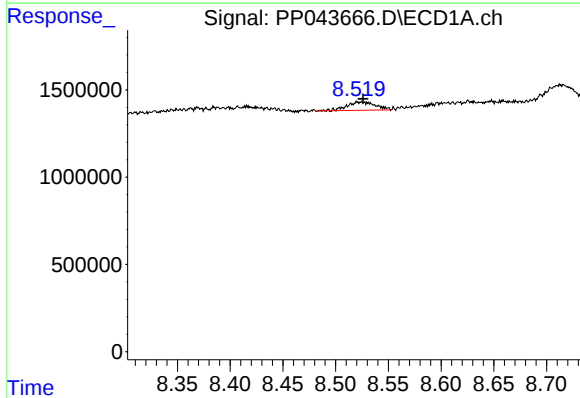


#38 AR-1262-3

R.T.: 8.524 min
Delta R.T.: -0.002 min
Response: 905112
Conc: 8.27 ng/ml

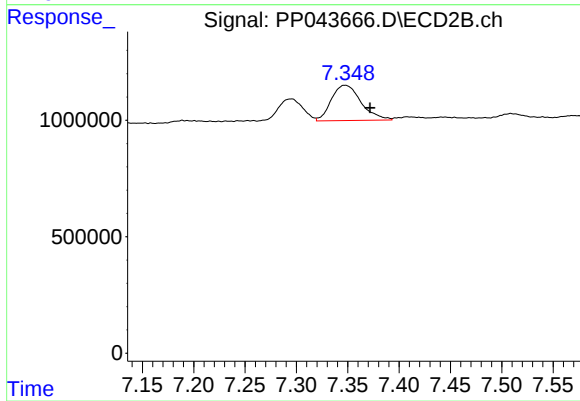

#38 AR-1262-3


R.T.: 7.347 min
Delta R.T.: -0.024 min
Response: 3064554
Conc: 35.96 ng/ml

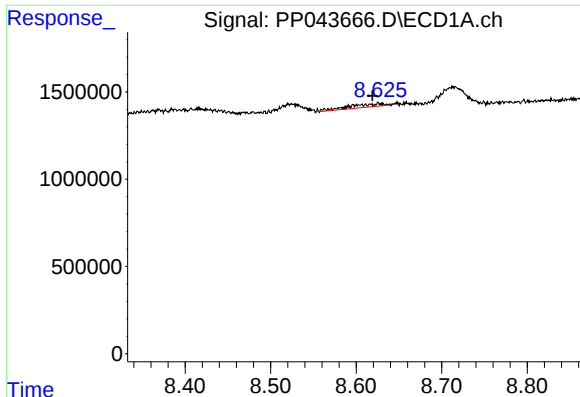

#39 AR-1262-4


R.T.: 8.627 min
Delta R.T.: 0.008 min
Response: 532520
Conc: 11.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

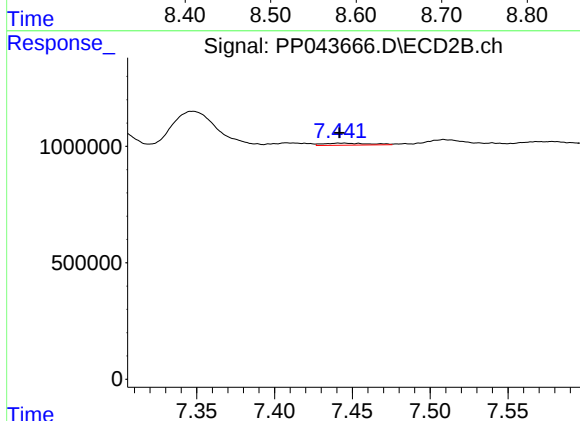


#39 AR-1262-4

R.T.: 7.444 min
Delta R.T.: 0.003 min
Response: 183551
Conc: 1.18 ng/ml

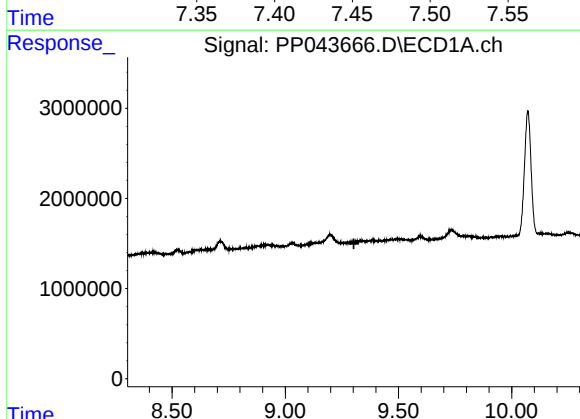


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.303 min
Response: 0
Conc: N.D.

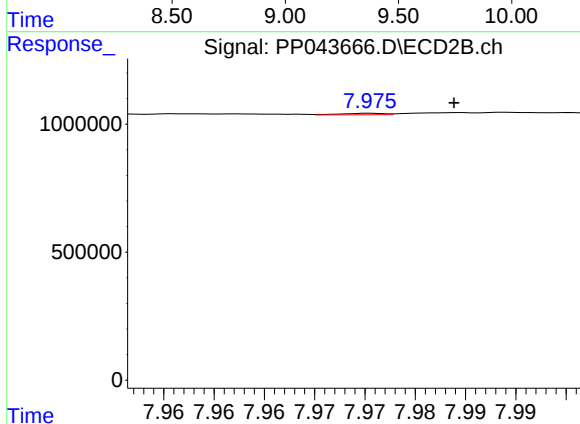

#40 AR-1262-5


R.T.: 7.976 min
Delta R.T.: -0.008 min
Response: 16796
Conc: 0.22 ng/ml

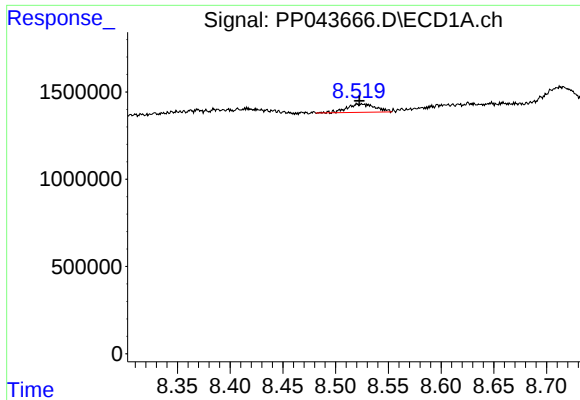

#41 AR-1268-1


R.T.: 8.524 min
Delta R.T.: 0.002 min
Response: 905112
Conc: 4.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

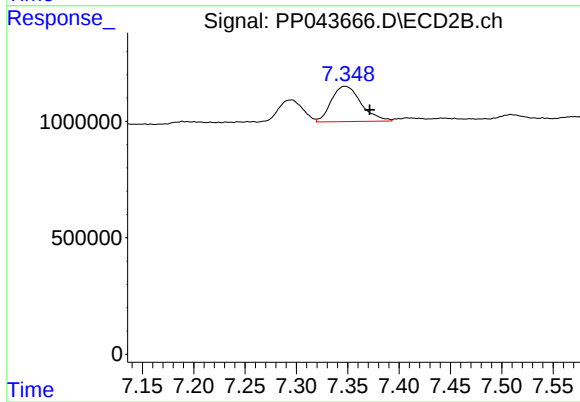


#41 AR-1268-1

R.T.: 7.347 min
Delta R.T.: -0.024 min
Response: 3064554
Conc: 12.10 ng/ml

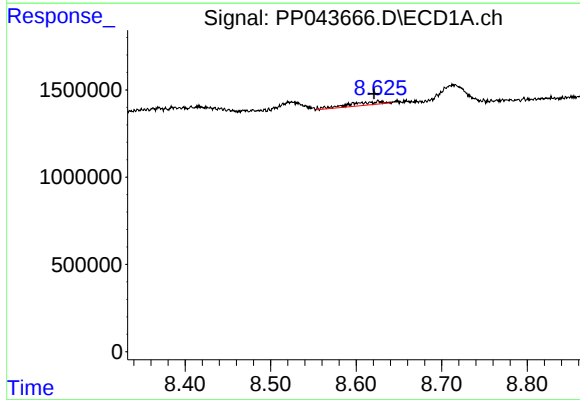


#42 AR-1268-2

R.T.: 8.627 min
Delta R.T.: 0.006 min
Response: 532520
Conc: 3.04 ng/ml

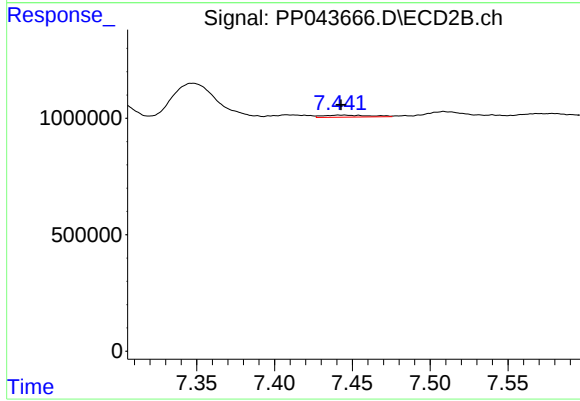

#42 AR-1268-2


R.T.: 7.444 min
Delta R.T.: 0.002 min
Response: 183551
Conc: 0.81 ng/ml

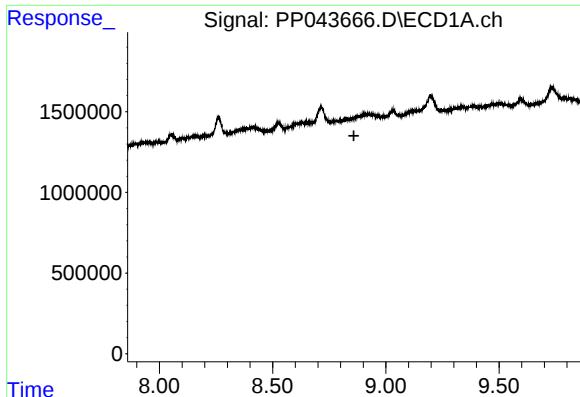

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.859 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

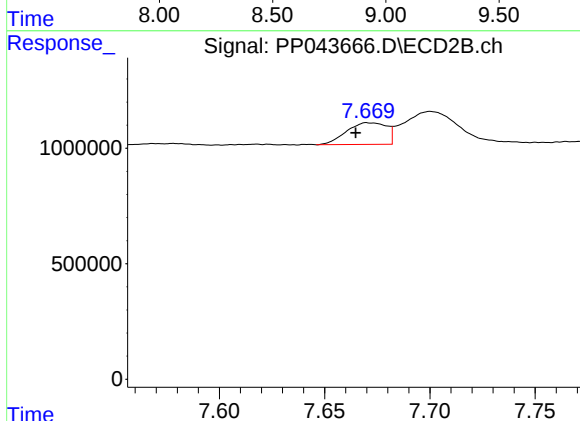


#43 AR-1268-3

R.T.: 7.671 min
Delta R.T.: 0.006 min
Response: 1249666
Conc: 6.42 ng/ml

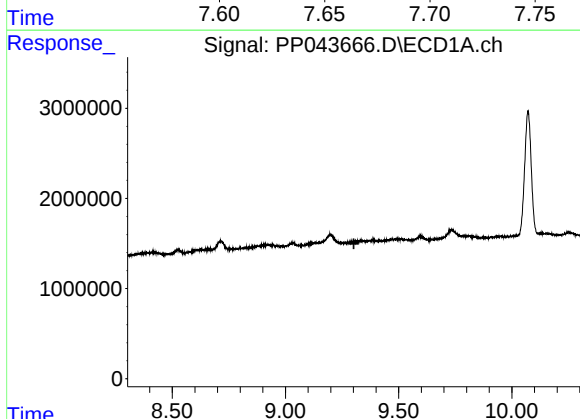


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

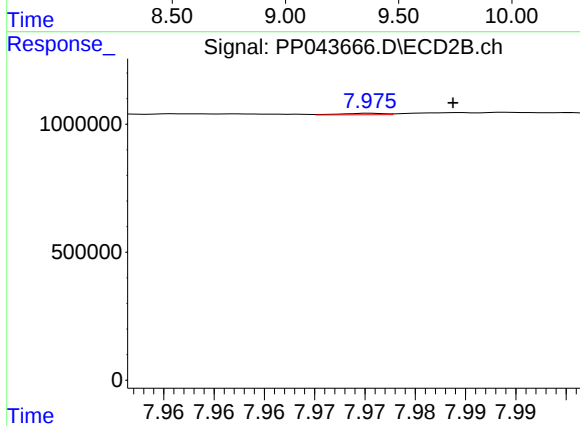

#44 AR-1268-4


R.T.: 7.976 min
Delta R.T.: -0.008 min
Response: 16796
Conc: 0.19 ng/ml

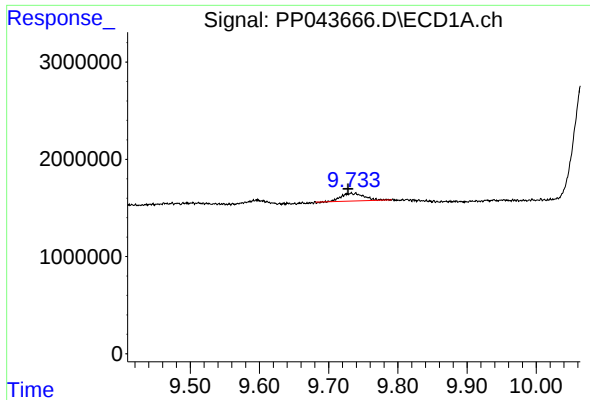

#45 AR-1268-5

R.T.: 9.733 min
Delta R.T.: 0.005 min
Response: 1832085
Conc: 4.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-01

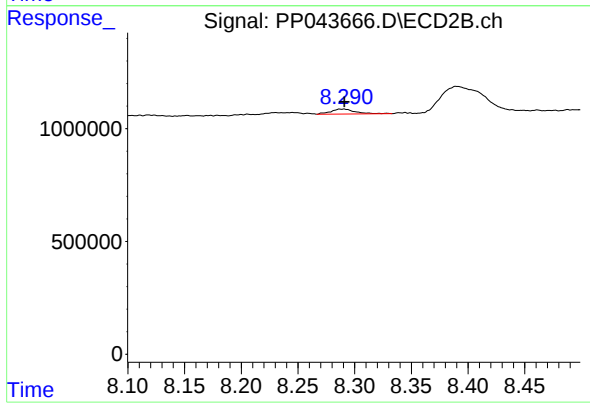

#45 AR-1268-5

R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 326112
Conc: 0.54 ng/ml