

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:32
 Operator : YP\AJ
 Sample : N1523-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:24:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.919	3.175	29568891	27662395	13.373	14.728
2) SA Decachlor...	10.071	8.554	17586335	23849168	14.805	14.700
Target Compounds						
3) L1 AR-1016-1	5.173	4.322	1226049	1461556	16.897	23.855 #
4) L1 AR-1016-2	5.197	4.342	1535600	1975439	14.559	23.381 #
5) L1 AR-1016-3	5.263	4.526	1565256	1489507	23.772	31.884 #
6) L1 AR-1016-4	5.368	4.574	1398587	1455215	25.790	38.940 #
7) L1 AR-1016-5	5.693	4.800	2546348	1594582	48.476	34.906 #
8) L2 AR-1221-1	4.138	3.396	1129273	83353	44.356	3.494 #
9) L2 AR-1221-2	4.248	3.489	709386	647372	36.950	35.846
10) L2 AR-1221-3	4.320	3.572	331924	873158	5.778	16.926 #
11) L3 AR-1232-1	4.320	3.572	331924	873158	6.839	20.294 #
12) L3 AR-1232-2	4.880	4.342	846137	1975439	35.706	55.338 #
13) L3 AR-1232-3	5.197	4.526	1535600	1489507	35.667	76.173 #
14) L3 AR-1232-4	5.368	4.619	1398587	1647292	64.072	95.261 #
15) L3 AR-1232-5	5.474	4.800	2406678	1594582	149.212	84.890 #
16) L4 AR-1242-1	5.173	4.322	1226049	1461556	21.819	29.982 #
17) L4 AR-1242-2	5.197	4.342	1535600	1975439	18.561	29.337 #
18) L4 AR-1242-3	5.263	4.526	1565256	1489507	30.241	39.679 #
19) L4 AR-1242-4	5.368	4.619	1398587	1647292	32.744	45.619 #
20) L4 AR-1242-5	6.166	5.178	857693	1713046	19.862	39.794 #
21) L5 AR-1248-1	5.173	4.322	1226049	1461556	29.905	39.236 #
22) L5 AR-1248-2	5.474	4.574	2406678	1455215	42.361	29.746 #
23) L5 AR-1248-3	5.693	4.619	2546348	1647292	38.167	32.101
24) L5 AR-1248-4	6.128	4.800	796481	1594582	11.400	27.199 #
25) L5 AR-1248-5	6.166	5.220	857693	879052	12.407	15.342
26) L6 AR-1254-1	6.102	5.178	1801954	1713046	23.849	19.615
27) L6 AR-1254-2	6.341	5.338	1079922	1063619	9.628	13.944 #
28) L6 AR-1254-3	6.742	5.772	1009284	1105096	8.722	9.017
29) L6 AR-1254-4	7.055	6.022	430708	418993	5.395	5.309
30) L6 AR-1254-5	7.518	6.472	988178	886896	11.522	7.669 #
31) L7 AR-1260-1	6.921	5.912	486621	737766	5.811	9.226 #
32) L7 AR-1260-2	7.204	6.120	444037	873315	4.905	8.943 #
33) L7 AR-1260-3	7.605	6.282	134107	656461	1.850	7.191 #
34) L7 AR-1260-4	7.851	6.793	624119	356044	7.269	4.400 #
35) L7 AR-1260-5	8.193	7.062	876747	366642	5.656	1.983 #
36) L8 AR-1262-1	7.605	6.517	134107	301729	1.358	2.745 #
37) L8 AR-1262-2	8.193	6.793	876747	356044	5.431	3.490 #
38) L8 AR-1262-3	8.515	7.379	301855	293010	2.759	3.438
39) L8 AR-1262-4	8.610	7.440	39752	267530	0.829	1.723 #
40) L8 AR-1262-5	9.298	7.982	230903	35182	4.146	0.452 #
41) L9 AR-1268-1	8.515	7.379	301855	293010	1.548	1.156 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:32
 Operator : YP\AJ
 Sample : N1523-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:24:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.610	7.440	39752	267530	0.227	1.184 #
43) L9	AR-1268-3	8.857	7.665	213350	67085	1.382	0.345 #
44) L9	AR-1268-4	9.298	7.982	230903	35182	3.690	0.391 #
45) L9	AR-1268-5	9.742	8.293	289152	253292	0.636	0.422 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
Data File : PP043667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2022 08:32
Operator : YP\AJ
Sample : N1523-02
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 01:24:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

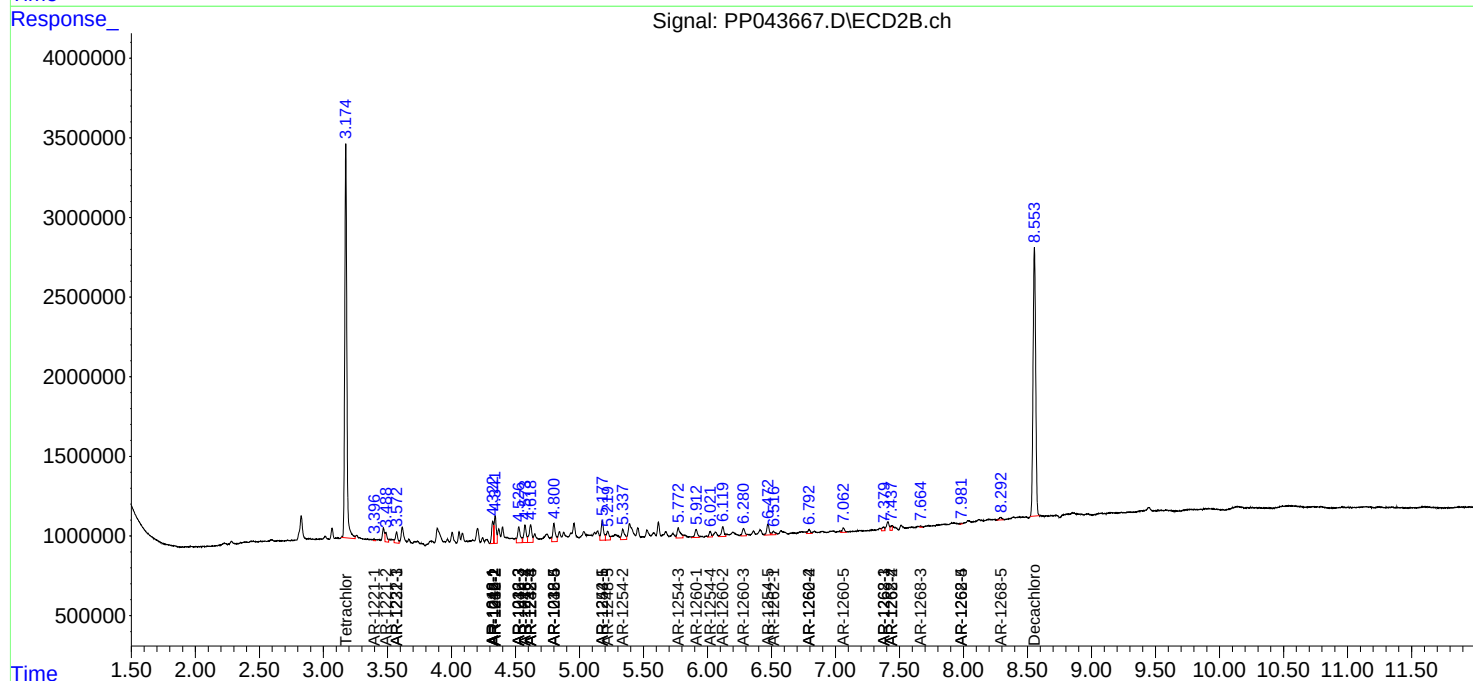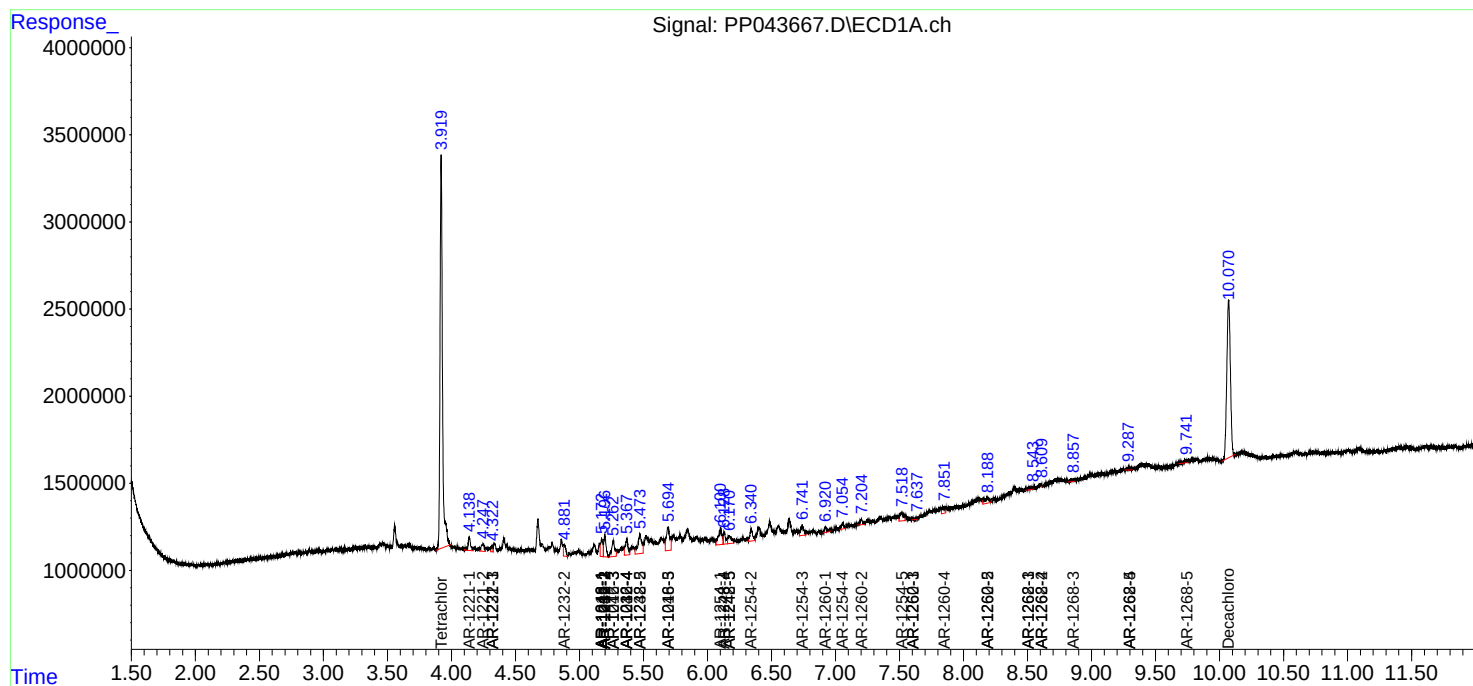


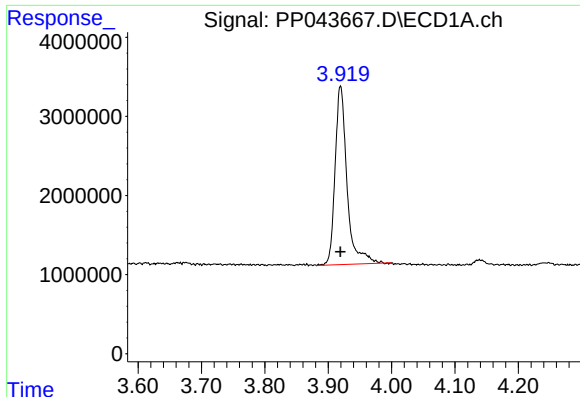

#1 Tetrachloro-m-xylene


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 29568891
Conc: 13.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

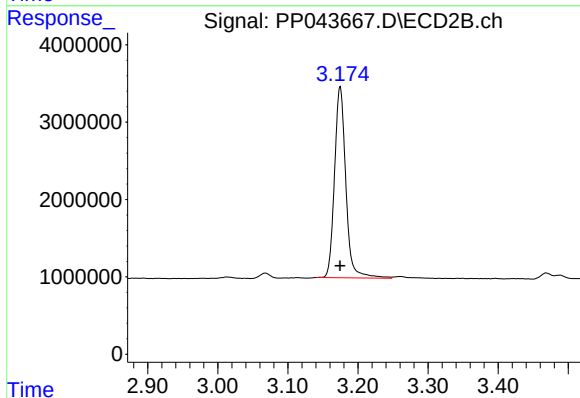


#1 Tetrachloro-m-xylene

R.T.: 3.175 min
Delta R.T.: 0.000 min
Response: 27662395
Conc: 14.73 ng/ml

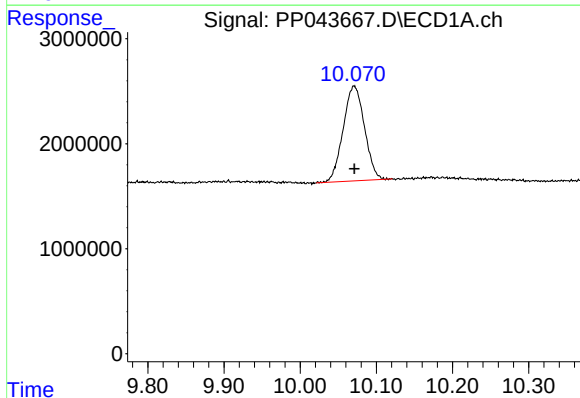


#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.000 min
Response: 17586335
Conc: 14.80 ng/ml

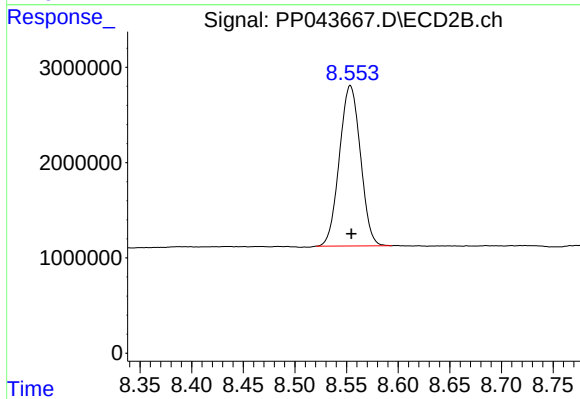

#2 Decachlorobiphenyl


R.T.: 8.554 min
Delta R.T.: -0.001 min
Response: 23849168
Conc: 14.70 ng/ml

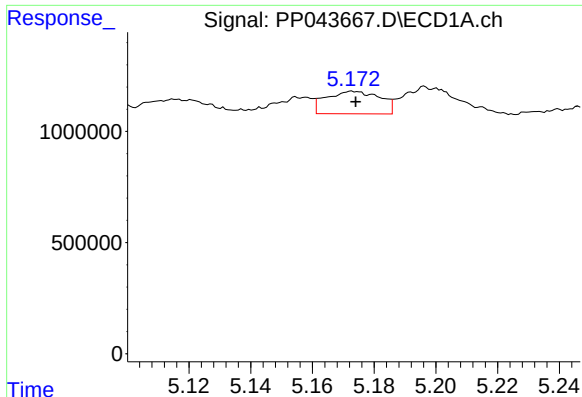

#3 AR-1016-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 1226049
Conc: 16.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

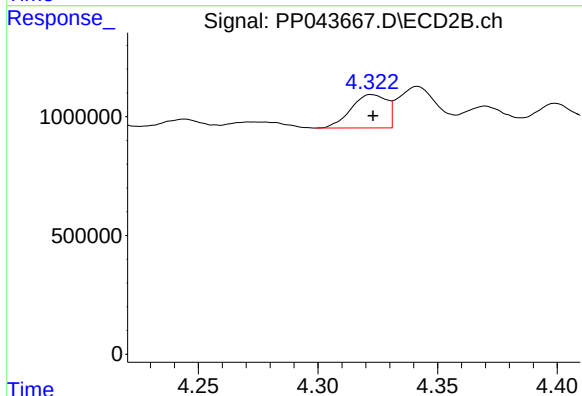


#3 AR-1016-1

R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 1461556
Conc: 23.85 ng/ml

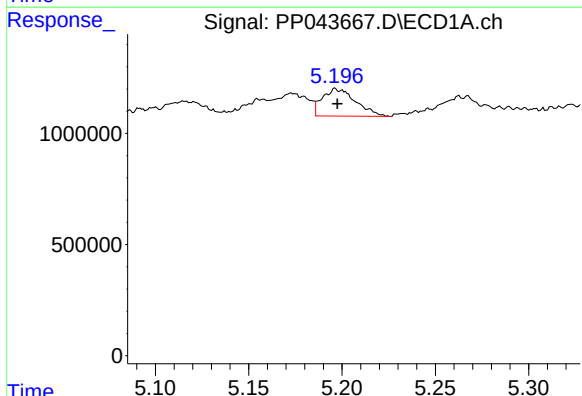


#4 AR-1016-2

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 1535600
Conc: 14.56 ng/ml

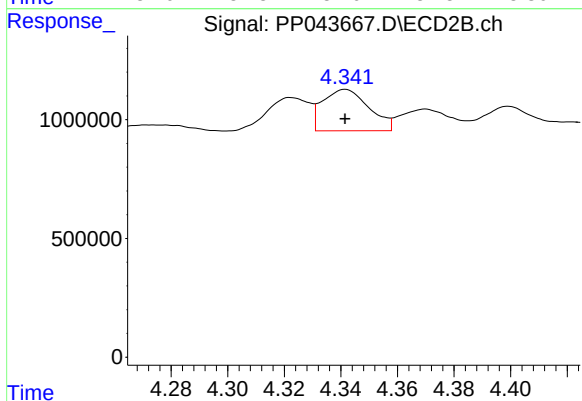

#4 AR-1016-2


R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 1975439
Conc: 23.38 ng/ml

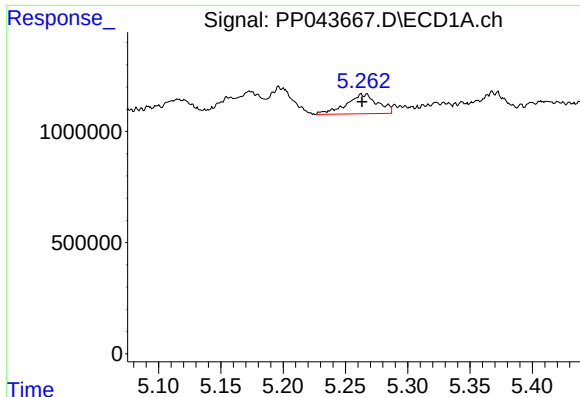

#5 AR-1016-3


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 1565256
Conc: 23.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

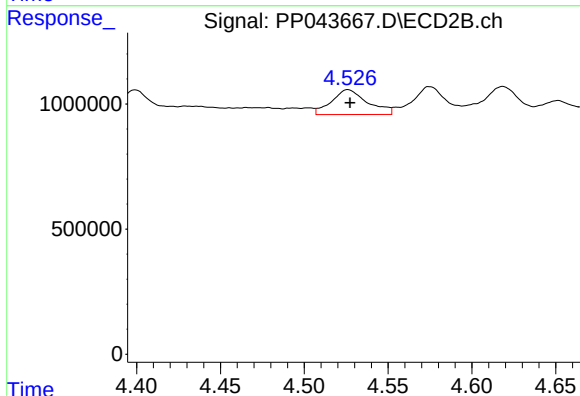


#5 AR-1016-3

R.T.: 4.526 min
Delta R.T.: -0.001 min
Response: 1489507
Conc: 31.88 ng/ml

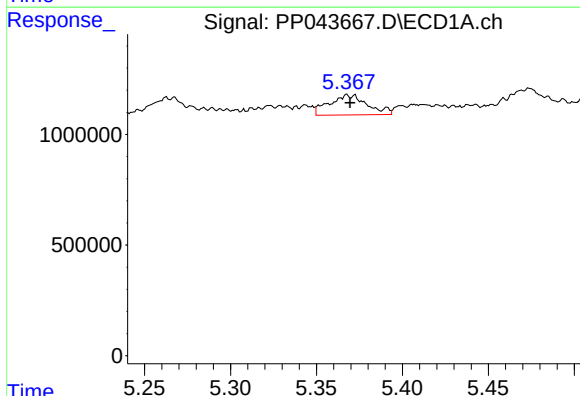


#6 AR-1016-4

R.T.: 5.368 min
Delta R.T.: -0.002 min
Response: 1398587
Conc: 25.79 ng/ml

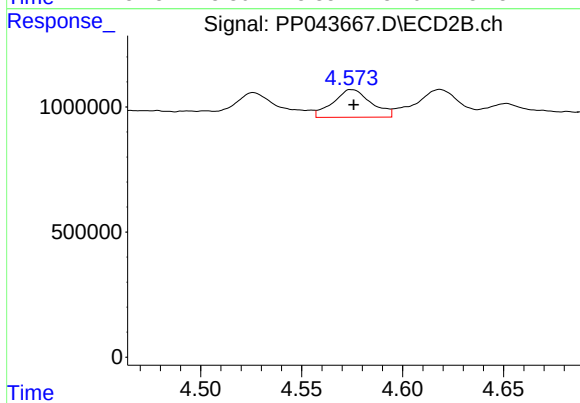

#6 AR-1016-4


R.T.: 4.574 min
Delta R.T.: -0.002 min
Response: 1455215
Conc: 38.94 ng/ml

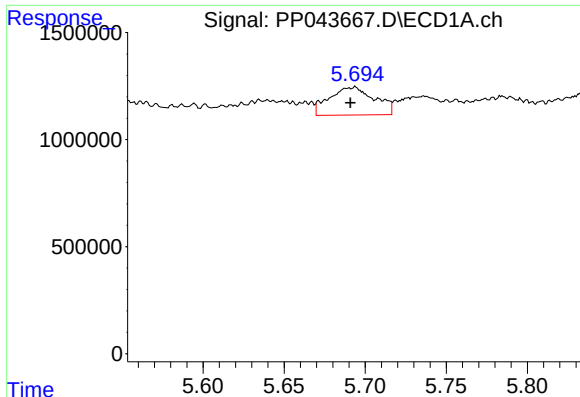

#7 AR-1016-5


R.T.: 5.693 min
Delta R.T.: 0.002 min
Response: 2546348
Conc: 48.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

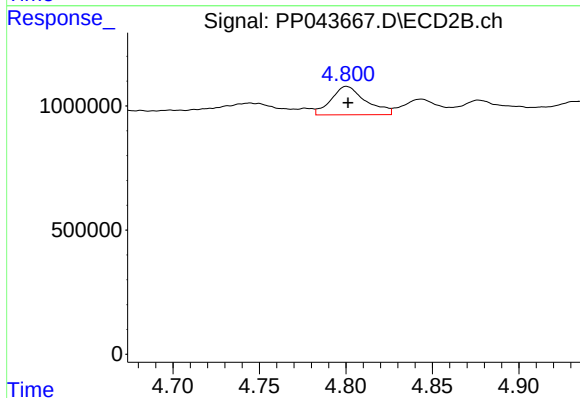


#7 AR-1016-5

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1594582
Conc: 34.91 ng/ml

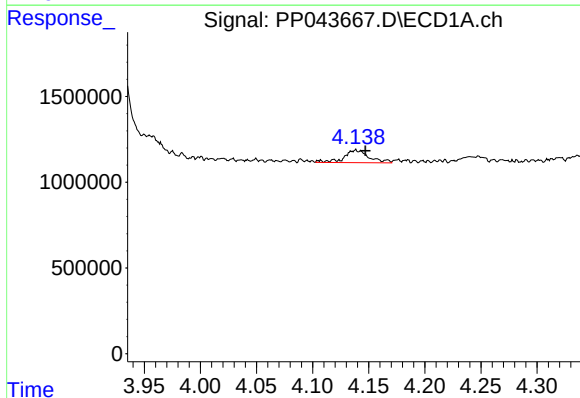


#8 AR-1221-1

R.T.: 4.138 min
Delta R.T.: -0.009 min
Response: 1129273
Conc: 44.36 ng/ml

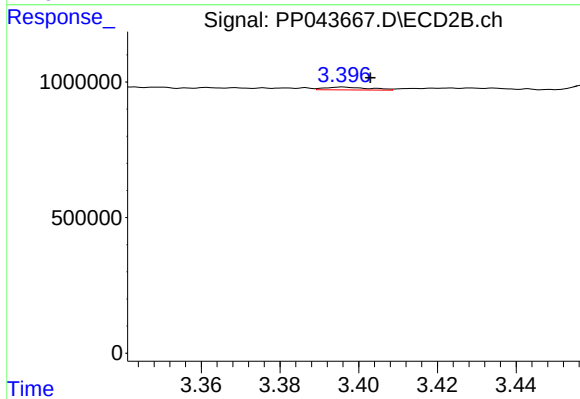

#8 AR-1221-1


R.T.: 3.396 min
Delta R.T.: -0.007 min
Response: 83353
Conc: 3.49 ng/ml

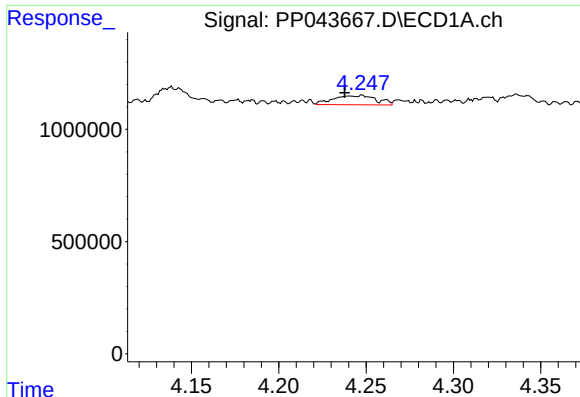

#9 AR-1221-2


R.T.: 4.248 min
Delta R.T.: 0.010 min
Response: 709386
Conc: 36.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

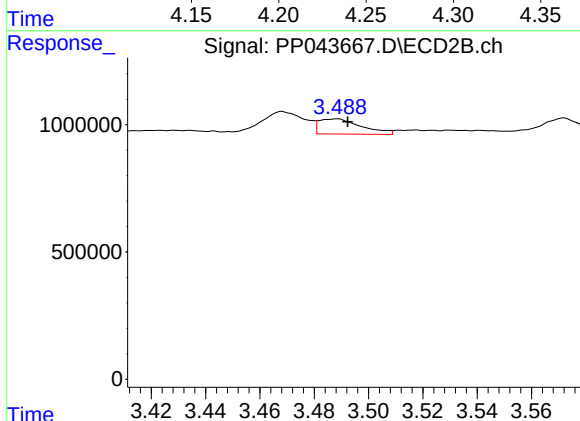


#9 AR-1221-2

R.T.: 3.489 min
Delta R.T.: -0.004 min
Response: 647372
Conc: 35.85 ng/ml

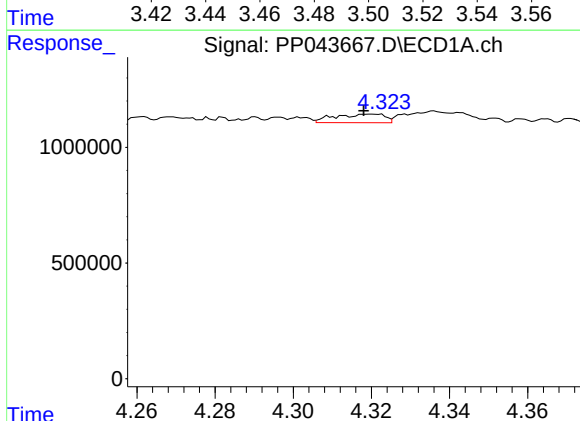


#10 AR-1221-3

R.T.: 4.320 min
Delta R.T.: 0.002 min
Response: 331924
Conc: 5.78 ng/ml

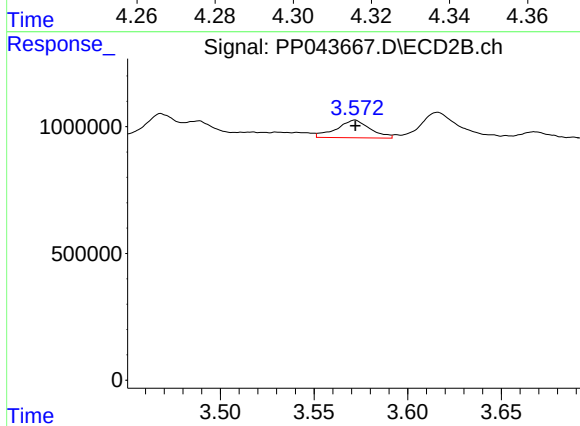

#10 AR-1221-3


R.T.: 3.572 min
Delta R.T.: 0.000 min
Response: 873158
Conc: 16.93 ng/ml

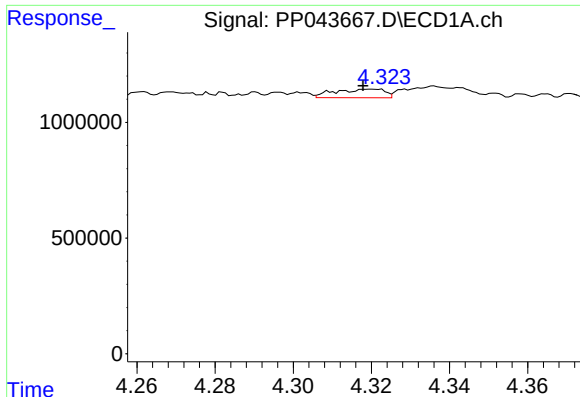

#11 AR-1232-1


R.T.: 4.320 min
Delta R.T.: 0.002 min
Response: 331924
Conc: 6.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

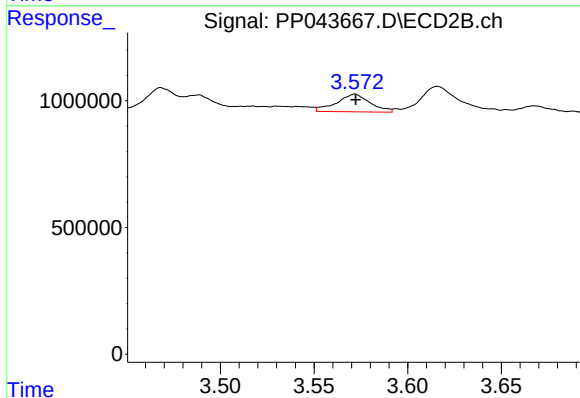


#11 AR-1232-1

R.T.: 3.572 min
Delta R.T.: 0.000 min
Response: 873158
Conc: 20.29 ng/ml

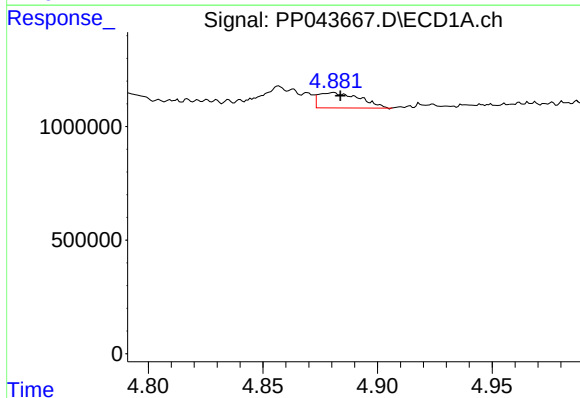


#12 AR-1232-2

R.T.: 4.880 min
Delta R.T.: -0.003 min
Response: 846137
Conc: 35.71 ng/ml

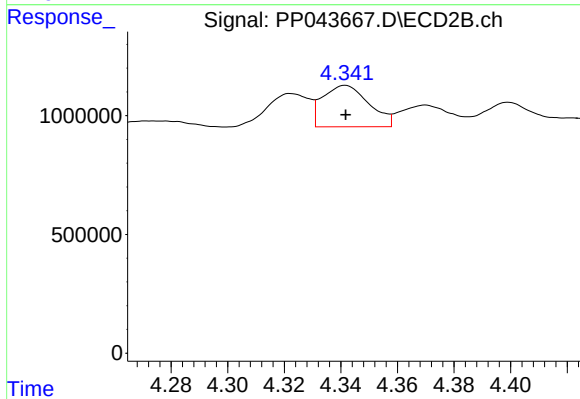

#12 AR-1232-2


R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 1975439
Conc: 55.34 ng/ml

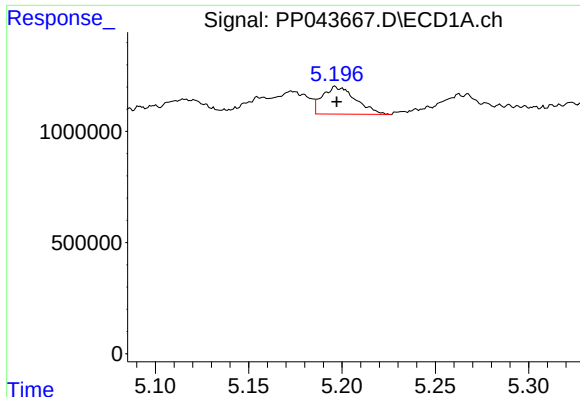

#13 AR-1232-3


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 1535600
Conc: 35.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

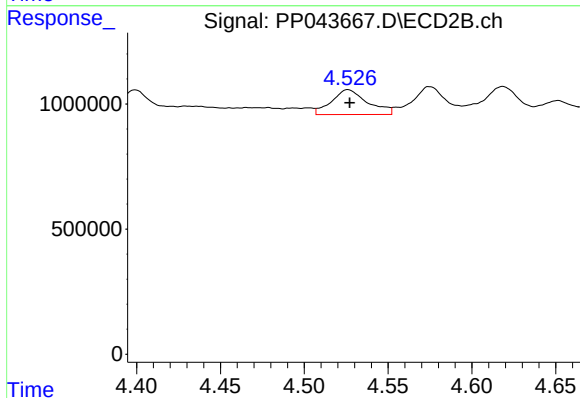


#13 AR-1232-3

R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 1489507
Conc: 76.17 ng/ml

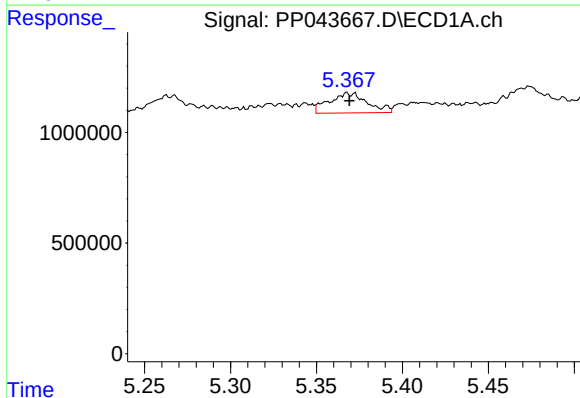


#14 AR-1232-4

R.T.: 5.368 min
Delta R.T.: -0.001 min
Response: 1398587
Conc: 64.07 ng/ml

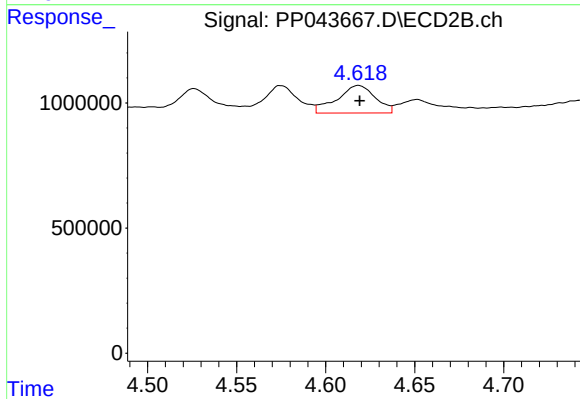

#14 AR-1232-4


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 1647292
Conc: 95.26 ng/ml

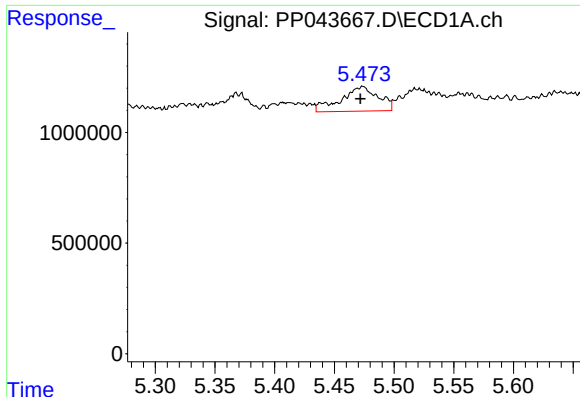

#15 AR-1232-5


R.T.: 5.474 min
Delta R.T.: 0.002 min
Response: 2406678
Conc: 149.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

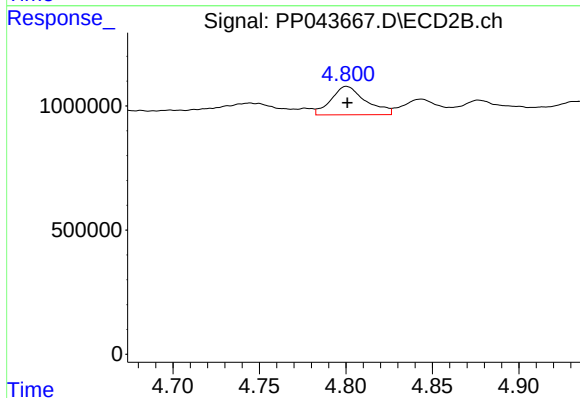


#15 AR-1232-5

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1594582
Conc: 84.89 ng/ml

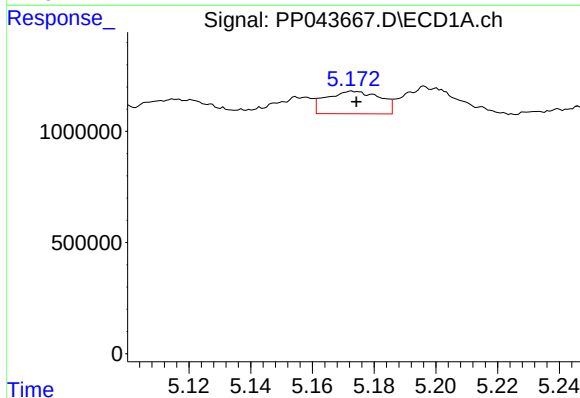


#16 AR-1242-1

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 1226049
Conc: 21.82 ng/ml

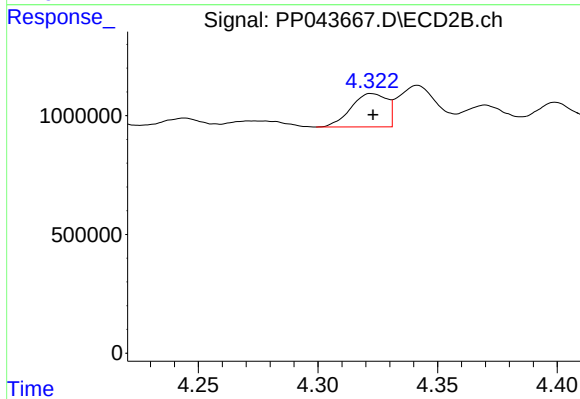

#16 AR-1242-1


R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 1461556
Conc: 29.98 ng/ml

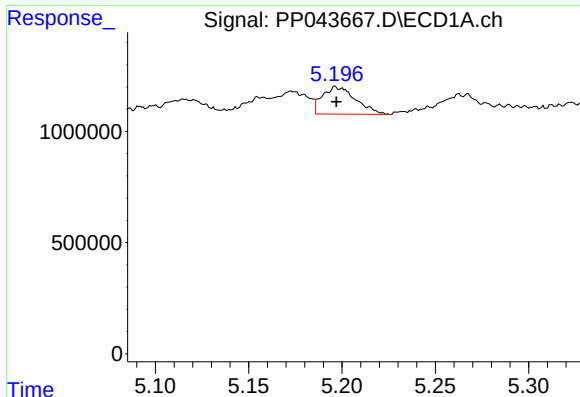

#17 AR-1242-2


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 1535600
Conc: 18.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

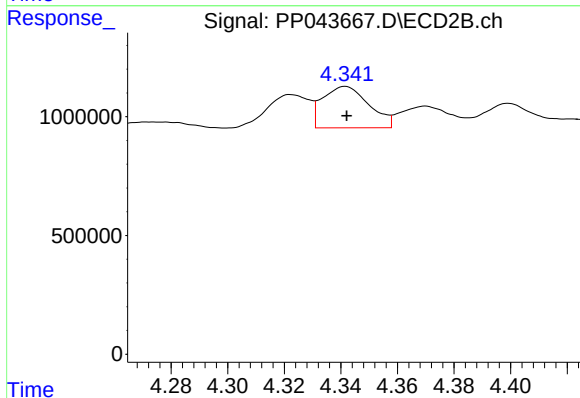


#17 AR-1242-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 1975439
Conc: 29.34 ng/ml

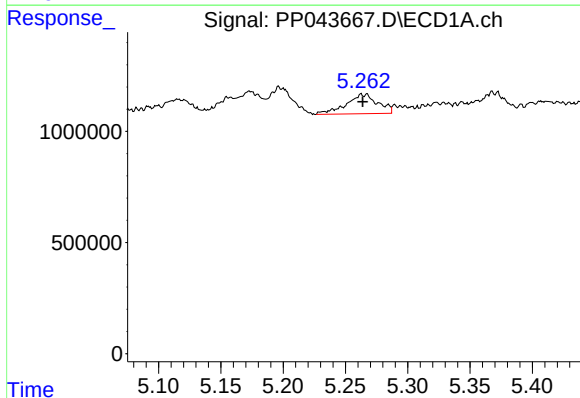


#18 AR-1242-3

R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 1565256
Conc: 30.24 ng/ml

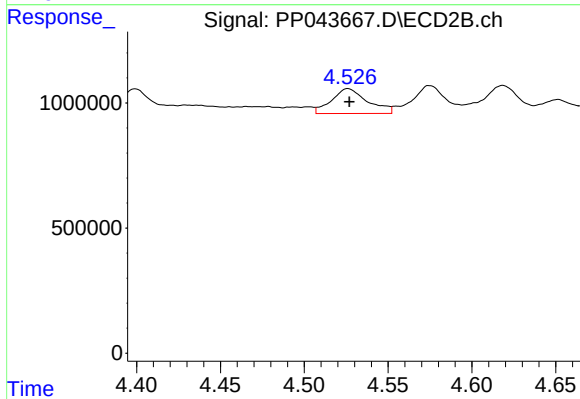

#18 AR-1242-3


R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 1489507
Conc: 39.68 ng/ml

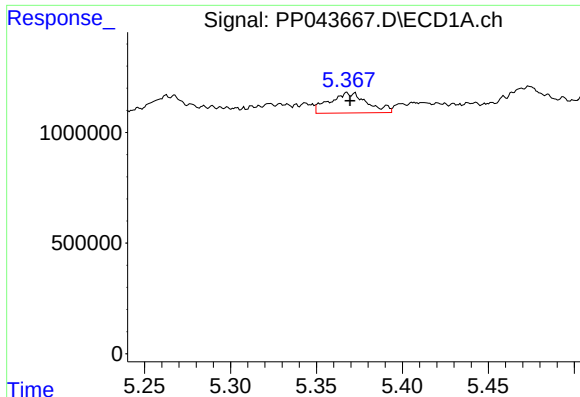

#19 AR-1242-4


R.T.: 5.368 min
Delta R.T.: -0.002 min
Response: 1398587
Conc: 32.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

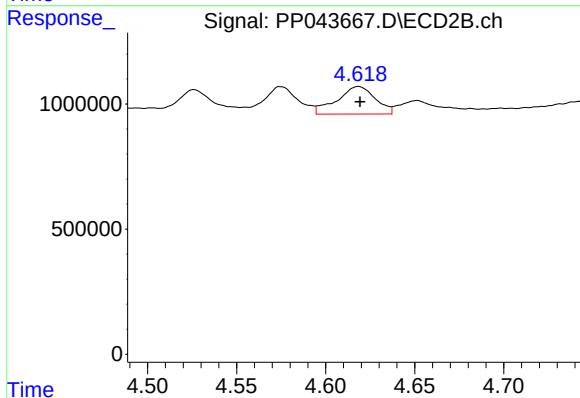


#19 AR-1242-4

R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 1647292
Conc: 45.62 ng/ml

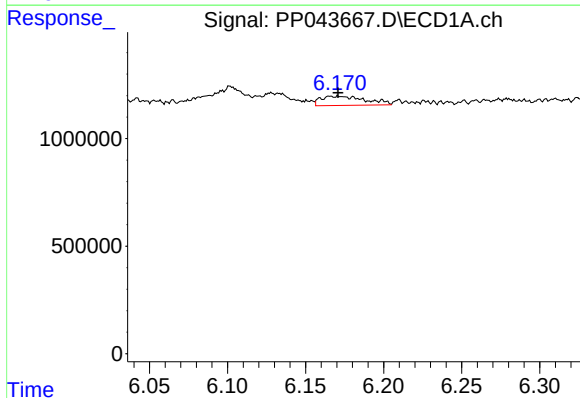


#20 AR-1242-5

R.T.: 6.166 min
Delta R.T.: -0.005 min
Response: 857693
Conc: 19.86 ng/ml

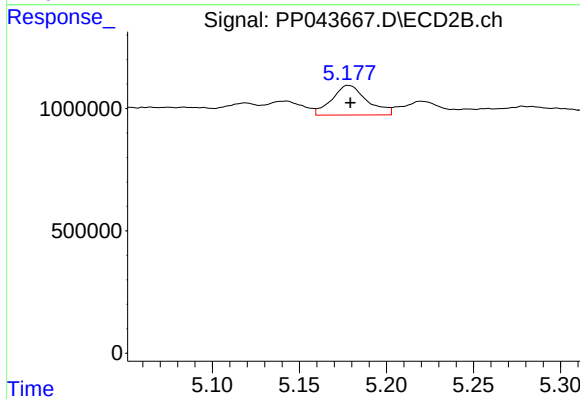

#20 AR-1242-5


R.T.: 5.178 min
Delta R.T.: -0.001 min
Response: 1713046
Conc: 39.79 ng/ml

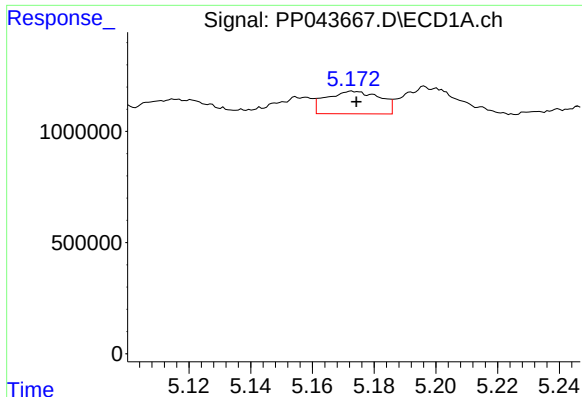

#21 AR-1248-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 1226049
Conc: 29.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

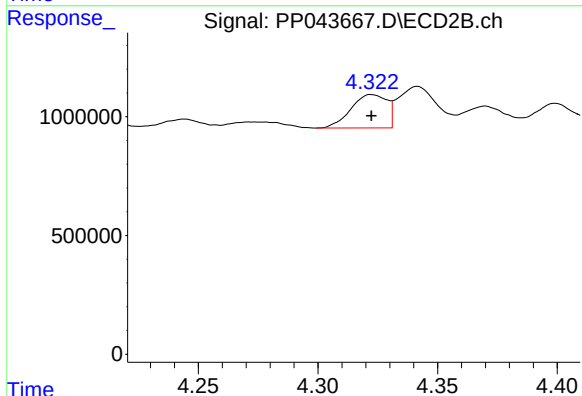


#21 AR-1248-1

R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 1461556
Conc: 39.24 ng/ml

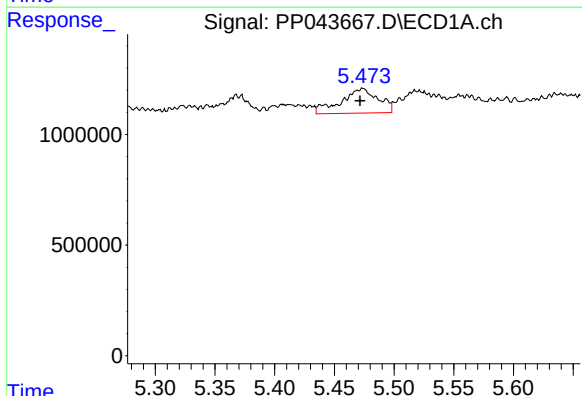


#22 AR-1248-2

R.T.: 5.474 min
Delta R.T.: 0.002 min
Response: 2406678
Conc: 42.36 ng/ml

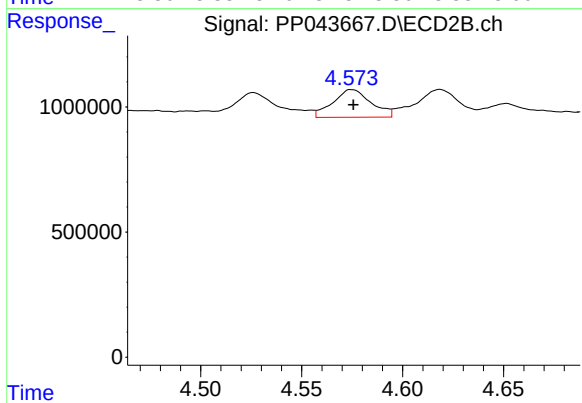

#22 AR-1248-2


R.T.: 4.574 min
Delta R.T.: -0.001 min
Response: 1455215
Conc: 29.75 ng/ml

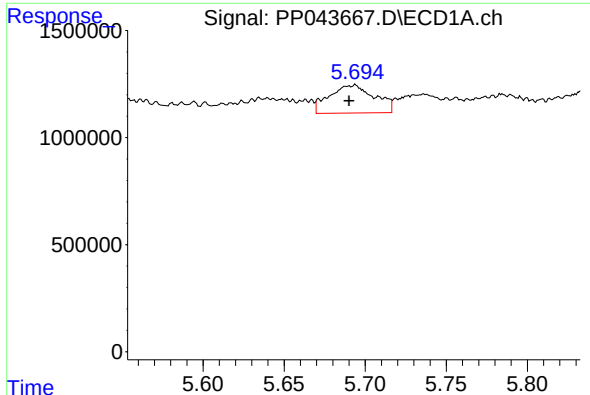

#23 AR-1248-3


R.T.: 5.693 min
Delta R.T.: 0.003 min
Response: 2546348
Conc: 38.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

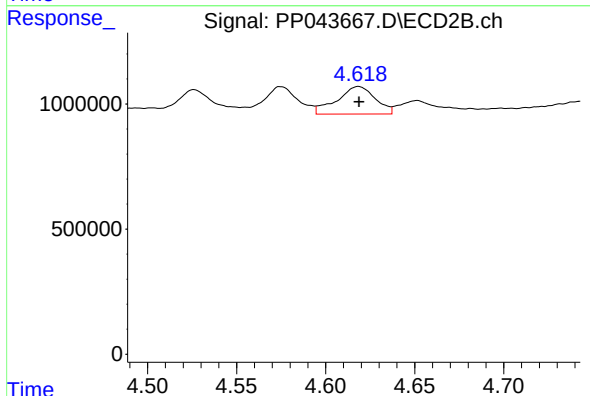


#23 AR-1248-3

R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 1647292
Conc: 32.10 ng/ml

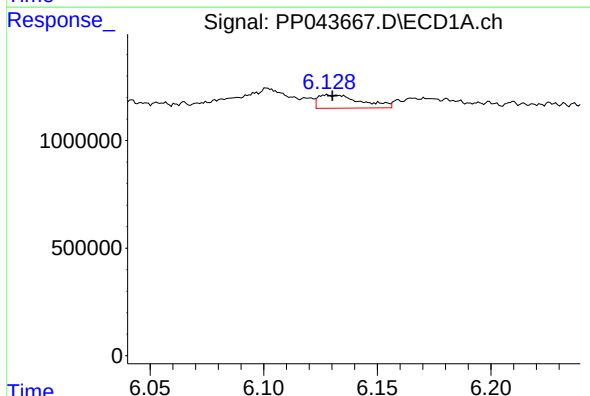


#24 AR-1248-4

R.T.: 6.128 min
Delta R.T.: -0.002 min
Response: 796481
Conc: 11.40 ng/ml

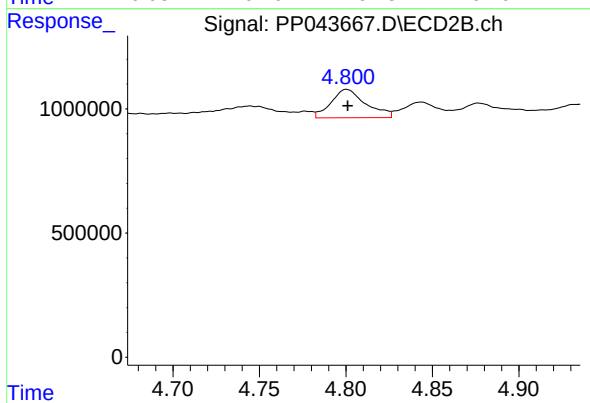

#24 AR-1248-4


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1594582
Conc: 27.20 ng/ml

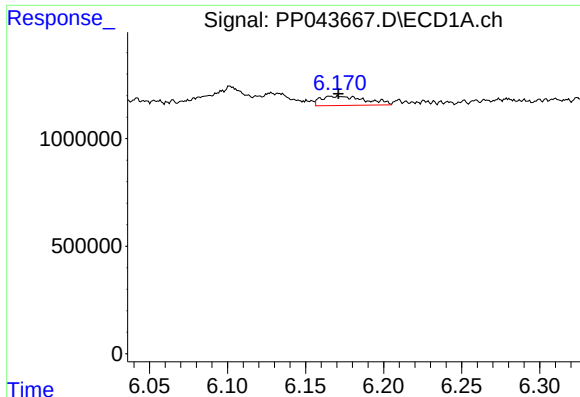

#25 AR-1248-5


R.T.: 6.166 min
Delta R.T.: -0.005 min
Response: 857693
Conc: 12.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

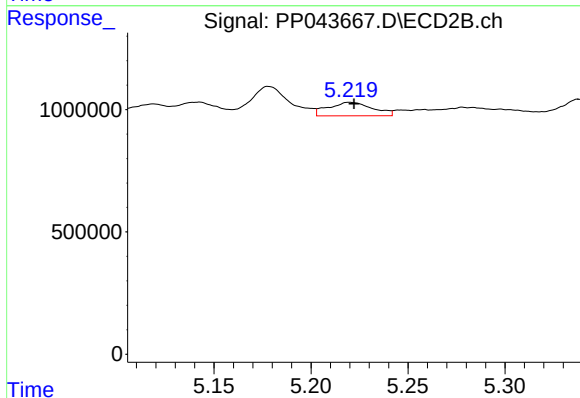


#25 AR-1248-5

R.T.: 5.220 min
Delta R.T.: -0.002 min
Response: 879052
Conc: 15.34 ng/ml

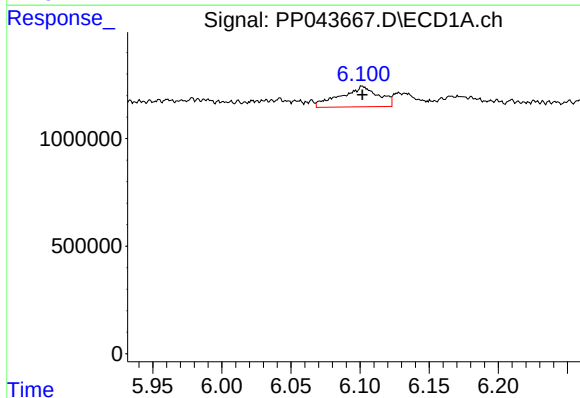


#26 AR-1254-1

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 1801954
Conc: 23.85 ng/ml

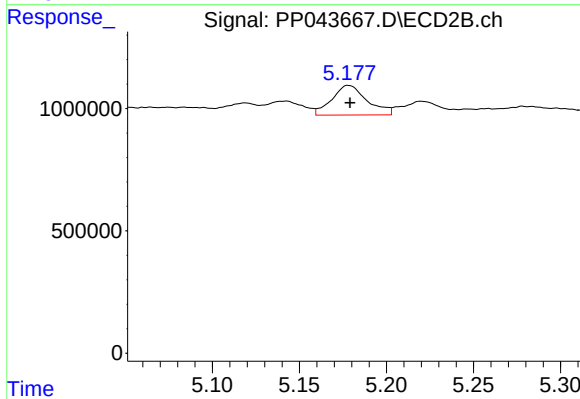

#26 AR-1254-1


R.T.: 5.178 min
Delta R.T.: -0.001 min
Response: 1713046
Conc: 19.62 ng/ml

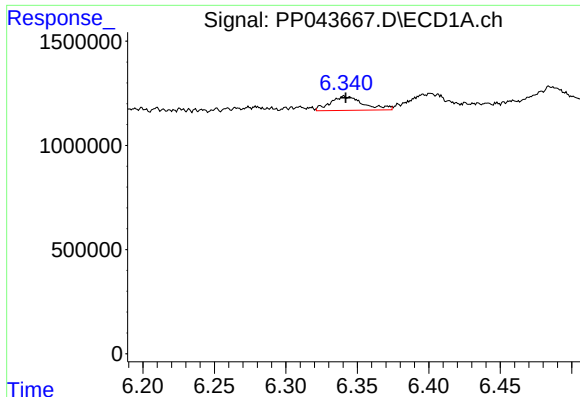

#27 AR-1254-2


R.T.: 6.341 min
Delta R.T.: -0.001 min
Response: 1079922
Conc: 9.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

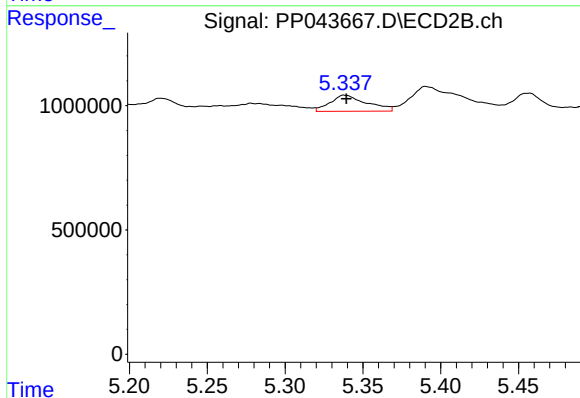


#27 AR-1254-2

R.T.: 5.338 min
Delta R.T.: -0.001 min
Response: 1063619
Conc: 13.94 ng/ml

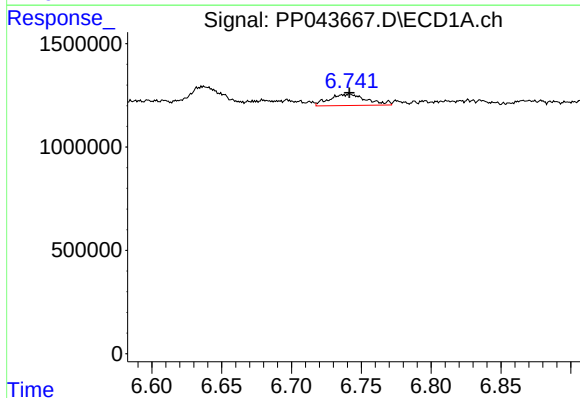


#28 AR-1254-3

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 1009284
Conc: 8.72 ng/ml

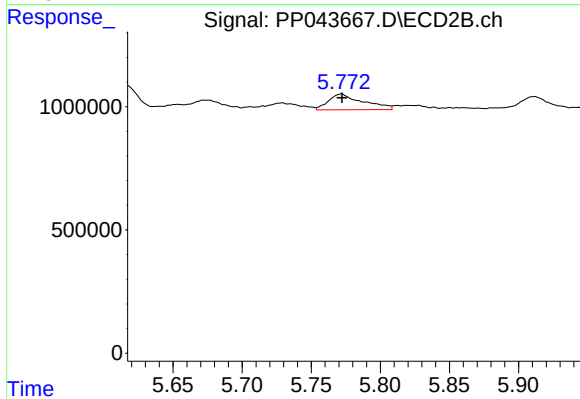

#28 AR-1254-3


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 1105096
Conc: 9.02 ng/ml

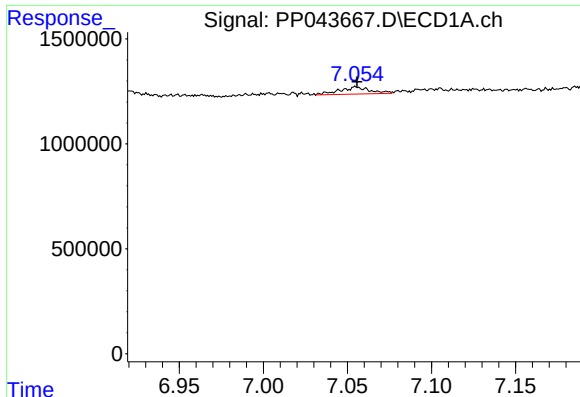

#29 AR-1254-4


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 430708
Conc: 5.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

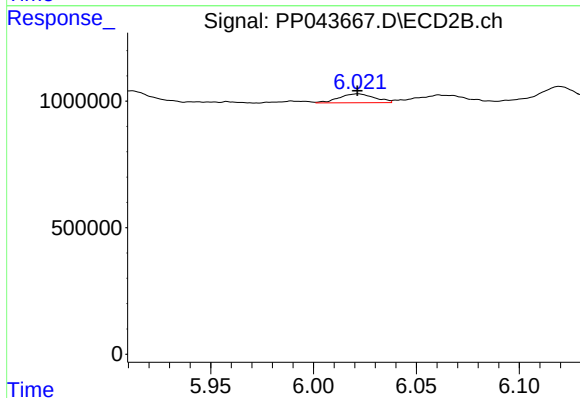


#29 AR-1254-4

R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 418993
Conc: 5.31 ng/ml

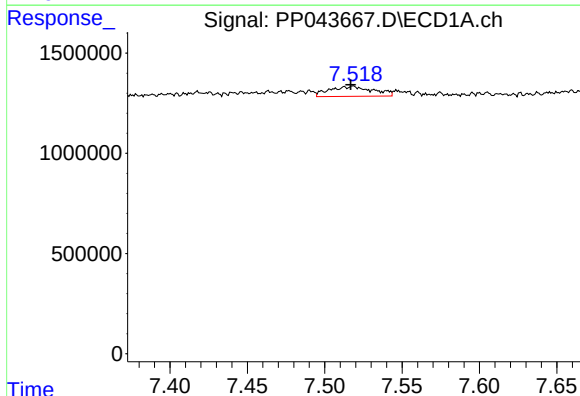


#30 AR-1254-5

R.T.: 7.518 min
Delta R.T.: 0.001 min
Response: 988178
Conc: 11.52 ng/ml

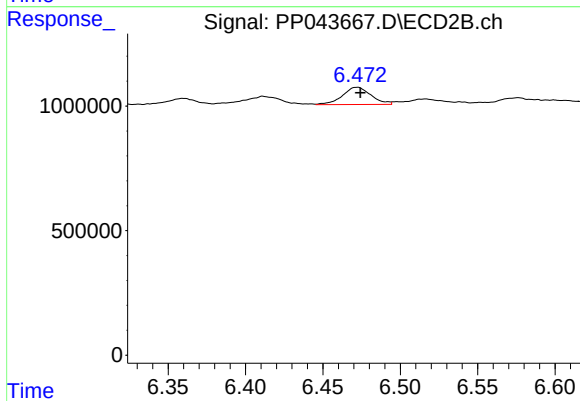

#30 AR-1254-5


R.T.: 6.472 min
Delta R.T.: -0.002 min
Response: 886896
Conc: 7.67 ng/ml

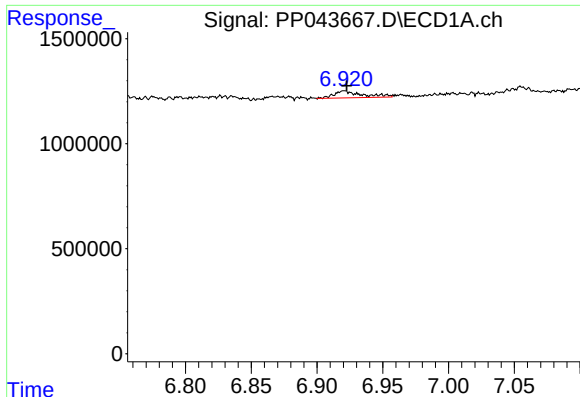

#31 AR-1260-1


R.T.: 6.921 min
Delta R.T.: -0.002 min
Response: 486621
Conc: 5.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

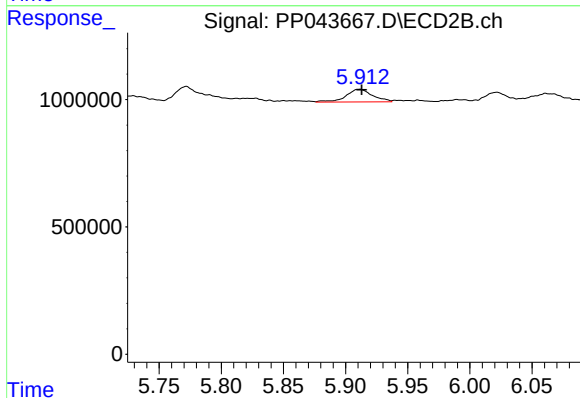


#31 AR-1260-1

R.T.: 5.912 min
Delta R.T.: -0.001 min
Response: 737766
Conc: 9.23 ng/ml

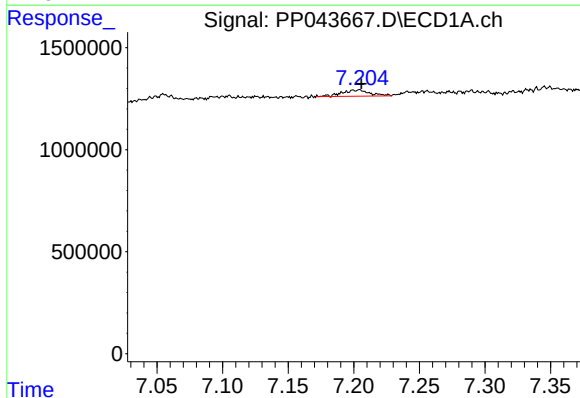


#32 AR-1260-2

R.T.: 7.204 min
Delta R.T.: -0.002 min
Response: 444037
Conc: 4.91 ng/ml

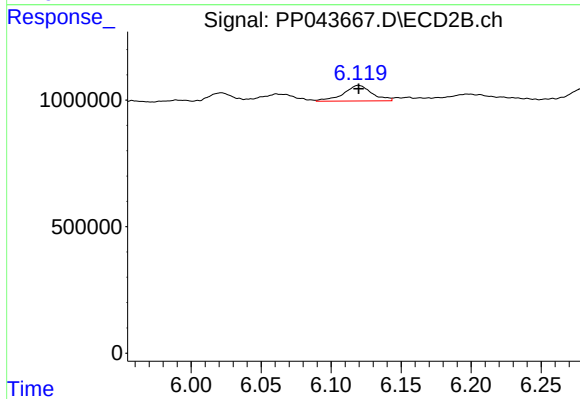

#32 AR-1260-2


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 873315
Conc: 8.94 ng/ml

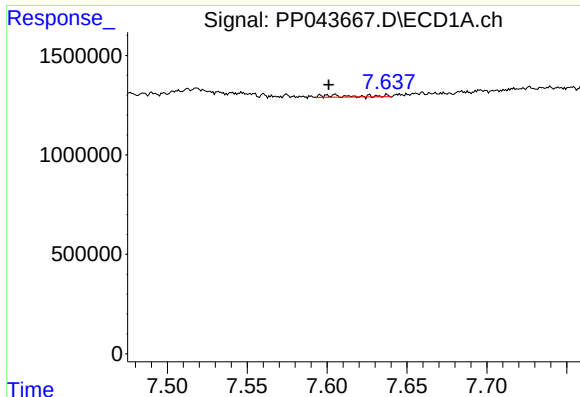

#33 AR-1260-3


R.T.: 7.605 min
Delta R.T.: 0.004 min
Response: 134107
Conc: 1.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

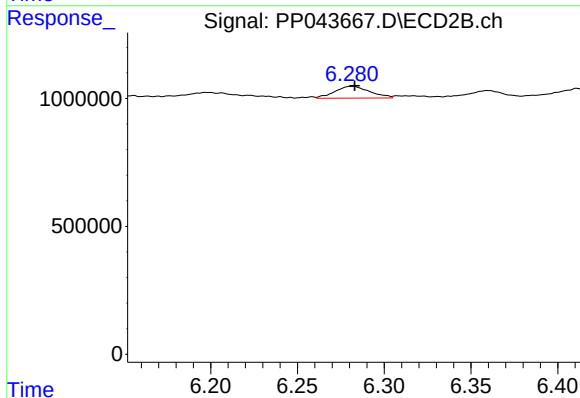


#33 AR-1260-3

R.T.: 6.282 min
Delta R.T.: -0.001 min
Response: 656461
Conc: 7.19 ng/ml

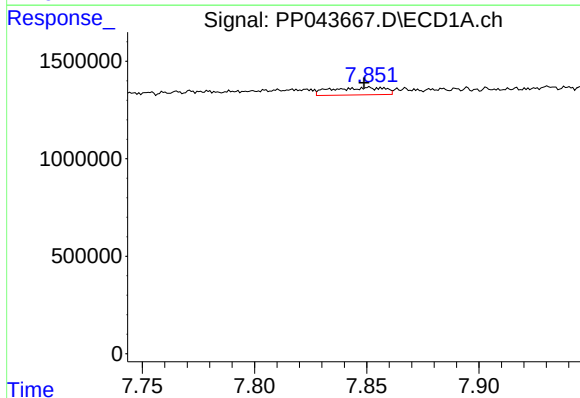


#34 AR-1260-4

R.T.: 7.851 min
Delta R.T.: 0.002 min
Response: 624119
Conc: 7.27 ng/ml

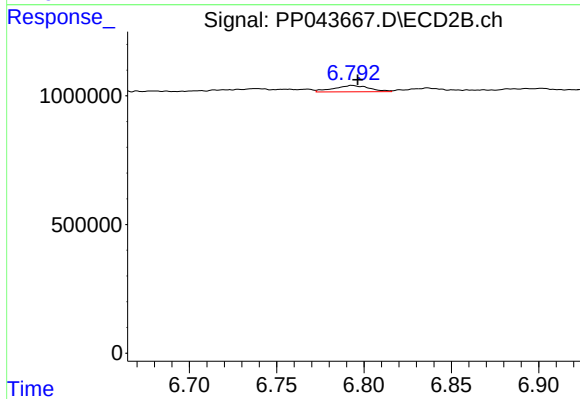

#34 AR-1260-4


R.T.: 6.793 min
Delta R.T.: -0.003 min
Response: 356044
Conc: 4.40 ng/ml

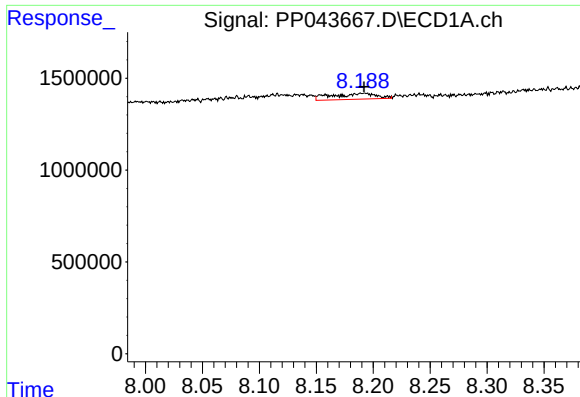

#35 AR-1260-5


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 876747
Conc: 5.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

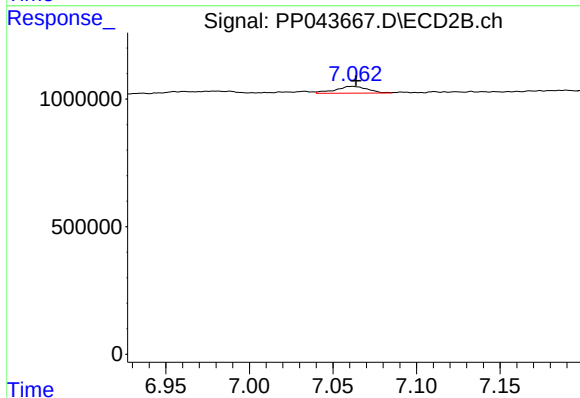


#35 AR-1260-5

R.T.: 7.062 min
Delta R.T.: -0.002 min
Response: 366642
Conc: 1.98 ng/ml

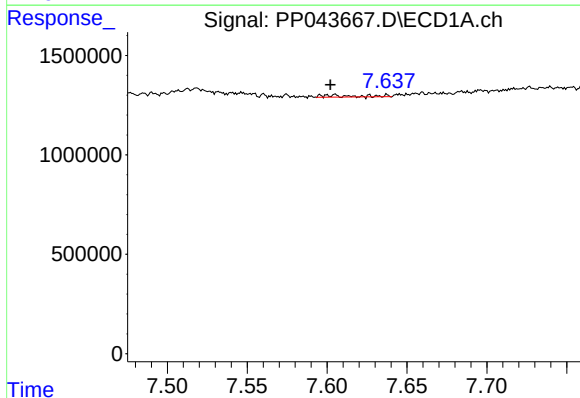


#36 AR-1262-1

R.T.: 7.605 min
Delta R.T.: 0.003 min
Response: 134107
Conc: 1.36 ng/ml

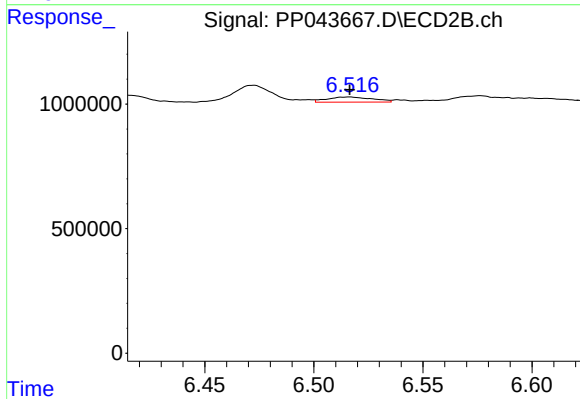

#36 AR-1262-1


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 301729
Conc: 2.74 ng/ml

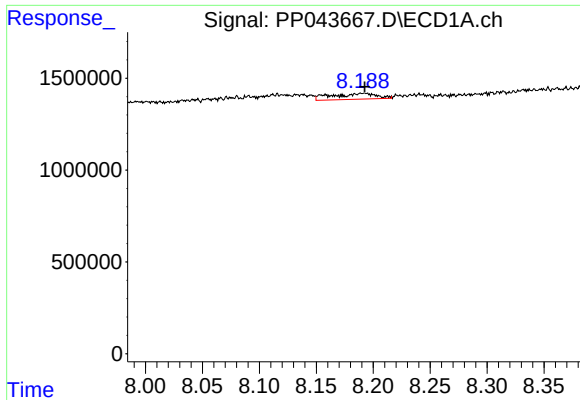

#37 AR-1262-2


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 876747
Conc: 5.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

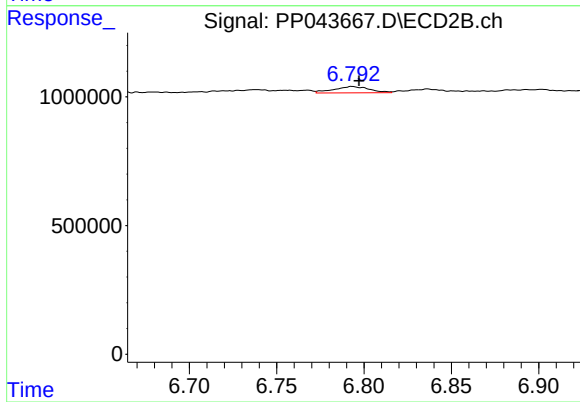


#37 AR-1262-2

R.T.: 6.793 min
Delta R.T.: -0.004 min
Response: 356044
Conc: 3.49 ng/ml

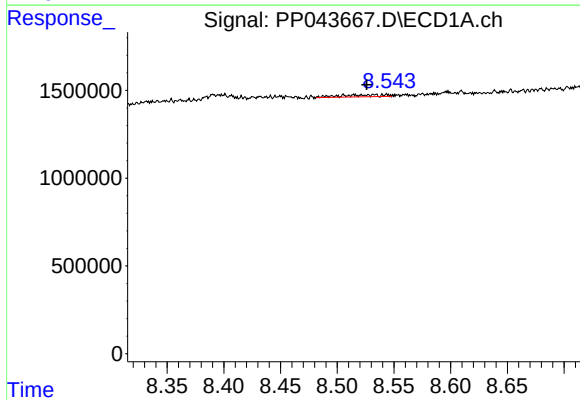


#38 AR-1262-3

R.T.: 8.515 min
Delta R.T.: -0.011 min
Response: 301855
Conc: 2.76 ng/ml

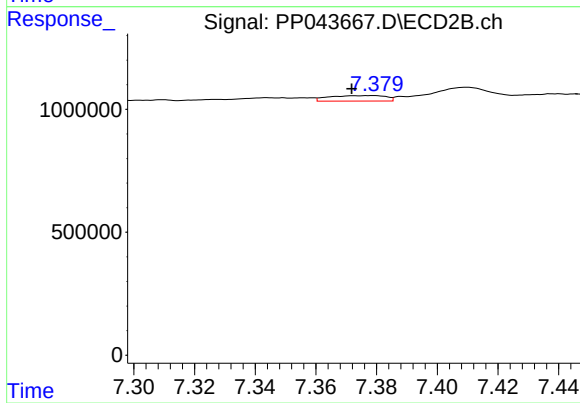

#38 AR-1262-3


R.T.: 7.379 min
Delta R.T.: 0.008 min
Response: 293010
Conc: 3.44 ng/ml

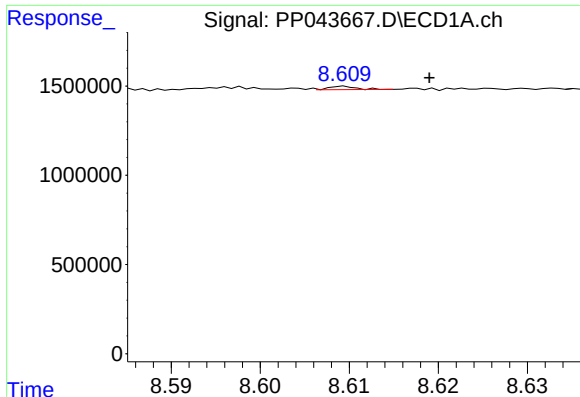

#39 AR-1262-4


R.T.: 8.610 min
Delta R.T.: -0.009 min
Response: 39752
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

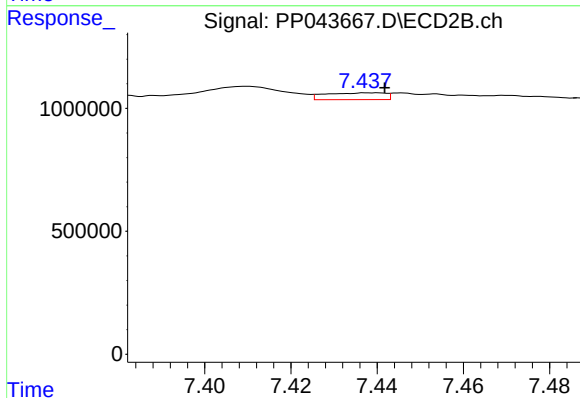


#39 AR-1262-4

R.T.: 7.440 min
Delta R.T.: -0.002 min
Response: 267530
Conc: 1.72 ng/ml

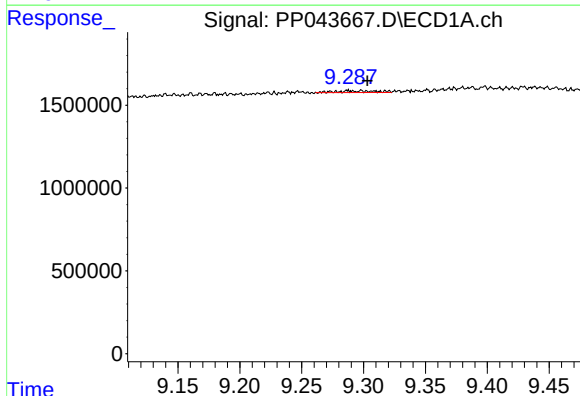


#40 AR-1262-5

R.T.: 9.298 min
Delta R.T.: -0.005 min
Response: 230903
Conc: 4.15 ng/ml

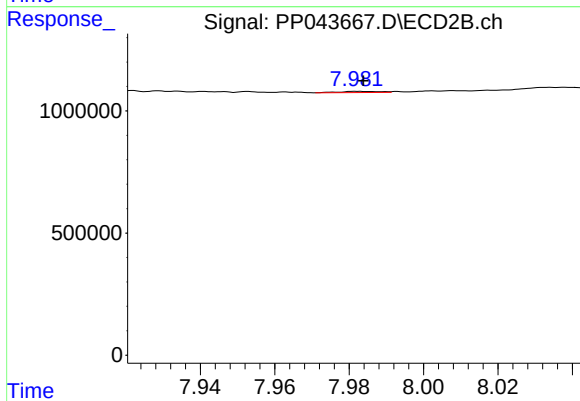

#40 AR-1262-5


R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 35182
Conc: 0.45 ng/ml

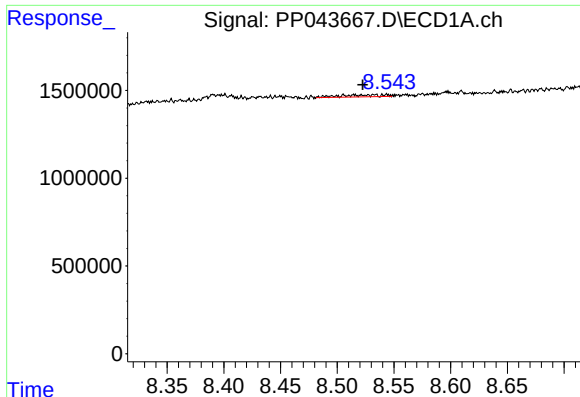

#41 AR-1268-1


R.T.: 8.515 min
Delta R.T.: -0.008 min
Response: 301855
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

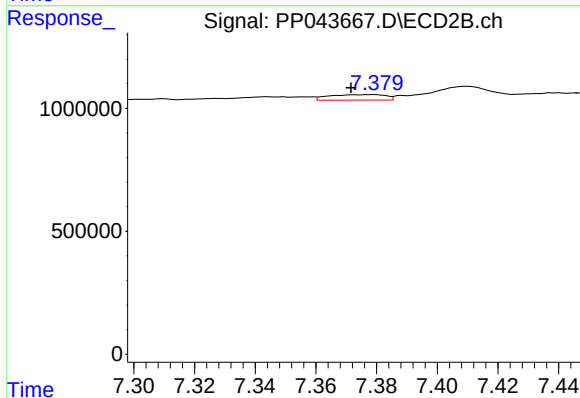


#41 AR-1268-1

R.T.: 7.379 min
Delta R.T.: 0.008 min
Response: 293010
Conc: 1.16 ng/ml

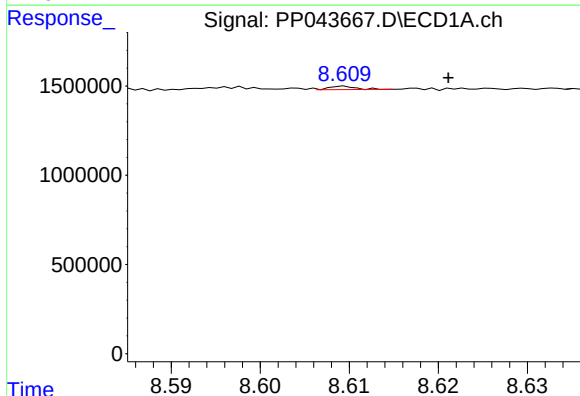


#42 AR-1268-2

R.T.: 8.610 min
Delta R.T.: -0.012 min
Response: 39752
Conc: 0.23 ng/ml

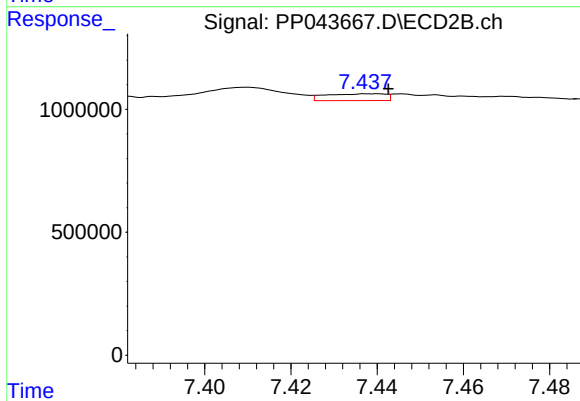

#42 AR-1268-2


R.T.: 7.440 min
Delta R.T.: -0.002 min
Response: 267530
Conc: 1.18 ng/ml

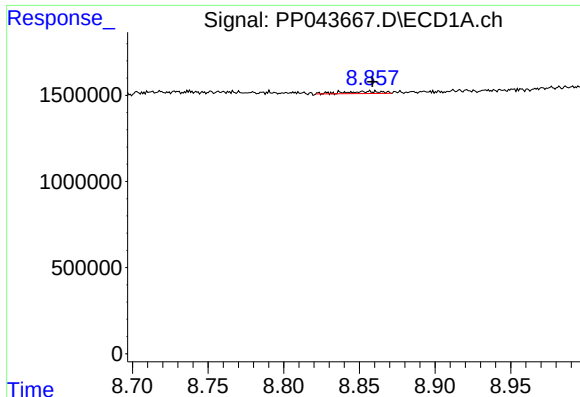

#43 AR-1268-3


R.T.: 8.857 min
Delta R.T.: -0.002 min
Response: 213350
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

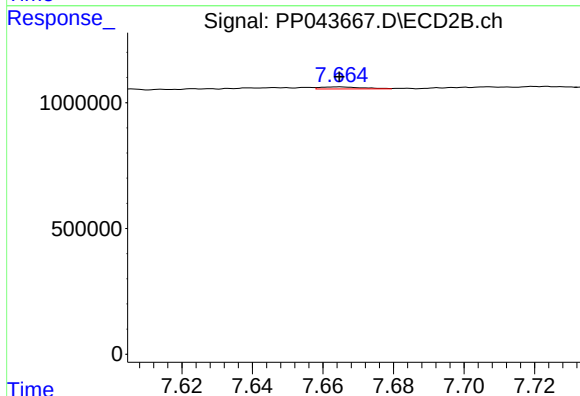


#43 AR-1268-3

R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 67085
Conc: 0.34 ng/ml

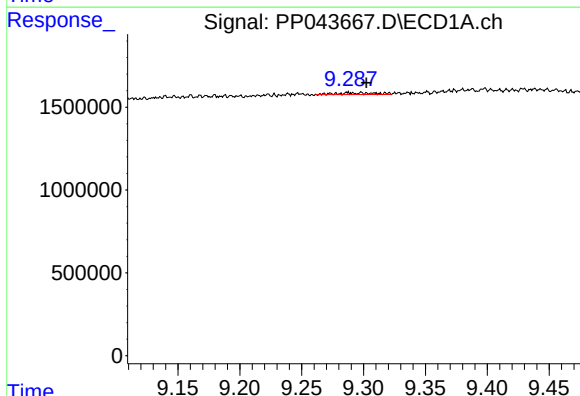


#44 AR-1268-4

R.T.: 9.298 min
Delta R.T.: -0.004 min
Response: 230903
Conc: 3.69 ng/ml

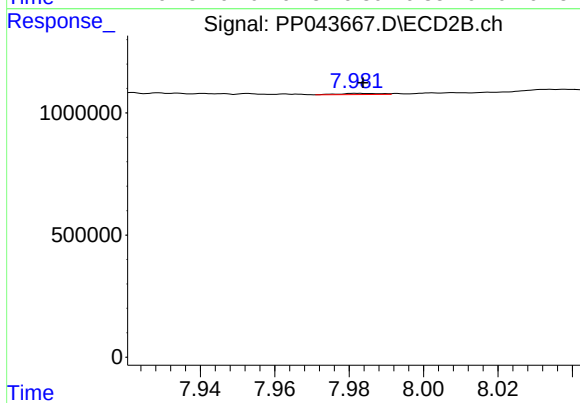

#44 AR-1268-4


R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 35182
Conc: 0.39 ng/ml

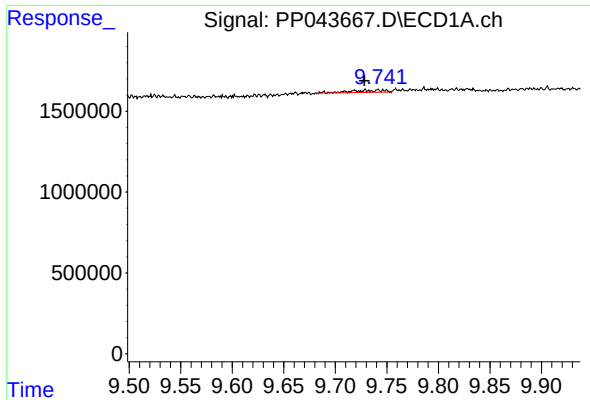

#45 AR-1268-5

R.T.: 9.742 min
Delta R.T.: 0.014 min
Response: 289152
Conc: 0.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-02

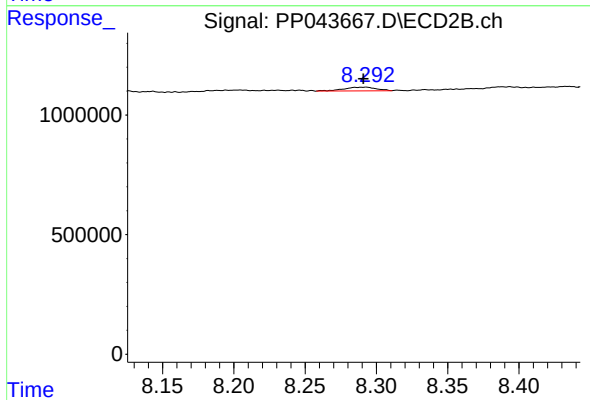

#45 AR-1268-5

R.T.: 8.293 min
Delta R.T.: 0.002 min
Response: 253292
Conc: 0.42 ng/ml