

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:47
 Operator : YP\AJ
 Sample : N1523-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:24:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.919	3.175	47900974	43557197	21.664	23.190
2) SA Decachlor...	10.071	8.553	29268511	38052466	24.639	23.455
Target Compounds						
3) L1 AR-1016-1	5.173	4.321	1799254	2279917	24.796	37.211 #
4) L1 AR-1016-2	5.197	4.340	2604466	2590989	24.694	30.667
5) L1 AR-1016-3	5.265	4.526	1395995	1604864	21.201	34.353 #
6) L1 AR-1016-4	5.368	4.575	998876	1135779	18.419	30.392 #
7) L1 AR-1016-5	5.689	4.803	2009856	931046	38.263	20.381 #
8) L2 AR-1221-1	4.153	3.399	171561	747168	6.739	31.323 #
9) L2 AR-1221-2	4.243	3.487	2520899	1710374	131.308	94.705 #
10) L2 AR-1221-3	4.319	3.571	1953235	3941002	34.001	76.394 #
11) L3 AR-1232-1	4.319	3.571	1953235	3941002	40.246	91.598 #
12) L3 AR-1232-2	4.883	4.340	1151448	2590989	48.590	72.581 #
13) L3 AR-1232-3	5.197	4.526	2604466	1604864	60.493	82.073 #
14) L3 AR-1232-4	5.368	4.618	998876	1130748	45.761	65.390 #
15) L3 AR-1232-5	5.473	4.803	1343786	931046	83.314	49.565 #
16) L4 AR-1242-1	5.173	4.321	1799254	2279917	32.020	46.770 #
17) L4 AR-1242-2	5.197	4.340	2604466	2590989	31.480	38.479
18) L4 AR-1242-3	5.265	4.526	1395995	1604864	26.971	42.753 #
19) L4 AR-1242-4	5.368	4.618	998876	1130748	23.386	31.314 #
20) L4 AR-1242-5	6.168	5.178	622469	2103419	14.415	48.862 #
21) L5 AR-1248-1	5.173	4.321	1799254	2279917	43.887	61.205 #
22) L5 AR-1248-2	5.473	4.575	1343786	1135779	23.653	23.216
23) L5 AR-1248-3	5.689	4.618	2009856	1130748	30.125	22.035 #
24) L5 AR-1248-4	6.130	4.803	994325	931046	14.232	15.881
25) L5 AR-1248-5	6.168	5.221	622469	1054470	9.004	18.403 #
26) L6 AR-1254-1	6.101	5.178	1305200	2103419	17.274	24.085 #
27) L6 AR-1254-2	6.353	5.339	3020438	1080047	26.928	14.159 #
28) L6 AR-1254-3	6.742	5.770	261971	2075750	2.264	16.937 #
29) L6 AR-1254-4	7.061	6.015	1458305	3162470	18.267	40.069 #
30) L6 AR-1254-5	7.512	6.468	1962696	3923529	22.885	33.927 #
31) L7 AR-1260-1	6.909	5.911	3191734	1966362	38.114	24.589 #
32) L7 AR-1260-2	7.201	6.119	592033	2204949	6.540	22.579 #
33) L7 AR-1260-3	7.602	6.294	1824011	3887376	25.163	42.582 #
34) L7 AR-1260-4	7.841	6.794	2937934	2543605	34.219	31.437
35) L7 AR-1260-5	8.196	7.059	1153222	1417891	7.440	7.670
36) L8 AR-1262-1	7.602	6.518	1824011	2254456	18.473	20.508
37) L8 AR-1262-2	8.196	6.794	1153222	2543605	7.143	24.936 #
38) L8 AR-1262-3	8.509f	7.344f	56239	65888053	0.514	773.112 #
39) L8 AR-1262-4	8.615	7.449	720909	4353430	15.033	28.030 #
40) L8 AR-1262-5	9.295	8.008f	21839	4167859	0.392	53.576 #
41) L9 AR-1268-1	8.509	7.344f	56239	65888053	0.289	260.056 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021122\
 Data File : PP043668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2022 08:47
 Operator : YP\AJ
 Sample : N1523-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-SF-021022-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 01:24:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.615	7.449	720909	4353430	4.119	19.266 #
44) L9	AR-1268-4	9.295	8.008f	21839	4167859	0.349	46.347 #
45) L9	AR-1268-5	9.733	8.290	303711	1257708	0.668	2.093 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

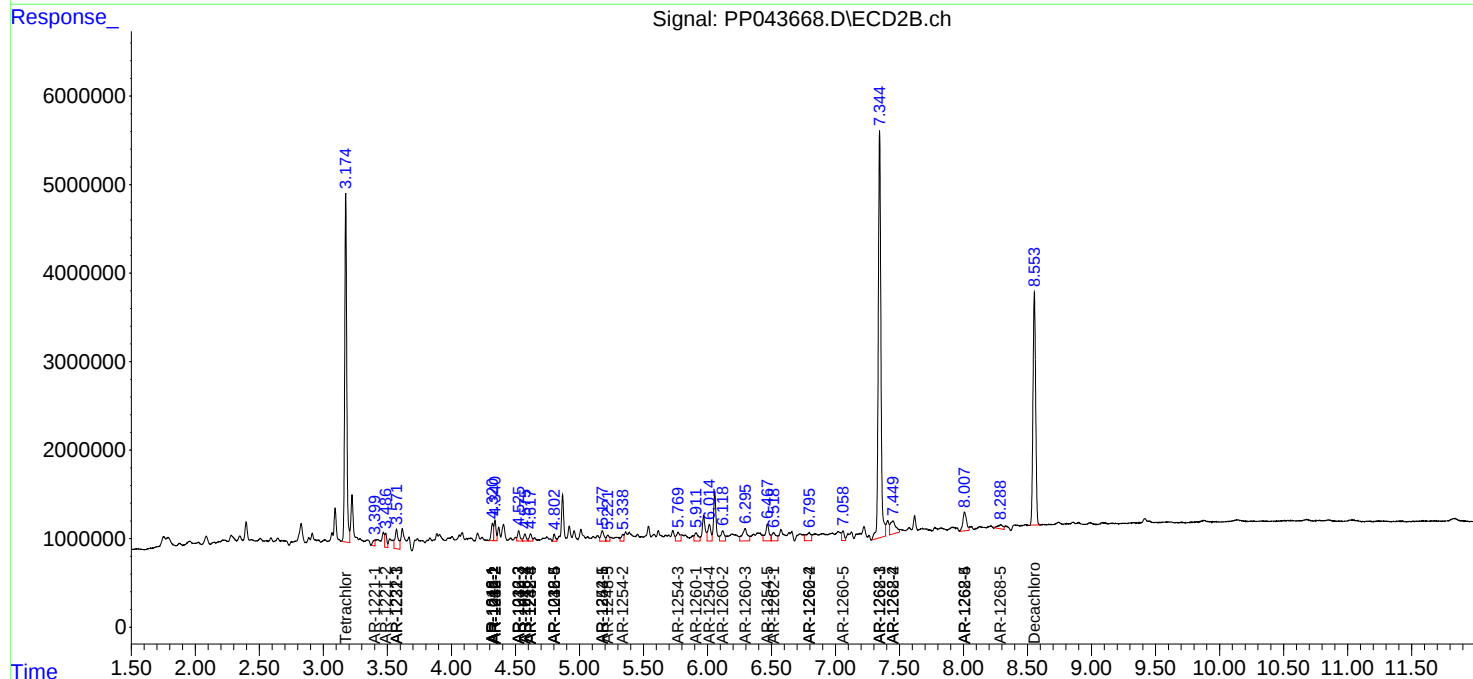


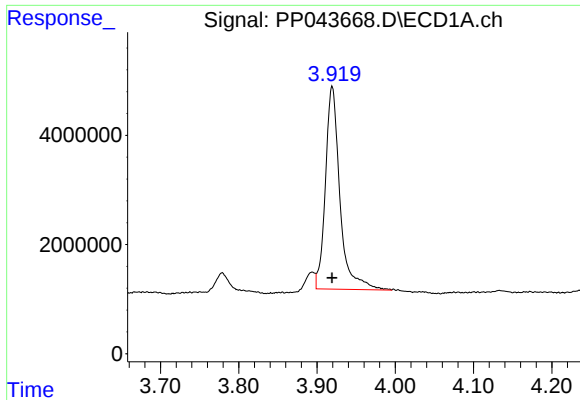

#1 Tetrachloro-m-xylene


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 47900974
Conc: 21.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

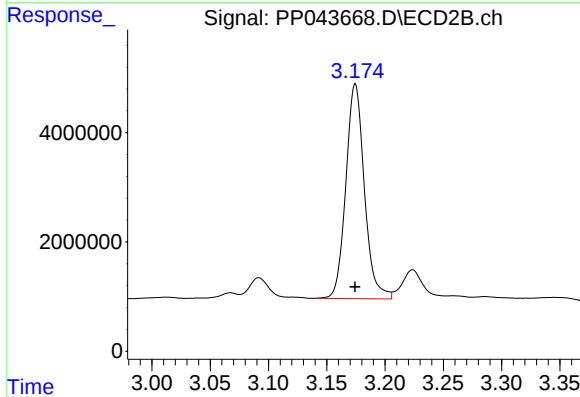


#1 Tetrachloro-m-xylene

R.T.: 3.175 min
Delta R.T.: 0.000 min
Response: 43557197
Conc: 23.19 ng/ml

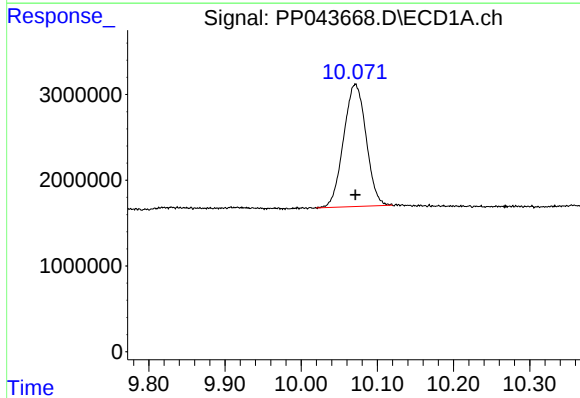


#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.000 min
Response: 29268511
Conc: 24.64 ng/ml

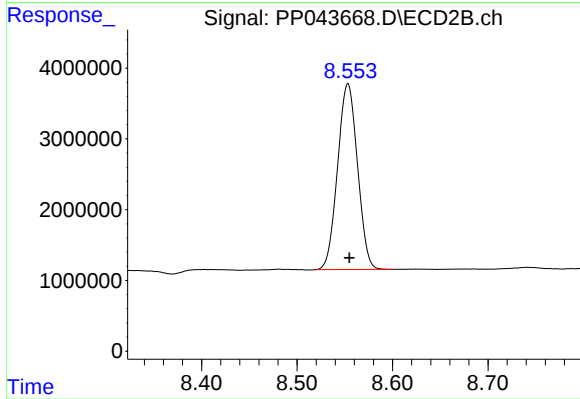

#2 Decachlorobiphenyl


R.T.: 8.553 min
Delta R.T.: -0.002 min
Response: 38052466
Conc: 23.45 ng/ml

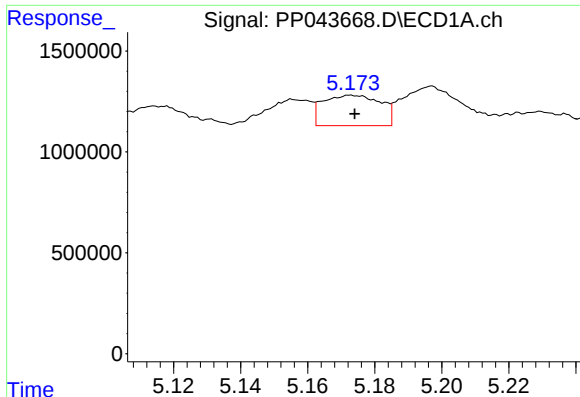

#3 AR-1016-1


R.T.: 5.173 min
Delta R.T.: -0.001 min
Response: 1799254
Conc: 24.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

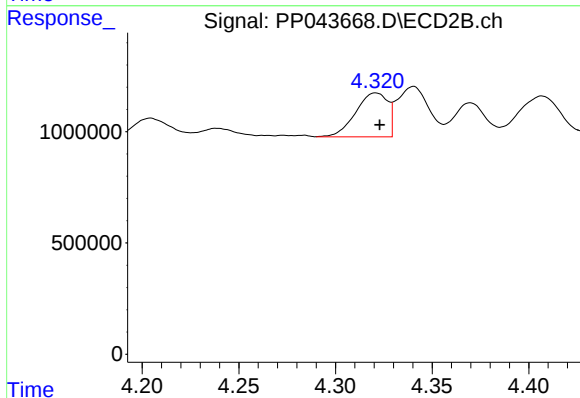


#3 AR-1016-1

R.T.: 4.321 min
Delta R.T.: -0.002 min
Response: 2279917
Conc: 37.21 ng/ml

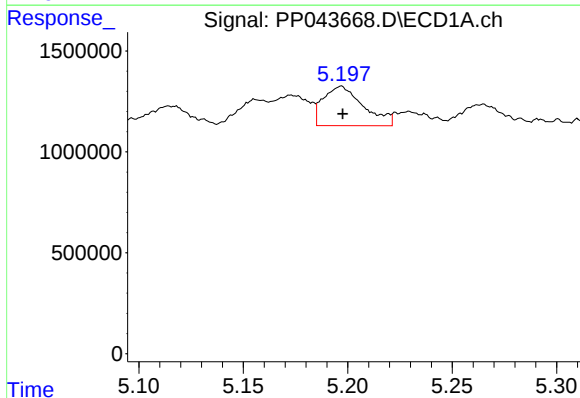


#4 AR-1016-2

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 2604466
Conc: 24.69 ng/ml

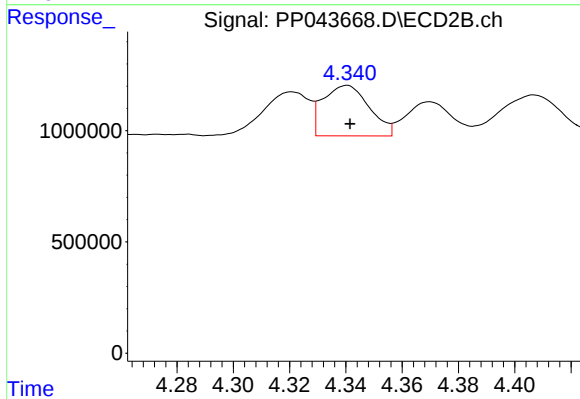

#4 AR-1016-2


R.T.: 4.340 min
Delta R.T.: -0.001 min
Response: 2590989
Conc: 30.67 ng/ml

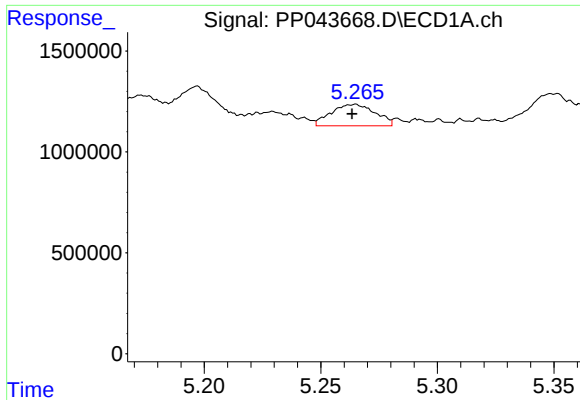

#5 AR-1016-3


R.T.: 5.265 min
Delta R.T.: 0.002 min
Response: 1395995
Conc: 21.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

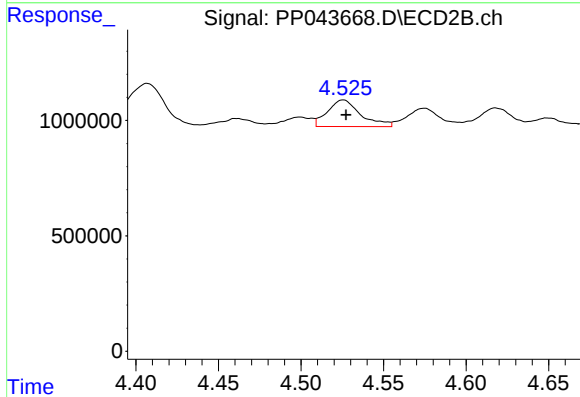


#5 AR-1016-3

R.T.: 4.526 min
Delta R.T.: -0.002 min
Response: 1604864
Conc: 34.35 ng/ml

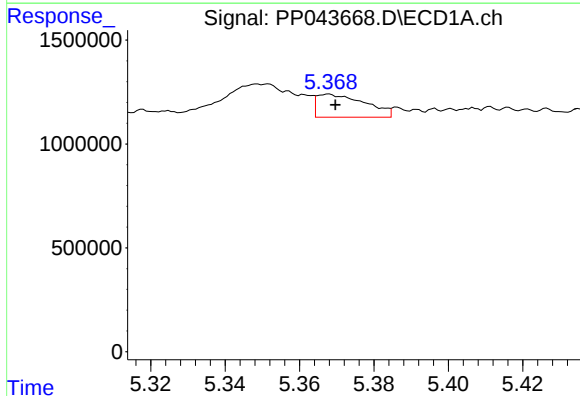


#6 AR-1016-4

R.T.: 5.368 min
Delta R.T.: -0.002 min
Response: 998876
Conc: 18.42 ng/ml

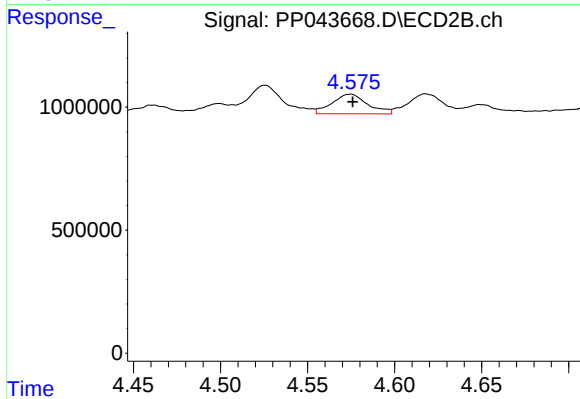

#6 AR-1016-4


R.T.: 4.575 min
Delta R.T.: -0.001 min
Response: 1135779
Conc: 30.39 ng/ml

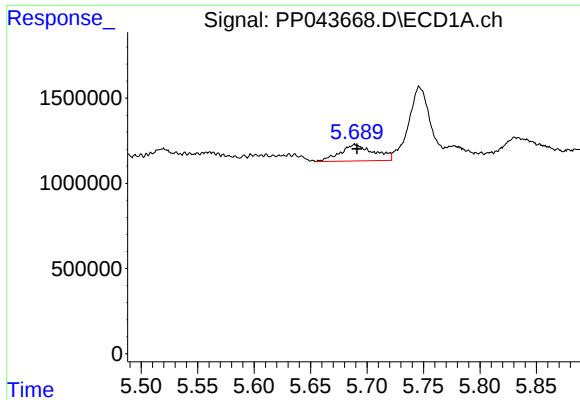

#7 AR-1016-5


R.T.: 5.689 min
Delta R.T.: -0.002 min
Response: 2009856
Conc: 38.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

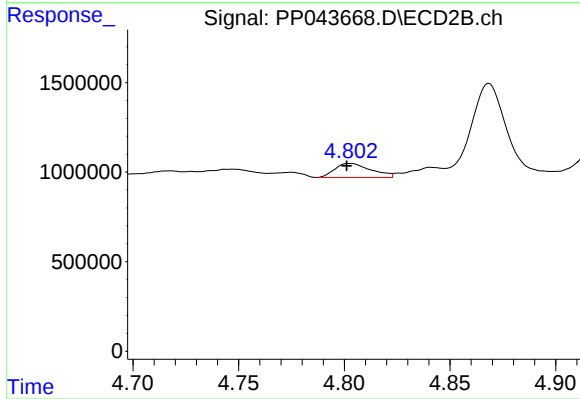


#7 AR-1016-5

R.T.: 4.803 min
Delta R.T.: 0.001 min
Response: 931046
Conc: 20.38 ng/ml

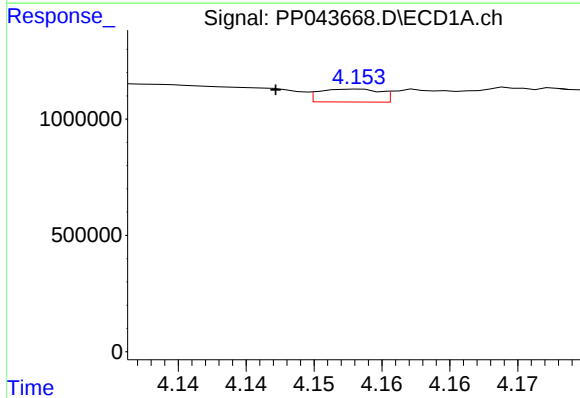


#8 AR-1221-1

R.T.: 4.153 min
Delta R.T.: 0.006 min
Response: 171561
Conc: 6.74 ng/ml

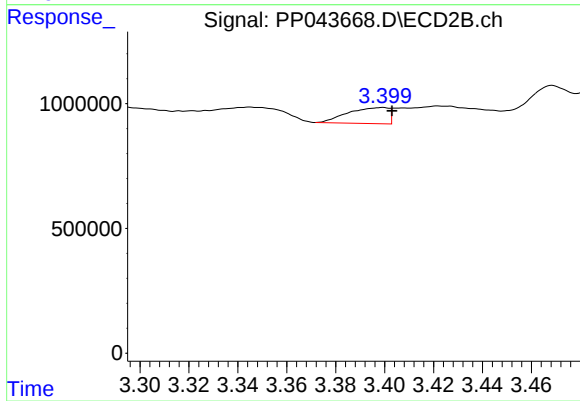

#8 AR-1221-1


R.T.: 3.399 min
Delta R.T.: -0.004 min
Response: 747168
Conc: 31.32 ng/ml

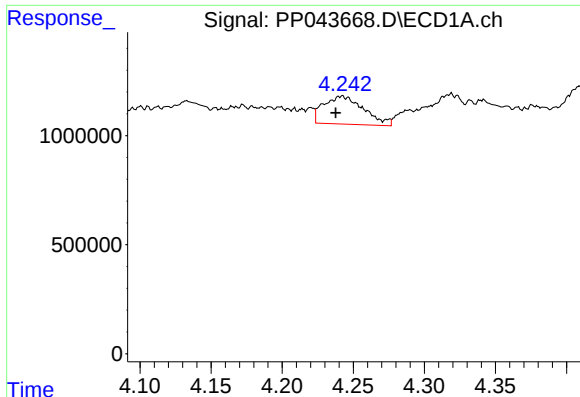

#9 AR-1221-2


R.T.: 4.243 min
Delta R.T.: 0.005 min
Response: 2520899
Conc: 131.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

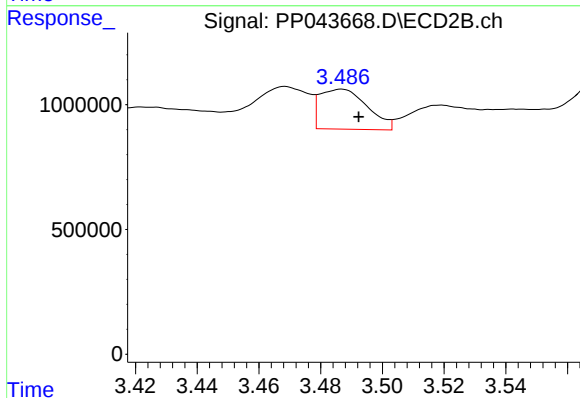


#9 AR-1221-2

R.T.: 3.487 min
Delta R.T.: -0.005 min
Response: 1710374
Conc: 94.70 ng/ml

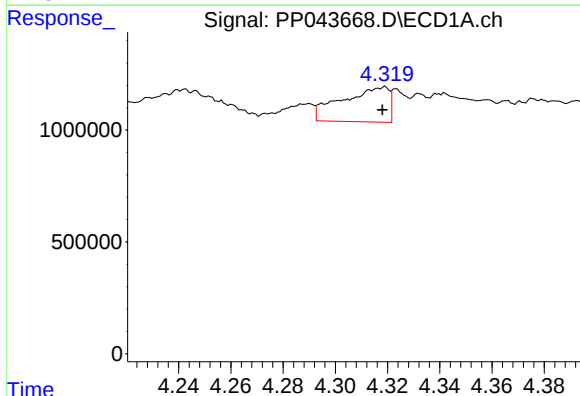


#10 AR-1221-3

R.T.: 4.319 min
Delta R.T.: 0.001 min
Response: 1953235
Conc: 34.00 ng/ml

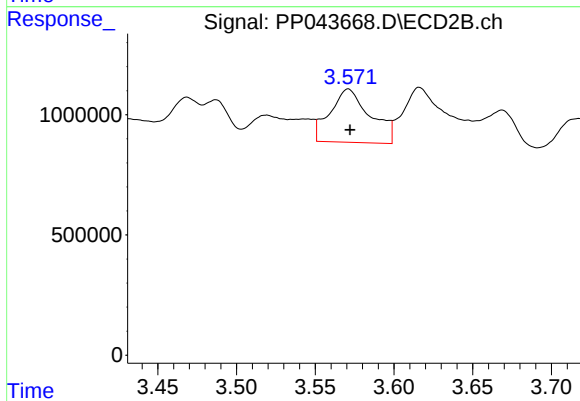

#10 AR-1221-3


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 3941002
Conc: 76.39 ng/ml

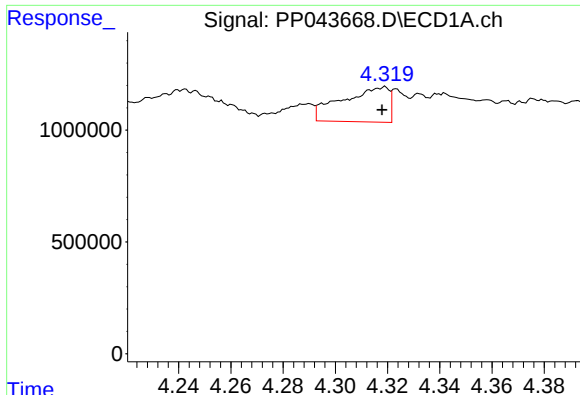

#11 AR-1232-1


R.T.: 4.319 min
Delta R.T.: 0.001 min
Response: 1953235
Conc: 40.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

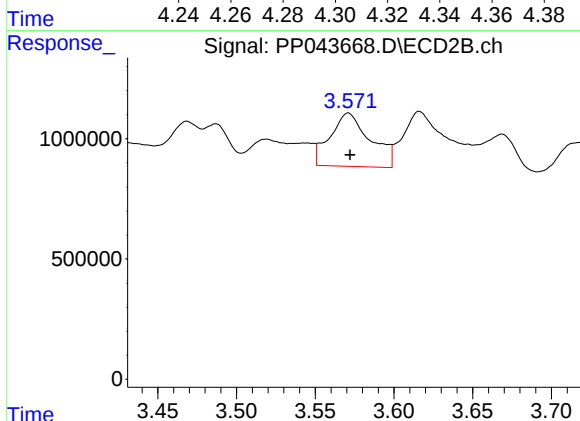


#11 AR-1232-1

R.T.: 3.571 min
Delta R.T.: -0.001 min
Response: 3941002
Conc: 91.60 ng/ml

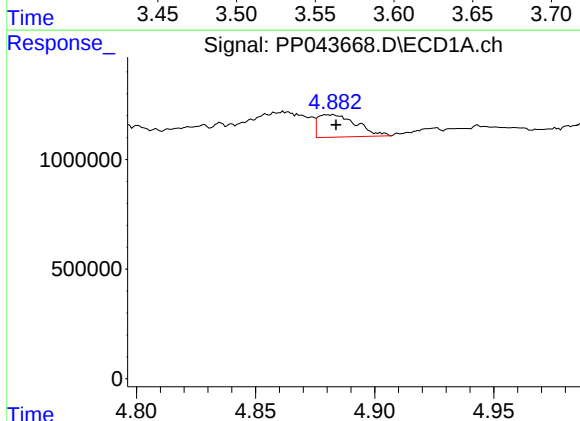


#12 AR-1232-2

R.T.: 4.883 min
Delta R.T.: -0.001 min
Response: 1151448
Conc: 48.59 ng/ml

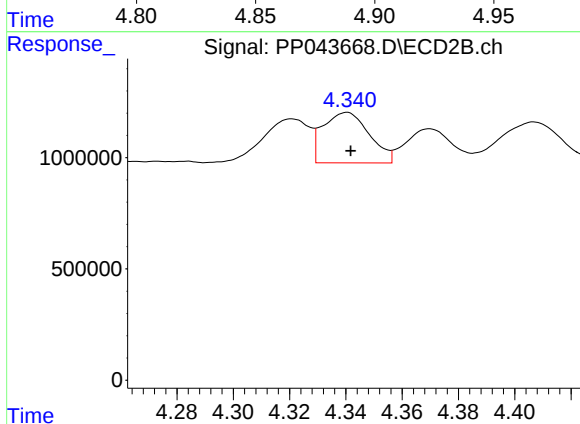

#12 AR-1232-2


R.T.: 4.340 min
Delta R.T.: -0.001 min
Response: 2590989
Conc: 72.58 ng/ml

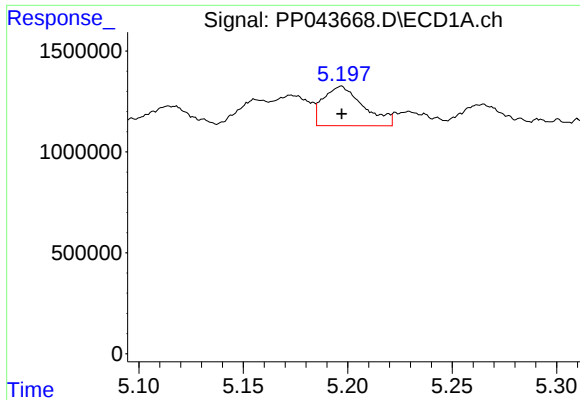

#13 AR-1232-3


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 2604466
Conc: 60.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

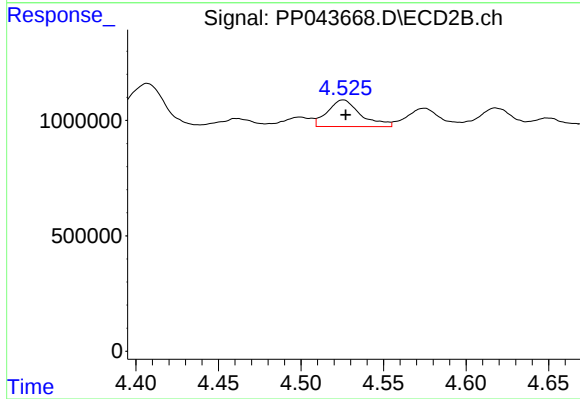


#13 AR-1232-3

R.T.: 4.526 min
Delta R.T.: -0.002 min
Response: 1604864
Conc: 82.07 ng/ml

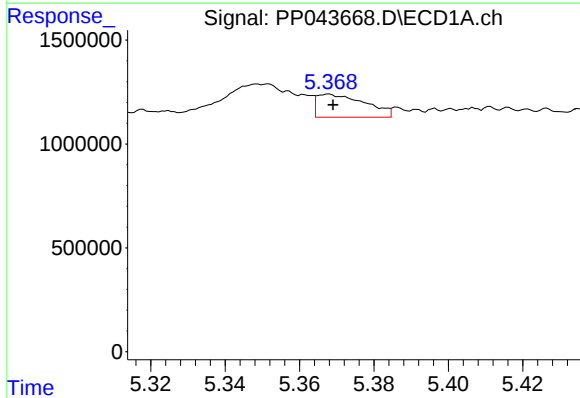


#14 AR-1232-4

R.T.: 5.368 min
Delta R.T.: -0.001 min
Response: 998876
Conc: 45.76 ng/ml

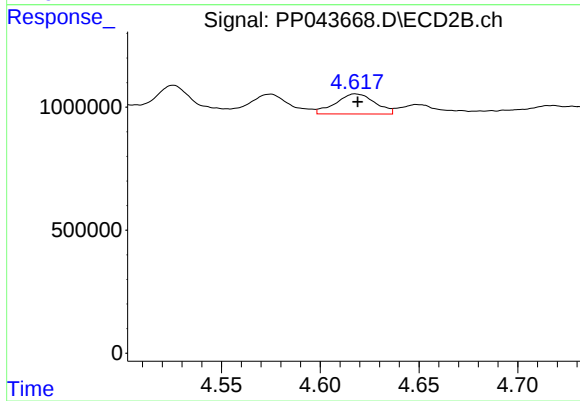

#14 AR-1232-4


R.T.: 4.618 min
Delta R.T.: -0.001 min
Response: 1130748
Conc: 65.39 ng/ml

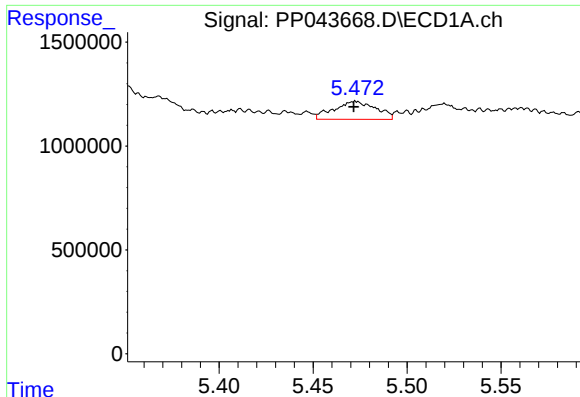

#15 AR-1232-5


R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 1343786
Conc: 83.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

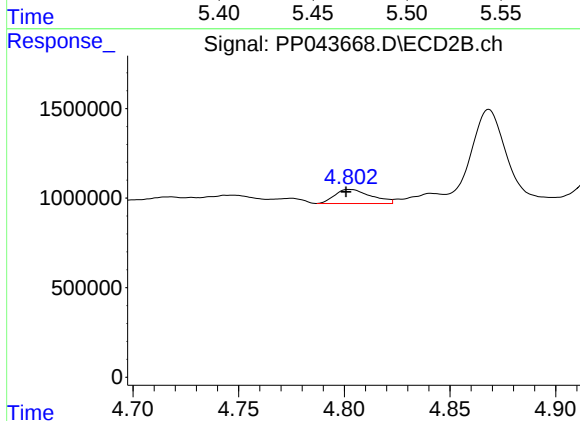


#15 AR-1232-5

R.T.: 4.803 min
Delta R.T.: 0.002 min
Response: 931046
Conc: 49.57 ng/ml

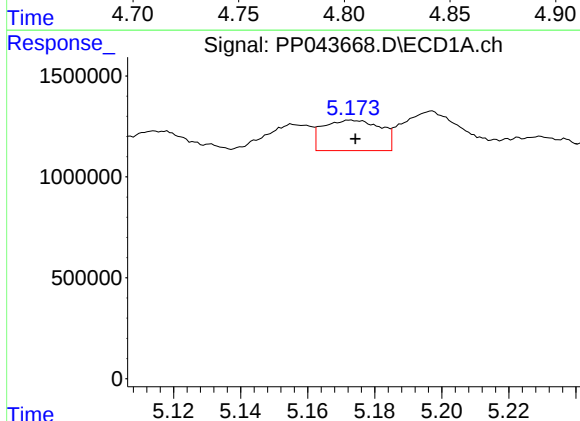


#16 AR-1242-1

R.T.: 5.173 min
Delta R.T.: -0.001 min
Response: 1799254
Conc: 32.02 ng/ml

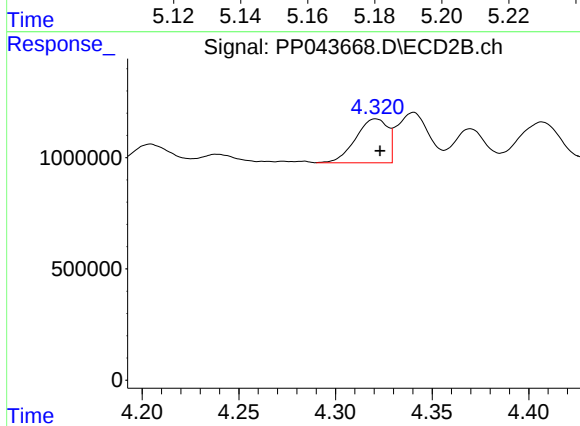

#16 AR-1242-1


R.T.: 4.321 min
Delta R.T.: -0.002 min
Response: 2279917
Conc: 46.77 ng/ml

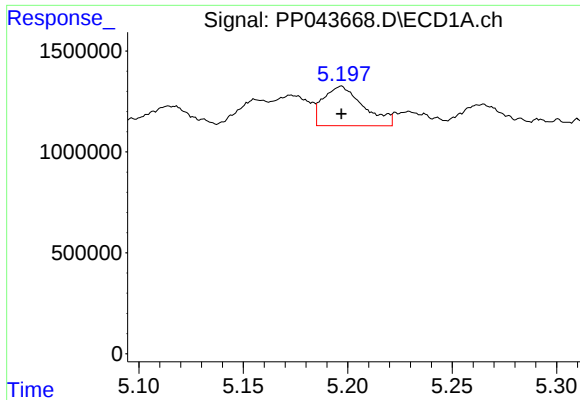

#17 AR-1242-2


R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 2604466
Conc: 31.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

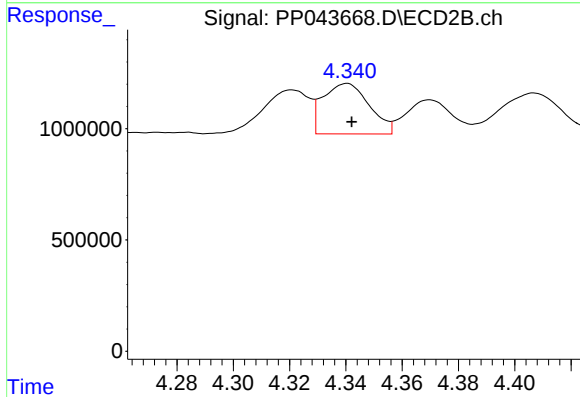


#17 AR-1242-2

R.T.: 4.340 min
Delta R.T.: -0.002 min
Response: 2590989
Conc: 38.48 ng/ml

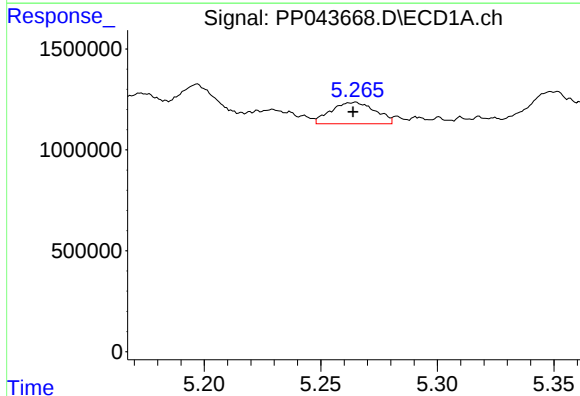


#18 AR-1242-3

R.T.: 5.265 min
Delta R.T.: 0.001 min
Response: 1395995
Conc: 26.97 ng/ml

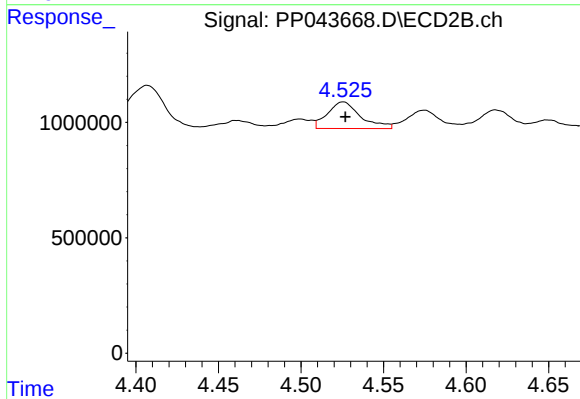

#18 AR-1242-3


R.T.: 4.526 min
Delta R.T.: -0.001 min
Response: 1604864
Conc: 42.75 ng/ml

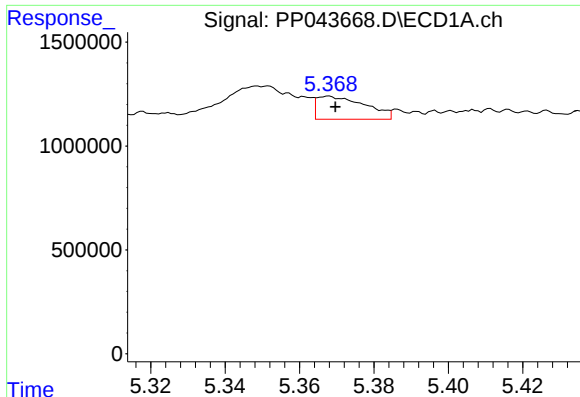

#19 AR-1242-4


R.T.: 5.368 min
Delta R.T.: -0.002 min
Response: 998876
Conc: 23.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

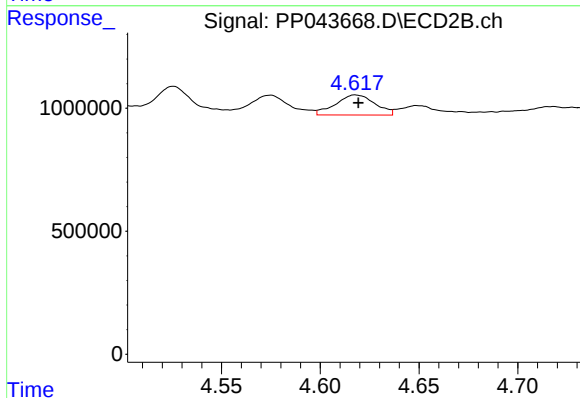


#19 AR-1242-4

R.T.: 4.618 min
Delta R.T.: -0.001 min
Response: 1130748
Conc: 31.31 ng/ml

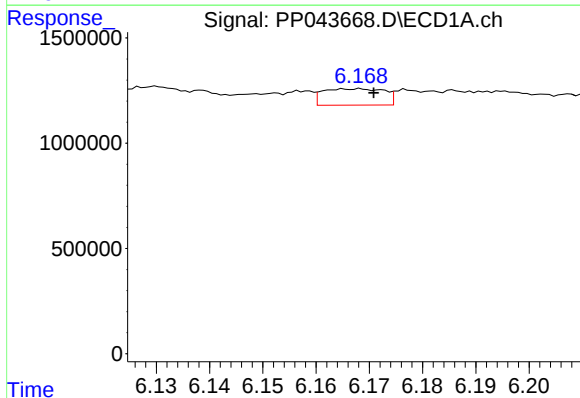


#20 AR-1242-5

R.T.: 6.168 min
Delta R.T.: -0.002 min
Response: 622469
Conc: 14.42 ng/ml

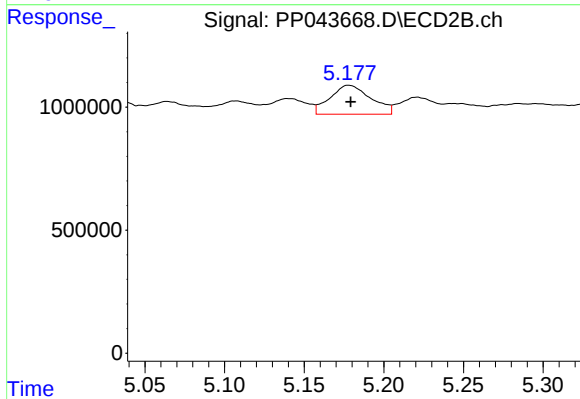

#20 AR-1242-5


R.T.: 5.178 min
Delta R.T.: -0.001 min
Response: 2103419
Conc: 48.86 ng/ml

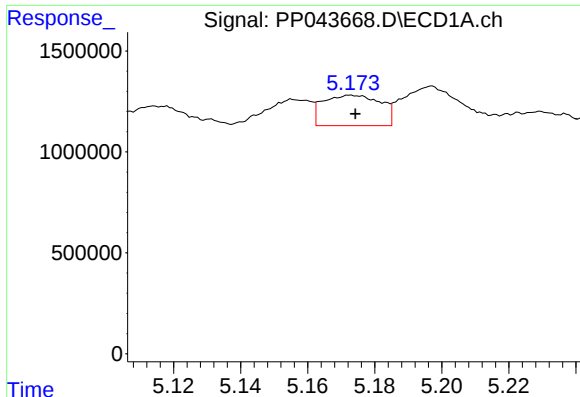

#21 AR-1248-1


R.T.: 5.173 min
Delta R.T.: -0.002 min
Response: 1799254
Conc: 43.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

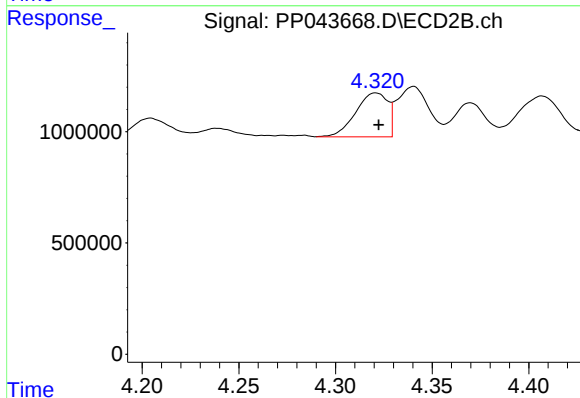


#21 AR-1248-1

R.T.: 4.321 min
Delta R.T.: -0.002 min
Response: 2279917
Conc: 61.21 ng/ml

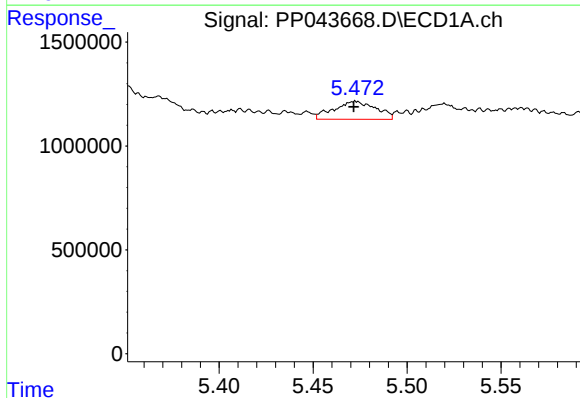


#22 AR-1248-2

R.T.: 5.473 min
Delta R.T.: 0.001 min
Response: 1343786
Conc: 23.65 ng/ml

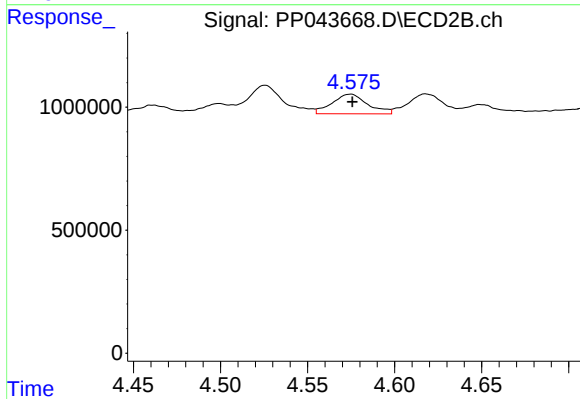

#22 AR-1248-2


R.T.: 4.575 min
Delta R.T.: -0.001 min
Response: 1135779
Conc: 23.22 ng/ml

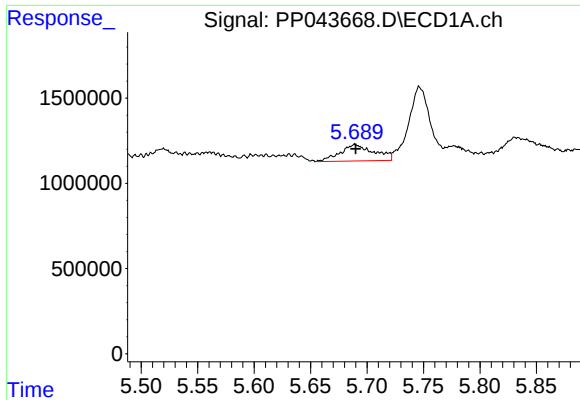

#23 AR-1248-3


R.T.: 5.689 min
Delta R.T.: 0.000 min
Response: 2009856
Conc: 30.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

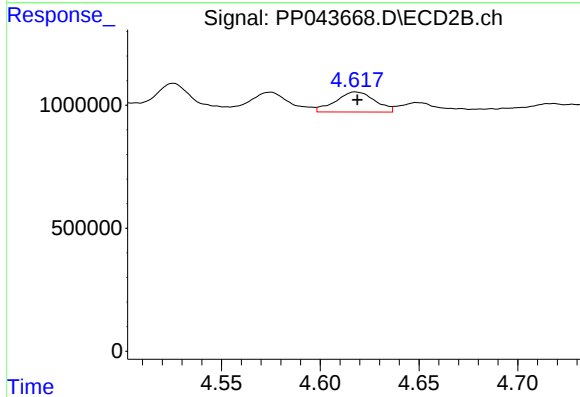


#23 AR-1248-3

R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 1130748
Conc: 22.04 ng/ml

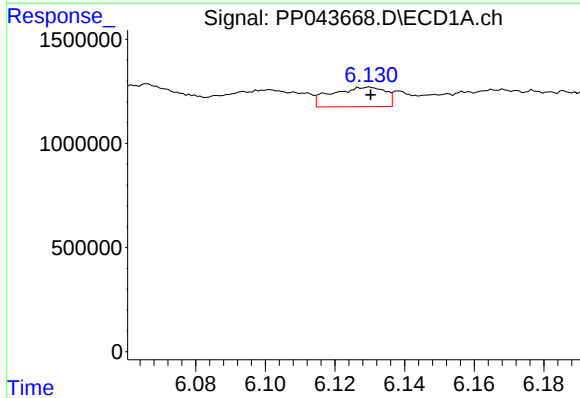


#24 AR-1248-4

R.T.: 6.130 min
Delta R.T.: 0.000 min
Response: 994325
Conc: 14.23 ng/ml

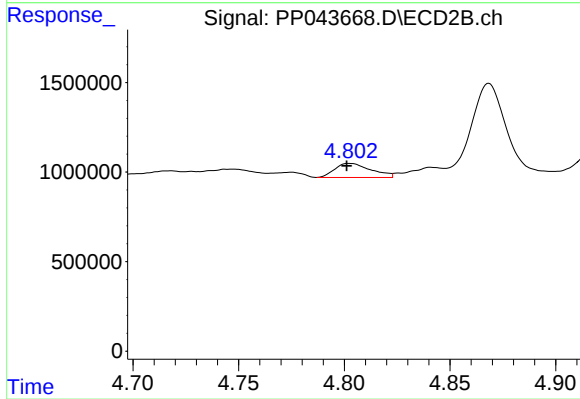

#24 AR-1248-4


R.T.: 4.803 min
Delta R.T.: 0.002 min
Response: 931046
Conc: 15.88 ng/ml

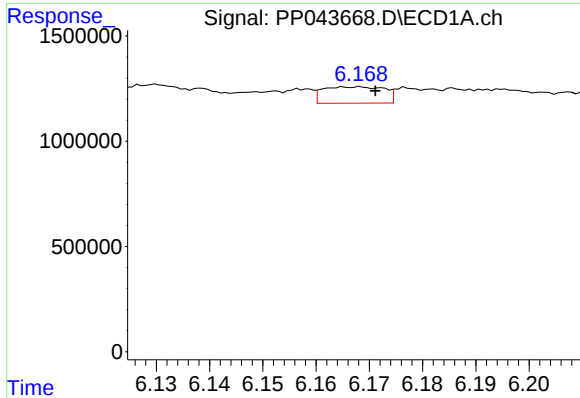

#25 AR-1248-5


R.T.: 6.168 min
Delta R.T.: -0.003 min
Response: 622469
Conc: 9.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

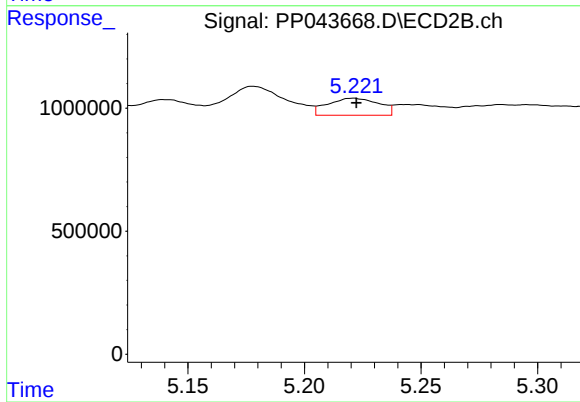


#25 AR-1248-5

R.T.: 5.221 min
Delta R.T.: -0.001 min
Response: 1054470
Conc: 18.40 ng/ml

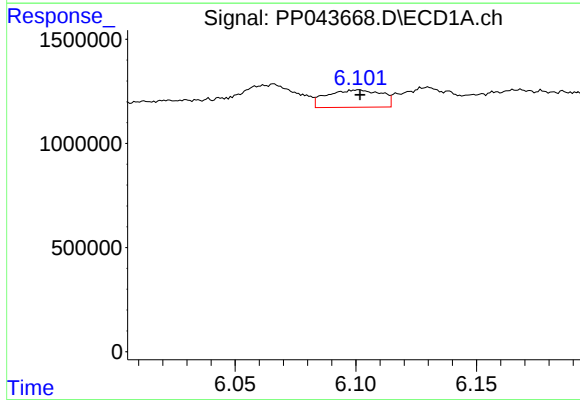


#26 AR-1254-1

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 1305200
Conc: 17.27 ng/ml

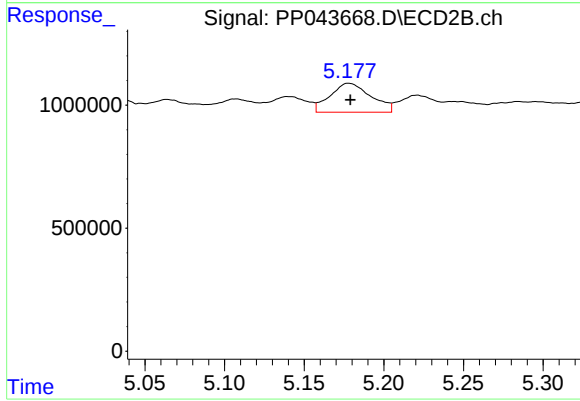

#26 AR-1254-1


R.T.: 5.178 min
Delta R.T.: -0.001 min
Response: 2103419
Conc: 24.09 ng/ml

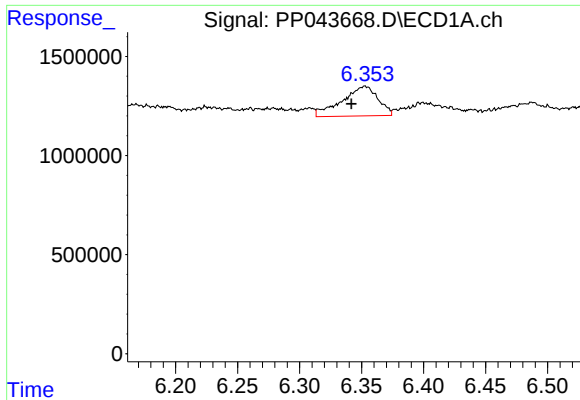

#27 AR-1254-2


R.T.: 6.353 min
Delta R.T.: 0.011 min
Response: 3020438
Conc: 26.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

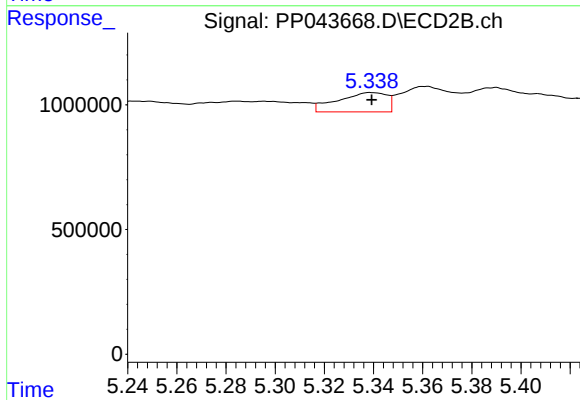


#27 AR-1254-2

R.T.: 5.339 min
Delta R.T.: 0.000 min
Response: 1080047
Conc: 14.16 ng/ml

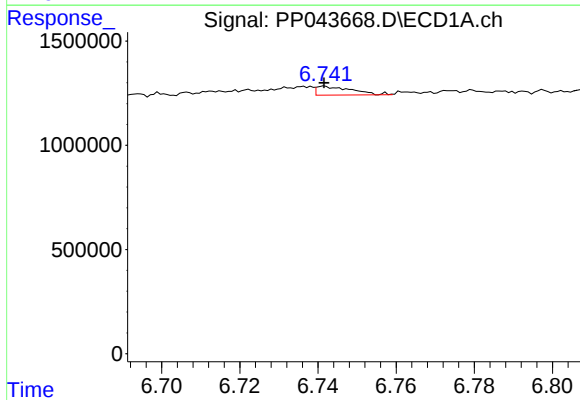


#28 AR-1254-3

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 261971
Conc: 2.26 ng/ml

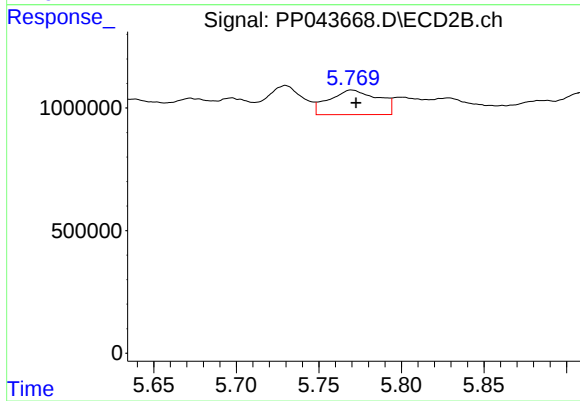

#28 AR-1254-3


R.T.: 5.770 min
Delta R.T.: -0.002 min
Response: 2075750
Conc: 16.94 ng/ml

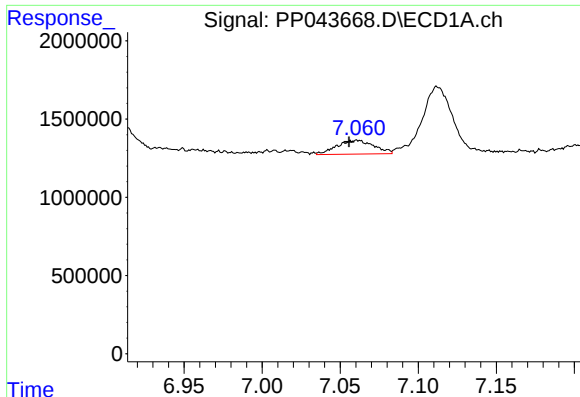

#29 AR-1254-4


R.T.: 7.061 min
Delta R.T.: 0.005 min
Response: 1458305
Conc: 18.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

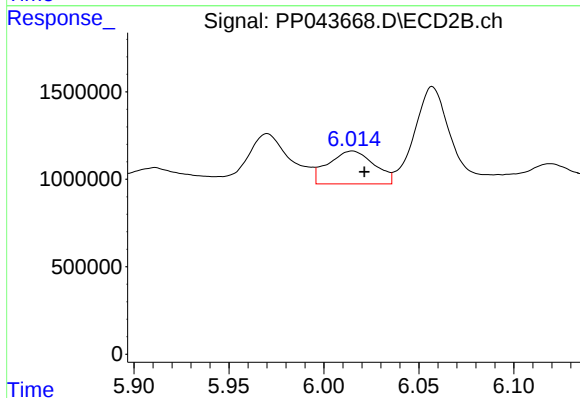


#29 AR-1254-4

R.T.: 6.015 min
Delta R.T.: -0.006 min
Response: 3162470
Conc: 40.07 ng/ml

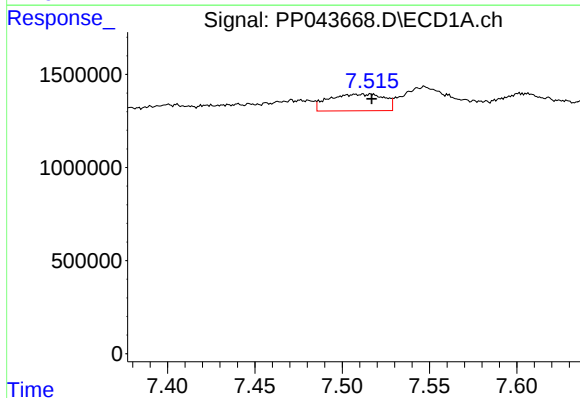


#30 AR-1254-5

R.T.: 7.512 min
Delta R.T.: -0.005 min
Response: 1962696
Conc: 22.89 ng/ml

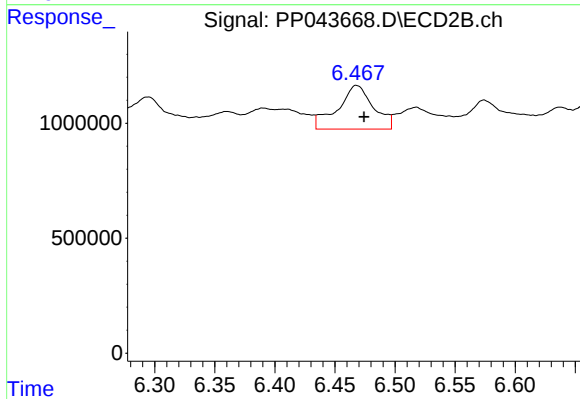

#30 AR-1254-5


R.T.: 6.468 min
Delta R.T.: -0.006 min
Response: 3923529
Conc: 33.93 ng/ml

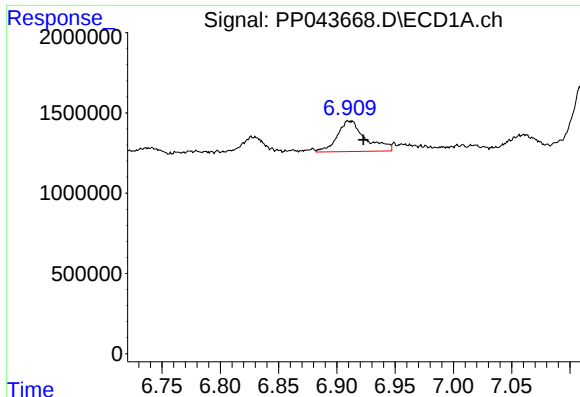

#31 AR-1260-1


R.T.: 6.909 min
Delta R.T.: -0.013 min
Response: 3191734
Conc: 38.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

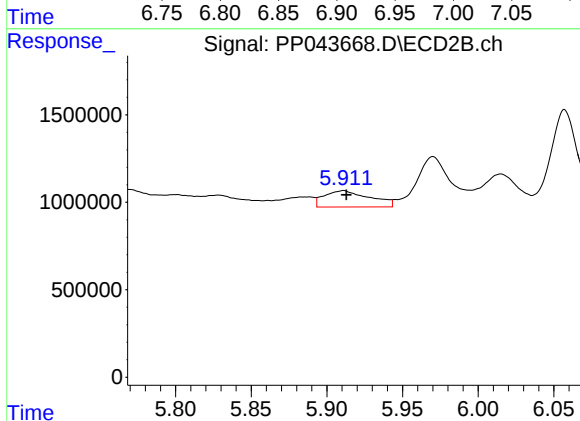


#31 AR-1260-1

R.T.: 5.911 min
Delta R.T.: -0.002 min
Response: 1966362
Conc: 24.59 ng/ml

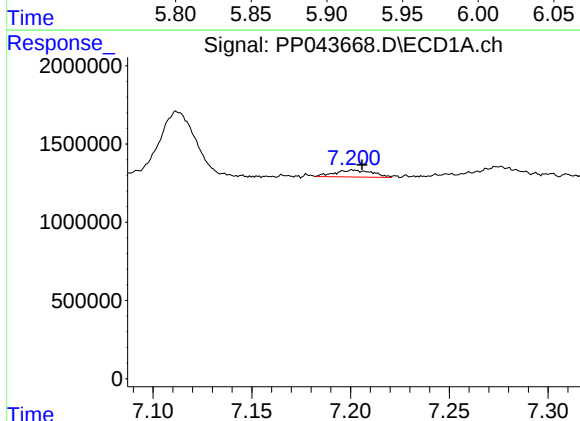


#32 AR-1260-2

R.T.: 7.201 min
Delta R.T.: -0.005 min
Response: 592033
Conc: 6.54 ng/ml

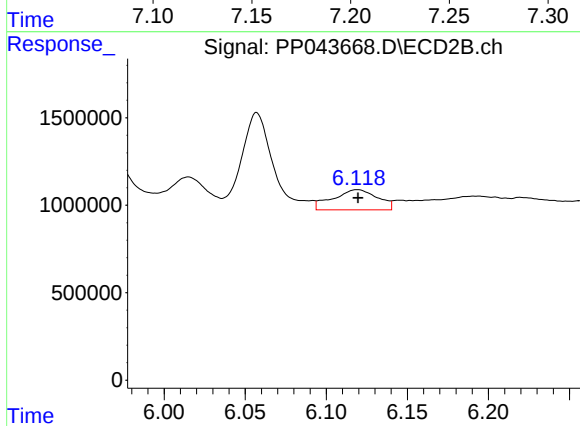

#32 AR-1260-2


R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 2204949
Conc: 22.58 ng/ml

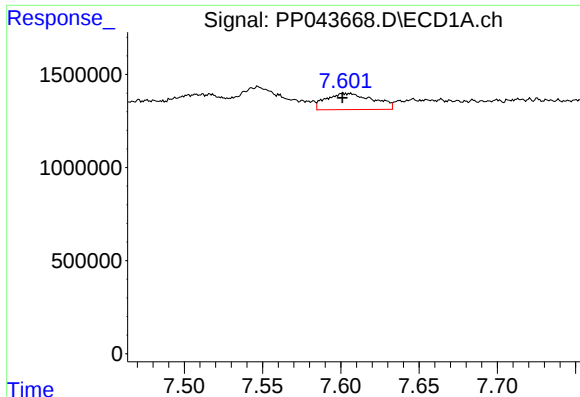

#33 AR-1260-3


R.T.: 7.602 min
Delta R.T.: 0.000 min
Response: 1824011
Conc: 25.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

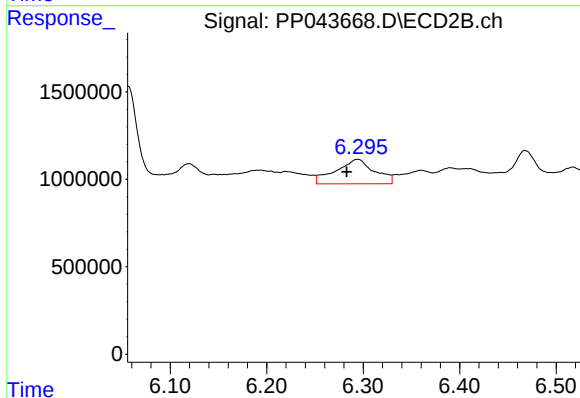


#33 AR-1260-3

R.T.: 6.294 min
Delta R.T.: 0.011 min
Response: 3887376
Conc: 42.58 ng/ml

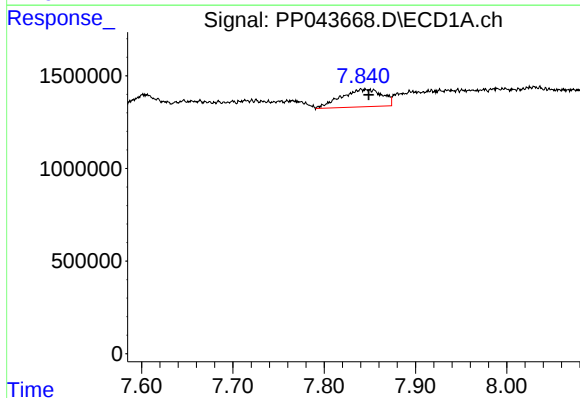


#34 AR-1260-4

R.T.: 7.841 min
Delta R.T.: -0.008 min
Response: 2937934
Conc: 34.22 ng/ml

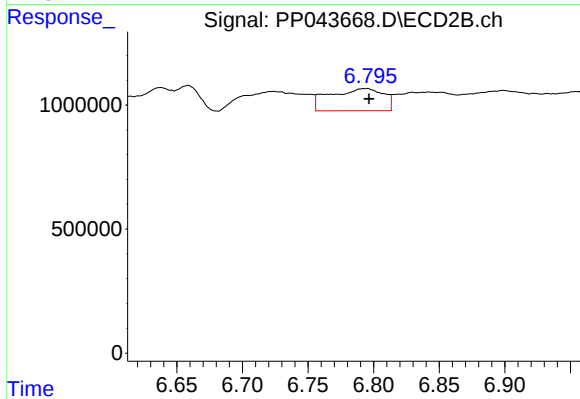

#34 AR-1260-4


R.T.: 6.794 min
Delta R.T.: -0.002 min
Response: 2543605
Conc: 31.44 ng/ml

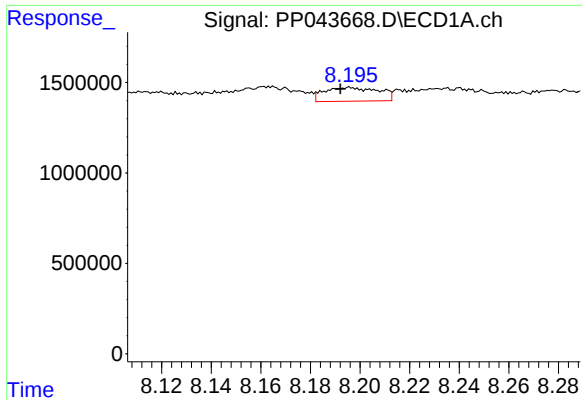

#35 AR-1260-5


R.T.: 8.196 min
Delta R.T.: 0.004 min
Response: 1153222
Conc: 7.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

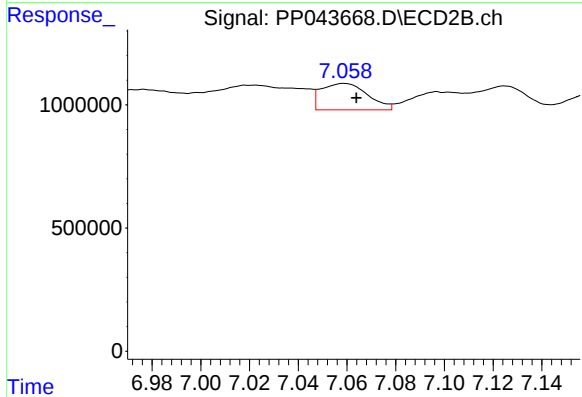


#35 AR-1260-5

R.T.: 7.059 min
Delta R.T.: -0.005 min
Response: 1417891
Conc: 7.67 ng/ml

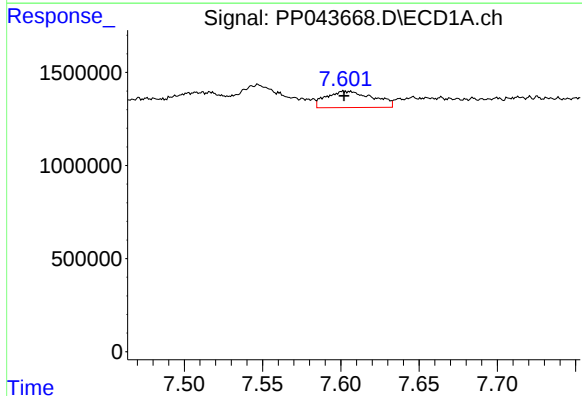


#36 AR-1262-1

R.T.: 7.602 min
Delta R.T.: 0.000 min
Response: 1824011
Conc: 18.47 ng/ml

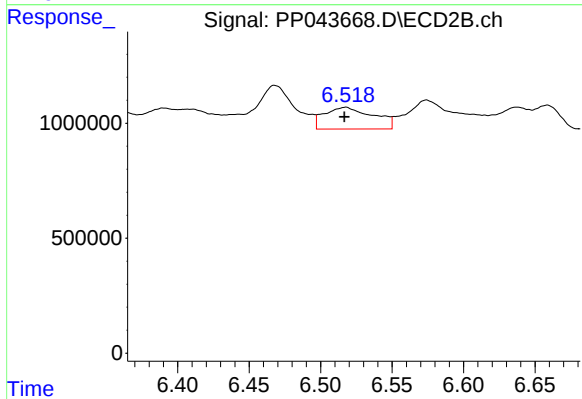

#36 AR-1262-1


R.T.: 6.518 min
Delta R.T.: 0.001 min
Response: 2254456
Conc: 20.51 ng/ml

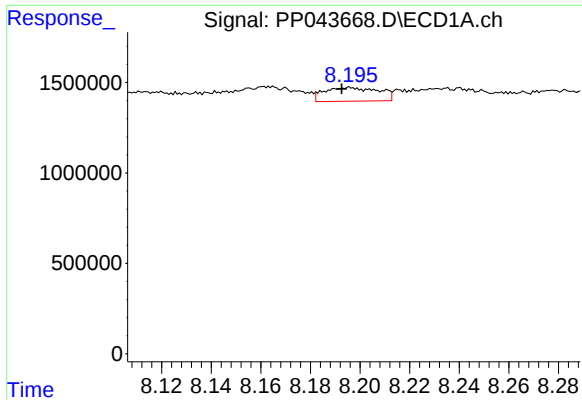

#37 AR-1262-2


R.T.: 8.196 min
Delta R.T.: 0.003 min
Response: 1153222
Conc: 7.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

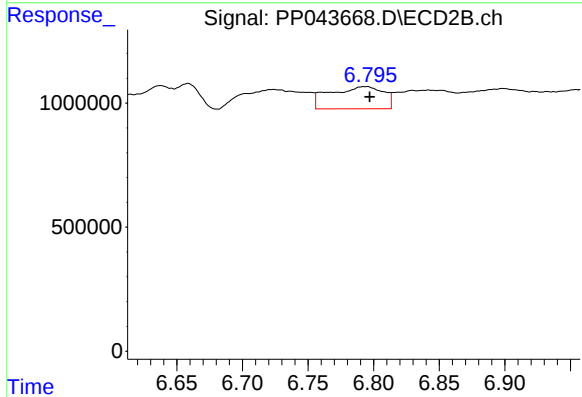


#37 AR-1262-2

R.T.: 6.794 min
Delta R.T.: -0.003 min
Response: 2543605
Conc: 24.94 ng/ml

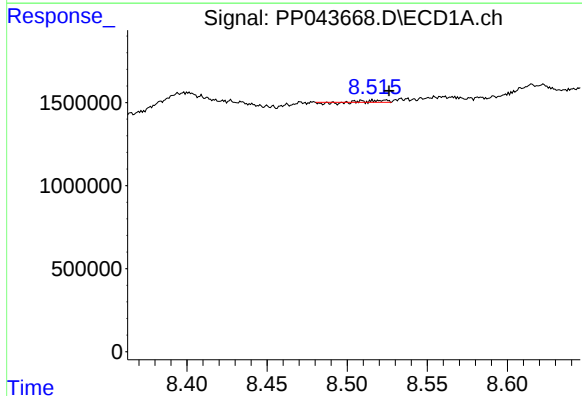


#38 AR-1262-3

R.T.: 8.509 min
Delta R.T.: -0.017 min
Response: 56239
Conc: 0.51 ng/ml

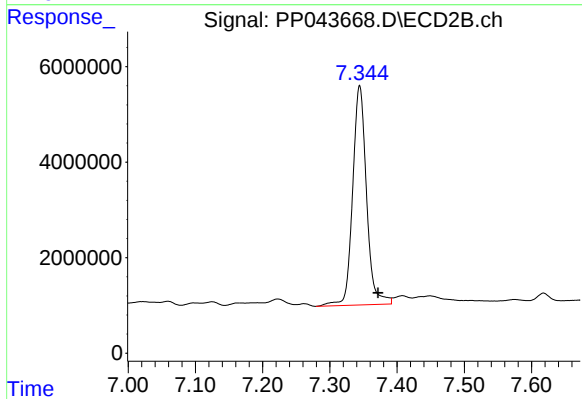

#38 AR-1262-3


R.T.: 7.344 min
Delta R.T.: -0.027 min
Response: 65888053
Conc: 773.11 ng/ml

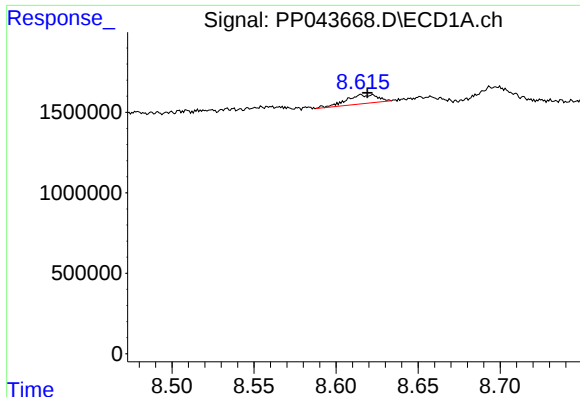

#39 AR-1262-4


R.T.: 8.615 min
Delta R.T.: -0.004 min
Response: 720909
Conc: 15.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

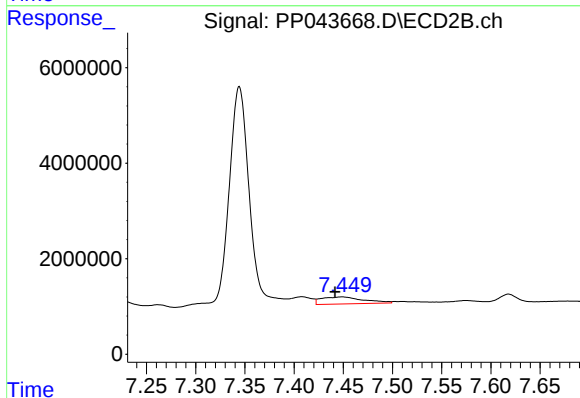


#39 AR-1262-4

R.T.: 7.449 min
Delta R.T.: 0.007 min
Response: 4353430
Conc: 28.03 ng/ml

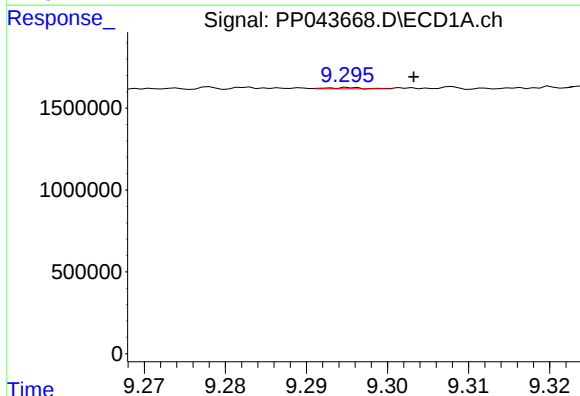


#40 AR-1262-5

R.T.: 9.295 min
Delta R.T.: -0.008 min
Response: 21839
Conc: 0.39 ng/ml

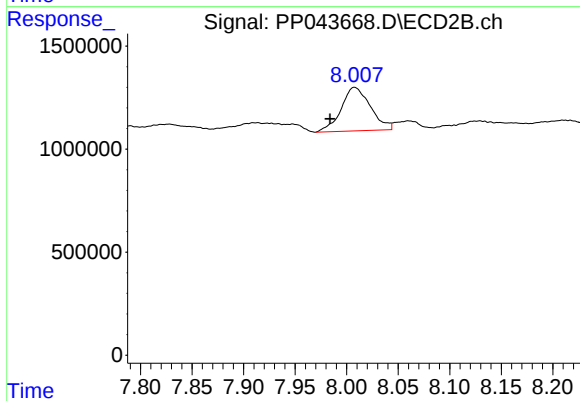

#40 AR-1262-5


R.T.: 8.008 min
Delta R.T.: 0.024 min
Response: 4167859
Conc: 53.58 ng/ml

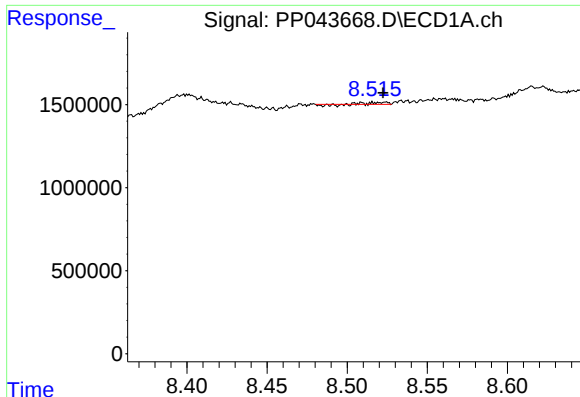

#41 AR-1268-1


R.T.: 8.509 min
Delta R.T.: -0.014 min
Response: 56239
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

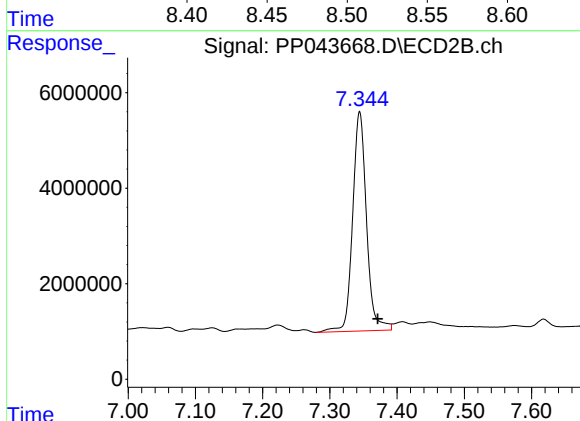


#41 AR-1268-1

R.T.: 7.344 min
Delta R.T.: -0.027 min
Response: 65888053
Conc: 260.06 ng/ml

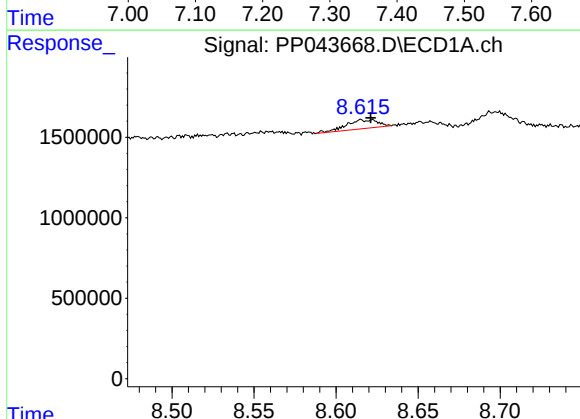


#42 AR-1268-2

R.T.: 8.615 min
Delta R.T.: -0.006 min
Response: 720909
Conc: 4.12 ng/ml

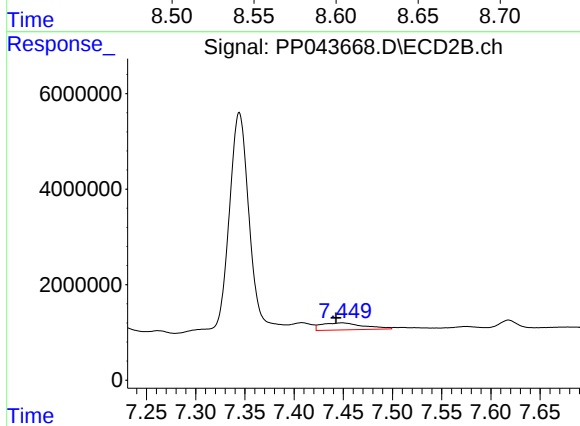

#42 AR-1268-2


R.T.: 7.449 min
Delta R.T.: 0.006 min
Response: 4353430
Conc: 19.27 ng/ml

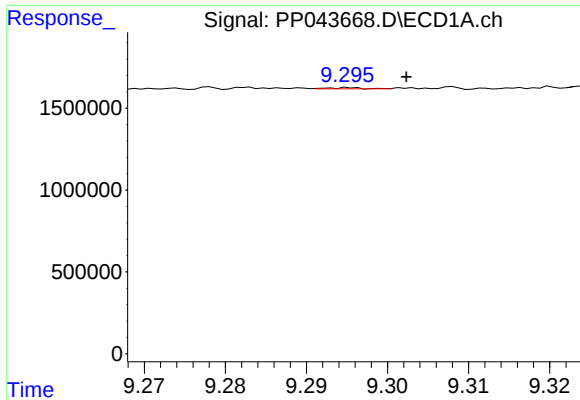

#44 AR-1268-4


R.T.: 9.295 min
Delta R.T.: -0.007 min
Response: 21839
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-SF-021022-03

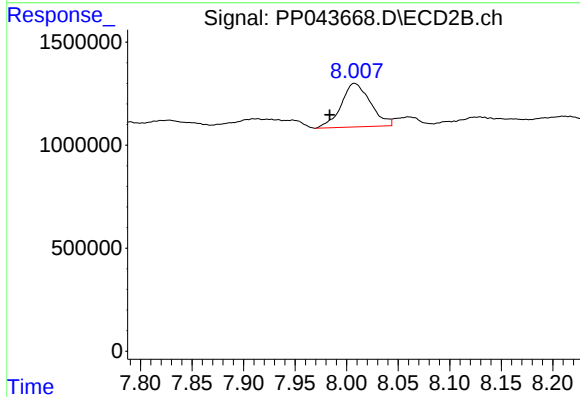


#44 AR-1268-4

R.T.: 8.008 min
Delta R.T.: 0.024 min
Response: 4167859
Conc: 46.35 ng/ml

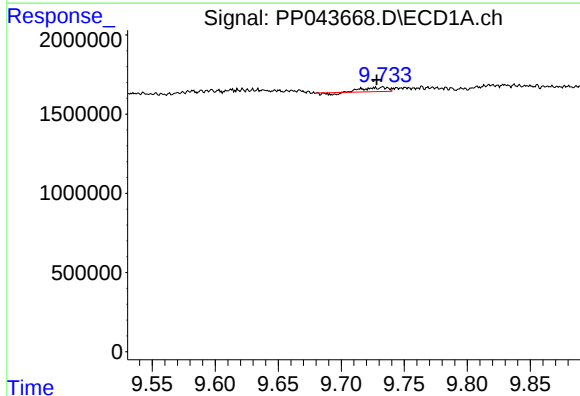

#45 AR-1268-5

R.T.: 9.733 min
Delta R.T.: 0.005 min
Response: 303711
Conc: 0.67 ng/ml

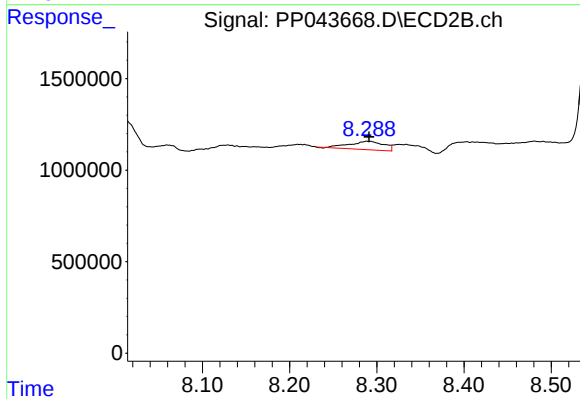

#45 AR-1268-5

R.T.: 8.290 min
Delta R.T.: -0.001 min
Response: 1257708
Conc: 2.09 ng/ml