

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
 Data File : PP033313.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Feb 2021 15:48
 Operator : DD\AJ
 Sample : M1396-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 16:54:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.727	4.000	1564393	1070643	25.511	26.182
2) SA Decachlor...	10.545	9.261	1158986	933503	26.606	27.866
Target Compounds						
8) L2 AR-1221-1	4.968	0.000	102817	0	166.665	N.D. #
9) L2 AR-1221-2	5.073	4.331f	21948	60199	47.178	190.498 #
28) L6 AR-1254-3	7.540	0.000	11111	0	3.658	N.D. #
29) L6 AR-1254-4	7.828	0.000	29491	0	12.749	N.D. #
32) L7 AR-1260-2	7.964	0.000	40492	0	13.855	N.D. #
34) L7 AR-1260-4	8.547	0.000	19562	0	8.007	N.D. #
45) L9 AR-1268-5	10.236	0.000	22157	0	1.353	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
Data File : PP033313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2021 15:48
Operator : DD\AJ
Sample : M1396-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 16:54:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

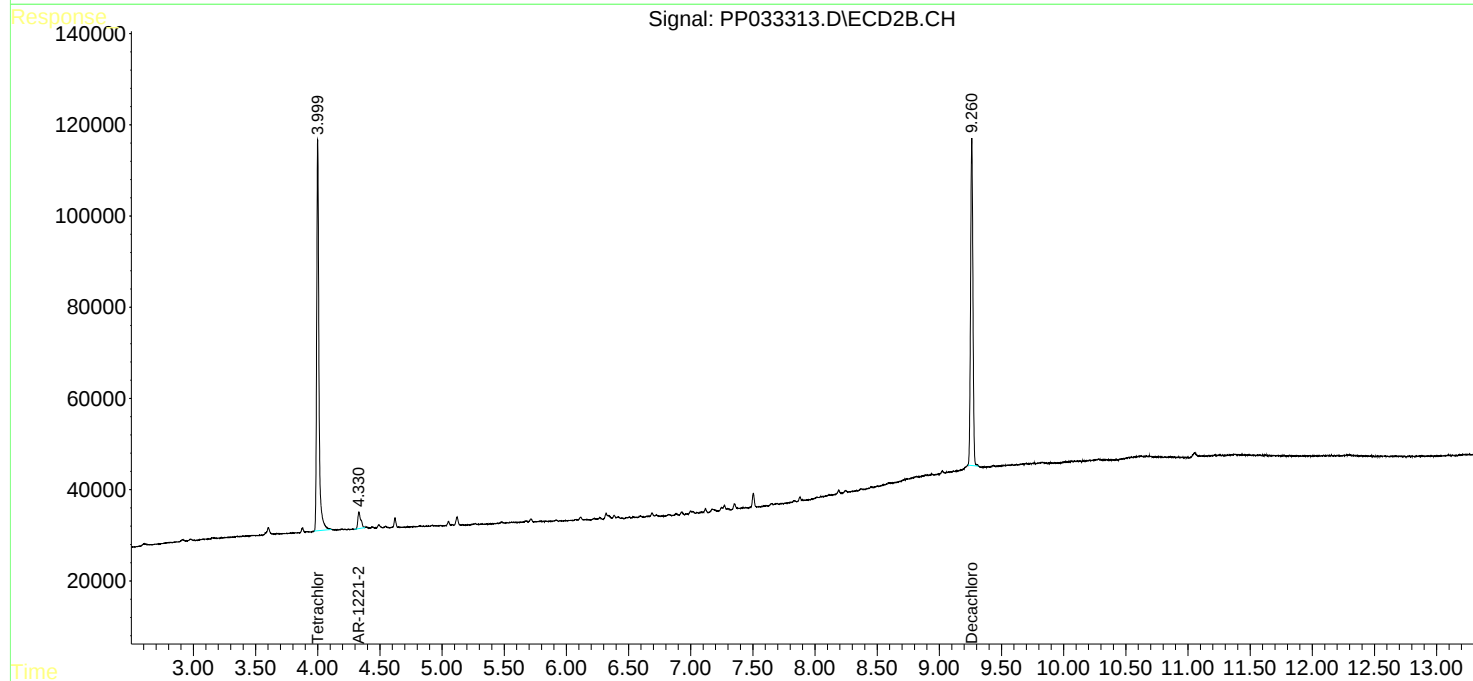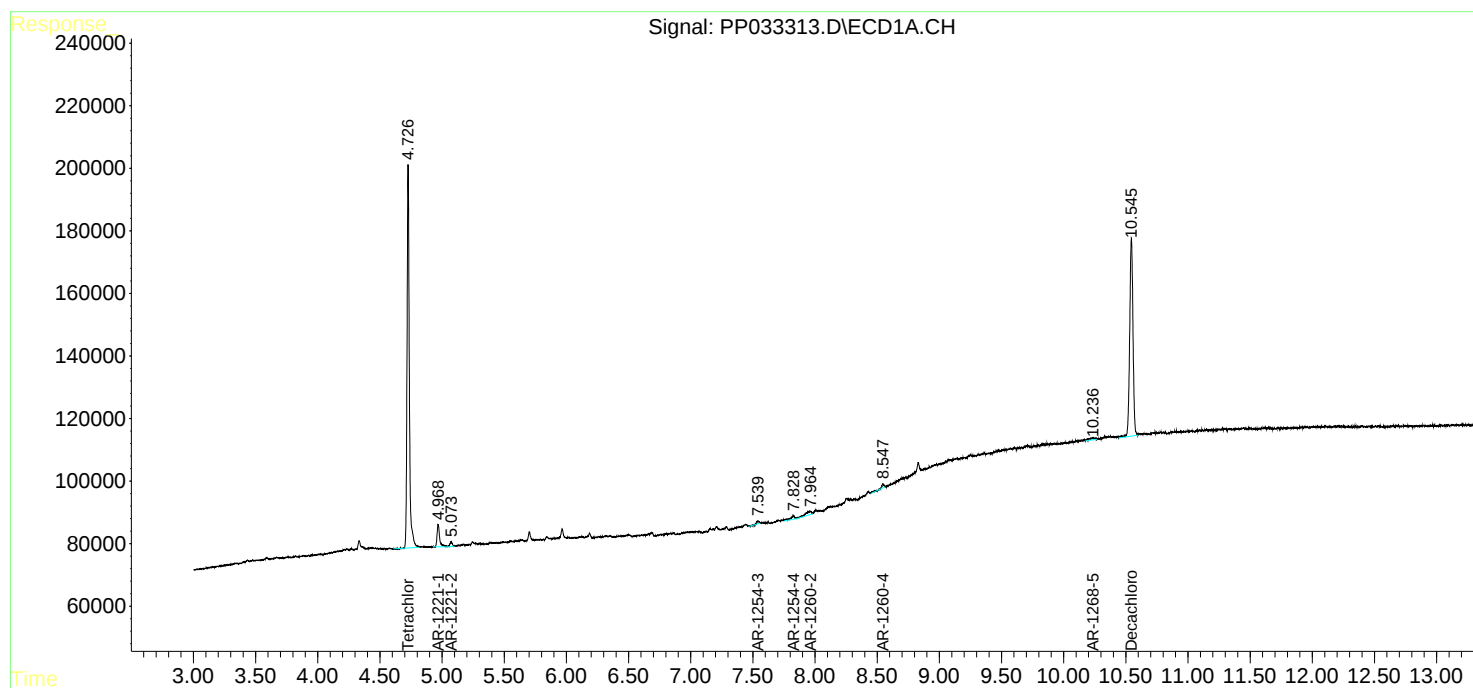


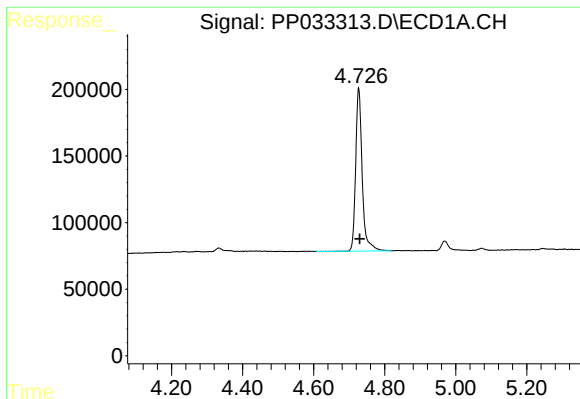

#1 Tetrachloro-m-xylene


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 1564393
Conc: 25.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

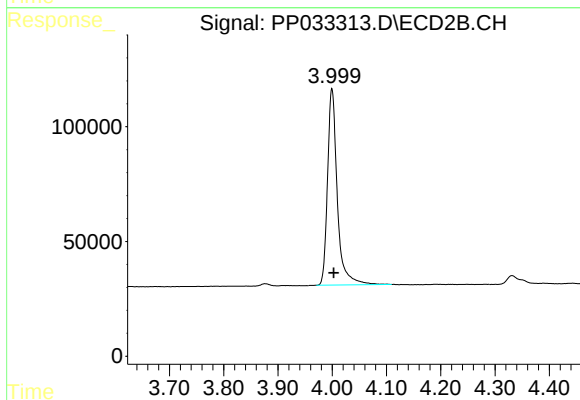


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1070643
Conc: 26.18 ng/ml

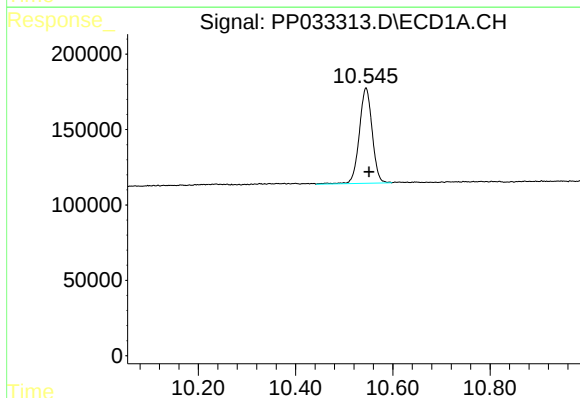


#2 Decachlorobiphenyl

R.T.: 10.545 min
Delta R.T.: -0.006 min
Response: 1158986
Conc: 26.61 ng/ml

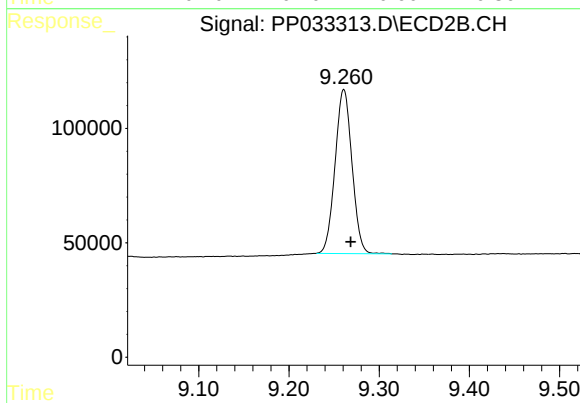

#2 Decachlorobiphenyl


R.T.: 9.261 min
Delta R.T.: -0.008 min
Response: 933503
Conc: 27.87 ng/ml

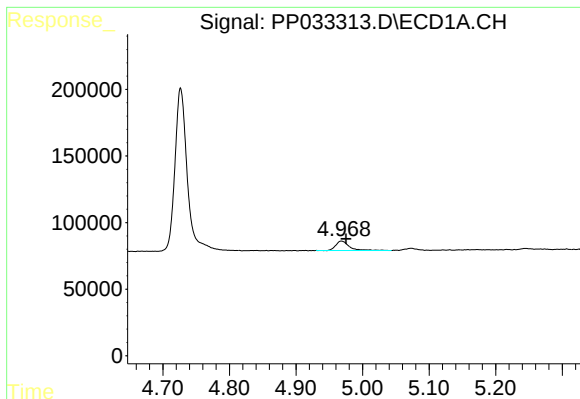

#8 AR-1221-1


R.T.: 4.968 min
Delta R.T.: -0.007 min
Response: 102817
Conc: 166.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

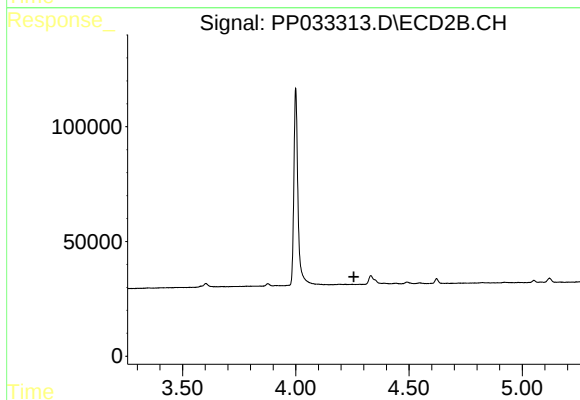


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.257 min
Response: 0
Conc: N.D.

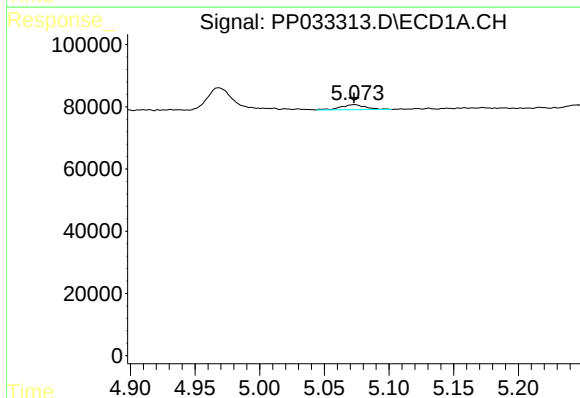


#9 AR-1221-2

R.T.: 5.073 min
Delta R.T.: 0.000 min
Response: 21948
Conc: 47.18 ng/ml

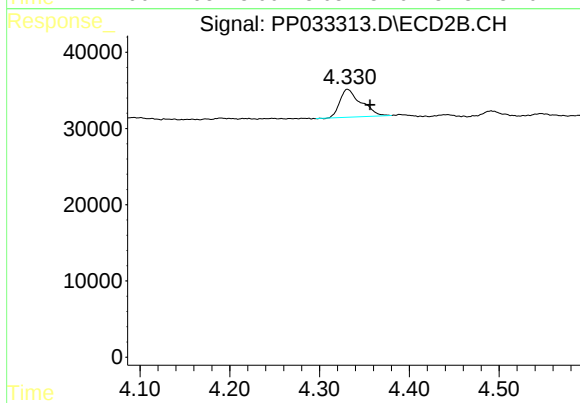

#9 AR-1221-2


R.T.: 4.331 min
Delta R.T.: -0.025 min
Response: 60199
Conc: 190.50 ng/ml

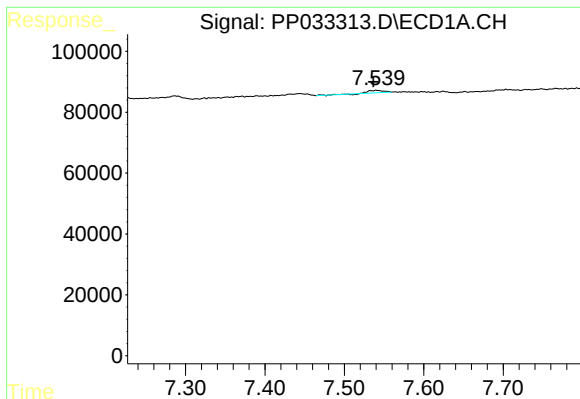

#28 AR-1254-3


R.T.: 7.540 min
Delta R.T.: 0.004 min
Response: 11111
Conc: 3.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

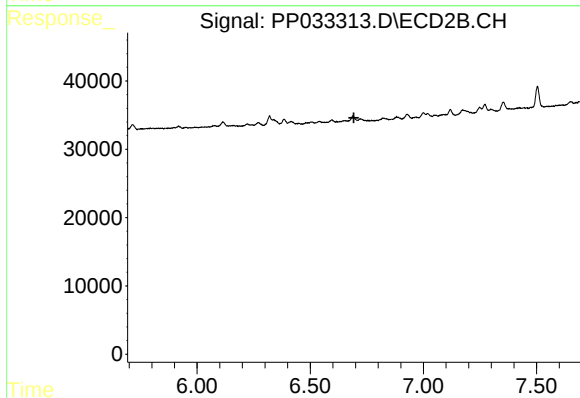


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

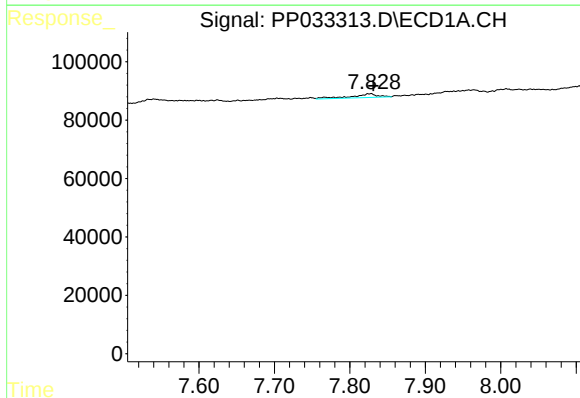


#29 AR-1254-4

R.T.: 7.828 min
Delta R.T.: -0.003 min
Response: 29491
Conc: 12.75 ng/ml

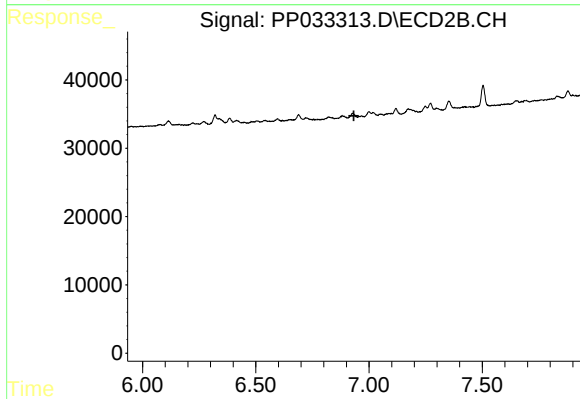

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

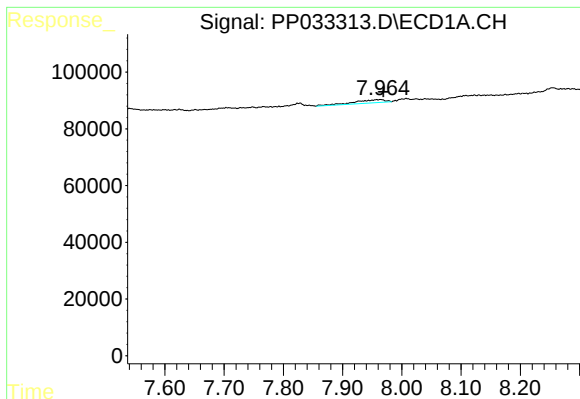

#32 AR-1260-2


R.T.: 7.964 min
Delta R.T.: -0.005 min
Response: 40492
Conc: 13.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

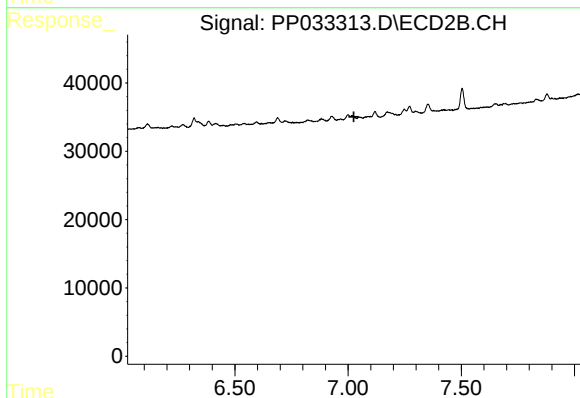


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

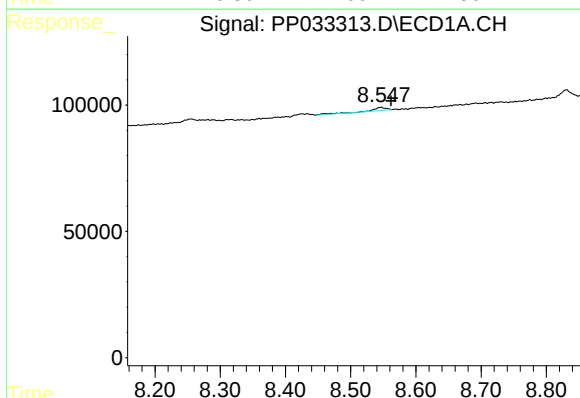


#34 AR-1260-4

R.T.: 8.547 min
Delta R.T.: -0.015 min
Response: 19562
Conc: 8.01 ng/ml

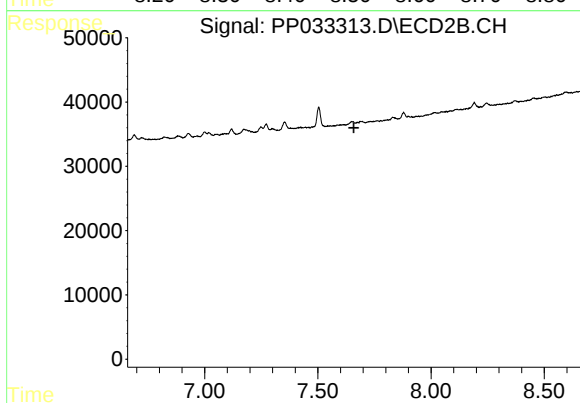

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

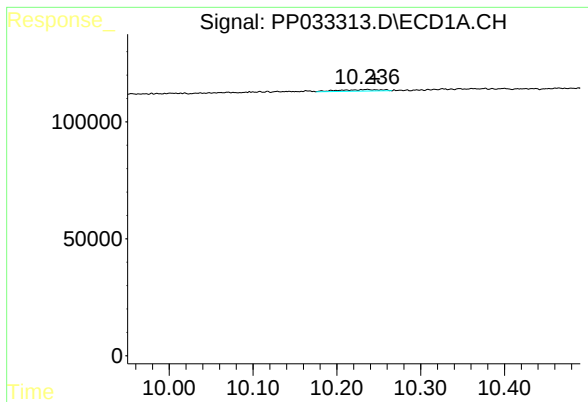

#45 AR-1268-5

R.T.: 10.236 min
Delta R.T.: -0.009 min
Response: 22157
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

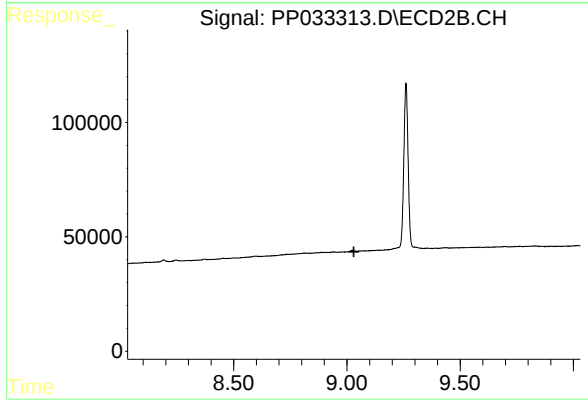

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.