

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
 Data File : PP033308.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Feb 2021 14:25
 Operator : DD\AJ
 Sample : M1385-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-04-021121

Manual Integrations
 APPROVED

Ankita
 2/15/2021 8:20:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 16:52:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.726	4.000	1793126	1403417	29.241m	34.320
2) SA Decachlor...	10.543	9.262	1398459	1102320	32.103m	32.905

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
Data File : PP033308.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2021 14:25
Operator : DD\AJ
Sample : M1385-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-04-021121


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 16:52:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

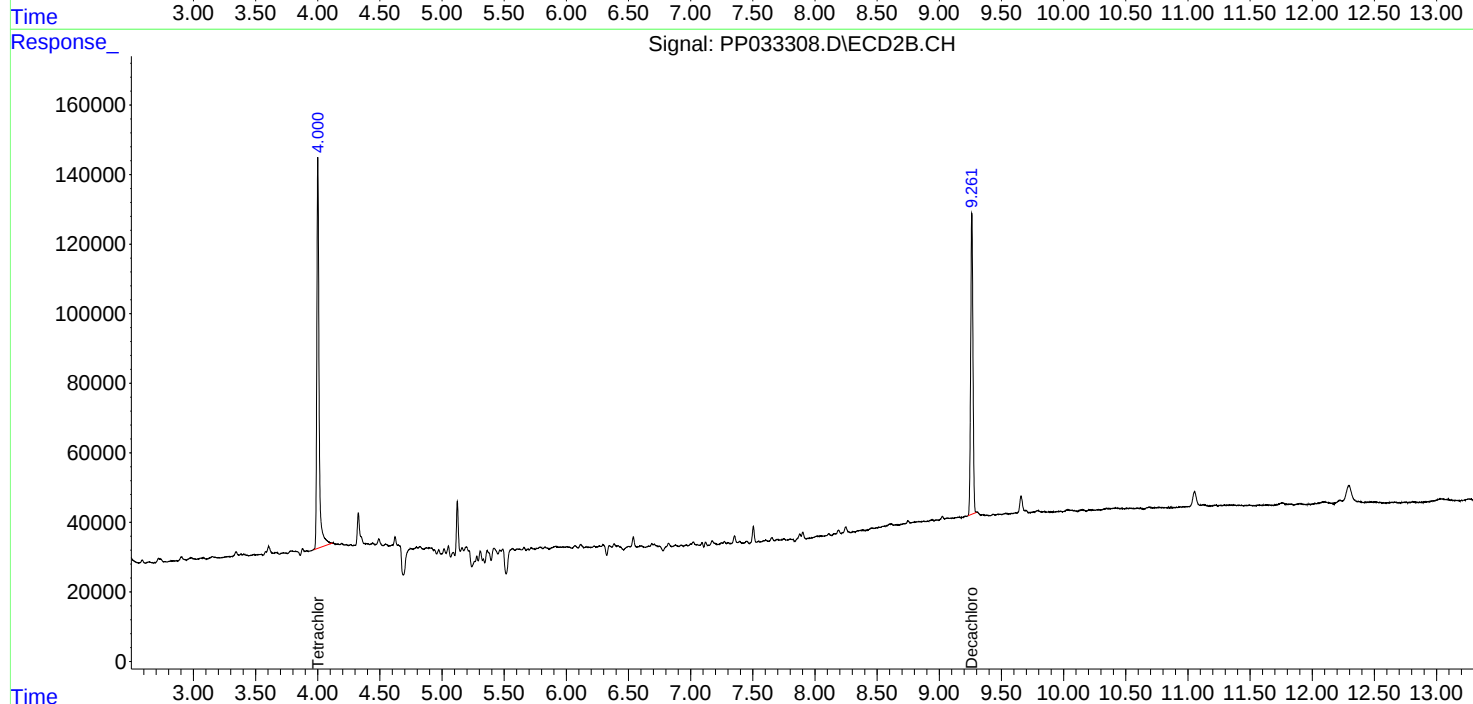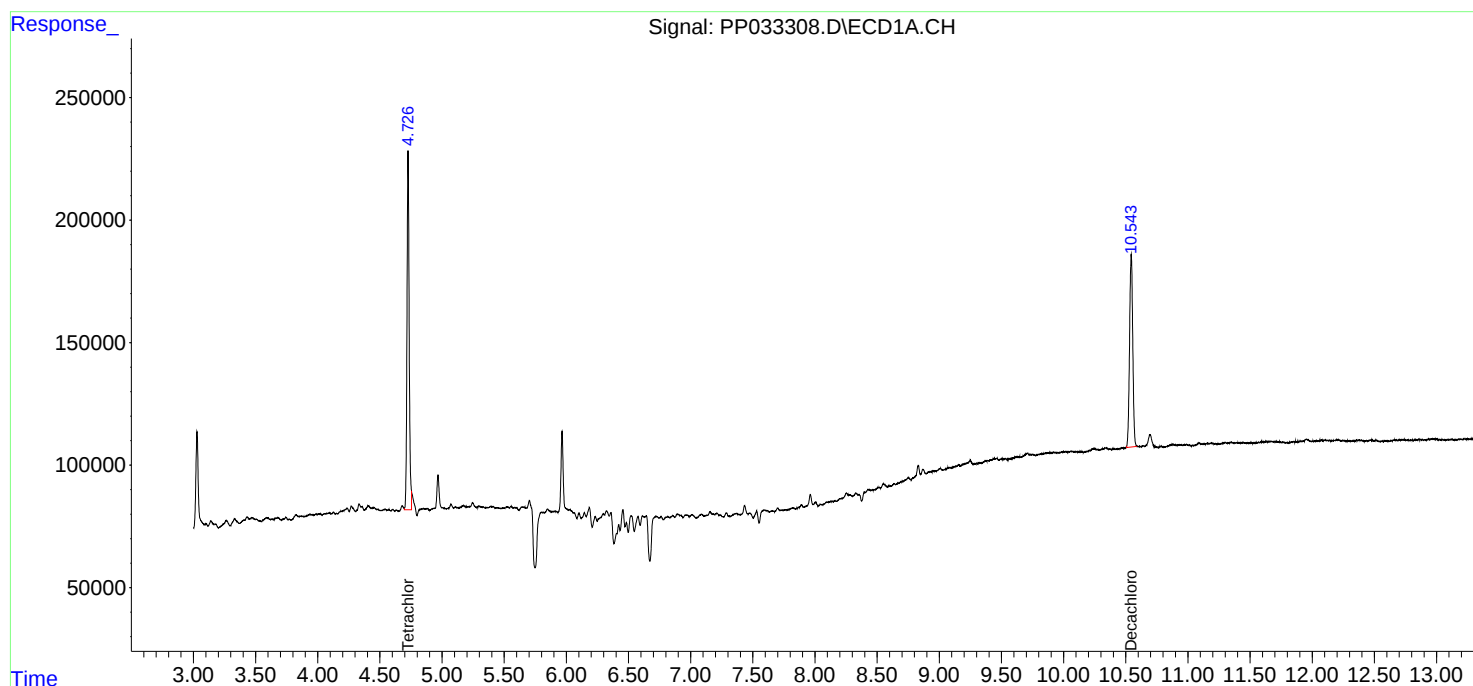

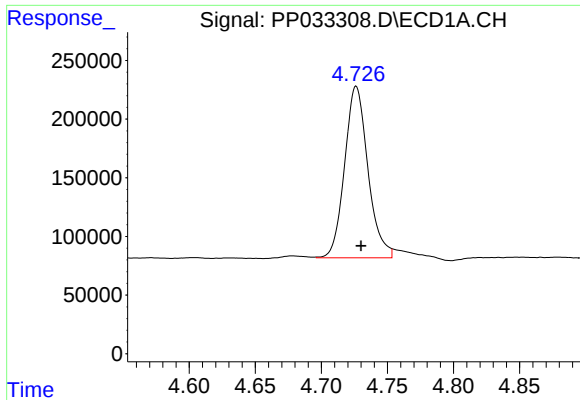


#1 Tetrachloro-m-xylene

R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1793126
Conc: 29.24 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TR-04-021121


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:24 AM

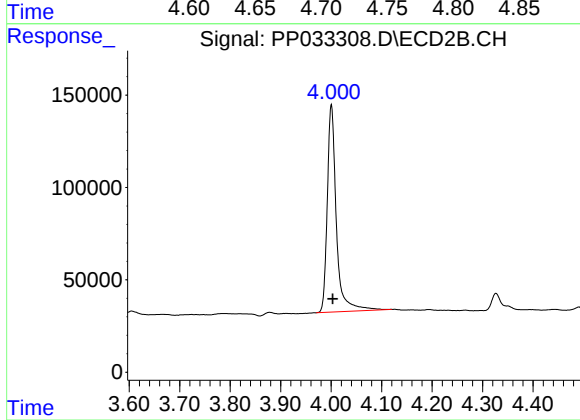


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1403417
Conc: 34.32 ng/ml

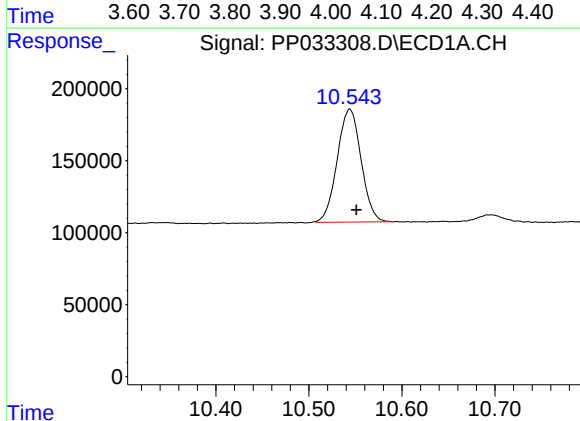

#2 Decachlorobiphenyl

R.T.: 10.543 min
Delta R.T.: -0.008 min
Response: 1398459
Conc: 32.10 ng/ml m

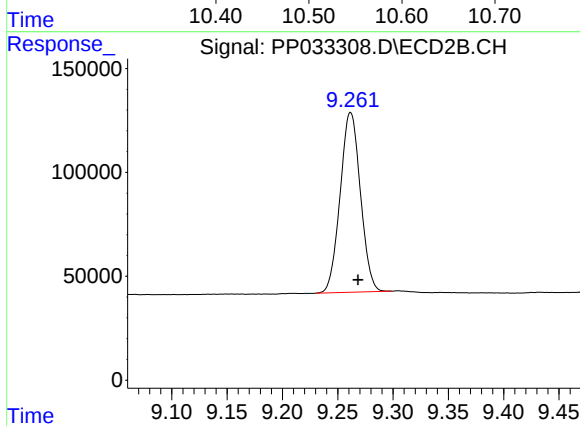

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: -0.007 min
Response: 1102320
Conc: 32.91 ng/ml