

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
 Data File : PP033311.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Feb 2021 15:15
 Operator : DD\AJ
 Sample : M1394-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-03-019-ABCD

Manual Integrations
 APPROVED

Ankita
 2/15/2021 8:20:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 04:55:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.726	4.000	1561517	1092806	25.464	26.724
2) SA Decachlor...	10.543	9.261	1046678	851209	24.028	25.409
Target Compounds						
21) L5 AR-1248-1	6.024	5.245	14803	14970	15.461m	23.019m#
22) L5 AR-1248-2	6.321	5.507	15471	10301	11.676m	10.738m
23) L5 AR-1248-3	6.530	5.553	24602	12045	15.193m	11.847m
24) L5 AR-1248-4	6.957	5.735	27275	19214	15.851	15.504m
25) L5 AR-1248-5	6.993	6.156	29410	14578	16.902	12.909m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
Data File : PP033311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2021 15:15
Operator : DD\AJ
Sample : M1394-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-019-ABCD


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 04:55:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

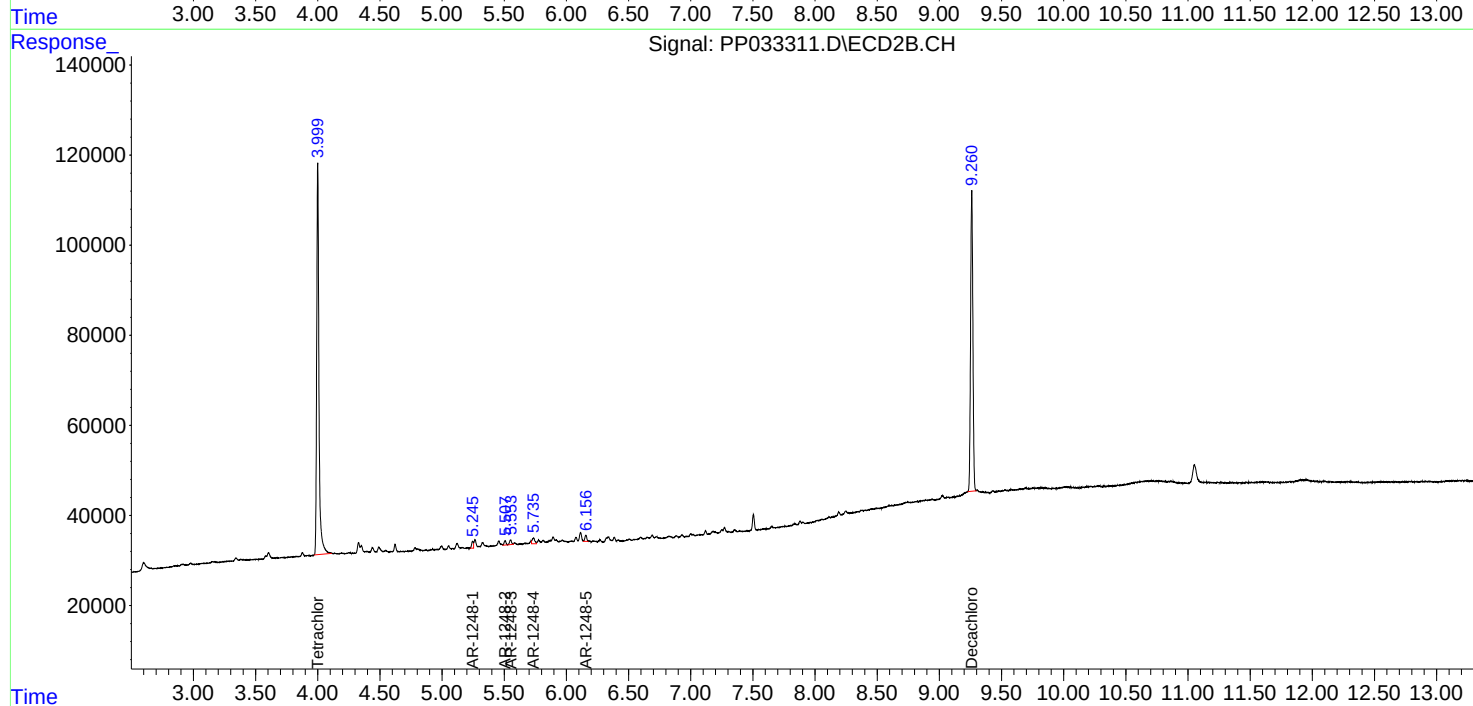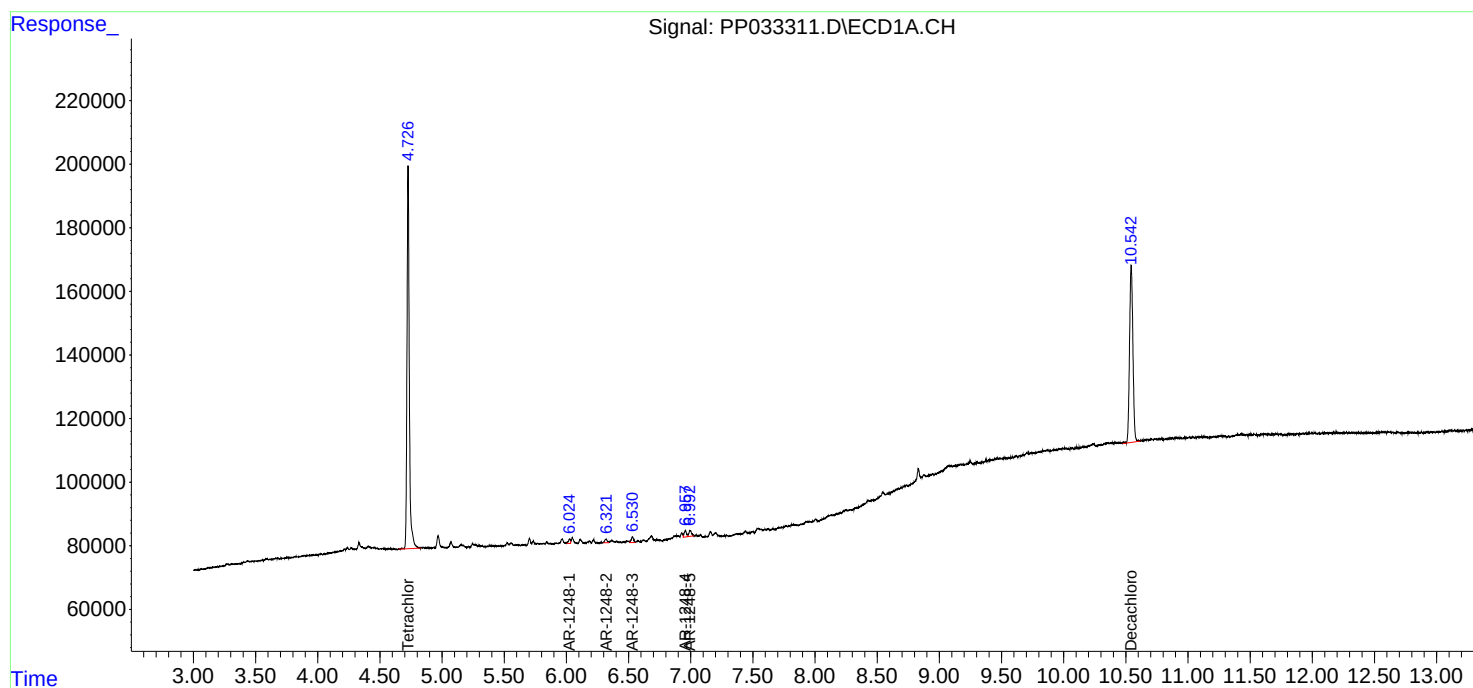

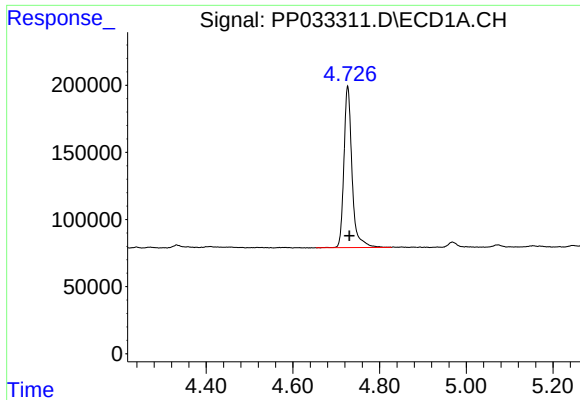


#1 Tetrachloro-m-xylene

R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1561517
Conc: 25.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-019-ABCD


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:26 AM

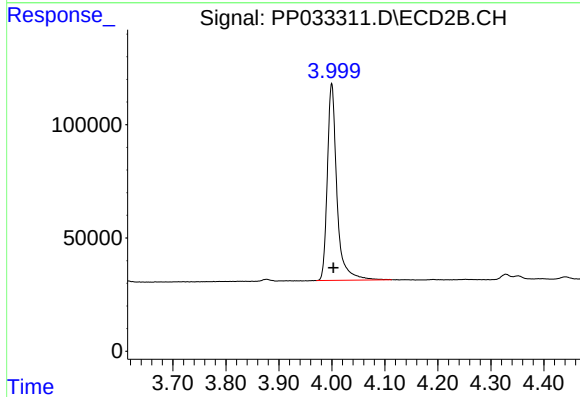


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1092806
Conc: 26.72 ng/ml

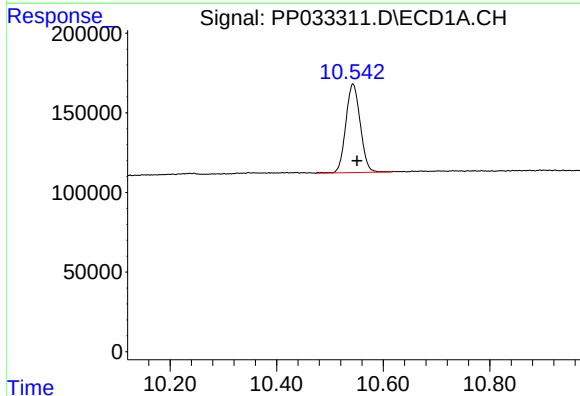


#2 Decachlorobiphenyl

R.T.: 10.543 min
Delta R.T.: -0.008 min
Response: 1046678
Conc: 24.03 ng/ml

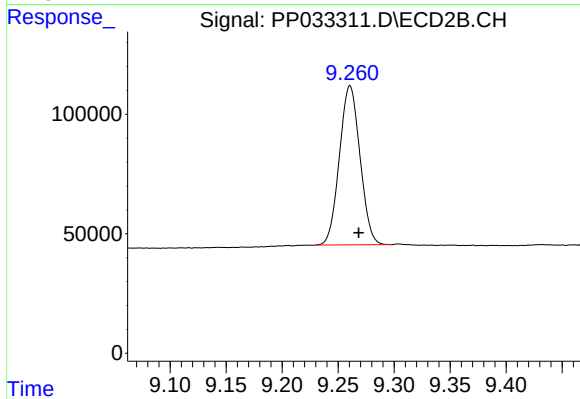

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: -0.008 min
Response: 851209
Conc: 25.41 ng/ml

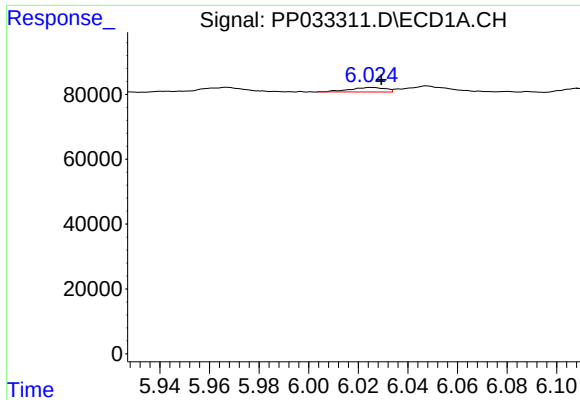


#21 AR-1248-1

R.T.: 6.024 min
Delta R.T.: -0.005 min
Response: 14803
Conc: 15.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-019-ABCD


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:26 AM

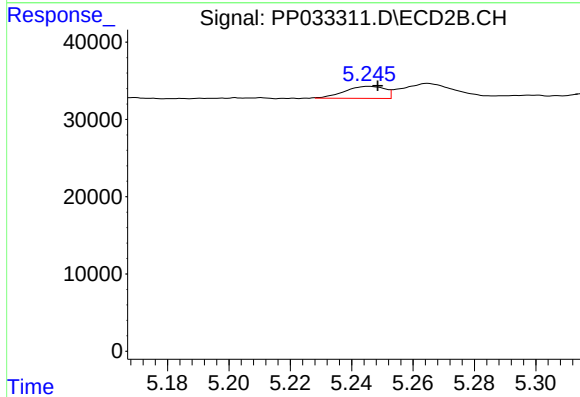


#21 AR-1248-1

R.T.: 5.245 min
Delta R.T.: -0.004 min
Response: 14970
Conc: 23.02 ng/ml m

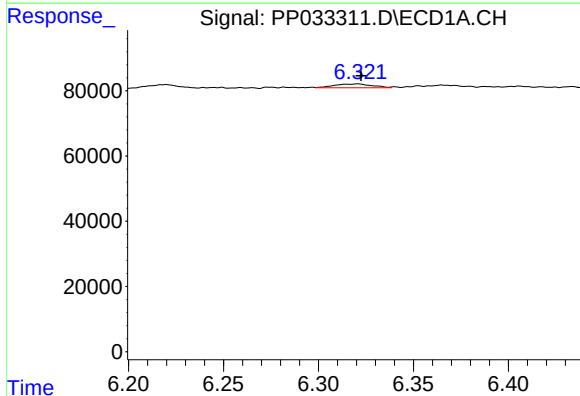


#22 AR-1248-2

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 15471
Conc: 11.68 ng/ml m

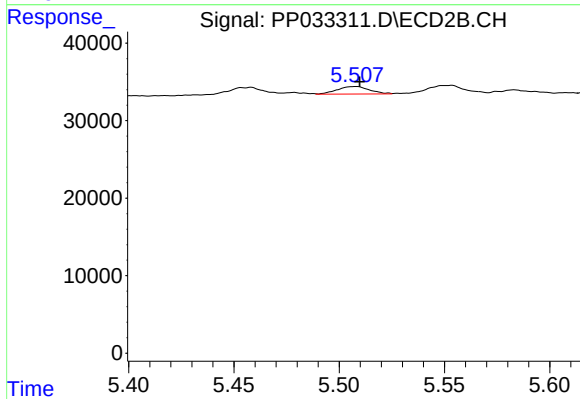

#22 AR-1248-2

R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 10301
Conc: 10.74 ng/ml m

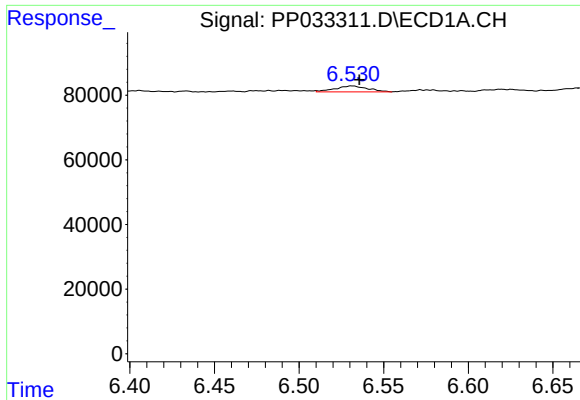


#23 AR-1248-3

R.T.: 6.530 min
Delta R.T.: -0.005 min
Response: 24602
Conc: 15.19 ng/ml m

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-019-ABCD


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:26 AM

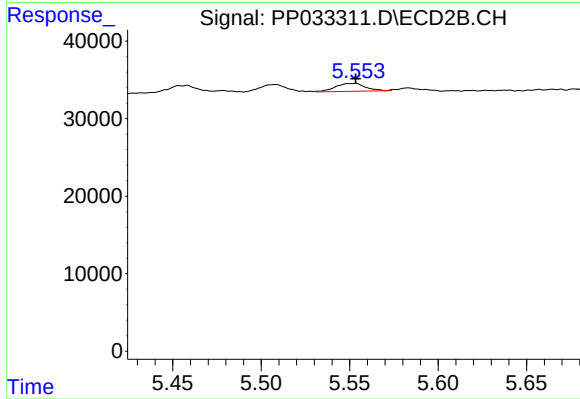


#23 AR-1248-3

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 12045
Conc: 11.85 ng/ml m

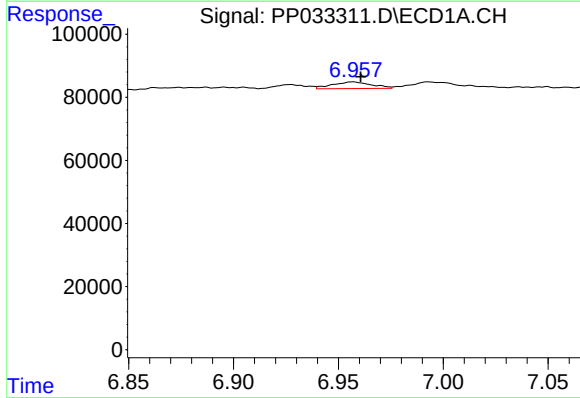


#24 AR-1248-4

R.T.: 6.957 min
Delta R.T.: -0.004 min
Response: 27275
Conc: 15.85 ng/ml

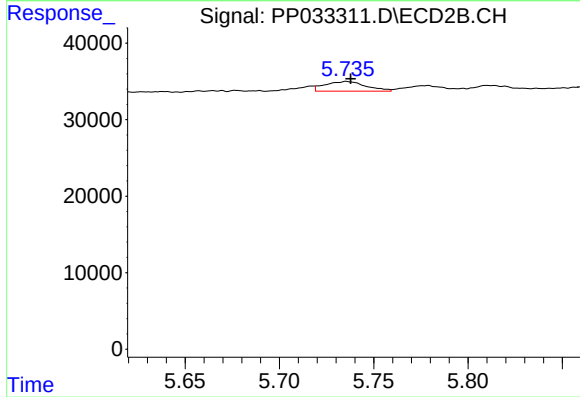

#24 AR-1248-4

R.T.: 5.735 min
Delta R.T.: -0.003 min
Response: 19214
Conc: 15.50 ng/ml m

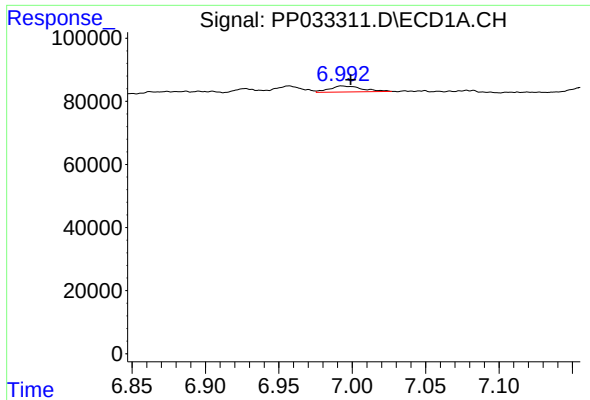


#25 AR-1248-5

R.T.: 6.993 min
Delta R.T.: -0.006 min
Response: 29410
Conc: 16.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-019-ABCD

Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:26 AM

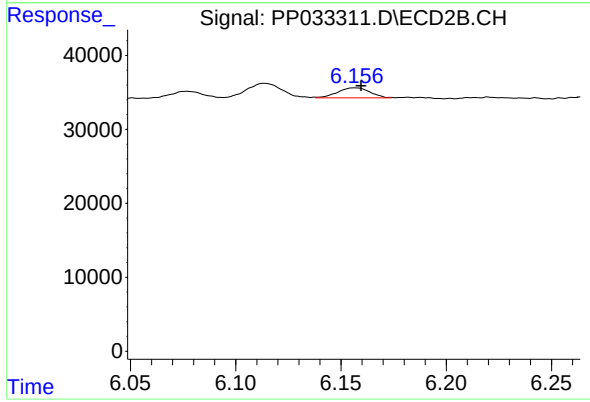

#25 AR-1248-5

R.T.: 6.156 min
Delta R.T.: -0.003 min
Response: 14578
Conc: 12.91 ng/ml m