

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
 Data File : PP033322.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Feb 2021 18:52
 Operator : DD\AJ
 Sample : PB134607BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB134607BL

Manual Integrations
 APPROVED

Ankita
 2/15/2021 8:20:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:07:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.726	3.999	1350189	896097	22.018m	21.914
2) SA Decachlor...	10.543	9.261	999204	842107	22.938m	25.137

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021221\
Data File : PP033322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2021 18:52
Operator : DD\AJ
Sample : PB134607BL
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB134607BL


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:07:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

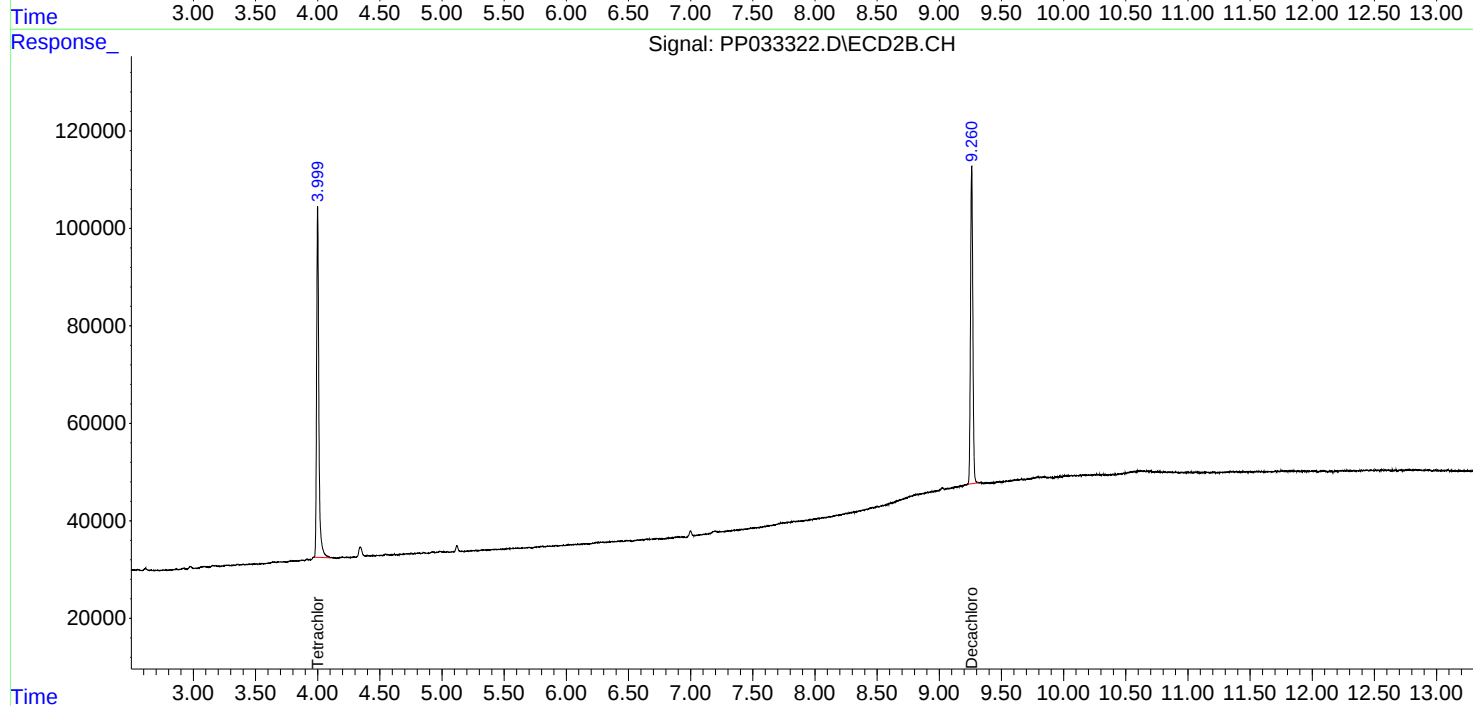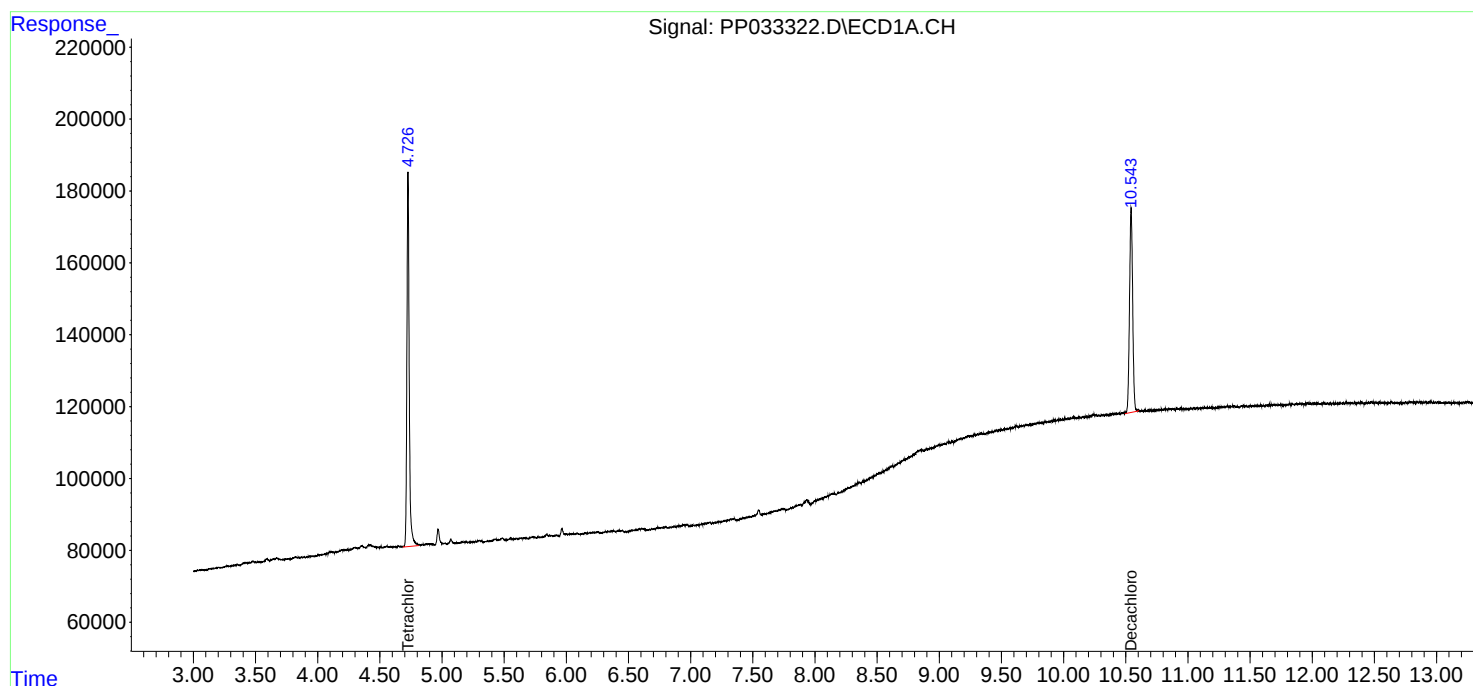

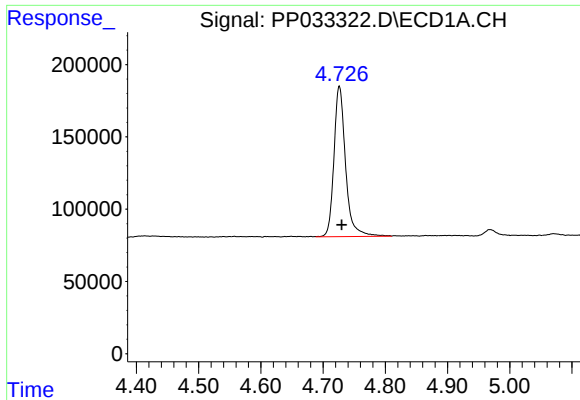


#1 Tetrachloro-m-xylene

R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1350189
Conc: 22.02 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PB134607BL


Manual Integrations
APPROVED

Ankita
2/15/2021 8:20:48 AM

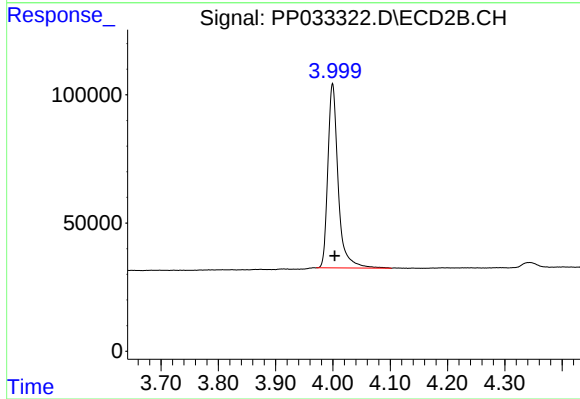


#1 Tetrachloro-m-xylene

R.T.: 3.999 min
Delta R.T.: -0.004 min
Response: 896097
Conc: 21.91 ng/ml

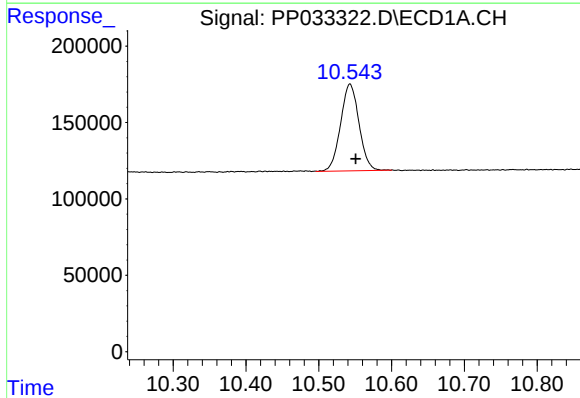

#2 Decachlorobiphenyl

R.T.: 10.543 min
Delta R.T.: -0.008 min
Response: 999204
Conc: 22.94 ng/ml m

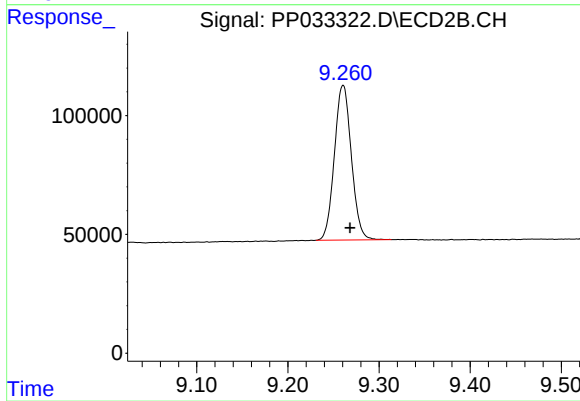

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: -0.008 min
Response: 842107
Conc: 25.14 ng/ml