

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 01:04
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 03:43:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.777	0	317.7E6	N.D.	743.159 #
Target Compounds							
1) T	Dalapon	2.836	2.308	37500703	378.3E6	67.979	705.809 #
3) T	4-Nitroph...	0.000	9.927	0	151.5E6	N.D.	724.878 #
8) T	DICHLORPROP	0.000	12.182	0	282.1E6	N.D.	737.881 #
9) T	2,4-D	0.000	12.655	0	170.7E6	N.D.	340.364 #
11) T	2,4,5-TP ...	14.376	13.815	1911.4E6	1795.0E6	758.963	723.701
12) T	2,4,5-T	14.776	14.347	1856.5E6	1895.3E6	761.038	990.477 #
14) T	DINOSEB	16.990	0.000	1420.2E6	0	754.912	N.D. #
15) T	Picloram	16.764	16.685	2267.2E6	2138.7E6	716.654	711.385
16) T	DCPA	0.000	16.685	0	2138.7E6	N.D.	690.443 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 01:04
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 03:43:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

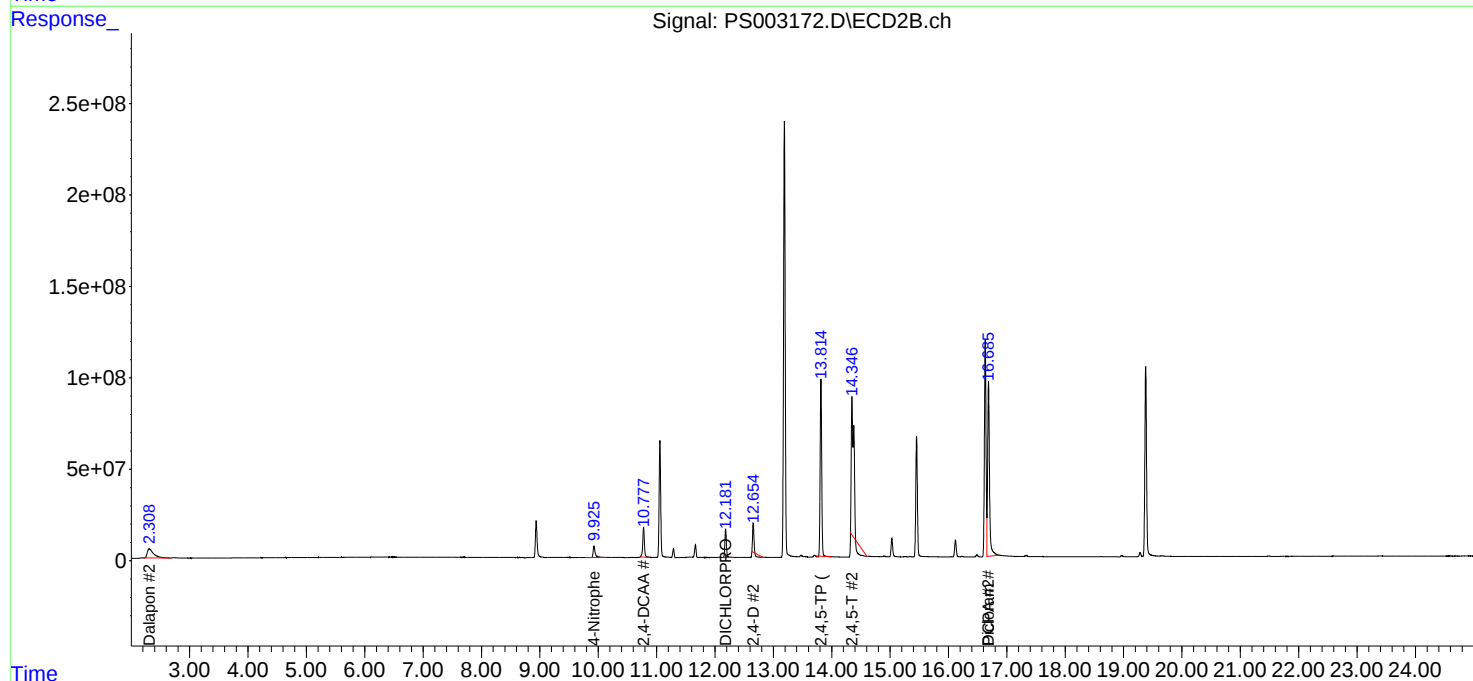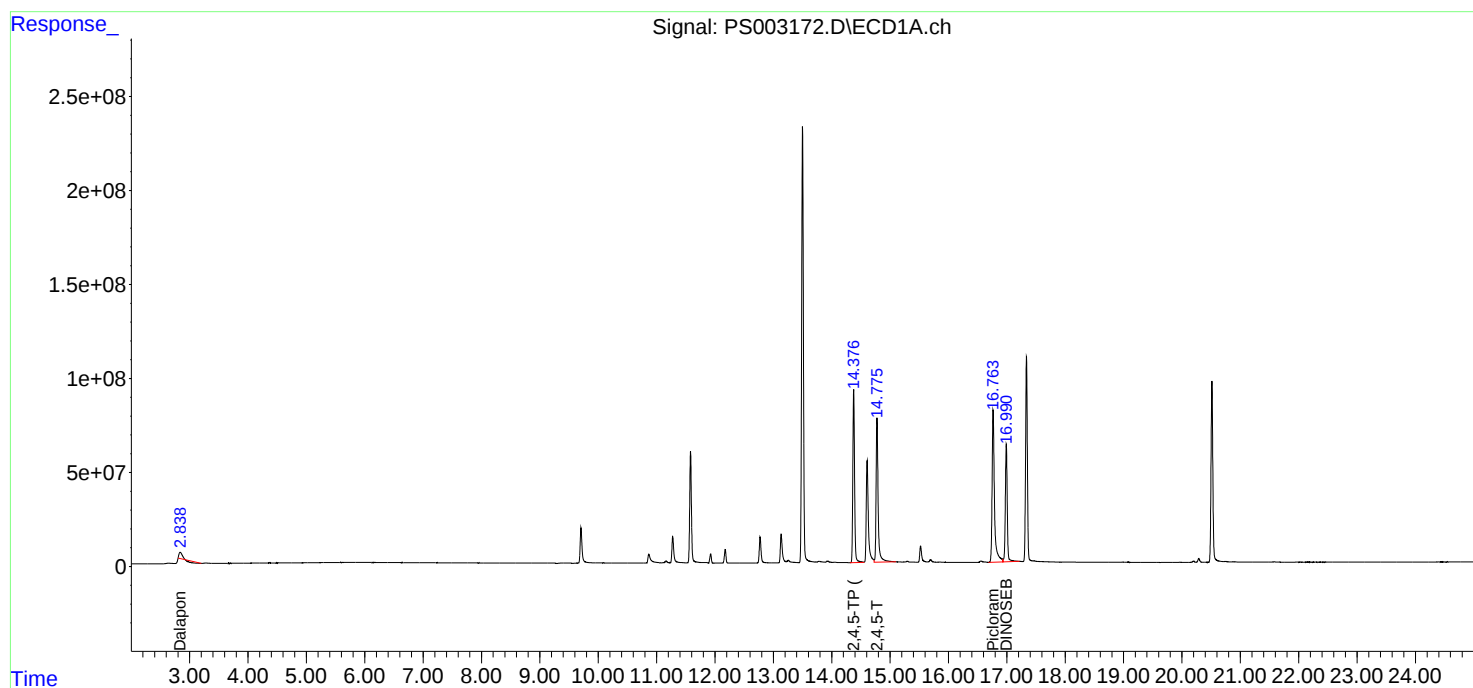


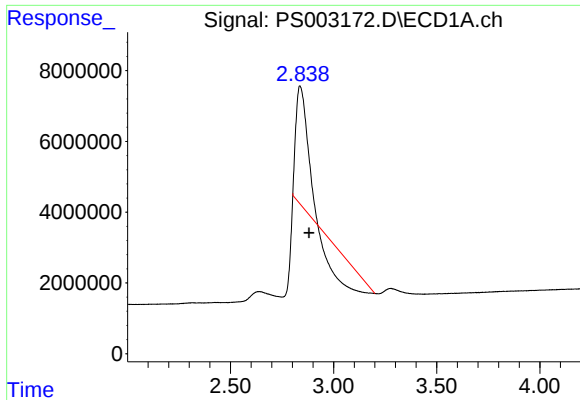

#1 Dalapon


R.T.: 2.836 min
Delta R.T.: -0.044 min
Response: 37500703
Conc: 67.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

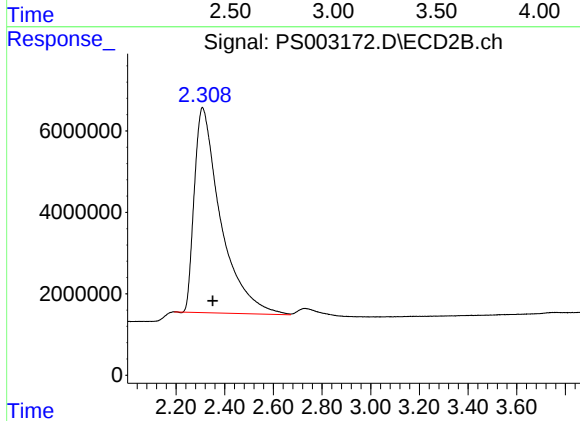


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.042 min
Response: 378257987
Conc: 705.81 ng/ml

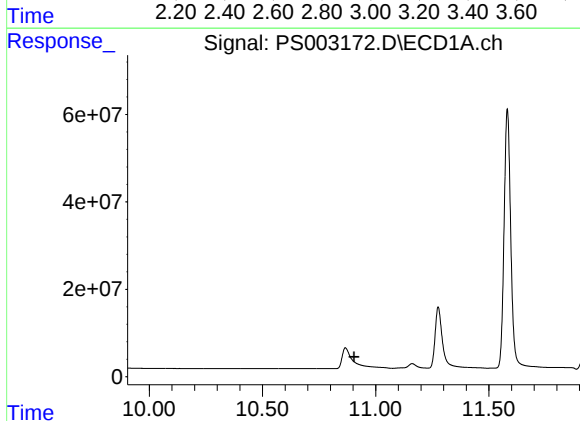


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

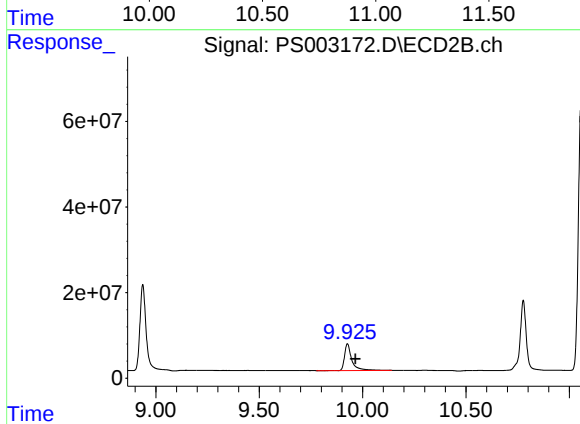

#3 4-Nitrophenol


R.T.: 9.927 min
Delta R.T.: -0.039 min
Response: 151515802
Conc: 724.88 ng/ml

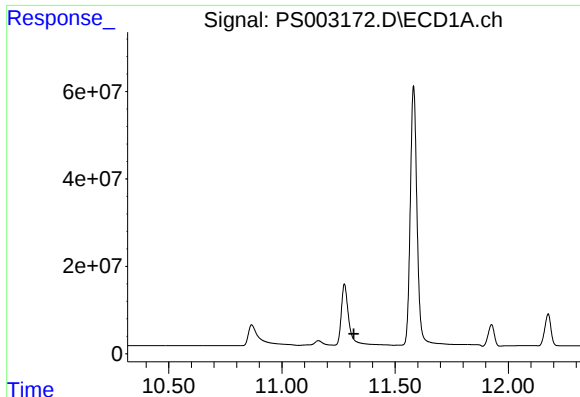

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

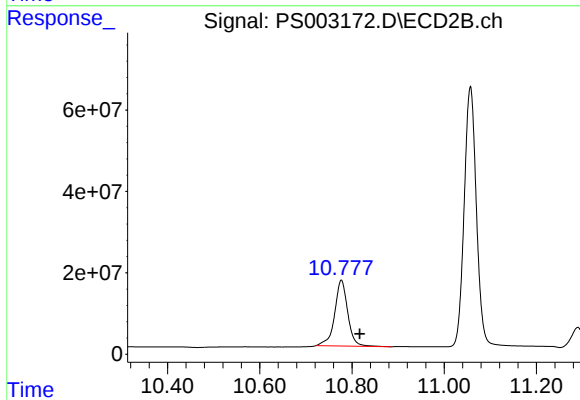


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 317734339
Conc: 743.16 ng/ml

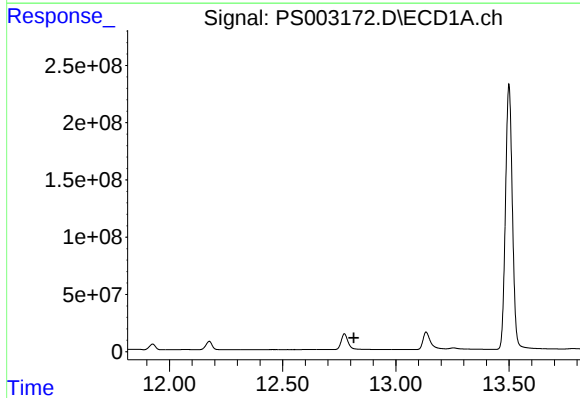


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

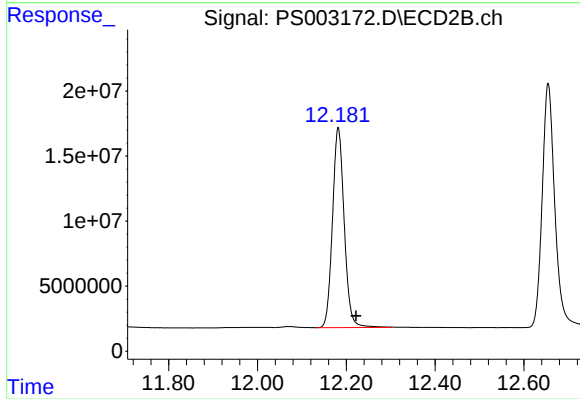

#8 DICHLORPROP


R.T.: 12.182 min
Delta R.T.: -0.040 min
Response: 282122111
Conc: 737.88 ng/ml

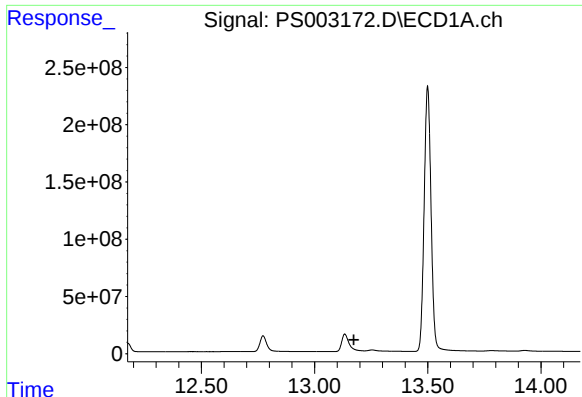

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

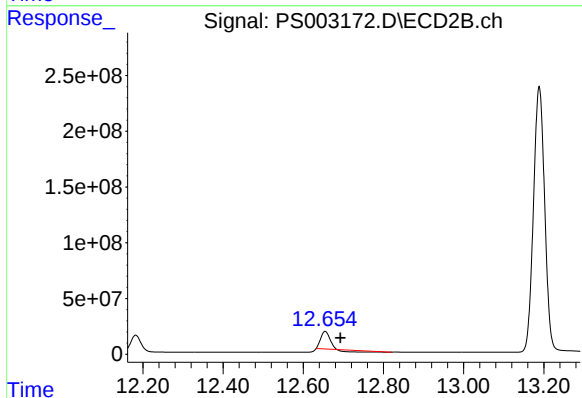


#9 2,4-D

R.T.: 12.655 min
Delta R.T.: -0.038 min
Response: 170653758
Conc: 340.36 ng/ml

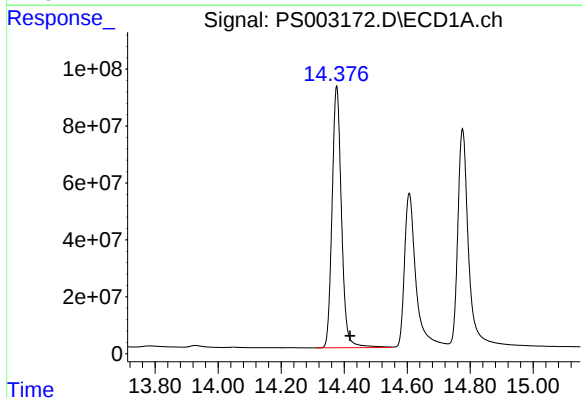


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.043 min
Response: 1911351782
Conc: 758.96 ng/ml

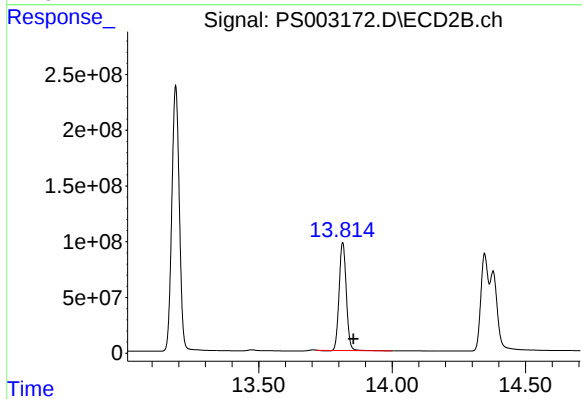

#11 2,4,5-TP (SILVEX)


R.T.: 13.815 min
Delta R.T.: -0.040 min
Response: 1795035538
Conc: 723.70 ng/ml

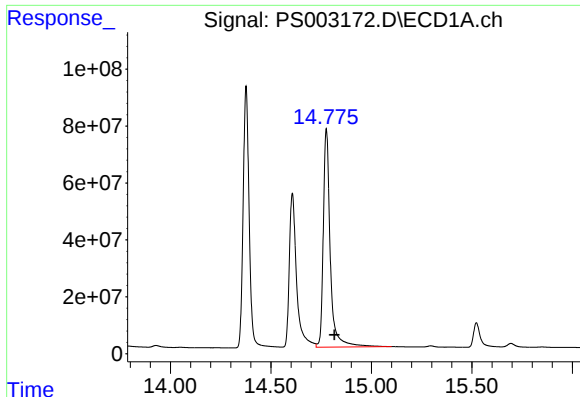

#12 2,4,5-T


R.T.: 14.776 min
Delta R.T.: -0.041 min
Response: 1856479081
Conc: 761.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

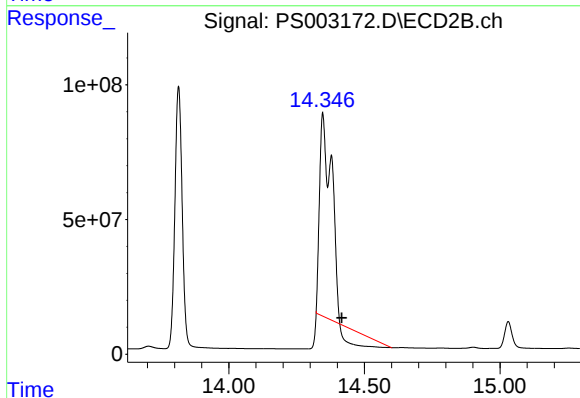


#12 2,4,5-T

R.T.: 14.347 min
Delta R.T.: -0.070 min
Response: 1895267667
Conc: 990.48 ng/ml

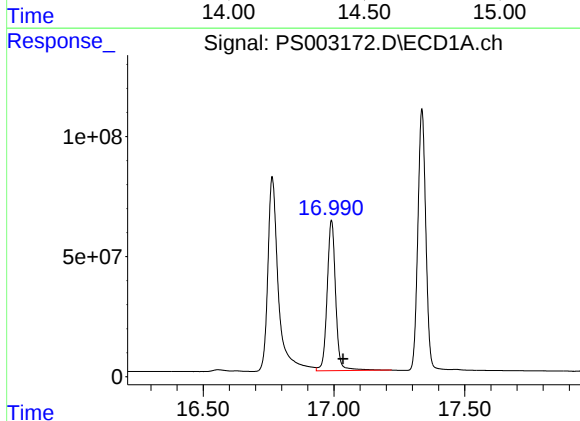


#14 DINOSEB

R.T.: 16.990 min
Delta R.T.: -0.045 min
Response: 1420236833
Conc: 754.91 ng/ml

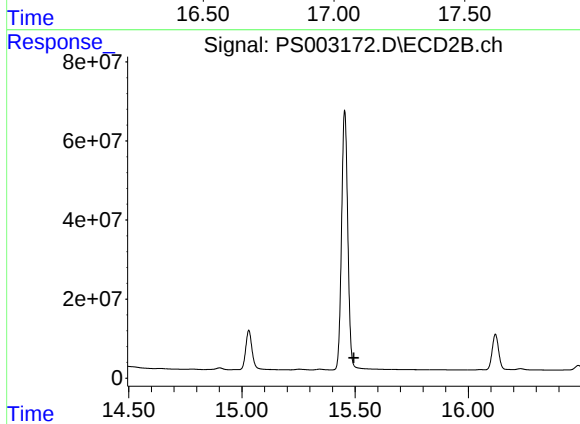

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

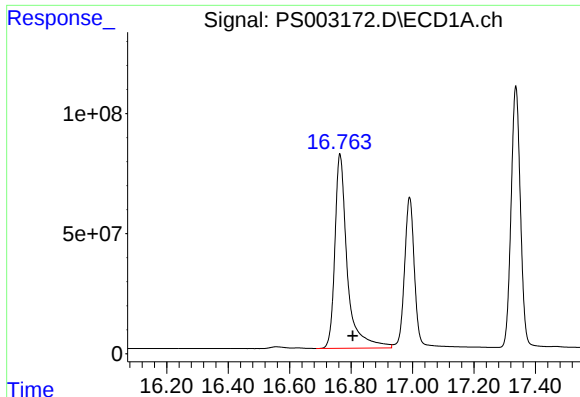

#15 Picloram


R.T.: 16.764 min
Delta R.T.: -0.041 min
Response: 2267229442
Conc: 716.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

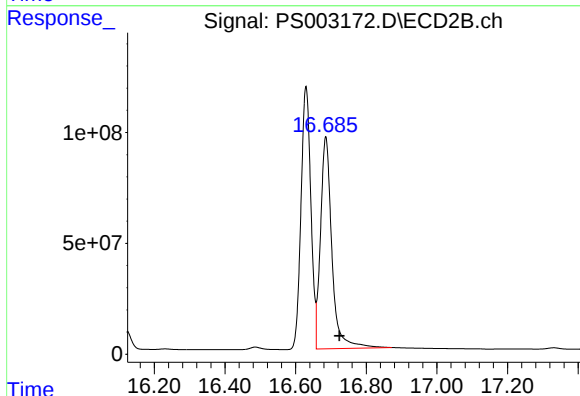


#15 Picloram

R.T.: 16.685 min
Delta R.T.: -0.039 min
Response: 2138708993
Conc: 711.38 ng/ml

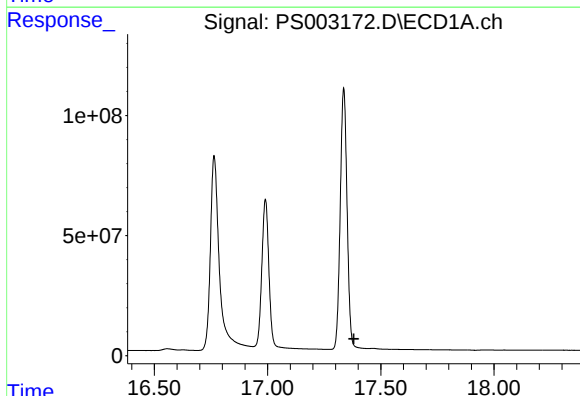

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

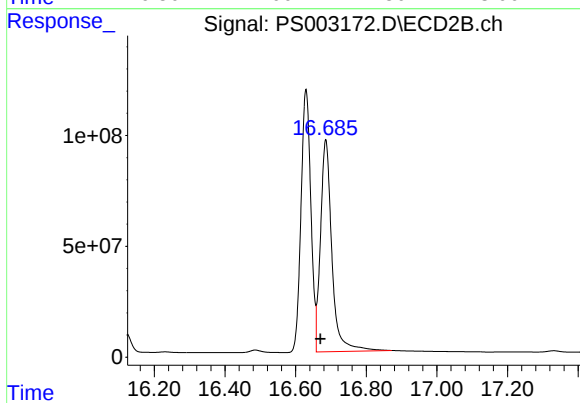

#16 DCPA

R.T.: 16.685 min
Delta R.T.: 0.016 min
Response: 2138708993
Conc: 690.44 ng/ml