

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 01:36
 Operator : EI\SJ
 Sample : PB117093BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 03:44:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.778	136.6E6	245.2E6	359.782	573.523 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.029	0	2305031	N.D.	4.090 #
6) T	MCPP	11.965	0.000	9222441	0	7.697	N.D. #
12) T	2,4,5-T	0.000	14.402	0	4630704	N.D.	2.420 #
14) T	DINOSEB	0.000	15.510	0	3279159	N.D.	1.871 #
15) T	Picloram	0.000	16.708	0	82062283	N.D.	27.296 #
16) T	DCPA	0.000	16.708	0	82062283	N.D.	26.492 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 01:36
Operator : EI\SJ
Sample : PB117093BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 03:44:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

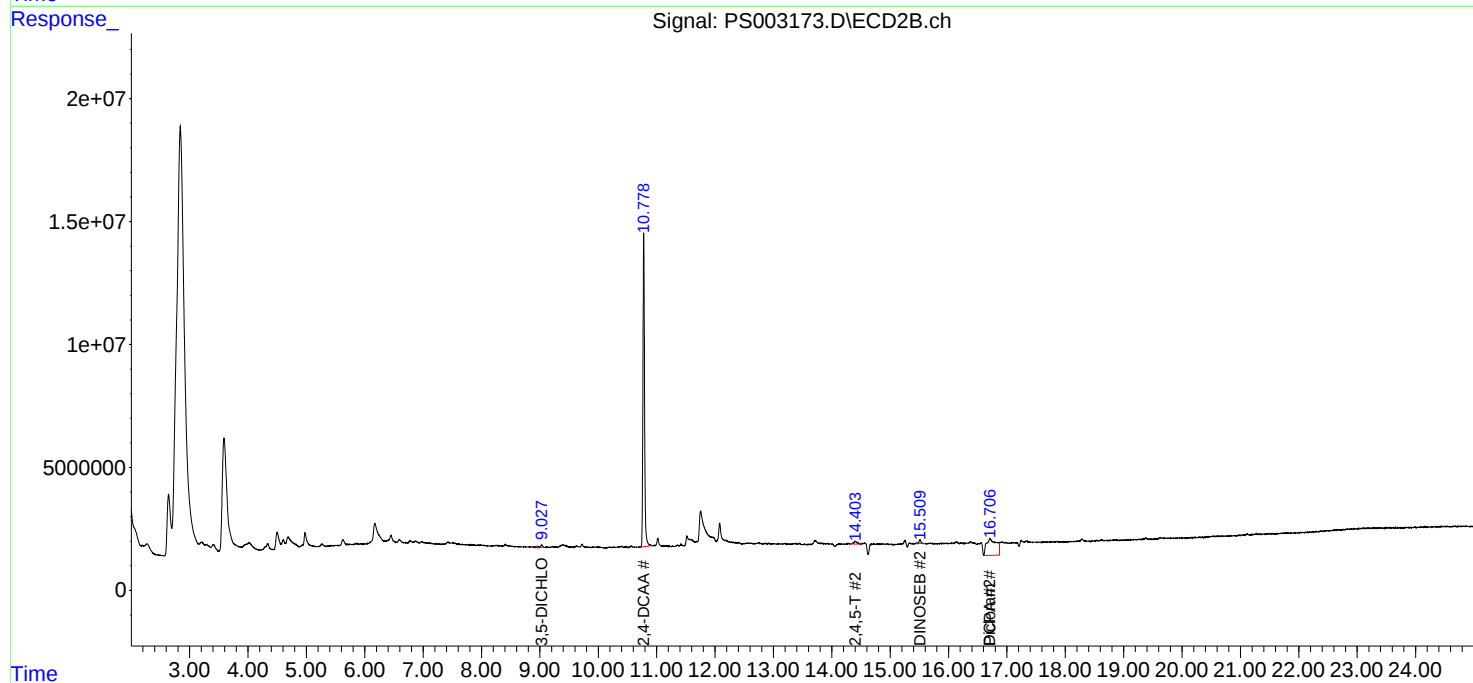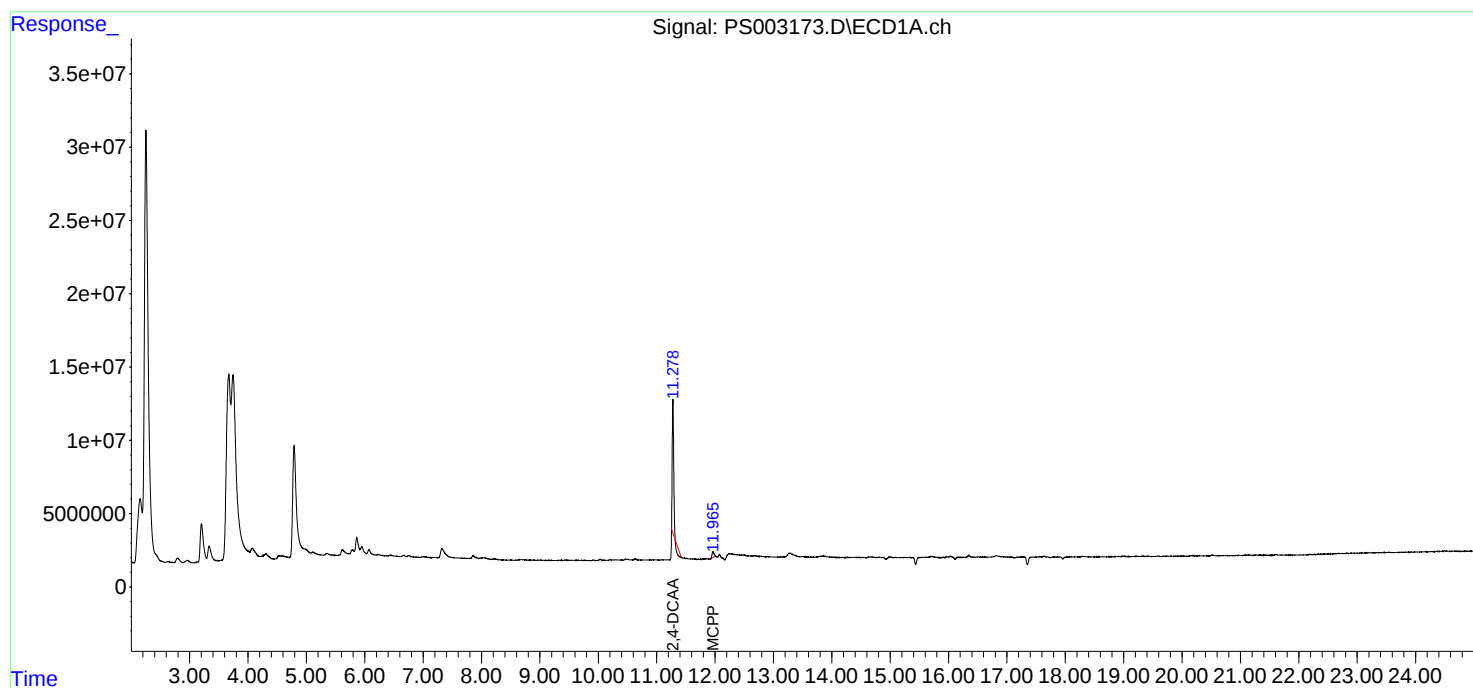


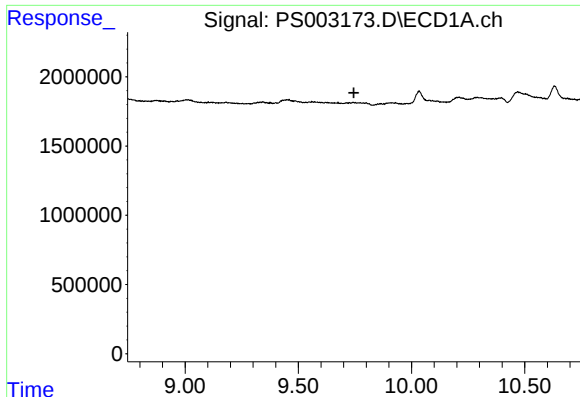

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

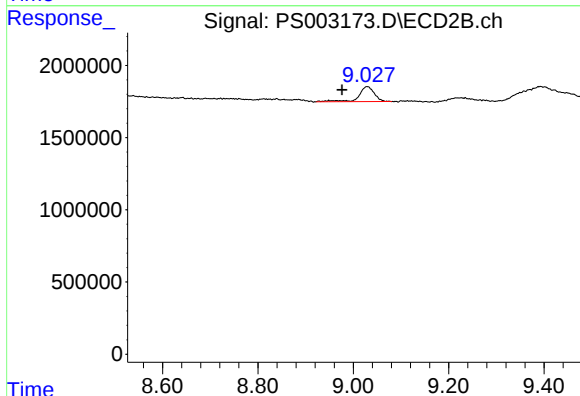


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.029 min
Delta R.T.: 0.053 min
Response: 2305031
Conc: 4.09 ng/ml

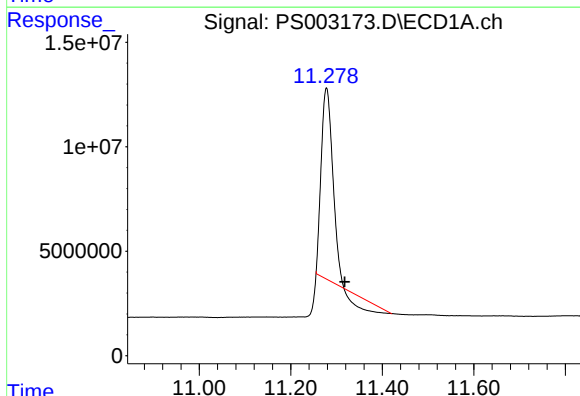


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: -0.040 min
Response: 136588056
Conc: 359.78 ng/ml

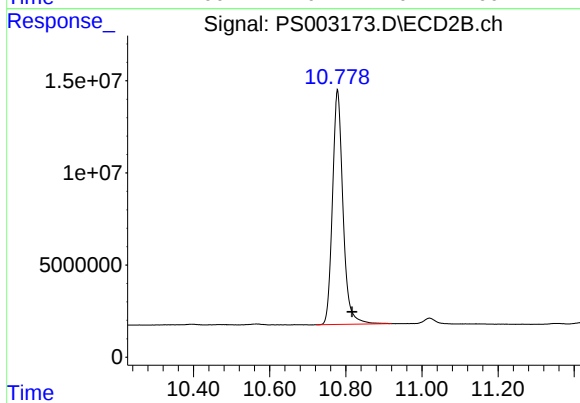

#4 2,4-DCAA


R.T.: 10.778 min
Delta R.T.: -0.038 min
Response: 245207304
Conc: 573.52 ng/ml

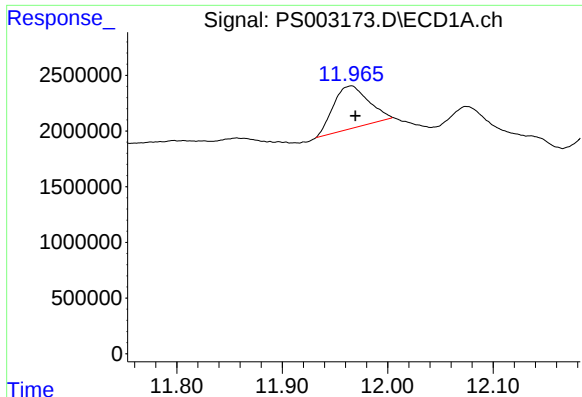

#6 MCP


R.T.: 11.965 min
Delta R.T.: -0.005 min
Response: 9222441
Conc: 7.70 ug/ml

Instrument :
ECD_P
ClientSampleId :

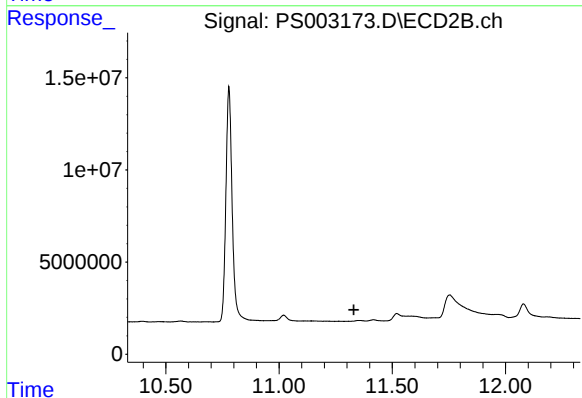


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

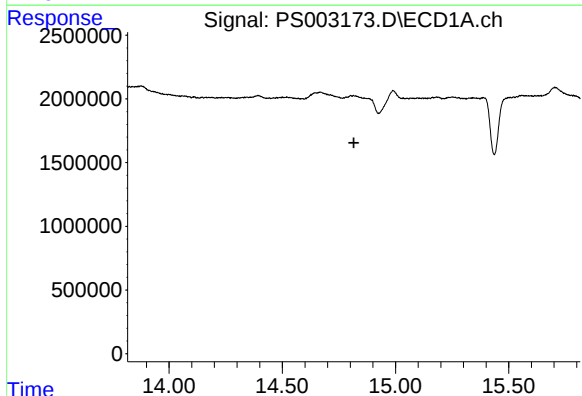


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

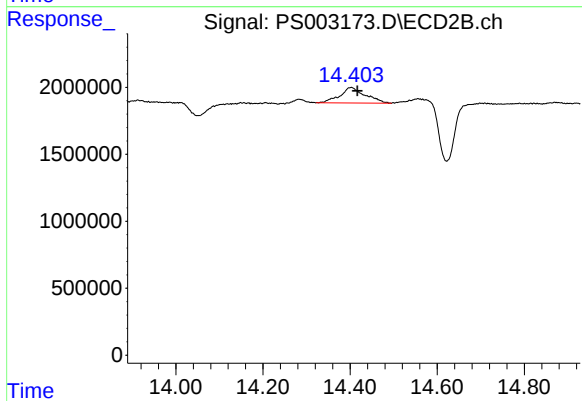

#12 2,4,5-T


R.T.: 14.402 min
Delta R.T.: -0.015 min
Response: 4630704
Conc: 2.42 ng/ml

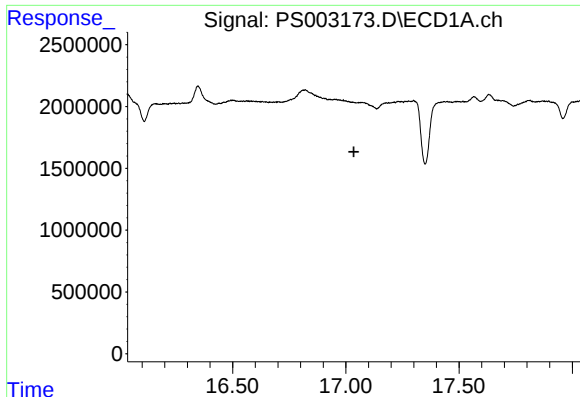

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

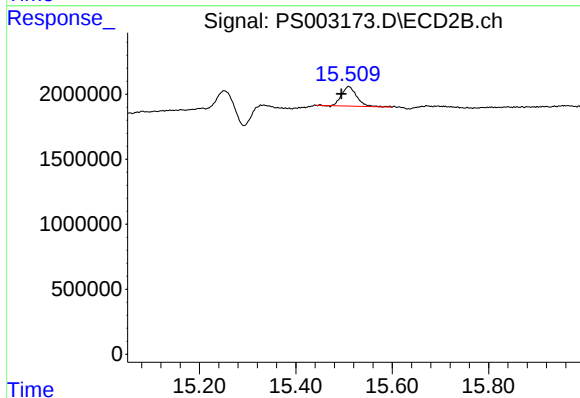


#14 DINOSEB

R.T.: 15.510 min
Delta R.T.: 0.015 min
Response: 3279159
Conc: 1.87 ng/ml

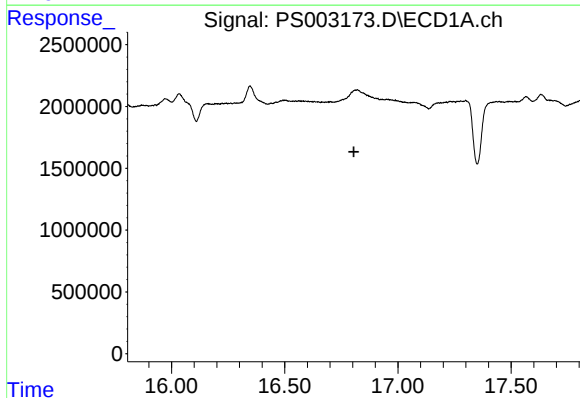


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

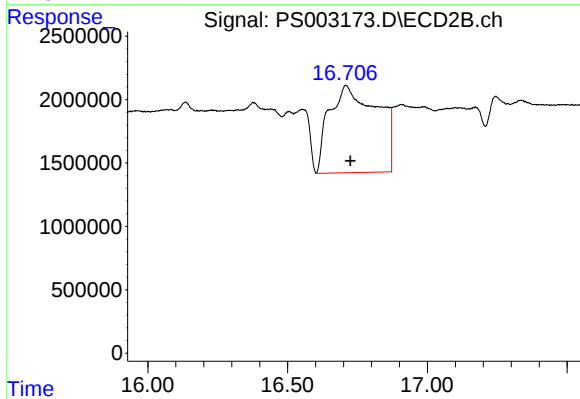

#15 Picloram


R.T.: 16.708 min
Delta R.T.: -0.016 min
Response: 82062283
Conc: 27.30 ng/ml

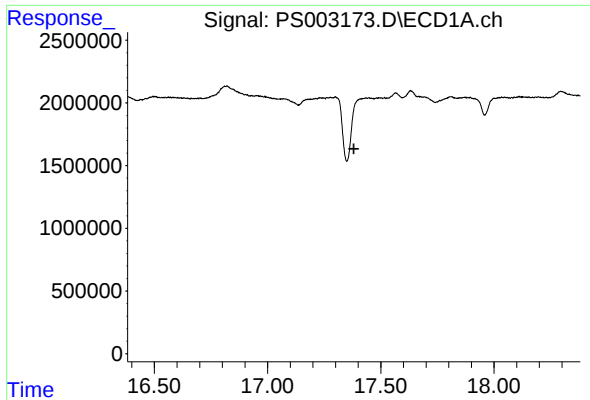

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

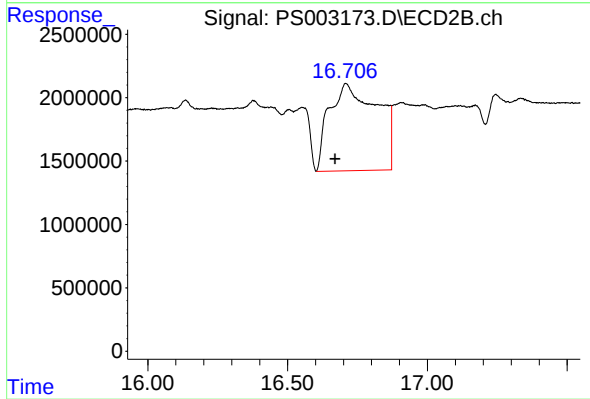

#16 DCPA

R.T.: 16.708 min
Delta R.T.: 0.038 min
Response: 82062283
Conc: 26.49 ng/ml