

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 02:07
 Operator : EI\SJ
 Sample : PB117093BS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 03:44:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.777	65204404	256.2E6	171.753	599.258 #
Target Compounds							
1) T	Dalapon	2.842	2.315	134.1E6	282.3E6	243.019	526.838 #
3) T	4-Nitroph...	0.000	9.927	0	113.0E6	N.D.	540.704 #
8) T	DICHLORPROP	0.000	12.182	0	258.6E6	N.D.	676.274 #
9) T	2,4-D	0.000	12.654	0	194.0E6	N.D.	386.845 #
11) T	2,4,5-TP ...	14.376	13.815	1613.3E6	1621.1E6	640.631	653.595
12) T	2,4,5-T	14.775	14.447	1521.4E6	-3193400	623.681	N.D. #
14) T	DINOSEB	16.990	0.000	1049.3E6	0	557.766	N.D. #
15) T	Picloram	16.765	16.685	1672.7E6	1557.9E6	528.743	518.193
16) T	DCPA	0.000	16.685	0	1557.9E6	N.D.	502.939 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 02:07
Operator : EI\SJ
Sample : PB117093BS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 03:44:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

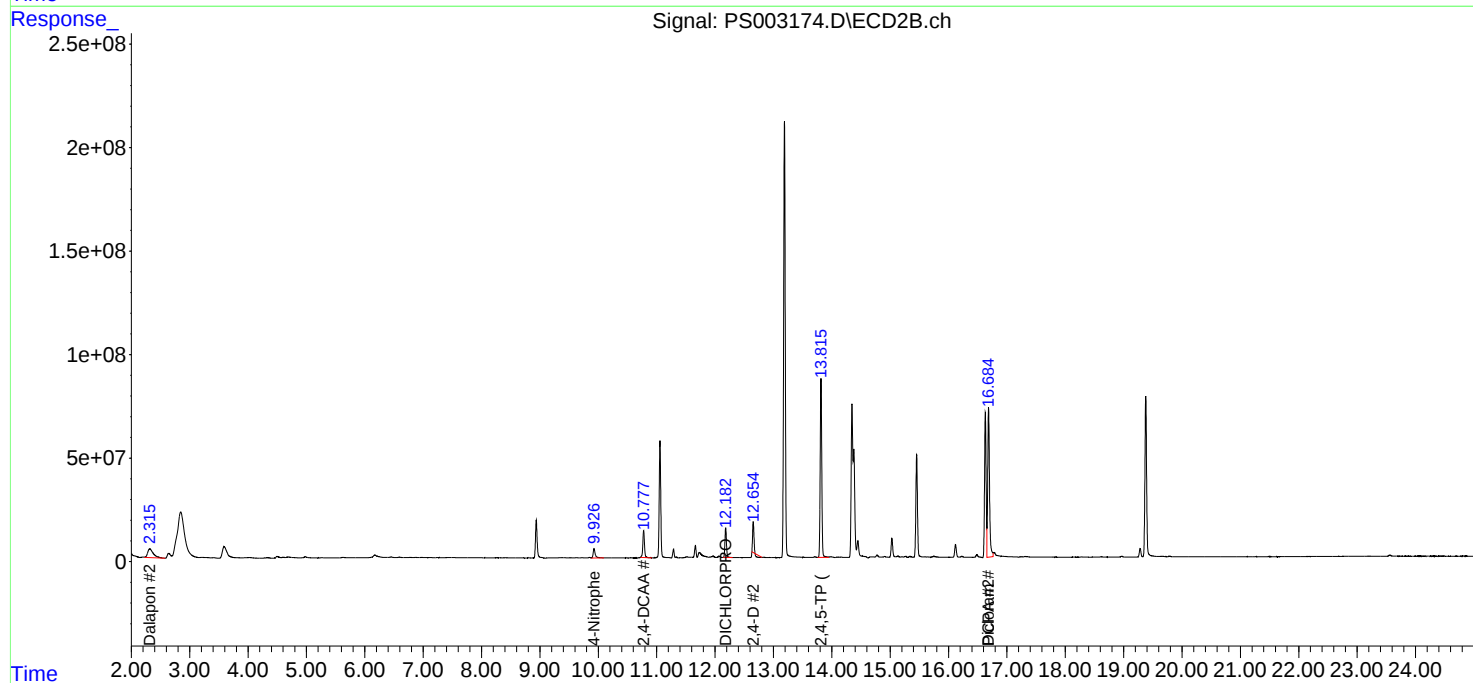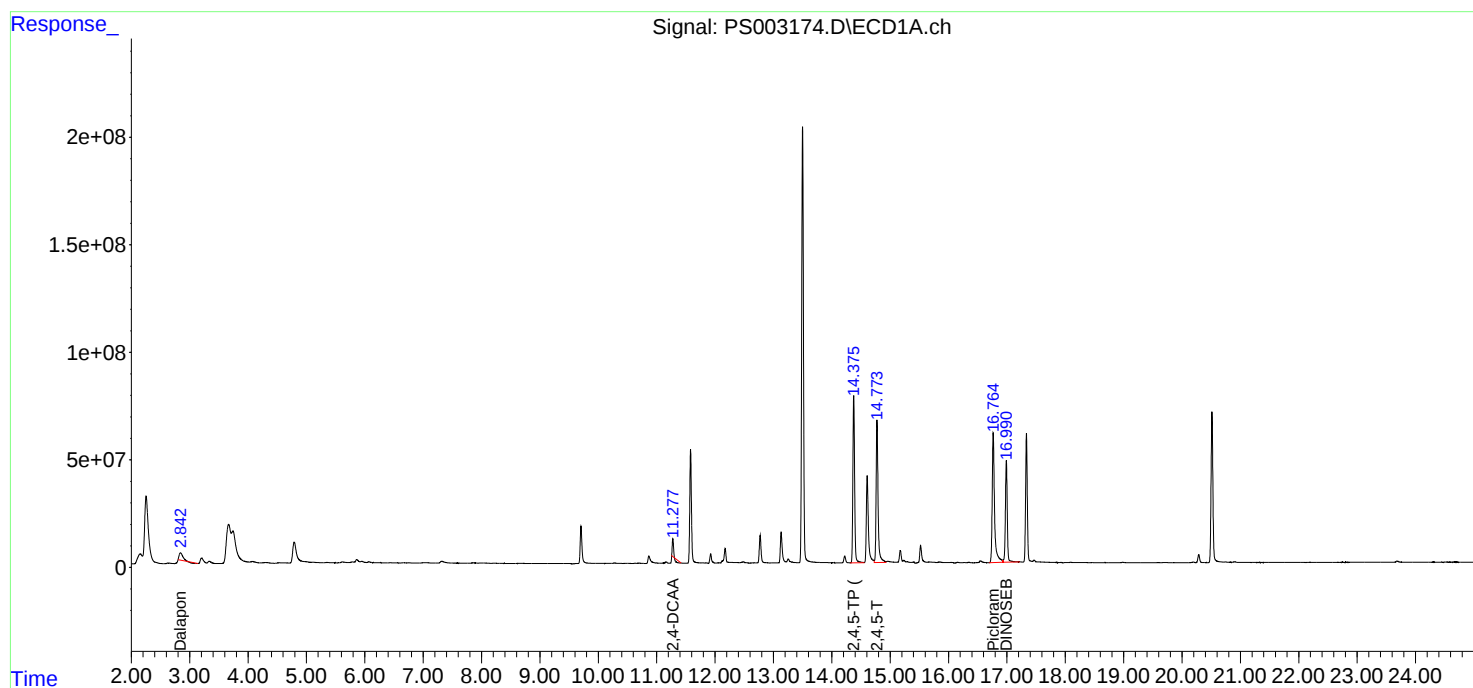


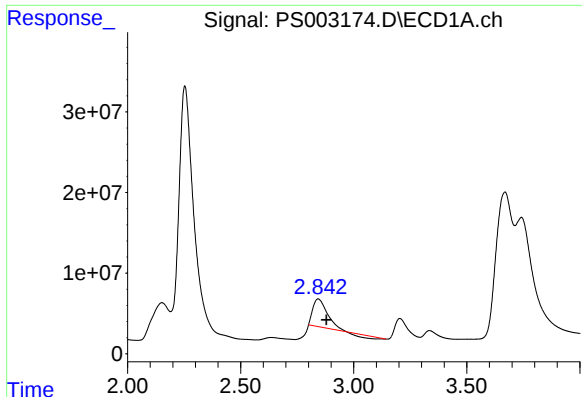

#1 Dalapon


R.T.: 2.842 min
Delta R.T.: -0.038 min
Response: 134060879
Conc: 243.02 ng/ml

Instrument :
ECD_P
ClientSampleId :

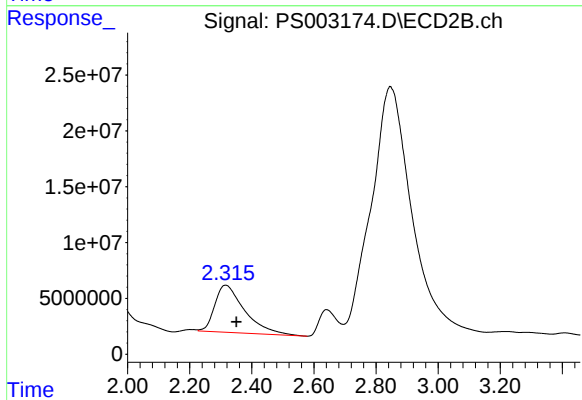


#1 Dalapon

R.T.: 2.315 min
Delta R.T.: -0.035 min
Response: 282343687
Conc: 526.84 ng/ml

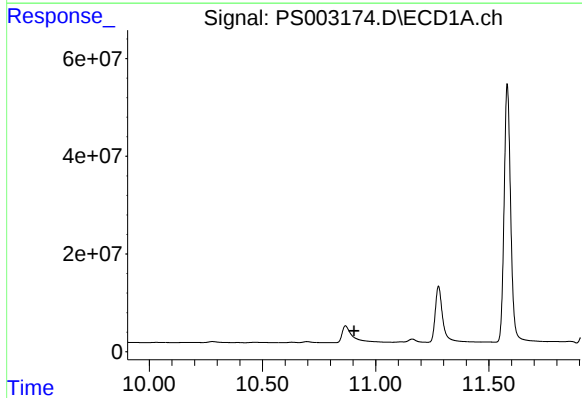


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

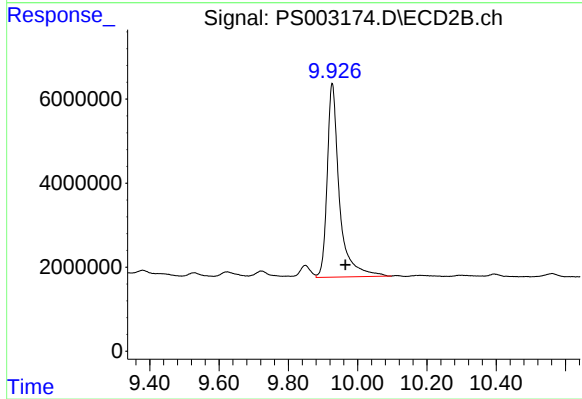

#3 4-Nitrophenol


R.T.: 9.927 min
Delta R.T.: -0.039 min
Response: 113019279
Conc: 540.70 ng/ml

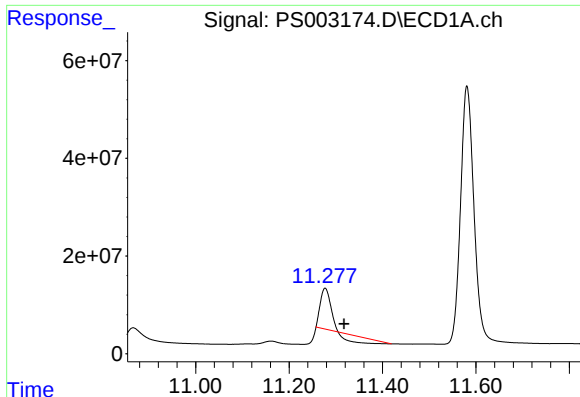

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: -0.041 min
Response: 65204404
Conc: 171.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

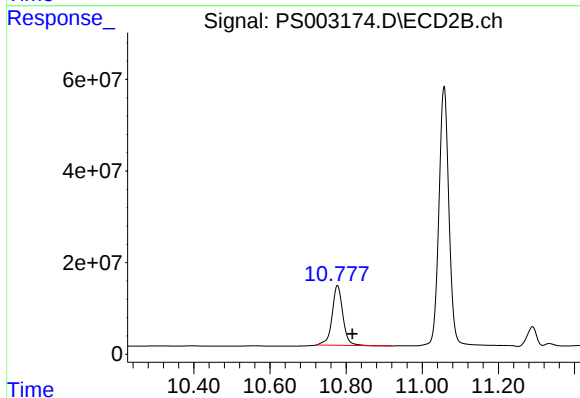


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.039 min
Response: 256210290
Conc: 599.26 ng/ml

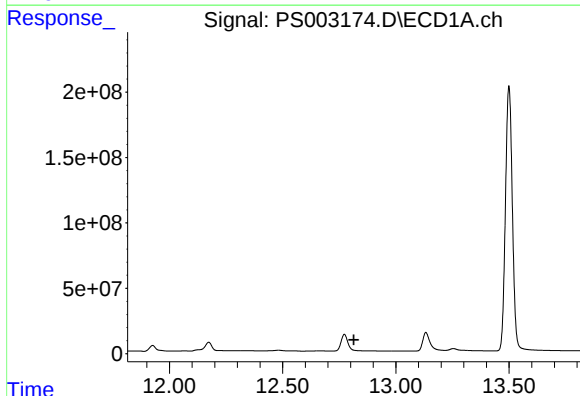


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

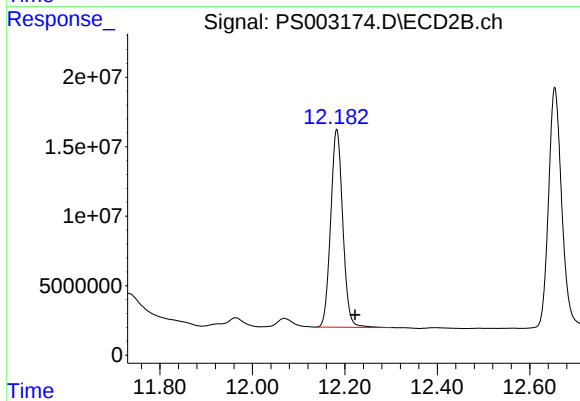

#8 DICHLORPROP


R.T.: 12.182 min
Delta R.T.: -0.040 min
Response: 258567498
Conc: 676.27 ng/ml

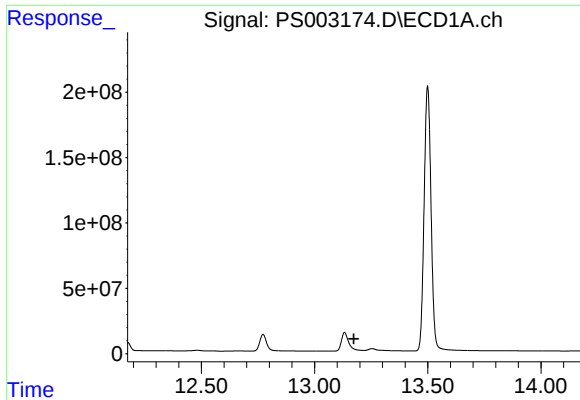

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

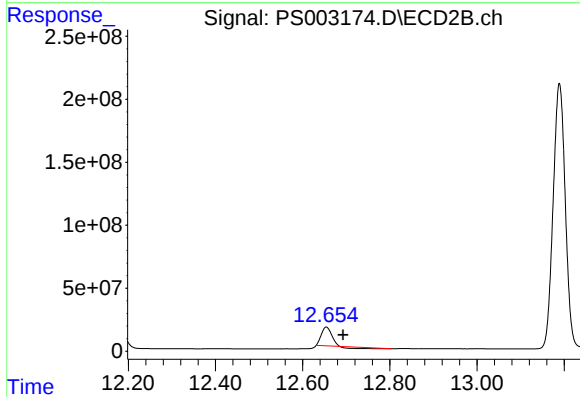


#9 2,4-D

R.T.: 12.654 min
Delta R.T.: -0.039 min
Response: 193958660
Conc: 386.85 ng/ml

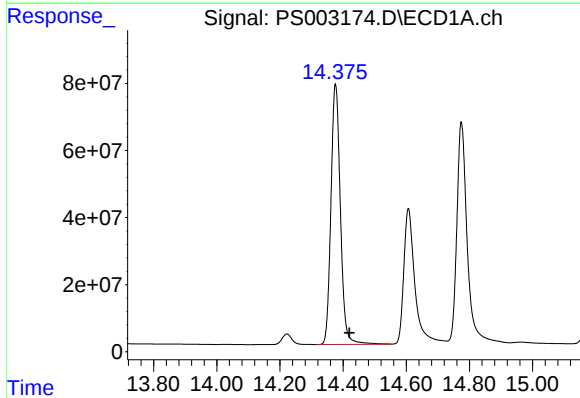


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.044 min
Response: 1613347444
Conc: 640.63 ng/ml

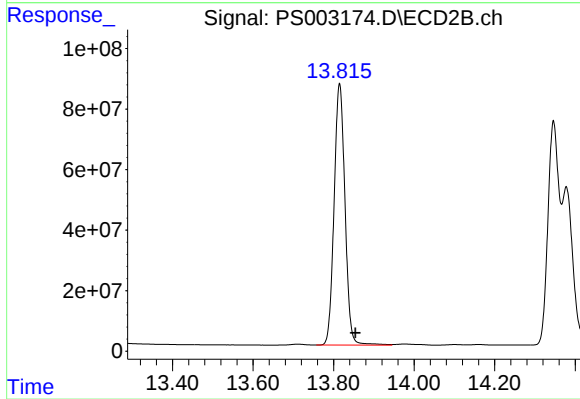

#11 2,4,5-TP (SILVEX)


R.T.: 13.815 min
Delta R.T.: -0.039 min
Response: 1621148287
Conc: 653.60 ng/ml

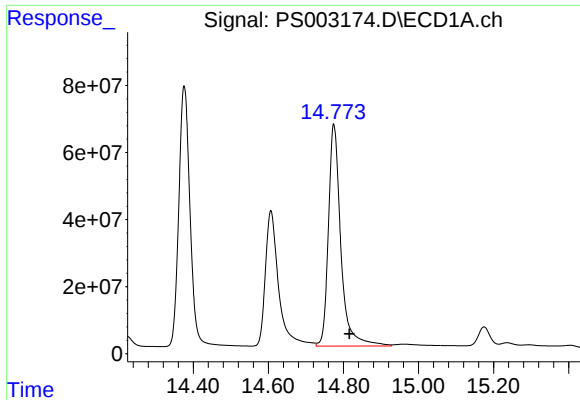

#12 2,4,5-T


R.T.: 14.775 min
Delta R.T.: -0.042 min
Response: 1521409986
Conc: 623.68 ng/ml

Instrument :
ECD_P
ClientSampleId :

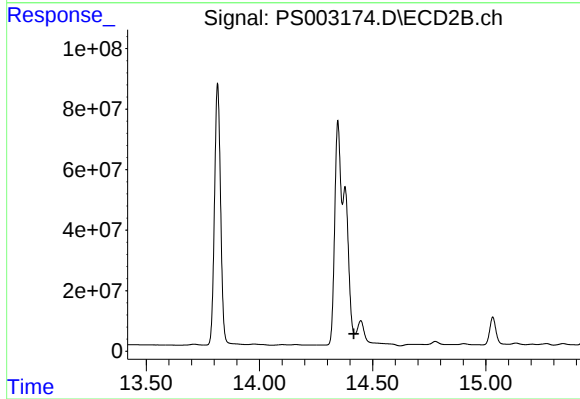


#12 2,4,5-T

R.T.: 14.447 min
Delta R.T.: 0.030 min
Response: -3193400
Conc: N.D.

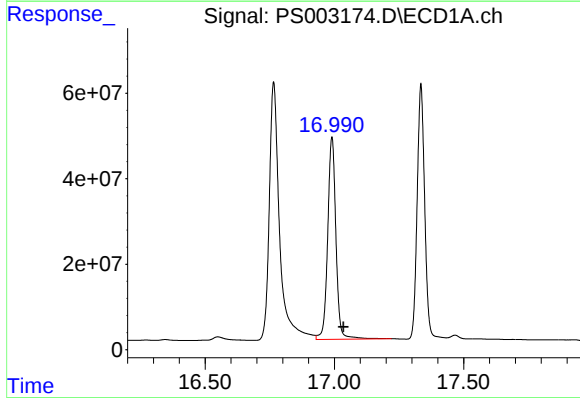


#14 DINOSEB

R.T.: 16.990 min
Delta R.T.: -0.045 min
Response: 1049340108
Conc: 557.77 ng/ml

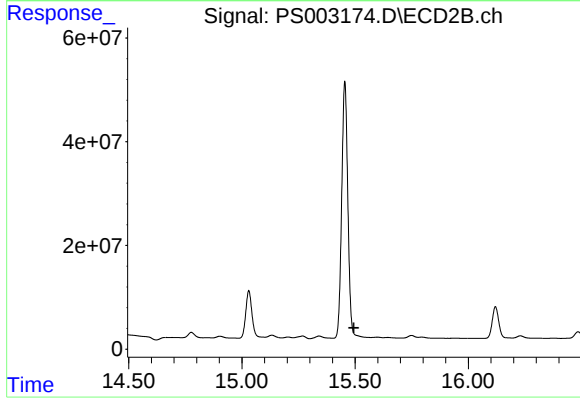

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

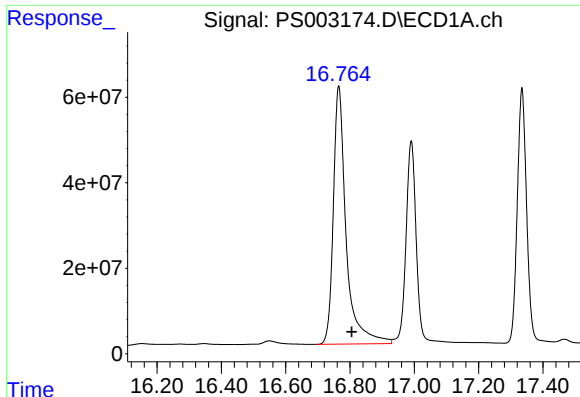

#15 Picloram


R.T.: 16.765 min
Delta R.T.: -0.041 min
Response: 1672747004
Conc: 528.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

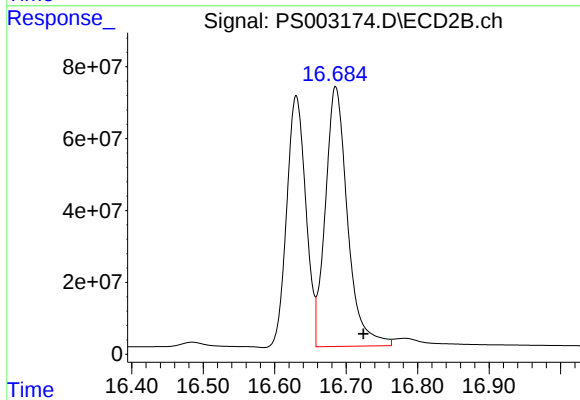


#15 Picloram

R.T.: 16.685 min
Delta R.T.: -0.039 min
Response: 1557897290
Conc: 518.19 ng/ml

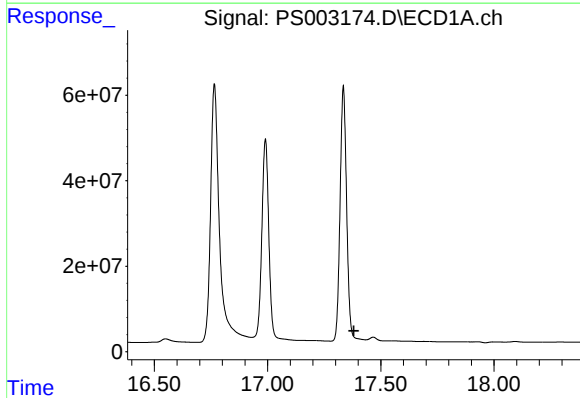

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

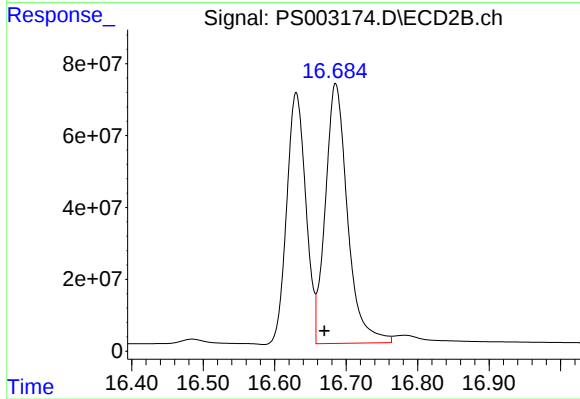

#16 DCPA

R.T.: 16.685 min
Delta R.T.: 0.016 min
Response: 1557897290
Conc: 502.94 ng/ml