

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
 Data File : PS003175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2019 02:38
 Operator : EI\SJ
 Sample : PB117093TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 03:44:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.298	10.798	122.9E6	124.2E6	323.760	290.389
Target Compounds							
1) T	Dalapon	2.865	0.000	77597865	0	140.666	N.D. #
5) T	DICAMBA	0.000	11.159	0	4035261	N.D.	2.543 #
6) T	MCPD	11.977	0.000	7615231	0	6.356	N.D. #
9) T	2,4-D	13.206	0.000	3431259	0	7.442	N.D. #
12) T	2,4,5-T	0.000	14.410	0	4820469	N.D.	2.519 #
15) T	Picloram	16.812	16.718	4326482	21121280	1.368	7.025 #
16) T	DCPA	0.000	16.718	0	21121280	N.D.	6.819 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS021319\
Data File : PS003175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2019 02:38
Operator : EI\SJ
Sample : PB117093TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 03:44:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

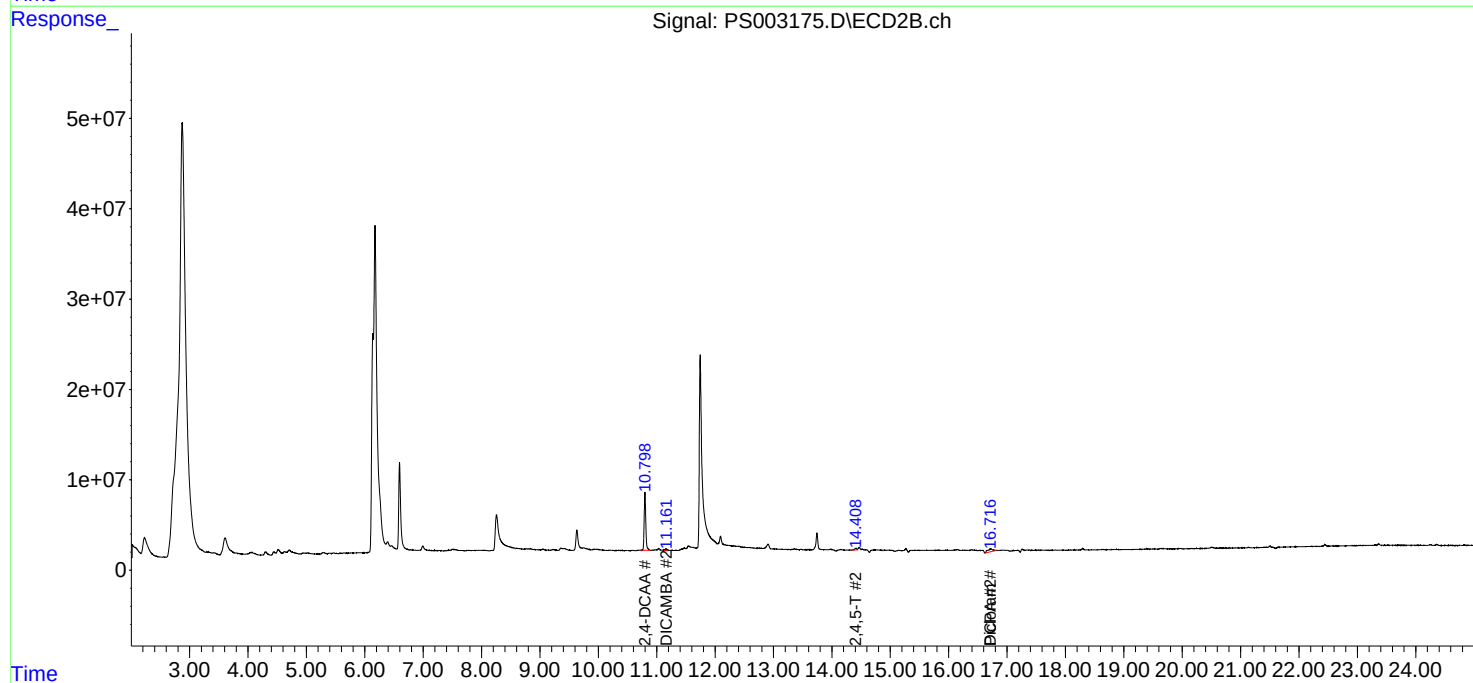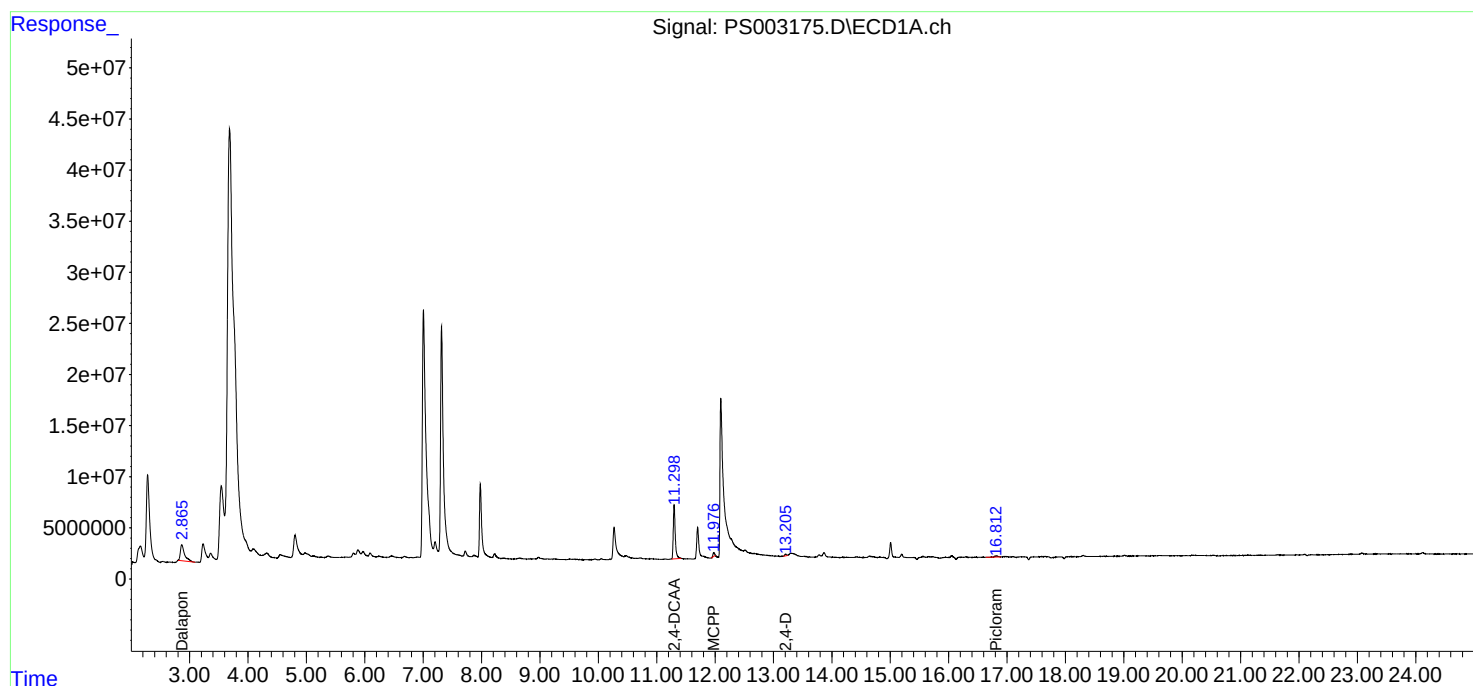


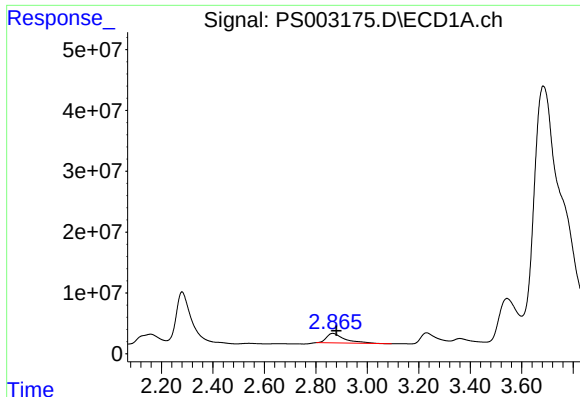

#1 Dalapon


R.T.: 2.865 min
Delta R.T.: -0.015 min
Response: 77597865
Conc: 140.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

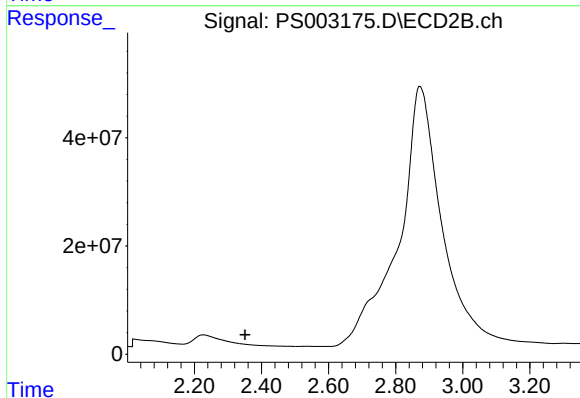


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.351 min
Response: 0
Conc: N.D.

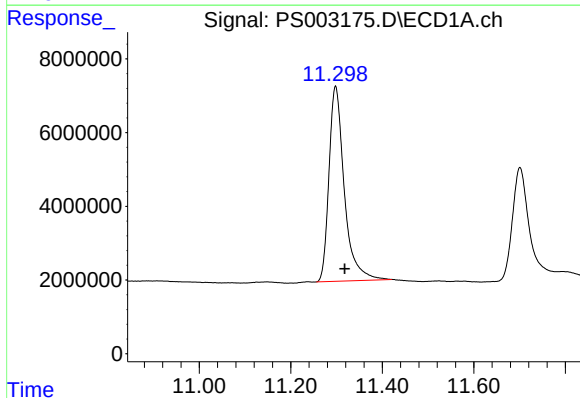


#4 2,4-DCAA

R.T.: 11.298 min
Delta R.T.: -0.020 min
Response: 122912682
Conc: 323.76 ng/ml

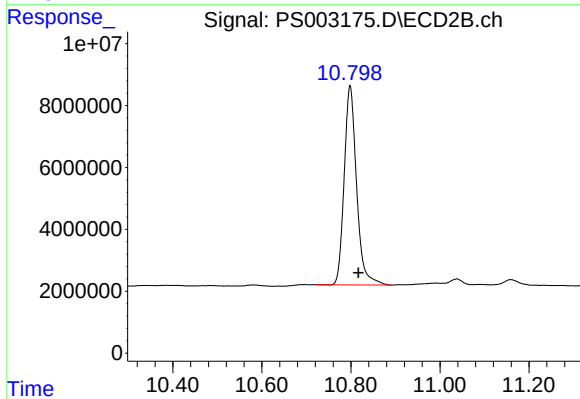

#4 2,4-DCAA


R.T.: 10.798 min
Delta R.T.: -0.018 min
Response: 124154684
Conc: 290.39 ng/ml

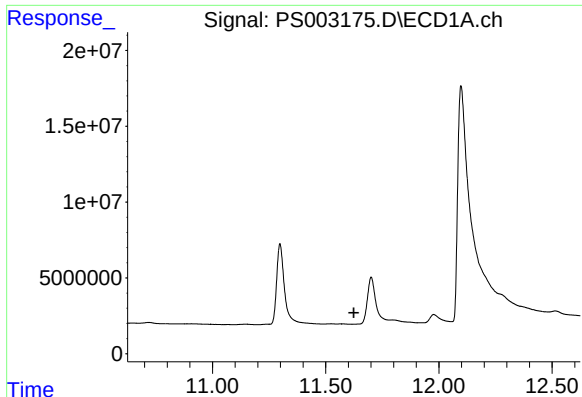

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

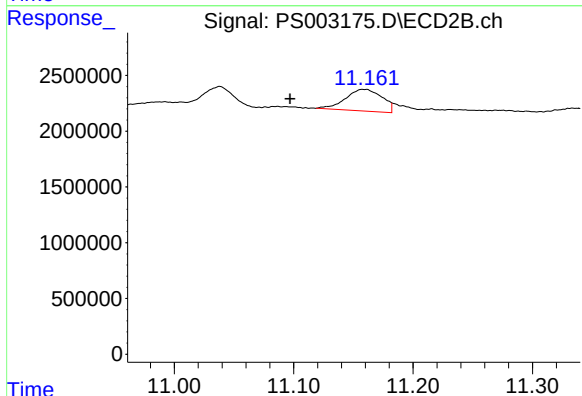


#5 DICAMBA

R.T.: 11.159 min
Delta R.T.: 0.062 min
Response: 4035261
Conc: 2.54 ng/ml

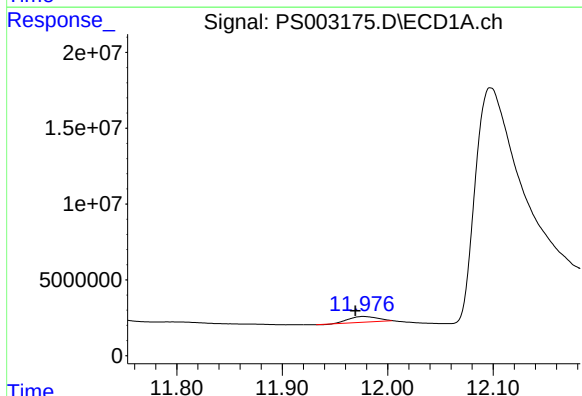


#6 MCP

R.T.: 11.977 min
Delta R.T.: 0.008 min
Response: 7615231
Conc: 6.36 ug/ml

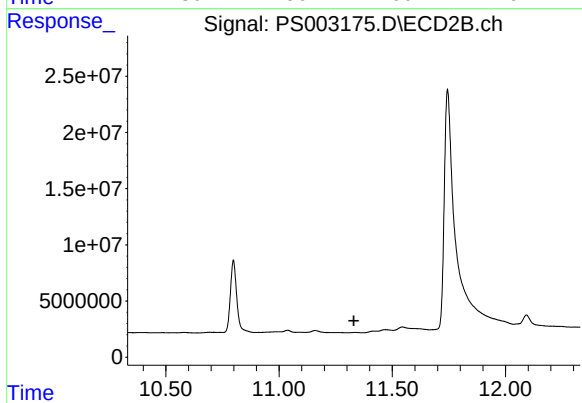

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

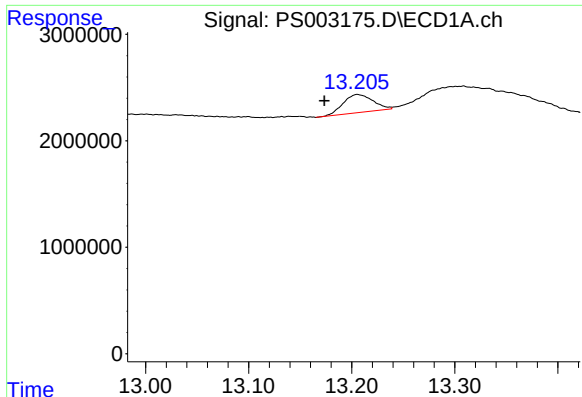

#9 2,4-D


R.T.: 13.206 min
Delta R.T.: 0.033 min
Response: 3431259
Conc: 7.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

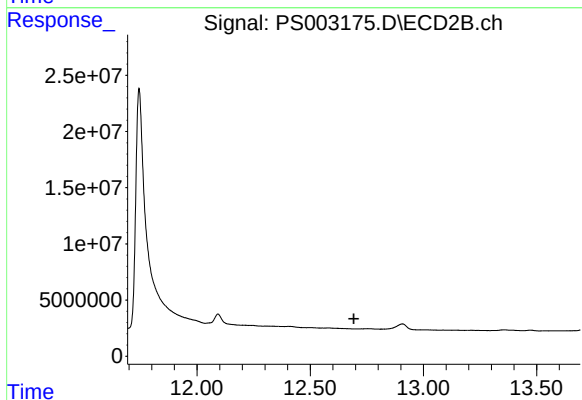


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

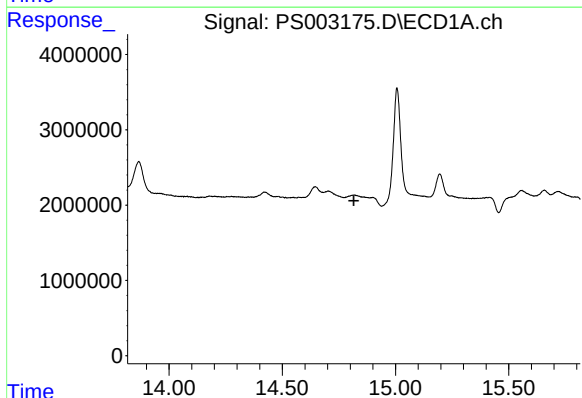


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

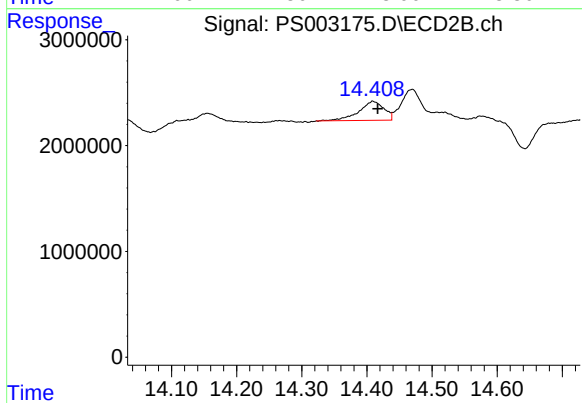

#12 2,4,5-T


R.T.: 14.410 min
Delta R.T.: -0.007 min
Response: 4820469
Conc: 2.52 ng/ml

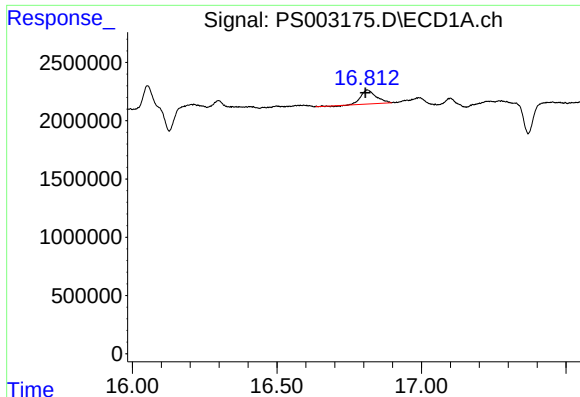

#15 Picloram


R.T.: 16.812 min
Delta R.T.: 0.007 min
Response: 4326482
Conc: 1.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

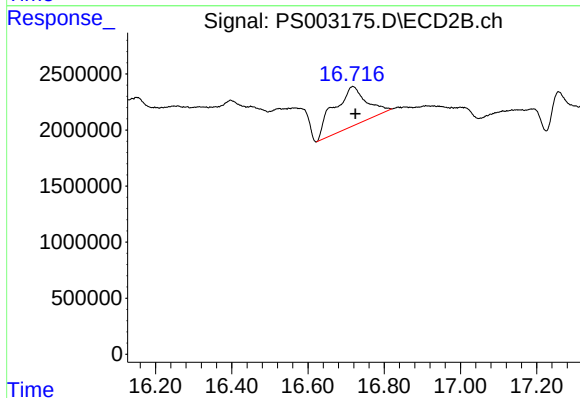


#15 Picloram

R.T.: 16.718 min
Delta R.T.: -0.007 min
Response: 21121280
Conc: 7.03 ng/ml

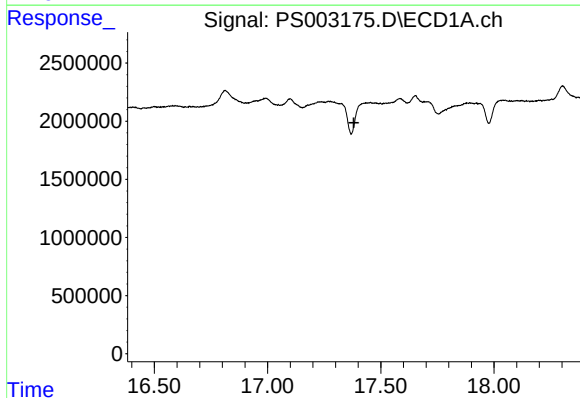

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

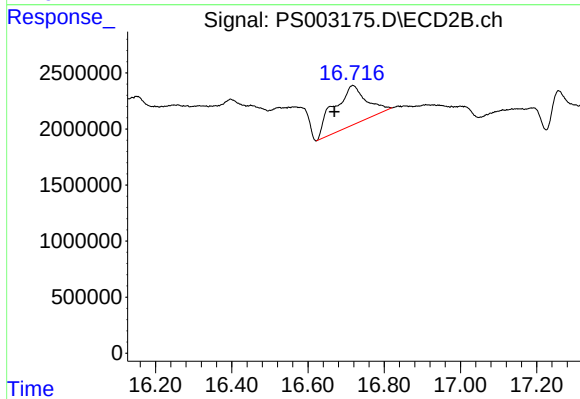

#16 DCPA

R.T.: 16.718 min
Delta R.T.: 0.048 min
Response: 21121280
Conc: 6.82 ng/ml