

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
 Data File : PP055583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2023 18:16
 Operator : YP\AJ
 Sample : 01526-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PL-01-021023

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
 Supervised By :Sohil Jodhani 02/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 20:24:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.329	3.576	29510340	28760377	16.972m	19.158
2) SA Decachlor...	10.089	8.588	35957452	27021241	20.765	20.007

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
Data File : PP055583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2023 18:16
Operator : YP\AJ
Sample : 01526-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PL-01-021023


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
Supervised By :Sohil Jodhani 02/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 20:24:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

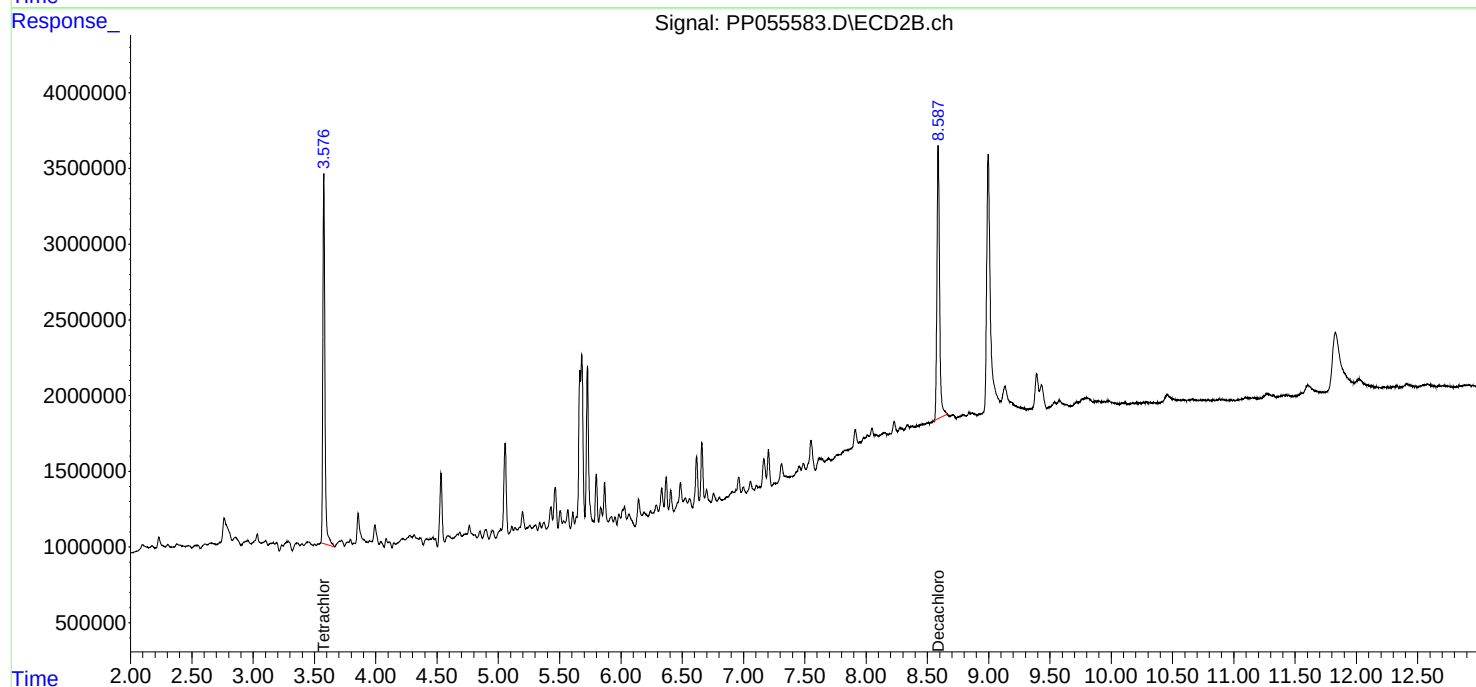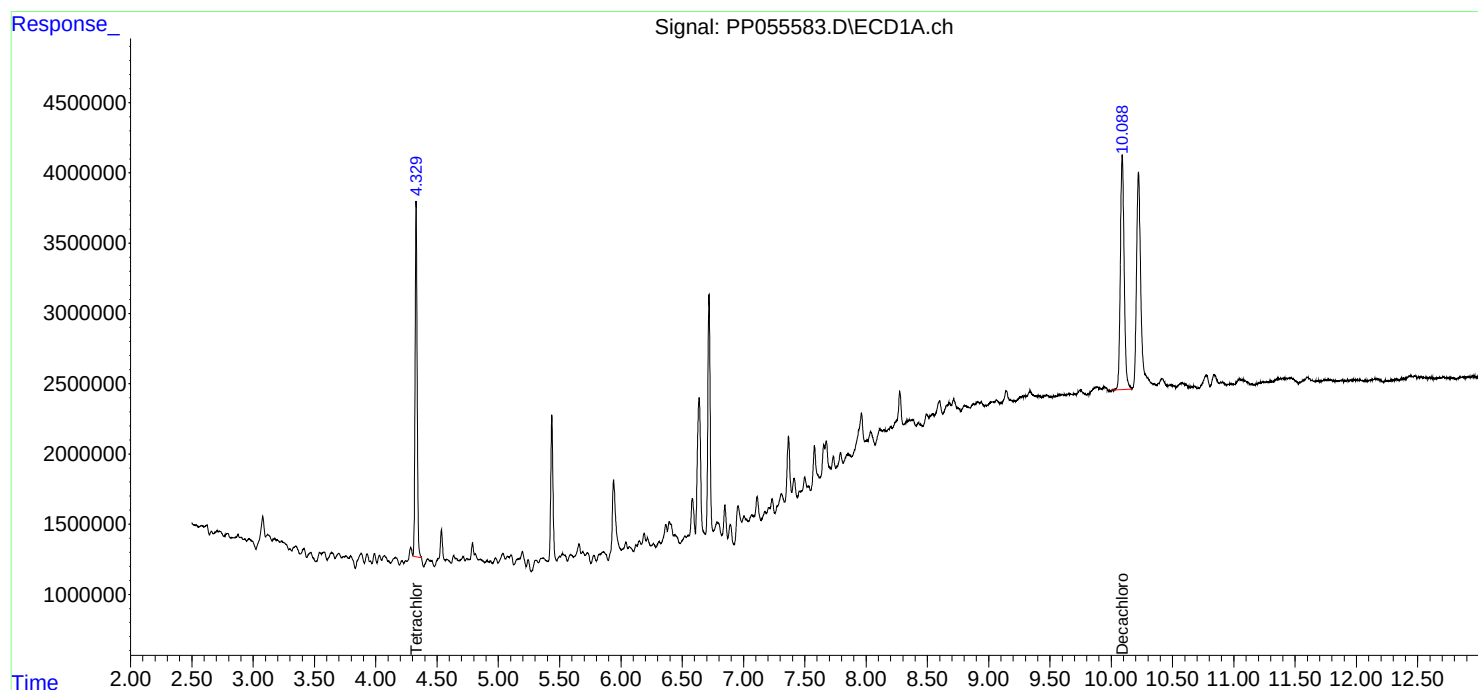

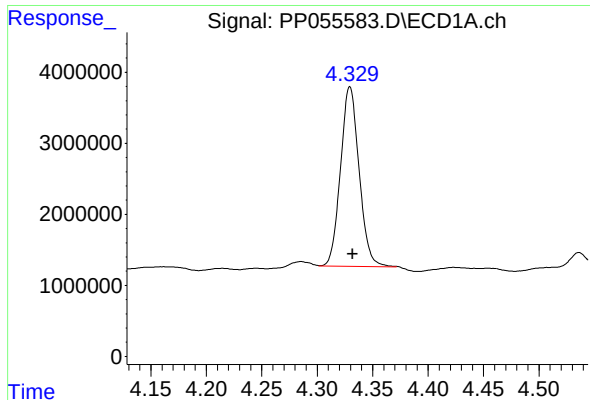

#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: -0.003 min
Response: 29510340
Conc: 16.97 ng/ml

Instrument :


ECD_P

ClientSampleId :

PL-01-021023


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
Supervised By :Sohil Jodhani 02/15/2023

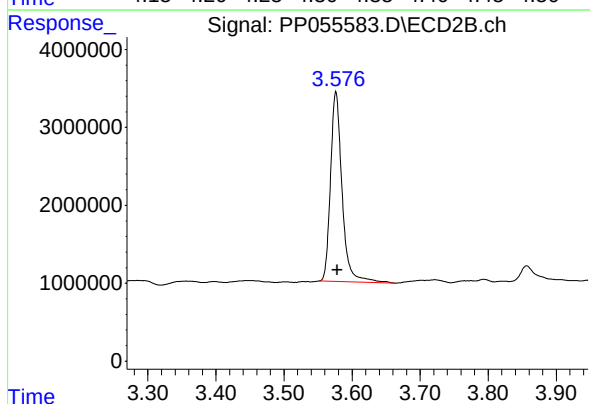


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.002 min
Response: 28760377
Conc: 19.16 ng/ml

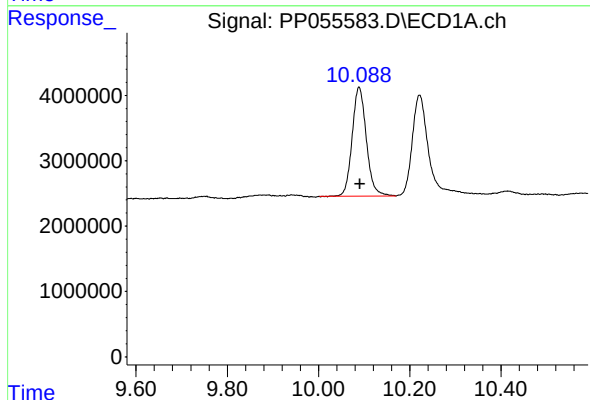

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.002 min
Response: 35957452
Conc: 20.76 ng/ml

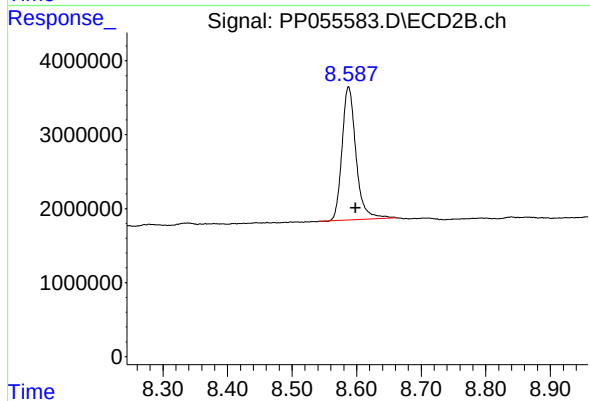

#2 Decachlorobiphenyl

R.T.: 8.588 min
Delta R.T.: -0.011 min
Response: 27021241
Conc: 20.01 ng/ml