

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
 Data File : PP055602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 00:00
 Operator : YP\AJ
 Sample : 01540-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-020723-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 04:07:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.575	30557768	20775659	17.575	13.839
2) SA Decachlor...	10.084	8.588	25203386	33579572	14.554	24.863 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
Data File : PP055602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 00:00
Operator : YP\AJ
Sample : 01540-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-020723-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 04:07:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

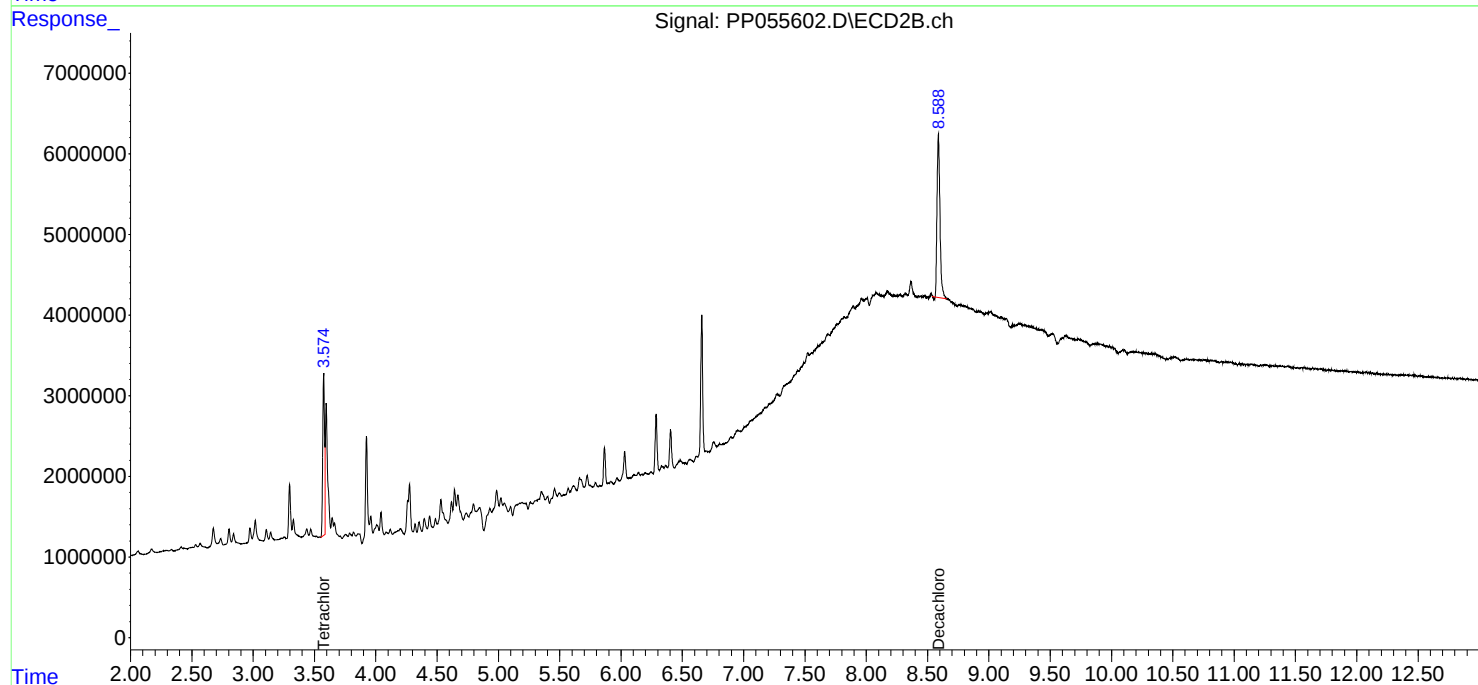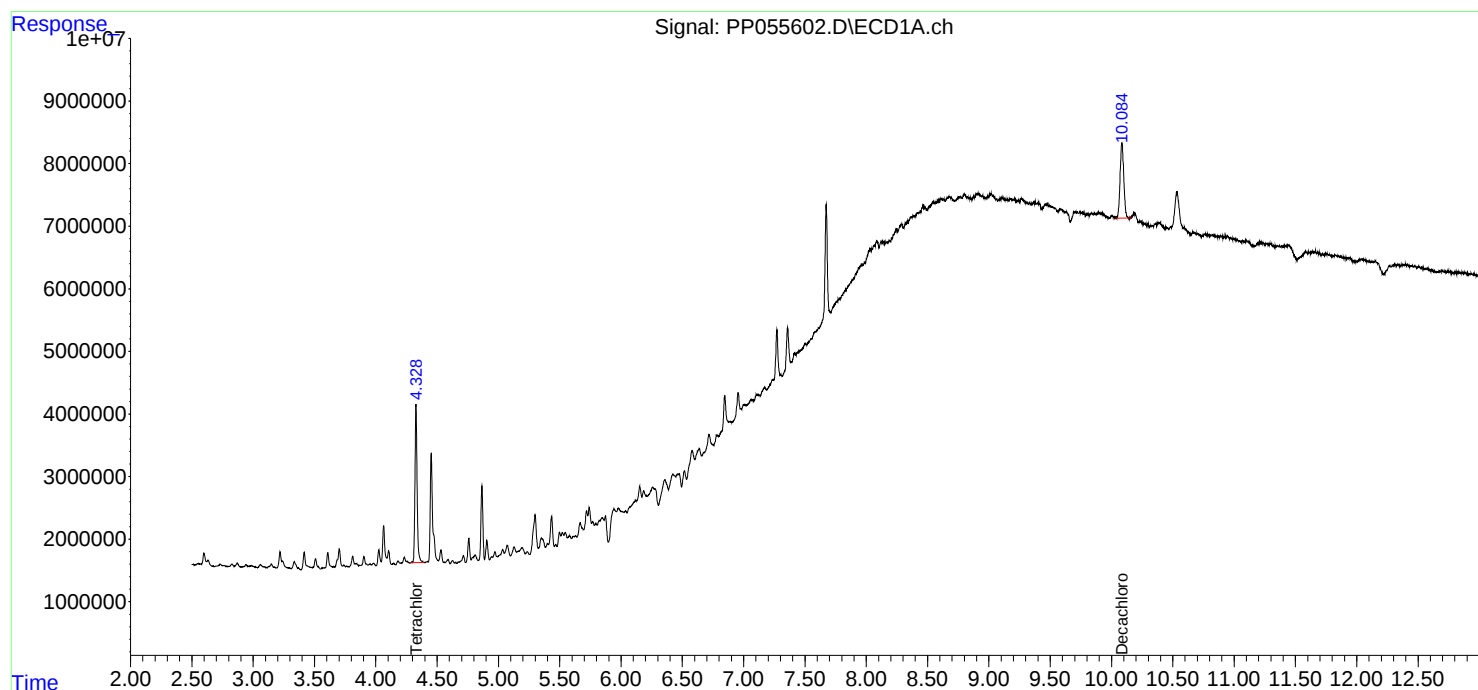


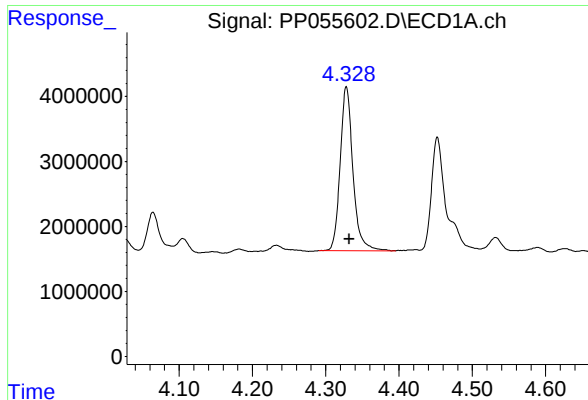

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: -0.004 min
Response: 30557768
Conc: 17.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-020723-03

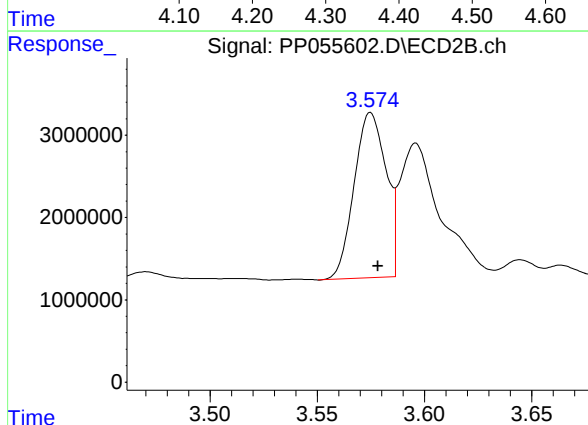


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: -0.003 min
Response: 20775659
Conc: 13.84 ng/ml

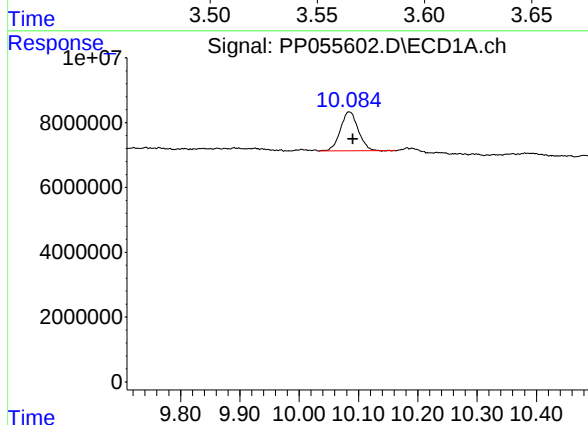

#2 Decachlorobiphenyl

R.T.: 10.084 min
Delta R.T.: -0.007 min
Response: 25203386
Conc: 14.55 ng/ml

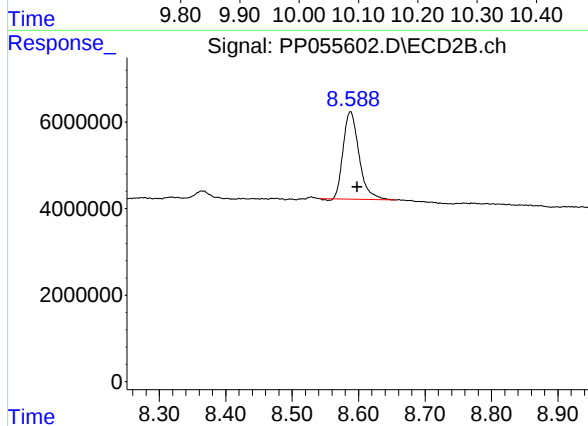

#2 Decachlorobiphenyl

R.T.: 8.588 min
Delta R.T.: -0.010 min
Response: 33579572
Conc: 24.86 ng/ml