

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
 Data File : PP055606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Feb 2023 01:05
 Operator : YP\AJ
 Sample : 01540-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-020723-07

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
 Supervised By :Sohil Jodhani 02/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 04:08:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 03:37:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.328	3.574	33176196	28977108	19.081	19.302
2) SA Decachlor...	10.083	8.583	26052503	24119094	15.045m	17.859

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021323\
Data File : PP055606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2023 01:05
Operator : YP\AJ
Sample : 01540-07
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-020723-07


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
Supervised By :Sohil Jodhani 02/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 04:08:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012423.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 03:37:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

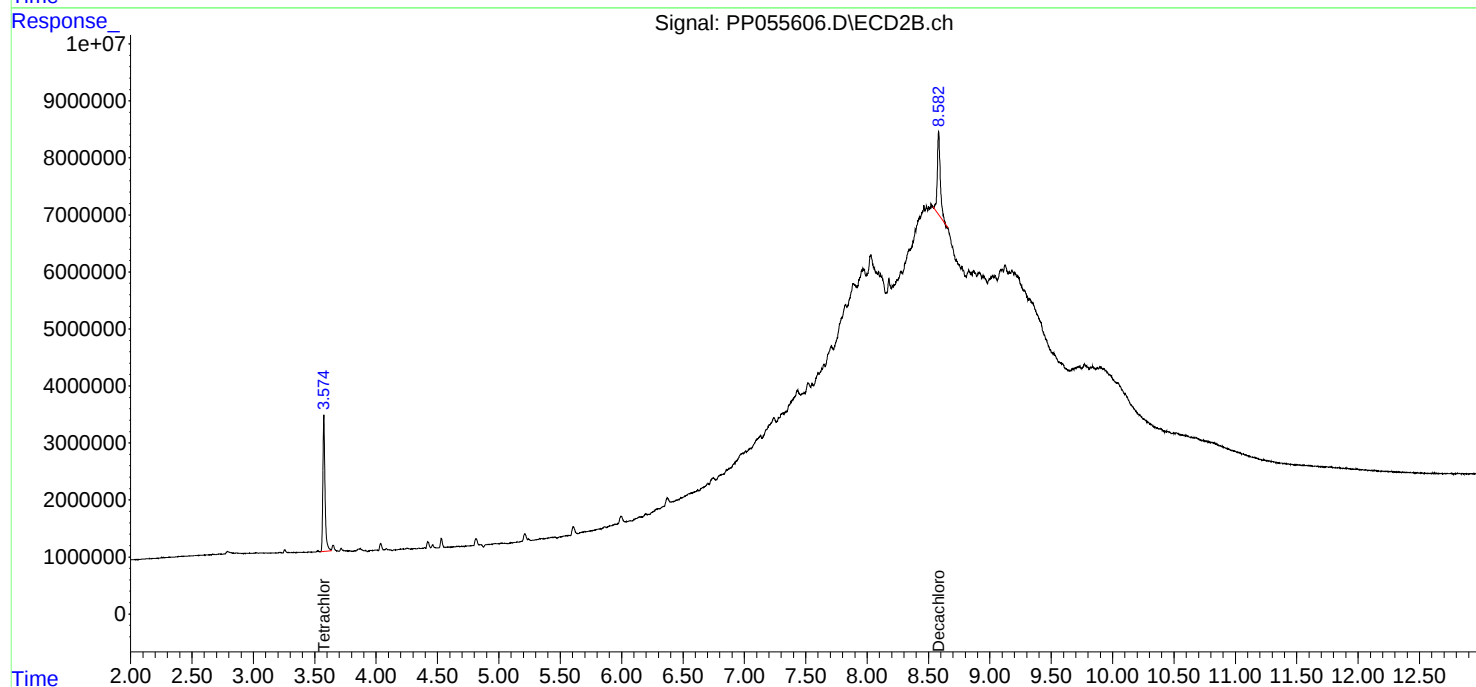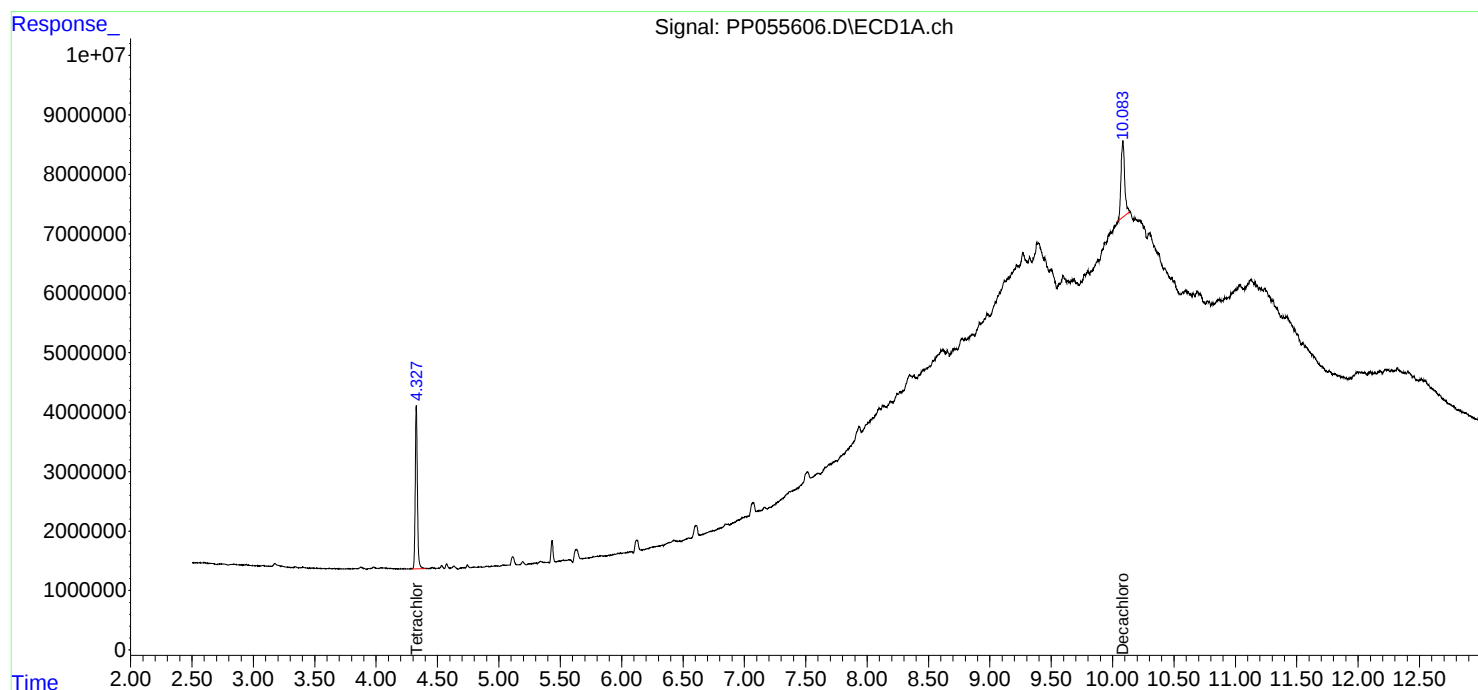

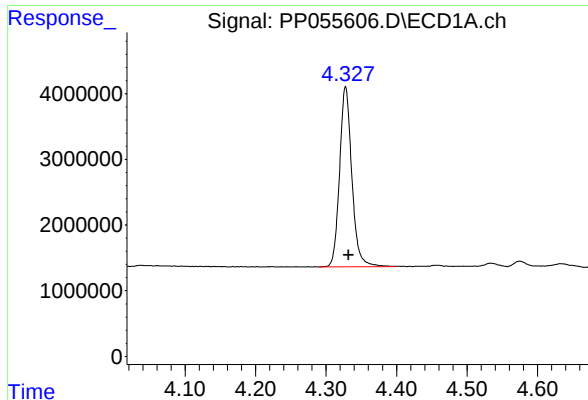


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.004 min
Response: 33176196
Conc: 19.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-020723-07


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/15/2023
Supervised By :Sohil Jodhani 02/15/2023

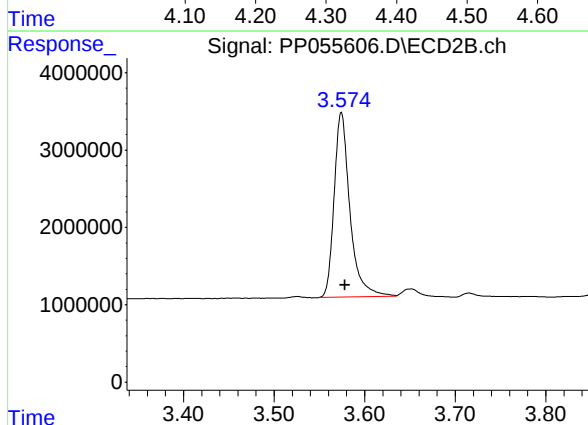


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: -0.004 min
Response: 28977108
Conc: 19.30 ng/ml

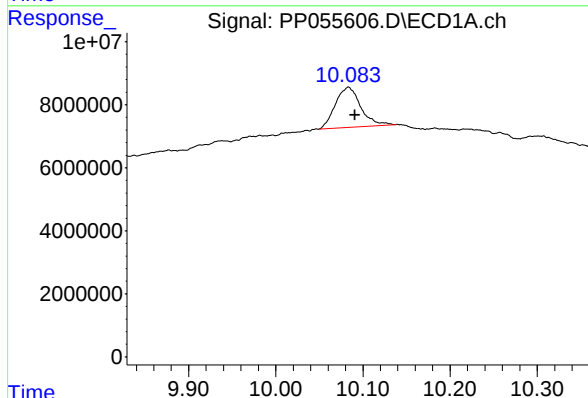

#2 Decachlorobiphenyl

R.T.: 10.083 min
Delta R.T.: -0.008 min
Response: 26052503
Conc: 15.04 ng/ml m

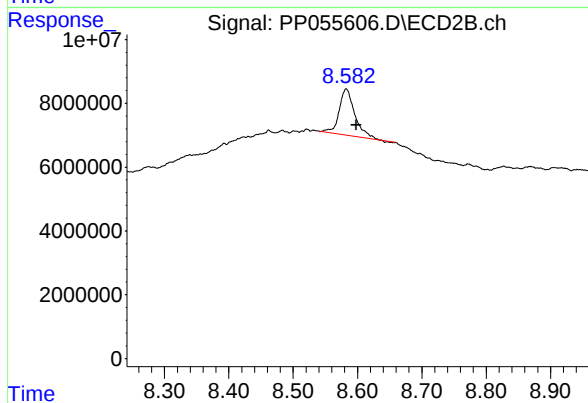

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.016 min
Response: 24119094
Conc: 17.86 ng/ml