

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021422\
Data File : PP043681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2022 14:41
Operator : YP\AJ
Sample : N1511-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20220041-AMENDED-NACOTE-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 00:32:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.919	3.175	46902762	42787242	21.213	22.780
2) SA Decachlor...	10.069	8.552	23783861	32335628	20.022	19.931

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021422\
Data File : PP043681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Feb 2022 14:41
Operator : YP\AJ
Sample : N1511-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20220041-AMENDED-NACOTE-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 00:32:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

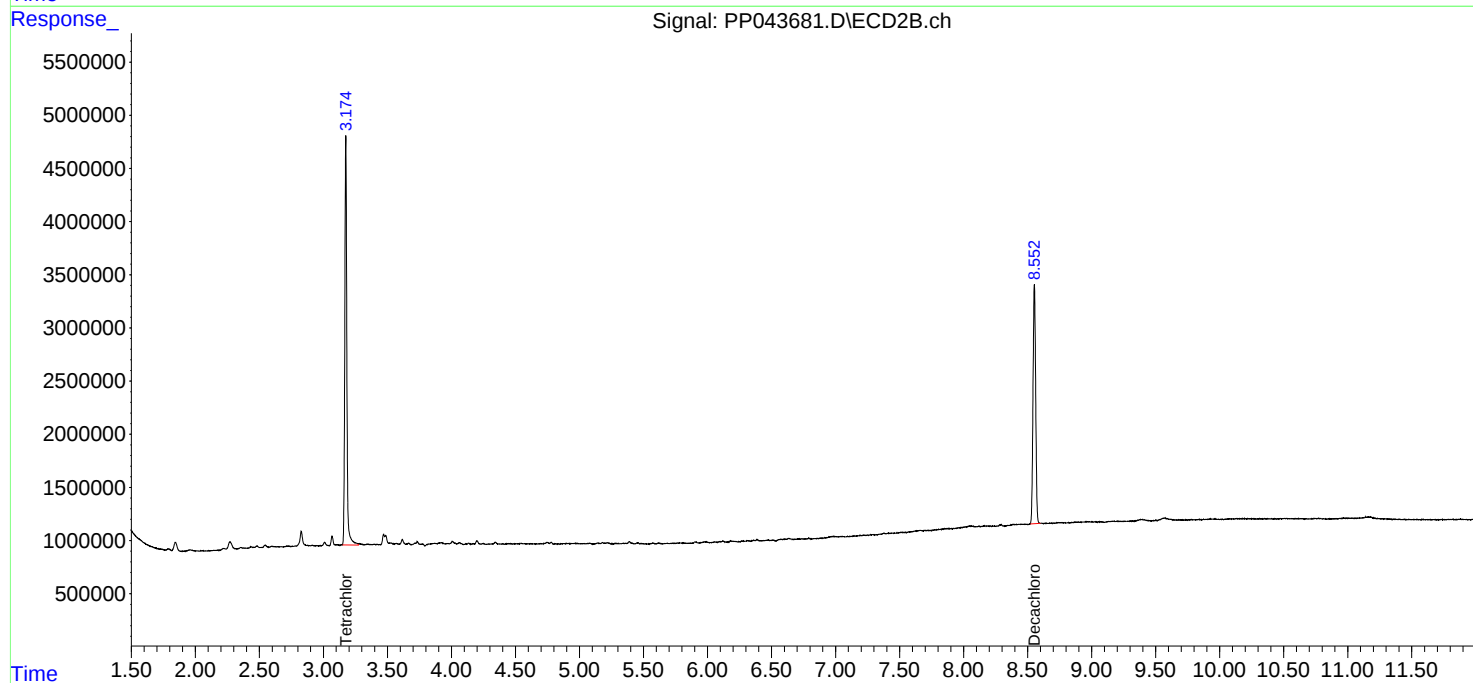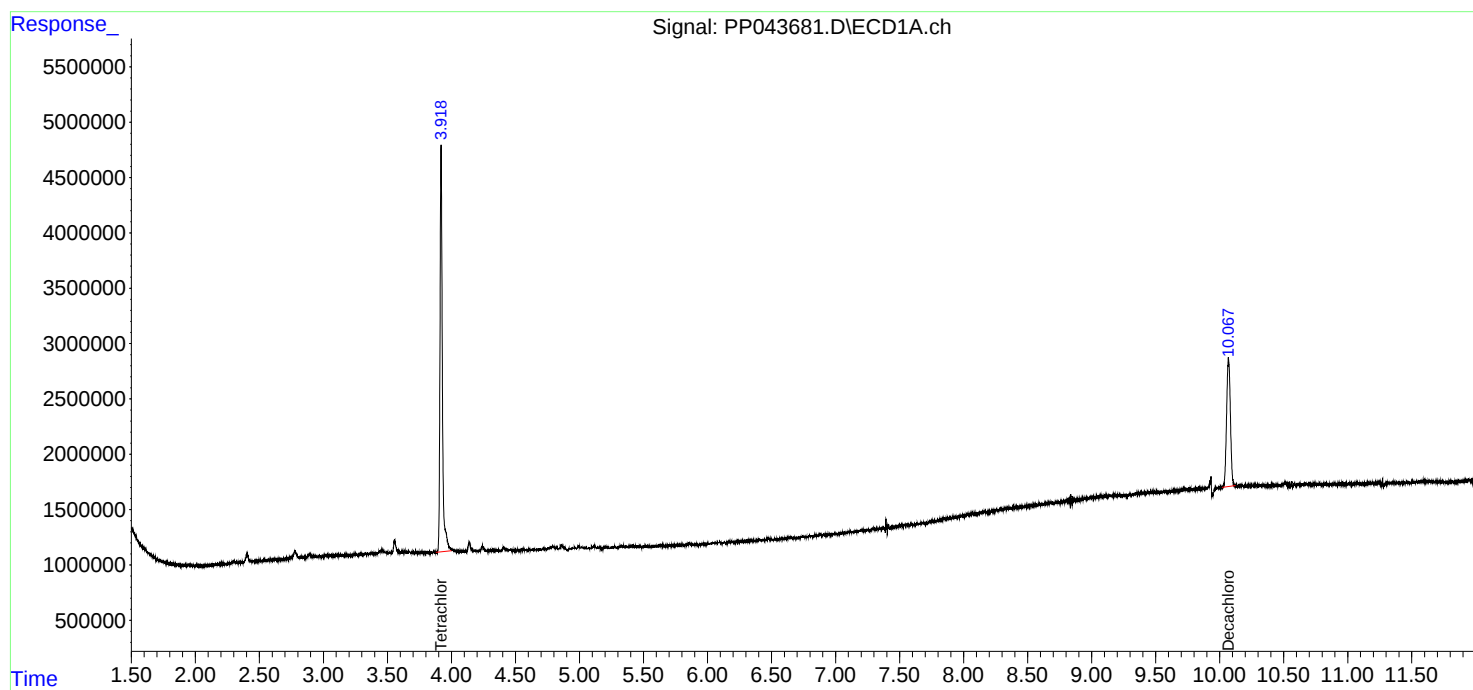


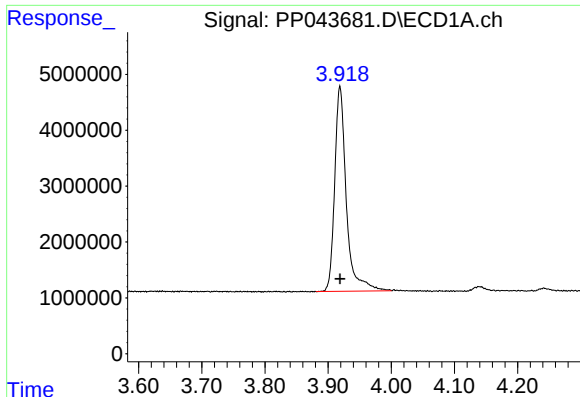

#1 Tetrachloro-m-xylene


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 46902762
Conc: 21.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
20220041-AMENDED-NACOTE-1-COMP

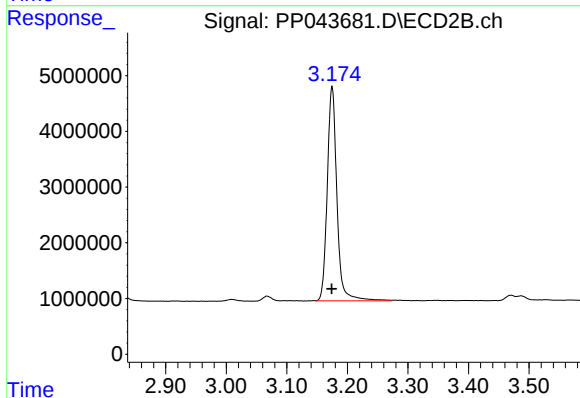


#1 Tetrachloro-m-xylene

R.T.: 3.175 min
Delta R.T.: 0.000 min
Response: 42787242
Conc: 22.78 ng/ml

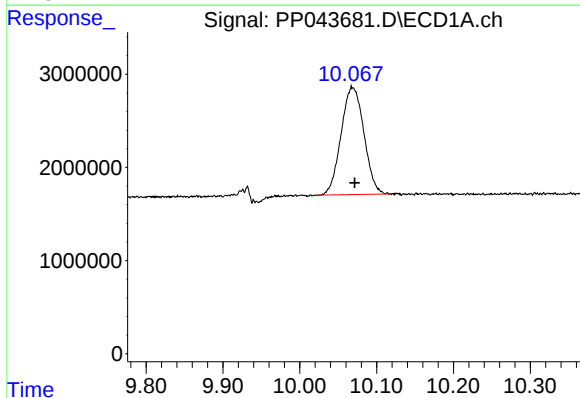

#2 Decachlorobiphenyl

R.T.: 10.069 min
Delta R.T.: -0.003 min
Response: 23783861
Conc: 20.02 ng/ml

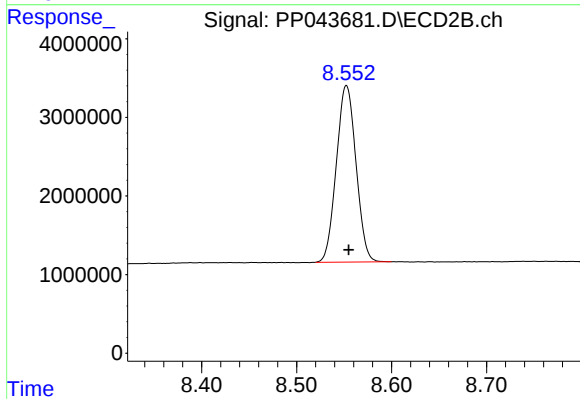

#2 Decachlorobiphenyl

R.T.: 8.552 min
Delta R.T.: -0.002 min
Response: 32335628
Conc: 19.93 ng/ml