

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033346.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 15:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 16:23:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.727	4.000	1391759	882020	22.696	21.570
2) SA Decachlor...	10.544	9.261	1034836	741329	23.756	22.129
Target Compounds						
9) L2 AR-1221-2	5.070	0.000	23765	0	51.086	N.D. #
24) L5 AR-1248-4	6.943f	0.000	33254	0	19.327	N.D. #
26) L6 AR-1254-1	6.943	0.000	33254	0	17.712	N.D. #
28) L6 AR-1254-3	7.547	0.000	38731	0	12.752	N.D. #
29) L6 AR-1254-4	7.834	0.000	25206	0	10.896	N.D. #
30) L6 AR-1254-5	8.263	0.000	21572	0	8.915	N.D. #
35) L7 AR-1260-5	8.898f	0.000	62735	0	11.654	N.D. #
37) L8 AR-1262-2	8.898f	0.000	62735	0	10.020	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033346.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 15:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 16:23:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

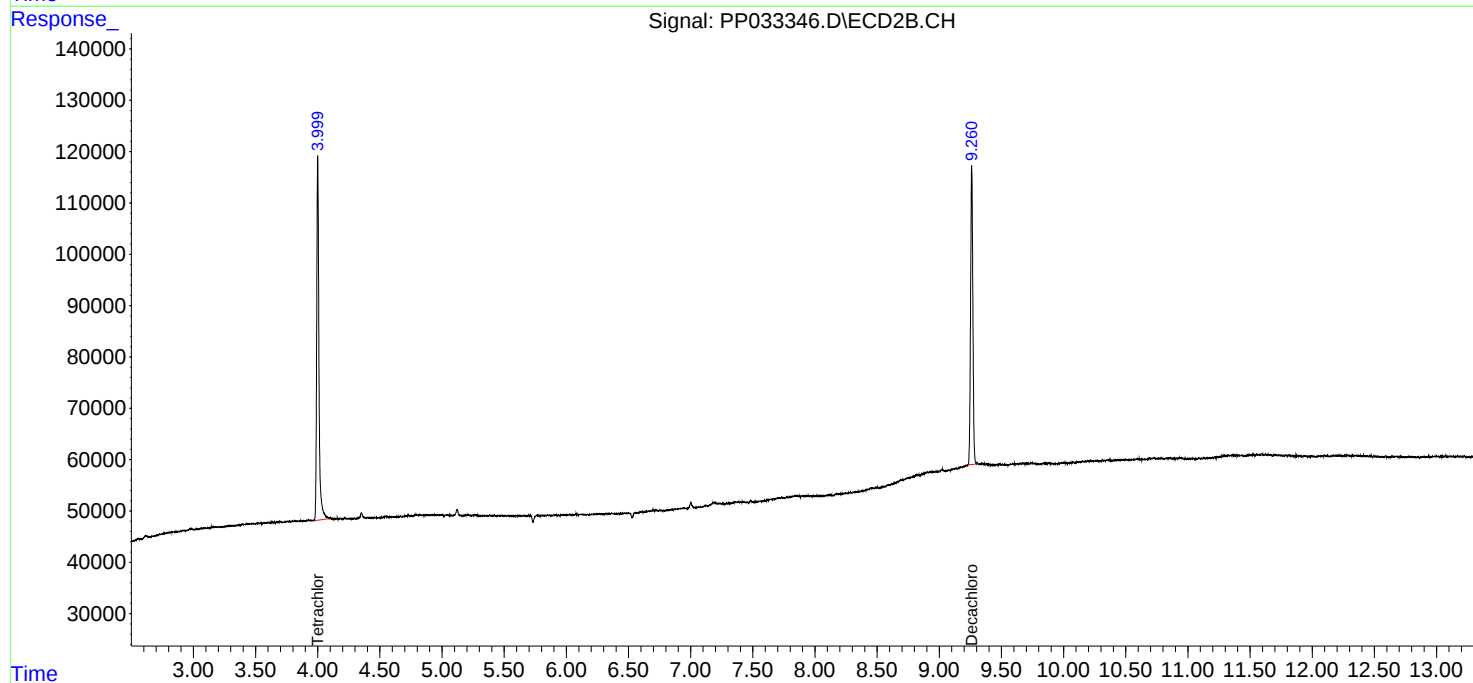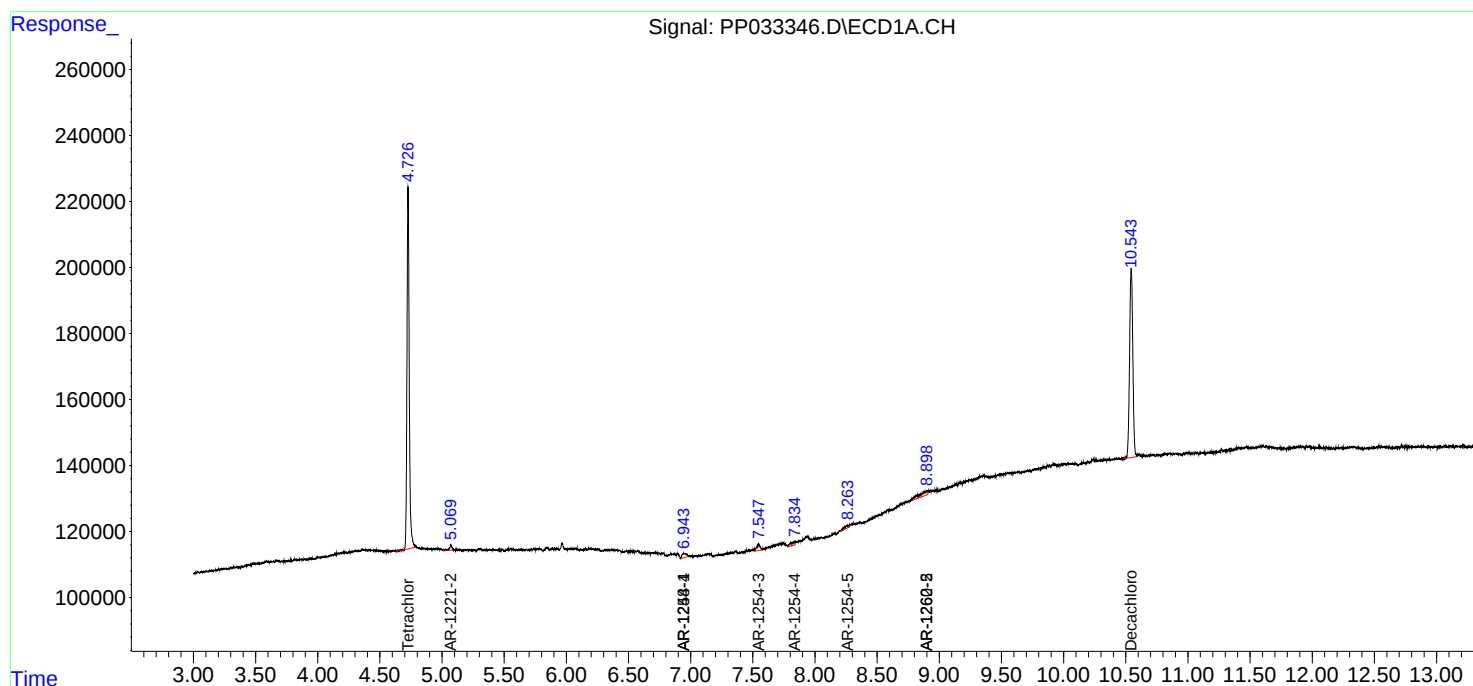


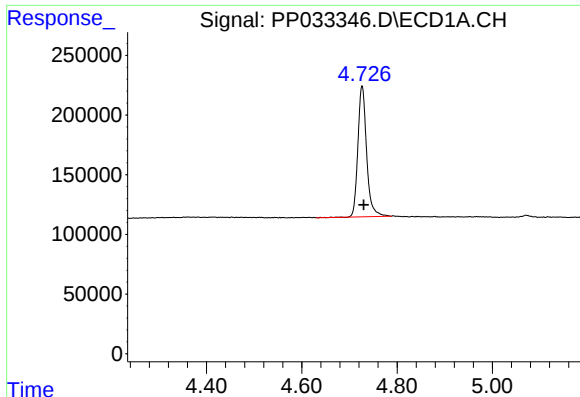

#1 Tetrachloro-m-xylene


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 1391759
Conc: 22.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

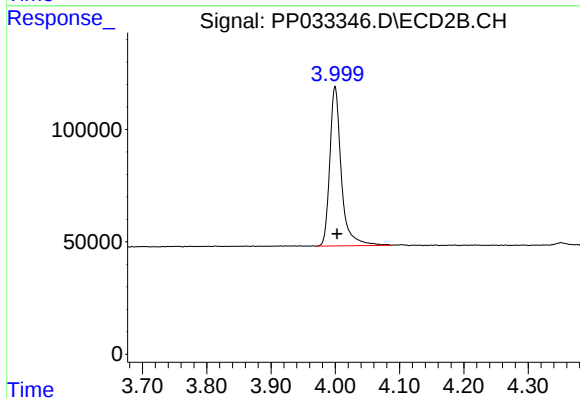


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 882020
Conc: 21.57 ng/ml

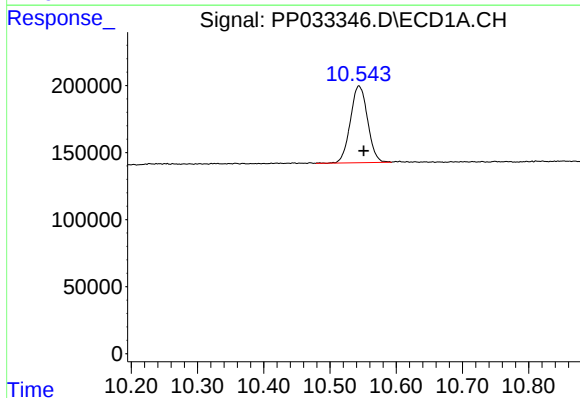


#2 Decachlorobiphenyl

R.T.: 10.544 min
Delta R.T.: -0.007 min
Response: 1034836
Conc: 23.76 ng/ml

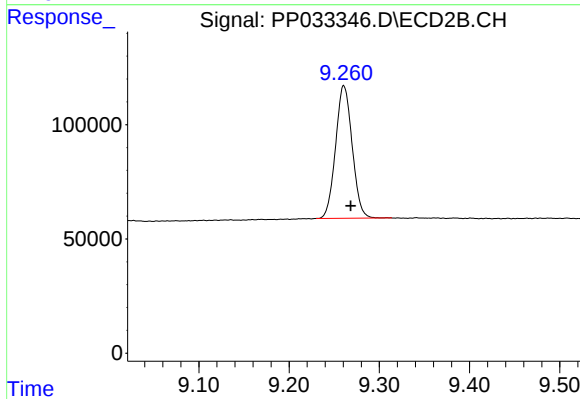

#2 Decachlorobiphenyl


R.T.: 9.261 min
Delta R.T.: -0.008 min
Response: 741329
Conc: 22.13 ng/ml

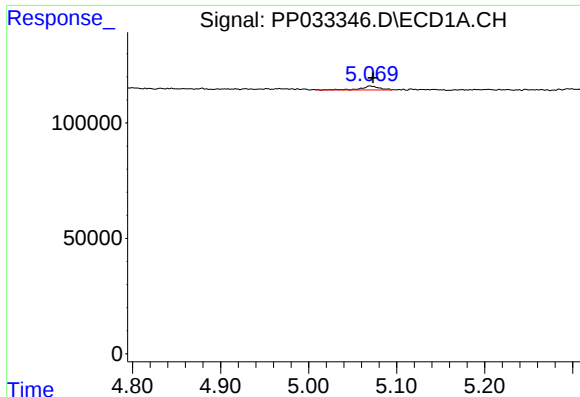

#9 AR-1221-2


R.T.: 5.070 min
Delta R.T.: -0.003 min
Response: 23765
Conc: 51.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

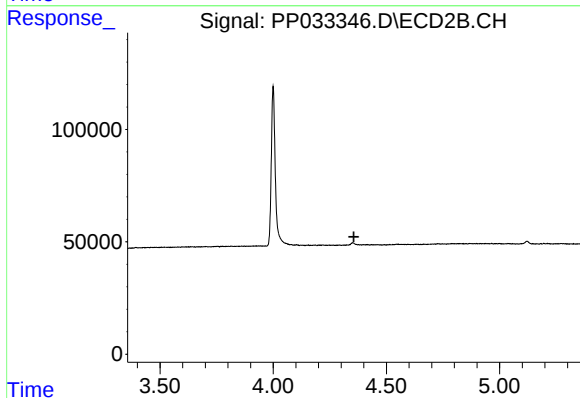


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.356 min
Response: 0
Conc: N.D.

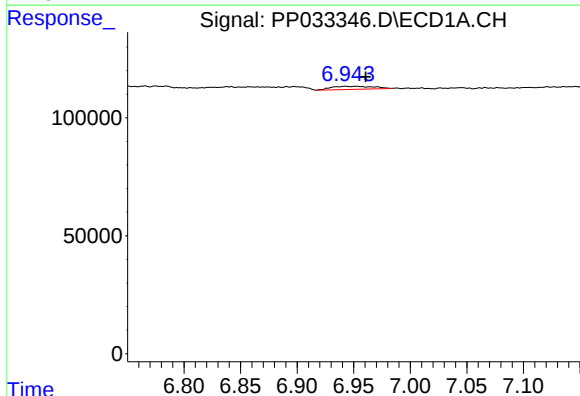


#24 AR-1248-4

R.T.: 6.943 min
Delta R.T.: -0.018 min
Response: 33254
Conc: 19.33 ng/ml

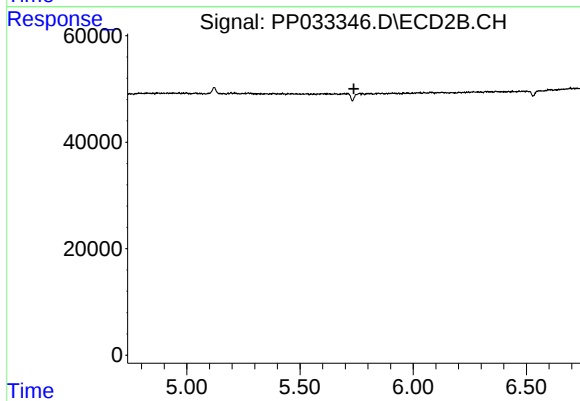

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.738 min
Response: 0
Conc: N.D.

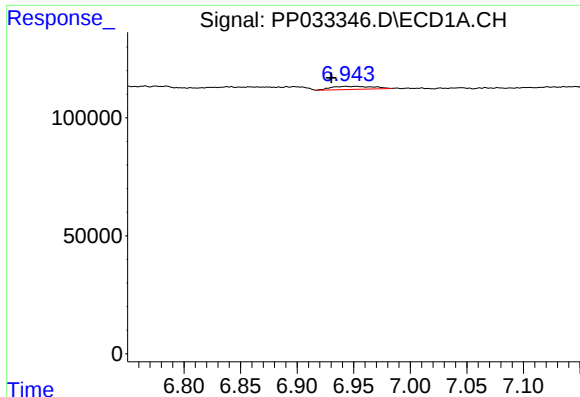

#26 AR-1254-1


R.T.: 6.943 min
Delta R.T.: 0.013 min
Response: 33254
Conc: 17.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

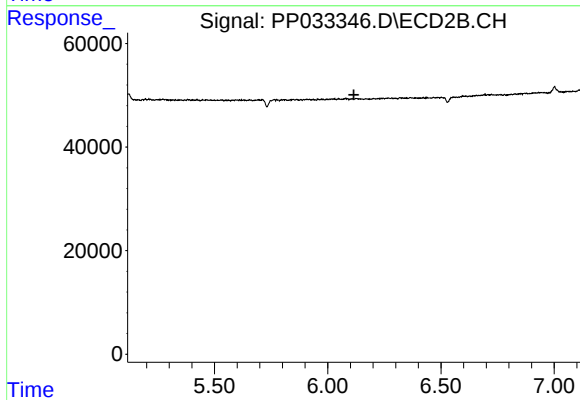


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

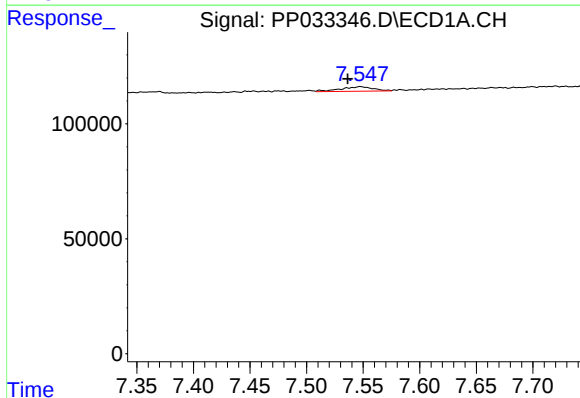


#28 AR-1254-3

R.T.: 7.547 min
Delta R.T.: 0.011 min
Response: 38731
Conc: 12.75 ng/ml

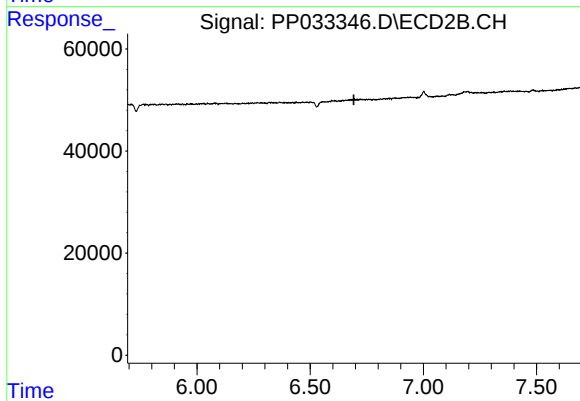

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

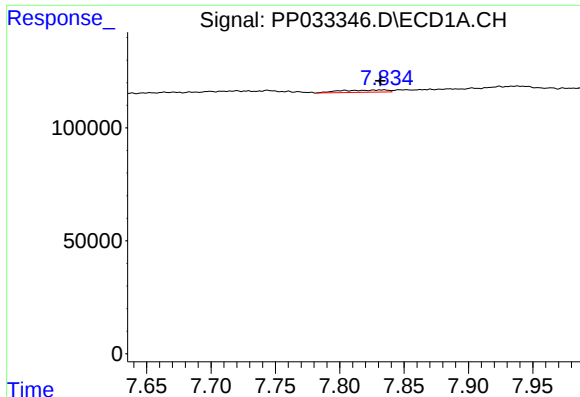

#29 AR-1254-4


R.T.: 7.834 min
Delta R.T.: 0.003 min
Response: 25206
Conc: 10.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

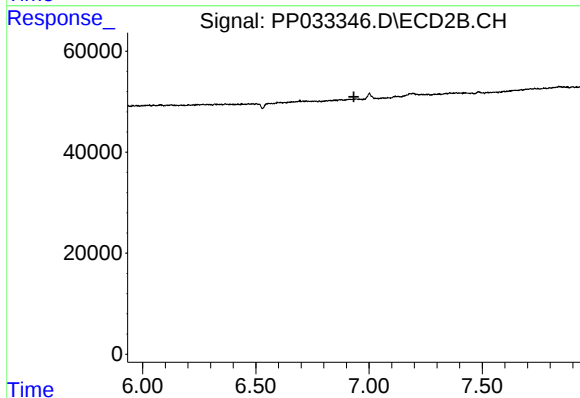


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

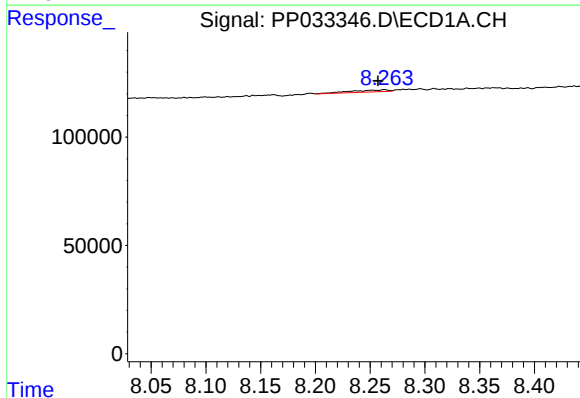


#30 AR-1254-5

R.T.: 8.263 min
Delta R.T.: 0.006 min
Response: 21572
Conc: 8.91 ng/ml

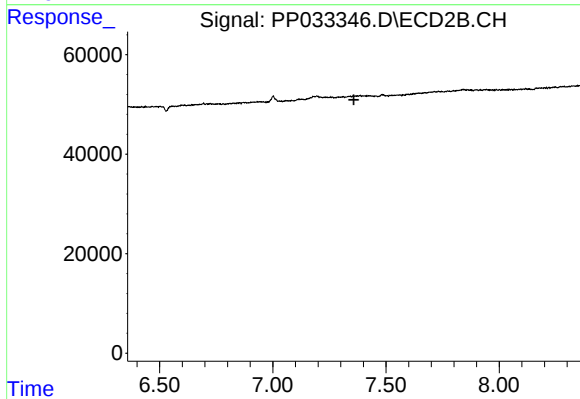

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

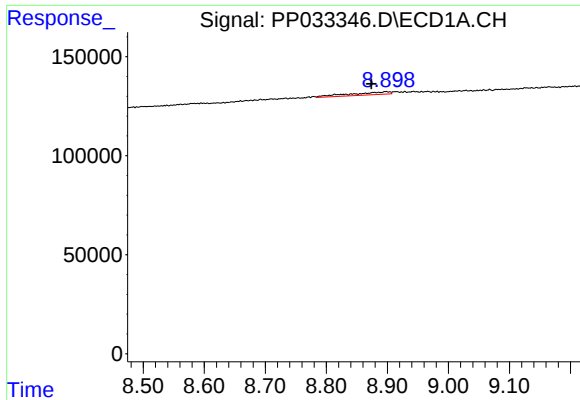

#35 AR-1260-5


R.T.: 8.898 min
Delta R.T.: 0.024 min
Response: 62735
Conc: 11.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

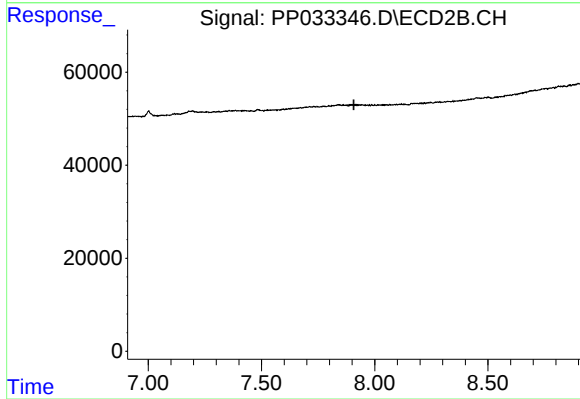


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.908 min
Response: 0
Conc: N.D.

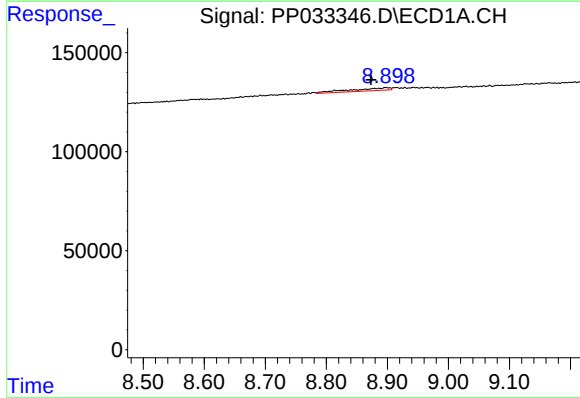

#37 AR-1262-2

R.T.: 8.898 min
Delta R.T.: 0.024 min
Response: 62735
Conc: 10.02 ng/ml

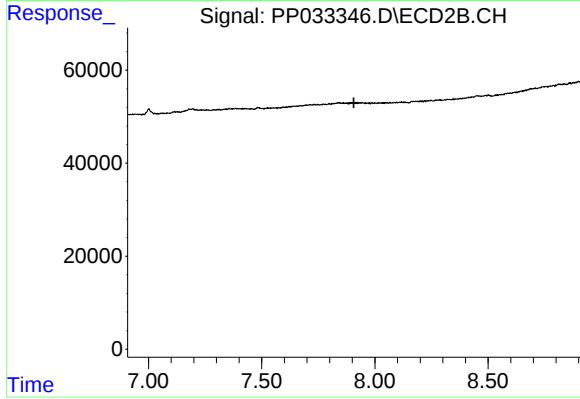

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.