

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033349.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 16:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 17:26:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.726	3.999	1389142	873024	22.653	21.350
2) SA Decachlor...	10.543	9.260	1418146	731359	32.555	21.832 #
Target Compounds						
9) L2 AR-1221-2	5.073	0.000	21284	0	45.753	N.D. #
20) L4 AR-1242-5	6.971f	0.000	85197	0	82.003	N.D. #
24) L5 AR-1248-4	6.971	0.000	85197	0	49.515	N.D. #
25) L5 AR-1248-5	6.971f	0.000	85197	0	48.964	N.D. #
28) L6 AR-1254-3	7.545	0.000	45910	0	15.116	N.D. #
29) L6 AR-1254-4	7.834	0.000	49294	0	21.309	N.D. #
32) L7 AR-1260-2	0.000	6.998f	0	22733	N.D.	11.251 #
45) L9 AR-1268-5	10.239	0.000	590118	0	36.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033349.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 16:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 17:26:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

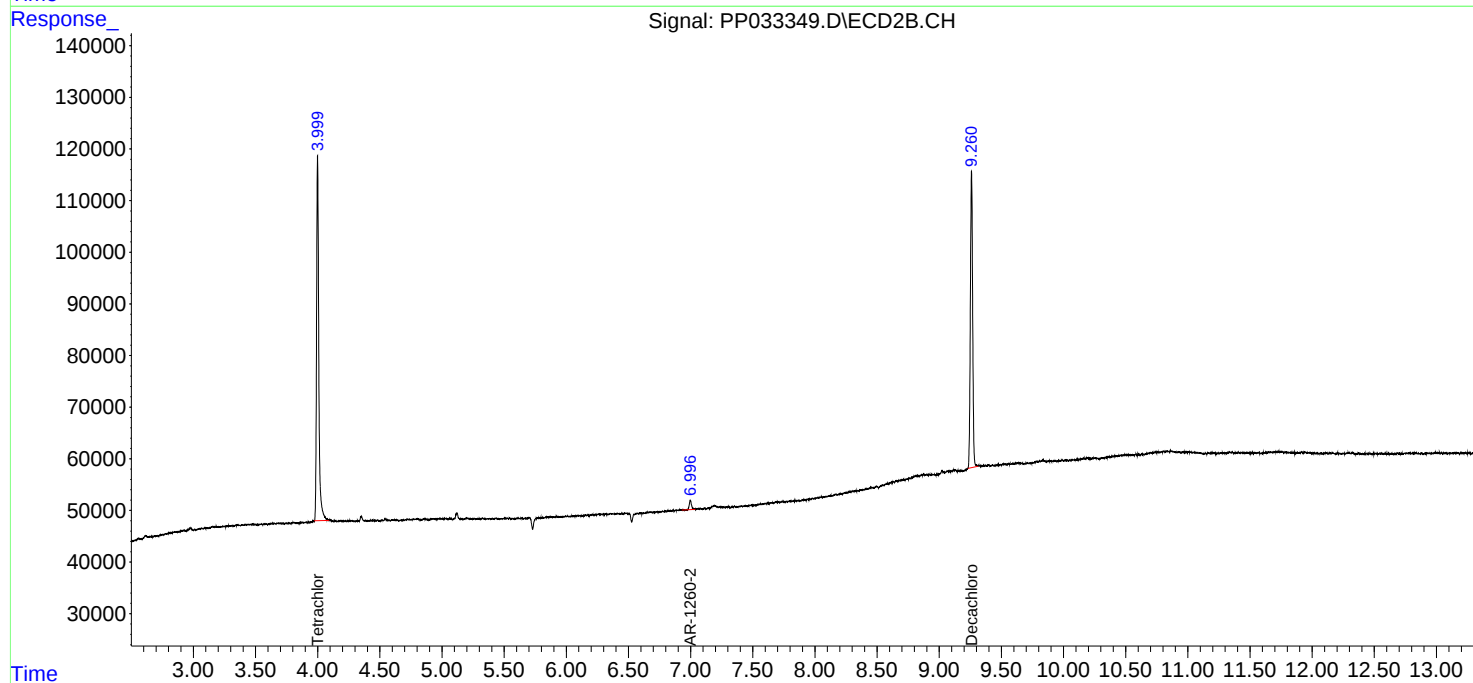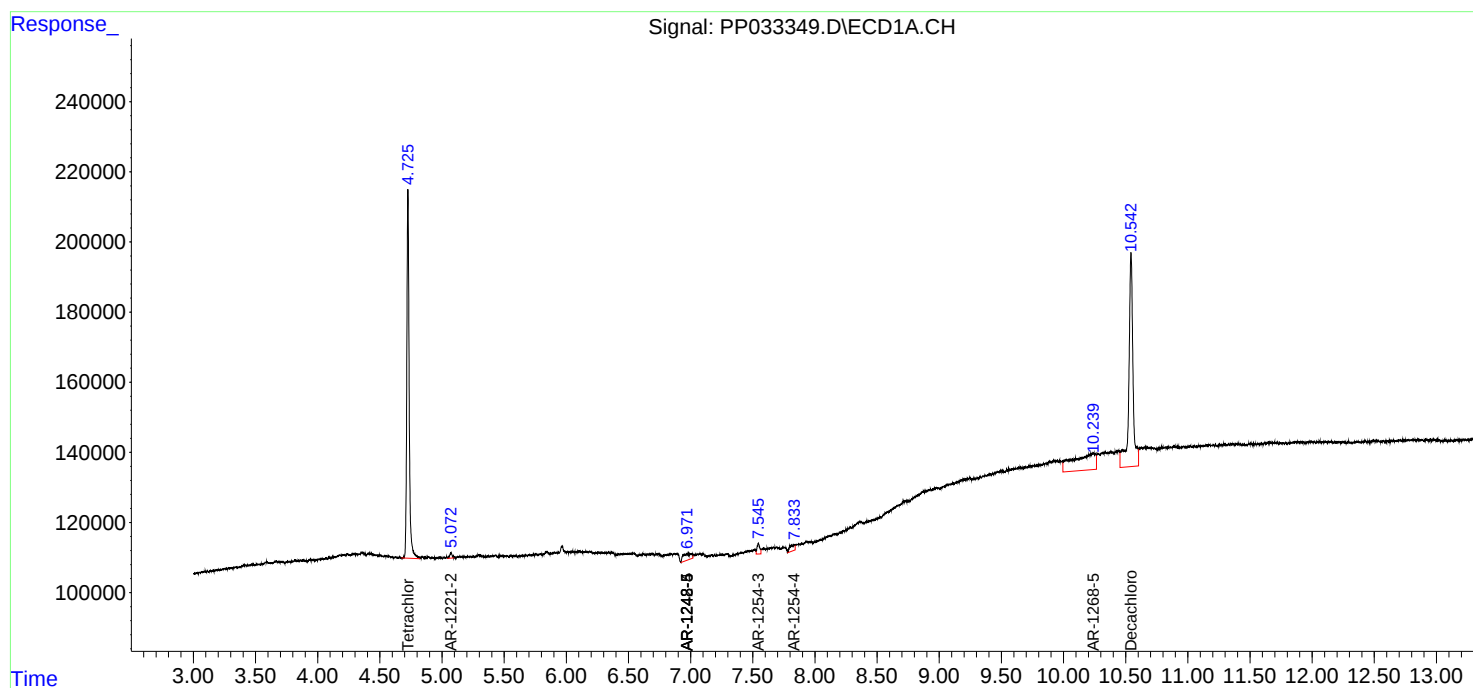


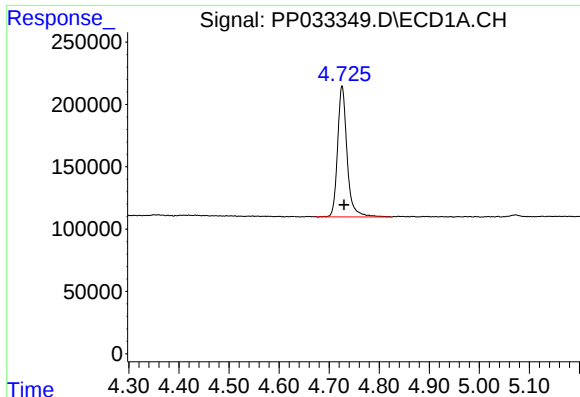

#1 Tetrachloro-m-xylene


R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1389142
Conc: 22.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

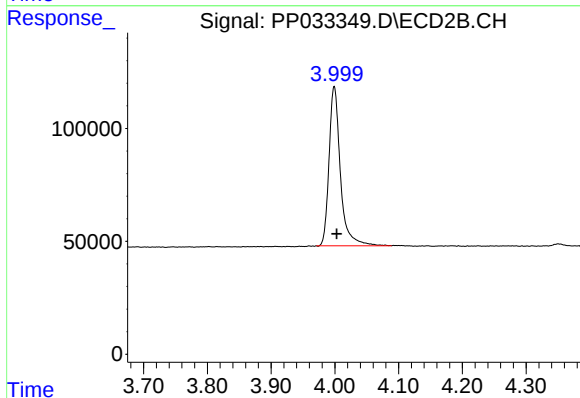


#1 Tetrachloro-m-xylene

R.T.: 3.999 min
Delta R.T.: -0.004 min
Response: 873024
Conc: 21.35 ng/ml

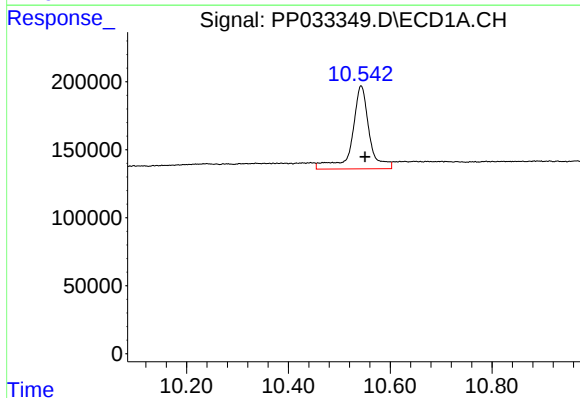


#2 Decachlorobiphenyl

R.T.: 10.543 min
Delta R.T.: -0.008 min
Response: 1418146
Conc: 32.56 ng/ml

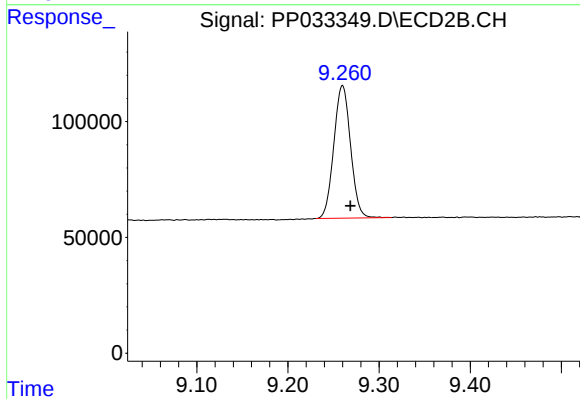

#2 Decachlorobiphenyl


R.T.: 9.260 min
Delta R.T.: -0.008 min
Response: 731359
Conc: 21.83 ng/ml

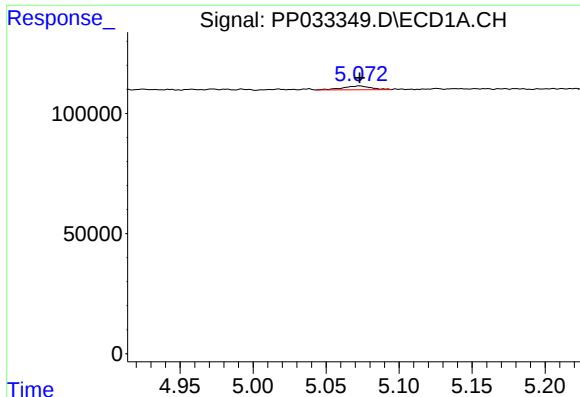

#9 AR-1221-2


R.T.: 5.073 min
Delta R.T.: 0.000 min
Response: 21284
Conc: 45.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

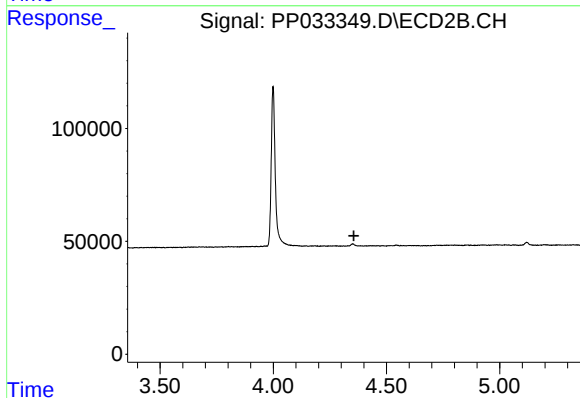


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.356 min
Response: 0
Conc: N.D.

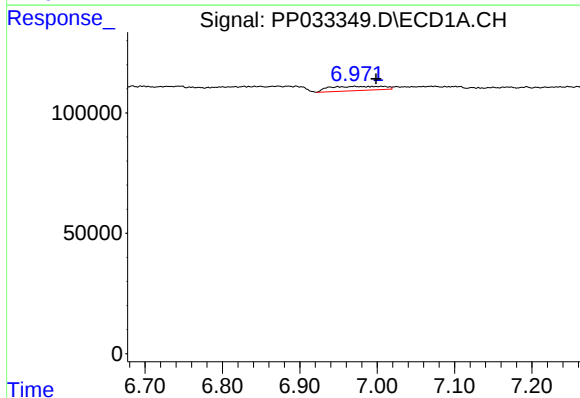


#20 AR-1242-5

R.T.: 6.971 min
Delta R.T.: -0.028 min
Response: 85197
Conc: 82.00 ng/ml

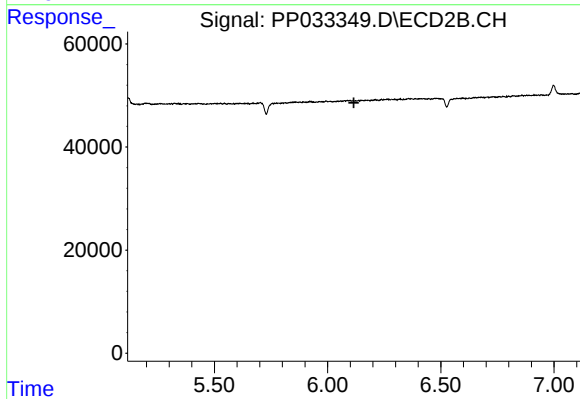

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.116 min
Response: 0
Conc: N.D.

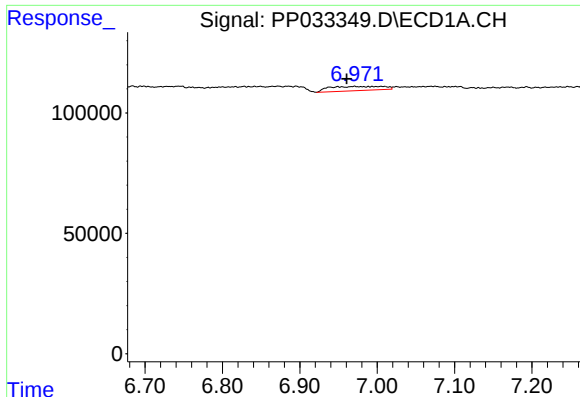

#24 AR-1248-4


R.T.: 6.971 min
Delta R.T.: 0.010 min
Response: 85197
Conc: 49.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

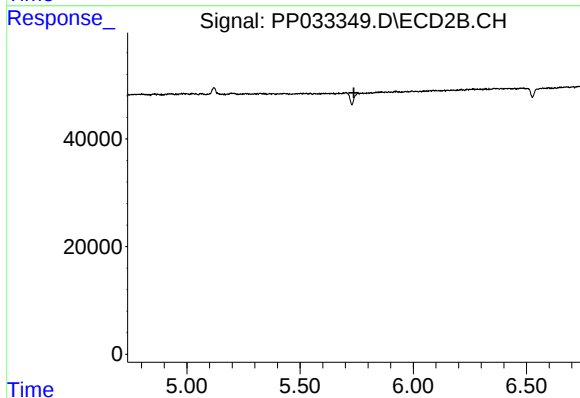


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.738 min
Response: 0
Conc: N.D.

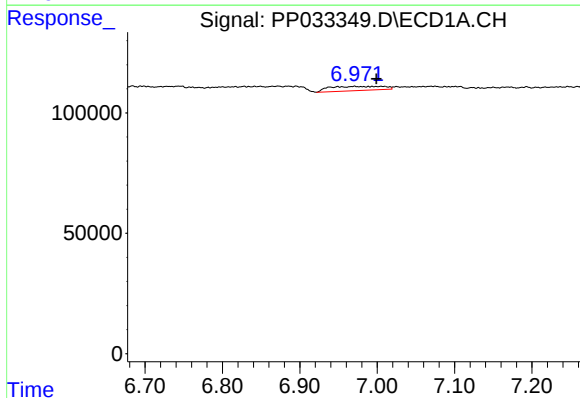


#25 AR-1248-5

R.T.: 6.971 min
Delta R.T.: -0.028 min
Response: 85197
Conc: 48.96 ng/ml

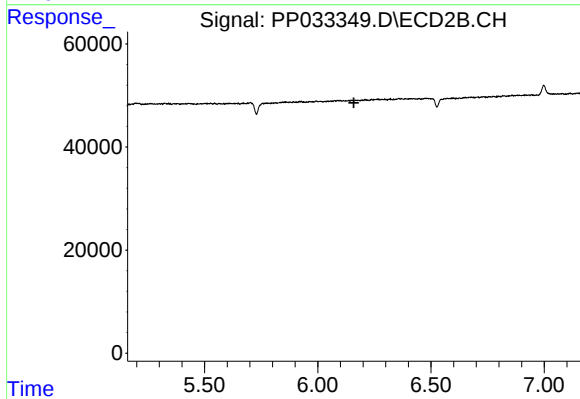

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

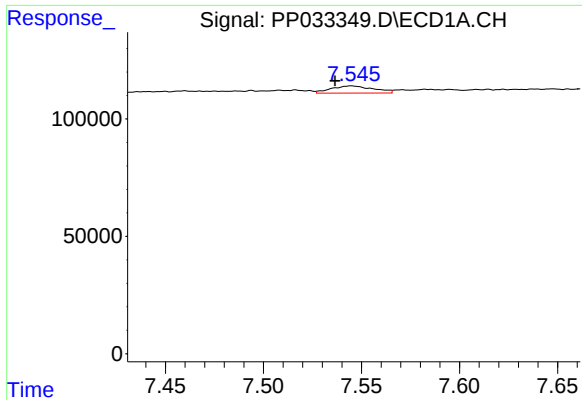

#28 AR-1254-3


R.T.: 7.545 min
Delta R.T.: 0.008 min
Response: 45910
Conc: 15.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

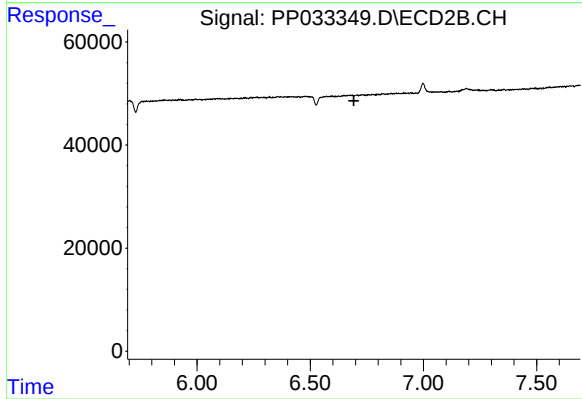


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

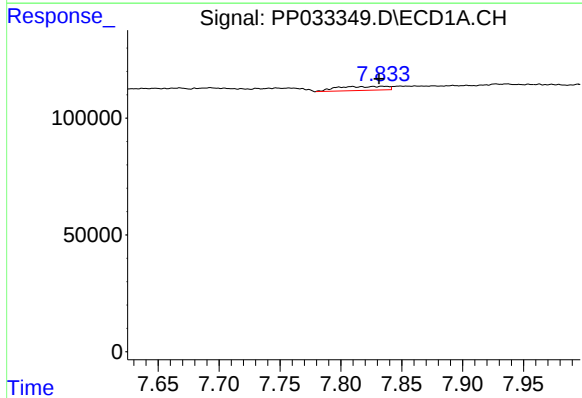


#29 AR-1254-4

R.T.: 7.834 min
Delta R.T.: 0.003 min
Response: 49294
Conc: 21.31 ng/ml

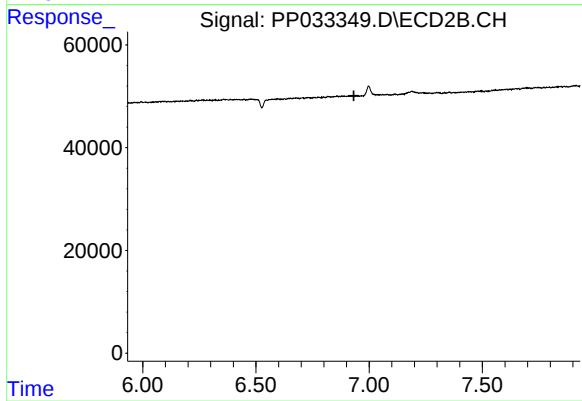

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

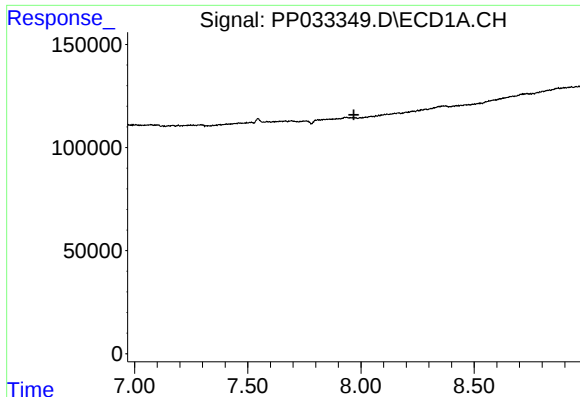

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

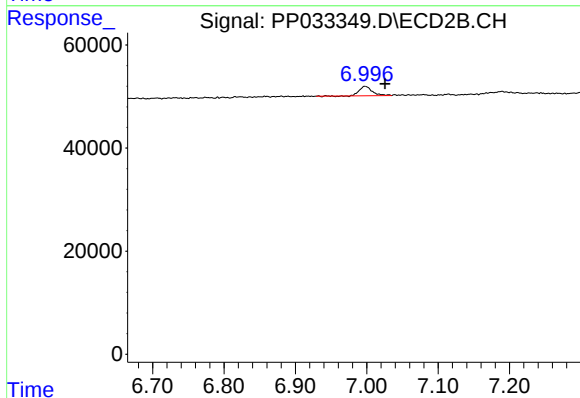


#32 AR-1260-2

R.T.: 6.998 min
Delta R.T.: -0.028 min
Response: 22733
Conc: 11.25 ng/ml

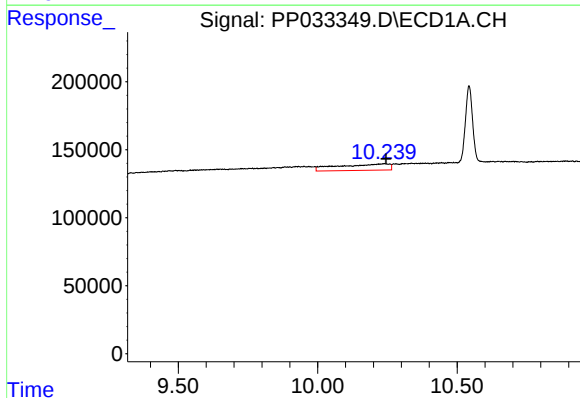

#45 AR-1268-5

R.T.: 10.239 min
Delta R.T.: -0.007 min
Response: 590118
Conc: 36.05 ng/ml

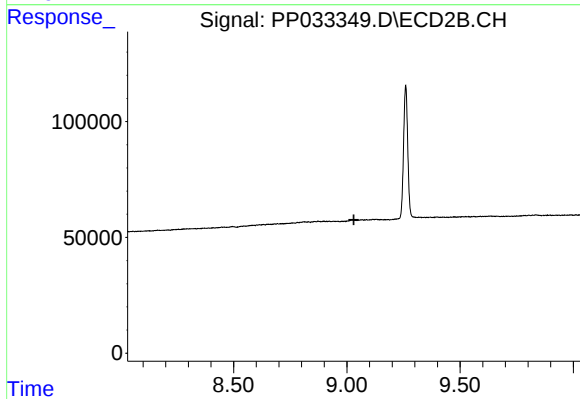

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.031 min
Response: 0
Conc: N.D.