

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 10:38
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/16/2021 8:56:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 13:20:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.736	4.000	3373967	1918264	55.020	46.911
2) SA Decachlor...	10.557	9.265	2505839	1680596	57.525	50.167
Target Compounds						
21) L5 AR-1248-1	6.035	5.245	534052	314805	557.779	484.064
22) L5 AR-1248-2	6.327	5.507	705711	443536	532.584	462.326
23) L5 AR-1248-3	6.541	5.551	843887	475643	521.149m	467.804
24) L5 AR-1248-4	6.965	5.735	944049	573460	548.660	462.738
25) L5 AR-1248-5	7.005	6.157	957872	544807	550.500	482.416

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 10:38
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 13:20:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

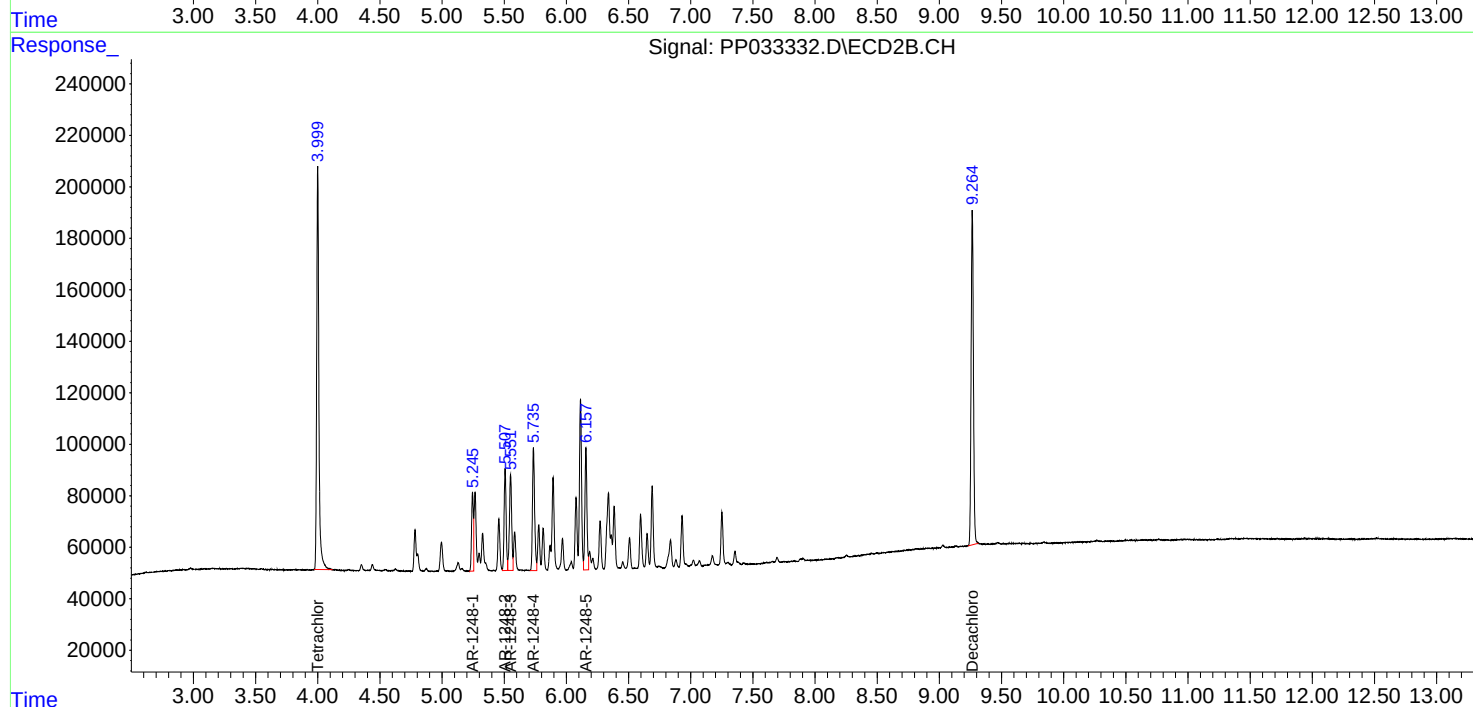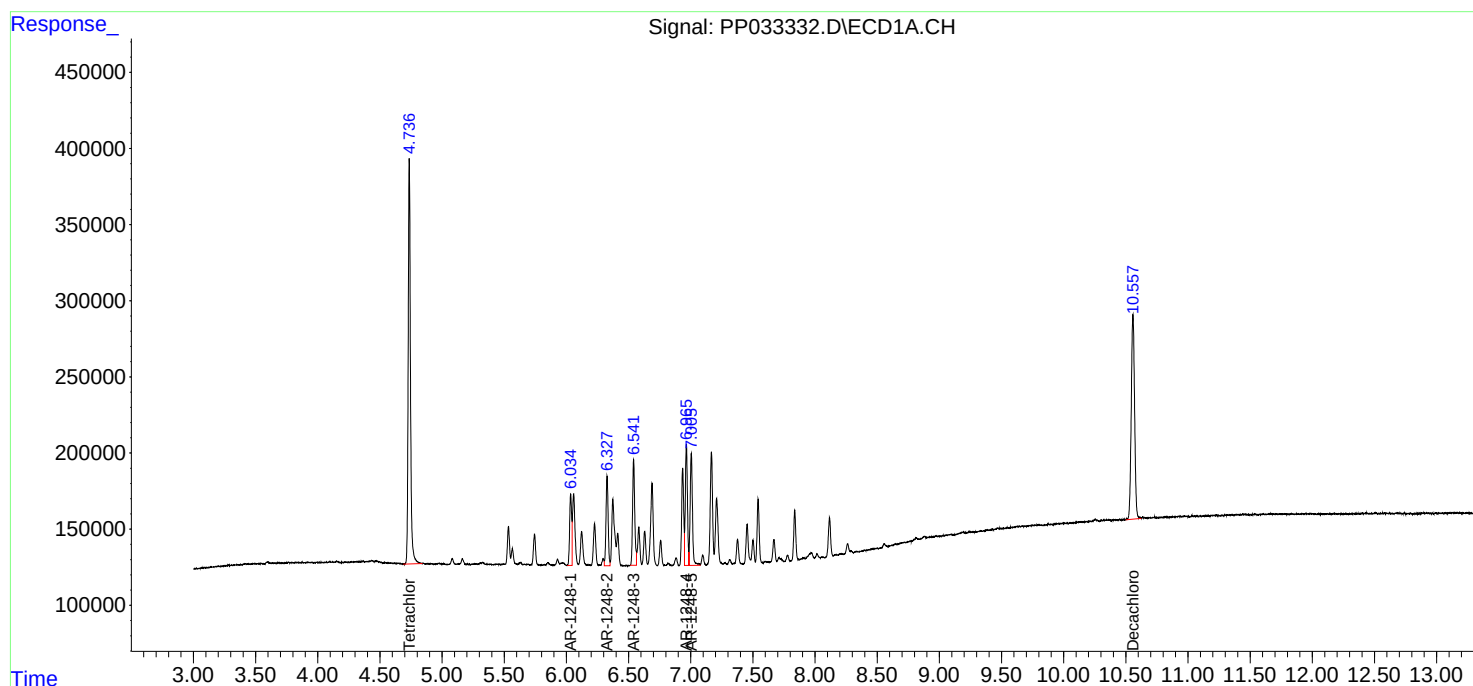

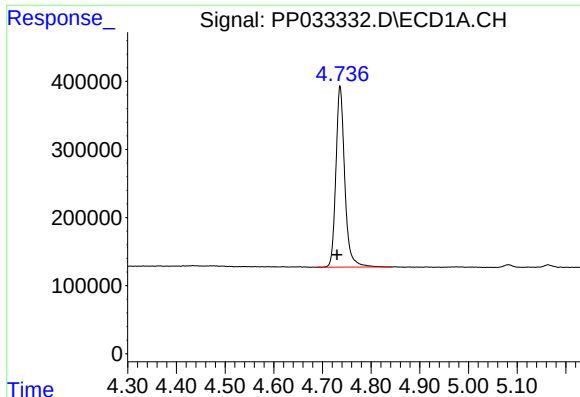


#1 Tetrachloro-m-xylene

R.T.: 4.736 min
Delta R.T.: 0.006 min
Response: 3373967
Conc: 55.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:48 AM

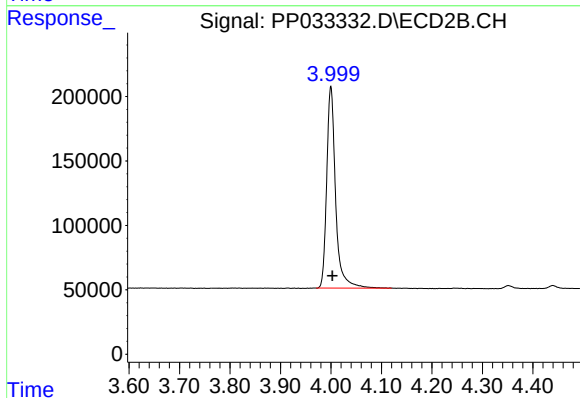


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1918264
Conc: 46.91 ng/ml

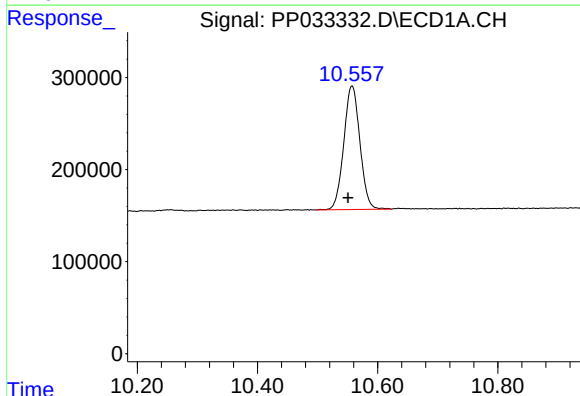


#2 Decachlorobiphenyl

R.T.: 10.557 min
Delta R.T.: 0.006 min
Response: 2505839
Conc: 57.52 ng/ml

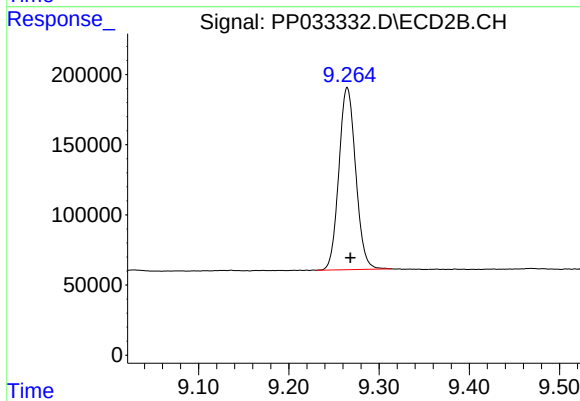

#2 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.004 min
Response: 1680596
Conc: 50.17 ng/ml

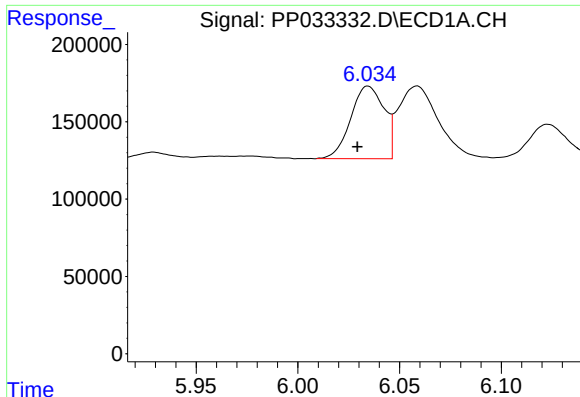


#21 AR-1248-1

R.T.: 6.035 min
Delta R.T.: 0.005 min
Response: 534052
Conc: 557.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:48 AM

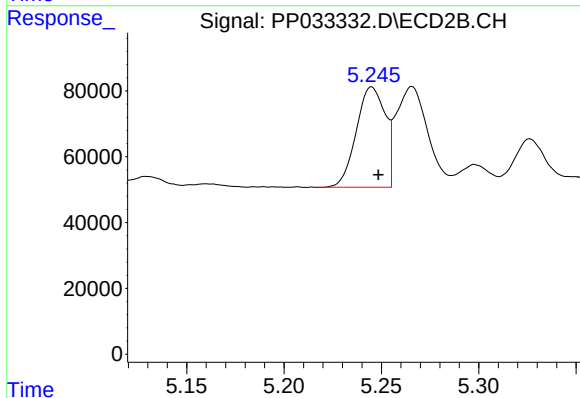


#21 AR-1248-1

R.T.: 5.245 min
Delta R.T.: -0.003 min
Response: 314805
Conc: 484.06 ng/ml

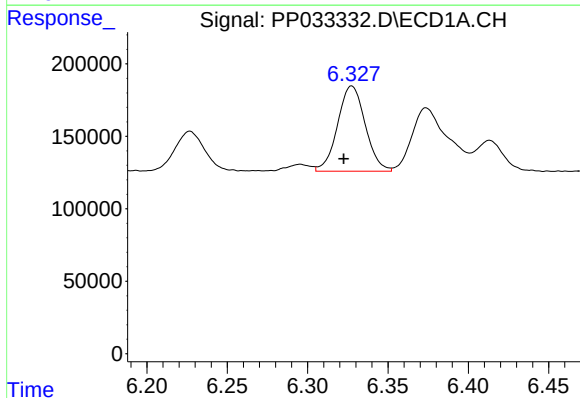


#22 AR-1248-2

R.T.: 6.327 min
Delta R.T.: 0.005 min
Response: 705711
Conc: 532.58 ng/ml

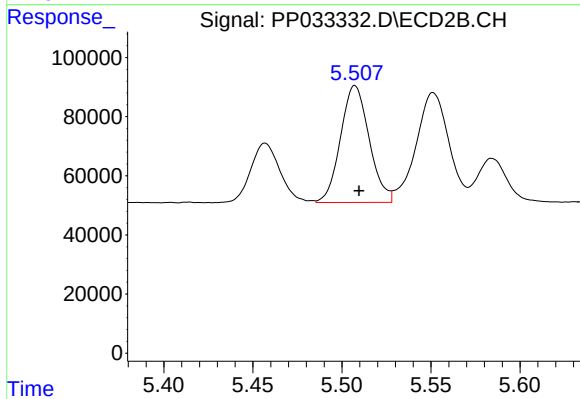

#22 AR-1248-2

R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 443536
Conc: 462.33 ng/ml

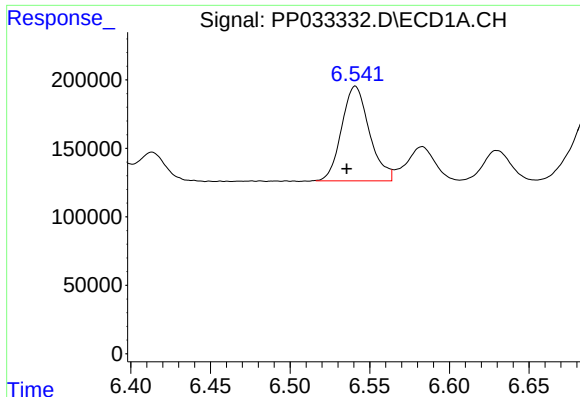


#23 AR-1248-3

R.T.: 6.541 min
Delta R.T.: 0.005 min
Response: 843887
Conc: 521.15 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:48 AM

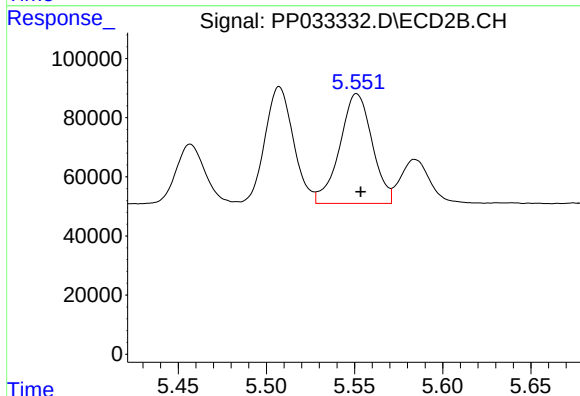


#23 AR-1248-3

R.T.: 5.551 min
Delta R.T.: -0.002 min
Response: 475643
Conc: 467.80 ng/ml

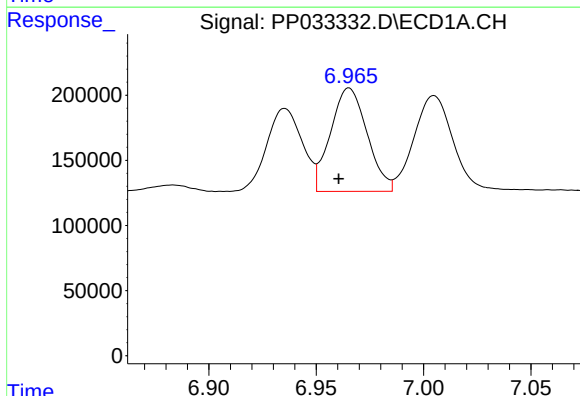


#24 AR-1248-4

R.T.: 6.965 min
Delta R.T.: 0.005 min
Response: 944049
Conc: 548.66 ng/ml

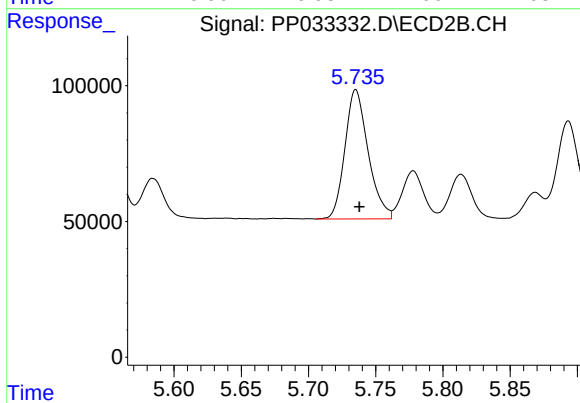

#24 AR-1248-4

R.T.: 5.735 min
Delta R.T.: -0.003 min
Response: 573460
Conc: 462.74 ng/ml

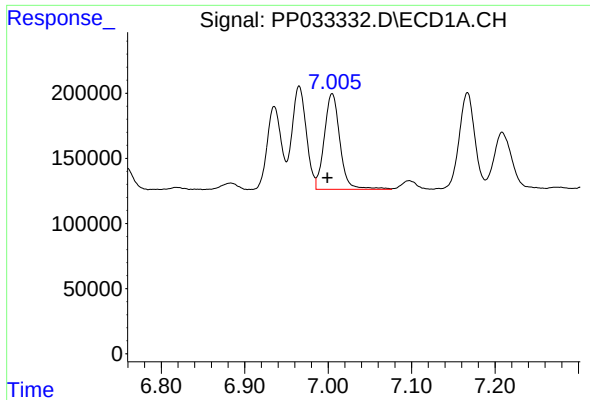


#25 AR-1248-5

R.T.: 7.005 min
Delta R.T.: 0.006 min
Response: 957872
Conc: 550.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:48 AM

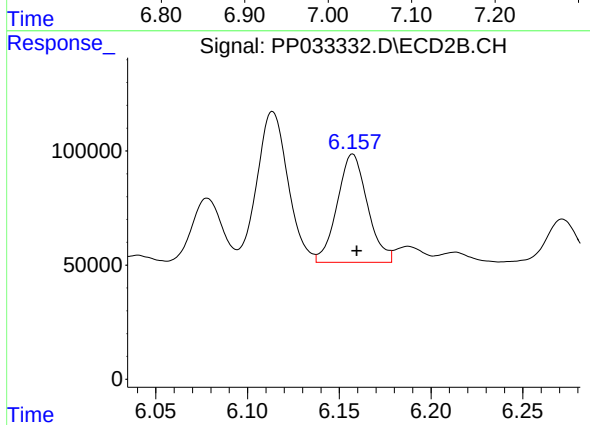

#25 AR-1248-5

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 544807
Conc: 482.42 ng/ml