

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 11:41
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 2/16/2021 8:56:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 13:20:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.739	4.000	3448521	1951337	56.236	47.719
2) SA Decachlor...	10.561	9.268	2512370	1706575	57.675m	50.942
Target Compounds						
26) L6 AR-1254-1	6.939	6.115	997279	874064	531.167	457.350
27) L6 AR-1254-2	7.167	6.274	1452214	749219	495.339	456.945
28) L6 AR-1254-3	7.546	6.692	1632312	1255369	537.423	467.082
29) L6 AR-1254-4	7.839	6.932	1318379	717187	569.919	480.338
30) L6 AR-1254-5	8.266	7.358	1320048	1120441	545.523	462.728

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 11:41
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 13:20:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

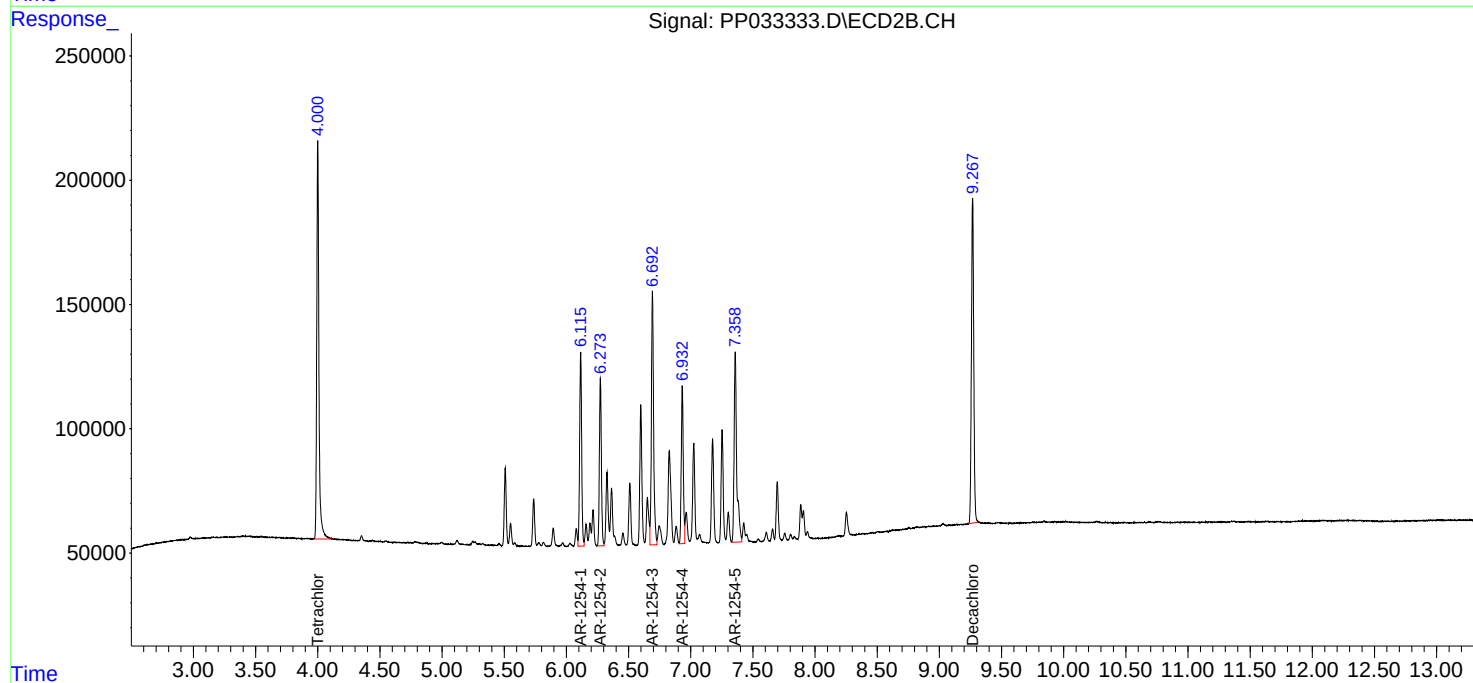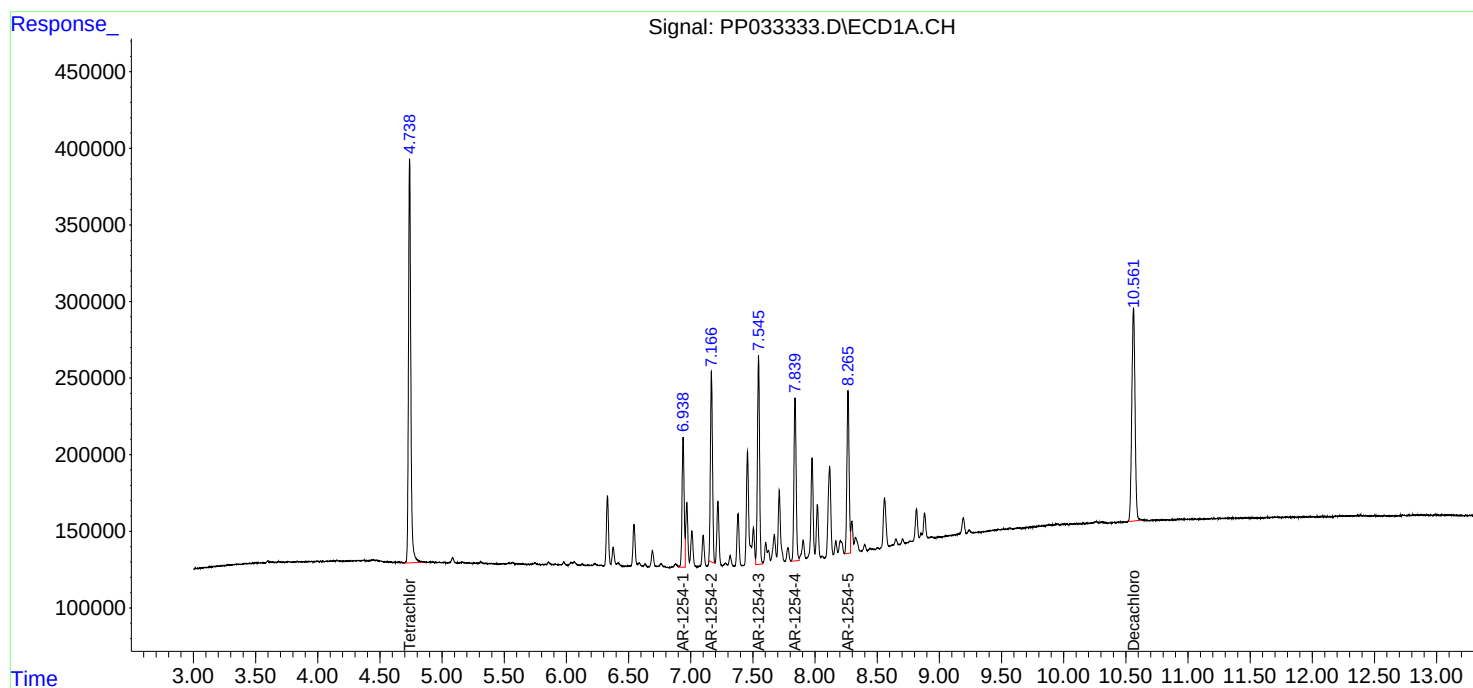

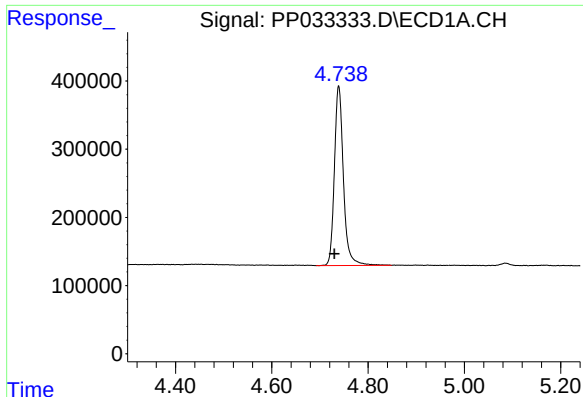


#1 Tetrachloro-m-xylene

R.T.: 4.739 min
Delta R.T.: 0.009 min
Response: 3448521
Conc: 56.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:52 AM

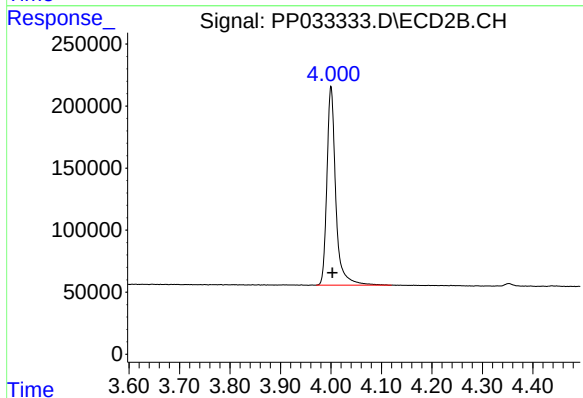


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1951337
Conc: 47.72 ng/ml

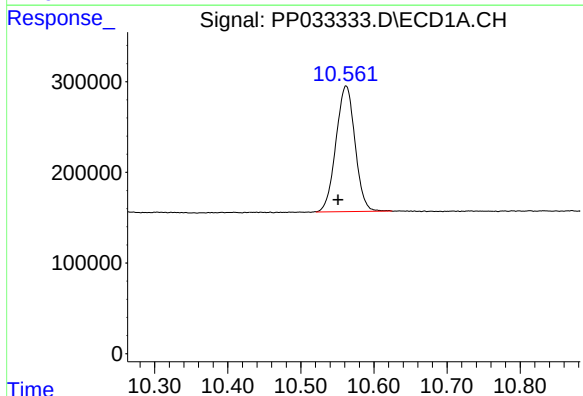


#2 Decachlorobiphenyl

R.T.: 10.561 min
Delta R.T.: 0.010 min
Response: 2512370
Conc: 57.67 ng/ml m

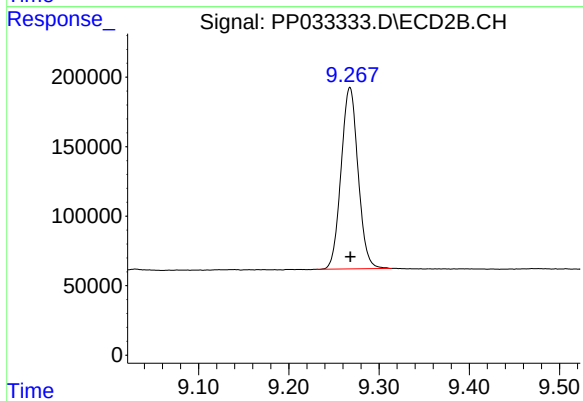

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 1706575
Conc: 50.94 ng/ml

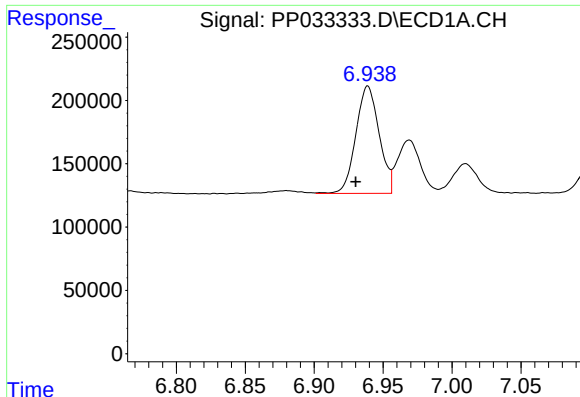


#26 AR-1254-1

R.T.: 6.939 min
Delta R.T.: 0.009 min
Response: 997279
Conc: 531.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:52 AM

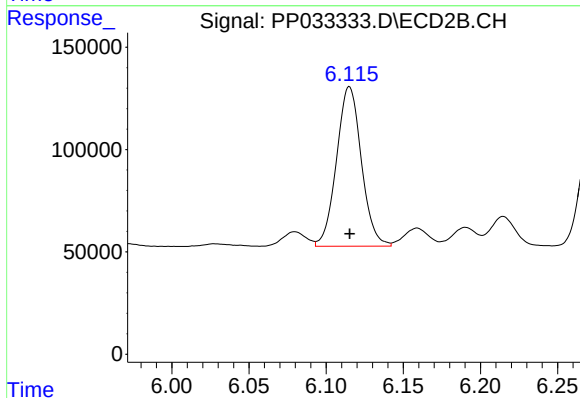


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 874064
Conc: 457.35 ng/ml

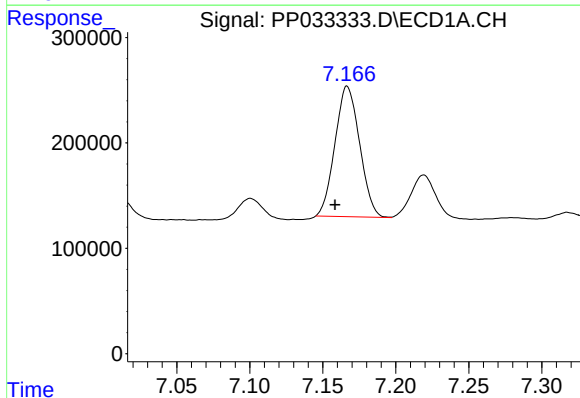


#27 AR-1254-2

R.T.: 7.167 min
Delta R.T.: 0.008 min
Response: 1452214
Conc: 495.34 ng/ml

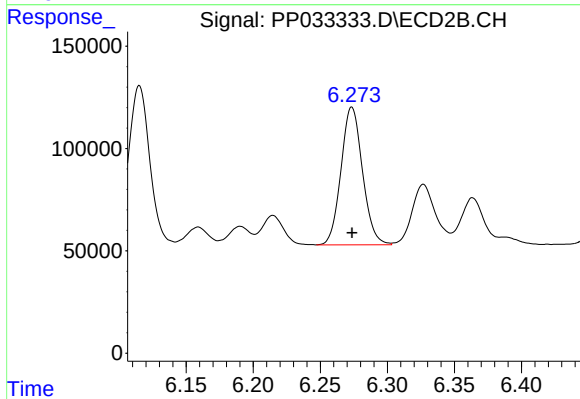

#27 AR-1254-2

R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 749219
Conc: 456.94 ng/ml

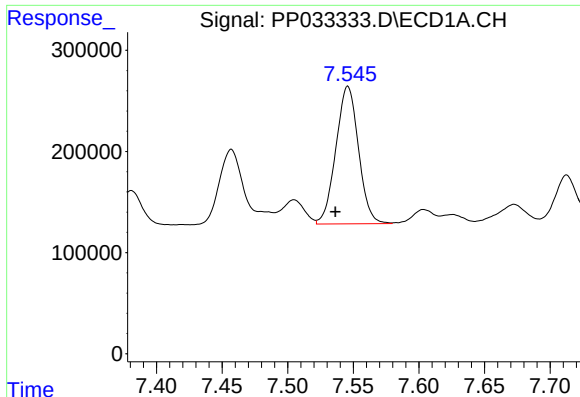


#28 AR-1254-3

R.T.: 7.546 min
Delta R.T.: 0.009 min
Response: 1632312
Conc: 537.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:52 AM

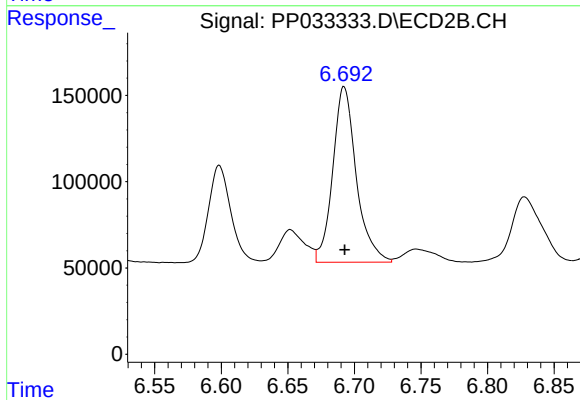


#28 AR-1254-3

R.T.: 6.692 min
Delta R.T.: 0.000 min
Response: 1255369
Conc: 467.08 ng/ml

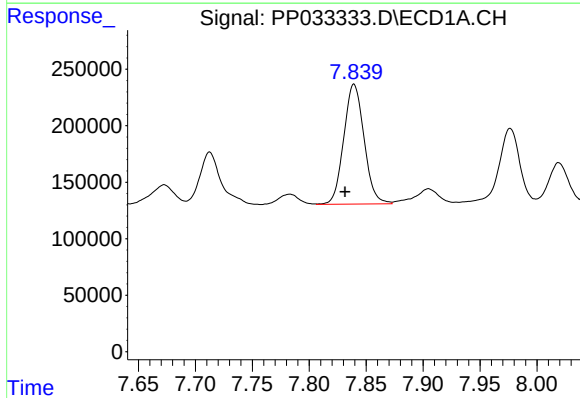


#29 AR-1254-4

R.T.: 7.839 min
Delta R.T.: 0.008 min
Response: 1318379
Conc: 569.92 ng/ml

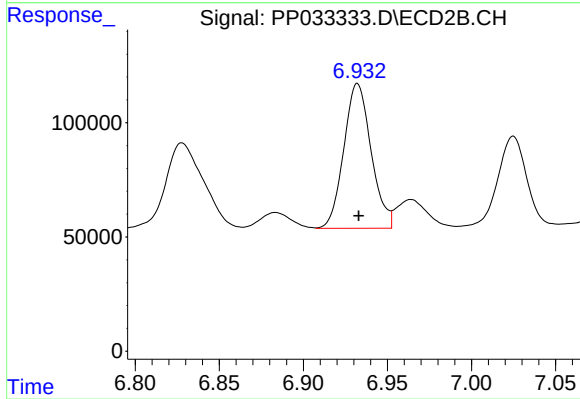

#29 AR-1254-4

R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 717187
Conc: 480.34 ng/ml

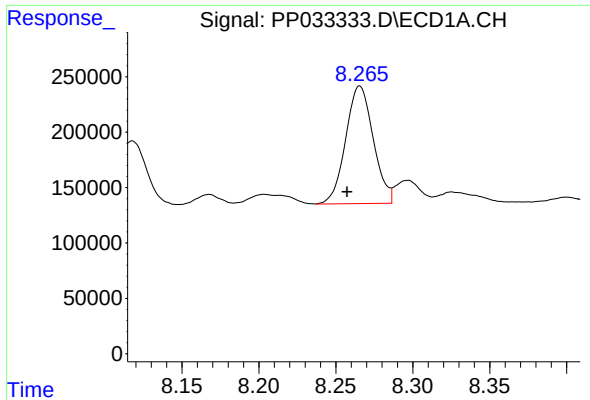


#30 AR-1254-5

R.T.: 8.266 min
Delta R.T.: 0.008 min
Response: 1320048
Conc: 545.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
2/16/2021 8:56:52 AM

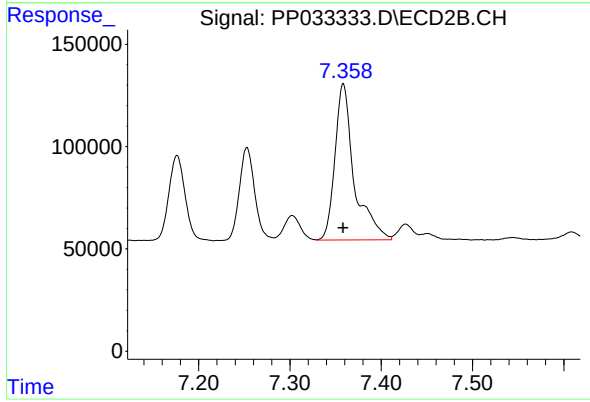

#30 AR-1254-5

R.T.: 7.358 min
Delta R.T.: 0.000 min
Response: 1120441
Conc: 462.73 ng/ml