

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 13:26
 Operator : DD\AJ
 Sample : M1402-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-N9994

Manual Integrations
 APPROVED

Ankita
 2/16/2021 8:57:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 14:51:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.726	4.000	1530258	930130	24.954	22.746
2)	SA Decachlor...	10.543	9.260	672089	483811	15.429m	14.442m
Target Compounds							
26)	L6 AR-1254-1	6.926	6.111	21257	34246	11.322	17.919 #
27)	L6 AR-1254-2	7.155	6.268	41143	30156	14.033m	18.392 #
28)	L6 AR-1254-3	7.534	6.689	97766	64264	32.188	23.911 #
29)	L6 AR-1254-4	7.827	6.928	82067	39445	35.476	26.418 #
30)	L6 AR-1254-5	8.253	7.353	154129	251487	63.695	103.861m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 13:26
Operator : DD\AJ
Sample : M1402-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 14:51:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

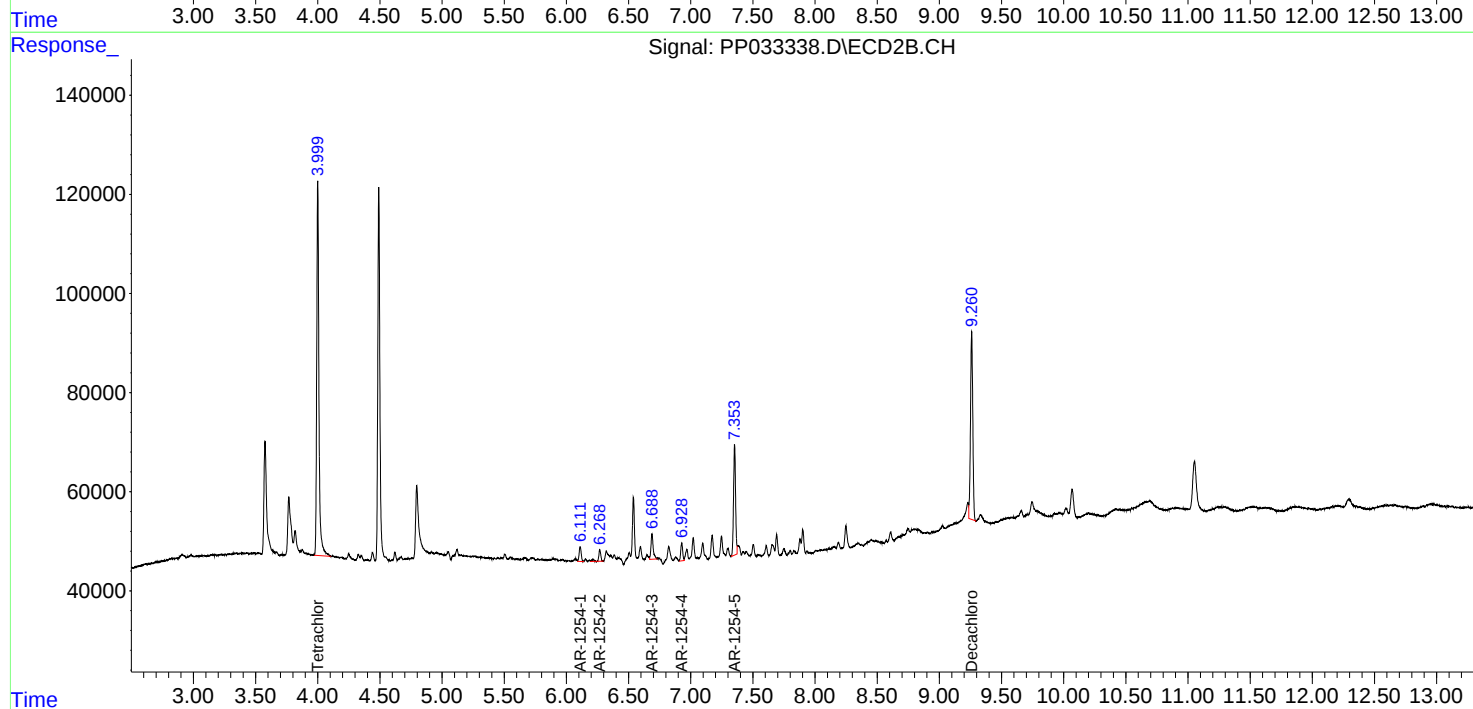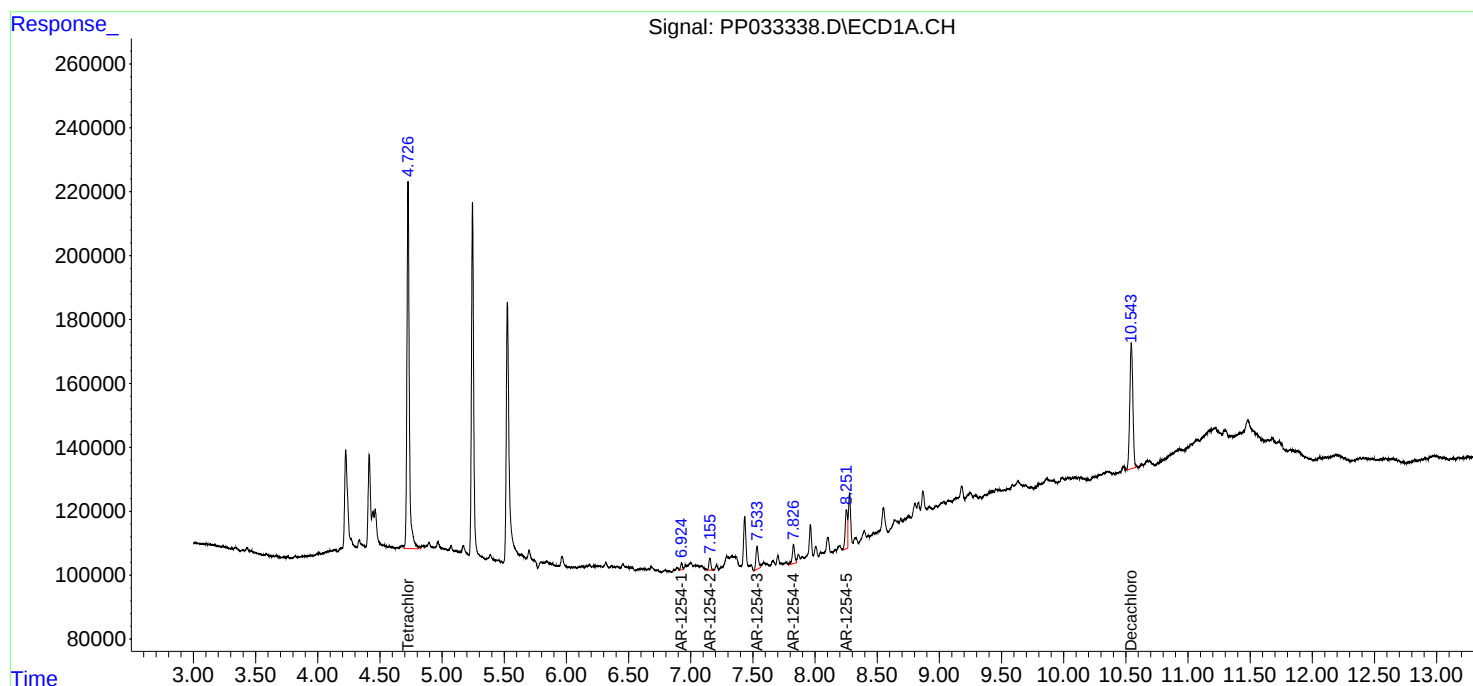

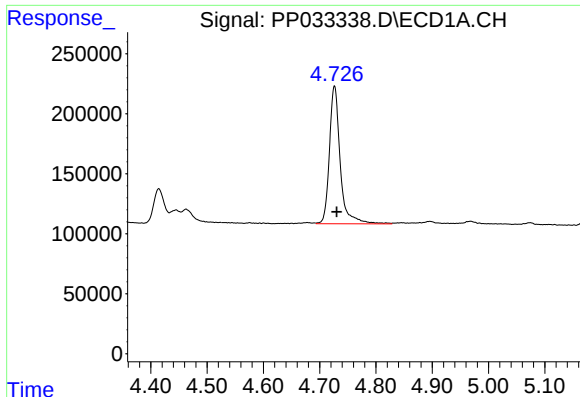


#1 Tetrachloro-m-xylene

R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1530258
Conc: 24.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:01 AM

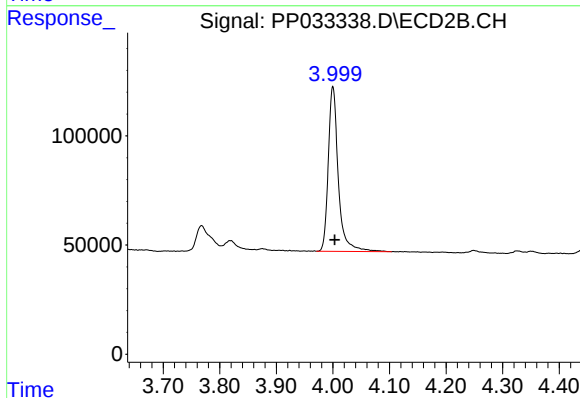


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 930130
Conc: 22.75 ng/ml

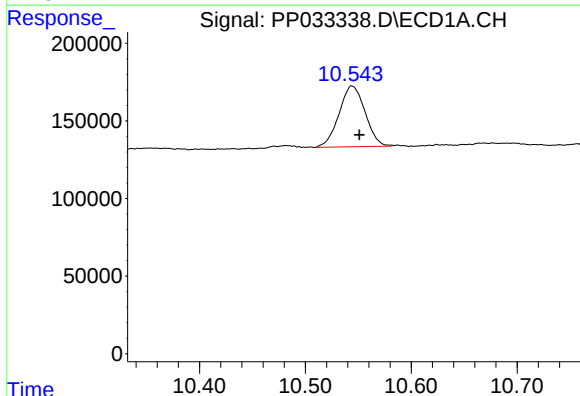


#2 Decachlorobiphenyl

R.T.: 10.543 min
Delta R.T.: -0.008 min
Response: 672089
Conc: 15.43 ng/ml m

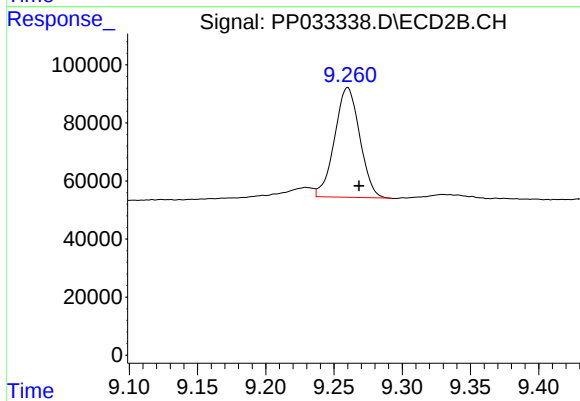

#2 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: -0.009 min
Response: 483811
Conc: 14.44 ng/ml m

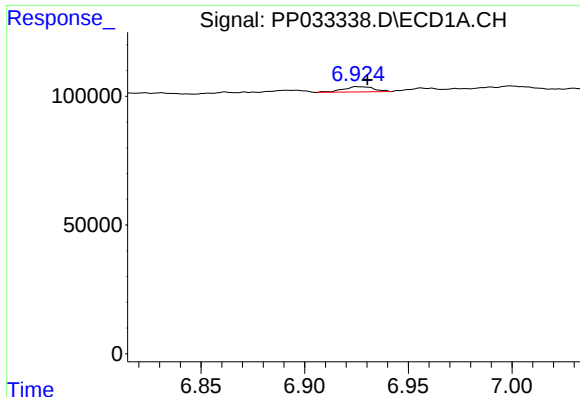


#26 AR-1254-1

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 21257
Conc: 11.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:01 AM

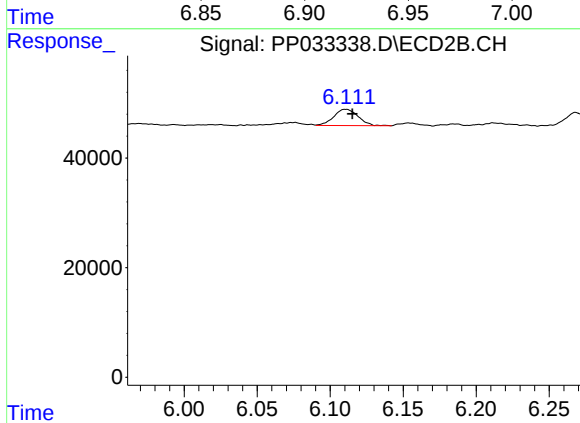


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.005 min
Response: 34246
Conc: 17.92 ng/ml

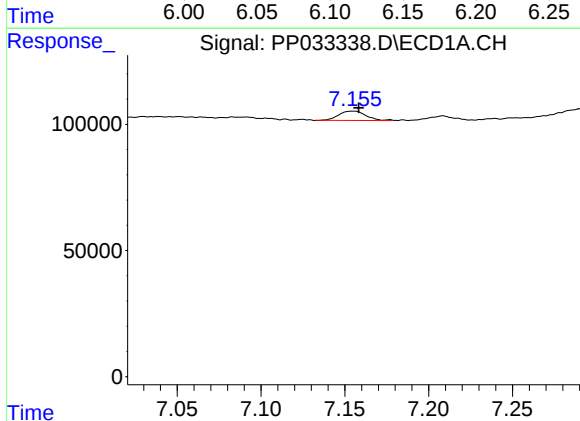


#27 AR-1254-2

R.T.: 7.155 min
Delta R.T.: -0.004 min
Response: 41143
Conc: 14.03 ng/ml m

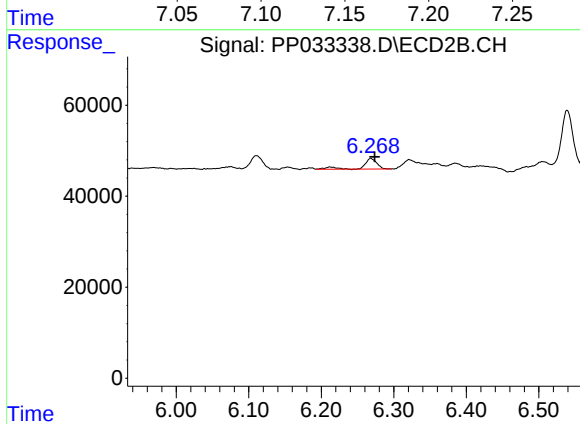

#27 AR-1254-2

R.T.: 6.268 min
Delta R.T.: -0.005 min
Response: 30156
Conc: 18.39 ng/ml

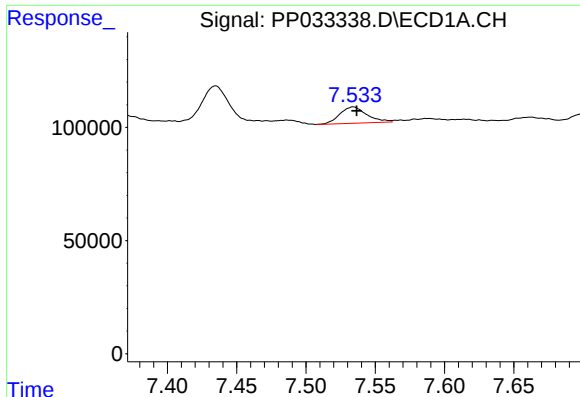


#28 AR-1254-3

R.T.: 7.534 min
Delta R.T.: -0.002 min
Response: 97766
Conc: 32.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-N9994


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:01 AM

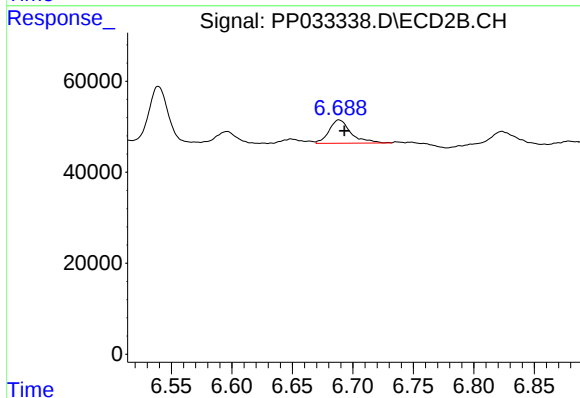


#28 AR-1254-3

R.T.: 6.689 min
Delta R.T.: -0.004 min
Response: 64264
Conc: 23.91 ng/ml

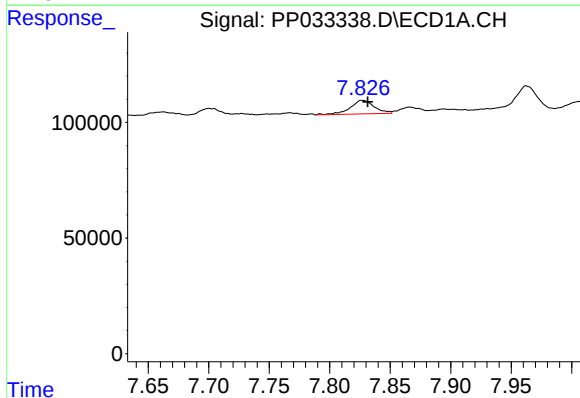


#29 AR-1254-4

R.T.: 7.827 min
Delta R.T.: -0.004 min
Response: 82067
Conc: 35.48 ng/ml

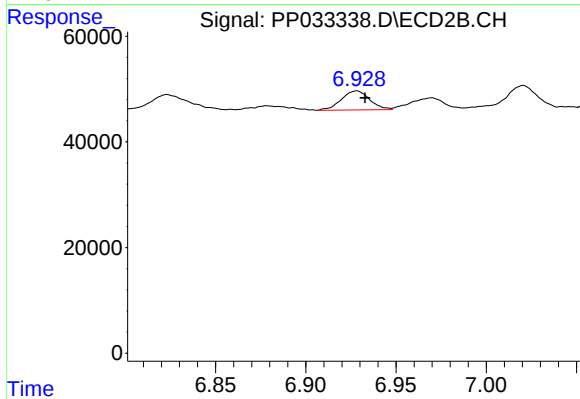

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.005 min
Response: 39445
Conc: 26.42 ng/ml

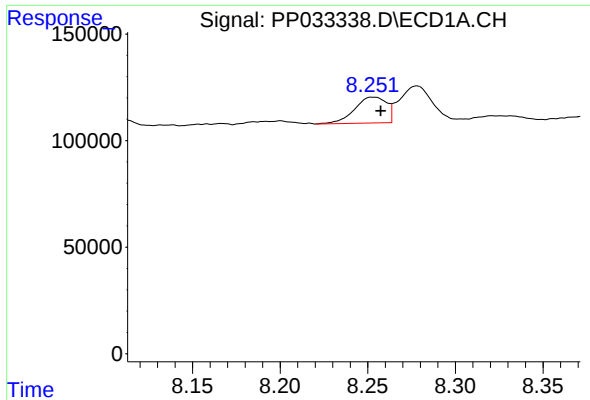


#30 AR-1254-5

R.T.: 8.253 min
Delta R.T.: -0.004 min
Response: 154129
Conc: 63.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-N9994

Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:01 AM

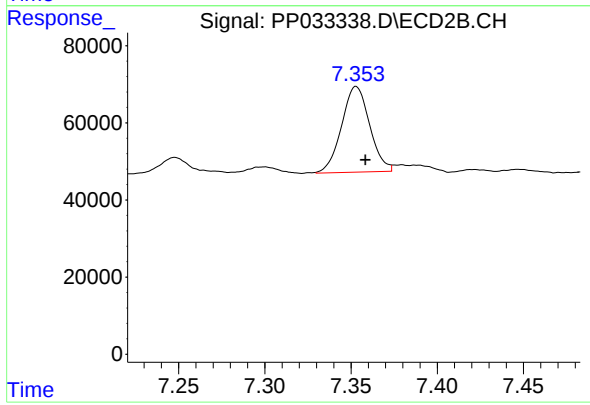

#30 AR-1254-5

R.T.: 7.353 min
Delta R.T.: -0.006 min
Response: 251487
Conc: 103.86 ng/ml m