

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
 Data File : PP033344.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2021 15:20
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/16/2021 8:57:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 15 16:22:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.733	4.000	3199583	1980714	52.177	48.438
2) SA Decachlor...	10.551	9.263	2281917	1652793	52.384m	49.337
Target Compounds						
21) L5 AR-1248-1	6.031	5.246	512166	332348	534.920	511.040
22) L5 AR-1248-2	6.323	5.508	644709	454150	486.547	473.390
23) L5 AR-1248-3	6.536	5.551	797207	484873	492.322m	476.882
24) L5 AR-1248-4	6.961	5.736	875701	586321	508.938	473.116
25) L5 AR-1248-5	7.001	6.157	855077	564097	491.423	499.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021521\
Data File : PP033344.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2021 15:20
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 15 16:22:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

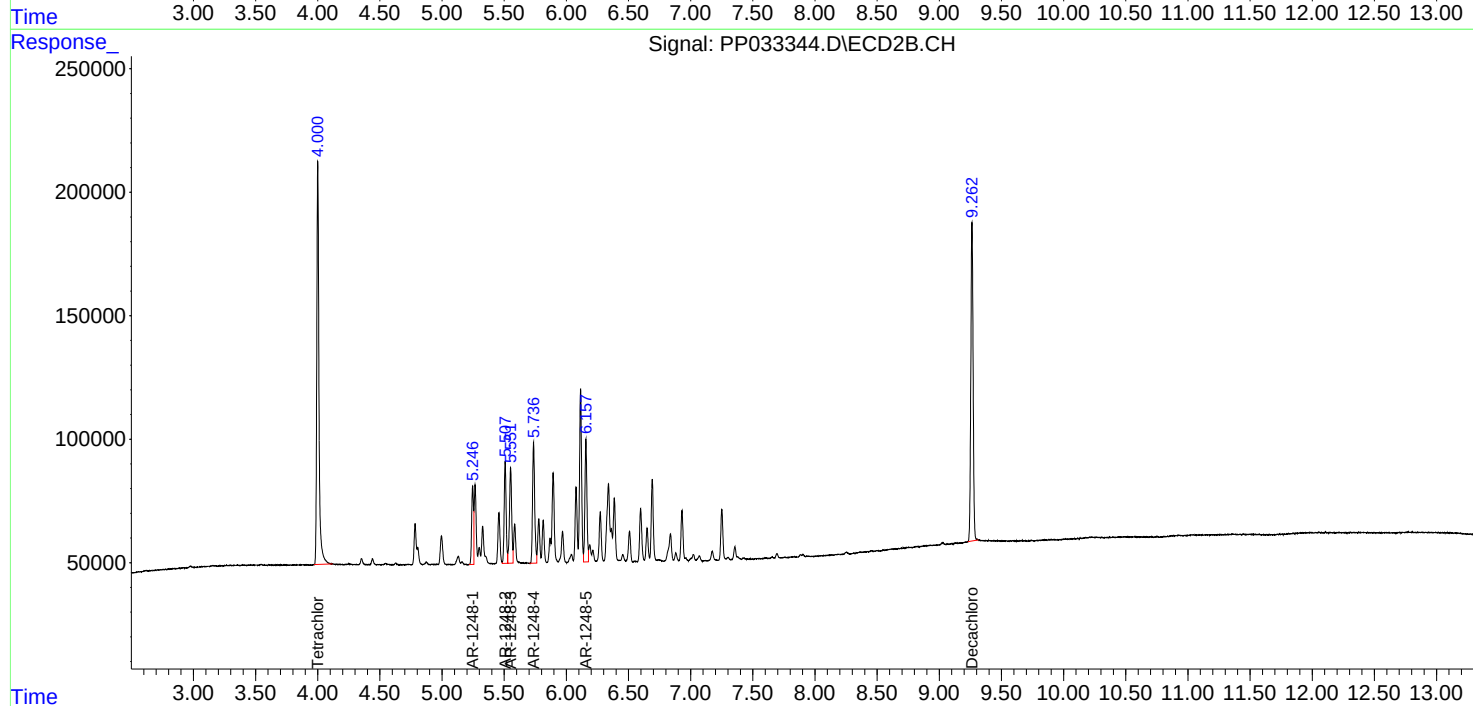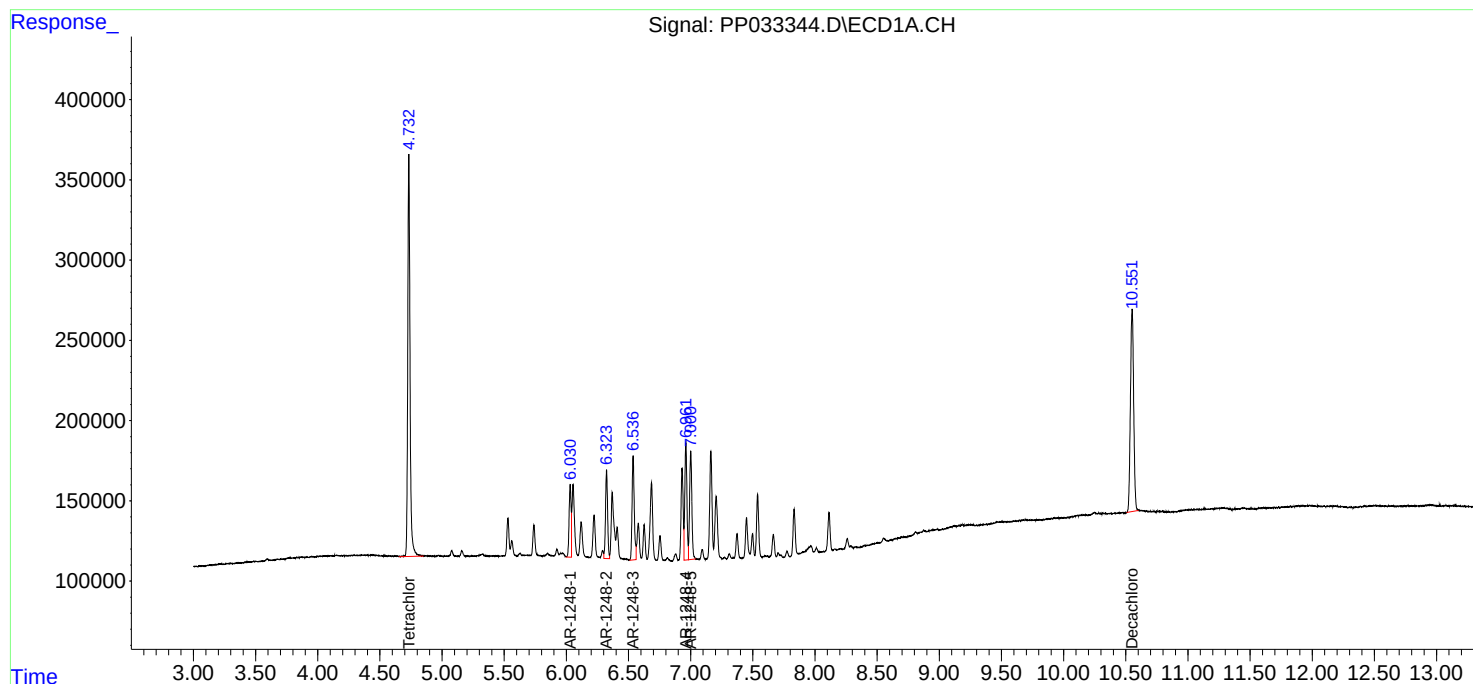

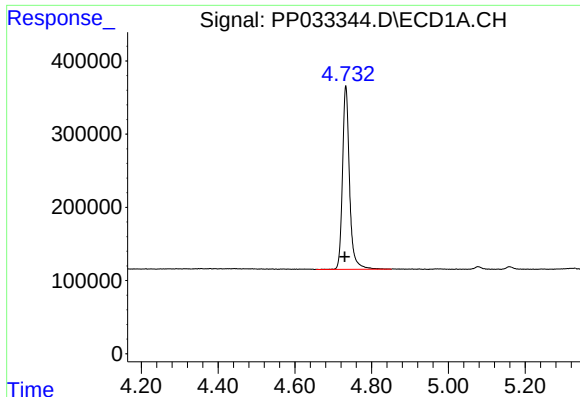


#1 Tetrachloro-m-xylene

R.T.: 4.733 min
Delta R.T.: 0.003 min
Response: 3199583
Conc: 52.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:25 AM

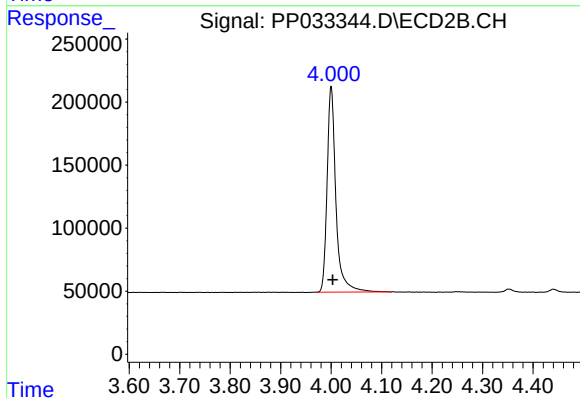


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1980714
Conc: 48.44 ng/ml

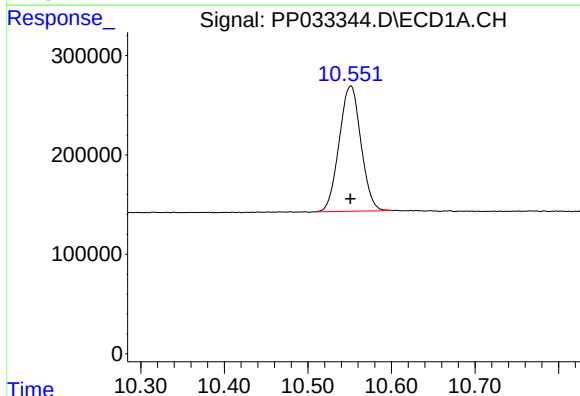


#2 Decachlorobiphenyl

R.T.: 10.551 min
Delta R.T.: 0.000 min
Response: 2281917
Conc: 52.38 ng/ml m

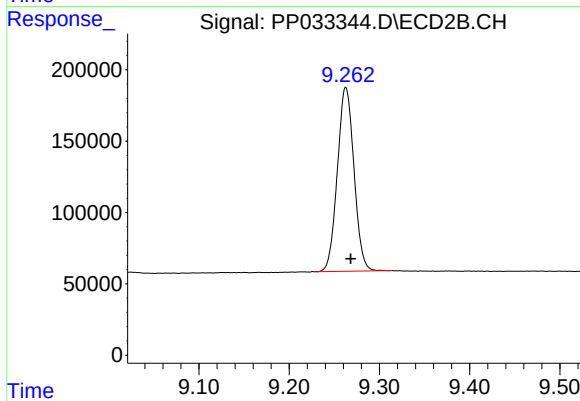

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: -0.006 min
Response: 1652793
Conc: 49.34 ng/ml

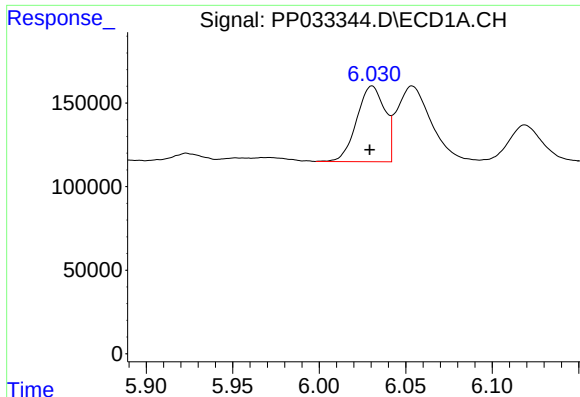


#21 AR-1248-1

R.T.: 6.031 min
Delta R.T.: 0.001 min
Response: 512166
Conc: 534.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:25 AM

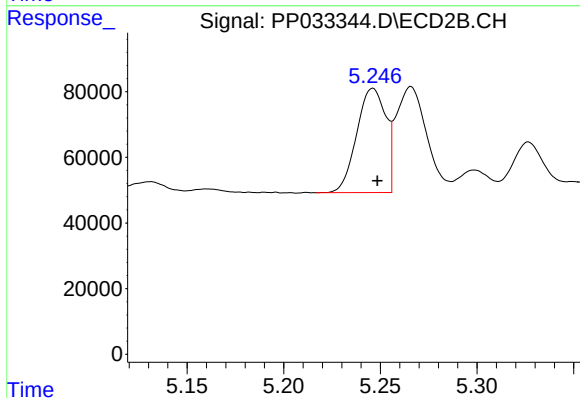


#21 AR-1248-1

R.T.: 5.246 min
Delta R.T.: -0.002 min
Response: 332348
Conc: 511.04 ng/ml

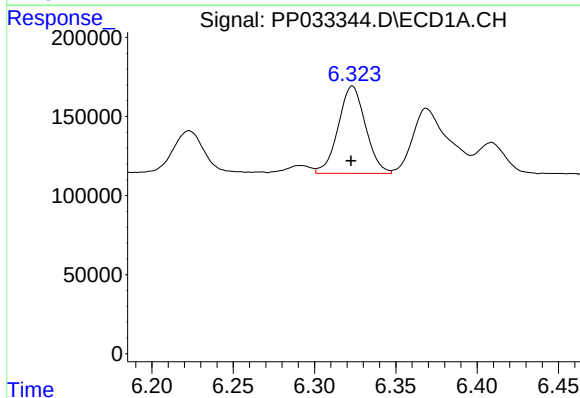


#22 AR-1248-2

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 644709
Conc: 486.55 ng/ml

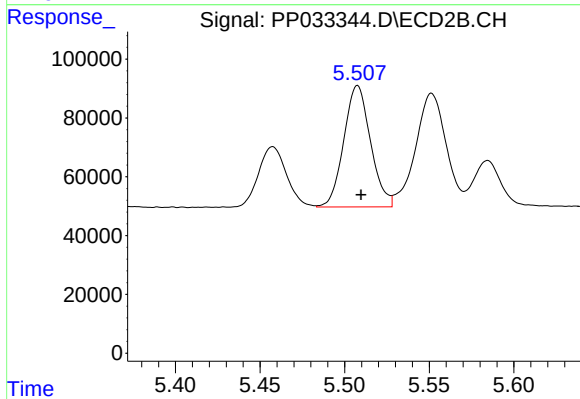

#22 AR-1248-2

R.T.: 5.508 min
Delta R.T.: -0.002 min
Response: 454150
Conc: 473.39 ng/ml

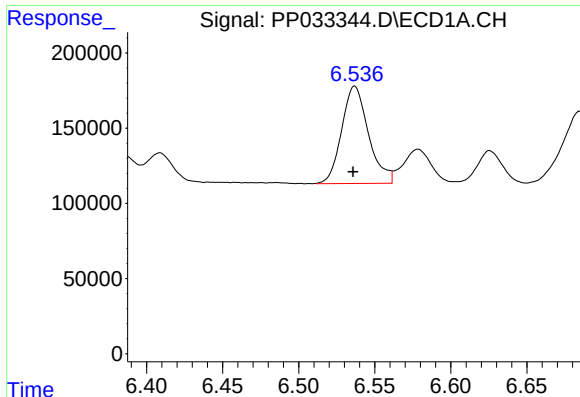


#23 AR-1248-3

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 797207
Conc: 492.32 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:25 AM

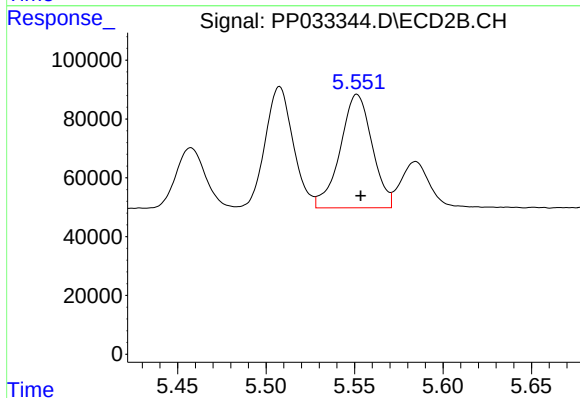


#23 AR-1248-3

R.T.: 5.551 min
Delta R.T.: -0.002 min
Response: 484873
Conc: 476.88 ng/ml

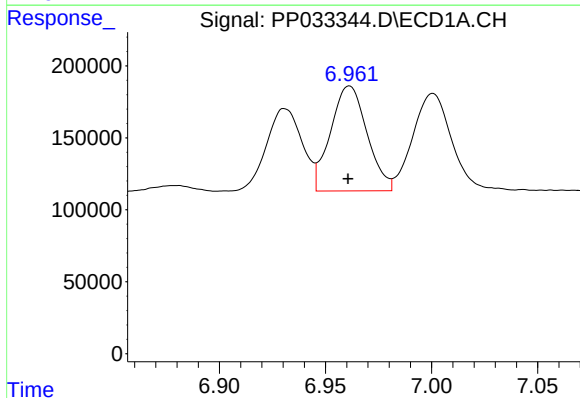


#24 AR-1248-4

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 875701
Conc: 508.94 ng/ml

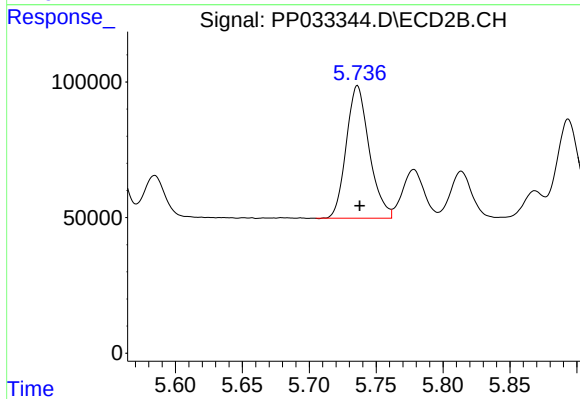

#24 AR-1248-4

R.T.: 5.736 min
Delta R.T.: -0.002 min
Response: 586321
Conc: 473.12 ng/ml

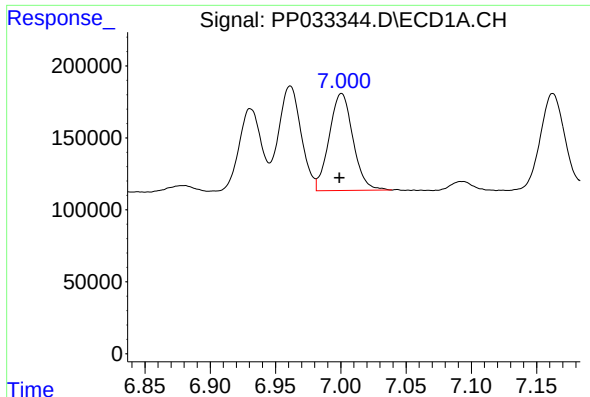


#25 AR-1248-5

R.T.: 7.001 min
Delta R.T.: 0.002 min
Response: 855077
Conc: 491.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/16/2021 8:57:25 AM

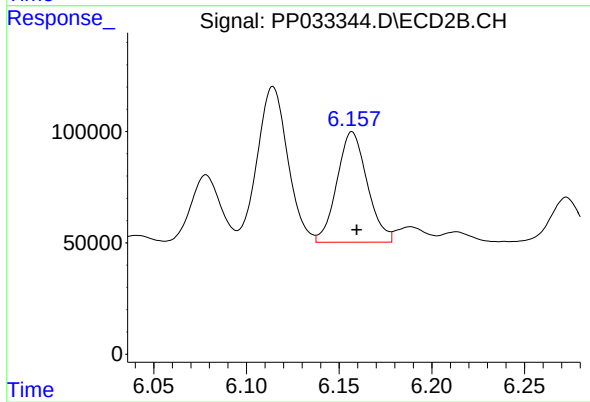

#25 AR-1248-5

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 564097
Conc: 499.50 ng/ml