

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021522\
 Data File : PP043766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2022 22:30
 Operator : YP\AJ
 Sample : N1537-29 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-2022-54A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:50:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.918	3.174	3799229	3873528	1.718	2.062
2) SA Decachlor...	10.063	8.549	2585483	3120927	2.177	1.924
Target Compounds						
26) L6 AR-1254-1	6.098	5.176	4175670	5416763	55.266m	62.025
27) L6 AR-1254-2	6.337	5.336	5933791	4871091	52.901	63.860
28) L6 AR-1254-3	6.737	5.769	5494487	6766779	47.484	55.213
29) L6 AR-1254-4	7.051	6.018	4218040	4643114	52.835	58.829
30) L6 AR-1254-5	7.511	6.470	4705068	6075862	54.861m	52.539



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021522\
Data File : PP043766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2022 22:30
Operator : YP\AJ
Sample : N1537-29 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IRV-2022-54A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:50:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

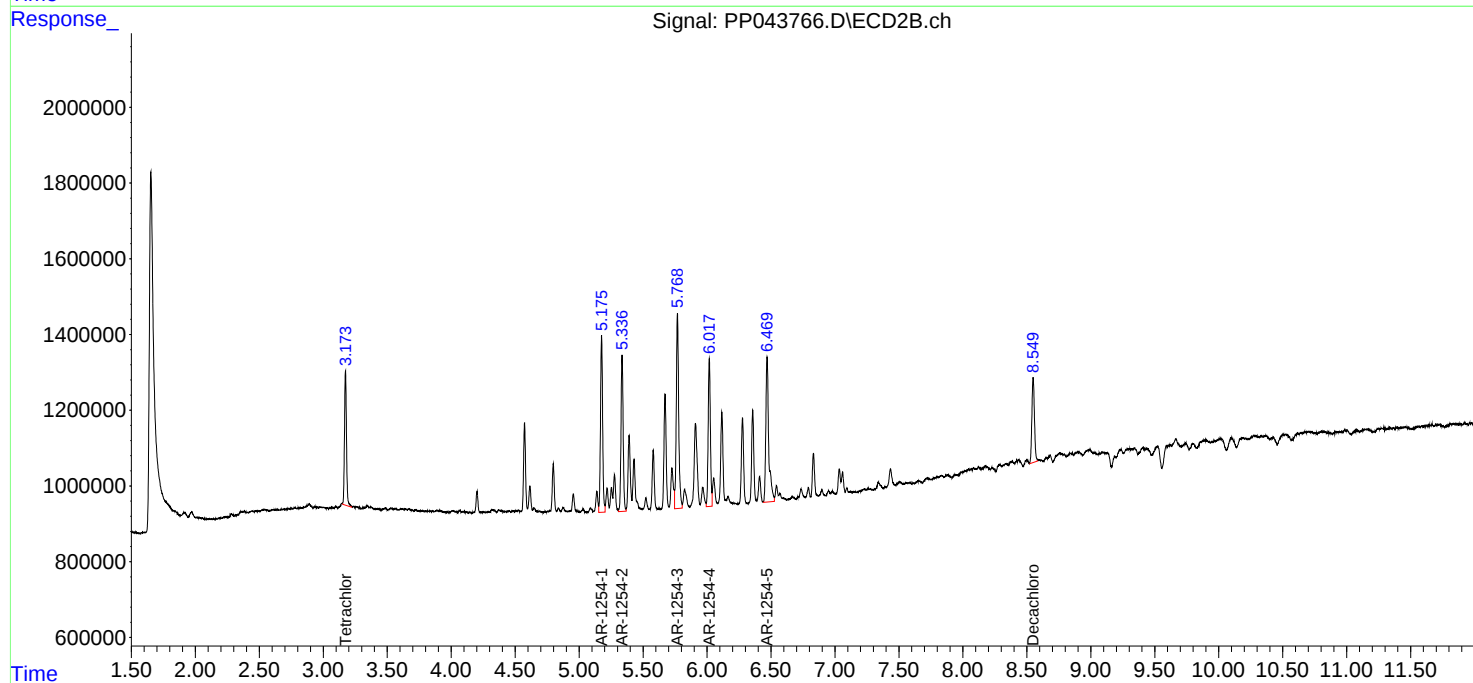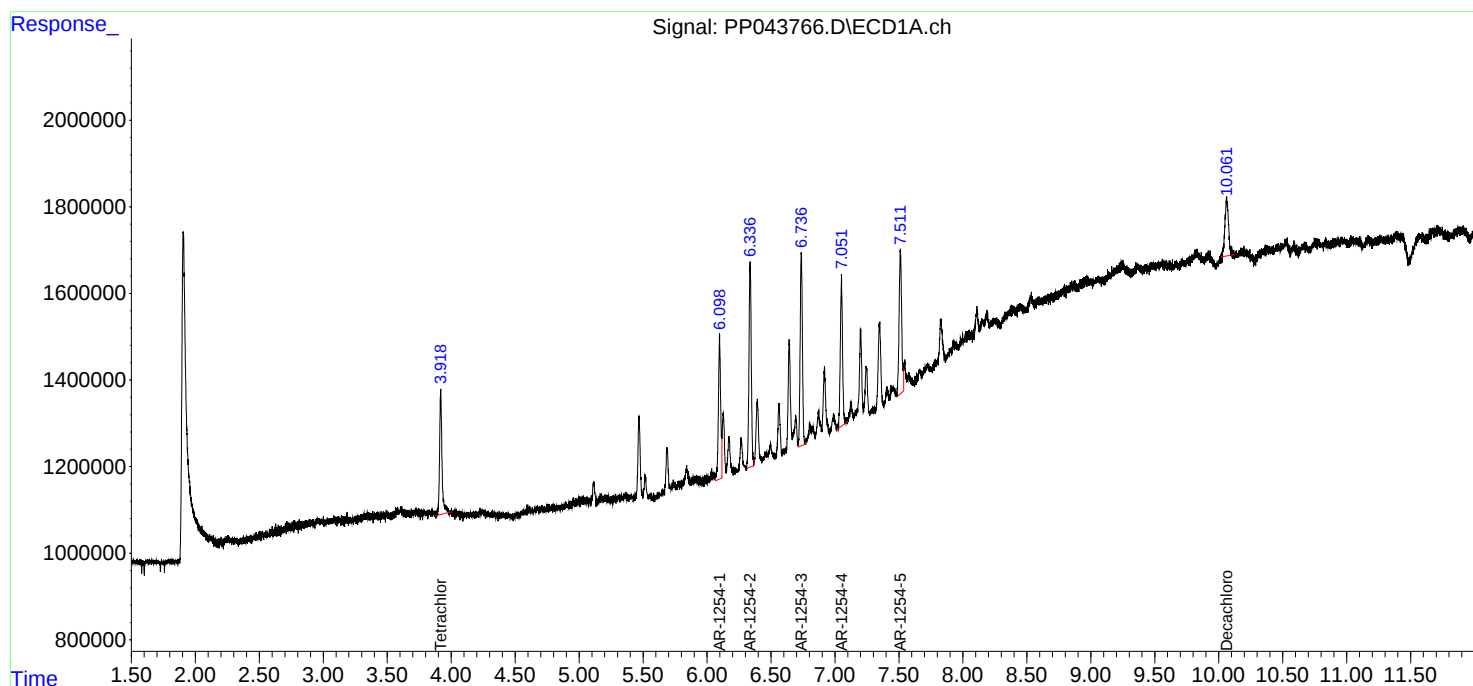


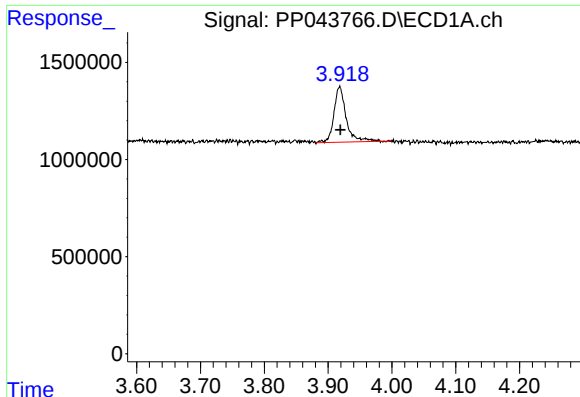

#1 Tetrachloro-m-xylene


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 3799229
Conc: 1.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-54A

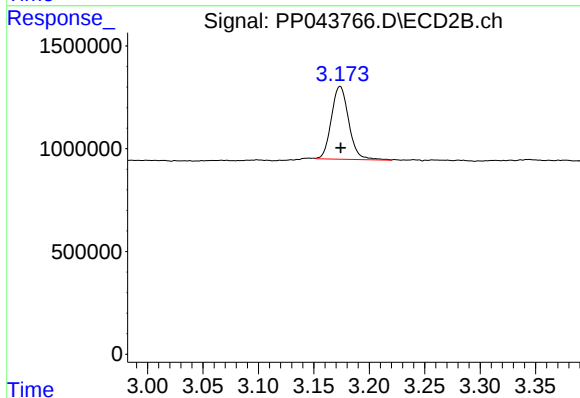


#1 Tetrachloro-m-xylene

R.T.: 3.174 min
Delta R.T.: 0.000 min
Response: 3873528
Conc: 2.06 ng/ml

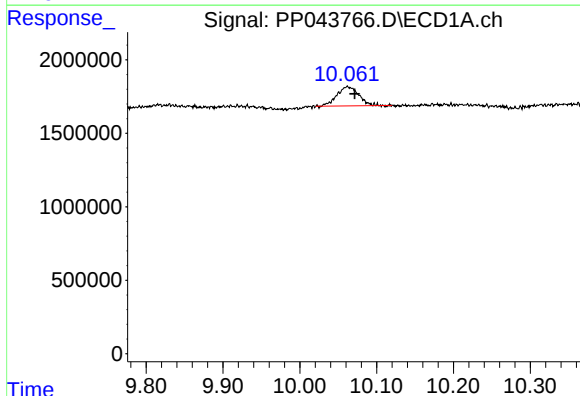


#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.009 min
Response: 2585483
Conc: 2.18 ng/ml

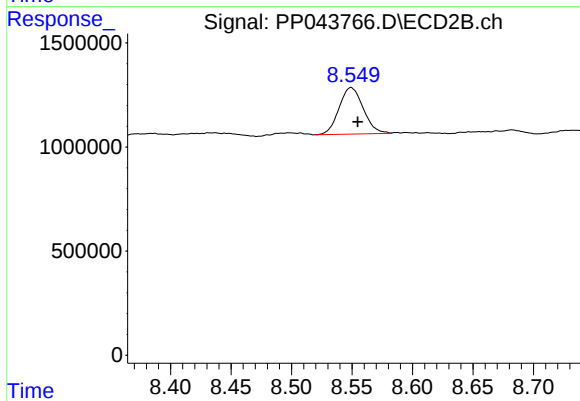

#2 Decachlorobiphenyl


R.T.: 8.549 min
Delta R.T.: -0.006 min
Response: 3120927
Conc: 1.92 ng/ml

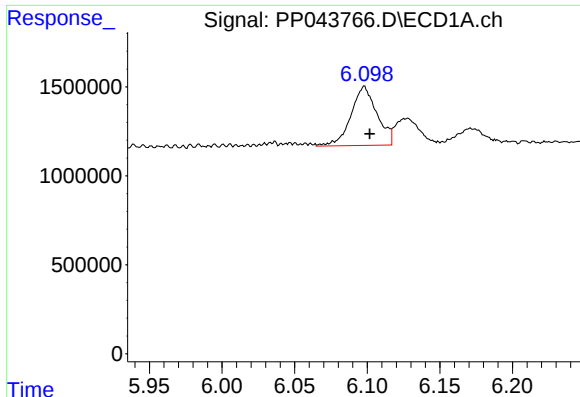

#26 AR-1254-1


R.T.: 6.098 min
Delta R.T.: -0.004 min
Response: 4175670
Conc: 55.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-54A

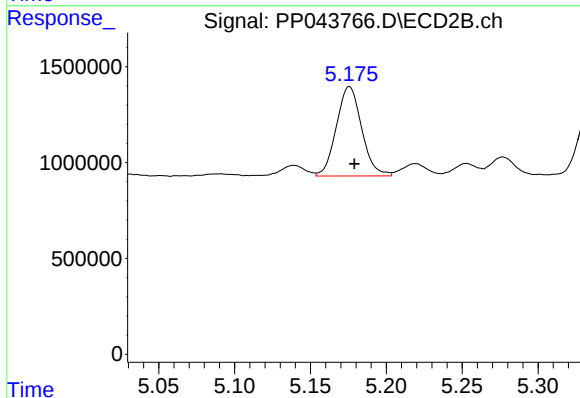


#26 AR-1254-1

R.T.: 5.176 min
Delta R.T.: -0.003 min
Response: 5416763
Conc: 62.02 ng/ml

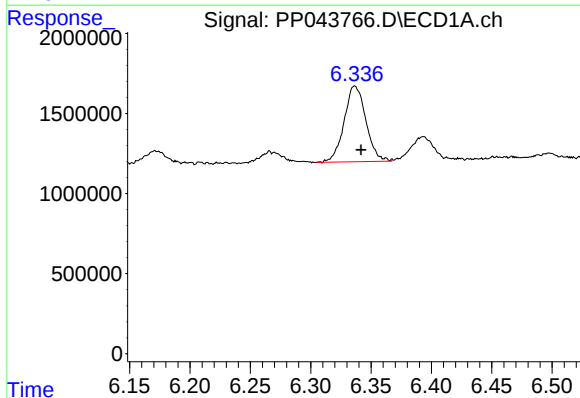


#27 AR-1254-2

R.T.: 6.337 min
Delta R.T.: -0.005 min
Response: 5933791
Conc: 52.90 ng/ml

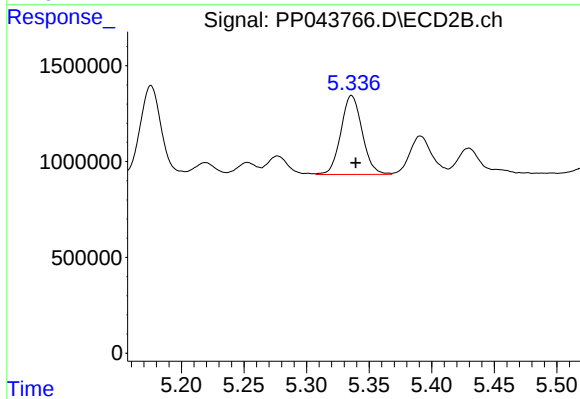

#27 AR-1254-2


R.T.: 5.336 min
Delta R.T.: -0.003 min
Response: 4871091
Conc: 63.86 ng/ml

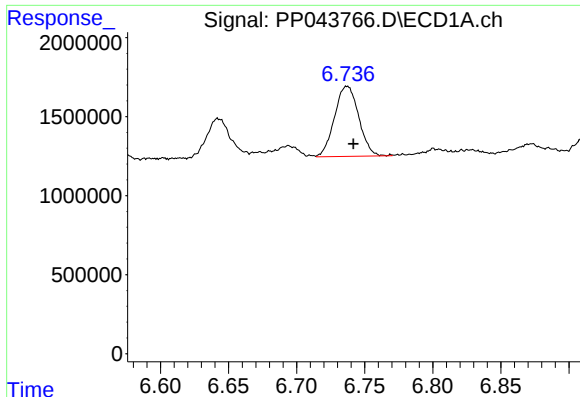

#28 AR-1254-3


R.T.: 6.737 min
Delta R.T.: -0.004 min
Response: 5494487
Conc: 47.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-54A

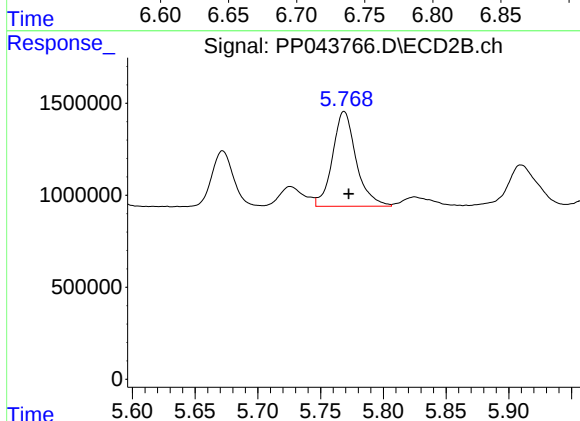


#28 AR-1254-3

R.T.: 5.769 min
Delta R.T.: -0.004 min
Response: 6766779
Conc: 55.21 ng/ml

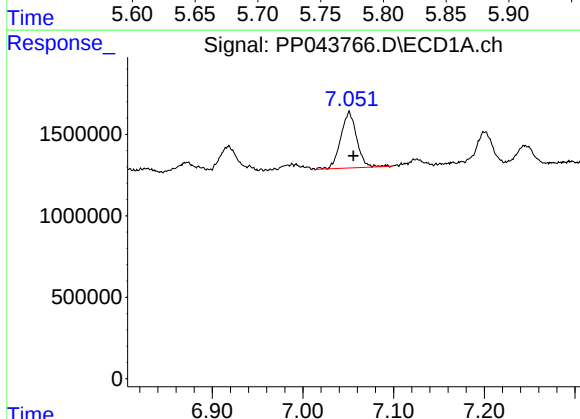


#29 AR-1254-4

R.T.: 7.051 min
Delta R.T.: -0.005 min
Response: 4218040
Conc: 52.84 ng/ml

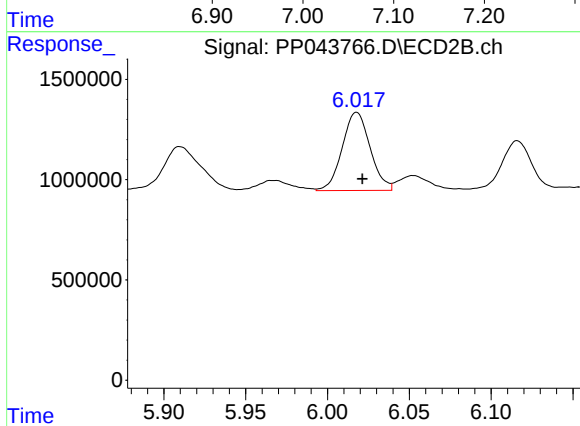

#29 AR-1254-4


R.T.: 6.018 min
Delta R.T.: -0.004 min
Response: 4643114
Conc: 58.83 ng/ml

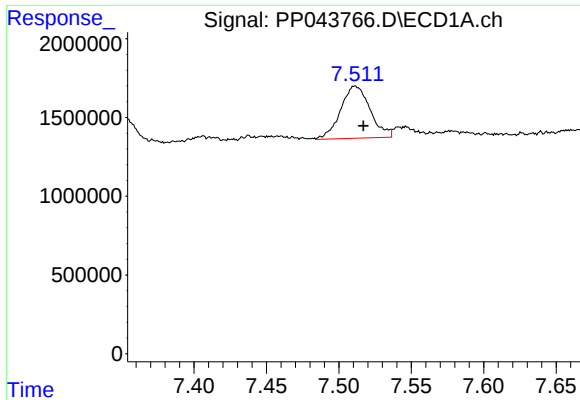

#30 AR-1254-5

R.T.: 7.511 min
Delta R.T.: -0.006 min
Response: 4705068
Conc: 54.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-54A

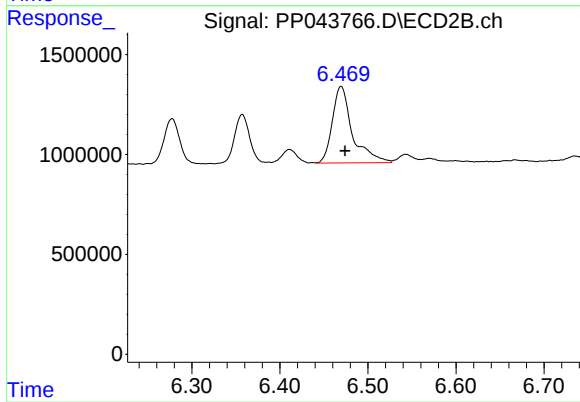

#30 AR-1254-5

R.T.: 6.470 min
Delta R.T.: -0.005 min
Response: 6075862
Conc: 52.54 ng/ml