

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP021621\  
 Data File : PP033354.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 16 Feb 2021 11:14  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 17 00:41:54 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP020821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Feb 09 04:00:57 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|---------|--------|--------|--------|
| -----                       |                 |        |       |         |        |        |        |
| System Monitoring Compounds |                 |        |       |         |        |        |        |
| 1)                          | SA Tetrachlo... | 4.736  | 4.002 | 1447861 | 834377 | 23.611 | 20.404 |
| 2)                          | SA Decachlor... | 10.560 | 9.269 | 1094156 | 739645 | 25.118 | 22.079 |

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP021621\  
Data File : PP033354.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 16 Feb 2021 11:14  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 17 00:41:54 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP020821.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Feb 09 04:00:57 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

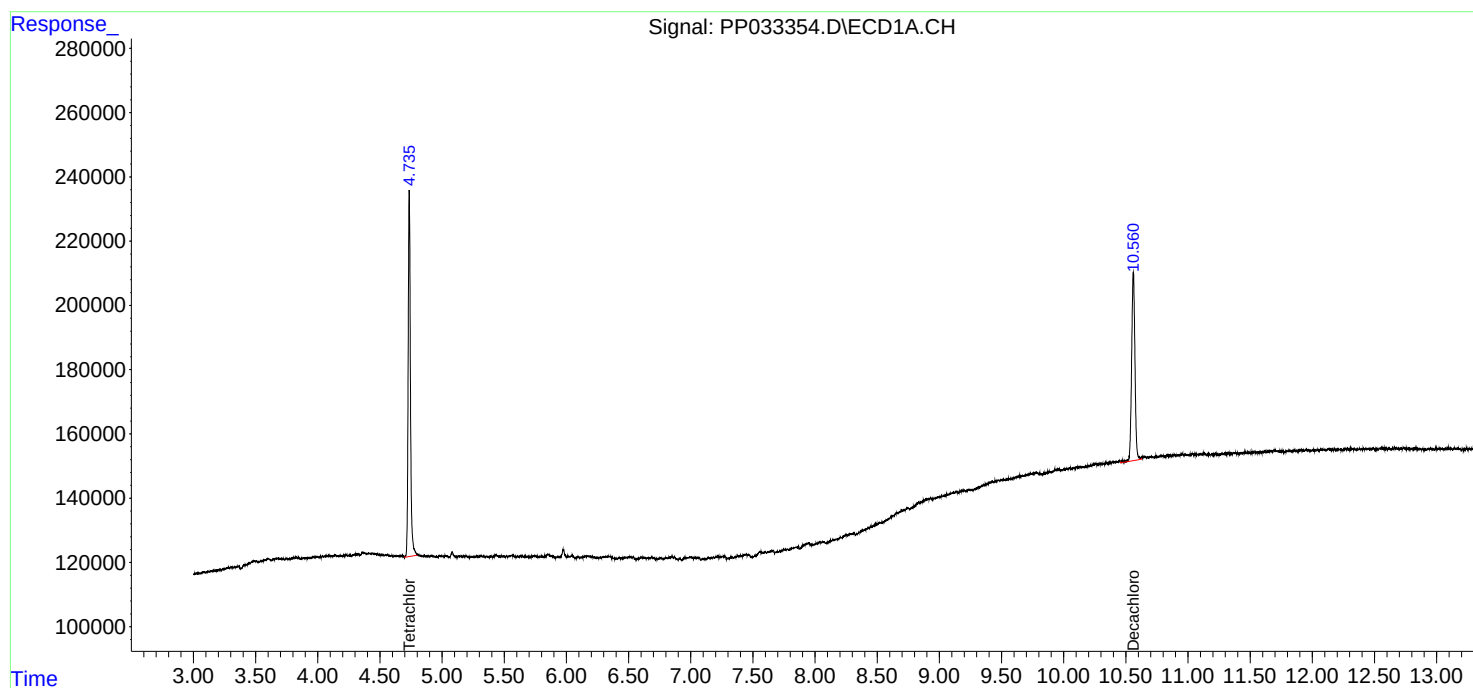


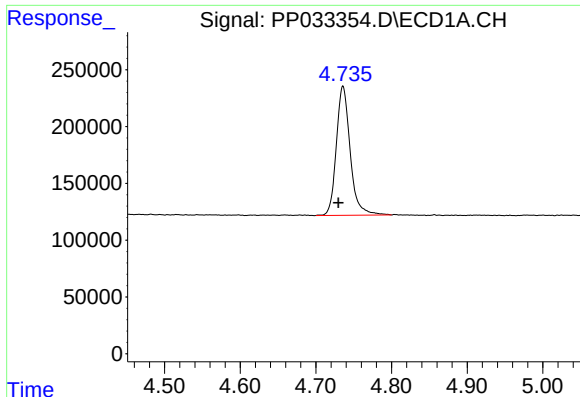

#1 Tetrachloro-m-xylene


R.T.: 4.736 min  
Delta R.T.: 0.006 min  
Response: 1447861  
Conc: 23.61 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

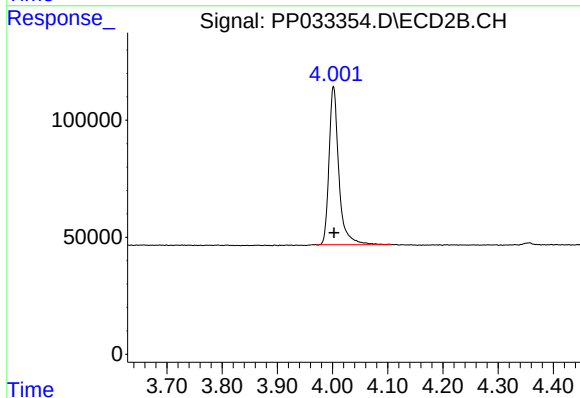


#1 Tetrachloro-m-xylene

R.T.: 4.002 min  
Delta R.T.: -0.001 min  
Response: 834377  
Conc: 20.40 ng/ml

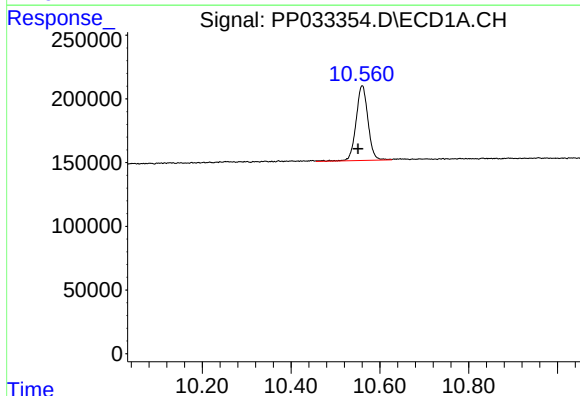

#2 Decachlorobiphenyl

R.T.: 10.560 min  
Delta R.T.: 0.009 min  
Response: 1094156  
Conc: 25.12 ng/ml

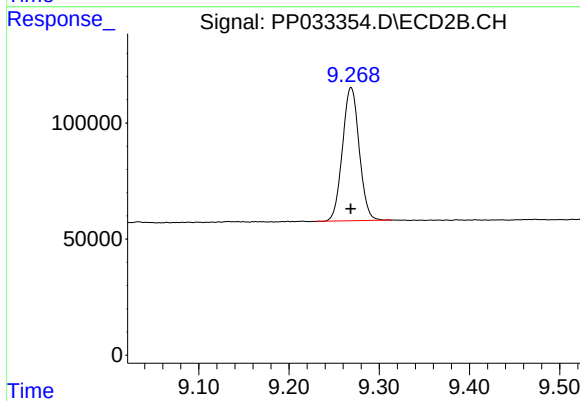

#2 Decachlorobiphenyl

R.T.: 9.269 min  
Delta R.T.: 0.000 min  
Response: 739645  
Conc: 22.08 ng/ml