

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021621\
 Data File : PP033355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Feb 2021 12:13
 Operator : DD\AJ
 Sample : 2.4 PEST/PCB SURR SPK TEST
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2.4 PEST/PCB SURR SPK TEST

Manual Integrations
 APPROVED

Ankita
 2/17/2021 11:38:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 00:42:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	4.004	14903228	8896953	243.031m	217.573
2) SA Decachlor...	10.571f	9.273	21917265	15216710	503.140	454.229

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021621\
Data File : PP033355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Feb 2021 12:13
Operator : DD\AJ
Sample : 2.4 PEST/PCB SURR SPK TEST
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
2.4 PEST/PCB SURR SPK TEST


Manual Integrations
APPROVED

Ankita
2/17/2021 11:38:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 00:42:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

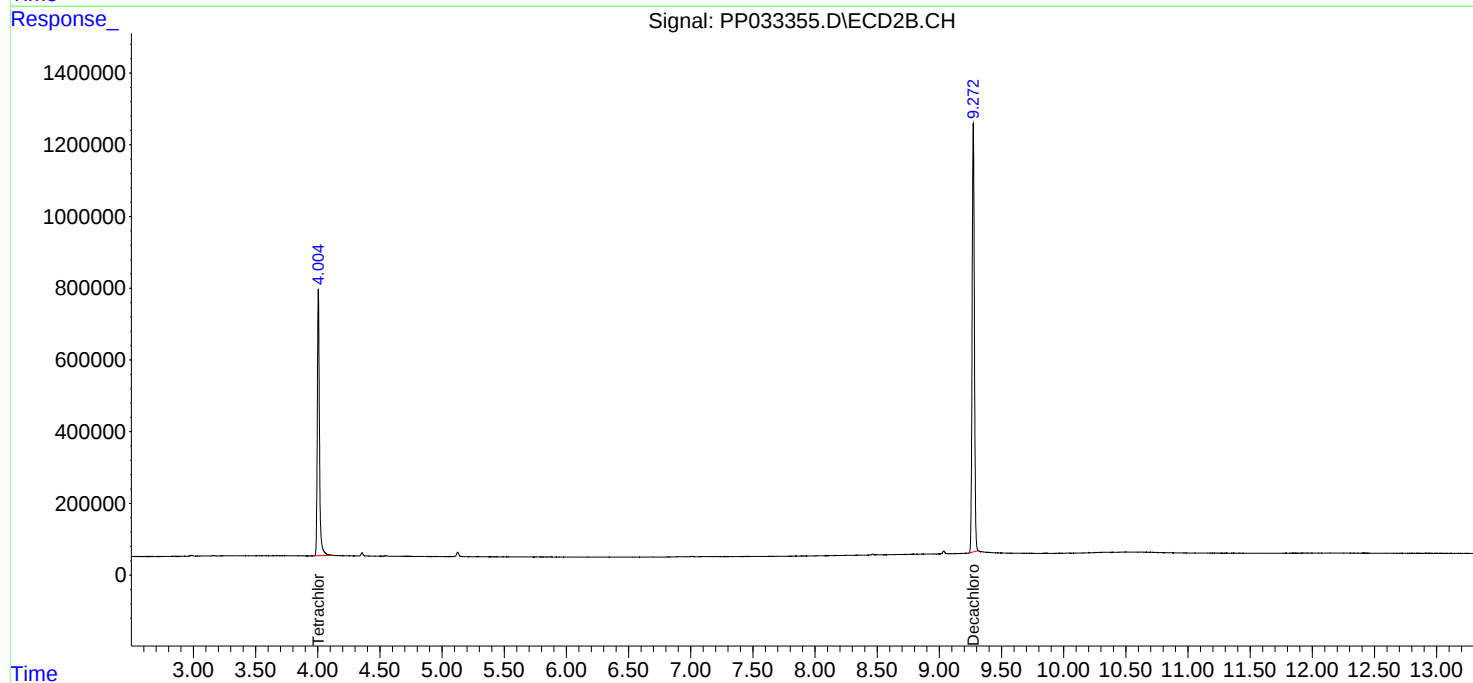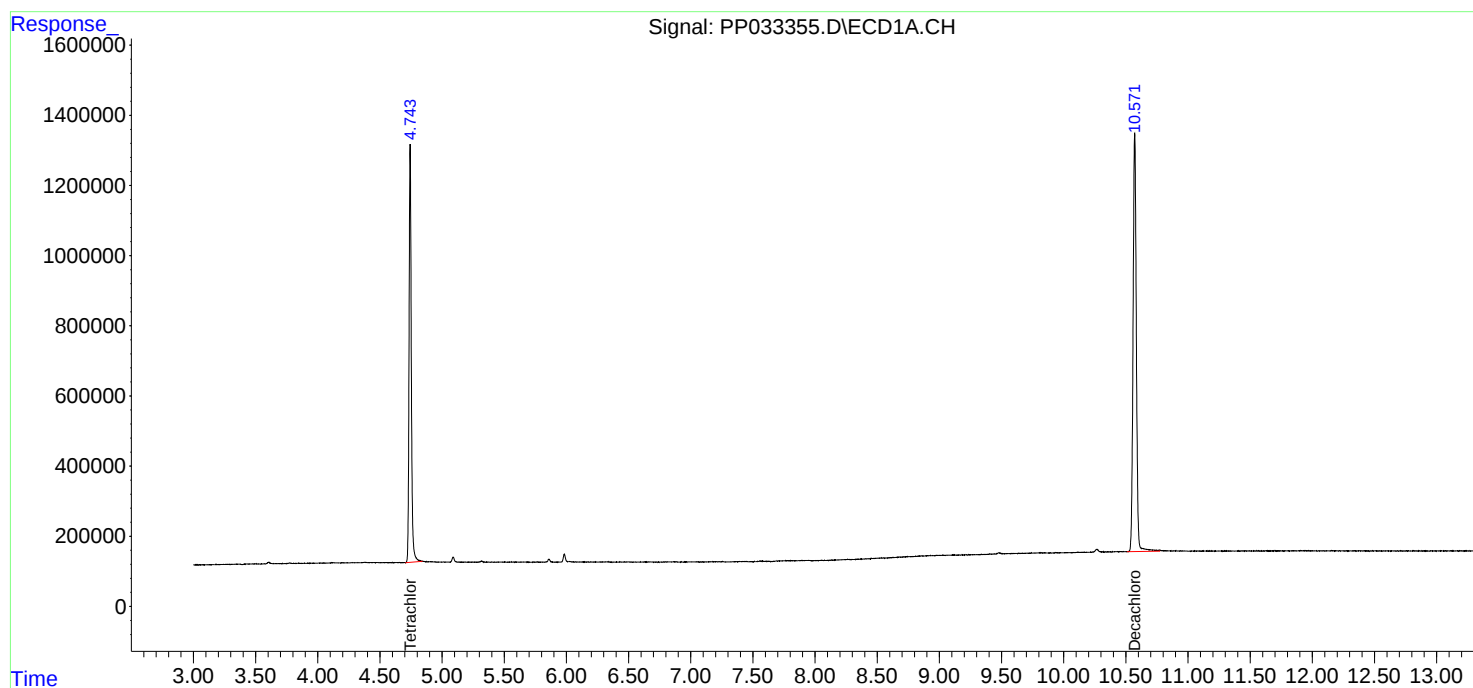

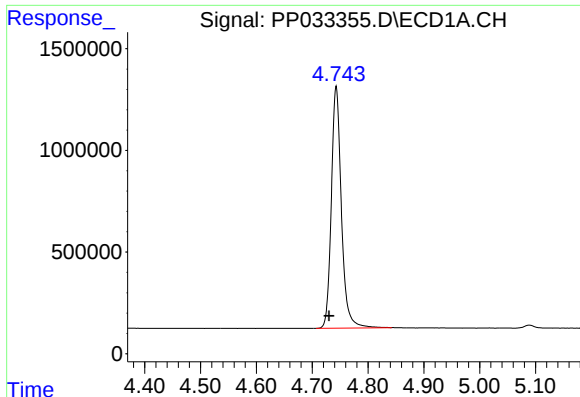


#1 Tetrachloro-m-xylene

R.T.: 4.743 min
Delta R.T.: 0.013 min
Response: 14903228
Conc: 243.03 ng/ml m

Instrument :
ECD_P
ClientSampleId :
2.4 PEST/PCB SURR SPK TEST


Manual Integrations
APPROVED

Ankita
2/17/2021 11:38:37 AM

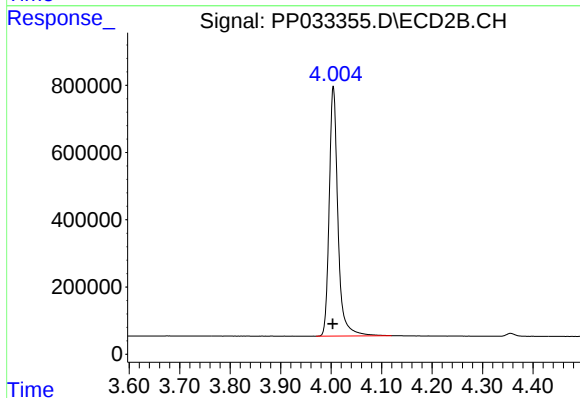


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: 0.001 min
Response: 8896953
Conc: 217.57 ng/ml

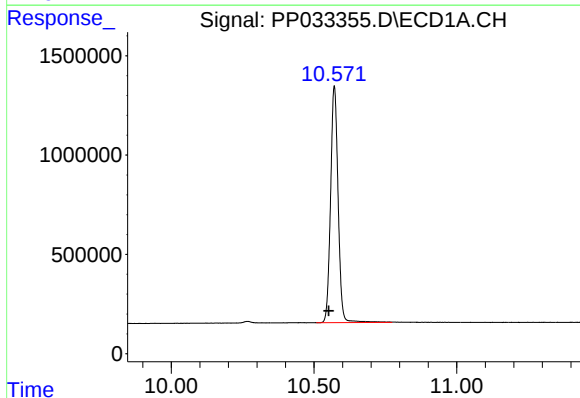

#2 Decachlorobiphenyl

R.T.: 10.571 min
Delta R.T.: 0.020 min
Response: 21917265
Conc: 503.14 ng/ml

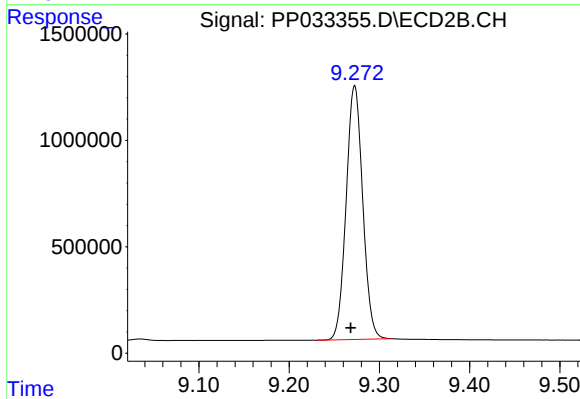

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 15216710
Conc: 454.23 ng/ml