

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021623\
 Data File : PD073979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 10:00
 Operator : AR\AJ
 Sample : PB150881BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 20:22:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.776	41367598	22022510	17.468	17.349
27)	SA Decachlor...	9.113	7.936	95221927	42232956	34.514	35.091
Target Compounds							
4)	MA Heptachlor	4.890f	0.000	128302	0	<MDL	N.D. #
6)	B beta-BHC	0.000	3.871f	0	300882	N.D.	0.368
7)	B delta-BHC	4.791	0.000	2320701	0	0.710	N.D. #
9)	A Endosulfan I	6.084	0.000	210654	0	<MDL	N.D. #
10)	B trans-Chl...	6.011f	0.000	946366	0	0.294	N.D. #
11)	B cis-Chlor...	6.011	0.000	946366	0	0.284	N.D. #
15)	B Endosulfa...	6.813	0.000	204581	0	<MDL	N.D. #
20)	A Methoxychlor	7.457f	0.000	297990	0	0.200	N.D. #
21)	B Endrin ke...	7.685	0.000	1521563	0	0.477	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD021623\
Data File : PD073979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 10:00
Operator : AR\AJ
Sample : PB150881BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 20:22:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

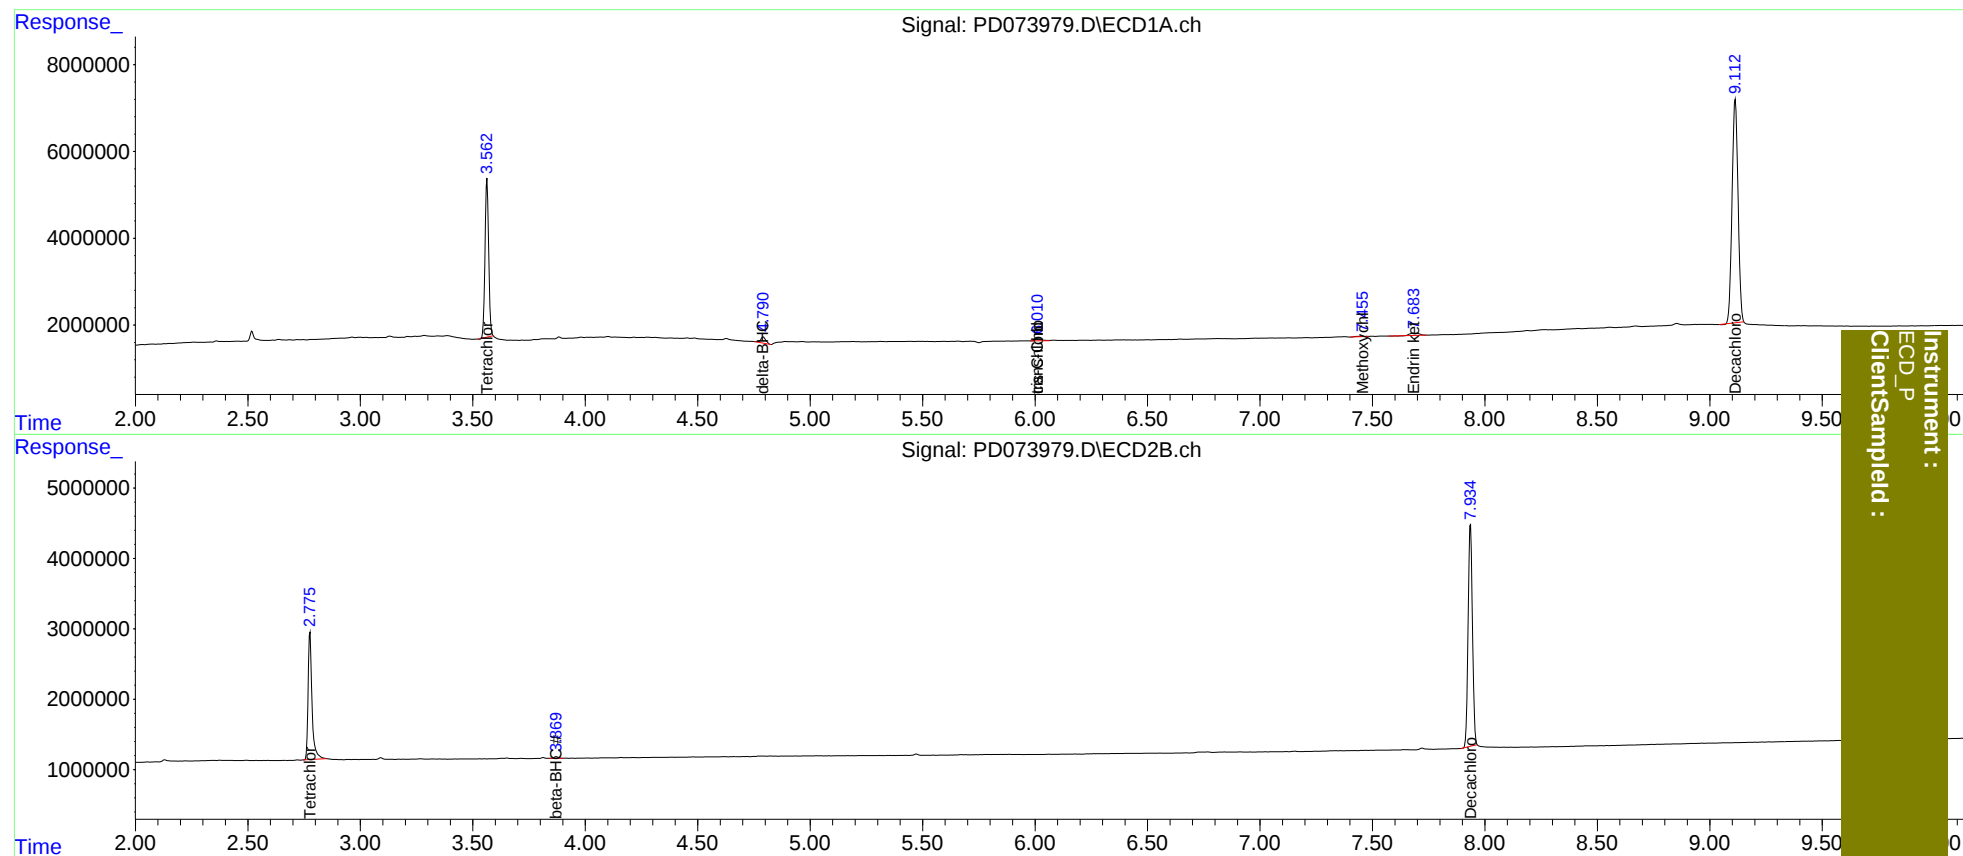


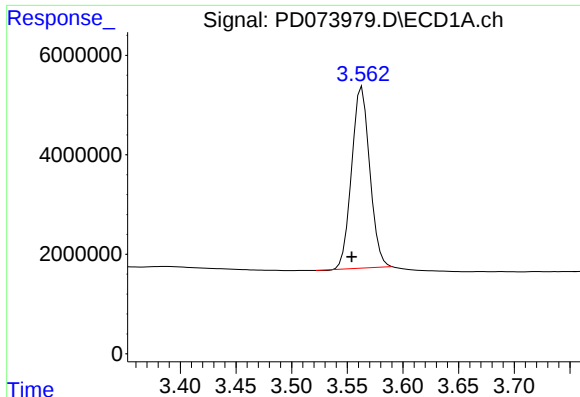

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.009 min
Response: 41367598
Conc: 17.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

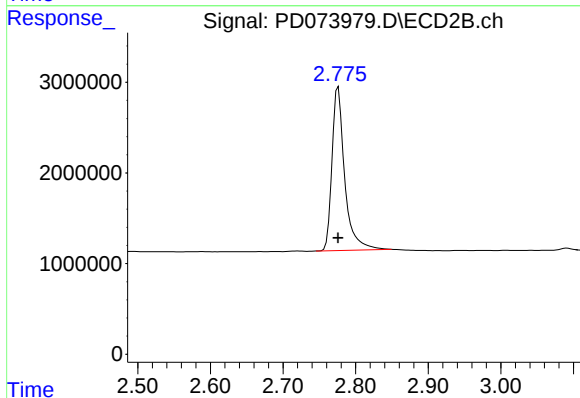


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 22022510
Conc: 17.35 ng/ml

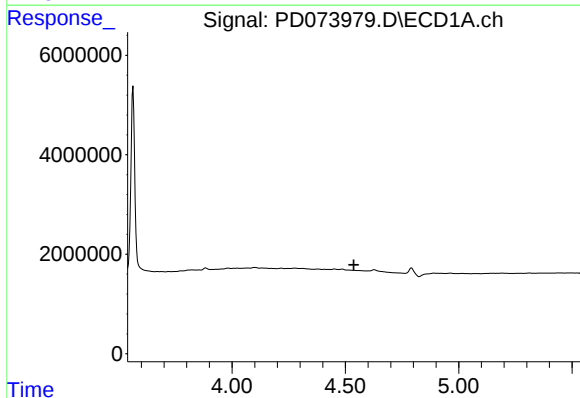


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.537 min
Response: 0
Conc: N.D.

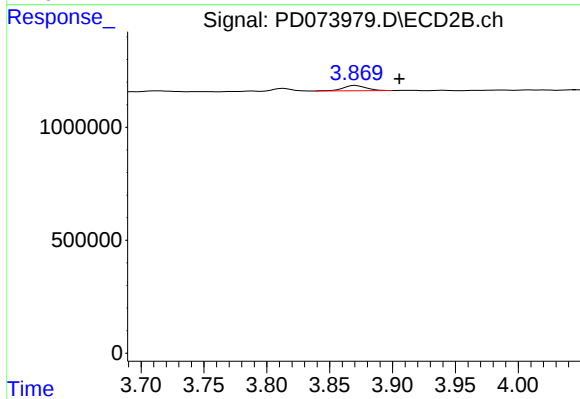

#6 beta-BHC


R.T.: 3.871 min
Delta R.T.: -0.035 min
Response: 300882
Conc: 0.37 ng/ml

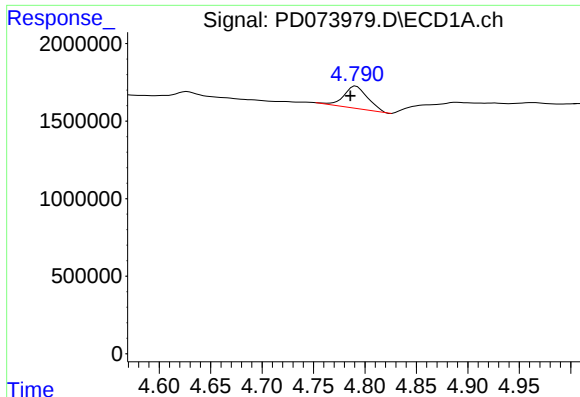

#7 delta-BHC


R.T.: 4.791 min
Delta R.T.: 0.006 min
Response: 2320701
Conc: 0.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

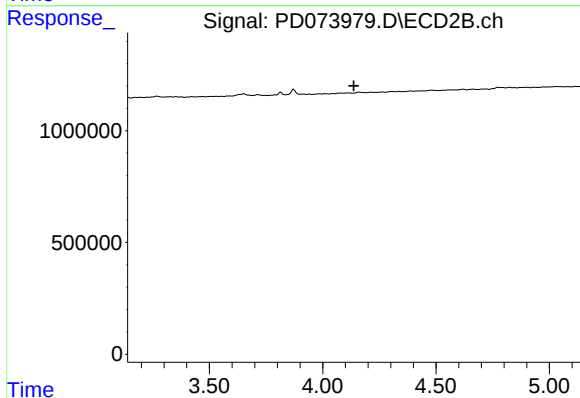


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

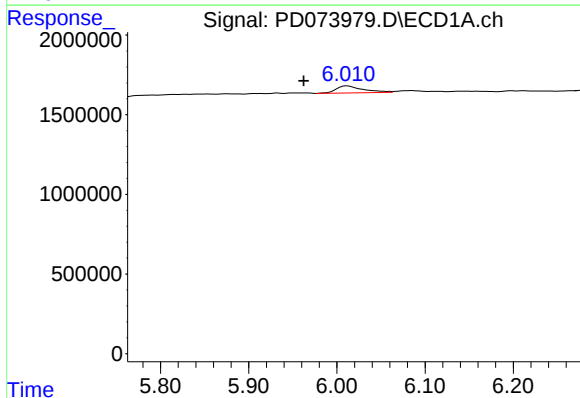


#10 trans-Chlordane

R.T.: 6.011 min
Delta R.T.: 0.049 min
Response: 946366
Conc: 0.29 ng/ml

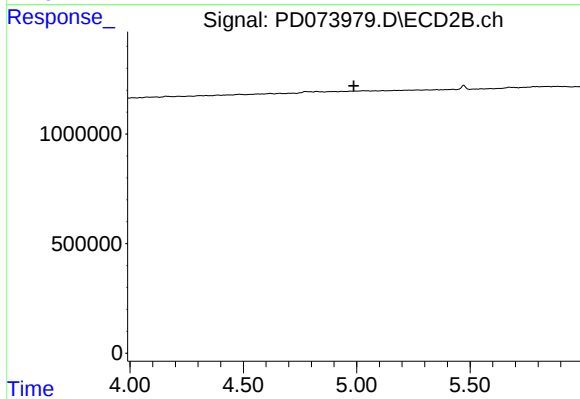

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

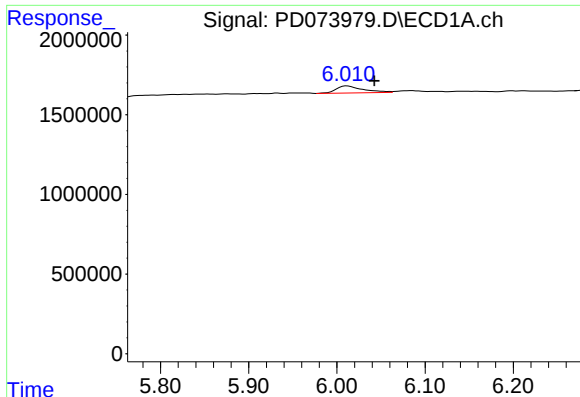

#11 cis-Chlordane


R.T.: 6.011 min
Delta R.T.: -0.031 min
Response: 946366
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

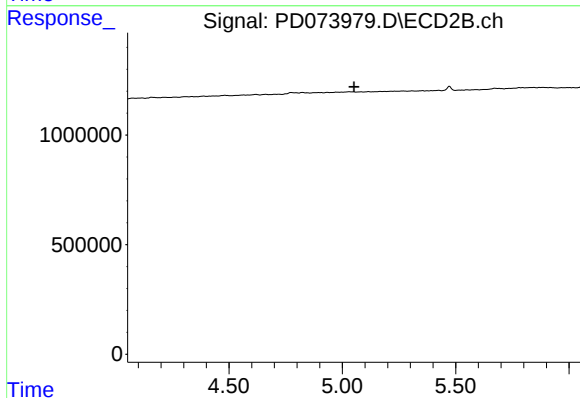


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.052 min
Response: 0
Conc: N.D.

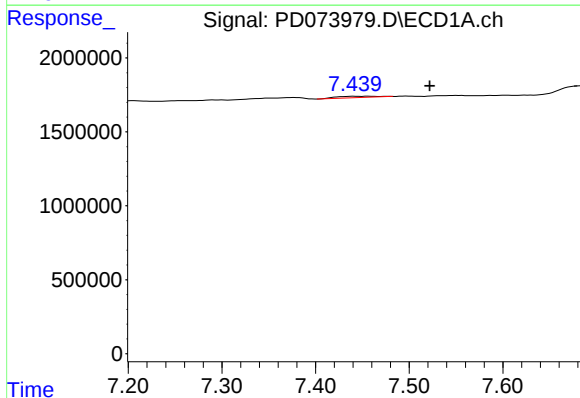


#20 Methoxychlor

R.T.: 7.457 min
Delta R.T.: -0.065 min
Response: 297990
Conc: 0.20 ng/ml

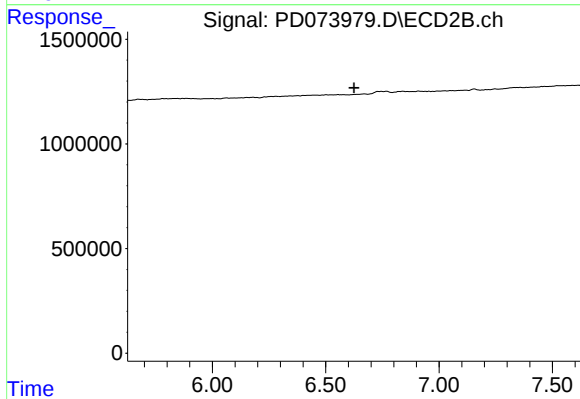

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.625 min
Response: 0
Conc: N.D.

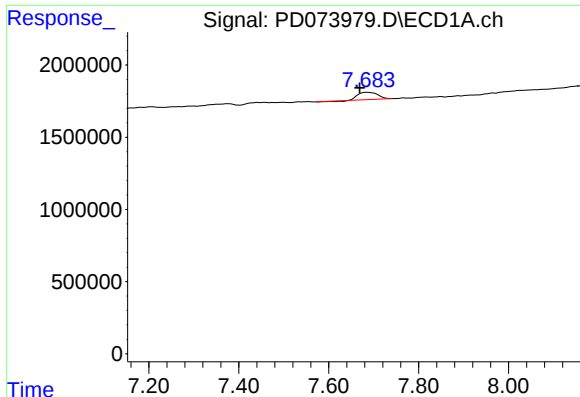

#21 Endrin ketone


R.T.: 7.685 min
Delta R.T.: 0.017 min
Response: 1521563
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

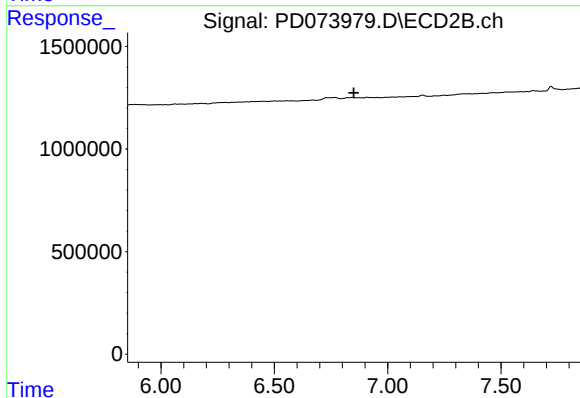


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.851 min
Response: 0
Conc: N.D.

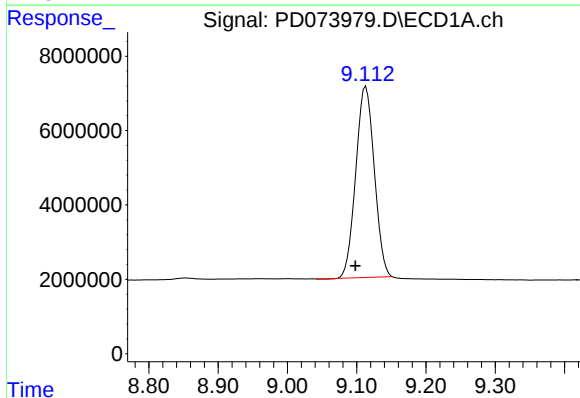

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.015 min
Response: 95221927
Conc: 34.51 ng/ml

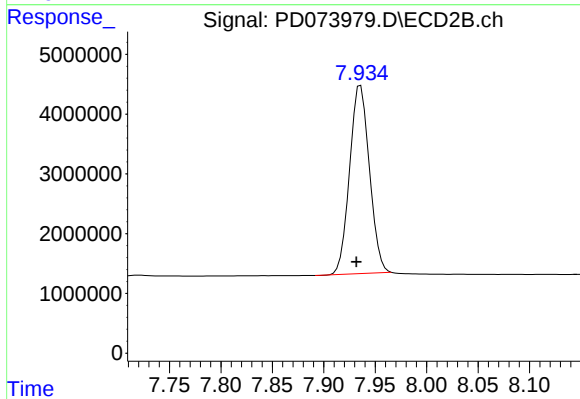

#27 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.004 min
Response: 42232956
Conc: 35.09 ng/ml