

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0021623\
 Data File : P0092471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 09:01
 Operator : YP/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 20:22:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7)	L1	AR-1016-5	0.000	5.219	0	552658	N.D. 13.898 #
15)	L3	AR-1232-5	0.000	5.219	0	552658	N.D. 30.898 #
20)	L4	AR-1242-5	0.000	5.560	0	428401	N.D. 11.834 #
24)	L5	AR-1248-4	0.000	5.219	0	552658	N.D. 10.286 #
25)	L5	AR-1248-5	0.000	5.560	0	428401	N.D. 9.049 #
26)	L6	AR-1254-1	0.000	5.560	0	428401	N.D. 5.465 #
28)	L6	AR-1254-3	0.000	6.105	0	141336	N.D. 1.324 #
38)	L8	AR-1262-3	8.816	0.000	1203861	0	7.122 N.D. #
39)	L8	AR-1262-4	8.880	0.000	568974	0	5.593 N.D. #
41)	L9	AR-1268-1	8.816	0.000	1203861	0	3.806 N.D. #
42)	L9	AR-1268-2	8.880	0.000	568974	0	1.885 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021623\
Data File : PO092471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 09:01
Operator : YP/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 20:22:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

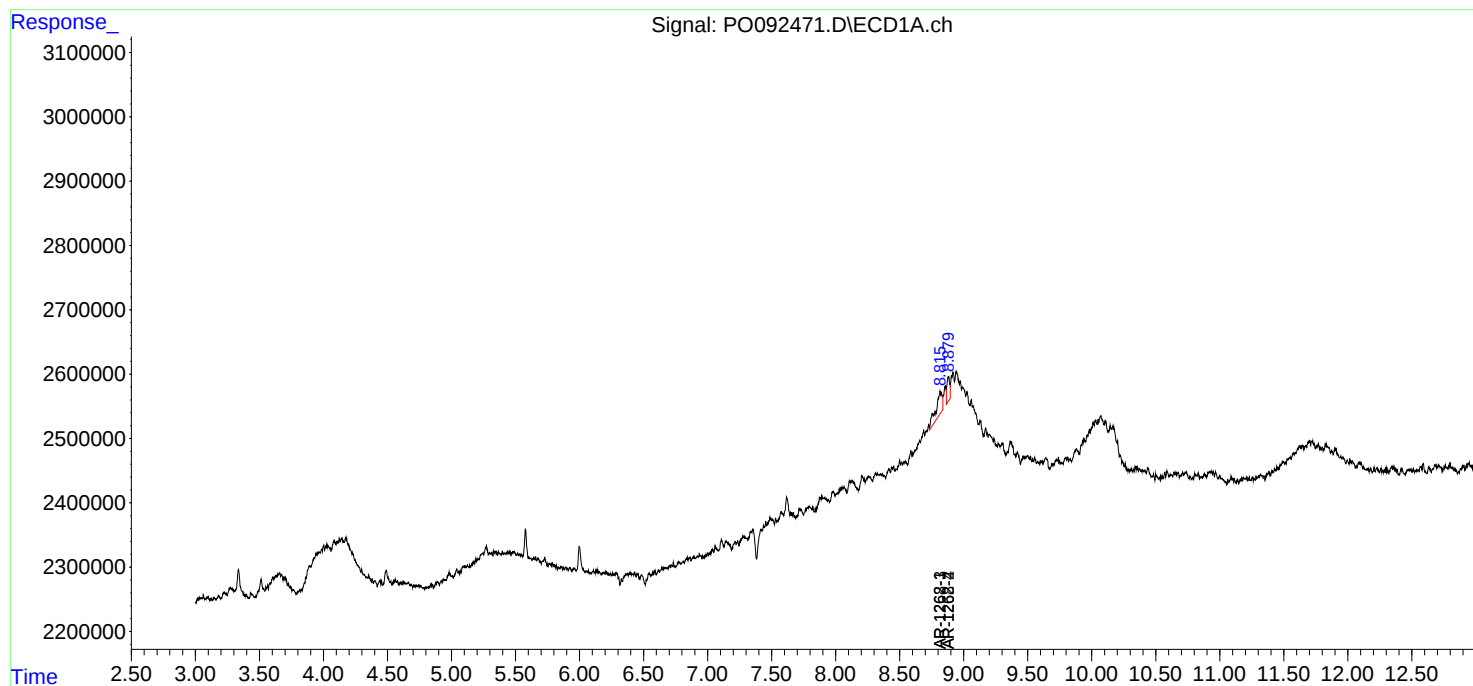


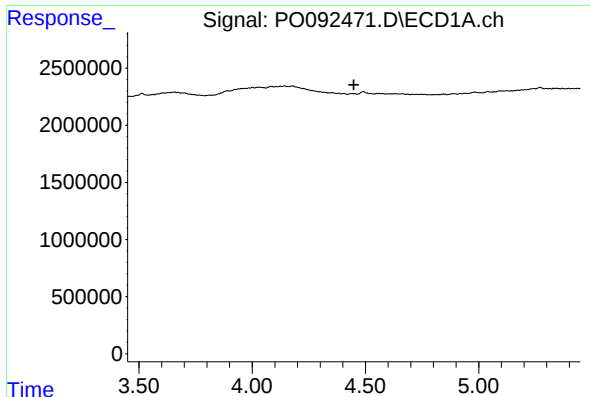

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

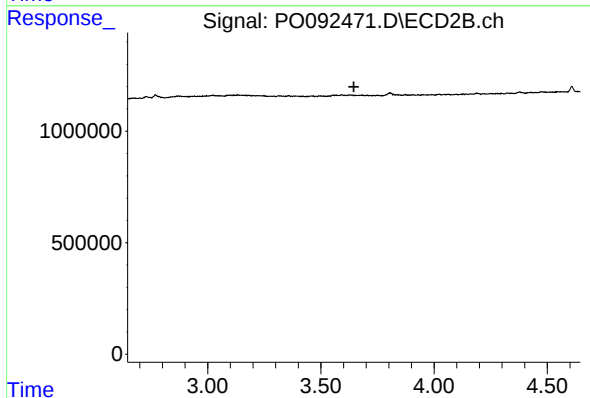


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.646 min
Response: 0
Conc: N.D.

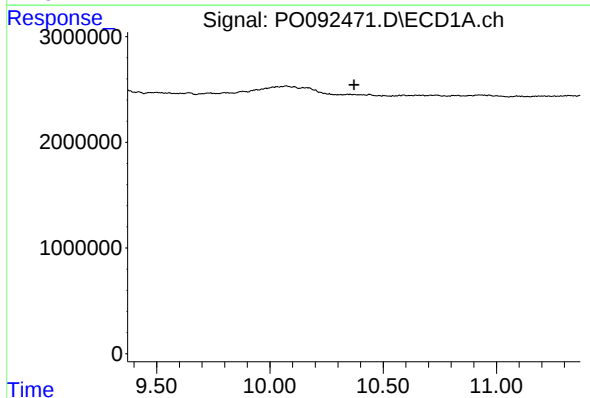


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.371 min
Response: 0
Conc: N.D.

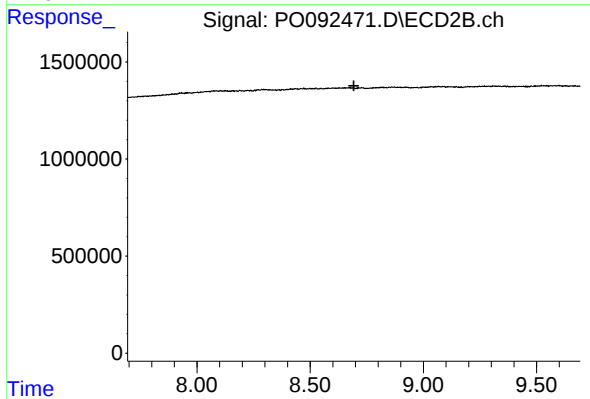

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.693 min
Response: 0
Conc: N.D.

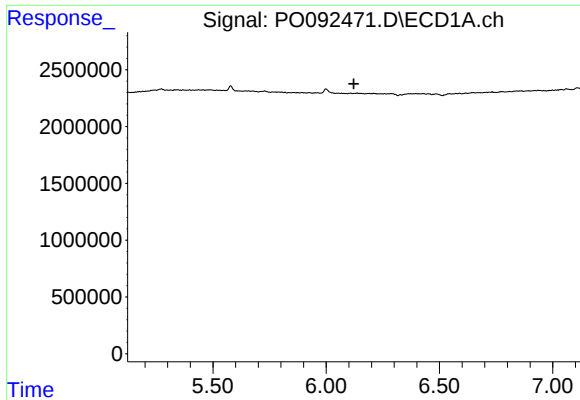

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

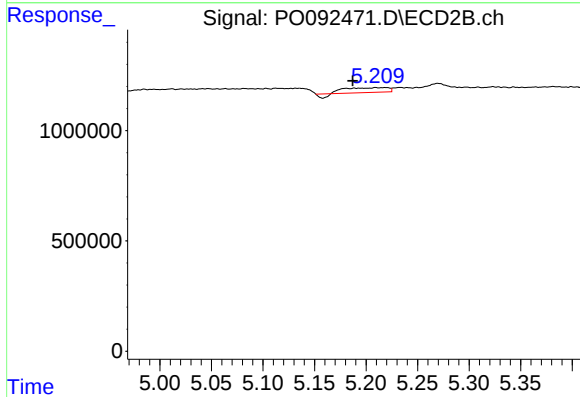


#7 AR-1016-5

R.T.: 5.219 min
Delta R.T.: 0.032 min
Response: 552658
Conc: 13.90 ng/ml

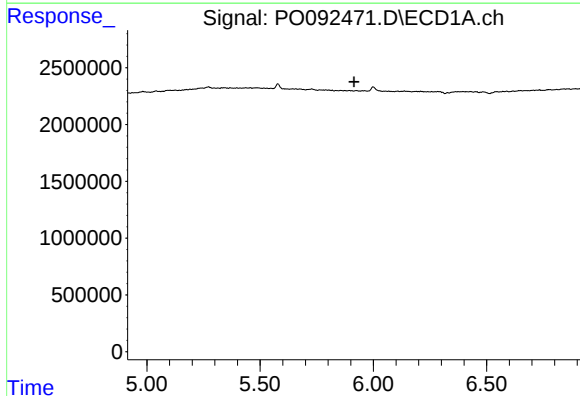


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.914 min
Response: 0
Conc: N.D.

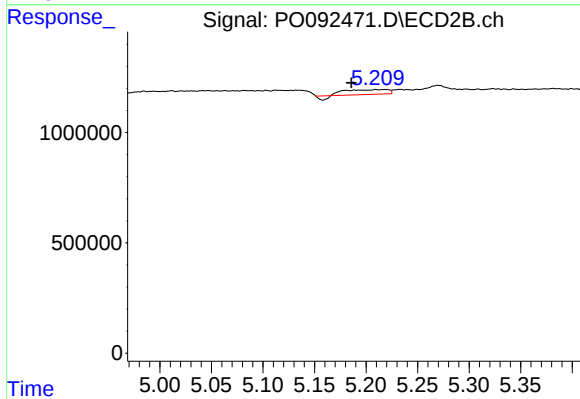

#15 AR-1232-5


R.T.: 5.219 min
Delta R.T.: 0.033 min
Response: 552658
Conc: 30.90 ng/ml

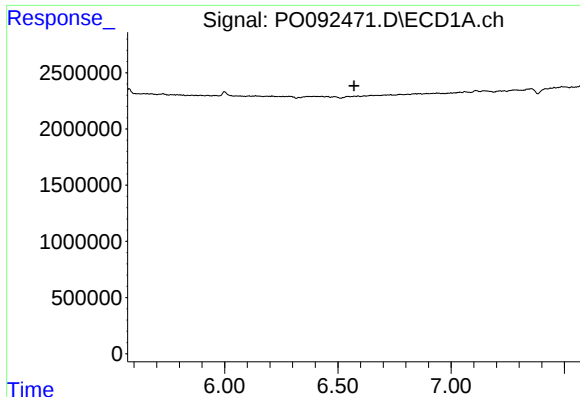

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

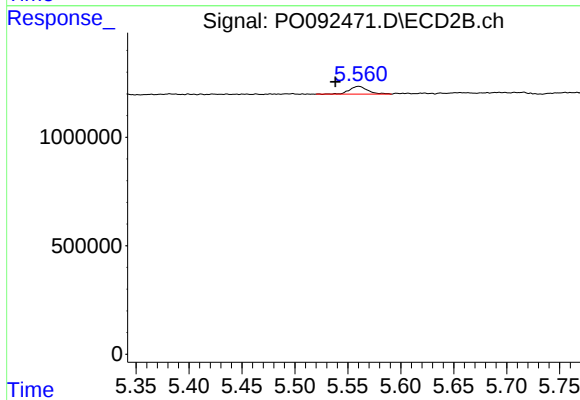


#20 AR-1242-5

R.T.: 5.560 min
Delta R.T.: 0.022 min
Response: 428401
Conc: 11.83 ng/ml

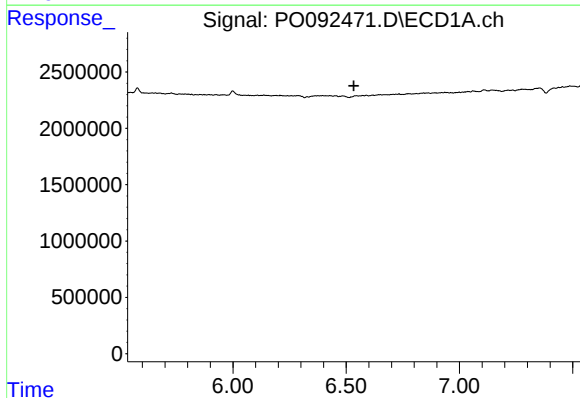


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.533 min
Response: 0
Conc: N.D.

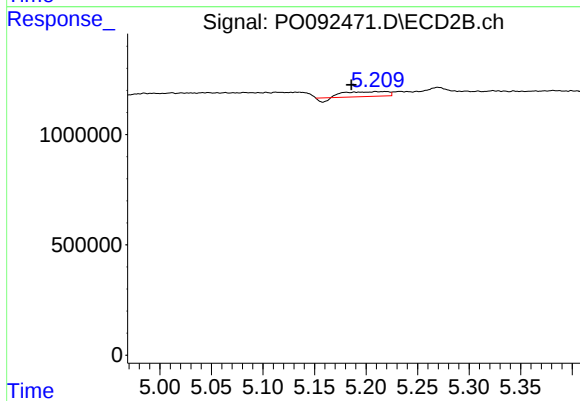

#24 AR-1248-4


R.T.: 5.219 min
Delta R.T.: 0.033 min
Response: 552658
Conc: 10.29 ng/ml

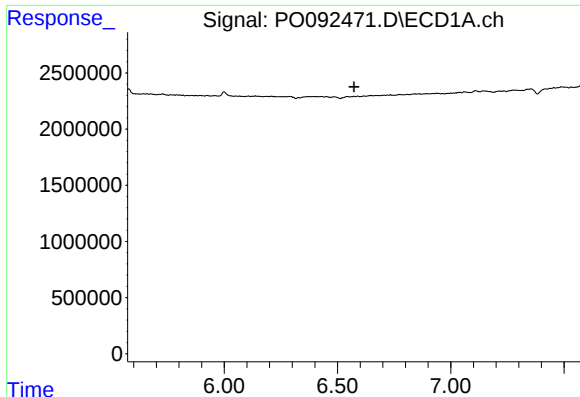

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

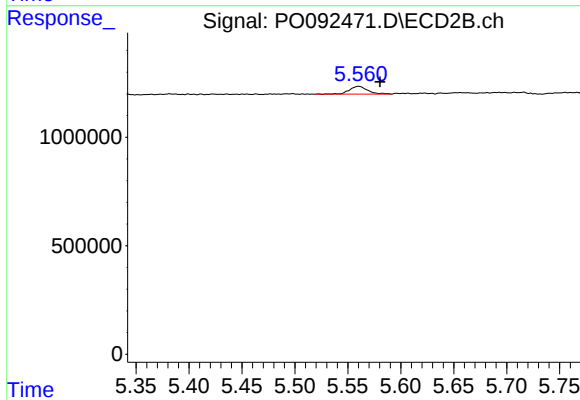


#25 AR-1248-5

R.T.: 5.560 min
Delta R.T.: -0.020 min
Response: 428401
Conc: 9.05 ng/ml

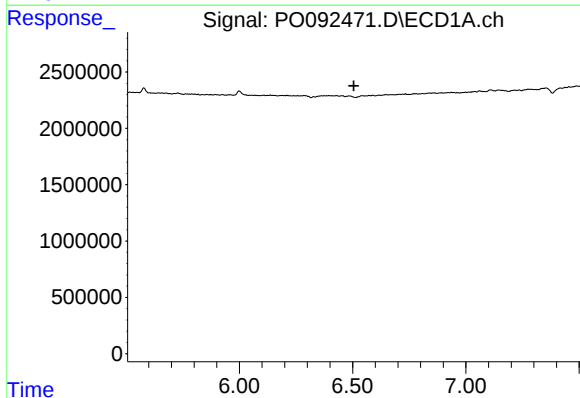


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

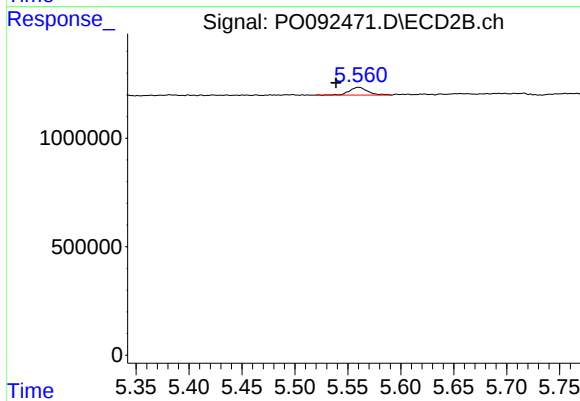

#26 AR-1254-1


R.T.: 5.560 min
Delta R.T.: 0.021 min
Response: 428401
Conc: 5.47 ng/ml

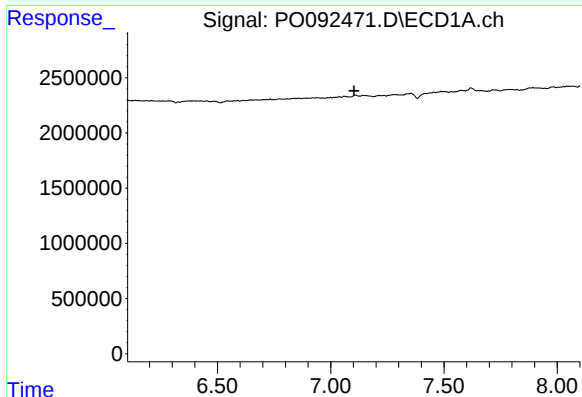

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

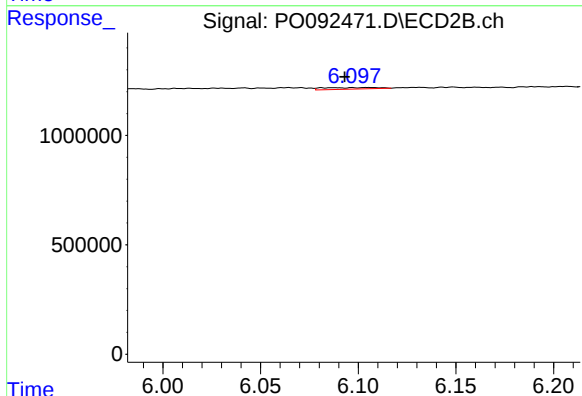


#28 AR-1254-3

R.T.: 6.105 min
Delta R.T.: 0.012 min
Response: 141336
Conc: 1.32 ng/ml

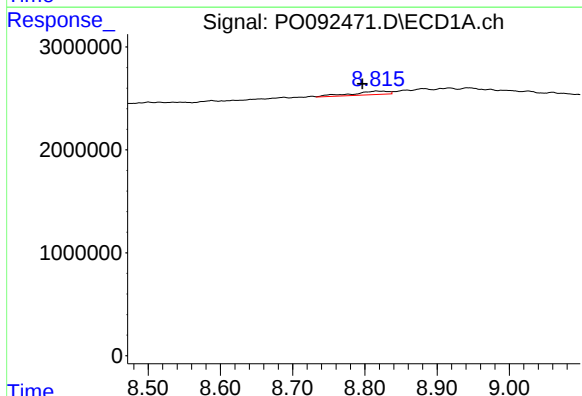


#38 AR-1262-3

R.T.: 8.816 min
Delta R.T.: 0.019 min
Response: 1203861
Conc: 7.12 ng/ml

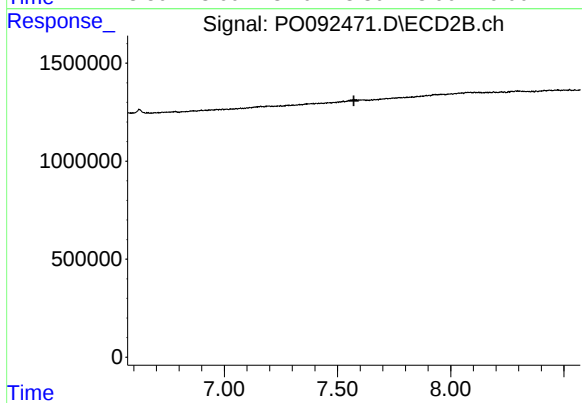

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.572 min
Response: 0
Conc: N.D.

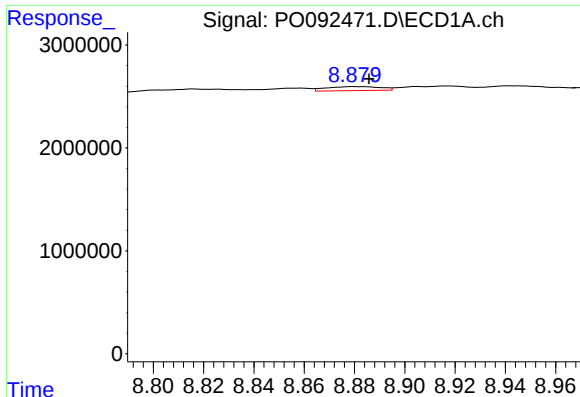

#39 AR-1262-4


R.T.: 8.880 min
Delta R.T.: -0.006 min
Response: 568974
Conc: 5.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

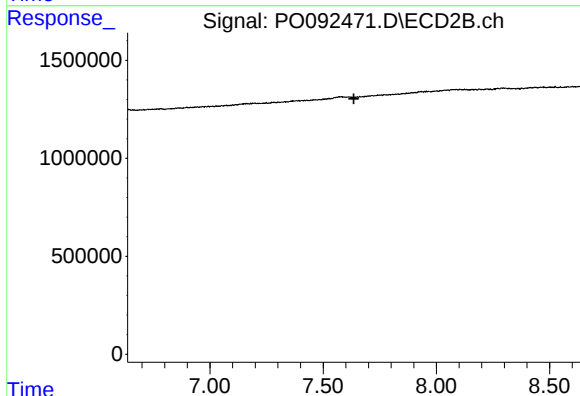


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.636 min
Response: 0
Conc: N.D.

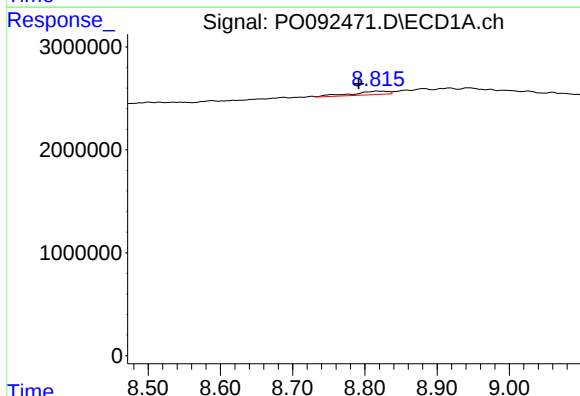


#41 AR-1268-1

R.T.: 8.816 min
Delta R.T.: 0.024 min
Response: 1203861
Conc: 3.81 ng/ml

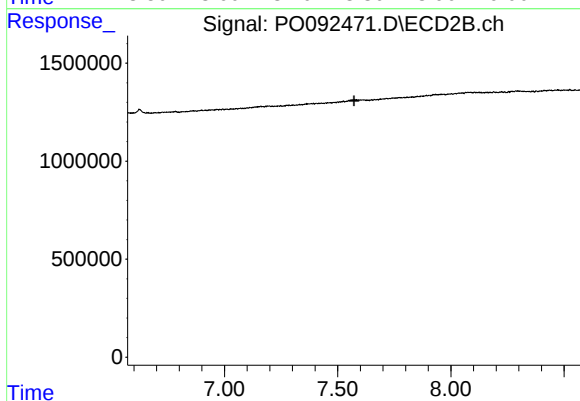

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

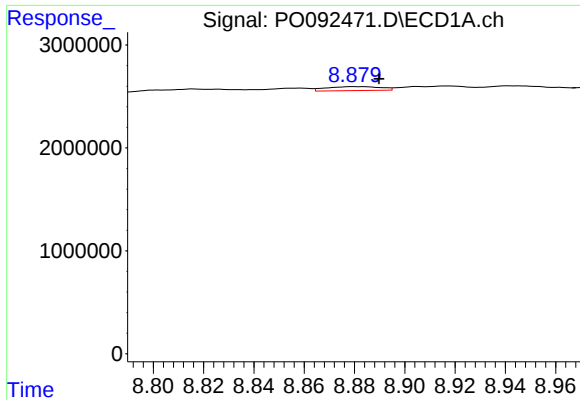

#42 AR-1268-2

R.T.: 8.880 min
Delta R.T.: -0.010 min
Response: 568974
Conc: 1.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

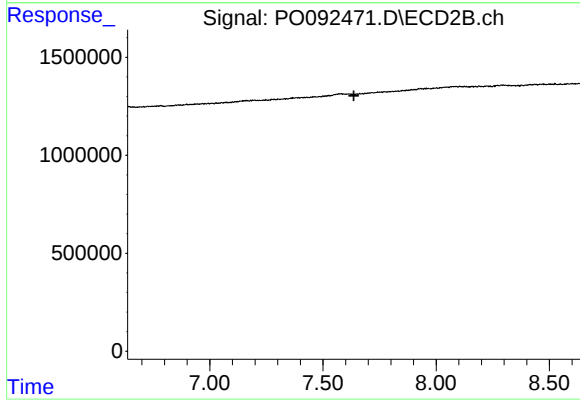

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.636 min
Response: 0
Conc: N.D.