

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
 Data File : PP033369.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Feb 2021 14:25
 Operator : DD\AJ
 Sample : PB134682BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:55:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.737	3.998	1768391	922981	28.838	22.571
2)	SA Decachlor...	10.558	9.264	1267220	864659	29.091	25.811
Target Compounds							
8)	L2 AR-1221-1	4.980	0.000	189080	0	306.497	N.D. #
9)	L2 AR-1221-2	5.082	4.328f	35796	85338	76.947	270.049 #
28)	L6 AR-1254-3	7.559f	0.000	37378	0	12.306	N.D. #
29)	L6 AR-1254-4	7.830	0.000	40866	0	17.666	N.D. #
30)	L6 AR-1254-5	8.255	0.000	22593	0	9.337	N.D. #
35)	L7 AR-1260-5	8.896f	0.000	77993	0	14.489	N.D. #
37)	L8 AR-1262-2	8.896f	0.000	77993	0	12.457	N.D. #
45)	L9 AR-1268-5	10.262f	0.000	19869	0	1.214	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
Data File : PP033369.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Feb 2021 14:25
Operator : DD\AJ
Sample : PB134682BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:55:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

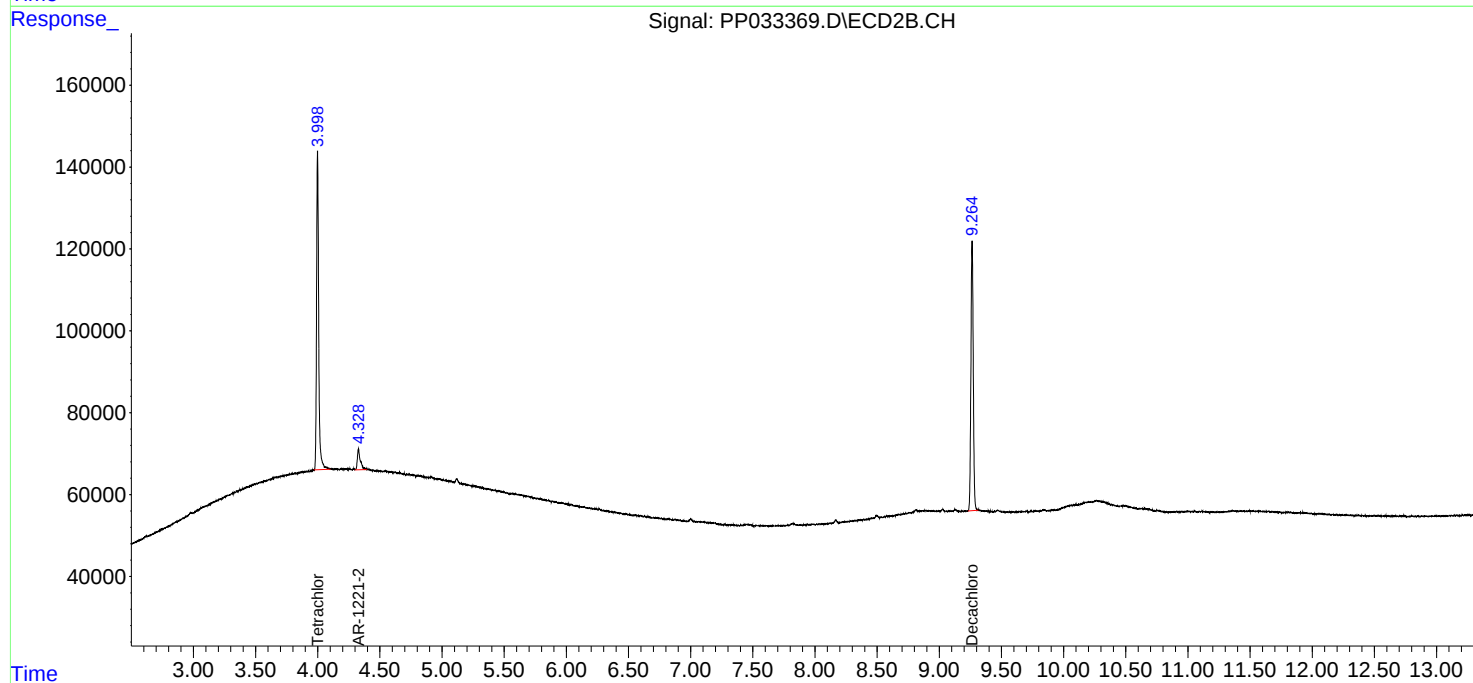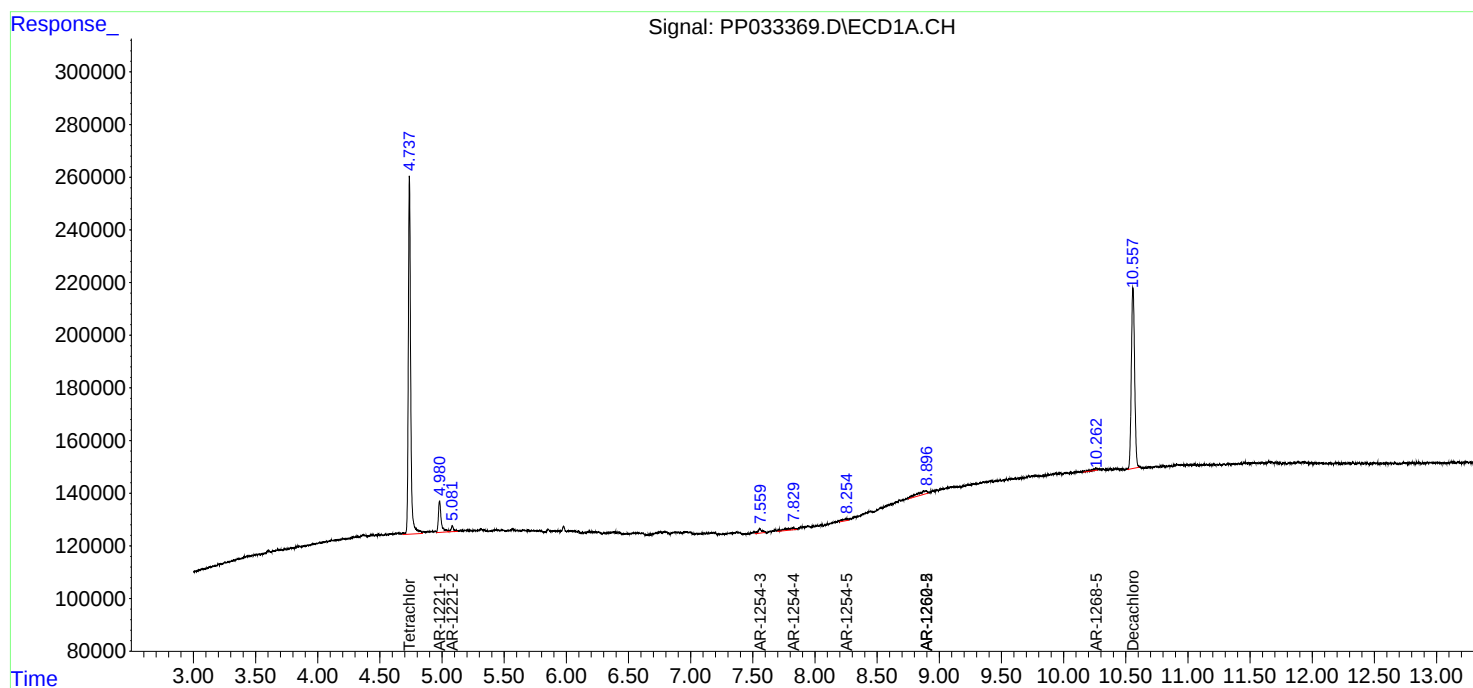


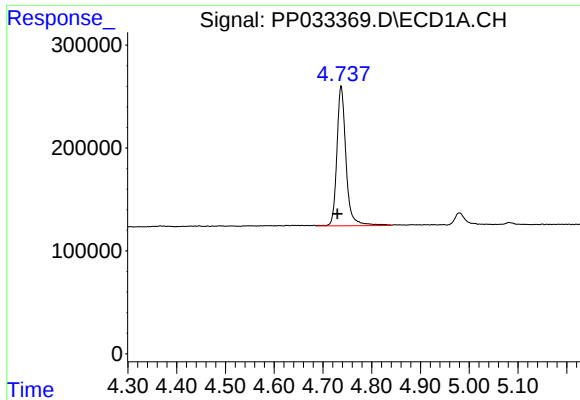

#1 Tetrachloro-m-xylene


R.T.: 4.737 min
Delta R.T.: 0.007 min
Response: 1768391
Conc: 28.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

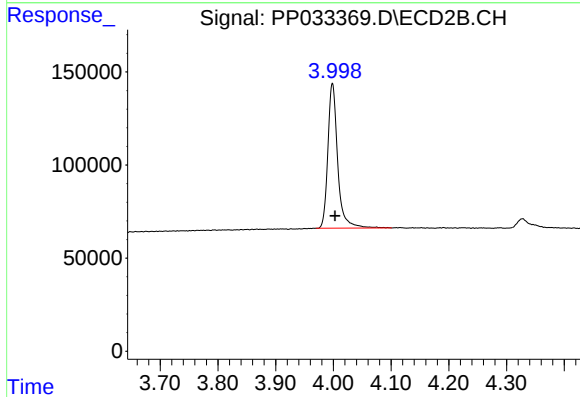


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 922981
Conc: 22.57 ng/ml

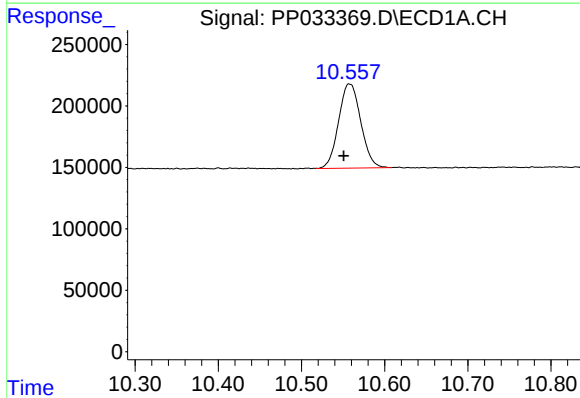


#2 Decachlorobiphenyl

R.T.: 10.558 min
Delta R.T.: 0.007 min
Response: 1267220
Conc: 29.09 ng/ml

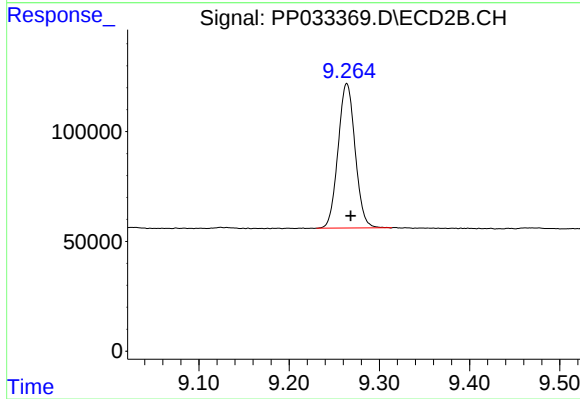

#2 Decachlorobiphenyl


R.T.: 9.264 min
Delta R.T.: -0.004 min
Response: 864659
Conc: 25.81 ng/ml

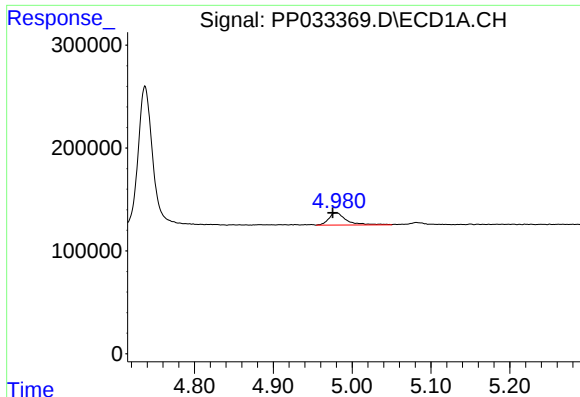

#8 AR-1221-1


R.T.: 4.980 min
Delta R.T.: 0.005 min
Response: 189080
Conc: 306.50 ng/ml

Instrument :
ECD_P
ClientSampleId :

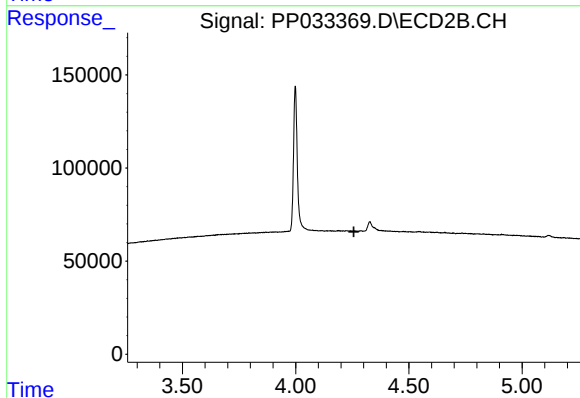


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.257 min
Response: 0
Conc: N.D.

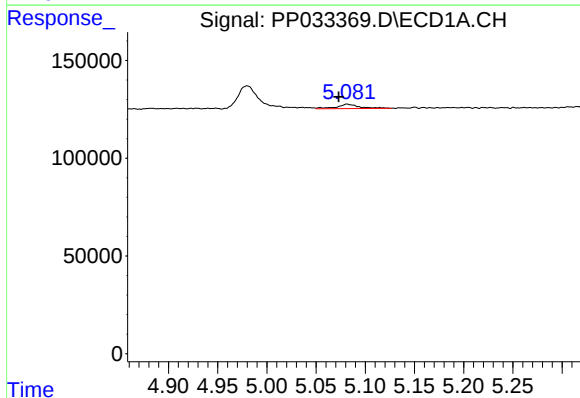


#9 AR-1221-2

R.T.: 5.082 min
Delta R.T.: 0.009 min
Response: 35796
Conc: 76.95 ng/ml

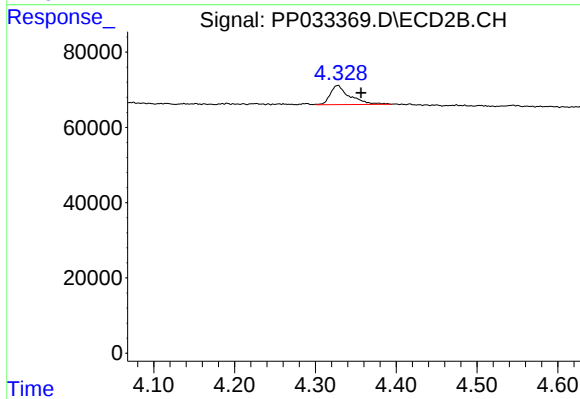

#9 AR-1221-2


R.T.: 4.328 min
Delta R.T.: -0.029 min
Response: 85338
Conc: 270.05 ng/ml

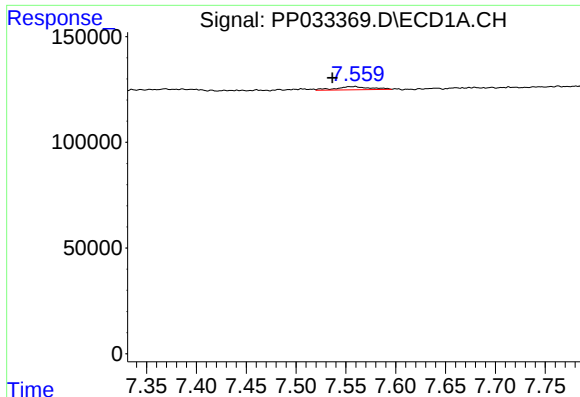

#28 AR-1254-3


R.T.: 7.559 min
Delta R.T.: 0.023 min
Response: 37378
Conc: 12.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

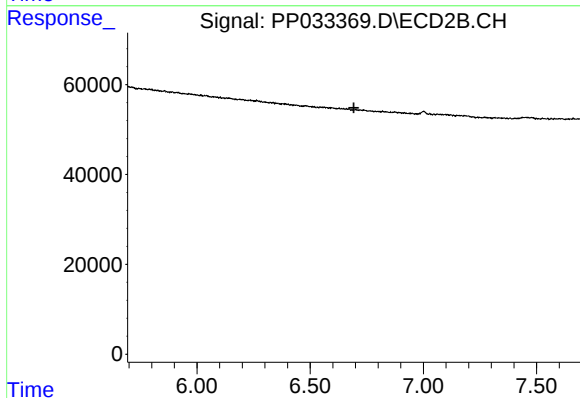


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

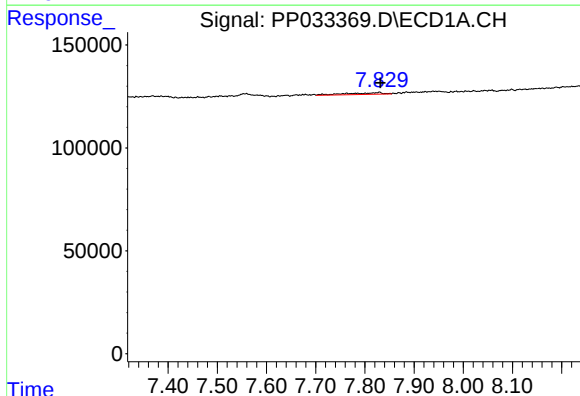


#29 AR-1254-4

R.T.: 7.830 min
Delta R.T.: -0.002 min
Response: 40866
Conc: 17.67 ng/ml

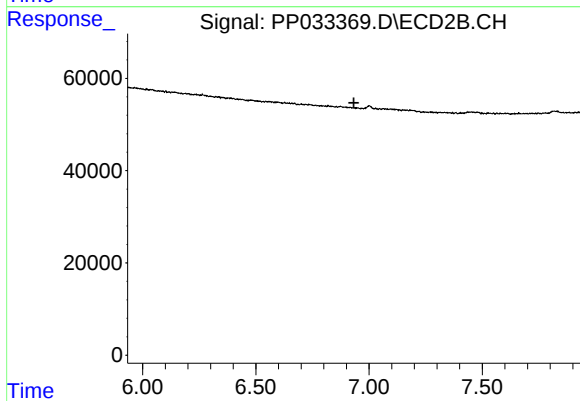

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

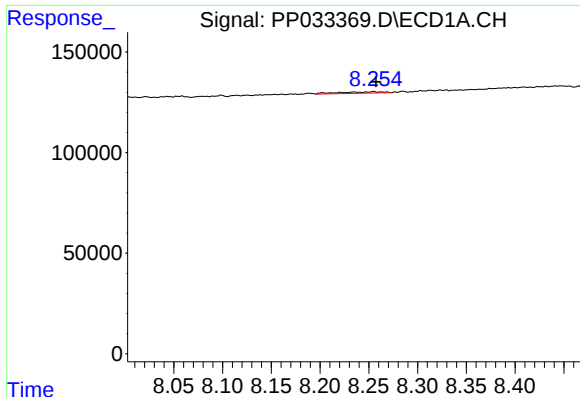

#30 AR-1254-5


R.T.: 8.255 min
Delta R.T.: -0.002 min
Response: 22593
Conc: 9.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

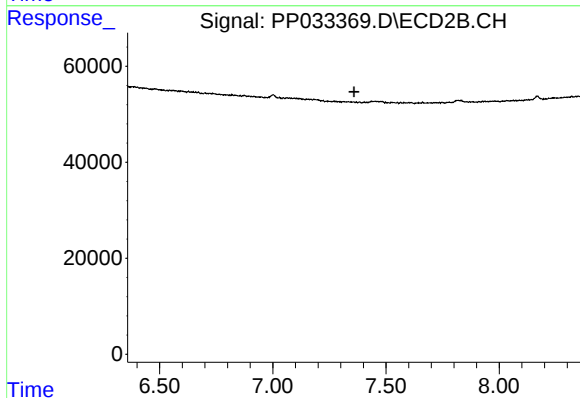


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

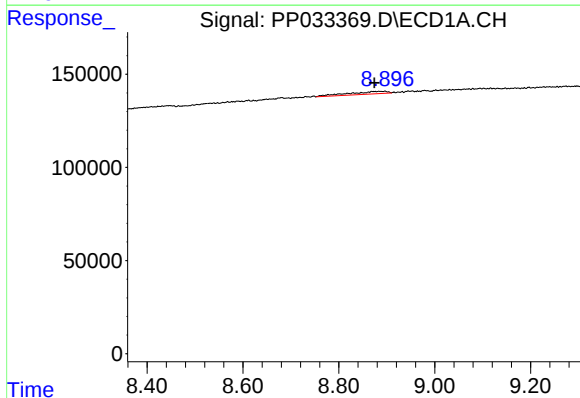


#35 AR-1260-5

R.T.: 8.896 min
Delta R.T.: 0.022 min
Response: 77993
Conc: 14.49 ng/ml

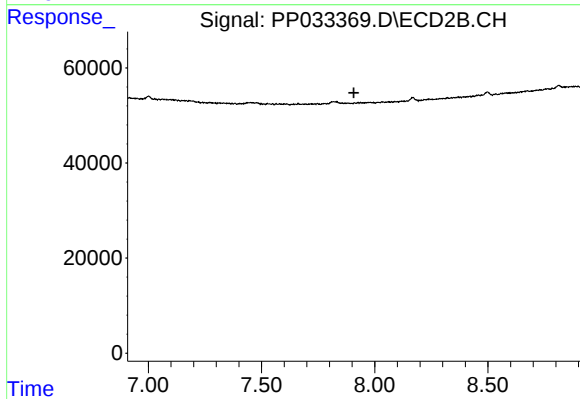

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.908 min
Response: 0
Conc: N.D.

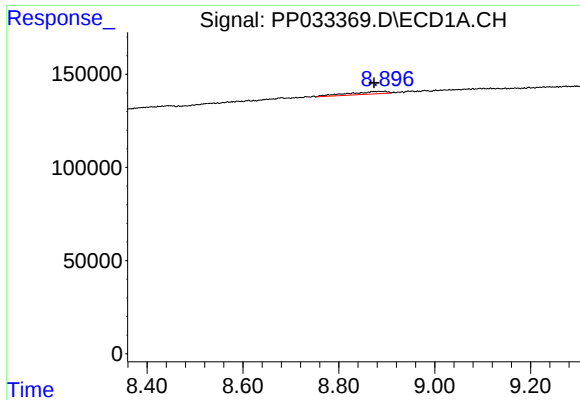

#37 AR-1262-2


R.T.: 8.896 min
Delta R.T.: 0.023 min
Response: 77993
Conc: 12.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

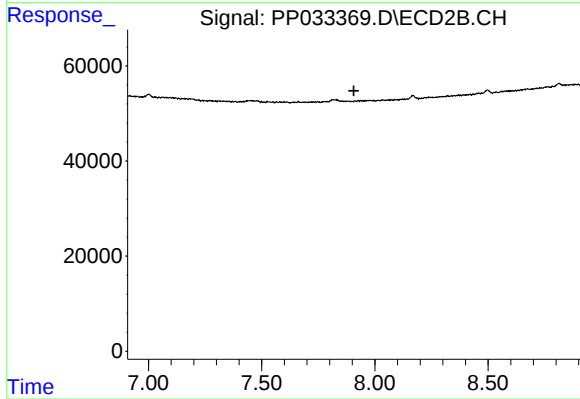


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.

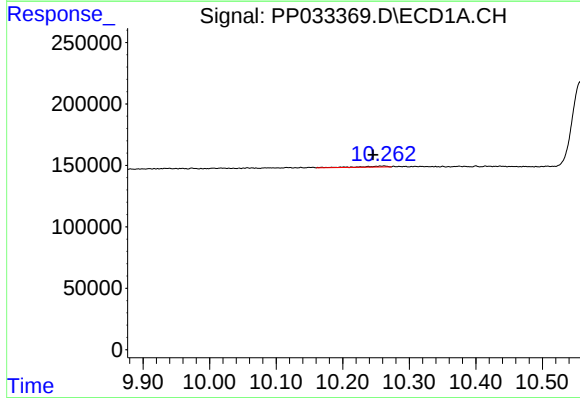

#45 AR-1268-5

R.T.: 10.262 min
Delta R.T.: 0.017 min
Response: 19869
Conc: 1.21 ng/ml

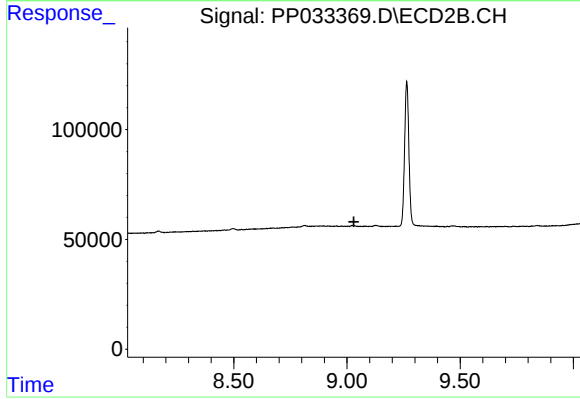

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.