

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
 Data File : PP033381.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Feb 2021 18:19
 Operator : DD\AJ
 Sample : M1426-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 T1090-181468

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:25:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 23:14:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.723	3.999	179439	77031	2.926m	1.884 #
2) SA Decachlor...	10.538	9.257	114100	98398	2.619m	2.937

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
Data File : PP033381.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Feb 2021 18:19
Operator : DD\AJ
Sample : M1426-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
T1090-181468


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 23:14:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

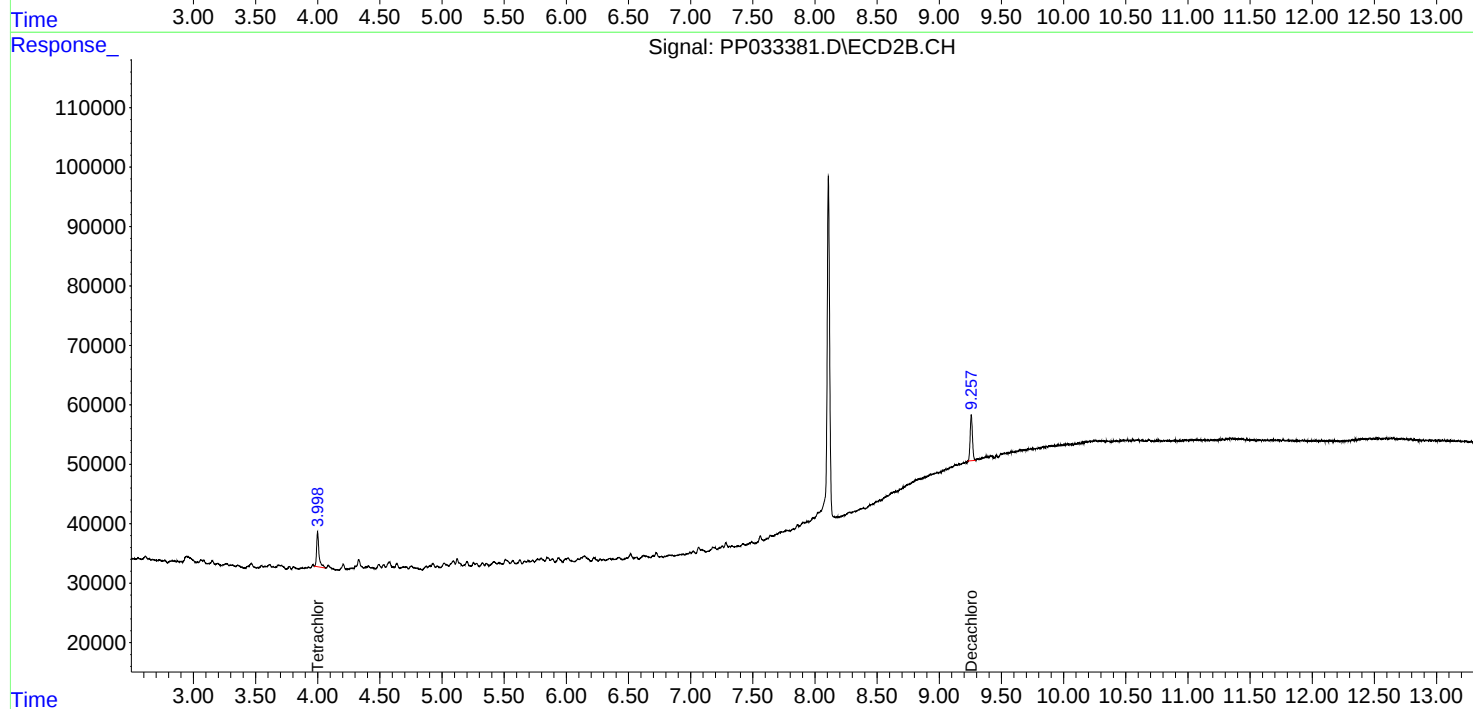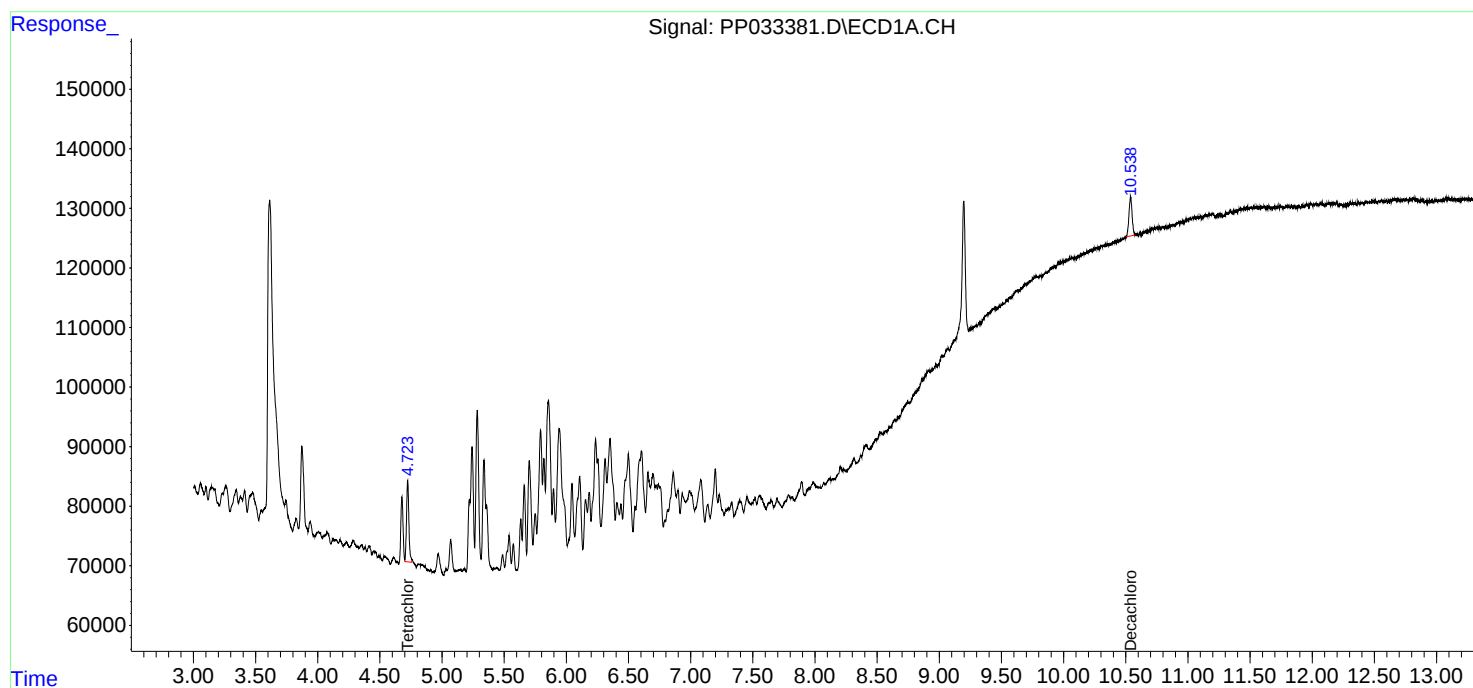

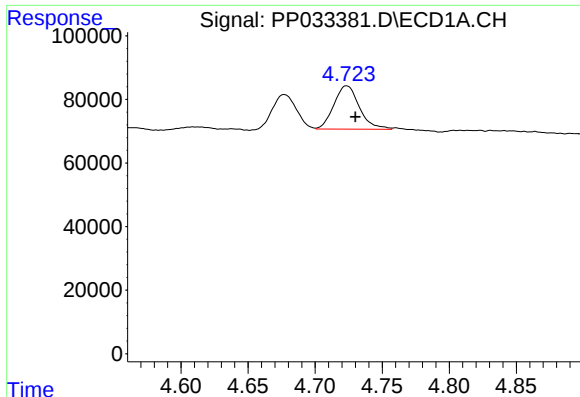


#1 Tetrachloro-m-xylene

R.T.: 4.723 min
Delta R.T.: -0.007 min
Response: 179439
Conc: 2.93 ng/ml m

Instrument :
ECD_P
ClientSampleId :
T1090-181468


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:39 AM

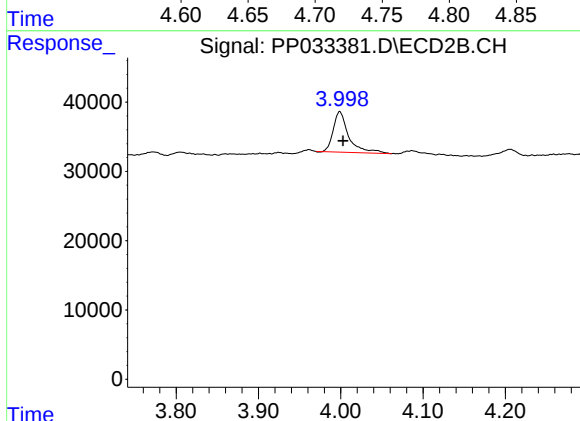


#1 Tetrachloro-m-xylene

R.T.: 3.999 min
Delta R.T.: -0.004 min
Response: 77031
Conc: 1.88 ng/ml

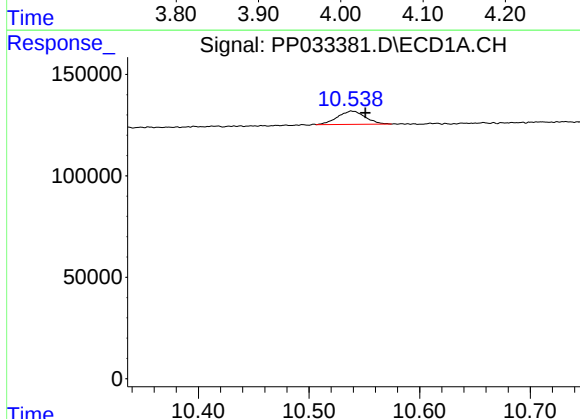

#2 Decachlorobiphenyl

R.T.: 10.538 min
Delta R.T.: -0.013 min
Response: 114100
Conc: 2.62 ng/ml m

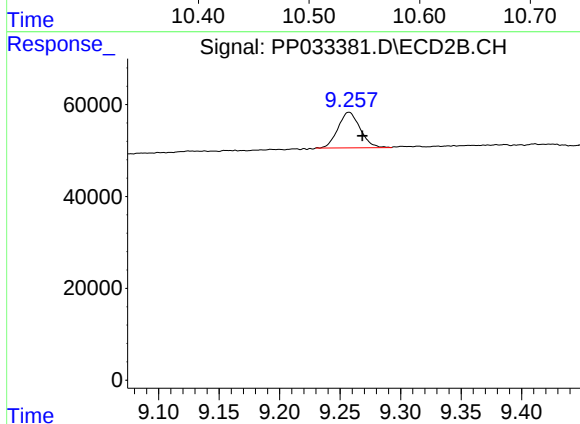

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.011 min
Response: 98398
Conc: 2.94 ng/ml